
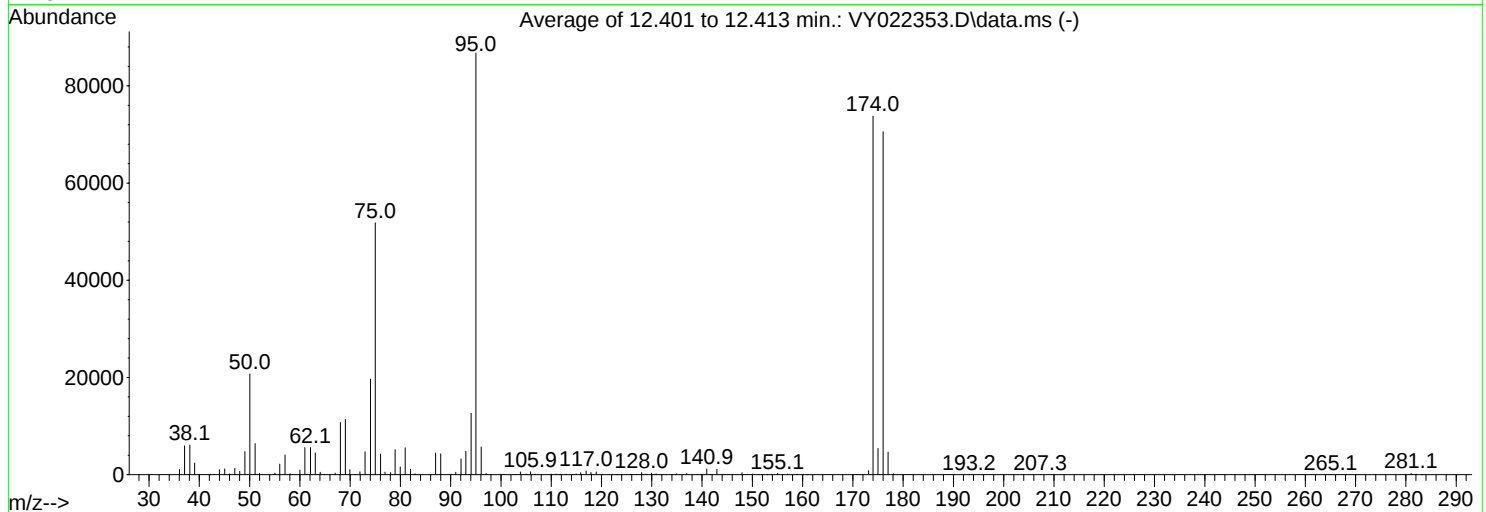


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY052125\  
Data File : VY022353.D  
Acq On : 21 May 2025 09:02  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y051525S.M  
Title : SW846 8260  
Last Update : Fri May 16 01:42:09 2025

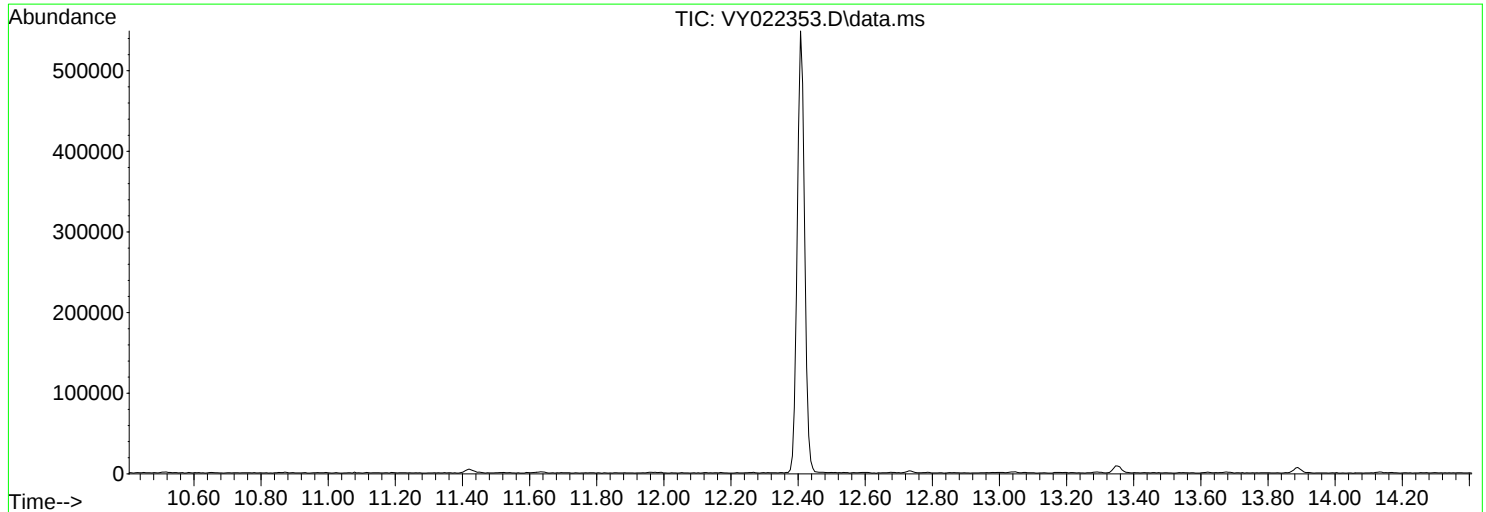

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 23.9  | 20739 | PASS      |
| 75     | 95      | 30     | 60     | 59.7  | 51821 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 86803 | PASS      |
| 96     | 95      | 5      | 9      | 6.6   | 5713  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.1   | 843   | PASS      |
| 174    | 95      | 50     | 100    | 85.0  | 73784 | PASS      |
| 175    | 174     | 5      | 9      | 7.3   | 5417  | PASS      |
| 176    | 174     | 95     | 101    | 95.6  | 70552 | PASS      |
| 177    | 176     | 5      | 9      | 6.6   | 4653  | PASS      |