
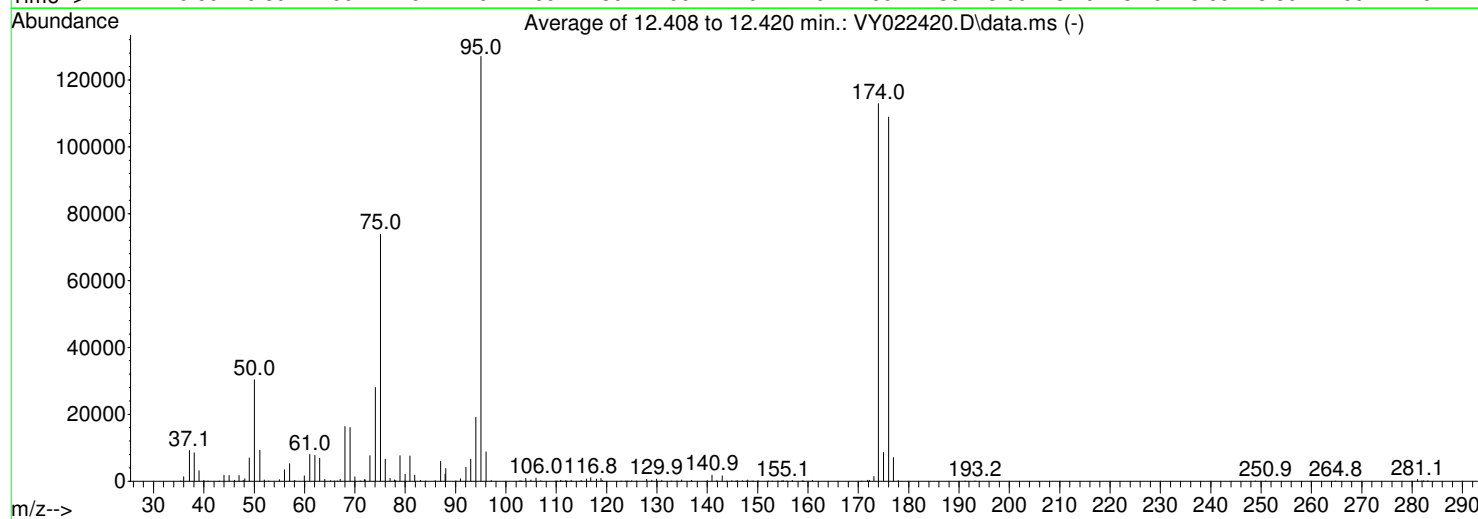


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052725\
Data File : VY022420.D
Acq On : 27 May 2025 08:20
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
Title : SW846 8260
Last Update : Wed May 28 10:34:06 2025

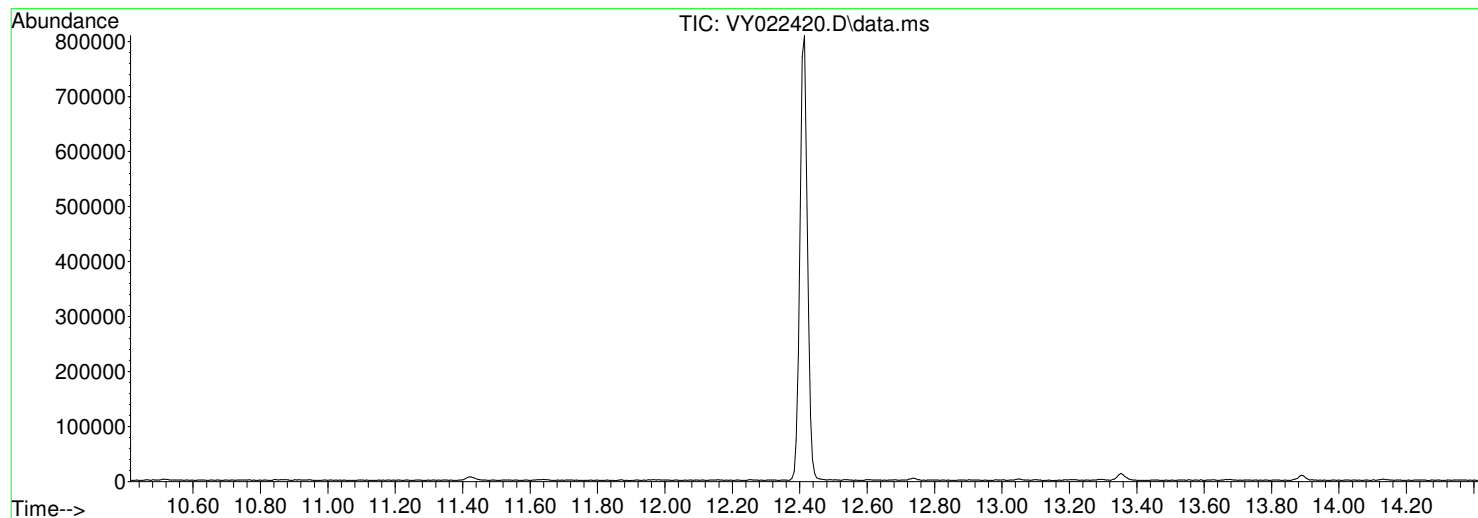

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.8	30285	PASS
75	95	30	60	58.1	73816	PASS
95	95	100	100	100.0	127085	PASS
96	95	5	9	6.9	8787	PASS
173	174	0.00	2	1.2	1405	PASS
174	95	50	100	88.8	112901	PASS
175	174	5	9	7.6	8537	PASS
176	174	95	101	96.4	108888	PASS
177	176	5	9	6.5	7038	PASS