


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052825\
Data File : VY022439.D
Acq On : 28 May 2025 08:48
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
Title : SW846 8260
Last Update : Wed May 28 10:34:06 2025

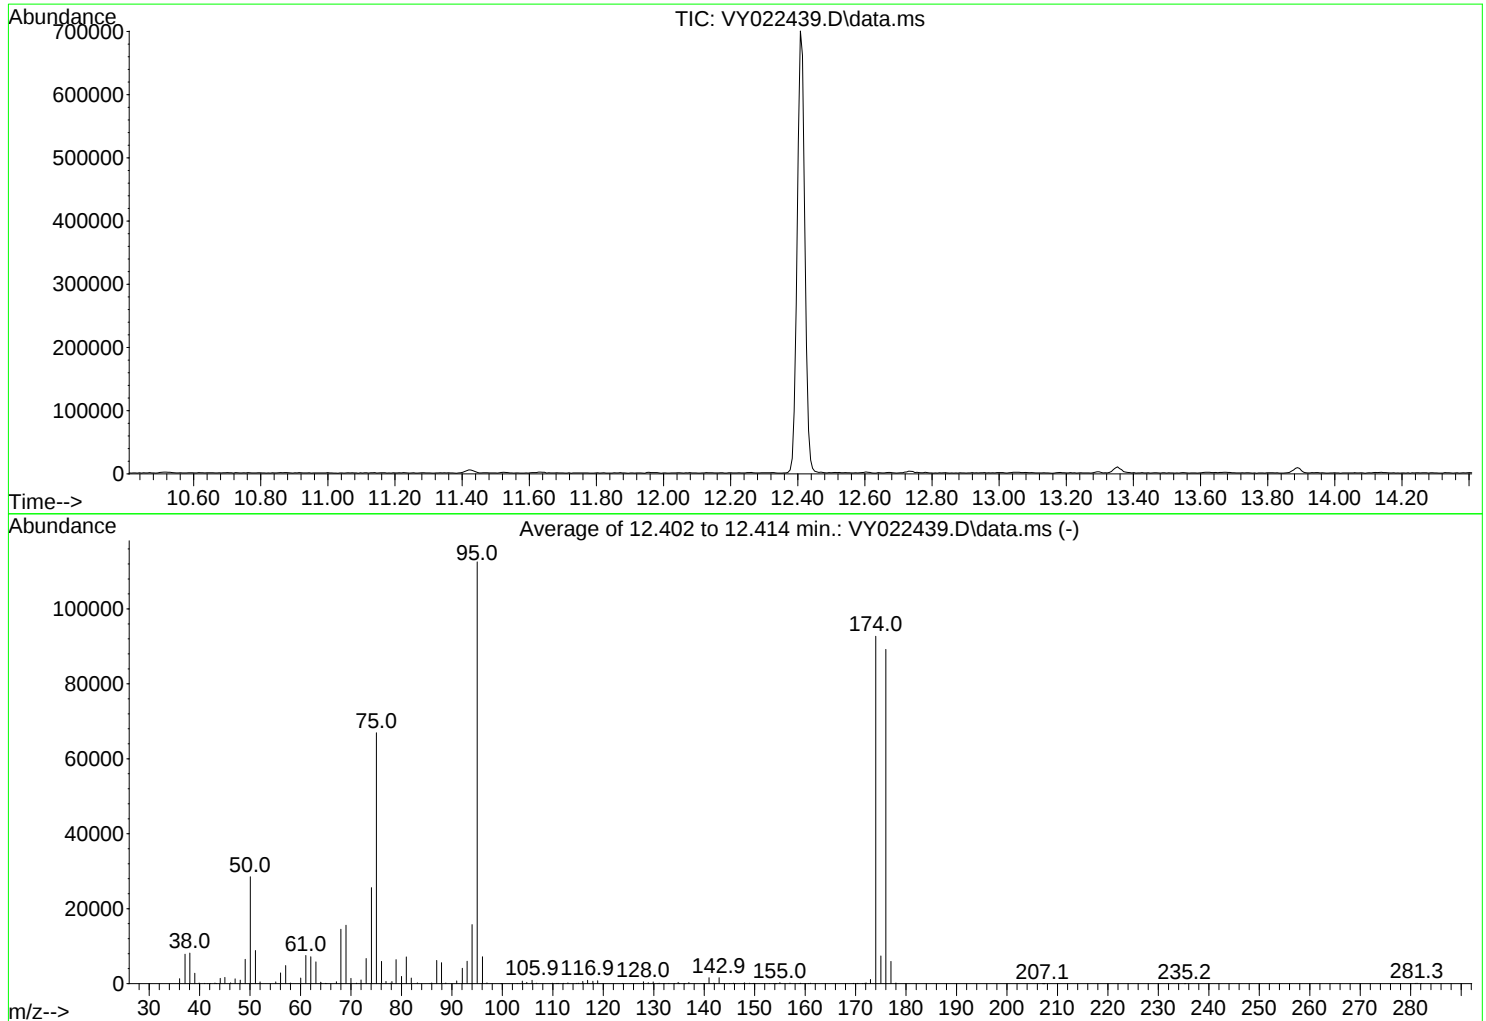

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.3	28525	PASS
75	95	30	60	59.5	66933	PASS
95	95	100	100	100.0	112560	PASS
96	95	5	9	6.4	7186	PASS
173	174	0.00	2	1.2	1127	PASS
174	95	50	100	82.4	92717	PASS
175	174	5	9	8.0	7373	PASS
176	174	95	101	96.2	89219	PASS
177	176	5	9	6.7	5947	PASS