
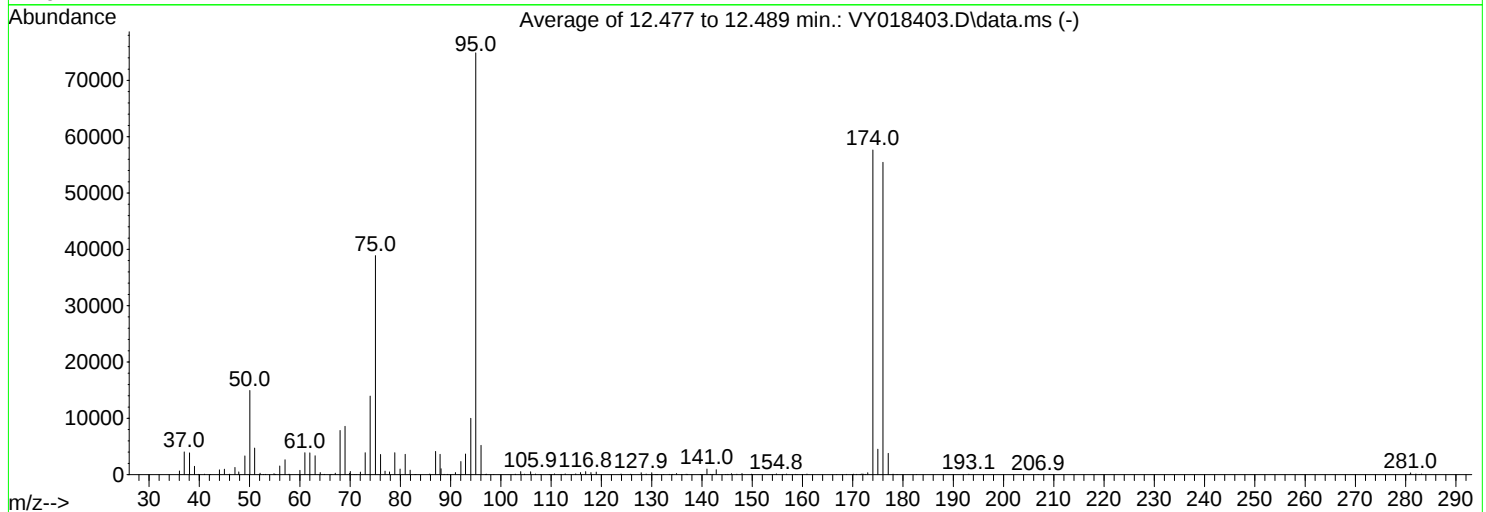


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY053024\
Data File : VY018403.D
Acq On : 30 May 2024 09:16
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052224S.M
Title : SW846 8260
Last Update : Thu May 23 01:40:36 2024

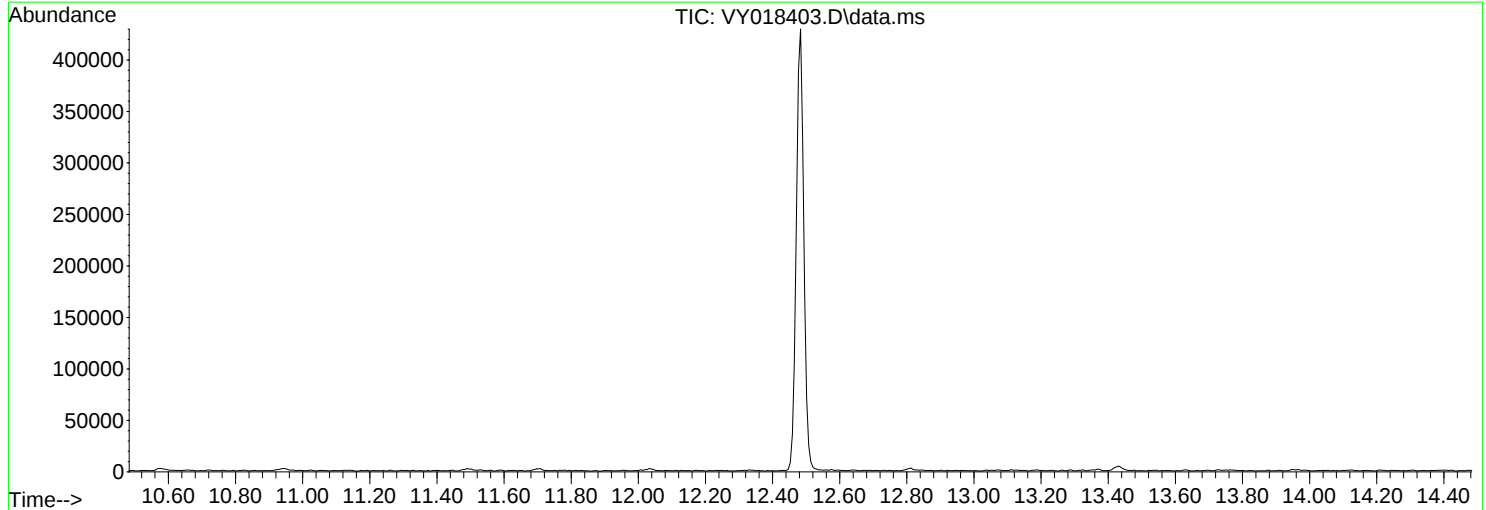

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	14938	PASS
75	95	30	60	51.9	38901	PASS
95	95	100	100	100.0	74893	PASS
96	95	5	9	6.9	5193	PASS
173	174	0.00	2	0.6	337	PASS
174	95	50	100	77.0	57648	PASS
175	174	5	9	7.8	4521	PASS
176	174	95	101	96.2	55448	PASS
177	176	5	9	6.8	3795	PASS