

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY053025\
 Data File : VY022481.D
 Acq On : 30 May 2025 16:15
 Operator : SY/MD
 Sample : Q2173-02
 Misc : 6.34g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OR-400-CF-402B-VOC-23

Quant Time: May 31 02:29:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 28 10:34:06 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	271397	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	490507	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.413	117	384908	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	121087	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.060	65	154575	54.073	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 108.140%	
35) Dibromofluoromethane	7.634	113	149226	51.949	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 103.900%	
50) Toluene-d8	10.103	98	591755	50.533	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 101.060%	
62) 4-Bromofluorobenzene	12.401	95	138637	39.139	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 78.280%	
Target Compounds						
					Qvalue	
20) Methylene Chloride	4.616	84	5286	1.594	ug/l	97
31) Cyclohexane	7.707	56	7372	1.341	ug/l #	27
36) 1,1-Dichloropropene	7.707	75	24021	5.270	ug/l #	50
38) Carbon Tetrachloride	7.707	117	28434	5.988	ug/l #	15
76) 1,2,3-Trichloropropane	12.401	75	81732	67.386	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.401	75	81732	152.392	ug/l #	12

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY053025\
Data File : VY022481.D
Acq On : 30 May 2025 16:15
Operator : SY/MD
Sample : Q2173-02
Misc : 6.34g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-23

Quant Time: May 31 02:29:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
Quant Title : SW846 8260
QLast Update : Wed May 28 10:34:06 2025
Response via : Initial Calibration




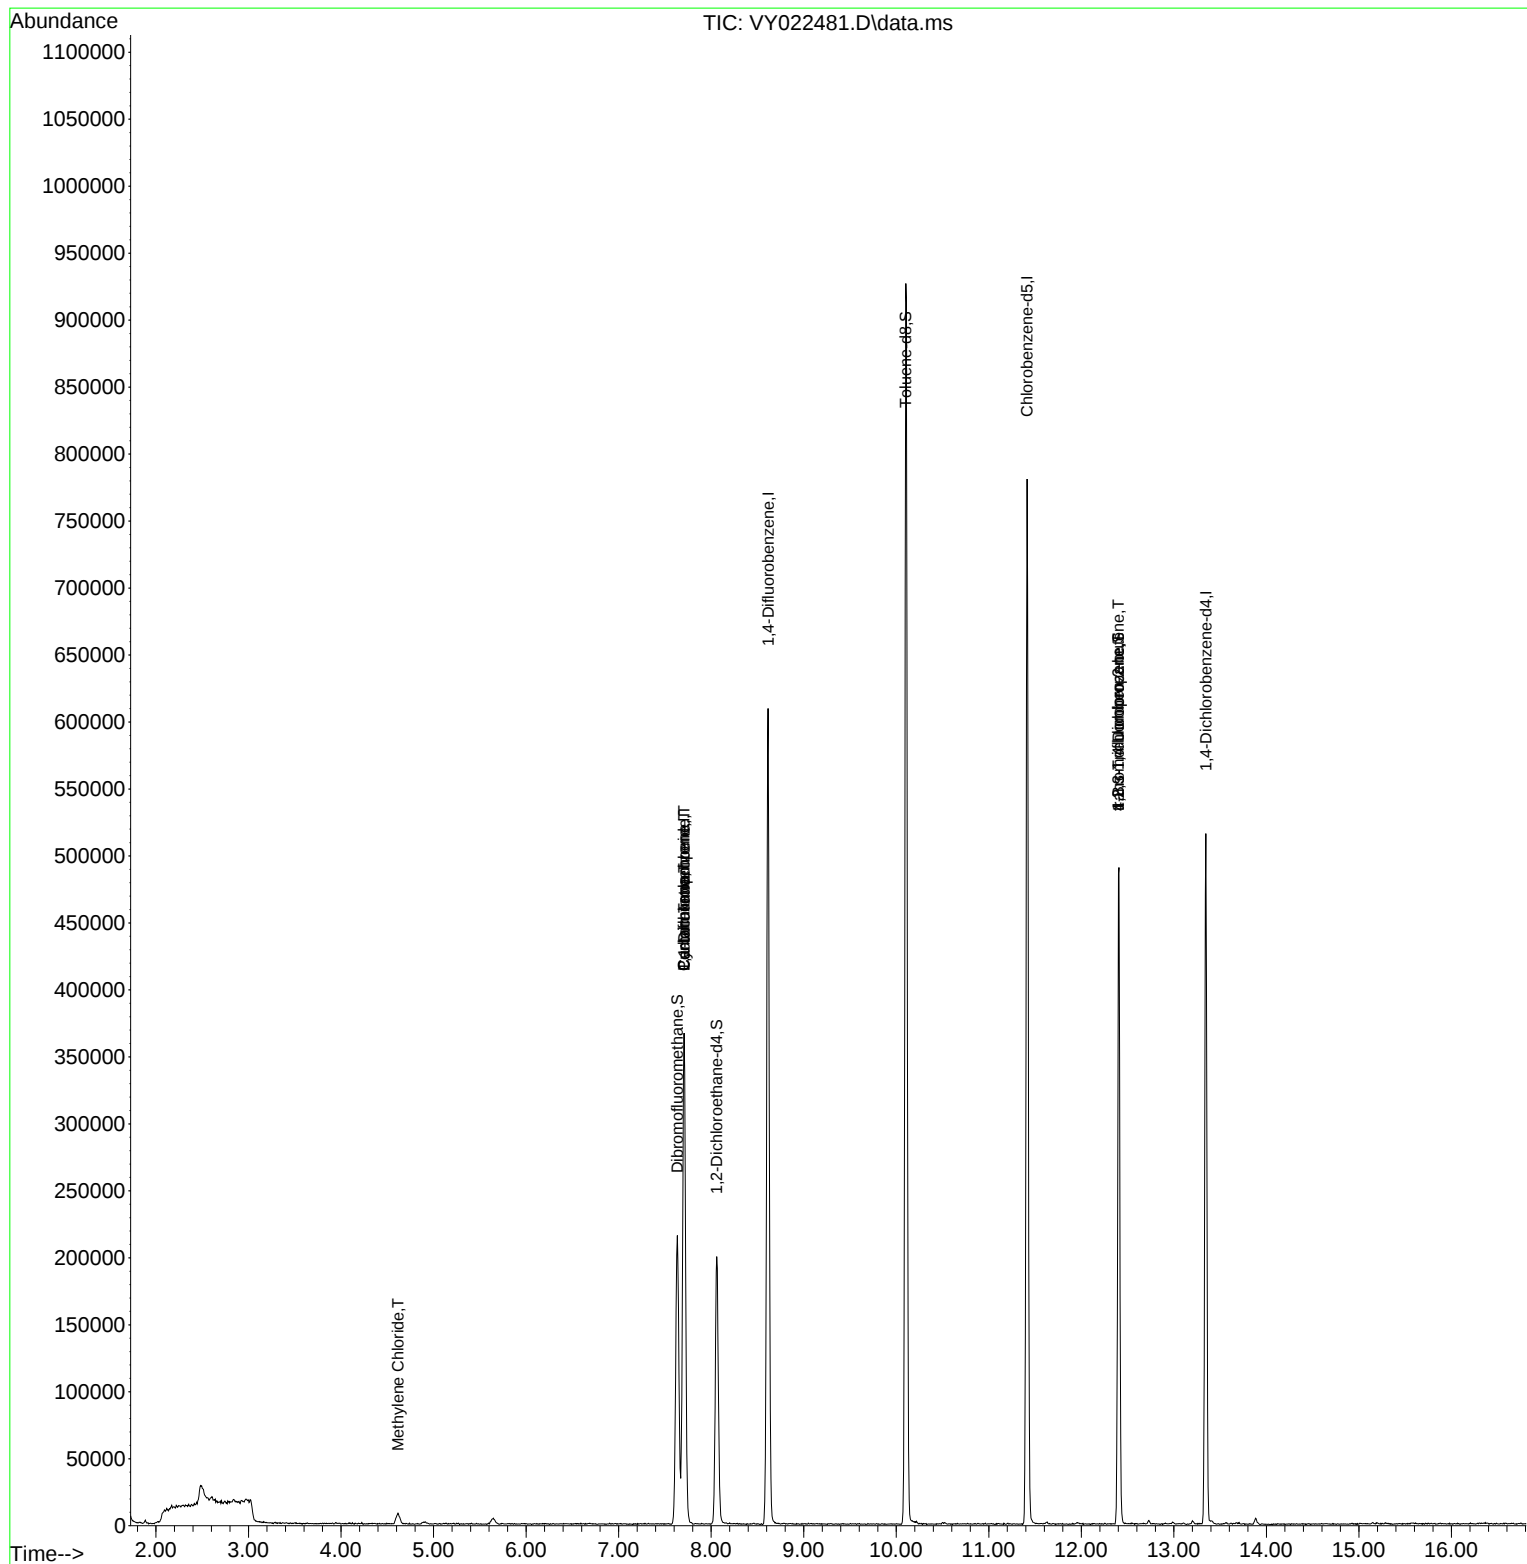




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15




Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-23


Tgt Ion:168 Resp: 271397
Ion Ratio Lower Upper
168 100
99 55.8 44.7 67.1

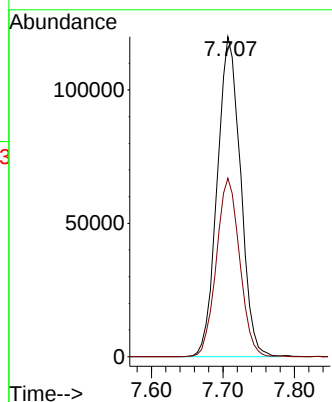

#20
Methylene Chloride
Concen: 1.594 ug/l
RT: 4.616 min Scan# 475
Delta R.T. -0.006 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15

Tgt Ion: 84 Resp: 5286
Ion Ratio Lower Upper
84 100
49 126.6 97.8 146.8
51 40.1 29.5 44.3
86 65.0 51.8 77.6


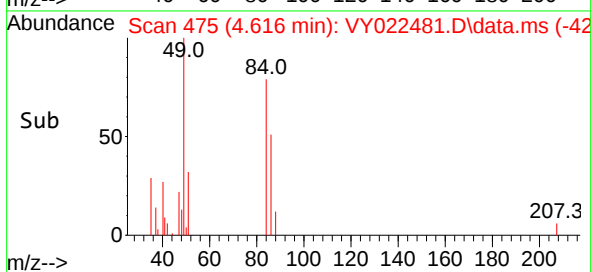
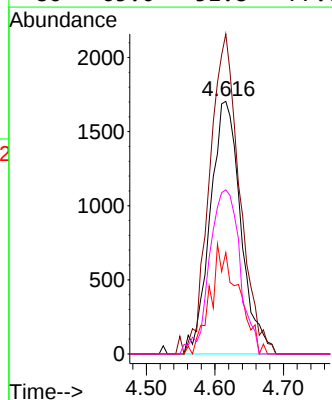





#31
Cyclohexane
Concen: 1.341 ug/l
RT: 7.707 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15




Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-23


Tgt Ion: 56 Resp: 7372
Ion Ratio Lower Upper
56 100
69 132.3 24.6 36.8#
84 119.9 70.4 105.6#

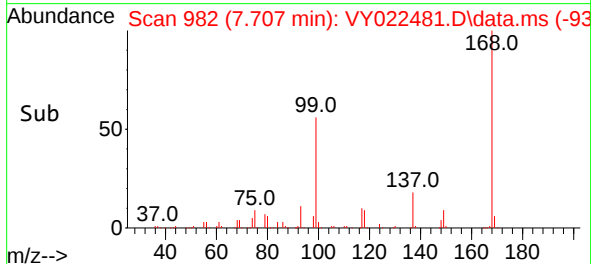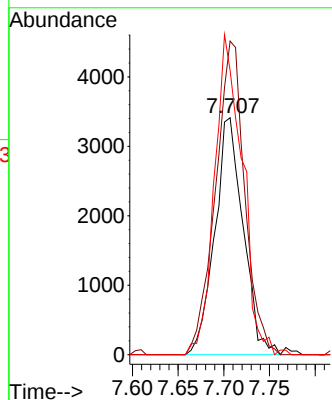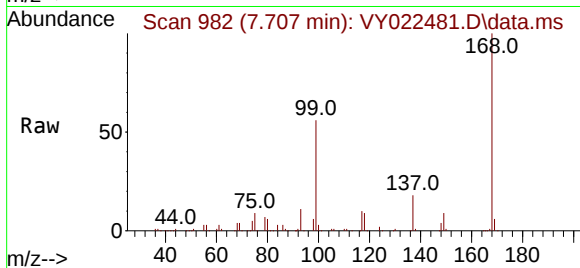

#33
1,2-Dichloroethane-d4
Concen: 54.073 ug/l
RT: 8.060 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15

Tgt Ion: 65 Resp: 154575
Ion Ratio Lower Upper
65 100
67 51.6 0.0 104.4

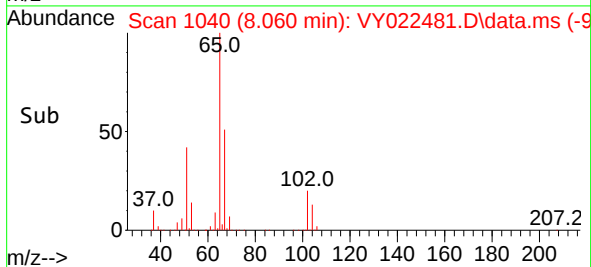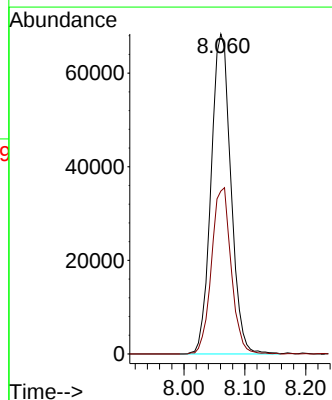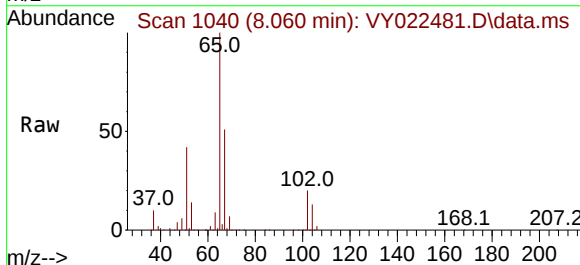



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY022481.D

Acq: 30 May 2025 16:15

Instrument :

MSVOA_Y

ClientSampleId :

OR-400-CF-402B-VOC-23





Tgt Ion:114 Resp: 490507

Ion Ratio Lower Upper

114 100

63 20.0 0.0 42.6

88 14.4 0.0 29.4

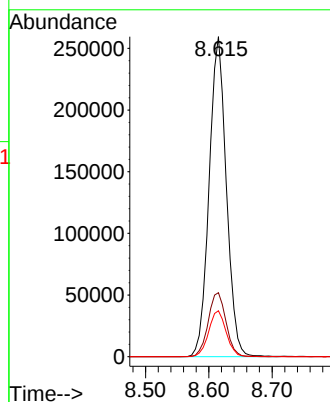

#35

Dibromofluoromethane

Concen: 51.949 ug/l

RT: 7.634 min Scan# 970

Delta R.T. -0.006 min

Lab File: VY022481.D

Acq: 30 May 2025 16:15




Tgt Ion:113 Resp: 149226


Ion Ratio Lower Upper

113 100

111 103.1 82.4 123.6

192 17.7 15.2 22.8

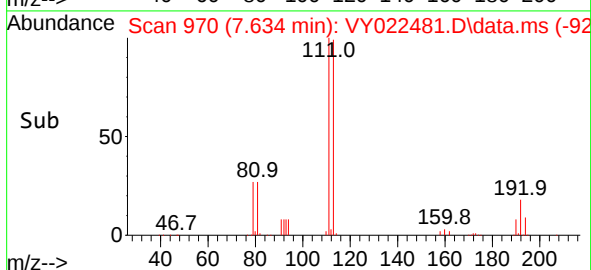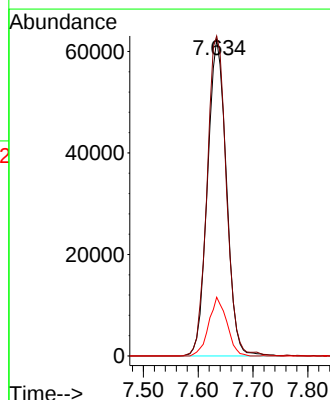



#36

1,1-Dichloropropene

Concen: 5.270 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.134 min

Lab File: VY022481.D


Acq: 30 May 2025 16:15

Instrument :

MSVOA_Y

ClientSampleId :

OR-400-CF-402B-VOC-23






Tgt Ion: 75 Resp: 24021

Ion Ratio Lower Upper

75 100

110 9.3 17.1 51.2#

77 0.0 25.1 37.7#

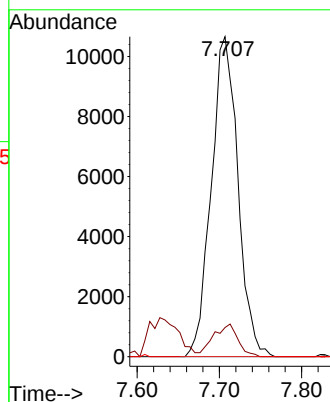

#38

Carbon Tetrachloride

Concen: 5.988 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.116 min

Lab File: VY022481.D

Acq: 30 May 2025 16:15




Tgt Ion: 117 Resp: 28434


Ion Ratio Lower Upper

117 100

119 3.9 76.3 114.5#

121 0.0 26.1 39.1#


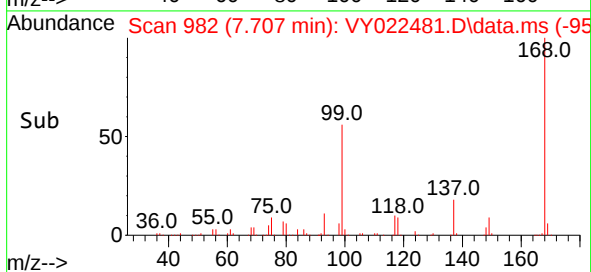

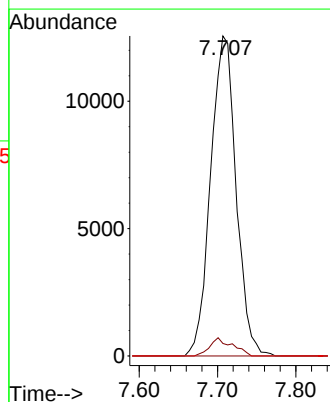




#50
Toluene-d8
Concen: 50.533 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15




Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-23


Tgt Ion: 98 Resp: 591755
Ion Ratio Lower Upper
98 100
100 64.0 52.2 78.2

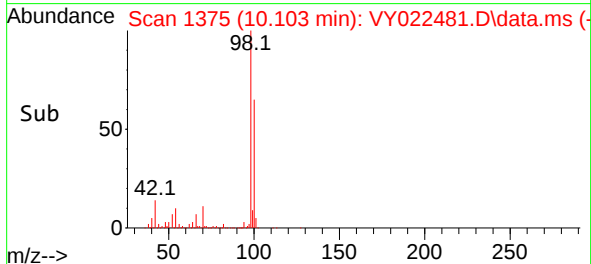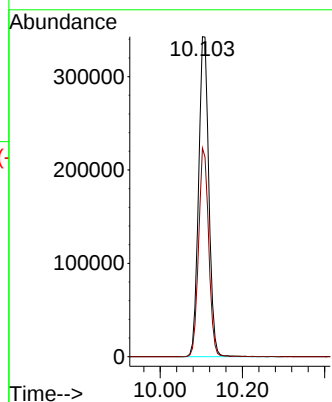

#62
4-Bromofluorobenzene
Concen: 39.139 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.006 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15

Tgt Ion: 95 Resp: 138637
Ion Ratio Lower Upper
95 100
174 84.9 0.0 171.6
176 80.7 0.0 164.6

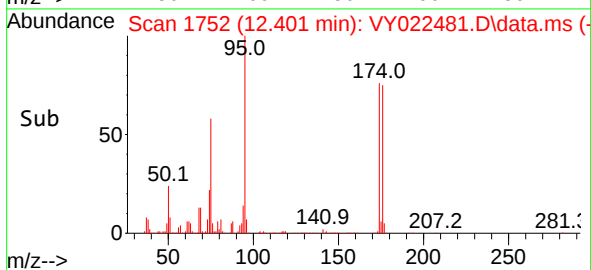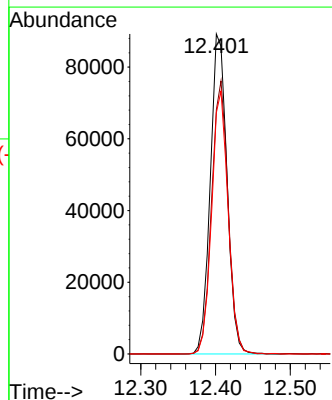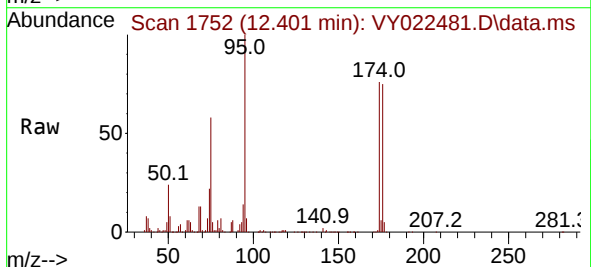



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.413 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY022481.D

Acq: 30 May 2025 16:15

Instrument :

MSVOA_Y

ClientSampleId :

OR-400-CF-402B-VOC-23





Tgt Ion:117 Resp: 384908

Ion Ratio Lower Upper

117 100

82 55.7 43.3 64.9

119 31.4 24.5 36.7

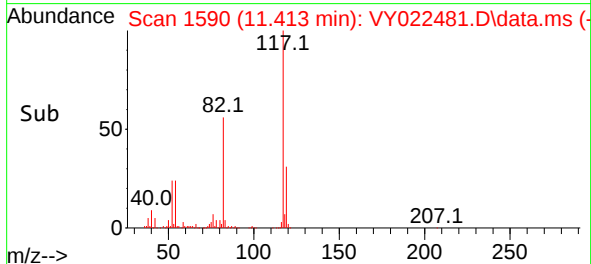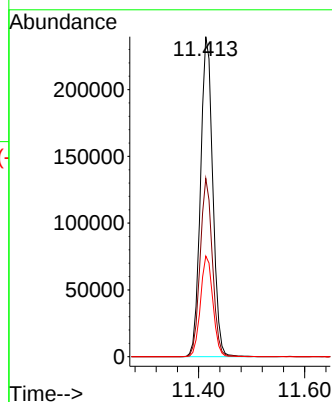

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY022481.D

Acq: 30 May 2025 16:15




Tgt Ion:152 Resp: 121087


Ion Ratio Lower Upper

152 100

115 57.5 28.4 85.3

150 156.3 0.0 345.8


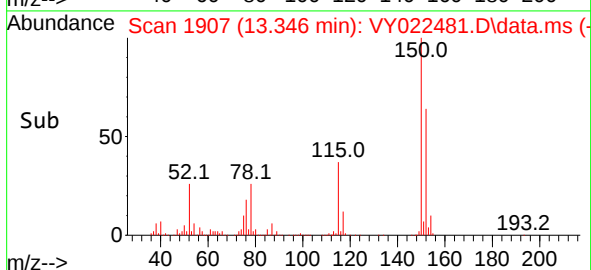
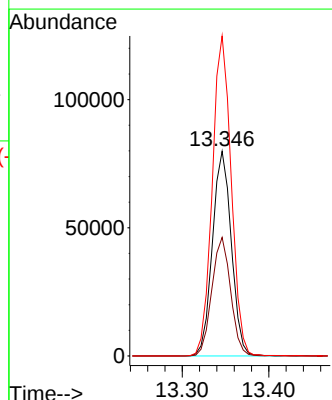





#76
1,2,3-Trichloropropane
Concen: 67.386 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.159 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15

Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-23

Tgt Ion: 75 Resp: 81732
Ion Ratio Lower Upper
75 100
77 1.3 0.0 0.0#

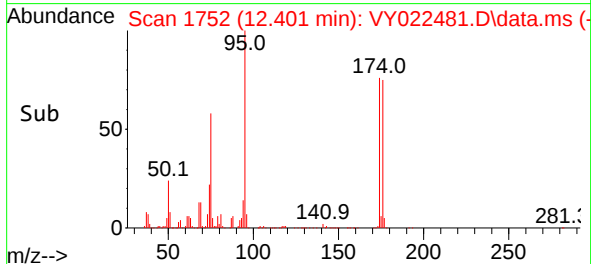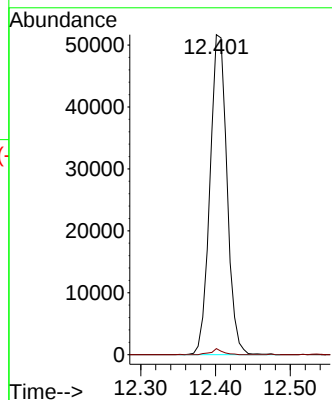

#81
trans-1,4-Dichloro-2-butene
Concen: 152.392 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. 0.097 min
Lab File: VY022481.D
Acq: 30 May 2025 16:15

Tgt Ion: 75 Resp: 81732
Ion Ratio Lower Upper
75 100
53 0.0 75.1 112.7#
89 0.1 37.4 56.0#

