

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY053025\
 Data File : VY022483.D
 Acq On : 30 May 2025 17:02
 Operator : SY/MD
 Sample : Q2173-14
 Misc : 5.09g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OR-400-CF-402B-VOC-25

Quant Time: May 31 02:30:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 28 10:34:06 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	270990	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	493166	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	396423	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	145554	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	156254	54.742	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	109.480%
35) Dibromofluoromethane	7.634	113	148102	51.280	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.560%
50) Toluene-d8	10.103	98	591788	50.264	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.520%
62) 4-Bromofluorobenzene	12.402	95	151727	42.604	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	85.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY053025\
Data File : VY022483.D
Acq On : 30 May 2025 17:02
Operator : SY/MD
Sample : Q2173-14
Misc : 5.09g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-25

Quant Time: May 31 02:30:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
Quant Title : SW846 8260
QLast Update : Wed May 28 10:34:06 2025
Response via : Initial Calibration




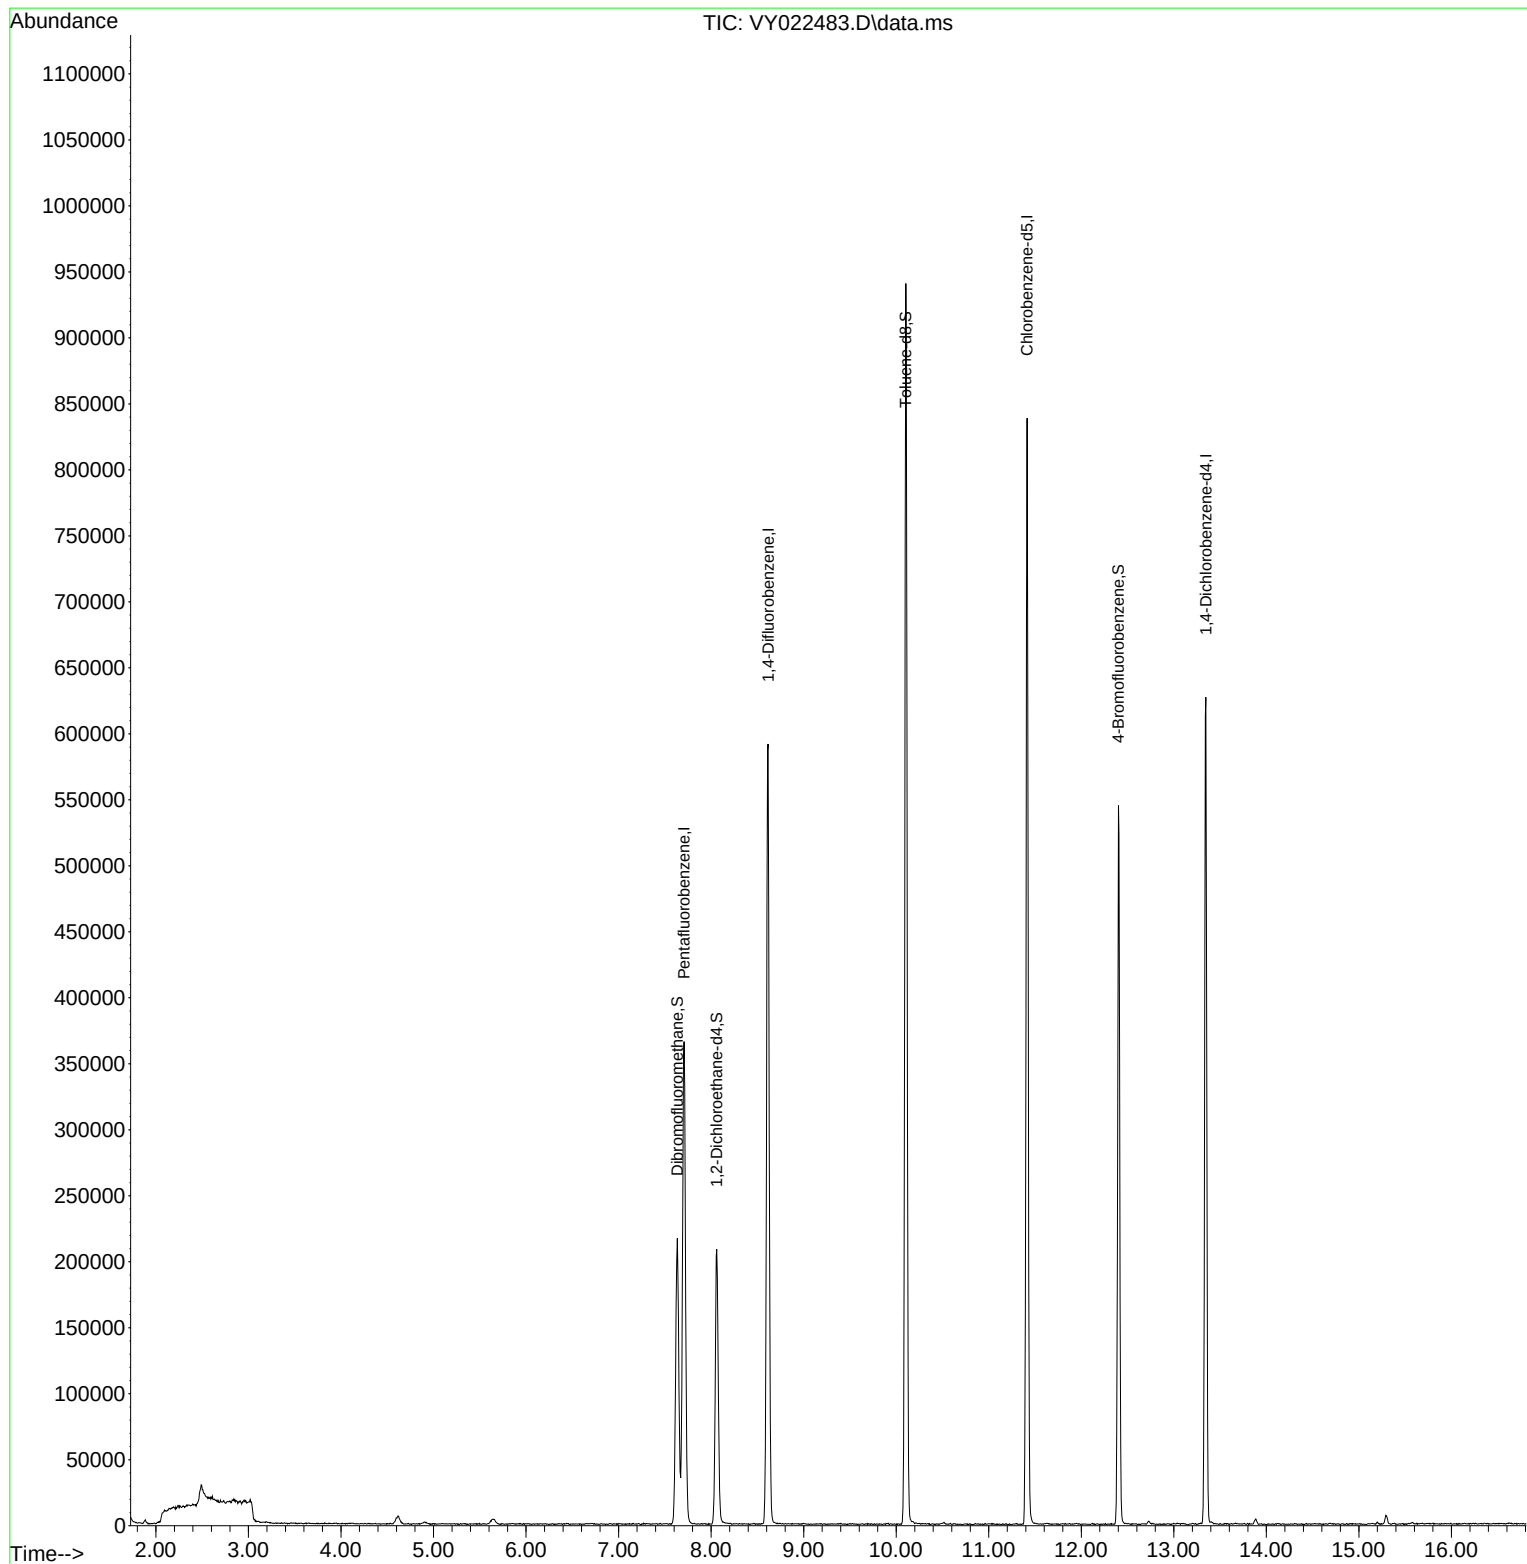


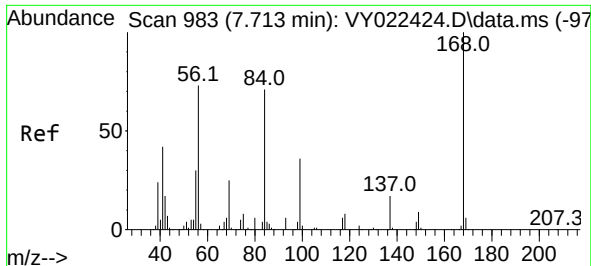

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02




Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-25


Tgt Ion:168 Resp: 270990
Ion Ratio Lower Upper
168 100
99 56.6 44.7 67.1

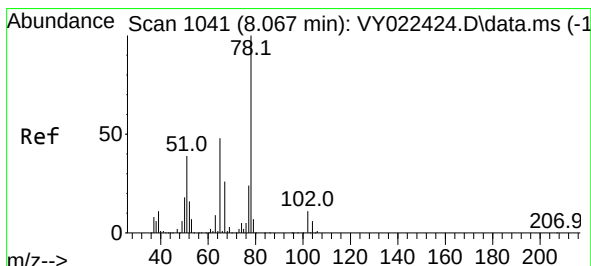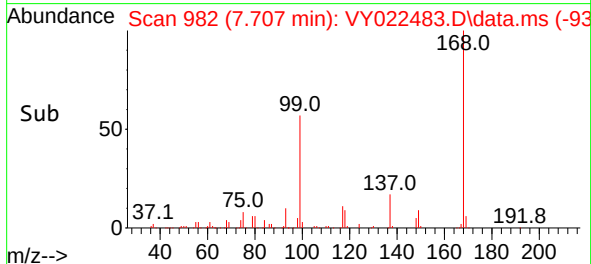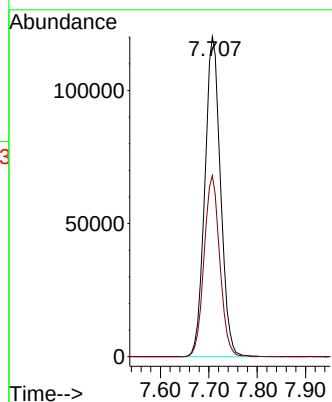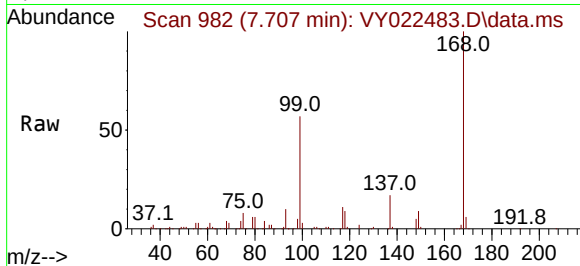

#33
1,2-Dichloroethane-d4
Concen: 54.742 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02


Tgt Ion: 65 Resp: 156254
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.4

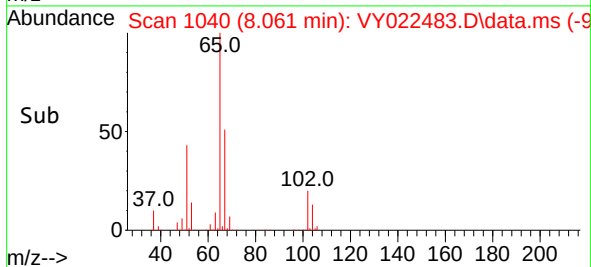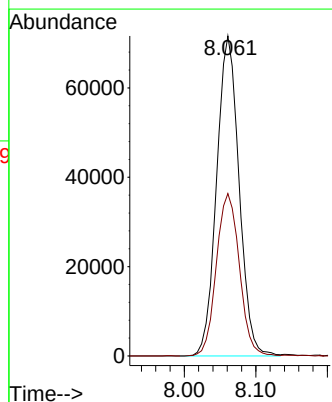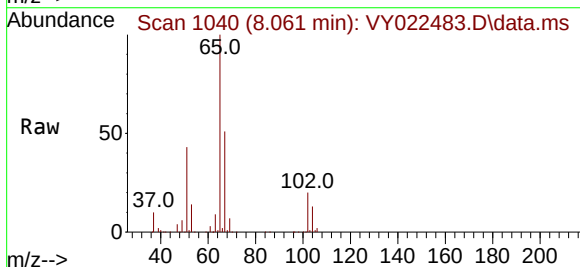



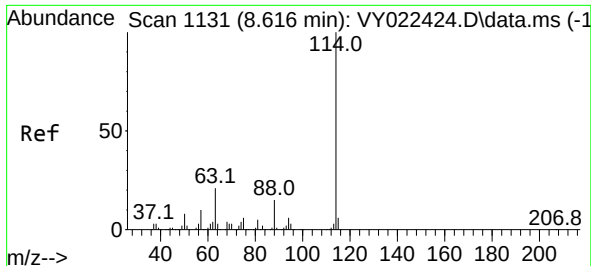


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02

Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-25



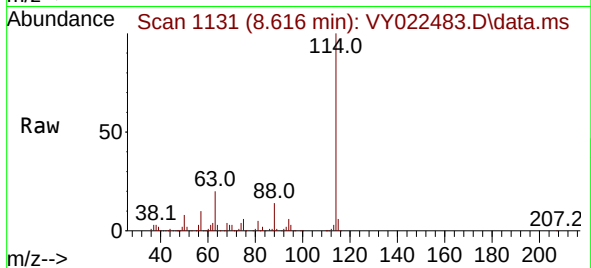



Tgt Ion:114 Resp: 493166
Ion Ratio Lower Upper
114 100
63 19.8 0.0 42.6
88 14.1 0.0 29.4

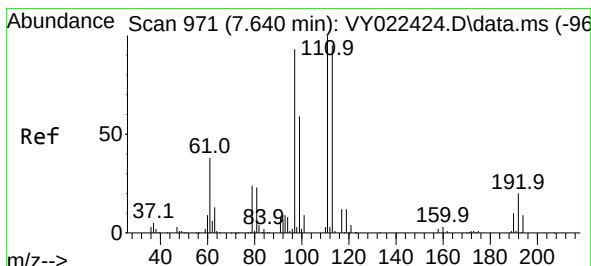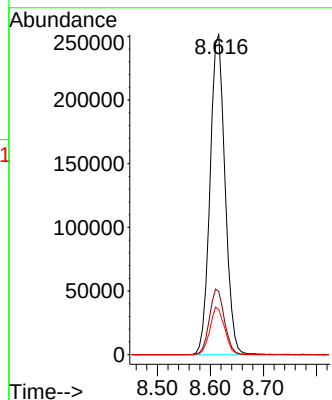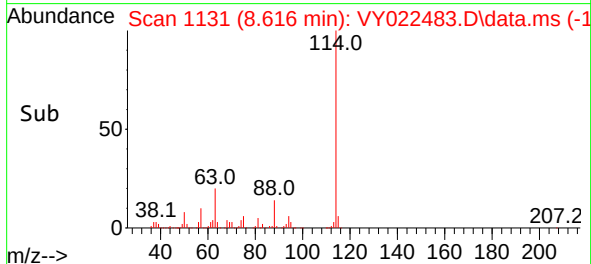

#35
Dibromofluoromethane
Concen: 51.280 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.006 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02

Tgt Ion:113 Resp: 148102
Ion Ratio Lower Upper
113 100
111 101.9 82.4 123.6
192 18.1 15.2 22.8


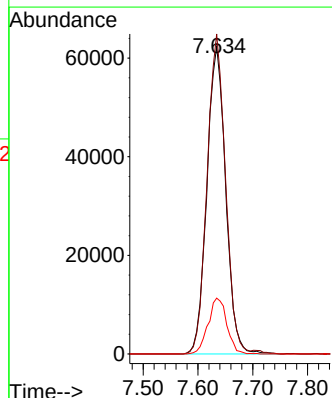
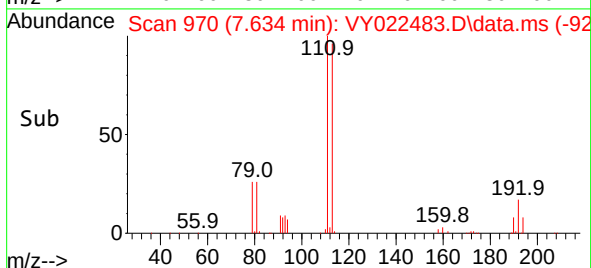
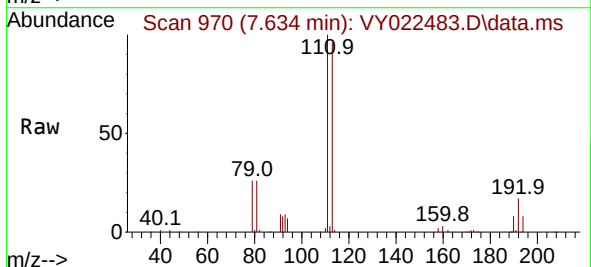


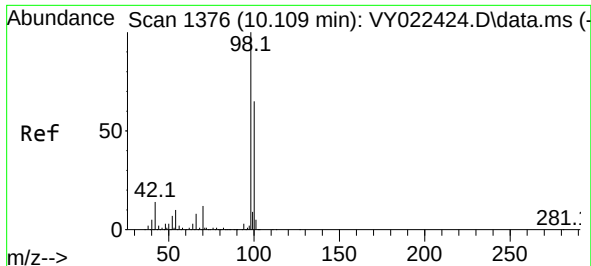

#50
Toluene-d8
Concen: 50.264 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02




Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-25


Tgt Ion: 98 Resp: 591788
Ion Ratio Lower Upper
98 100
100 63.9 52.2 78.2

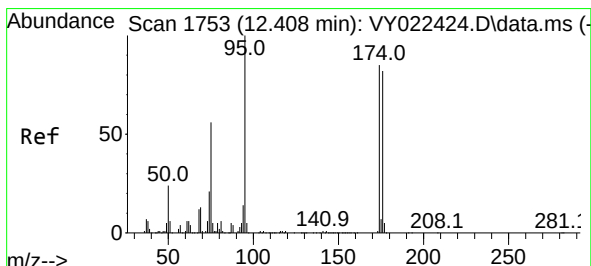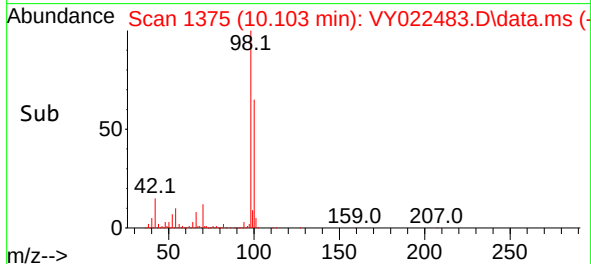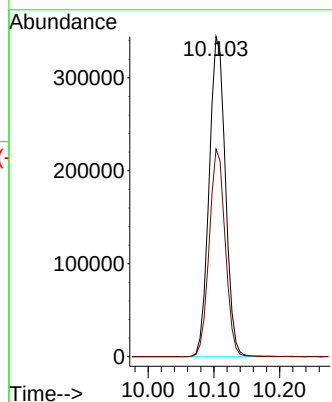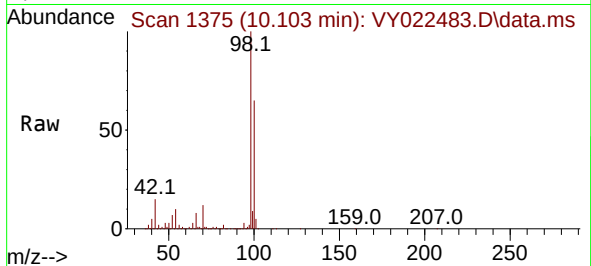

#62
4-Bromofluorobenzene
Concen: 42.604 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. -0.006 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02

Tgt Ion: 95 Resp: 151727
Ion Ratio Lower Upper
95 100
174 86.1 0.0 171.6
176 81.8 0.0 164.6


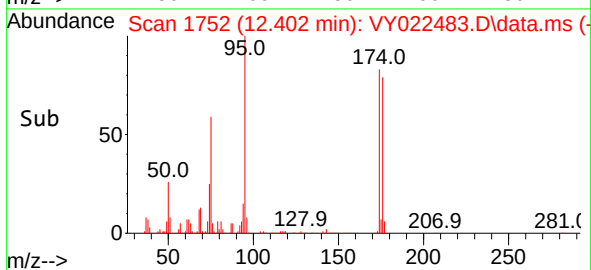
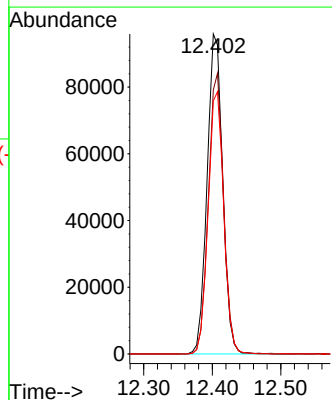
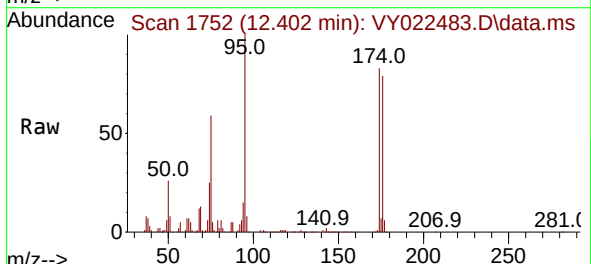


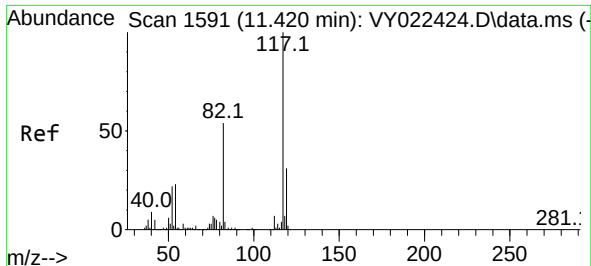

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02

Instrument :
MSVOA_Y
ClientSampleId :
OR-400-CF-402B-VOC-25

Tgt Ion:117 Resp: 396423
Ion Ratio Lower Upper
117 100
82 55.5 43.3 64.9
119 31.1 24.5 36.7

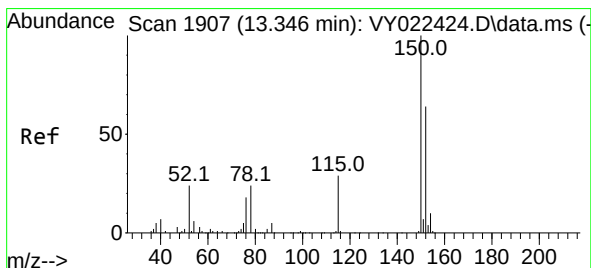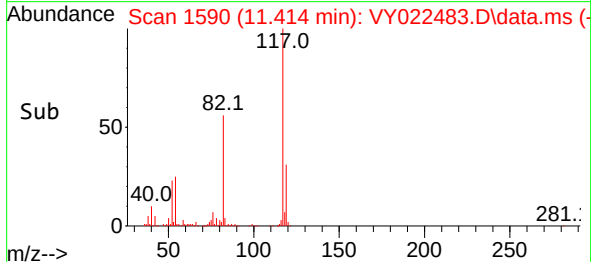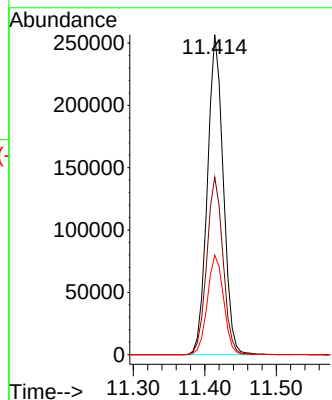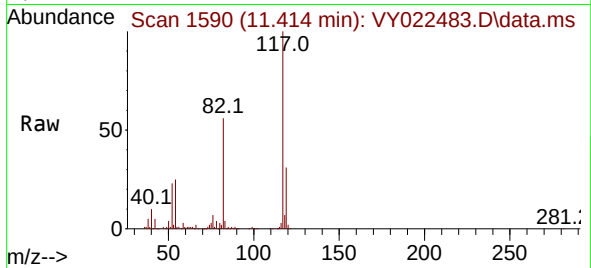

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY022483.D
Acq: 30 May 2025 17:02

Tgt Ion:152 Resp: 145554
Ion Ratio Lower Upper
152 100
115 57.4 28.4 85.3
150 159.2 0.0 345.8

