
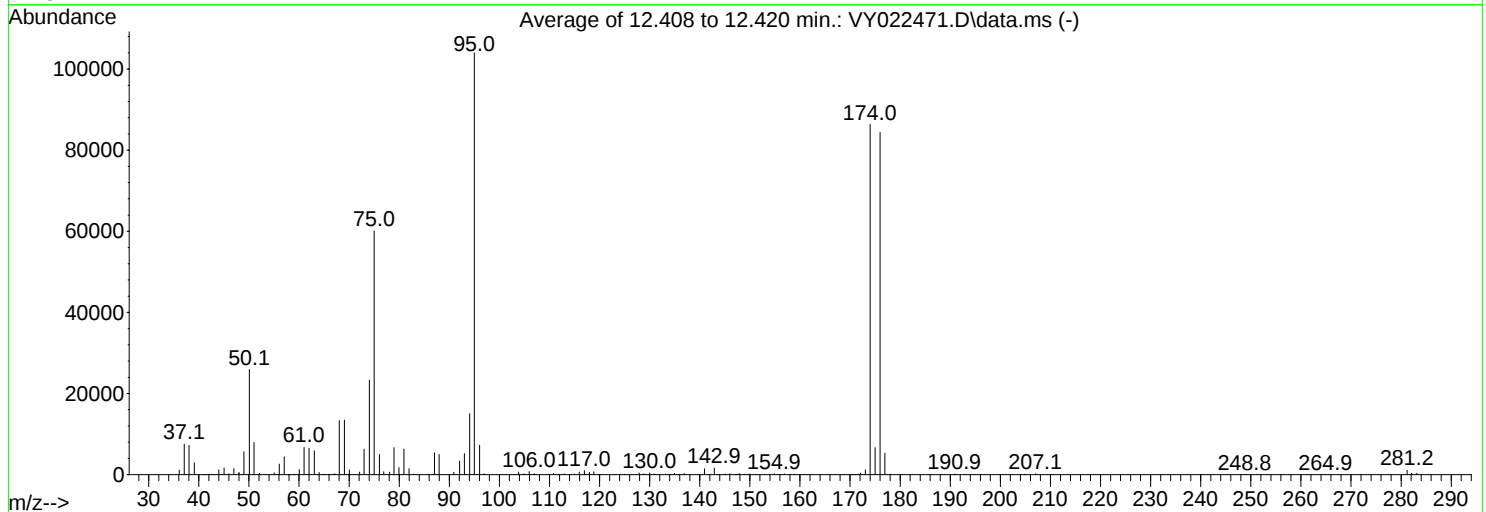


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY053025\
Data File : VY022471.D
Acq On : 30 May 2025 07:54
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
Title : SW846 8260
Last Update : Wed May 28 10:34:06 2025

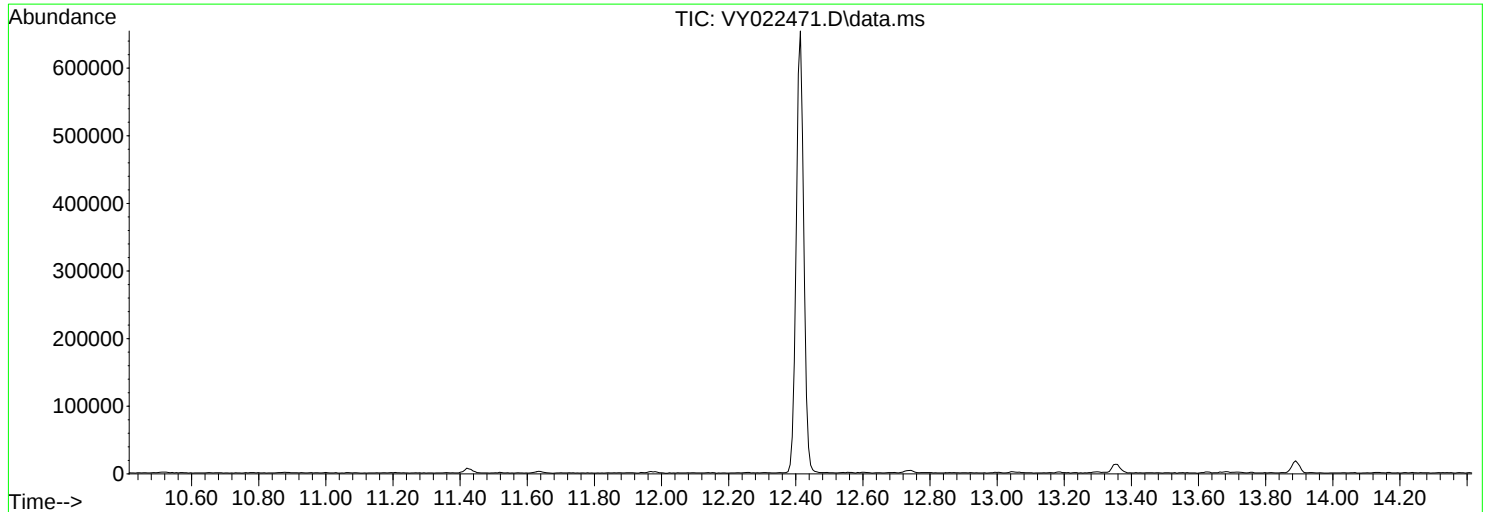

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	25928	PASS
75	95	30	60	57.8	60075	PASS
95	95	100	100	100.0	104000	PASS
96	95	5	9	7.0	7276	PASS
173	174	0.00	2	1.4	1187	PASS
174	95	50	100	83.0	86352	PASS
175	174	5	9	7.7	6672	PASS
176	174	95	101	97.7	84392	PASS
177	176	5	9	6.3	5296	PASS