

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060324\
 Data File : VY018441.D
 Acq On : 03 Jun 2024 15:25
 Operator : SY/MD
 Sample : P2662-03
 Misc : 6.04g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WCS-TPR-VOC

Quant Time: Jun 04 05:42:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060324S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 04 05:38:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	95188	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.679	114	188525	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	168092	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	60129	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	55553	29.718	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	59.440%
35) Dibromofluoromethane	7.710	113	56881	23.793	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	47.580%#
50) Toluene-d8	10.173	98	225984	23.761	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	47.520%#
62) 4-Bromofluorobenzene	12.477	95	66934	22.604	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	45.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060324\
Data File : VY018441.D
Acq On : 03 Jun 2024 15:25
Operator : SY/MD
Sample : P2662-03
Misc : 6.04g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WCS-TPR-VOC

Quant Time: Jun 04 05:42:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060324S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 04 05:38:21 2024
Response via : Initial Calibration




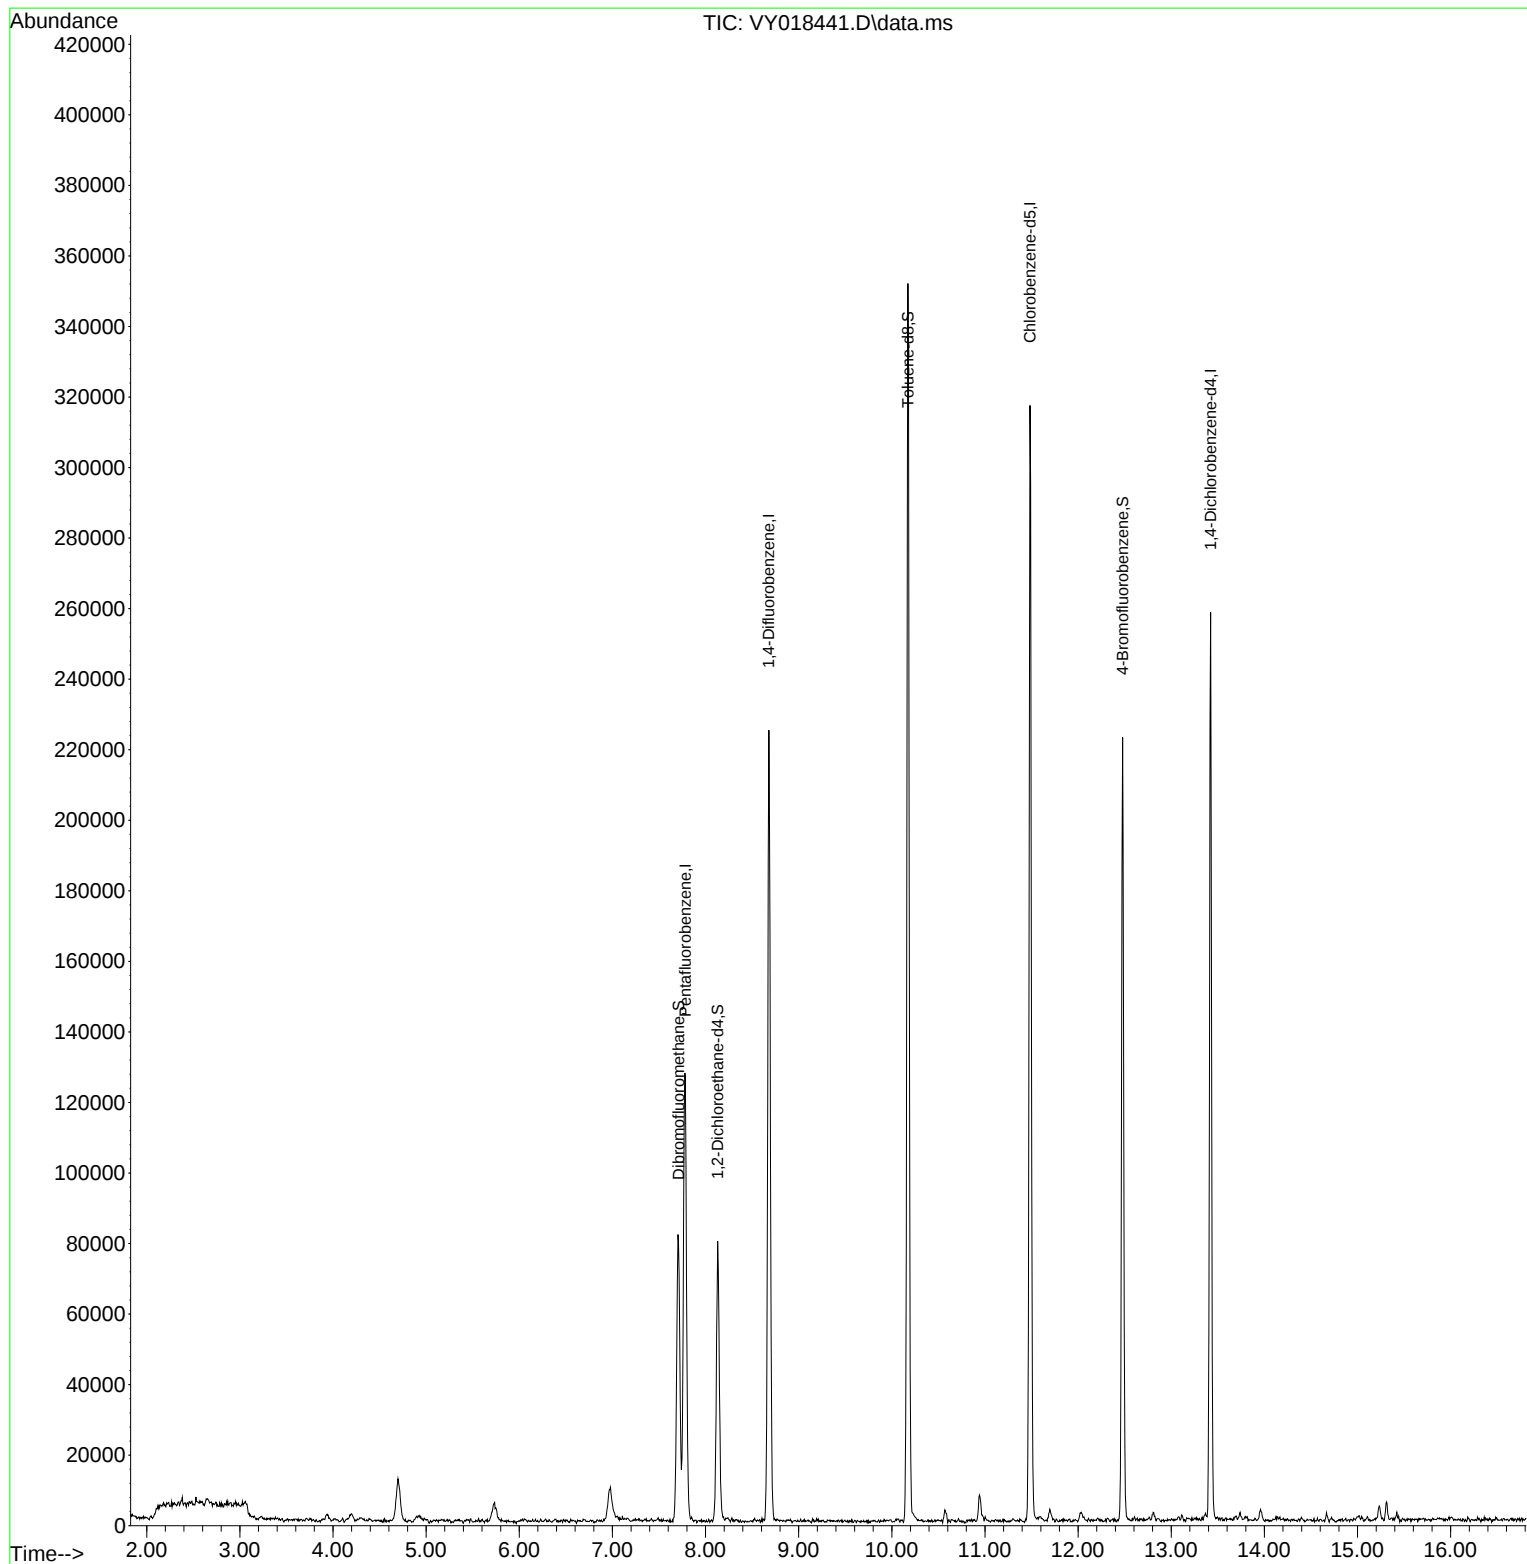


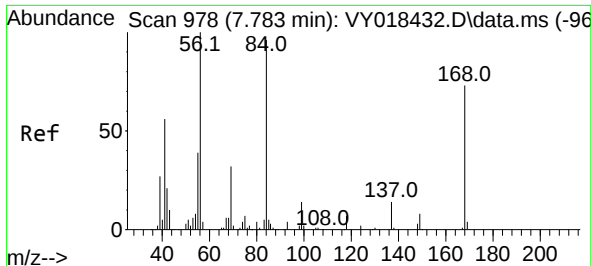

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY018441.D
Acq: 03 Jun 2024 15:25




Instrument :
MSVOA_Y
ClientSampleId :
WCS-TPR-VOC


Tgt Ion:168 Resp: 95188
Ion Ratio Lower Upper
168 100
99 57.1 39.1 58.7

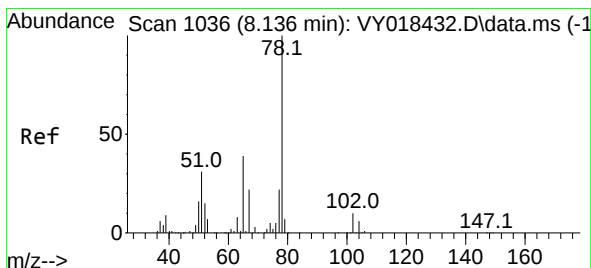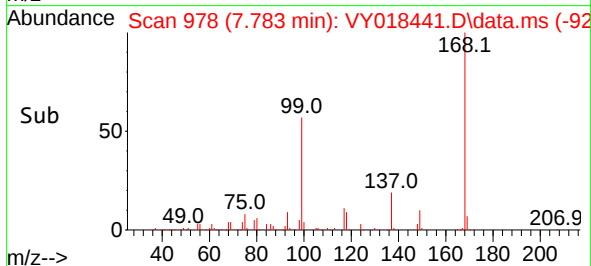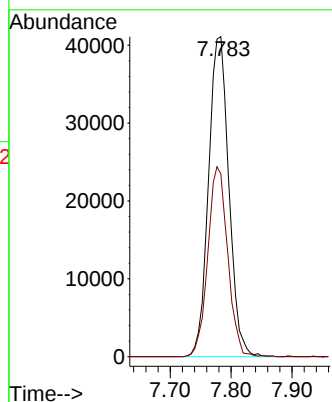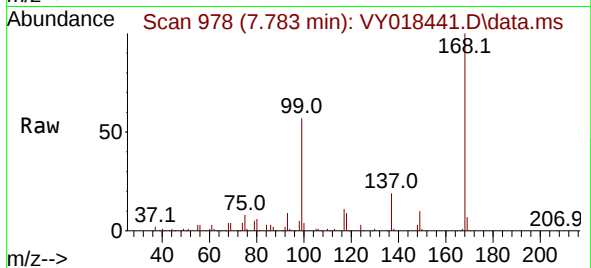

#33
1,2-Dichloroethane-d4
Concen: 29.718 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY018441.D
Acq: 03 Jun 2024 15:25

Tgt Ion: 65 Resp: 55553
Ion Ratio Lower Upper
65 100
67 55.0 0.0 109.6

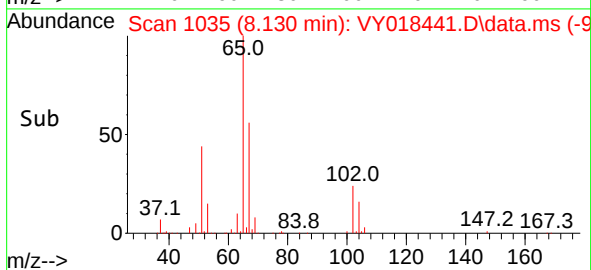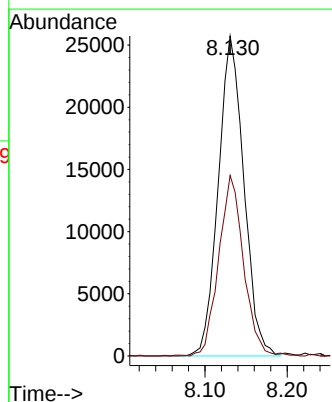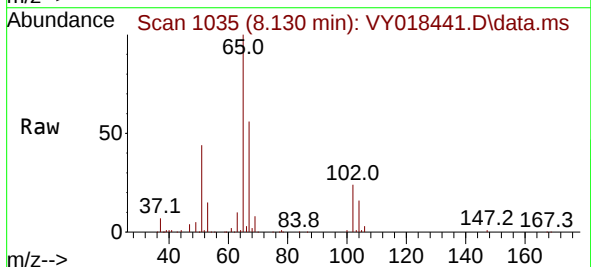

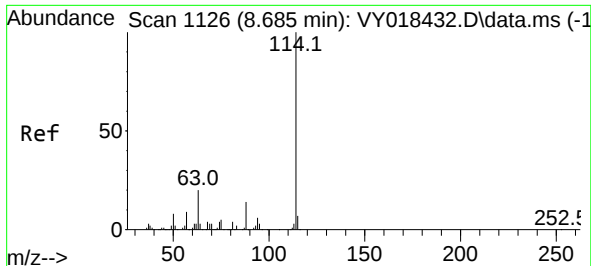

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.679 min Scan# 1125

Delta R.T. -0.006 min

Lab File: VY018441.D

Acq: 03 Jun 2024 15:25

Instrument :

MSVOA_Y

ClientSampleId :

WCS-TPR-VOC





Tgt Ion:114 Resp: 188525

Ion Ratio Lower Upper

114 100

63 19.9 0.0 35.0

88 15.4 0.0 27.2

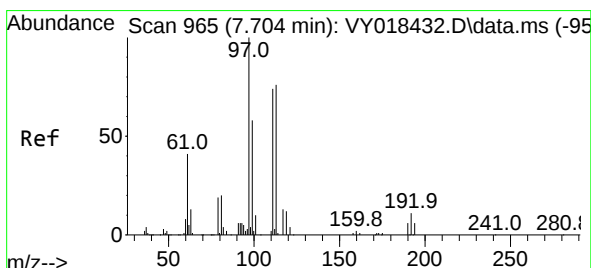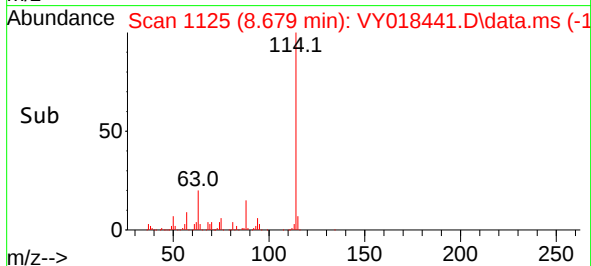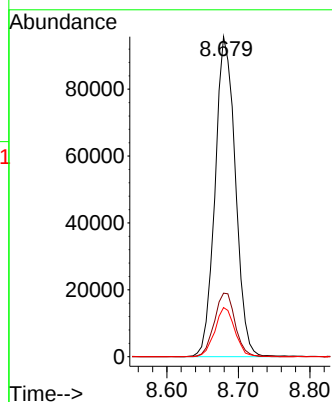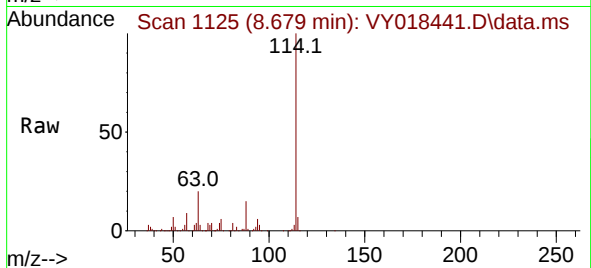

#35

Dibromofluoromethane

Concen: 23.793 ug/l

RT: 7.710 min Scan# 966

Delta R.T. 0.006 min

Lab File: VY018441.D

Acq: 03 Jun 2024 15:25




Tgt Ion:113 Resp: 56881


Ion Ratio Lower Upper

113 100

111 104.1 82.2 123.4

192 17.2 15.9 23.9


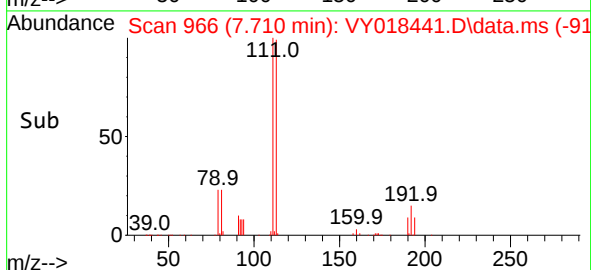
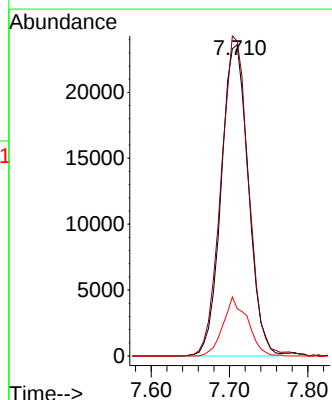
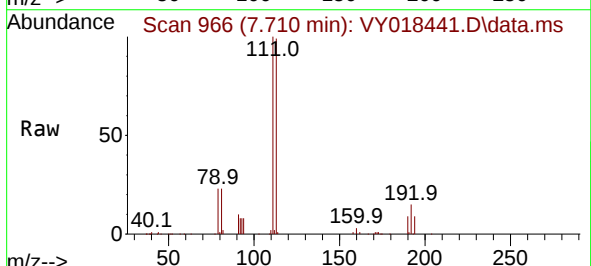


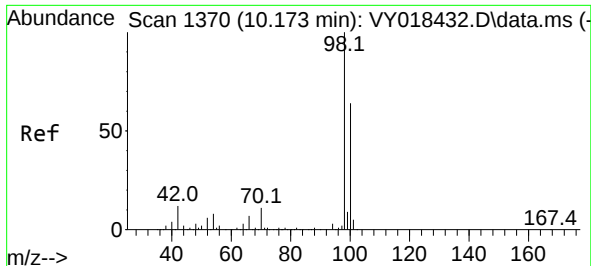

#50
Toluene-d8
Concen: 23.761 ug/l
RT: 10.173 min Scan# 1370
Delta R.T. 0.000 min
Lab File: VY018441.D
Acq: 03 Jun 2024 15:25




Instrument :
MSVOA_Y
ClientSampleId :
WCS-TPR-VOC


Tgt Ion: 98 Resp: 225984
Ion Ratio Lower Upper
98 100
100 65.8 52.0 78.0

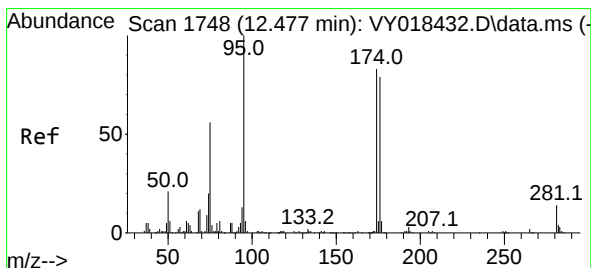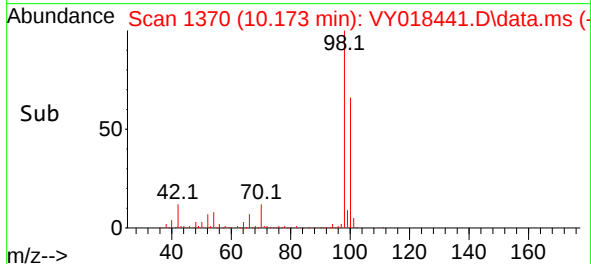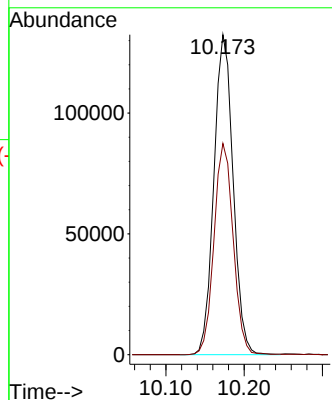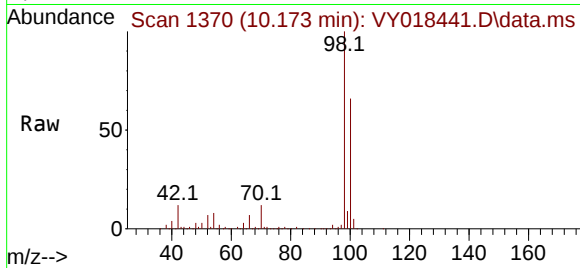

#62
4-Bromofluorobenzene
Concen: 22.604 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY018441.D
Acq: 03 Jun 2024 15:25

Tgt Ion: 95 Resp: 66934
Ion Ratio Lower Upper
95 100
174 78.3 0.0 175.6
176 73.9 0.0 171.4

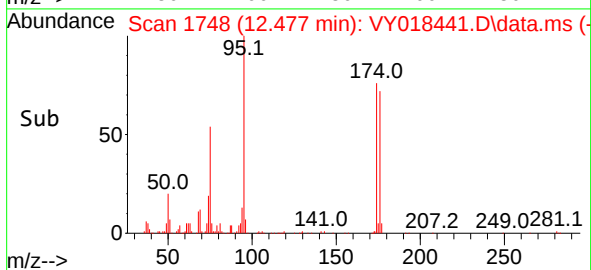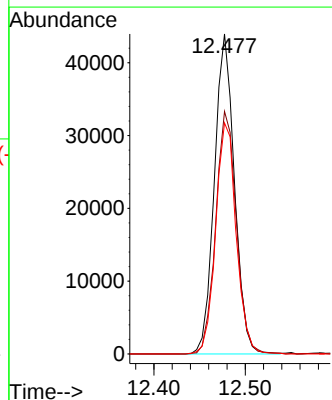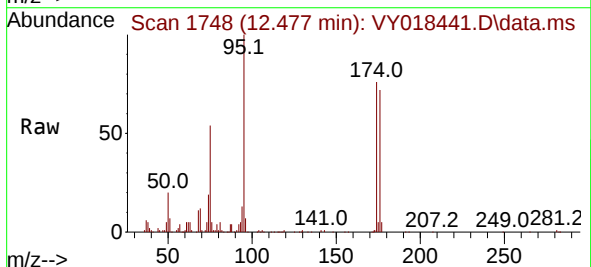

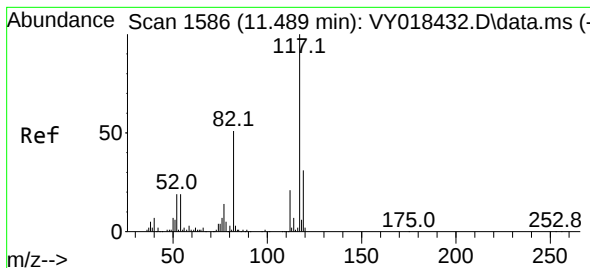

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.483 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY018441.D

Acq: 03 Jun 2024 15:25

Instrument :

MSVOA_Y

ClientSampleId :

WCS-TPR-VOC





Tgt Ion:117 Resp: 168092

Ion Ratio Lower Upper

117 100

82 56.1 42.4 63.6

119 30.7 25.9 38.9

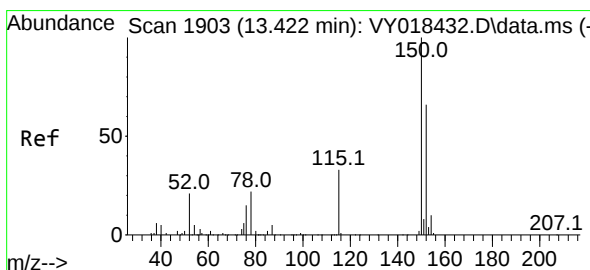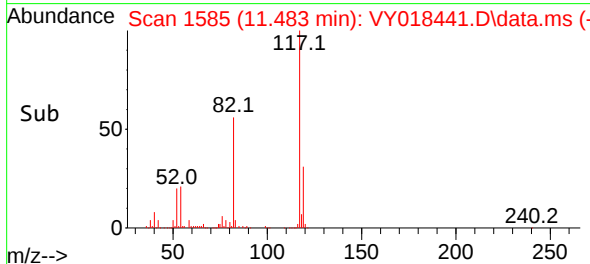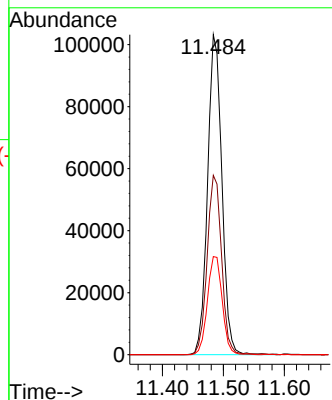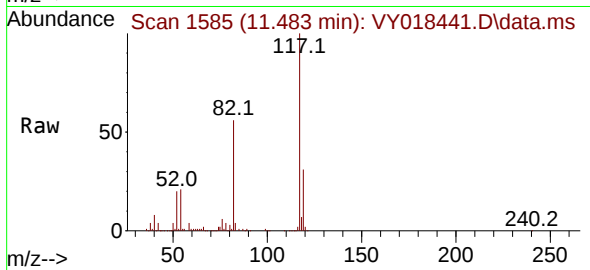

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY018441.D

Acq: 03 Jun 2024 15:25

Tgt Ion:152 Resp: 60129

Ion Ratio Lower Upper

152 100

115 60.4 28.2 84.7

150 157.1 0.0 345.6

