

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060325\
 Data File : VY022526.D
 Acq On : 03 Jun 2025 16:35
 Operator : SY/MD
 Sample : Q2176-01
 Misc : 7.12g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-46

Quant Time: Jun 04 04:15:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 03 03:22:04 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	268876	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	504814	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.413	117	411331	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	154553	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.060	65	155741	51.789	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.580%
35) Dibromofluoromethane	7.634	113	151120	50.154	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.300%
50) Toluene-d8	10.103	98	603269	49.550	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.100%
62) 4-Bromofluorobenzene	12.401	95	156250	43.073	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	86.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060325\
Data File : VY022526.D
Acq On : 03 Jun 2025 16:35
Operator : SY/MD
Sample : Q2176-01
Misc : 7.12g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-46

Quant Time: Jun 04 04:15:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 03 03:22:04 2025
Response via : Initial Calibration




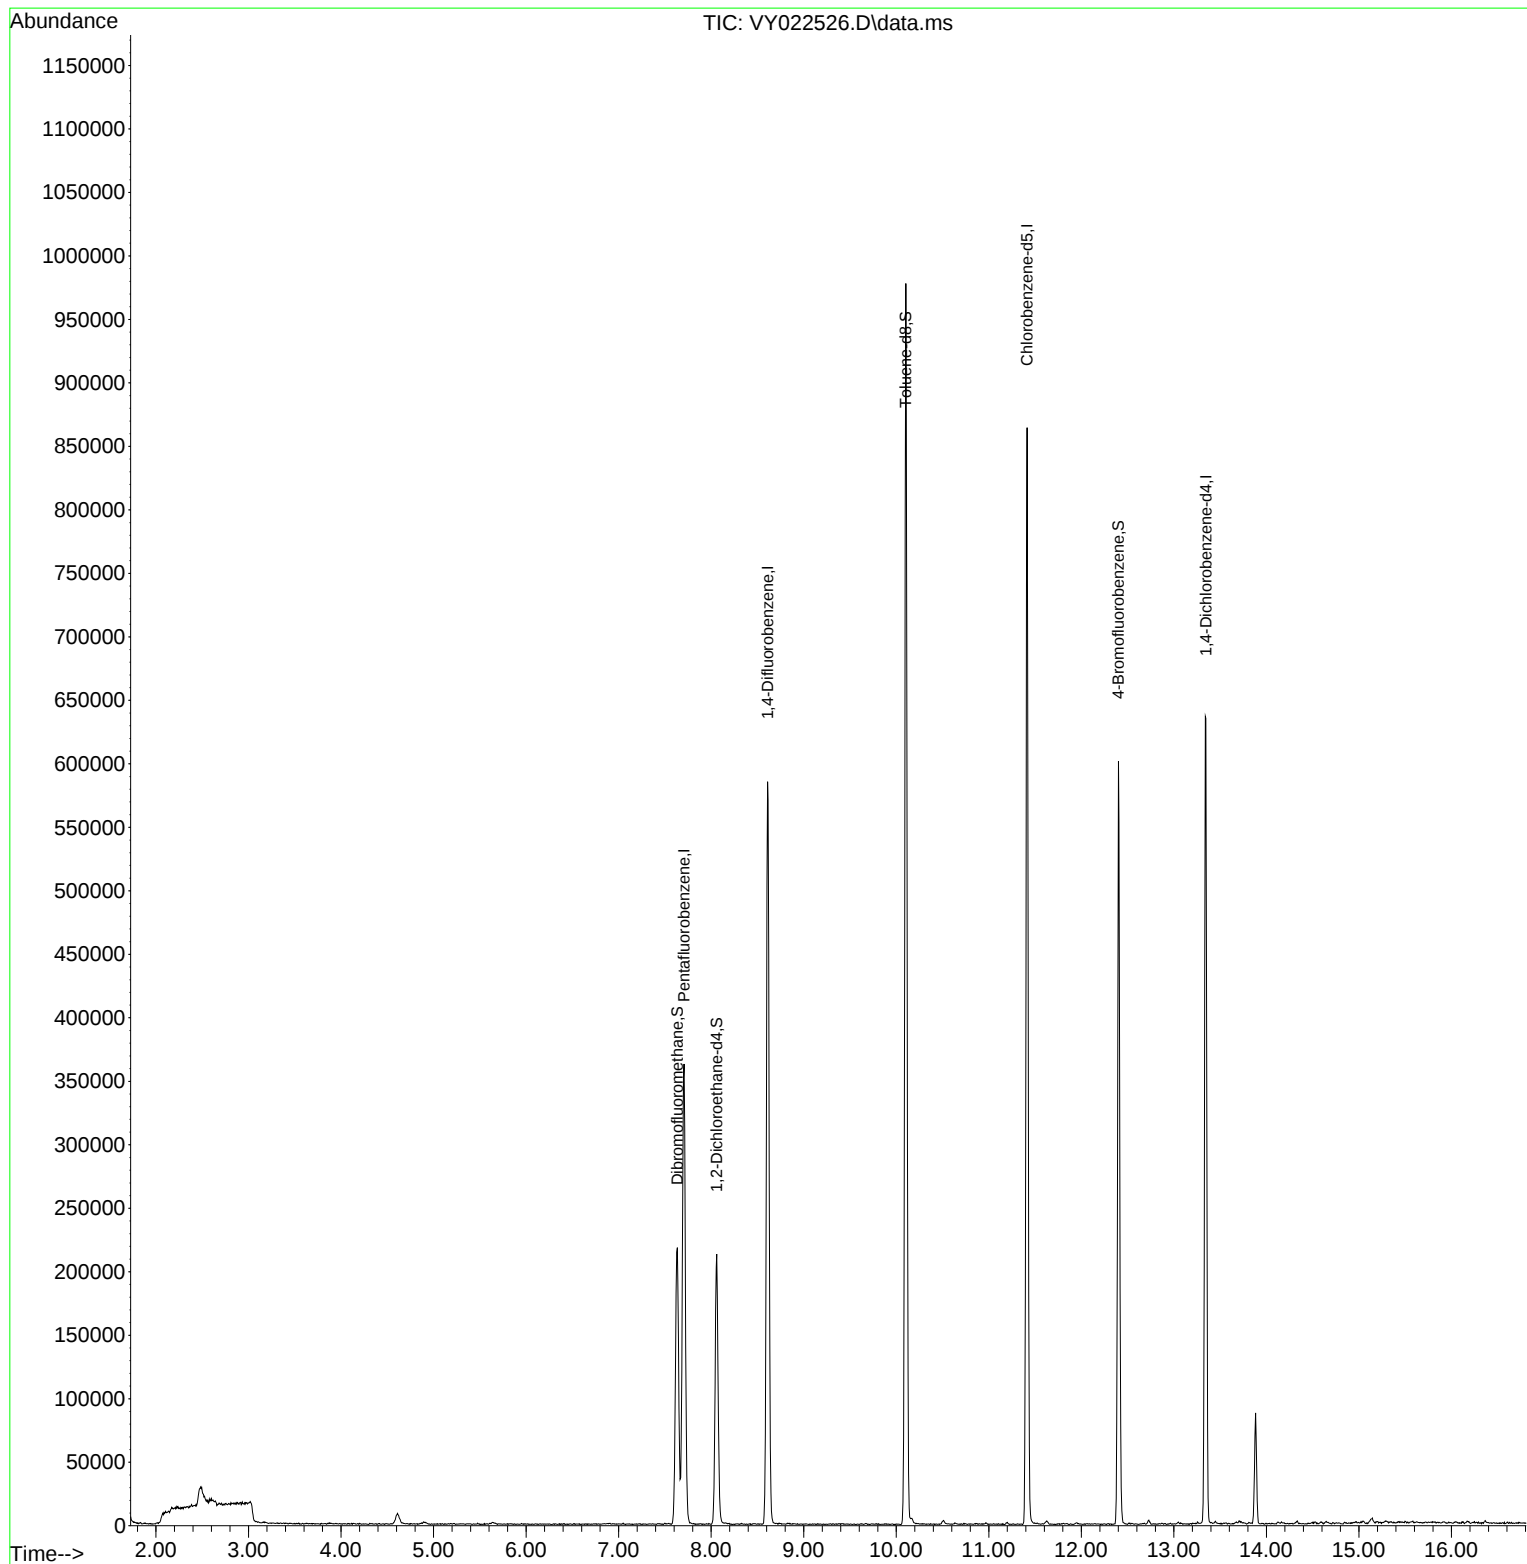


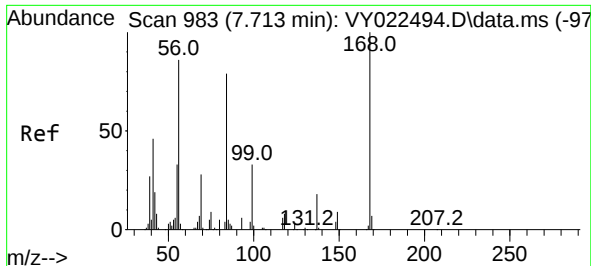

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022526.D
Acq: 03 Jun 2025 16:35




Instrument :
MSVOA_Y
ClientSampleId :
TP-46

Tgt Ion:168 Resp: 268876
Ion Ratio Lower Upper
168 100
99 54.0 44.3 66.5

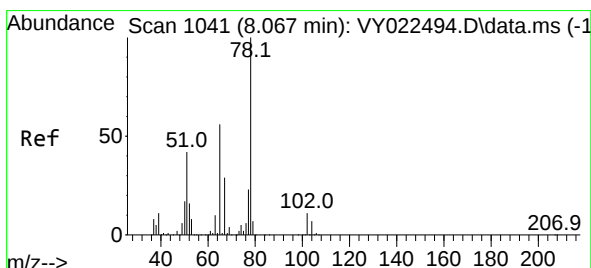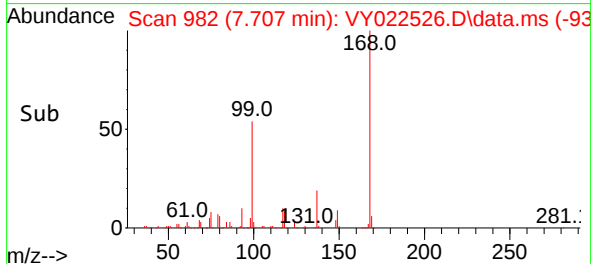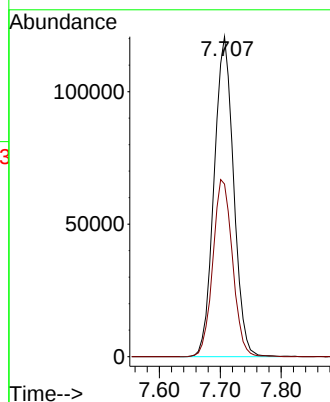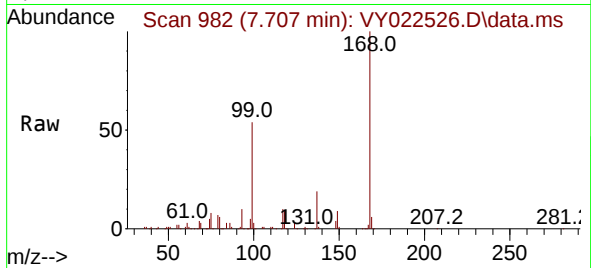

#33
1,2-Dichloroethane-d4
Concen: 51.789 ug/l
RT: 8.060 min Scan# 1040
Delta R.T. -0.007 min
Lab File: VY022526.D
Acq: 03 Jun 2025 16:35

Tgt Ion: 65 Resp: 155741
Ion Ratio Lower Upper
65 100
67 52.5 0.0 103.4

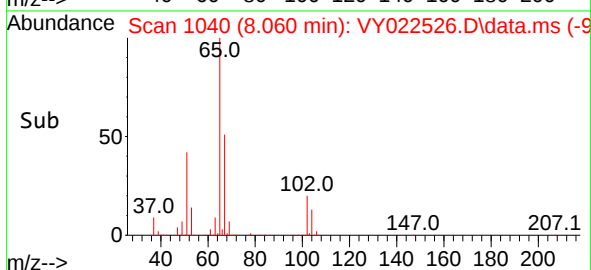
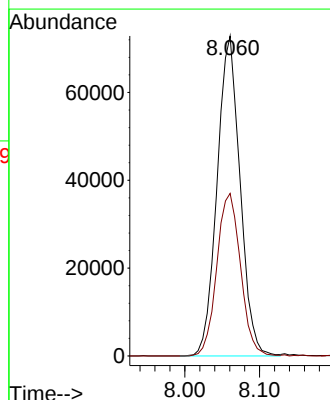
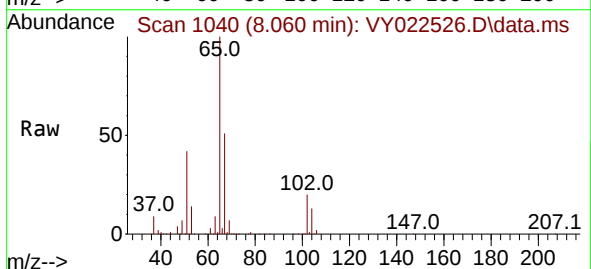




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.609 min Scan# 1131
Delta R.T. -0.007 min
Lab File: VY022526.D
Acq: 03 Jun 2025 16:35




Instrument :
MSVOA_Y
ClientSampleId :
TP-46


Tgt Ion:114 Resp: 504814
Ion Ratio Lower Upper
114 100
63 20.3 0.0 40.8
88 13.8 0.0 27.8

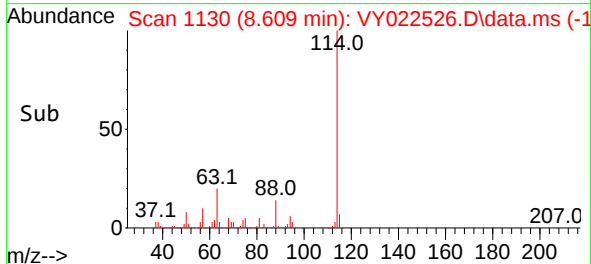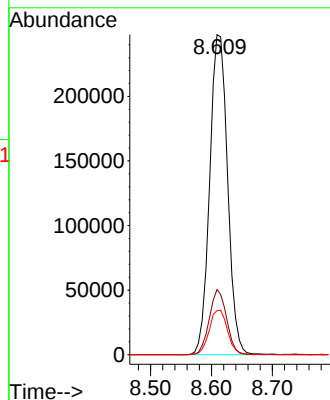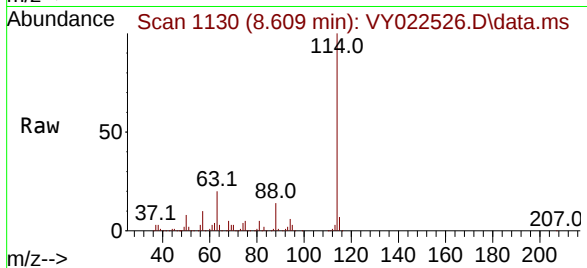

#35
Dibromofluoromethane
Concen: 50.154 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.007 min
Lab File: VY022526.D
Acq: 03 Jun 2025 16:35

Tgt Ion:113 Resp: 151120
Ion Ratio Lower Upper
113 100
111 103.8 81.1 121.7
192 18.2 14.2 21.2


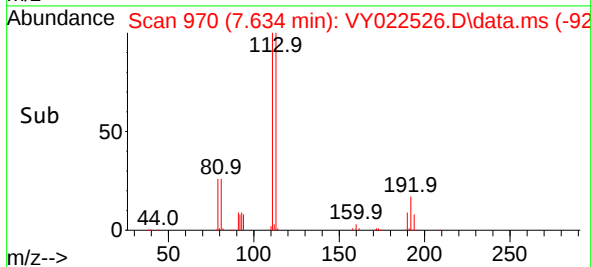
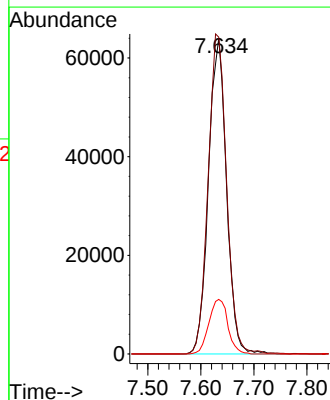
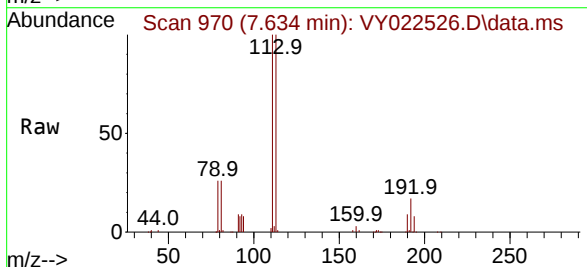


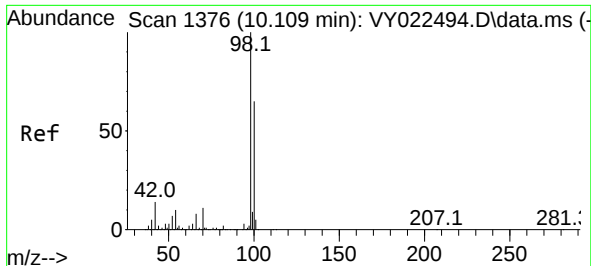

#50
Toluene-d8
Concen: 49.550 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.007 min
Lab File: VY022526.D
Acq: 03 Jun 2025 16:35




Instrument :
MSVOA_Y
ClientSampleId :
TP-46


Tgt Ion: 98 Resp: 603269
Ion Ratio Lower Upper
98 100
100 64.6 51.4 77.0

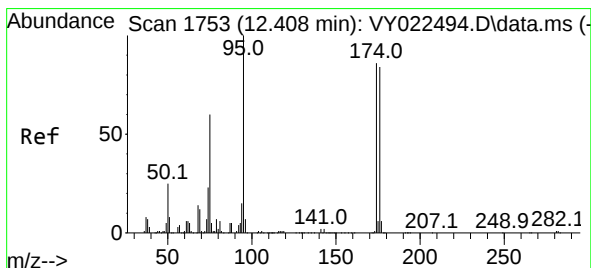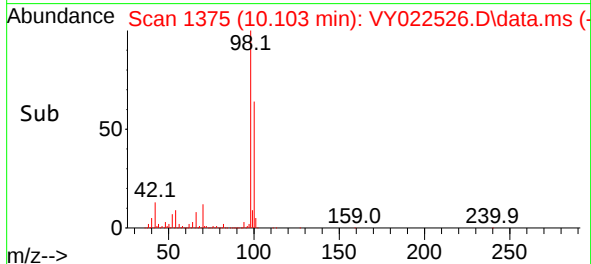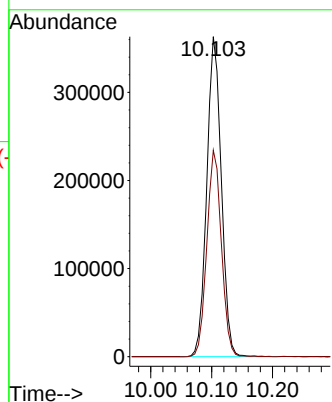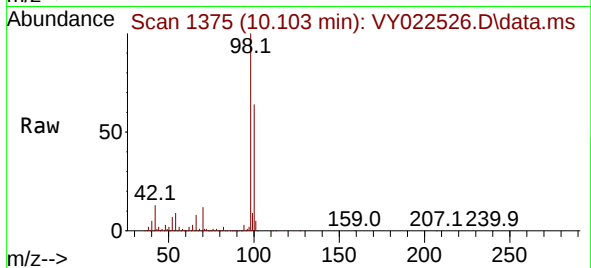

#62
4-Bromofluorobenzene
Concen: 43.073 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.007 min
Lab File: VY022526.D
Acq: 03 Jun 2025 16:35

Tgt Ion: 95 Resp: 156250
Ion Ratio Lower Upper
95 100
174 86.6 0.0 170.0
176 82.8 0.0 166.2

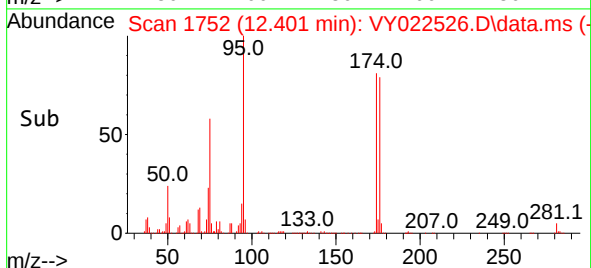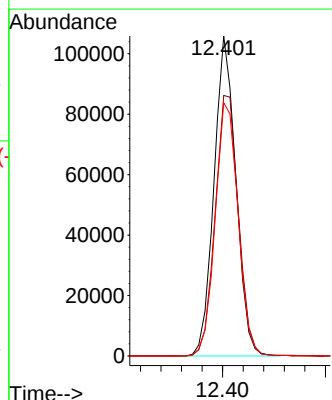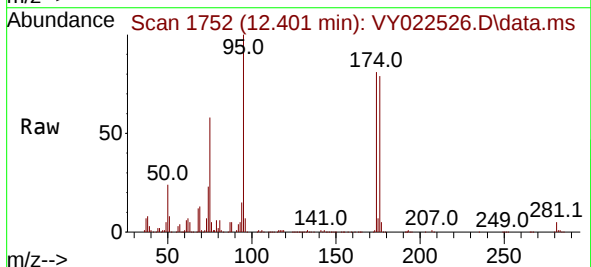

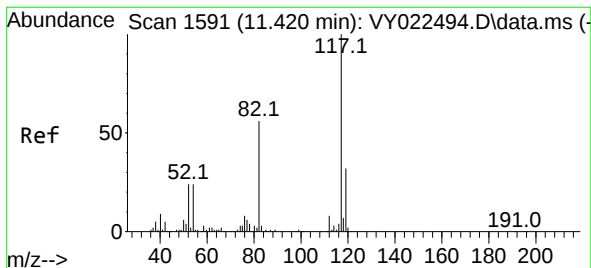

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.413 min Scan# 1

Delta R.T. -0.007 min

Lab File: VY022526.D

Acq: 03 Jun 2025 16:35

Instrument :

MSVOA_Y

ClientSampleId :

TP-46





Tgt Ion:117 Resp: 411331

Ion Ratio Lower Upper

117 100

82 55.8 44.6 66.8

119 31.9 25.4 38.0

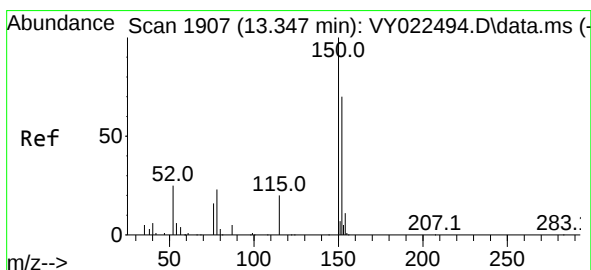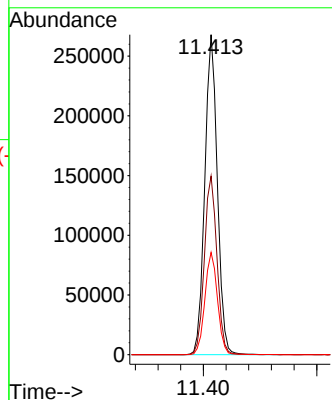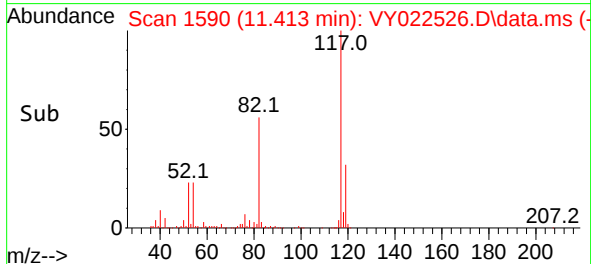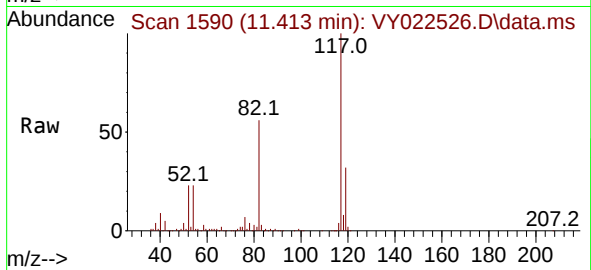

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.001 min

Lab File: VY022526.D

Acq: 03 Jun 2025 16:35

Tgt Ion:152 Resp: 154553

Ion Ratio Lower Upper

152 100

115 57.2 28.9 86.7

150 156.7 0.0 349.6

