
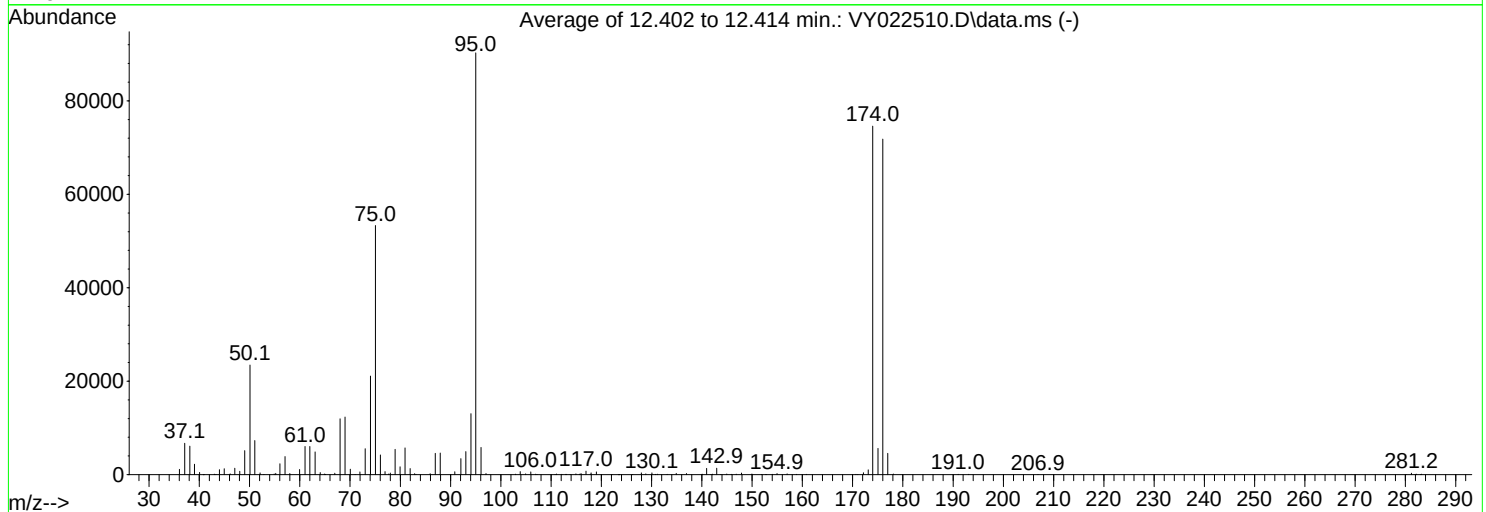


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060325\
Data File : VY022510.D
Acq On : 03 Jun 2025 09:03
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Title : SW846 8260
Last Update : Tue Jun 03 03:22:04 2025

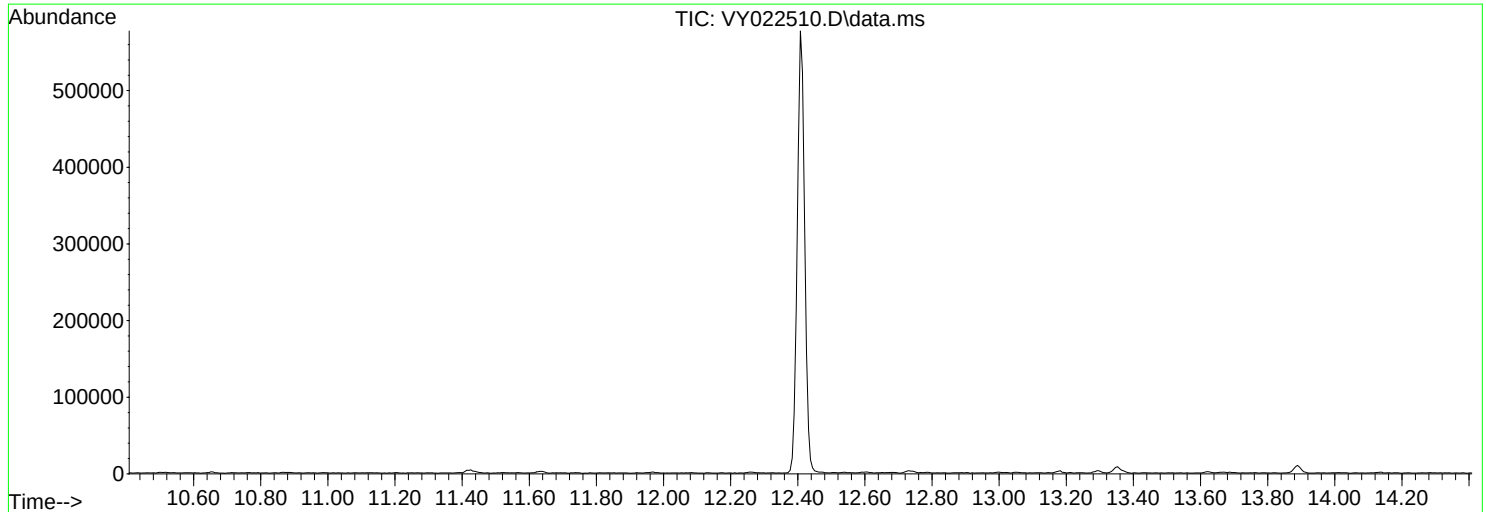

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.0	23445	PASS
75	95	30	60	59.1	53331	PASS
95	95	100	100	100.0	90275	PASS
96	95	5	9	6.5	5832	PASS
173	174	0.00	2	1.4	1029	PASS
174	95	50	100	82.6	74597	PASS
175	174	5	9	7.6	5633	PASS
176	174	95	101	96.3	71808	PASS
177	176	5	9	6.3	4541	PASS