


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060625\
Data File : VY022586.D
Acq On : 06 Jun 2025 08:27
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Title : SW846 8260
Last Update : Tue Jun 03 03:22:04 2025

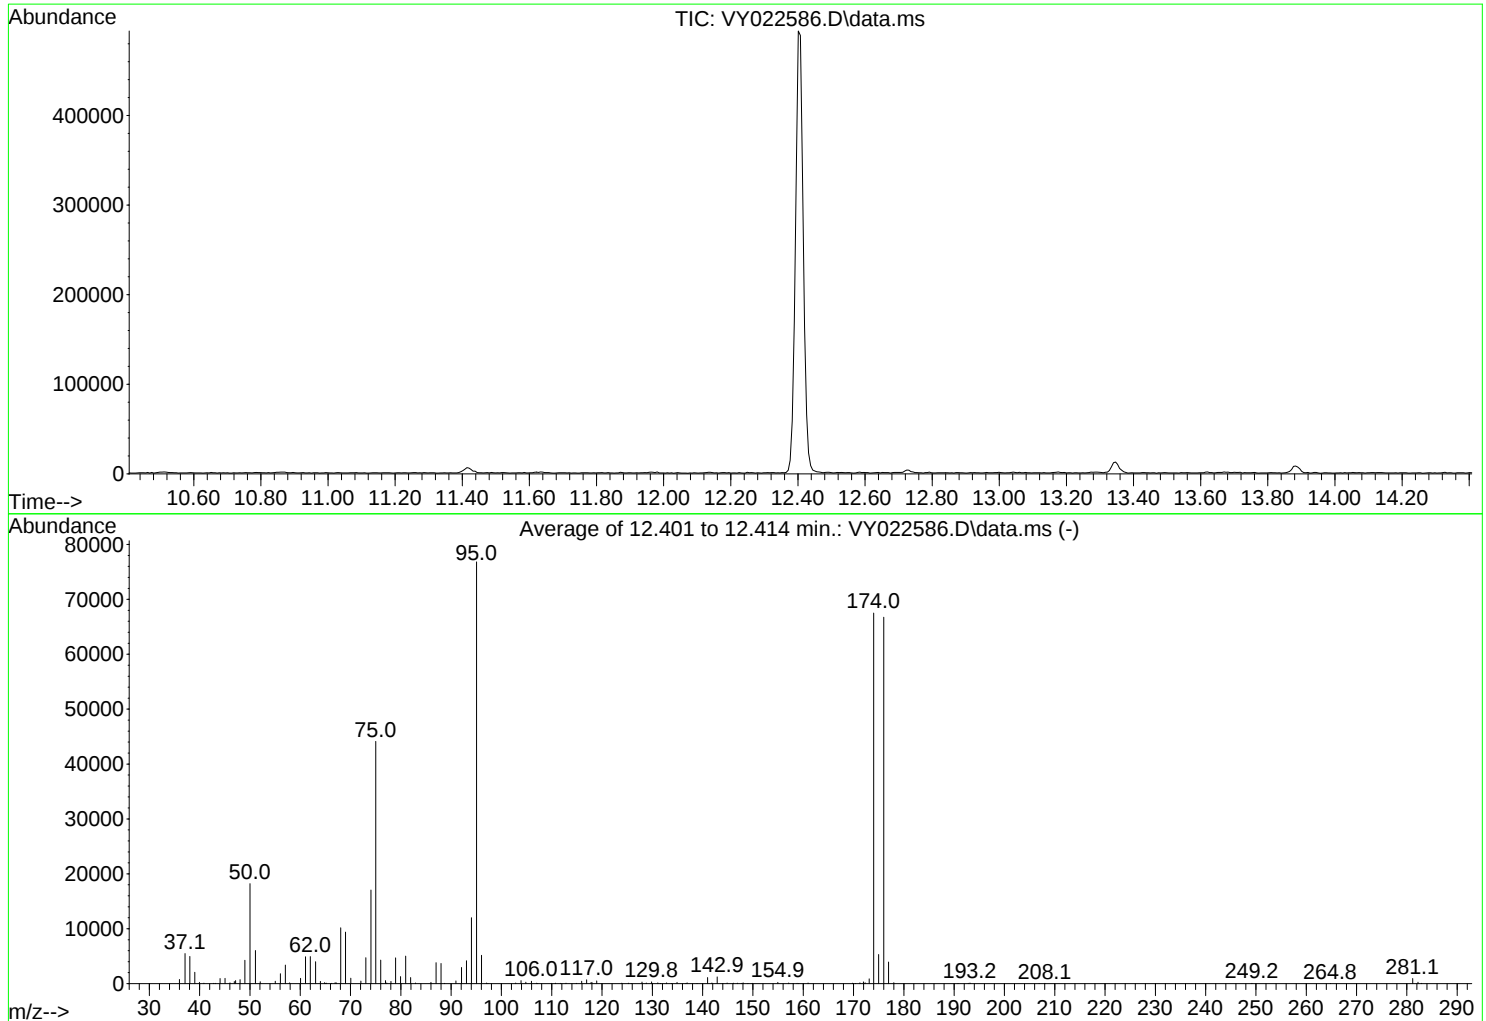

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	18221	PASS
75	95	30	60	57.4	44123	PASS
95	95	100	100	100.0	76832	PASS
96	95	5	9	6.7	5164	PASS
173	174	0.00	2	1.3	876	PASS
174	95	50	100	87.8	67488	PASS
175	174	5	9	7.9	5302	PASS
176	174	95	101	98.9	66739	PASS
177	176	5	9	5.9	3940	PASS