
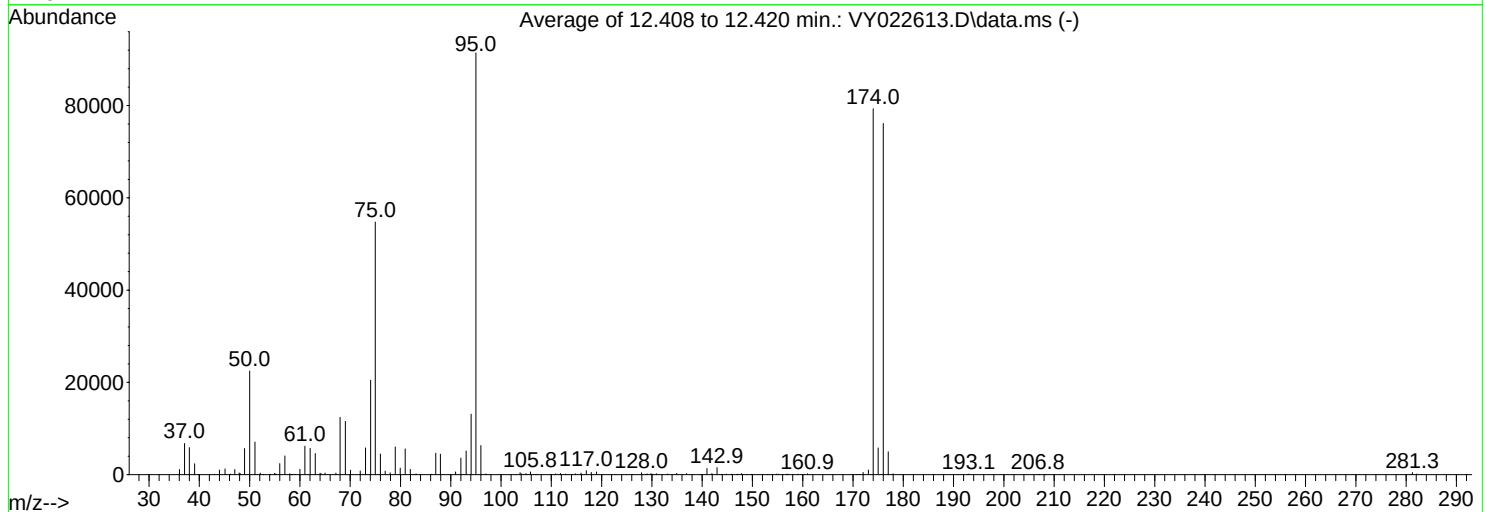


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060925\
Data File : VY022613.D
Acq On : 09 Jun 2025 07:54
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Title : SW846 8260
Last Update : Tue Jun 10 15:26:14 2025

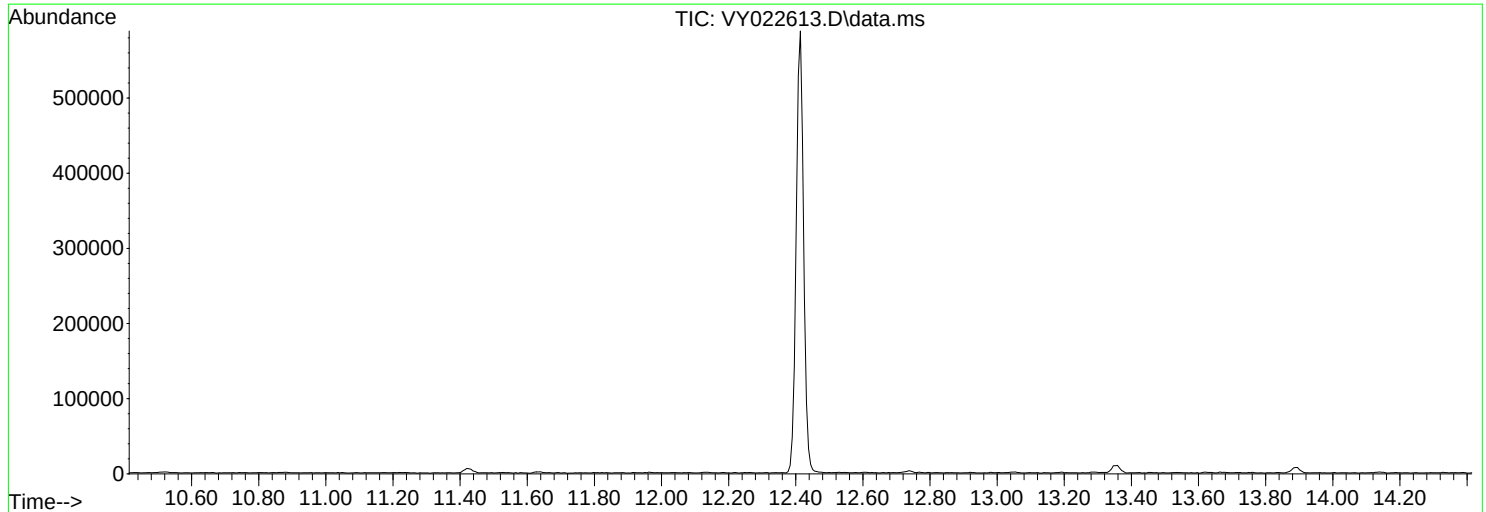

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	22493	PASS
75	95	30	60	59.9	54776	PASS
95	95	100	100	100.0	91432	PASS
96	95	5	9	6.9	6305	PASS
173	174	0.00	2	1.3	1019	PASS
174	95	50	100	86.7	79312	PASS
175	174	5	9	7.3	5782	PASS
176	174	95	101	96.0	76125	PASS
177	176	5	9	6.5	4967	PASS