
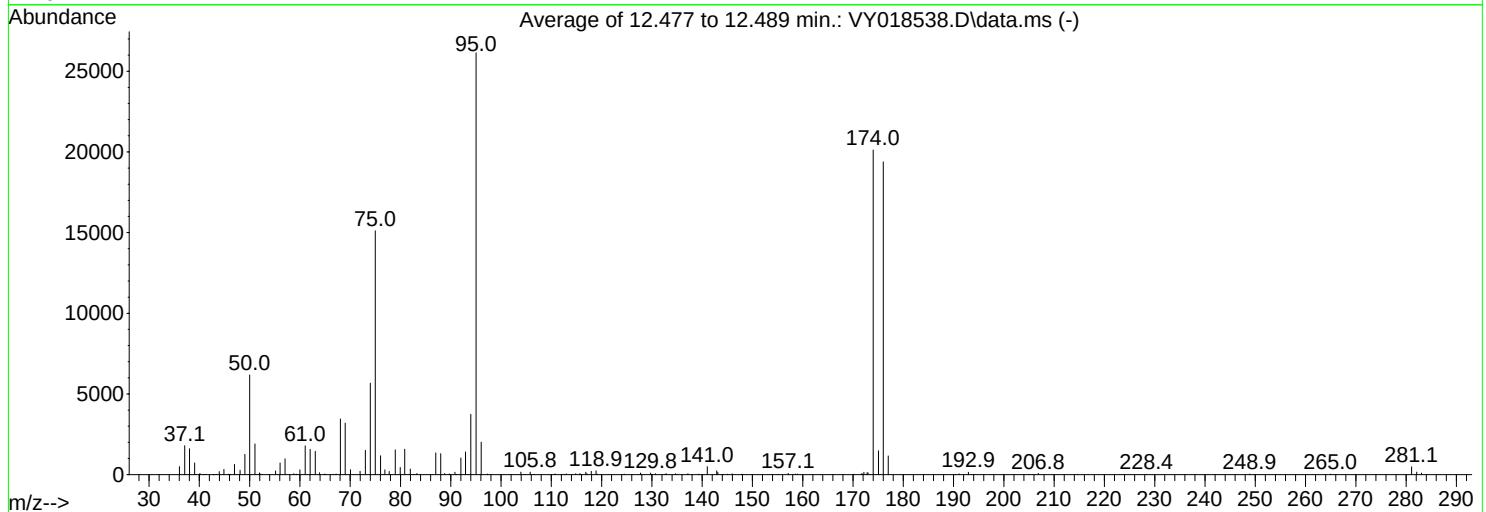


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061024\
Data File : VY018538.D
Acq On : 10 Jun 2024 08:30
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060324S.M
Title : SW846 8260
Last Update : Tue Jun 04 07:11:56 2024

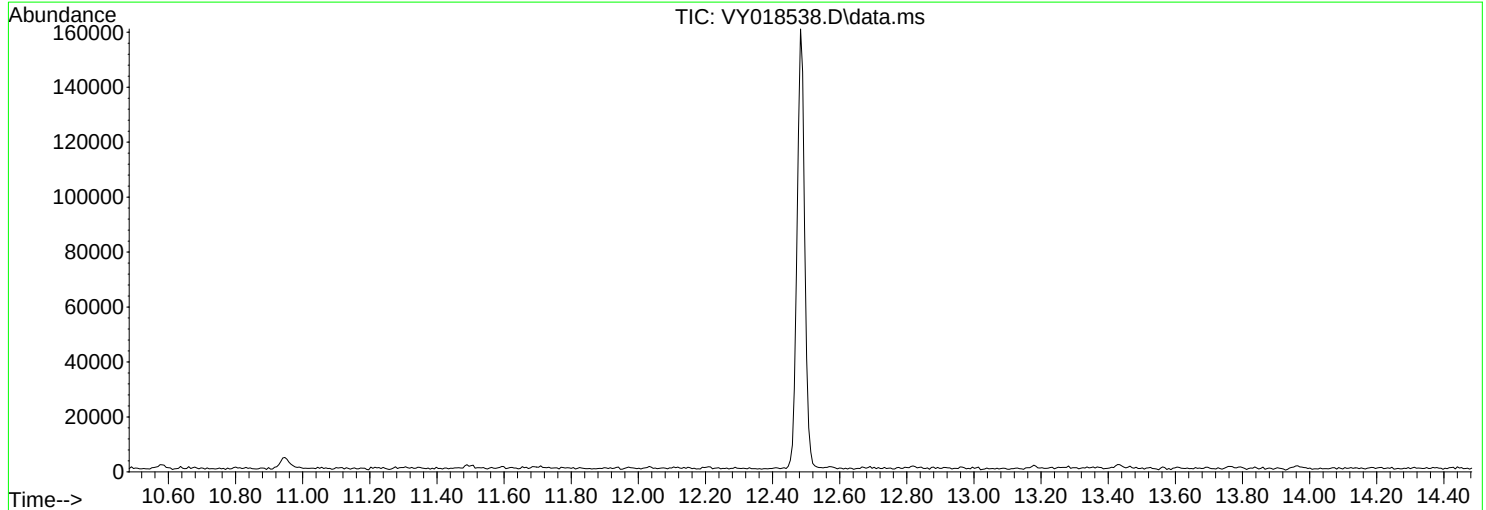

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	6174	PASS
75	95	30	60	57.8	15109	PASS
95	95	100	100	100.0	26139	PASS
96	95	5	9	7.7	2010	PASS
173	174	0.00	2	0.6	127	PASS
174	95	50	100	77.0	20123	PASS
175	174	5	9	7.3	1475	PASS
176	174	95	101	96.3	19385	PASS
177	176	5	9	6.0	1158	PASS