
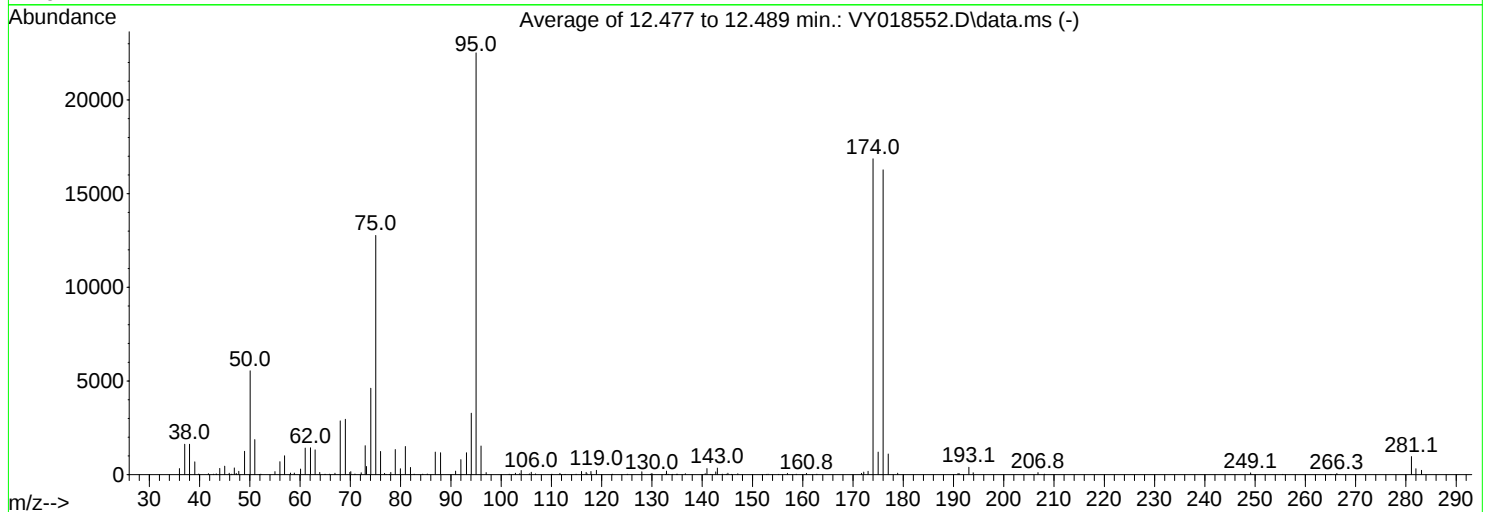


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061124\
Data File : VY018552.D
Acq On : 11 Jun 2024 09:38
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060324S.M
Title : SW846 8260
Last Update : Tue Jun 04 07:11:56 2024

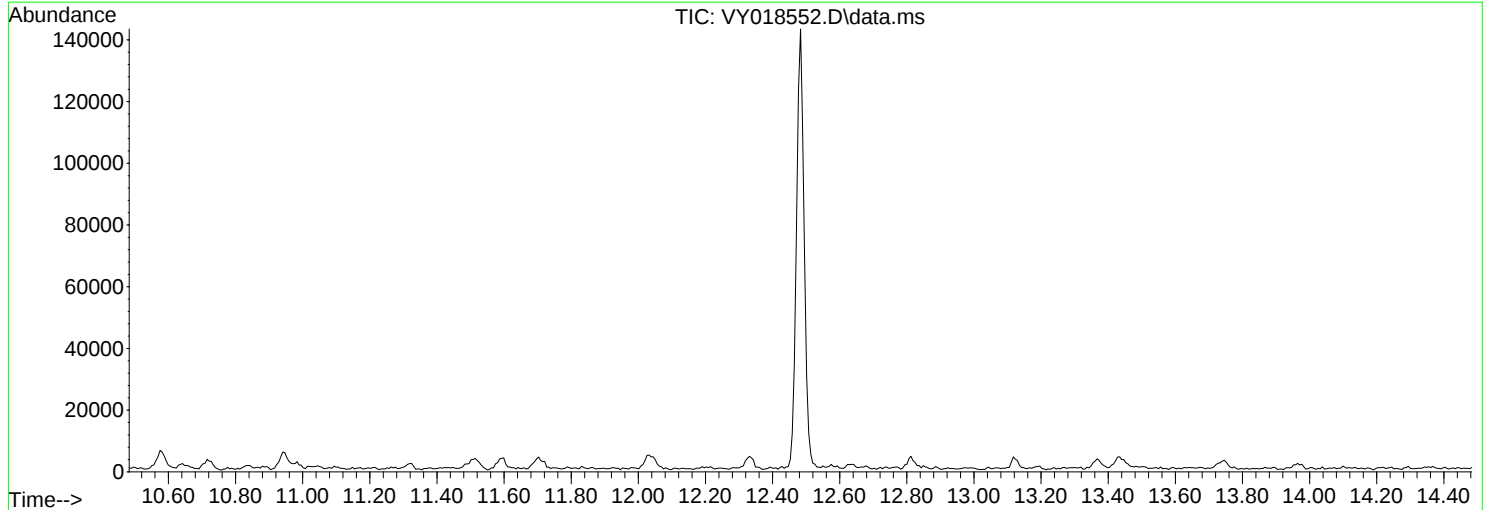

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.6	5546	PASS
75	95	30	60	56.7	12771	PASS
95	95	100	100	100.0	22515	PASS
96	95	5	9	6.8	1527	PASS
173	174	0.00	2	1.1	183	PASS
174	95	50	100	74.9	16862	PASS
175	174	5	9	7.2	1207	PASS
176	174	95	101	96.5	16273	PASS
177	176	5	9	6.8	1105	PASS