

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061225\
 Data File : VY022672.D
 Acq On : 12 Jun 2025 14:33
 Operator : SY/MD
 Sample : Q2296-11
 Misc : 5.65g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-3-VOC

Quant Time: Jun 13 05:41:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 10 15:26:14 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	117553	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	213204	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	171852	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	62966	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.060	65	65452	49.782	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	99.560%
35) Dibromofluoromethane	7.634	113	63219	49.678	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.360%
50) Toluene-d8	10.103	98	251997	49.008	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	98.020%
62) 4-Bromofluorobenzene	12.401	95	62623	40.875	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	81.760%
Target Compounds						
					Qvalue	
20) Methylene Chloride	4.604	84	5721	3.772	ug/l #	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061225\
Data File : VY022672.D
Acq On : 12 Jun 2025 14:33
Operator : SY/MD
Sample : Q2296-11
Misc : 5.65g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-3-VOC

Quant Time: Jun 13 05:41:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 10 15:26:14 2025
Response via : Initial Calibration




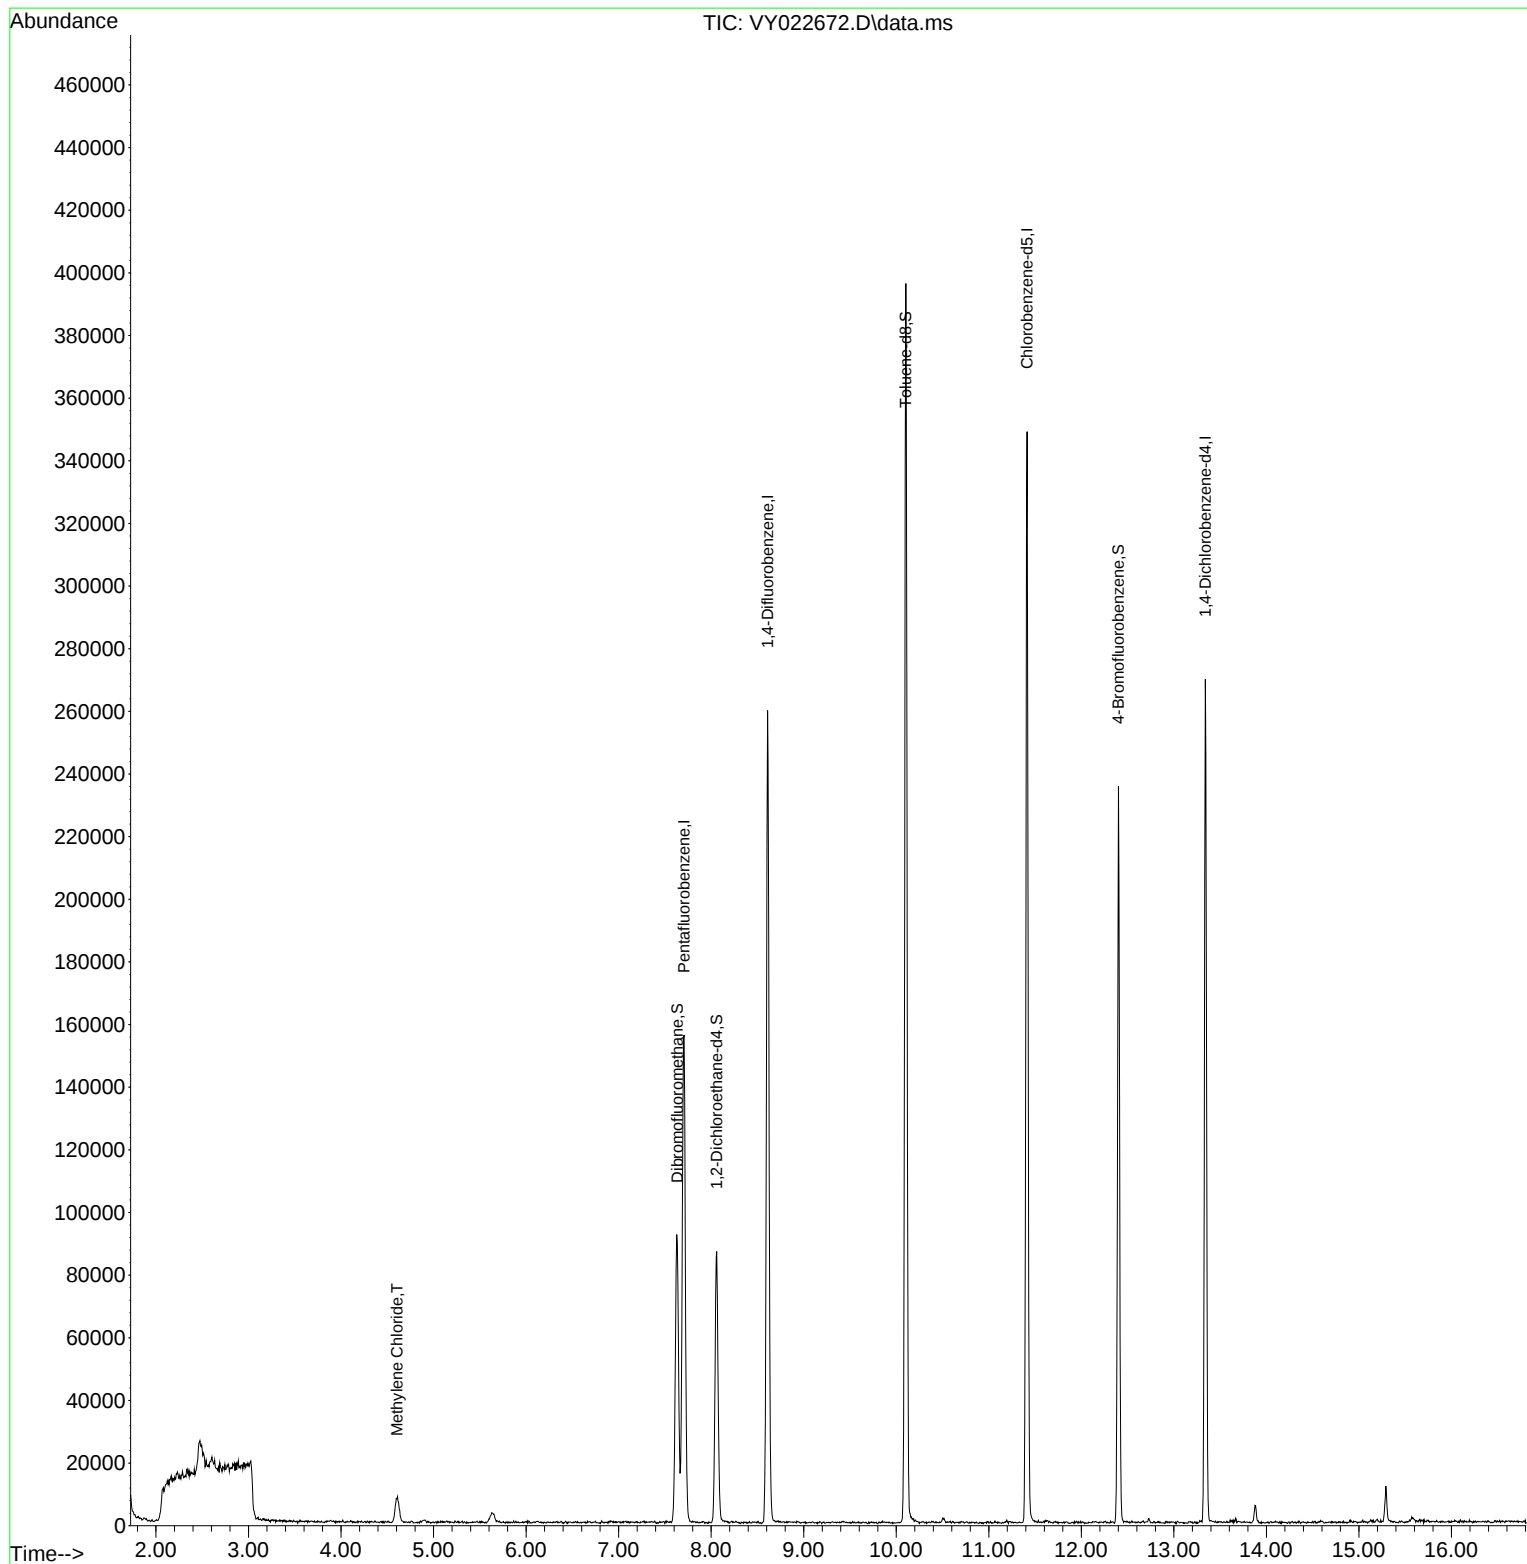




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022672.D
Acq: 12 Jun 2025 14:33




Instrument :
MSVOA_Y
ClientSampleId :
WC-3-VOC


Tgt Ion:168 Resp: 117553
Ion Ratio Lower Upper
168 100
99 56.3 44.3 66.5

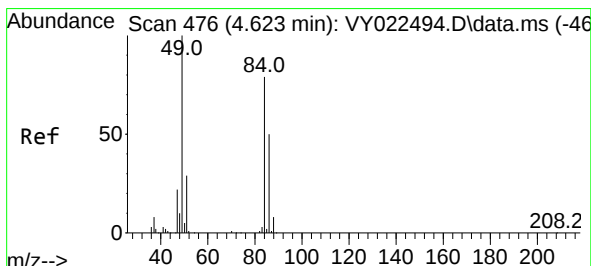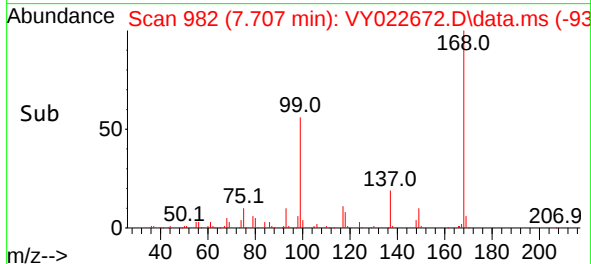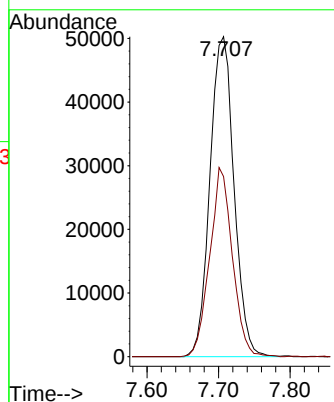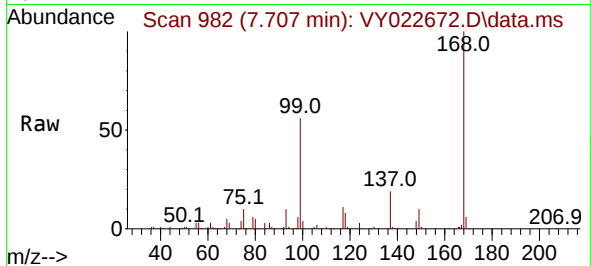

#20
Methylene Chloride
Concen: 3.772 ug/l
RT: 4.604 min Scan# 473
Delta R.T. -0.019 min
Lab File: VY022672.D
Acq: 12 Jun 2025 14:33

Tgt Ion: 84 Resp: 5721
Ion Ratio Lower Upper
84 100
49 121.5 101.9 152.9
51 25.5 29.8 44.8#
86 63.2 51.3 76.9

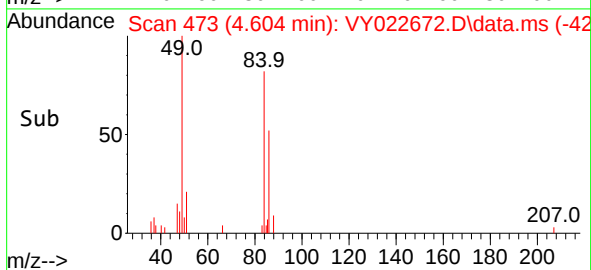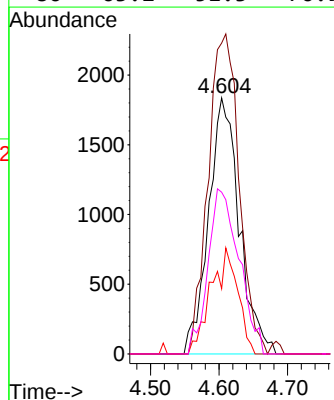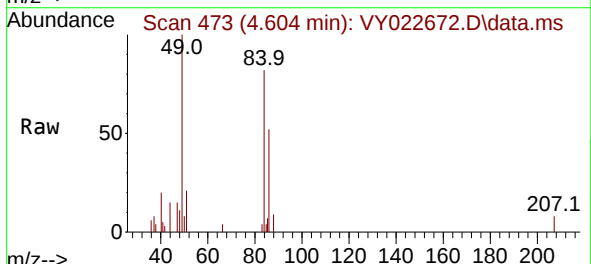

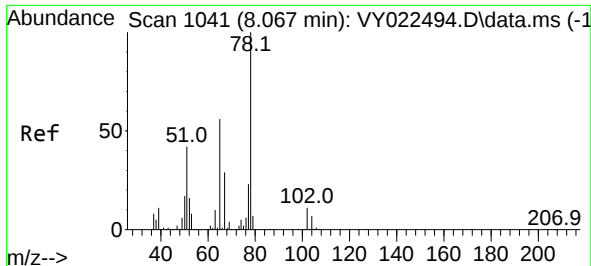

#33

1,2-Dichloroethane-d4

Concen: 49.782 ug/l

RT: 8.060 min Scan# 1

Delta R.T. -0.007 min

Lab File: VY022672.D

Acq: 12 Jun 2025 14:33

Instrument :

MSVOA_Y

ClientSampleId :





WC-3-VOC

Tgt Ion: 65 Resp: 65452

Ion Ratio Lower Upper

65 100

67 53.1 0.0 103.4

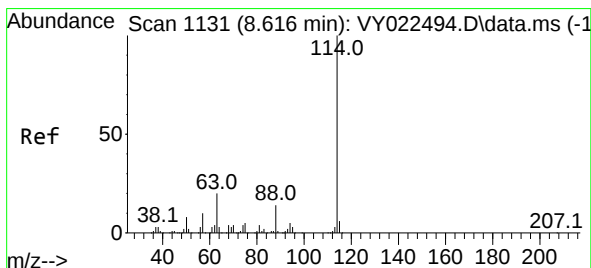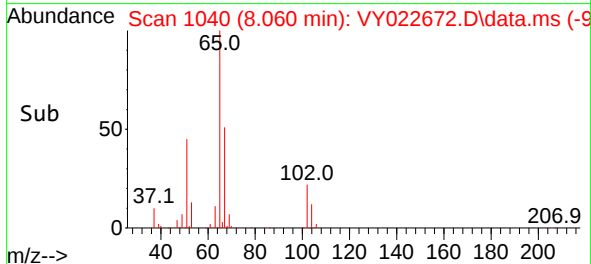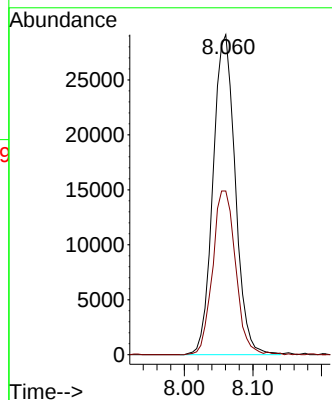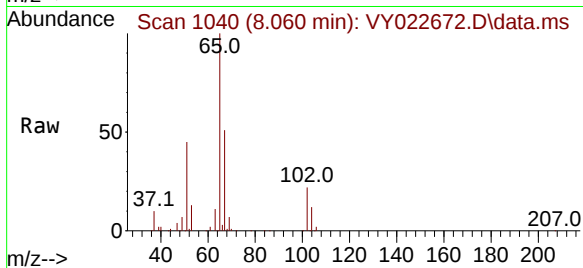

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.609 min Scan# 1130

Delta R.T. -0.007 min

Lab File: VY022672.D

Acq: 12 Jun 2025 14:33




Tgt Ion: 114 Resp: 213204

Ion Ratio Lower Upper

114 100

63 20.5 0.0 40.8

88 14.4 0.0 27.8


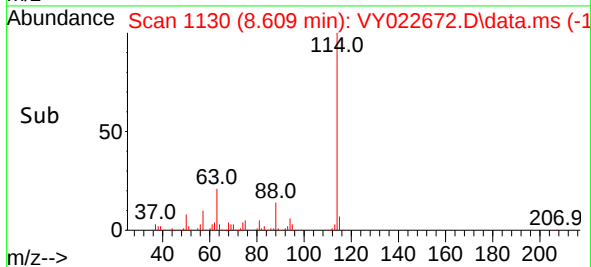
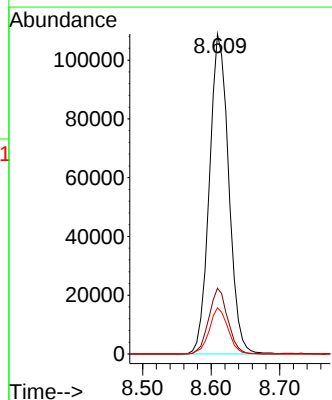
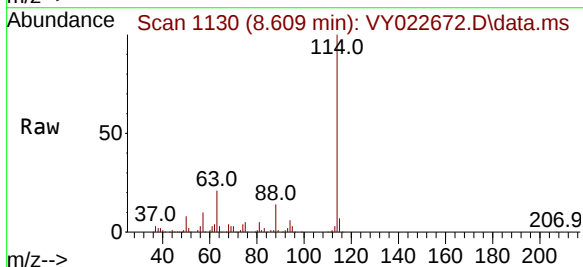




#35
Dibromofluoromethane
Concen: 49.678 ug/l
RT: 7.634 min Scan# 91
Delta R.T. -0.007 min
Lab File: VY022672.D
Acq: 12 Jun 2025 14:33




Instrument :
MSVOA_Y
ClientSampleId :
WC-3-VOC


Tgt Ion:113 Resp: 63219
Ion Ratio Lower Upper
113 100
111 104.8 81.1 121.7
192 18.6 14.2 21.2

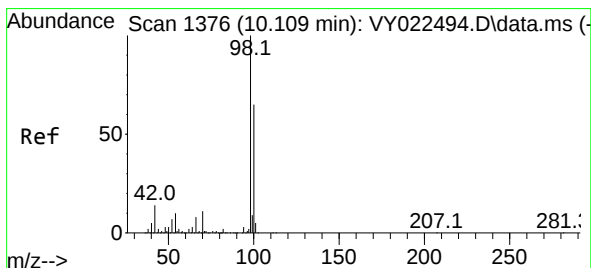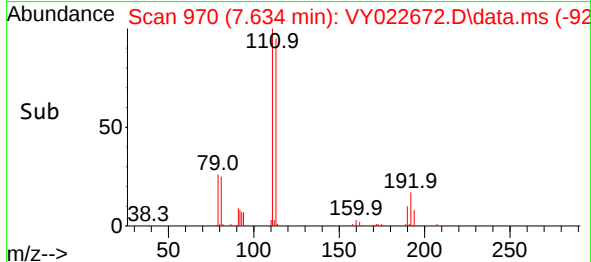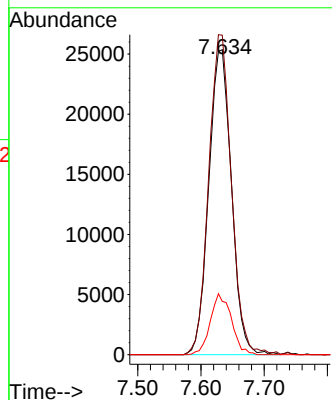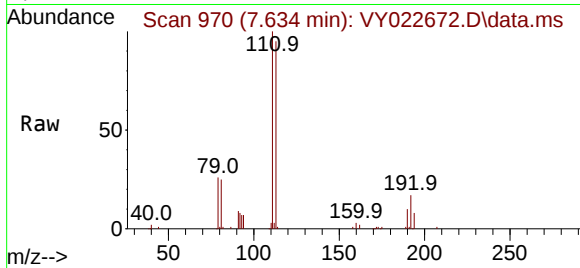

#50
Toluene-d8
Concen: 49.008 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. -0.007 min
Lab File: VY022672.D
Acq: 12 Jun 2025 14:33

Tgt Ion: 98 Resp: 251997
Ion Ratio Lower Upper
98 100
100 64.8 51.4 77.0


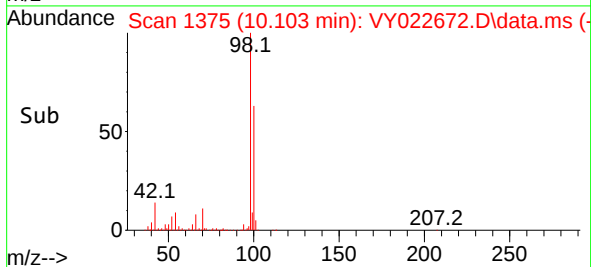
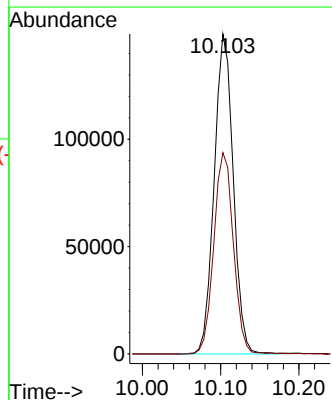
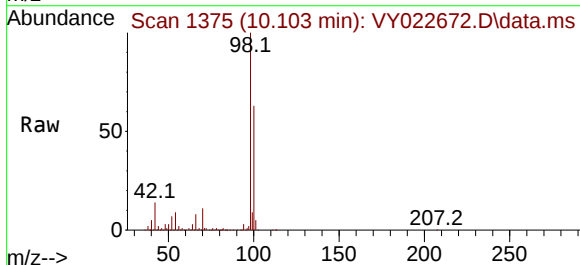


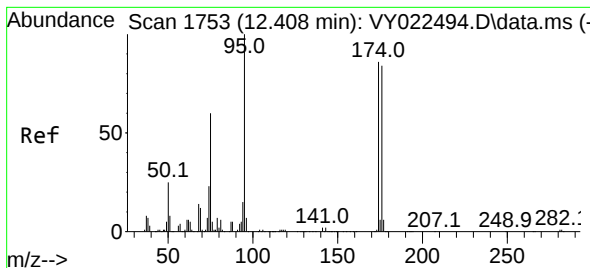

#62
4-Bromofluorobenzene
Concen: 40.875 ug/l
RT: 12.401 min Scan# 11
Delta R.T. -0.007 min
Lab File: VY022672.D
Acq: 12 Jun 2025 14:33




Instrument :
MSVOA_Y
ClientSampleId :
WC-3-VOC


Tgt Ion: 95 Resp: 62623
Ion Ratio Lower Upper
95 100
174 87.0 0.0 170.0
176 85.3 0.0 166.2

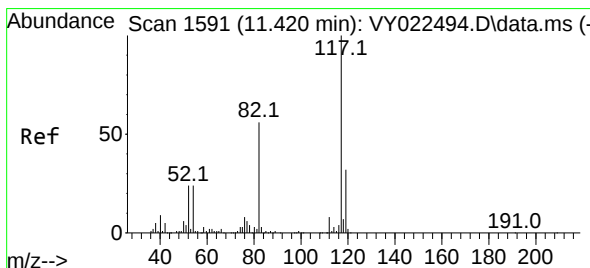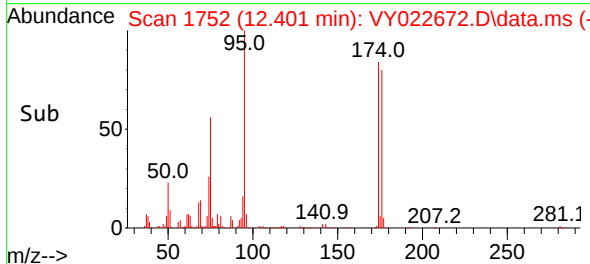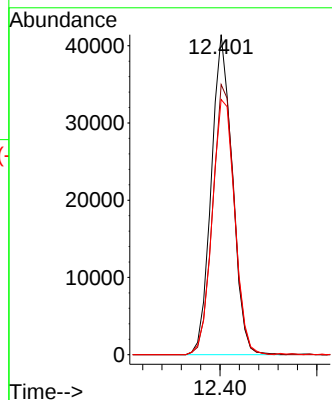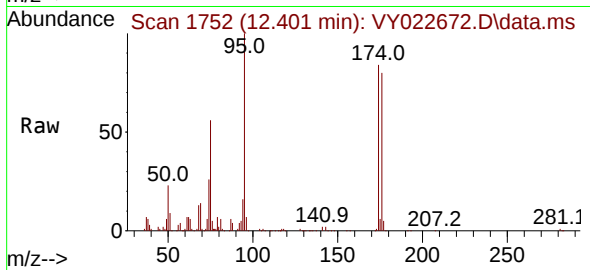

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.007 min
Lab File: VY022672.D
Acq: 12 Jun 2025 14:33

Tgt Ion: 117 Resp: 171852
Ion Ratio Lower Upper
117 100
82 56.1 44.6 66.8
119 33.2 25.4 38.0

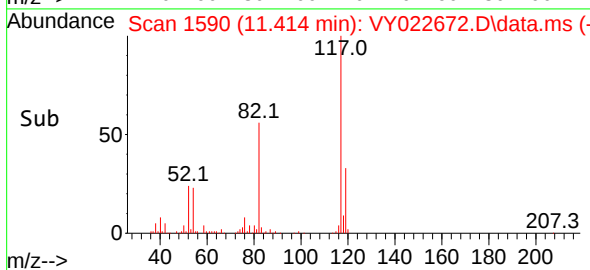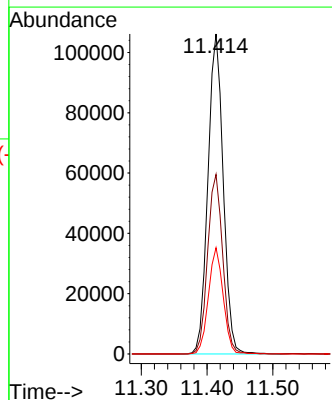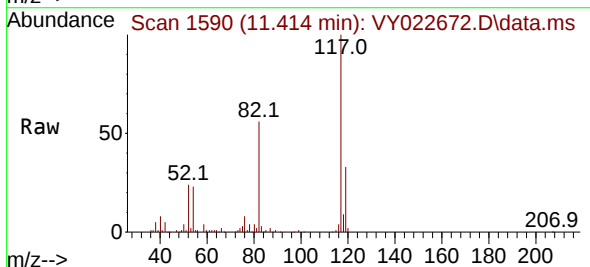

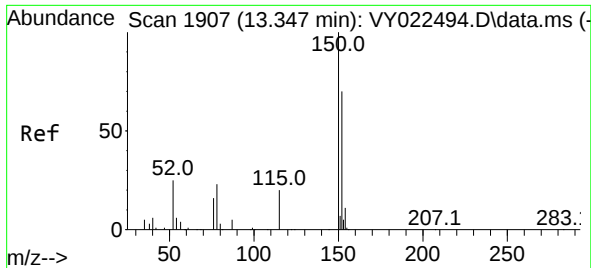

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.340 min Scan# 1906
 Delta R.T. -0.007 min
 Lab File: VY022672.D
 Acq: 12 Jun 2025 14:33

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-3-VOC

Tgt Ion:152 Resp: 62966
 Ion Ratio Lower Upper
 152 100
 115 56.6 28.9 86.7
 150 157.0 0.0 349.6

