

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061225\
 Data File : VY022673.D
 Acq On : 12 Jun 2025 14:57
 Operator : SY/MD
 Sample : Q2296-15
 Misc : 5.13g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-4-VOC

Quant Time: Jun 13 05:41:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 10 15:26:14 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	169048	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	308701	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	251430	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	92298	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	91973	48.645	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	97.280%
35) Dibromofluoromethane	7.628	113	92569	50.239	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.480%
50) Toluene-d8	10.103	98	369113	49.577	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.160%
62) 4-Bromofluorobenzene	12.401	95	92807	41.837	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	83.680%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061225\
Data File : VY022673.D
Acq On : 12 Jun 2025 14:57
Operator : SY/MD
Sample : Q2296-15
Misc : 5.13g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-4-VOC

Quant Time: Jun 13 05:41:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 10 15:26:14 2025
Response via : Initial Calibration




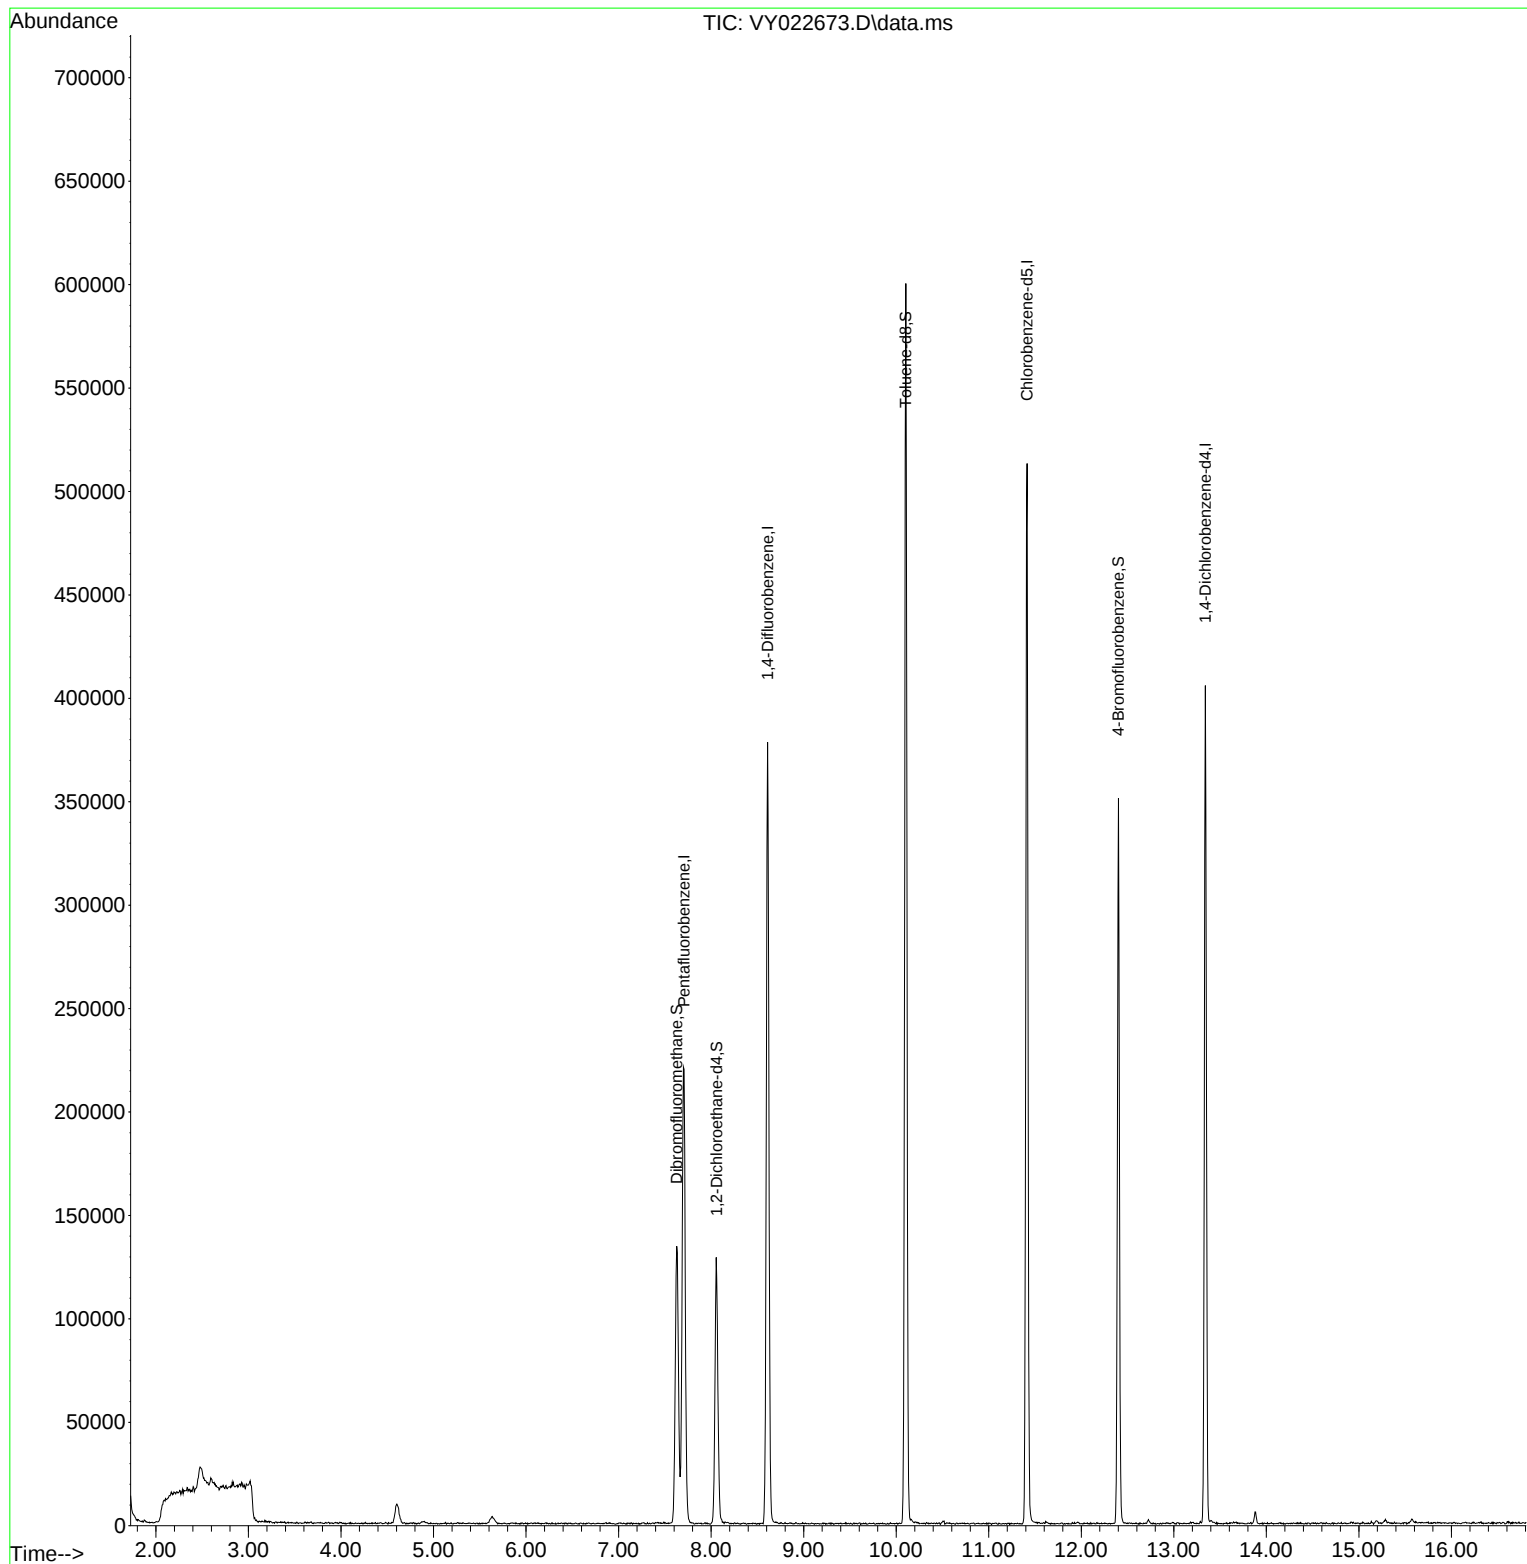




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 99
Delta R.T. -0.006 min
Lab File: VY022673.D
Acq: 12 Jun 2025 14:57




Instrument :
MSVOA_Y
ClientSampleId :
WC-4-VOC

Tgt Ion:168 Resp: 169048
Ion Ratio Lower Upper
168 100
99 50.1 44.3 66.5

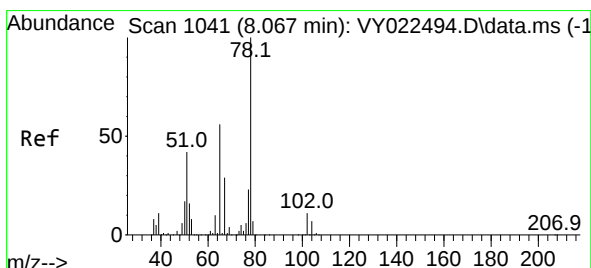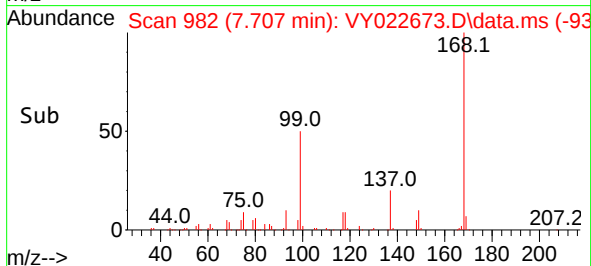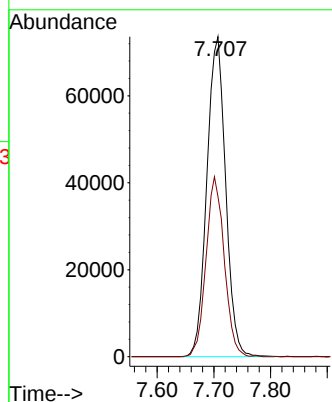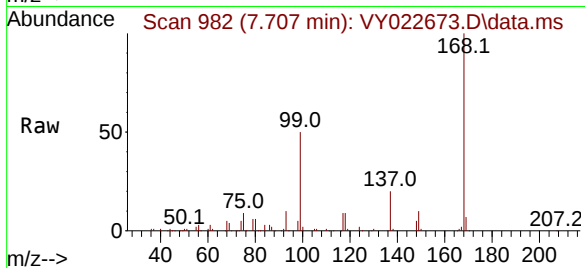

#33
1,2-Dichloroethane-d4
Concen: 48.645 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY022673.D
Acq: 12 Jun 2025 14:57

Tgt Ion: 65 Resp: 91973
Ion Ratio Lower Upper
65 100
67 53.2 0.0 103.4


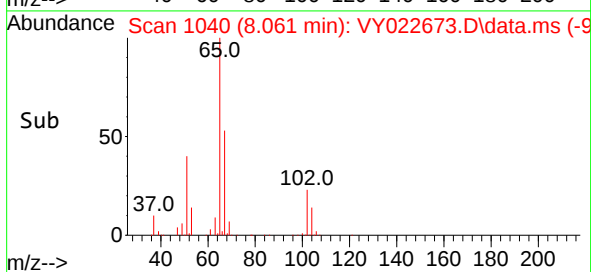
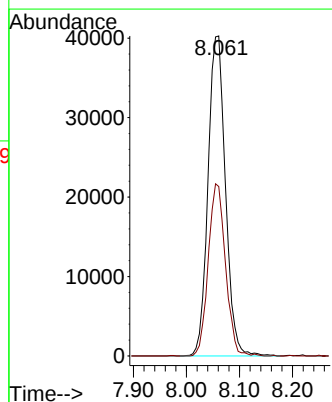
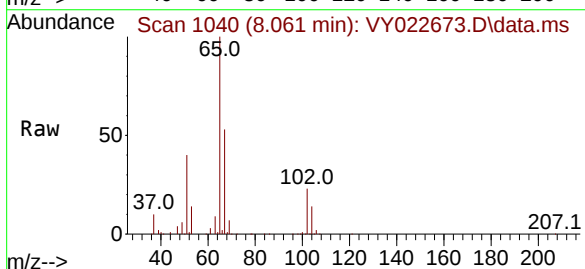




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.609 min Scan# 1131
Delta R.T. -0.006 min
Lab File: VY022673.D
Acq: 12 Jun 2025 14:57




Instrument :
MSVOA_Y
ClientSampleId :
WC-4-VOC


Tgt Ion:114 Resp: 308701
Ion Ratio Lower Upper
114 100
63 19.3 0.0 40.8
88 14.2 0.0 27.8

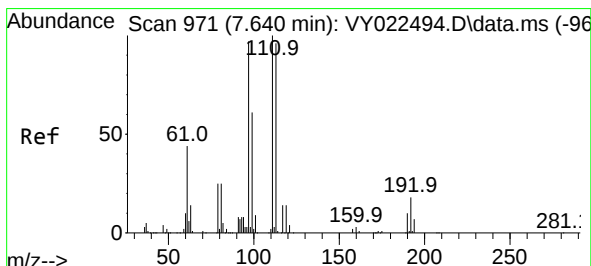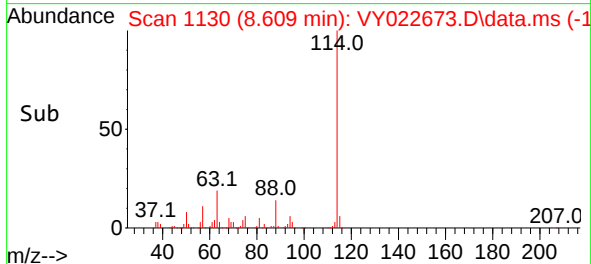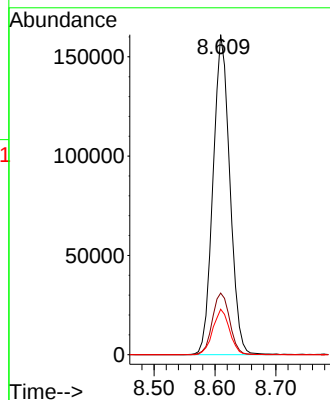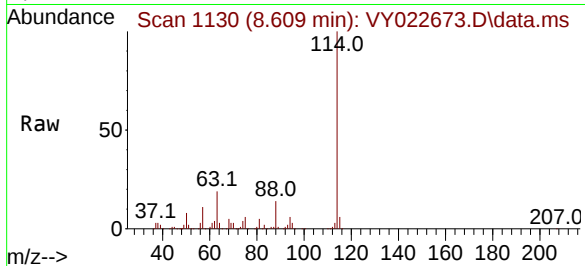

#35
Dibromofluoromethane
Concen: 50.239 ug/l
RT: 7.628 min Scan# 969
Delta R.T. -0.012 min
Lab File: VY022673.D
Acq: 12 Jun 2025 14:57

Tgt Ion:113 Resp: 92569
Ion Ratio Lower Upper
113 100
111 102.0 81.1 121.7
192 17.7 14.2 21.2


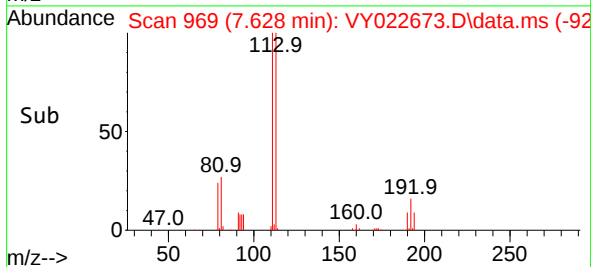
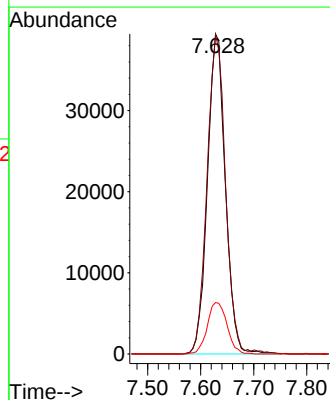
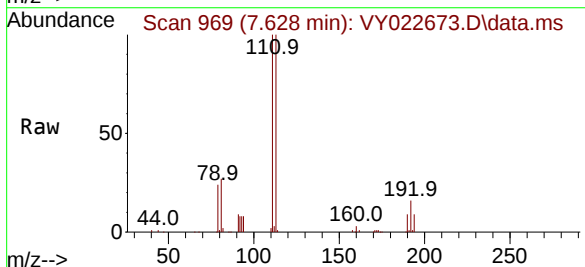


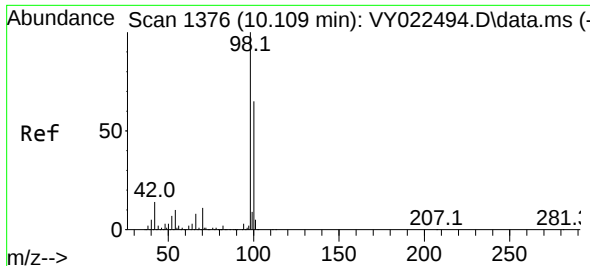

#50
Toluene-d8
Concen: 49.577 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY022673.D
Acq: 12 Jun 2025 14:57




Instrument :
MSVOA_Y
ClientSampleId :
WC-4-VOC


Tgt Ion: 98 Resp: 369113
Ion Ratio Lower Upper
98 100
100 64.8 51.4 77.0

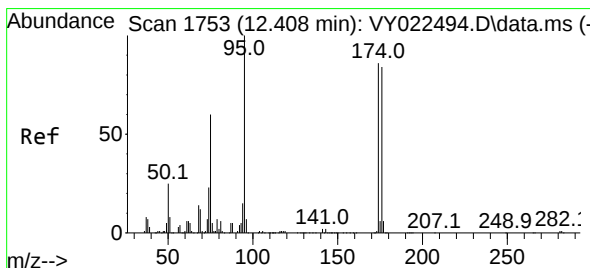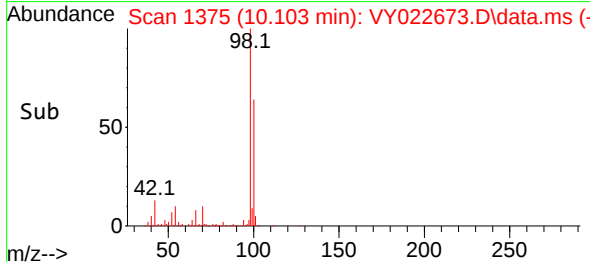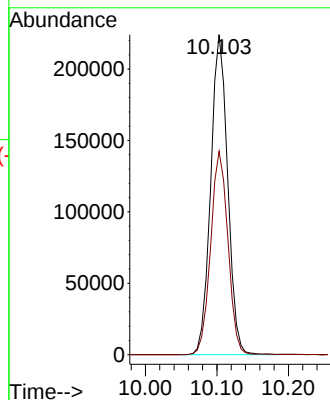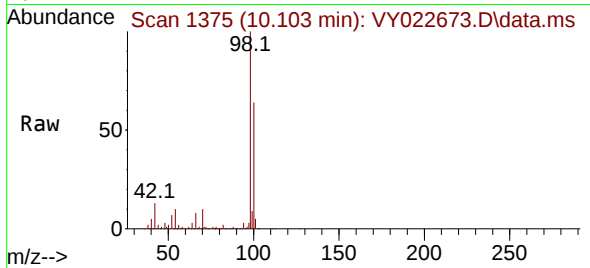

#62
4-Bromofluorobenzene
Concen: 41.837 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.006 min
Lab File: VY022673.D
Acq: 12 Jun 2025 14:57

Tgt Ion: 95 Resp: 92807
Ion Ratio Lower Upper
95 100
174 87.1 0.0 170.0
176 83.6 0.0 166.2

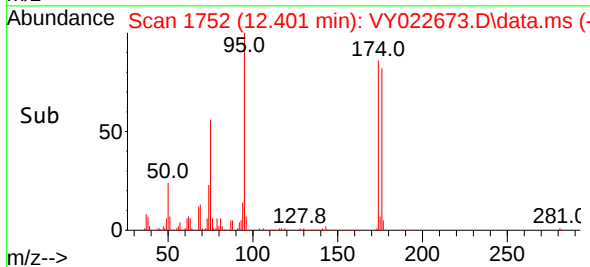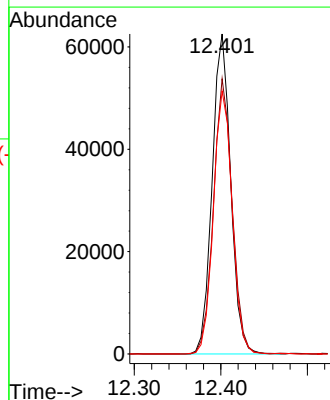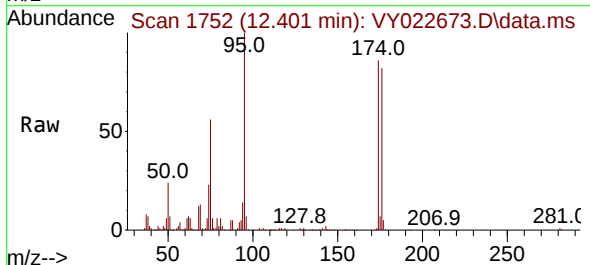

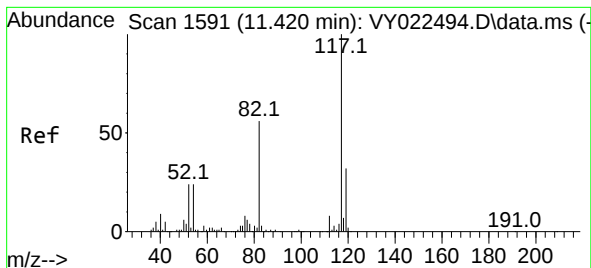

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY022673.D

Acq: 12 Jun 2025 14:57

Instrument :

MSVOA_Y

ClientSampleId :

WC-4-VOC





Tgt Ion:117 Resp: 251430

Ion Ratio Lower Upper

117 100

82 55.7 44.6 66.8

119 33.6 25.4 38.0

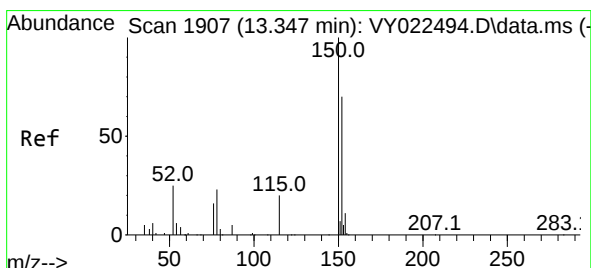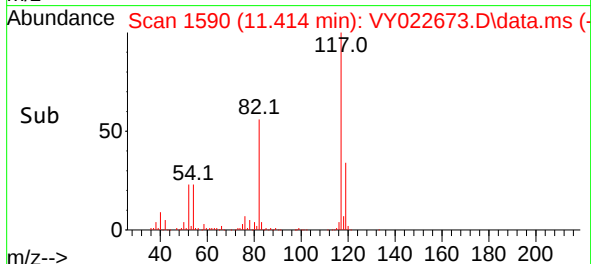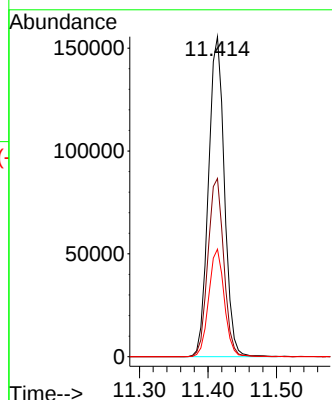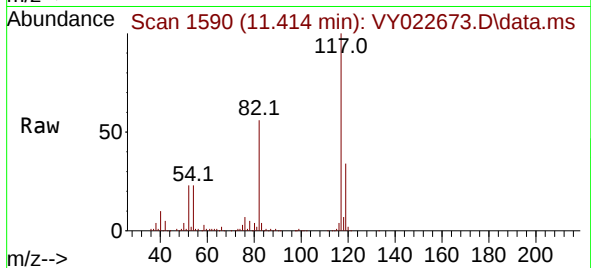

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.340 min Scan# 1906

Delta R.T. -0.006 min

Lab File: VY022673.D

Acq: 12 Jun 2025 14:57

Tgt Ion:152 Resp: 92298

Ion Ratio Lower Upper

152 100

115 58.4 28.9 86.7

150 157.4 0.0 349.6

