



Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061325\
Data File : VY022690.D
Acq On : 13 Jun 2025 12:18
Operator : SY/MD
Sample : Q2298-02
Misc : 5.74g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
AU-05-061125

Quant Time: Jun 14 02:03:53 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 10 15:26:14 2025
Response via : Initial Calibration




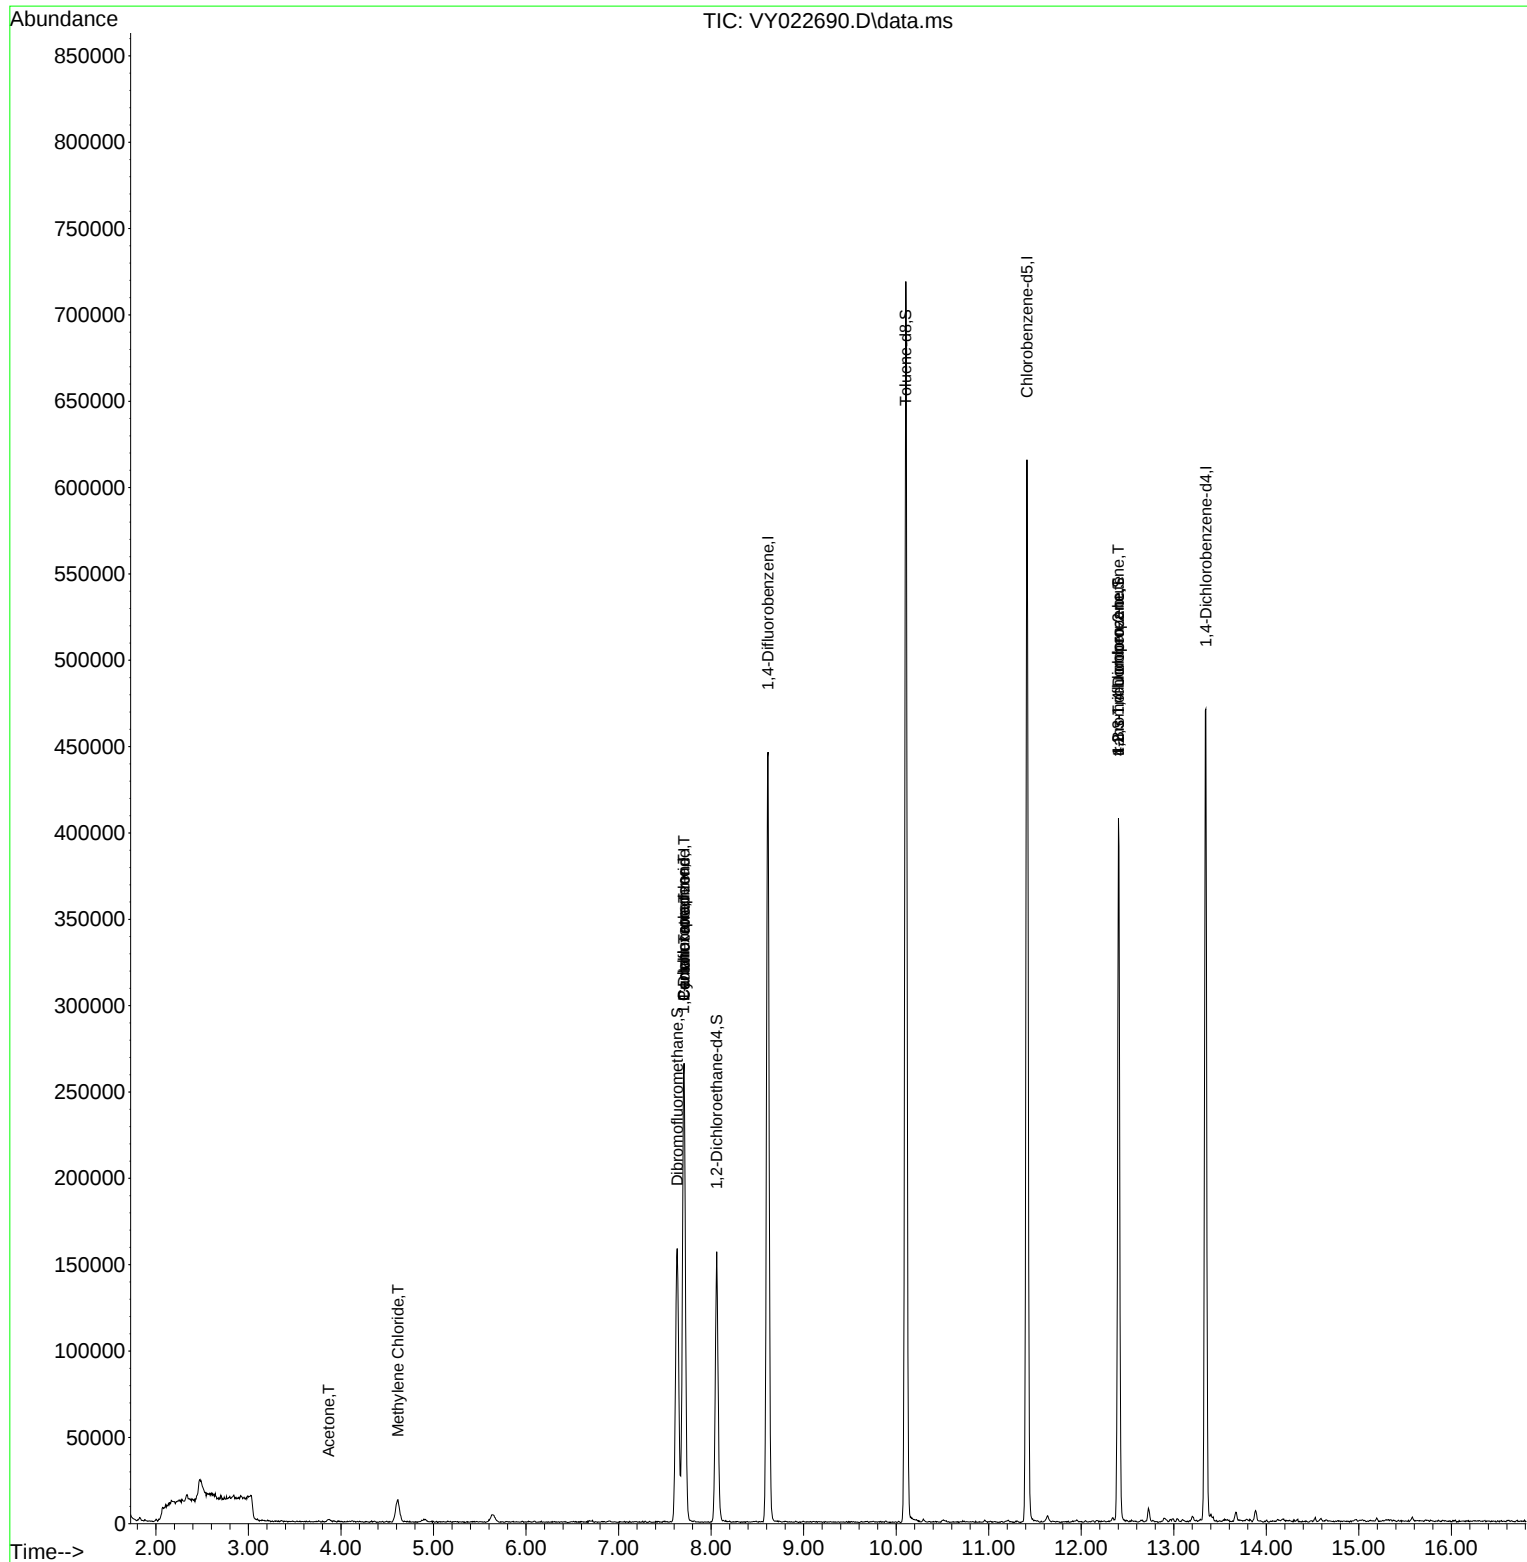


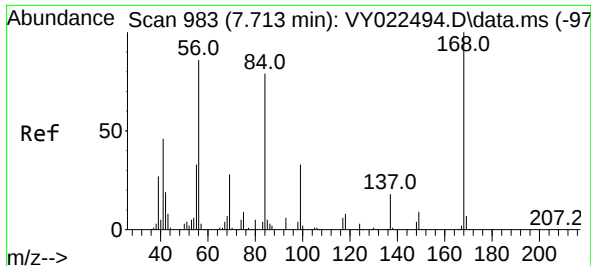

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022690.D
Acq: 13 Jun 2025 12:18




Instrument :
MSVOA_Y
ClientSampleId :
AU-05-061125


Tgt Ion:168 Resp: 194561
Ion Ratio Lower Upper
168 100
99 55.7 44.3 66.5

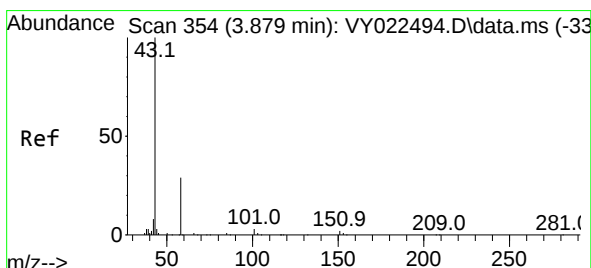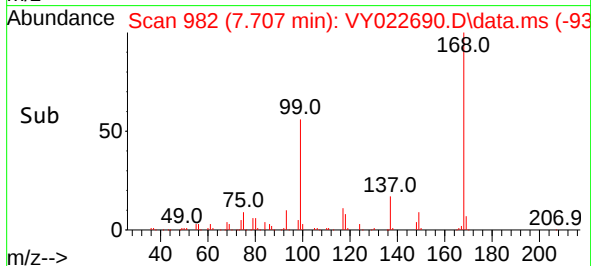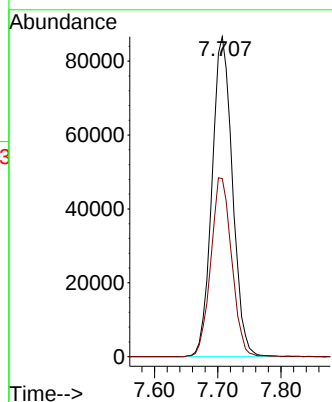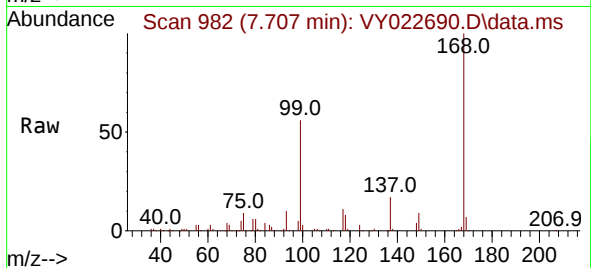

#16
Acetone
Concen: 5.897 ug/l
RT: 3.866 min Scan# 352
Delta R.T. -0.012 min
Lab File: VY022690.D
Acq: 13 Jun 2025 12:18

Tgt Ion: 43 Resp: 2606
Ion Ratio Lower Upper
43 100
58 40.9 24.0 36.0#


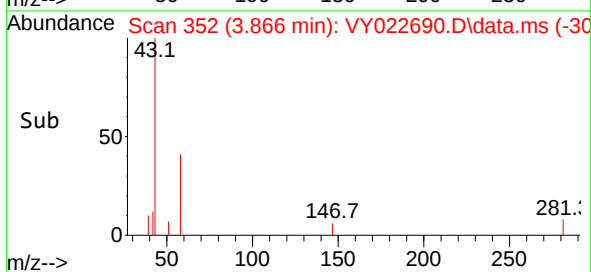
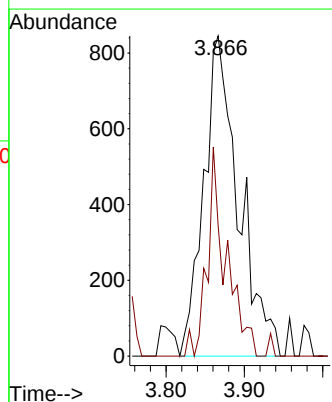
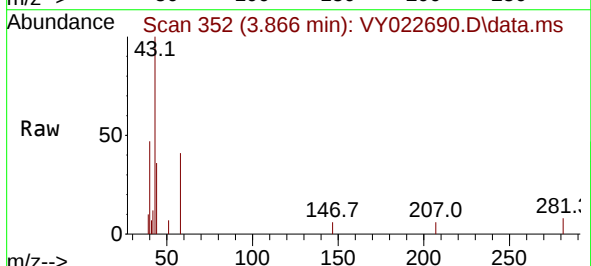


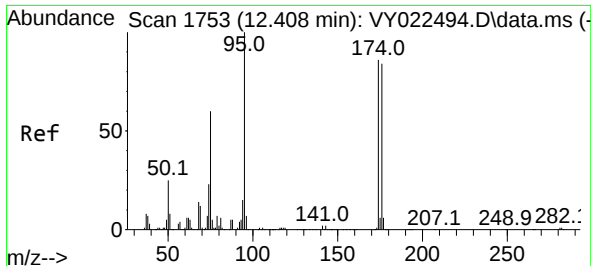

#62
4-Bromofluorobenzene
Concen: 42.230 ug/l
RT: 12.401 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY022690.D
Acq: 13 Jun 2025 12:18




Instrument :
MSVOA_Y
ClientSampleId :
AU-05-061125


Tgt Ion: 95 Resp: 111501
Ion Ratio Lower Upper
95 100
174 85.5 0.0 170.0
176 81.5 0.0 166.2

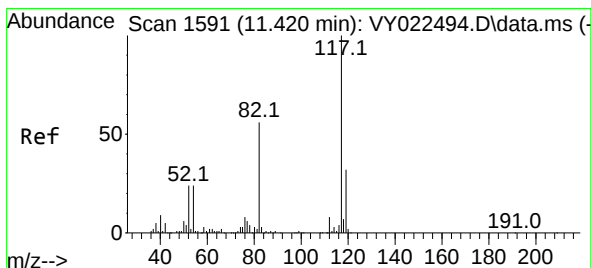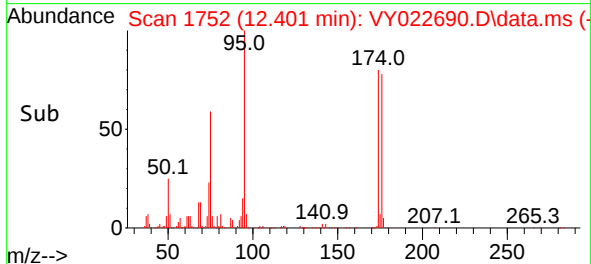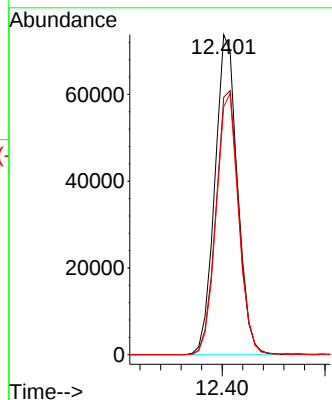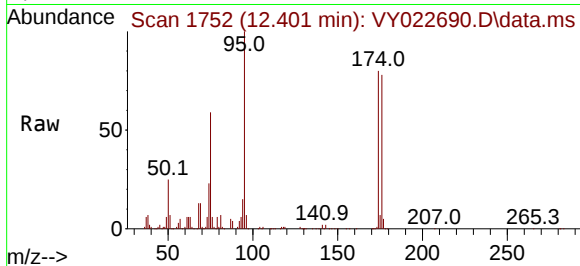

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 1590
Delta R.T. -0.006 min
Lab File: VY022690.D
Acq: 13 Jun 2025 12:18


Tgt Ion: 117 Resp: 305494
Ion Ratio Lower Upper
117 100
82 56.1 44.6 66.8
119 32.5 25.4 38.0

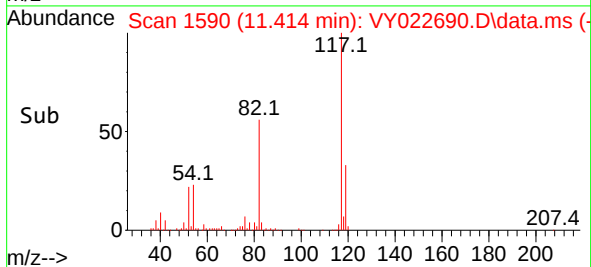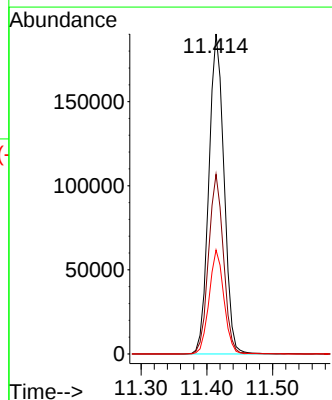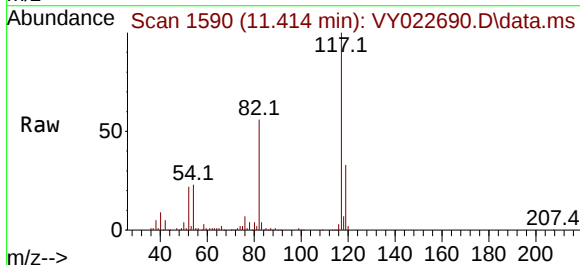

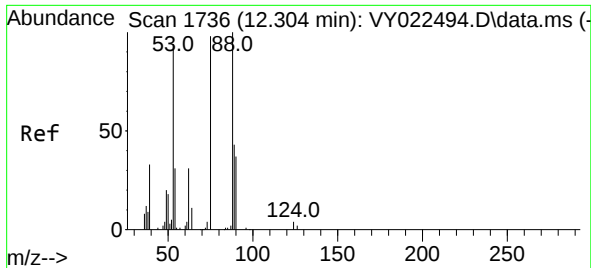

#81
 trans-1,4-Dichloro-2-butene
 Concen: 124.562 ug/l
 RT: 12.401 min Scan# 11
 Delta R.T. 0.097 min
 Lab File: VY022690.D
 Acq: 13 Jun 2025 12:18

Instrument :
 MSVOA_Y
 ClientSampleId :
 AU-05-061125

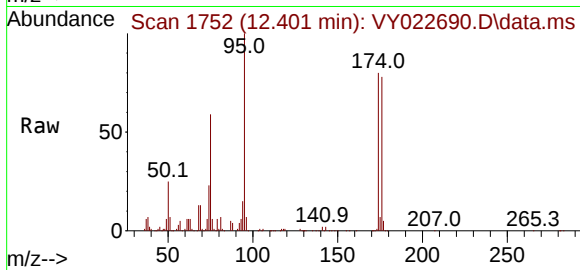

Tgt Ion: 75 Resp: 64850
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.5 117.7#
 89 0.0 35.7 53.5#

