



Acrolein

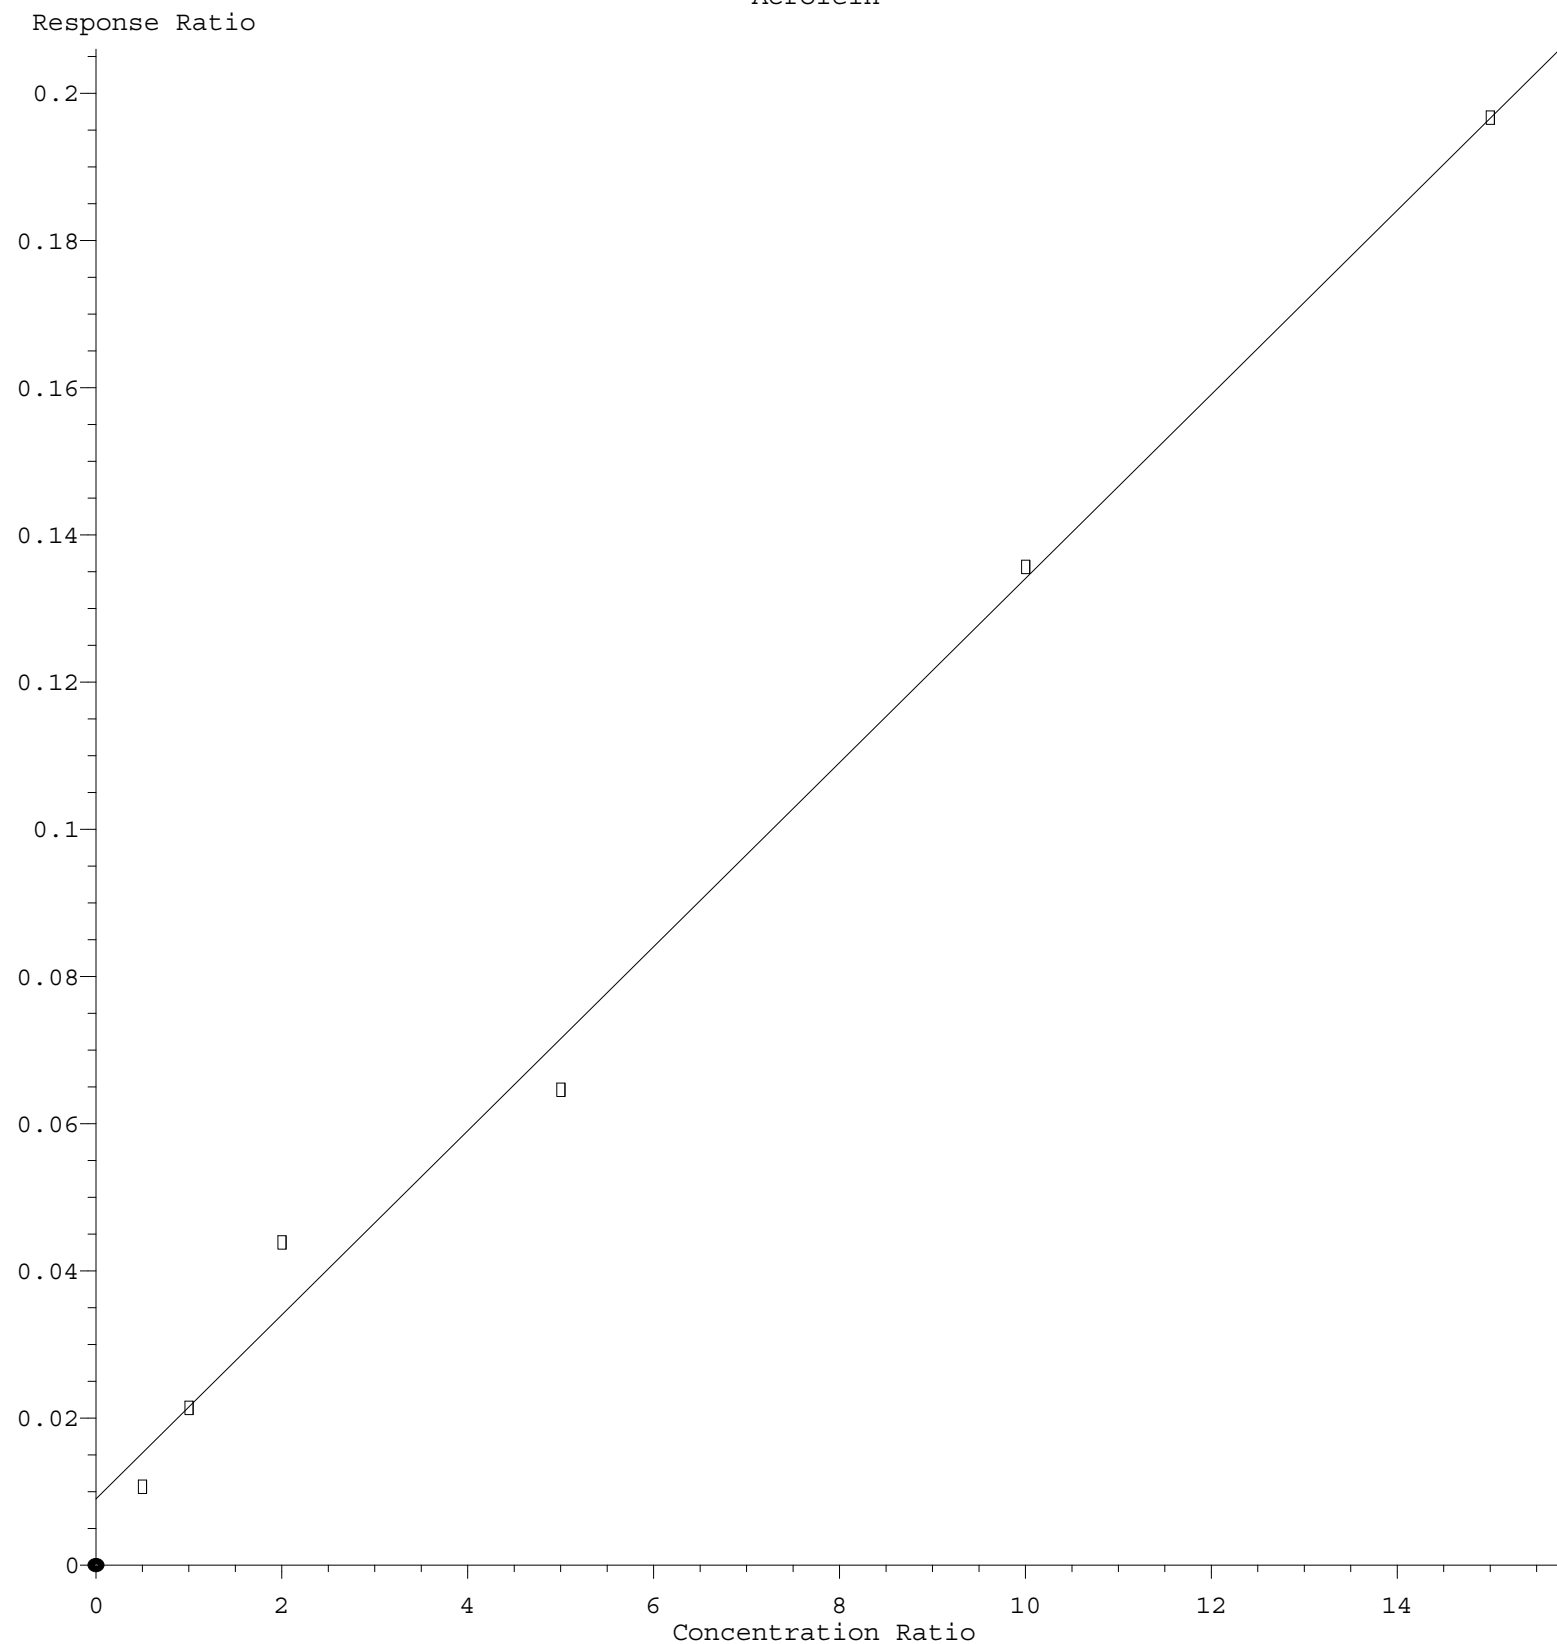

Response = $1.251e-002 * Amt + 8.949e-003$
 Coef of Det (r^2) = 0.993642 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y061522S.M
 Calibration Table Last Updated: Thu Jun 16 02:54:06 2022

Methyl Acetate

Response Ratio

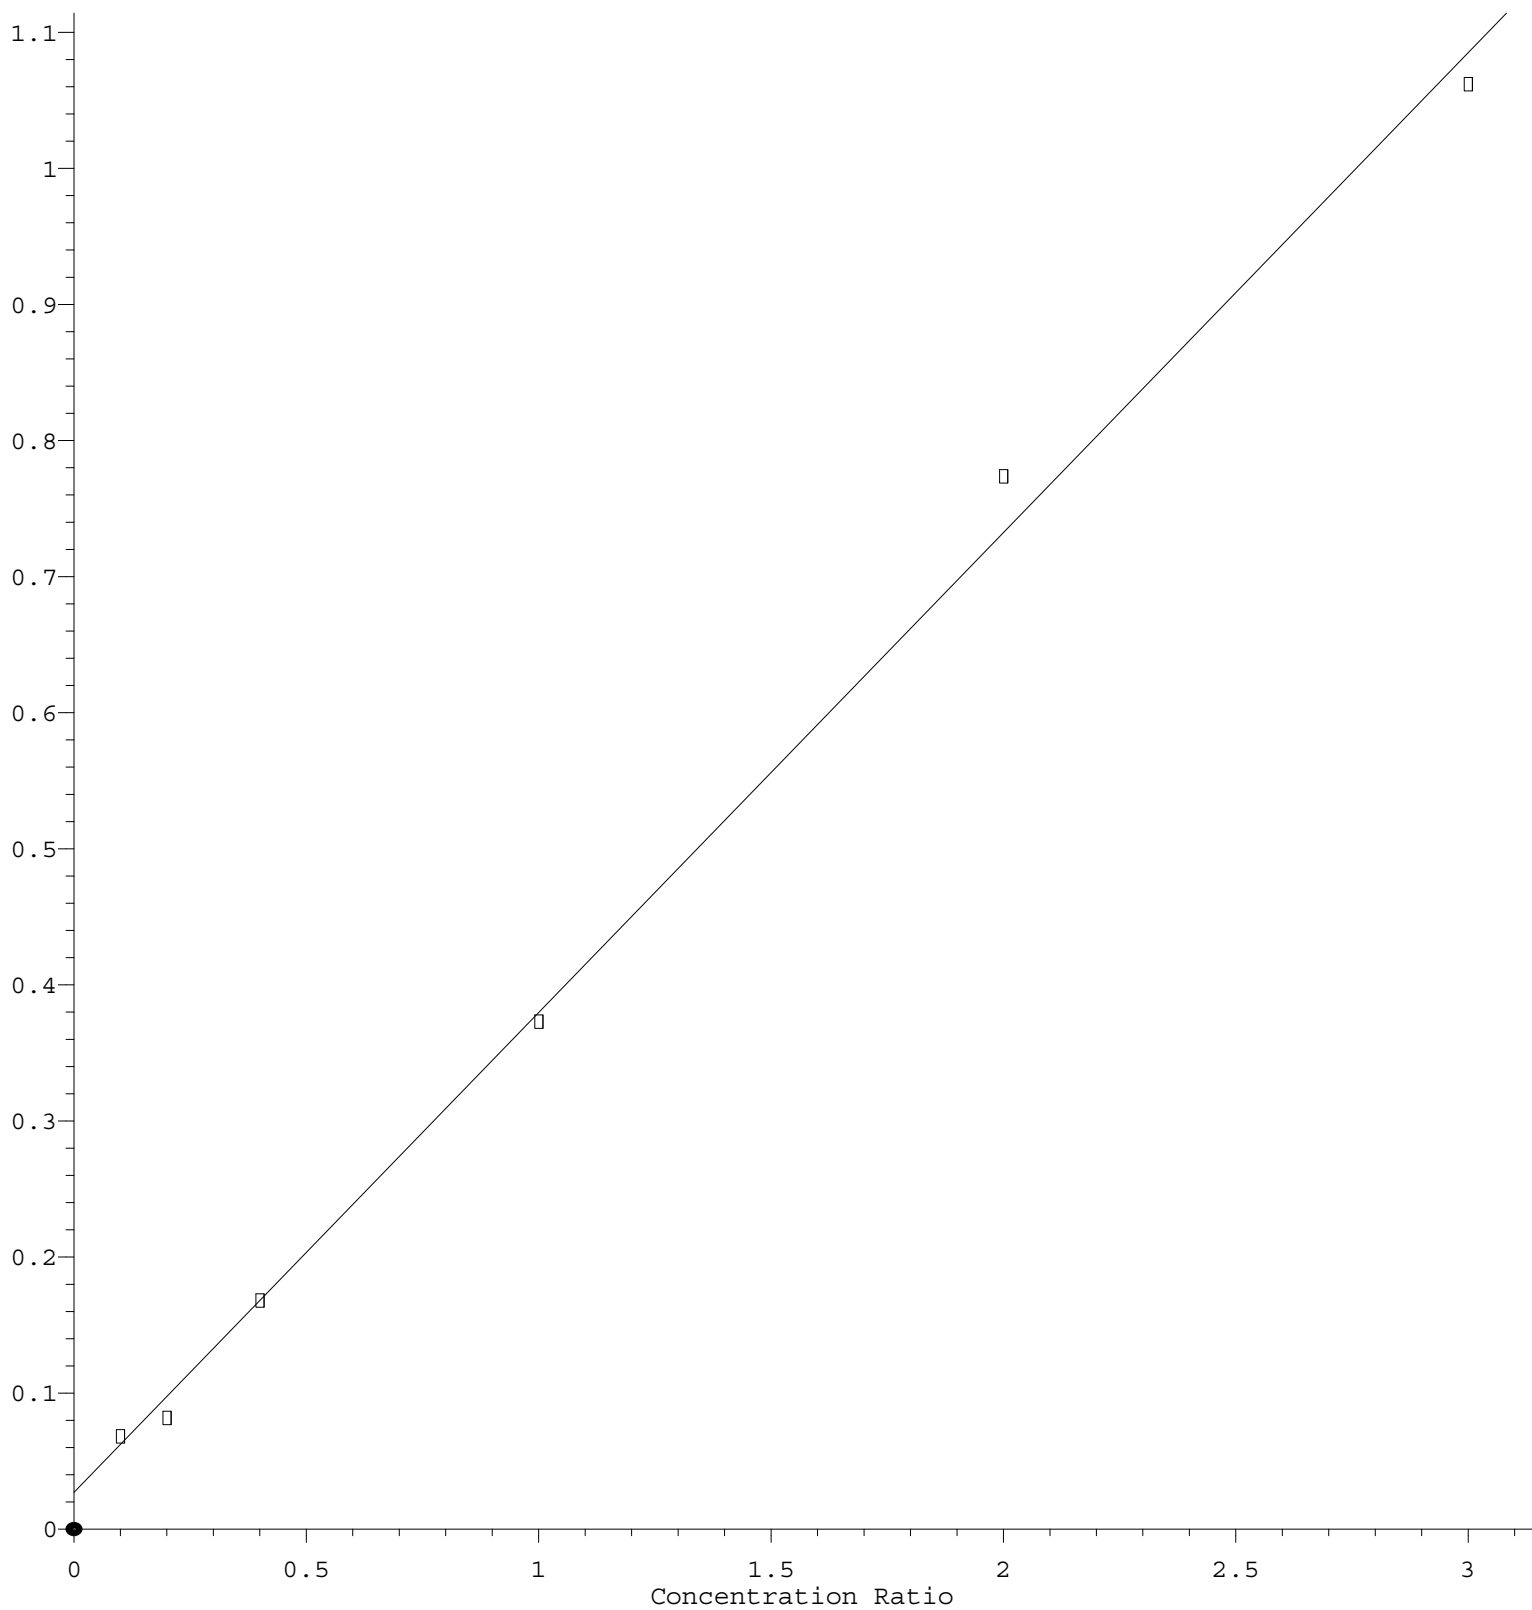

$$\text{Response} = 3.530\text{e-}001 * \text{Amt} + 2.690\text{e-}002$$


Coef of Det (r^2) = 0.996937 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y061522S.M

Calibration Table Last Updated: Thu Jun 16 02:54:06 2022

Methylene Chloride

Response Ratio

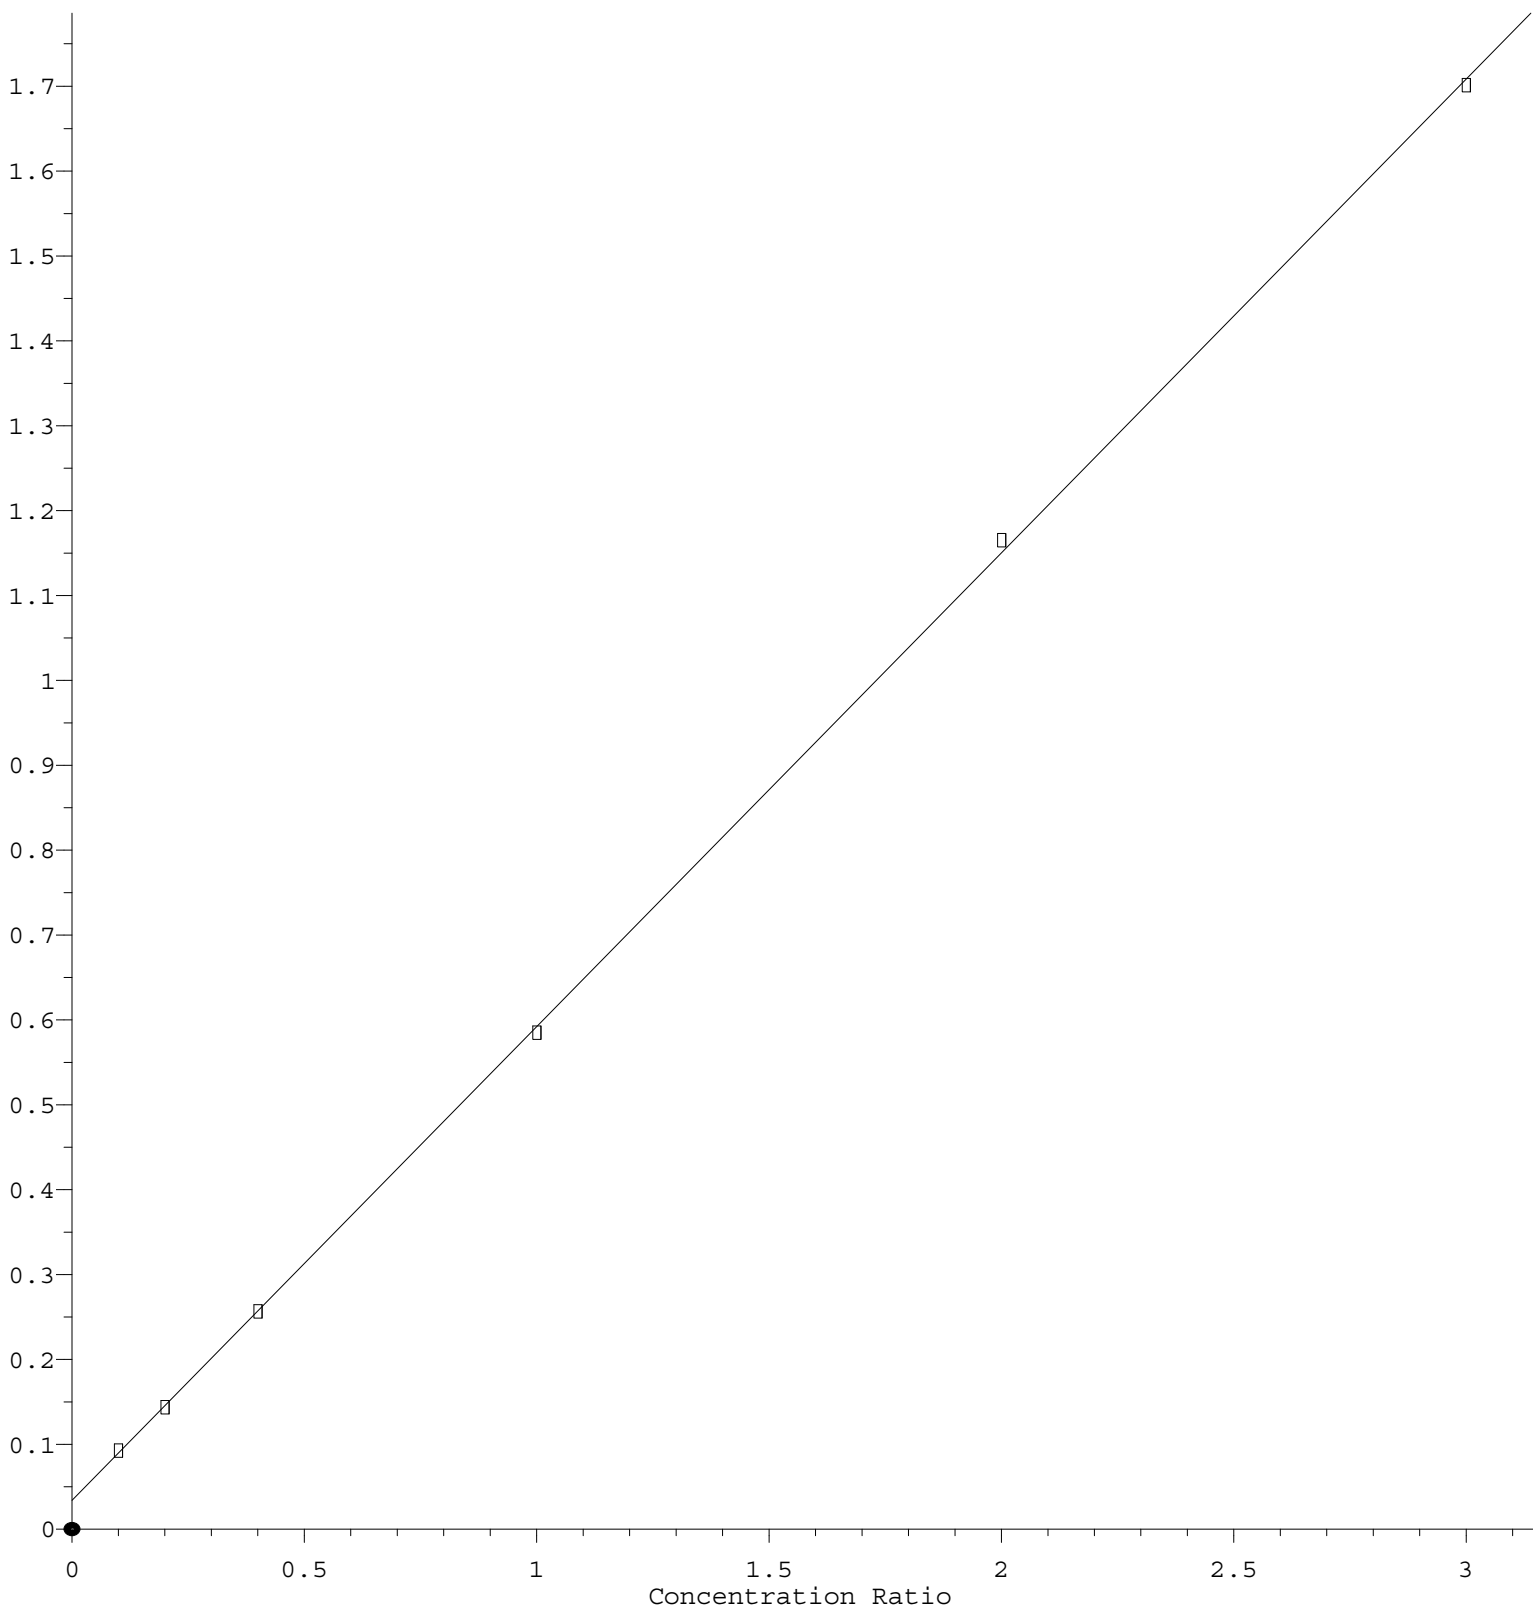

$$\text{Response} = 5.581\text{e-}001 * \text{Amt} + 3.408\text{e-}002$$

Coef of Det (r^2) = 0.999840 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y061522S.M

Calibration Table Last Updated: Thu Jun 16 02:54:06 2022