
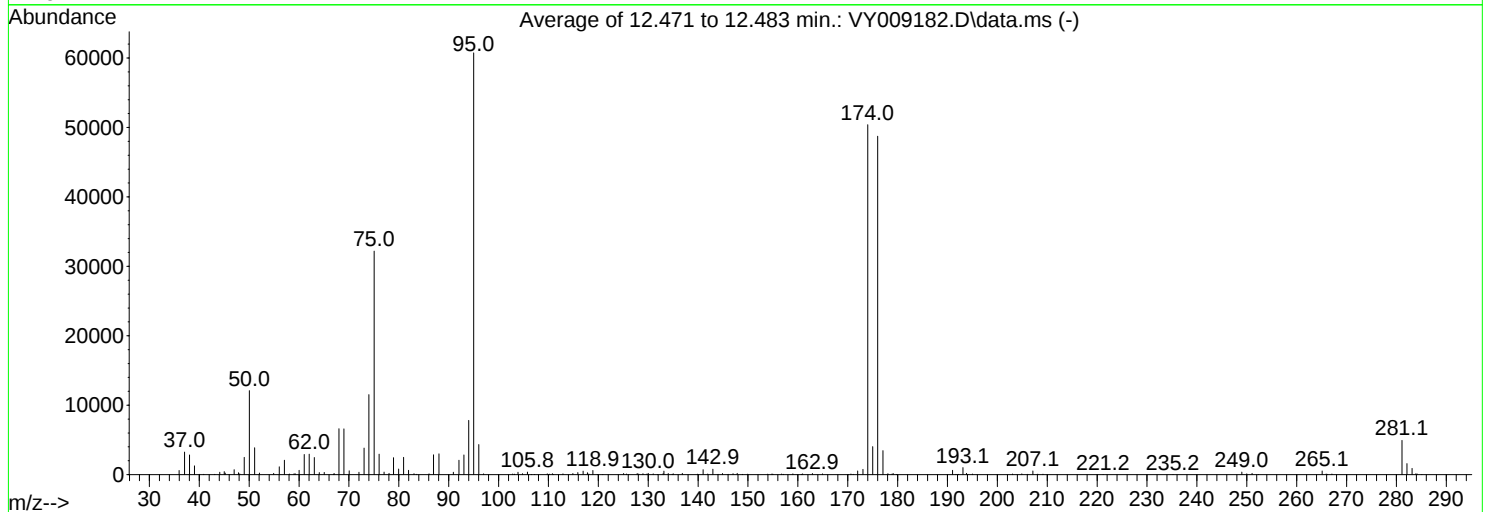


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061522\
 Data File : VY009182.D
 Acq On : 15 Jun 2022 12:24
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061522S.M
 Title : SW846 8260
 Last Update : Thu Jun 16 02:54:06 2022

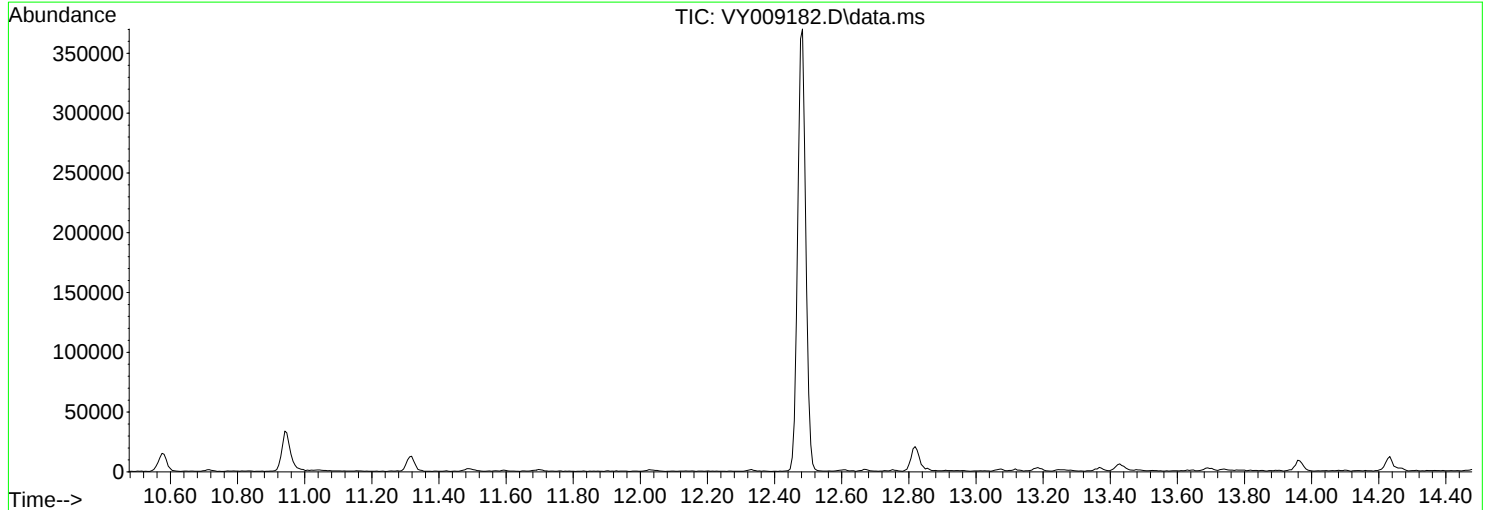

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	12108	PASS
75	95	30	60	53.0	32203	PASS
95	95	100	100	100.0	60747	PASS
96	95	5	9	7.1	4339	PASS
173	174	0.00	2	1.5	753	PASS
174	95	50	100	83.0	50395	PASS
175	174	5	9	8.0	4041	PASS
176	174	95	101	96.7	48739	PASS
177	176	5	9	7.1	3454	PASS