
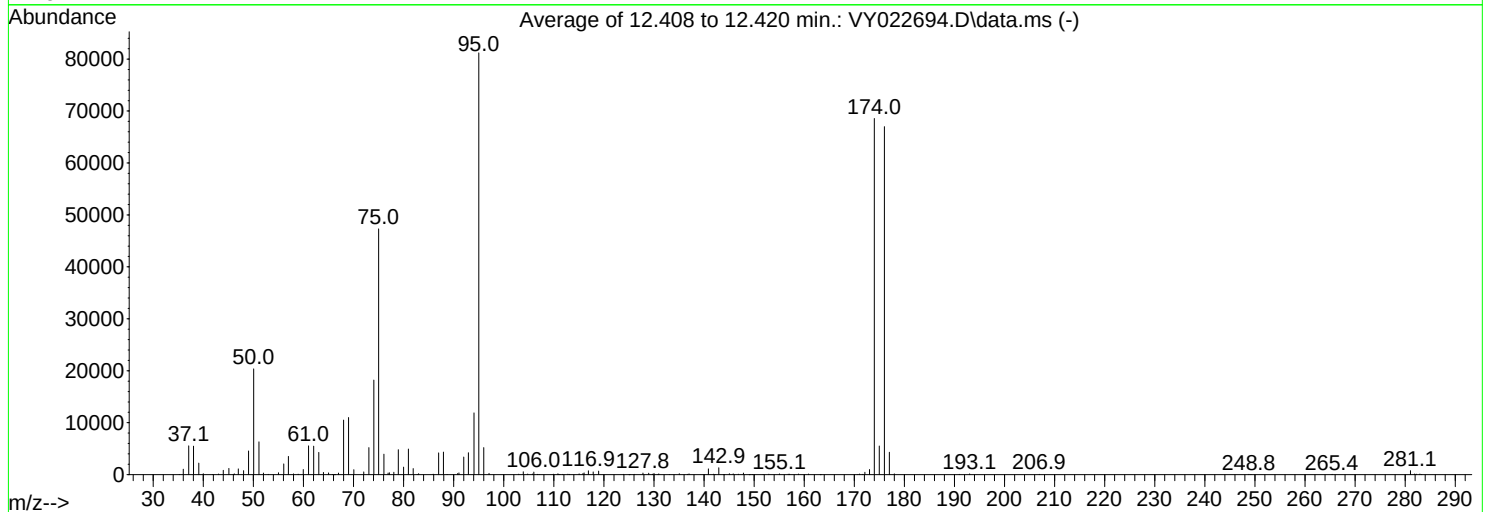


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061625\
Data File : VY022694.D
Acq On : 16 Jun 2025 07:59
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Title : SW846 8260
Last Update : Tue Jun 10 15:26:14 2025

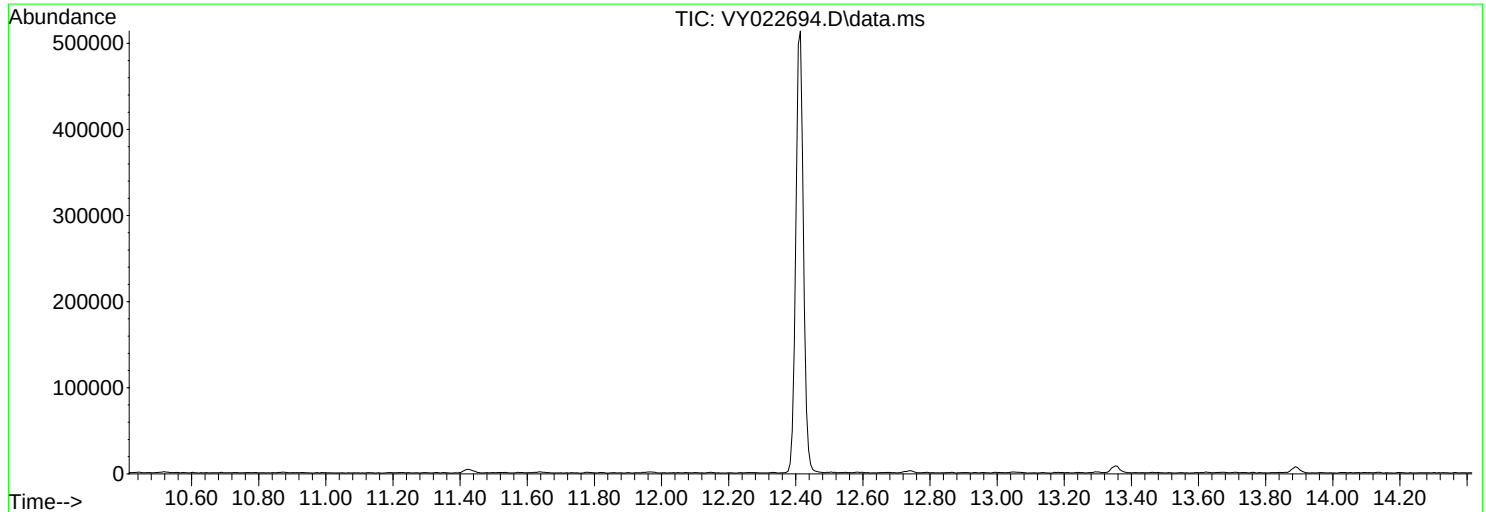

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	20367	PASS
75	95	30	60	58.3	47301	PASS
95	95	100	100	100.0	81200	PASS
96	95	5	9	6.4	5203	PASS
173	174	0.00	2	1.4	994	PASS
174	95	50	100	84.4	68565	PASS
175	174	5	9	8.0	5518	PASS
176	174	95	101	97.7	66984	PASS
177	176	5	9	6.5	4322	PASS