

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061725\
 Data File : VY022716.D
 Acq On : 17 Jun 2025 11:03
 Operator : SY/MD
 Sample : Q2324-01
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Jun 18 04:39:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 10 15:26:14 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.719	168	14795	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.622	114	21459	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	12782	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	3028	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	5165	31.213	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	62.420%
35) Dibromofluoromethane	7.646	113	5465	42.667	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	85.340%
50) Toluene-d8	10.109	98	22909	44.265	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	88.520%
62) 4-Bromofluorobenzene	12.408	95	3565	23.119	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	46.240%


Target Compounds			Qvalue			
3) Chloromethane	2.080	50	647	1.653	ug/l #	81
5) Bromomethane	2.611	94	2173	4.994	ug/l #	54
10) Methyl Iodide	4.025	142	370	2.106	ug/l #	38
11) Tert butyl alcohol	4.738	59	19	1.608	ug/l #	73
13) Acrolein	3.458	56	65	4.413	ug/l #	14
16) Acetone	3.903	43	151	4.493	ug/l #	45
25) 2-Butanone	6.896	43	49	1.011	ug/l #	46
29) Tetrahydrofuran	7.335	42	36	1.151	ug/l #	31
31) Cyclohexane	7.713	56	463	1.456	ug/l #	55
36) 1,1-Dichloropropene	7.707	75	1468	7.062	ug/l #	42
38) Carbon Tetrachloride	7.707	117	1737	8.145	ug/l #	13
59) 2-Hexanone	10.768	43	99	1.483	ug/l	68
68) m/p-Xylenes	11.627	106	203	1.021	ug/l	91
73) Isopropylbenzene	12.255	105	330	1.327	ug/l #	49
74) N-ethyl acetate	12.078	43	74	1.180	ug/l #	43
76) 1,2,3-Trichloropropane	12.536	75	85	2.454	ug/l #	100
77) Bromobenzene	12.536	156	153	2.916	ug/l #	55
78) n-propylbenzene	12.603	91	585	1.927	ug/l #	54
79) 2-Chlorotoluene	12.670	91	345	2.144	ug/l #	41
80) 1,3,5-Trimethylbenzene	12.743	105	242	1.240	ug/l #	49
81) trans-1,4-Dichloro-2-b...	12.408	75	2188	152.531	ug/l #	10
82) 4-Chlorotoluene	12.792	91	284	1.711	ug/l #	70
83) tert-Butylbenzene	12.999	119	188	1.073	ug/l #	78
85) sec-Butylbenzene	13.176	105	369	1.375	ug/l #	57
86) p-Isopropyltoluene	13.298	119	315	1.424	ug/l #	51
88) 1,4-Dichlorobenzene	13.371	146	244	2.367	ug/l #	61
89) n-Butylbenzene	13.615	91	335	1.597	ug/l #	34
91) 1,2-Dichlorobenzene	13.663	146	243	2.693	ug/l #	38
92) 1,2-Dibromo-3-Chloropr...	14.371	75	22	3.703	ug/l #	2
93) 1,2,4-Trichlorobenzene	14.919	180	283	5.750	ug/l #	42
95) Naphthalene	15.139	128	549	5.813	ug/l #	81
96) 1,2,3-Trichlorobenzene	15.334	180	120	2.845	ug/l #	37

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061725\
Data File : VY022716.D
Acq On : 17 Jun 2025 11:03
Operator : SY/MD
Sample : Q2324-01
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL/B
ALS Vial : 6 Sample Multiplier: 1





Quant Time: Jun 18 04:39:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 10 15:26:14 2025
Response via : Initial Calibration

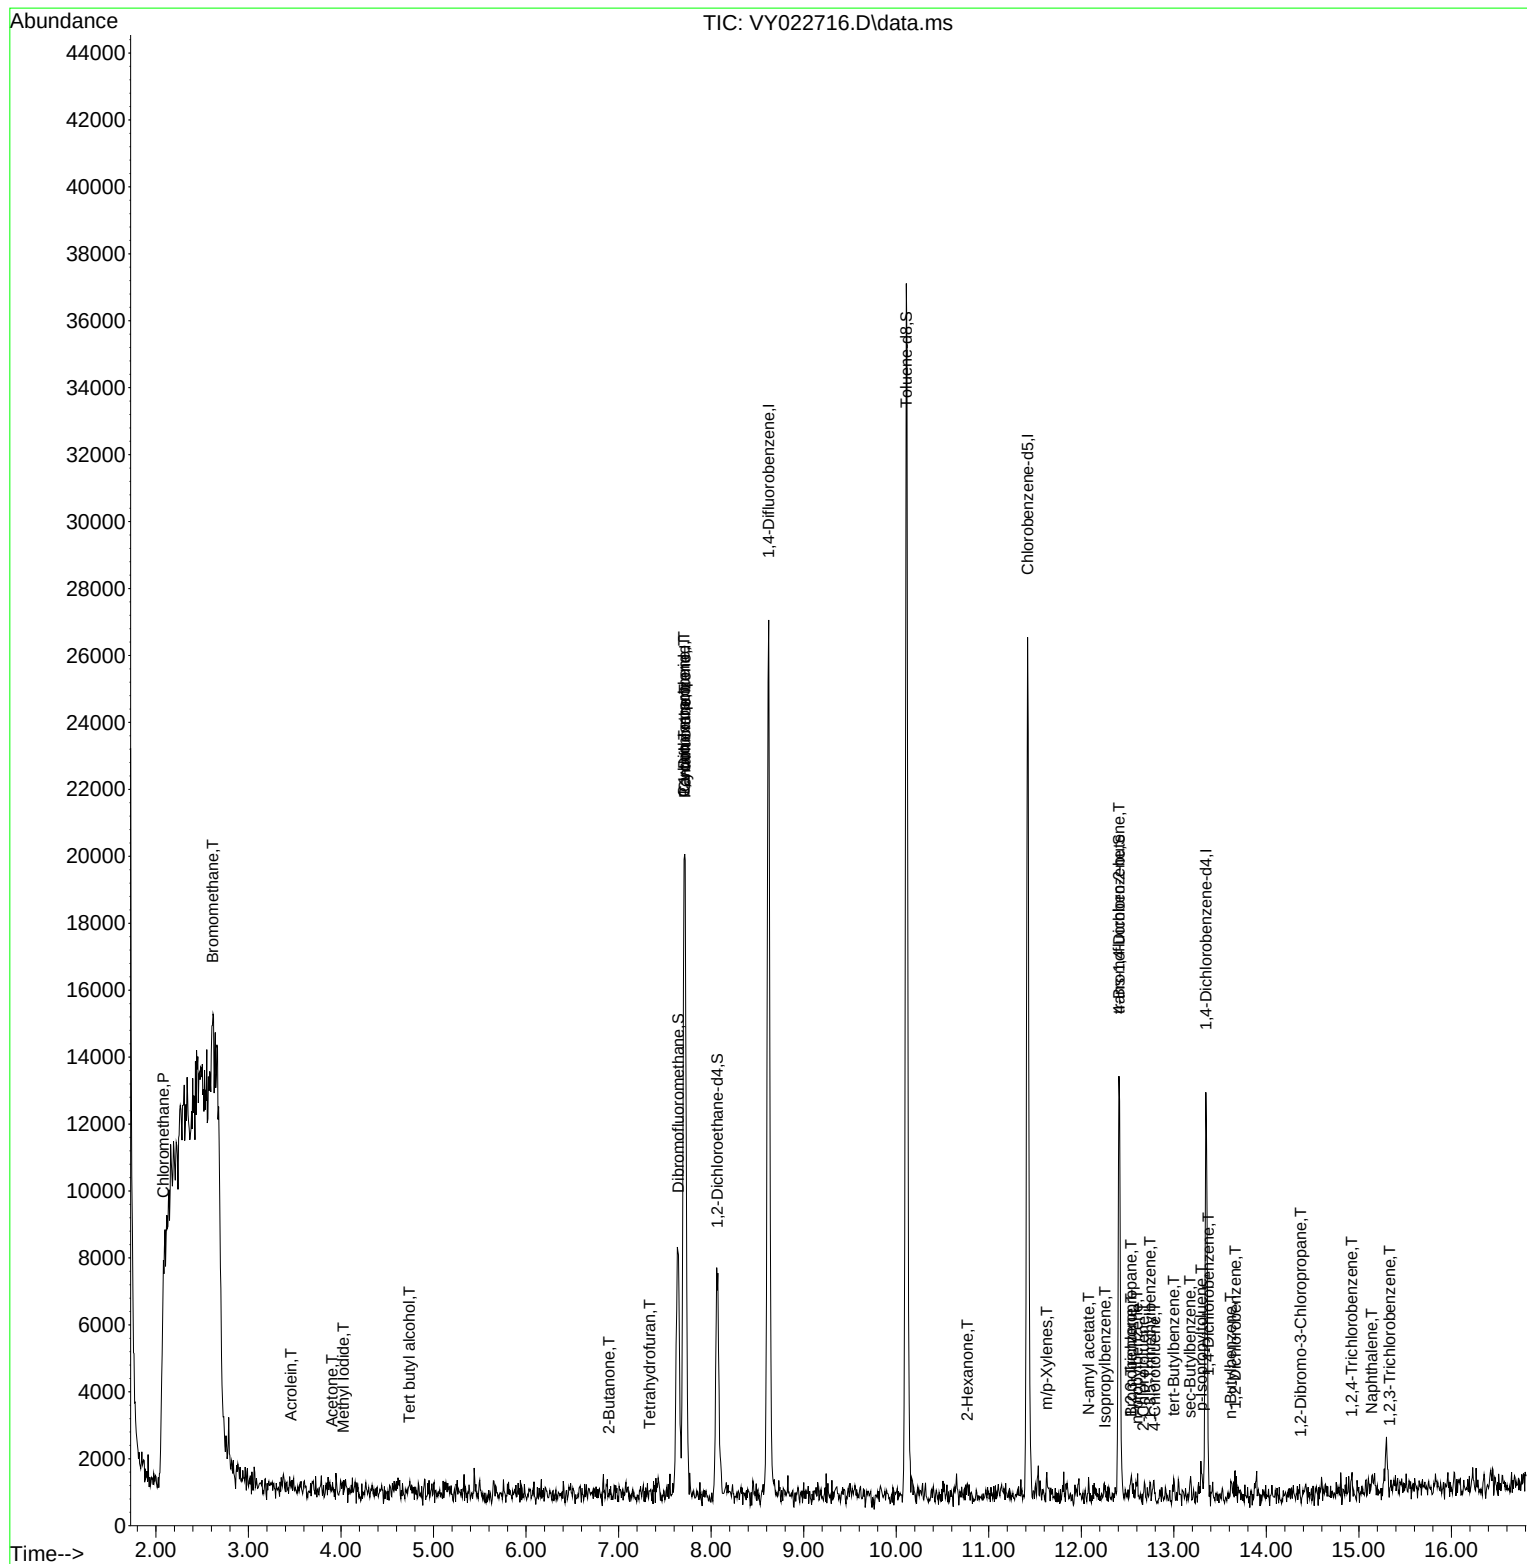






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.719 min Scan# 984
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion:168 Resp: 14795
Ion Ratio Lower Upper
168 100
99 56.6 44.3 66.5

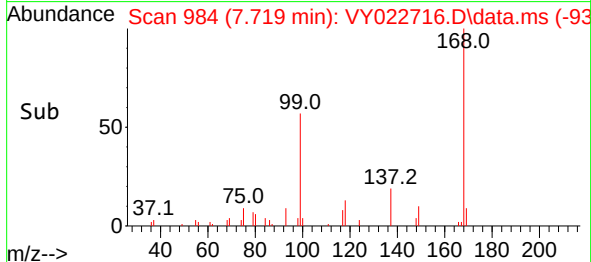

#3
Chloromethane
Concen: 1.653 ug/l
RT: 2.080 min Scan# 59
Delta R.T. 0.012 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 50 Resp: 647
Ion Ratio Lower Upper
50 100
52 42.9 26.0 39.0#

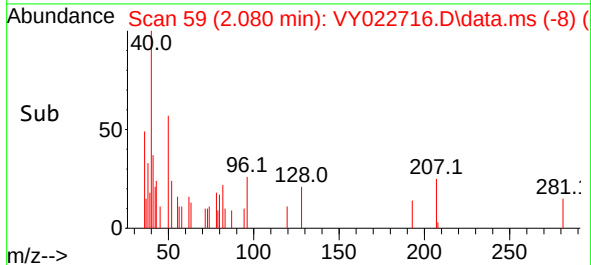






#5
Bromomethane
Concen: 4.994 ug/l
RT: 2.611 min Scan# 146
Delta R.T. 0.012 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion: 94 Resp: 2173
Ion Ratio Lower Upper
94 100
96 48.1 74.0 111.0#

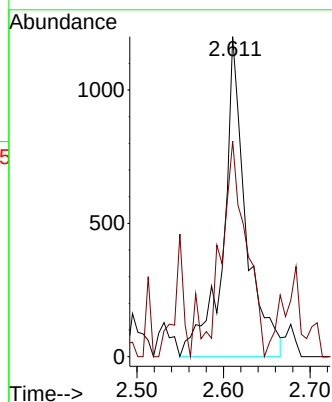

#10
Methyl Iodide
Concen: 2.106 ug/l
RT: 4.025 min Scan# 378
Delta R.T. 0.018 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion:142 Resp: 370
Ion Ratio Lower Upper
142 100
127 0.0 37.1 55.7#
141 0.0 11.4 17.2#

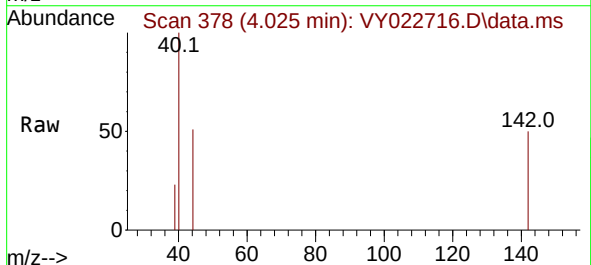






#11
Tert butyl alcohol
Concen: 1.608 ug/l
RT: 4.738 min Scan# 495
Delta R.T. -0.146 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion: 59 Resp: 19
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#



#13
Acrolein
Concen: 4.413 ug/l
RT: 3.458 min Scan# 285
Delta R.T. -0.201 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 56 Resp: 65
Ion Ratio Lower Upper
56 100
55 0.0 57.0 85.6#

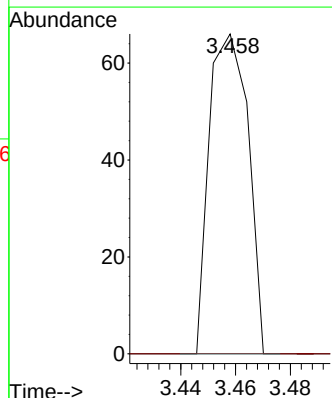






#16
Acetone
Concen: 4.493 ug/l
RT: 3.903 min Scan# 358
Delta R.T. 0.024 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion: 43 Resp: 151
Ion Ratio Lower Upper
43 100
58 0.0 24.0 36.0#

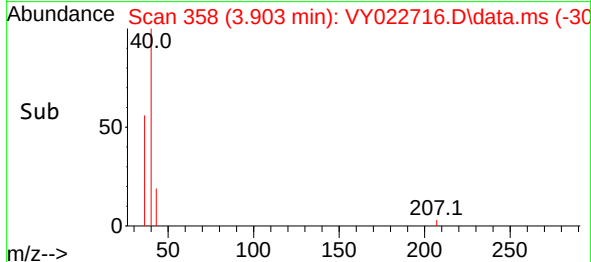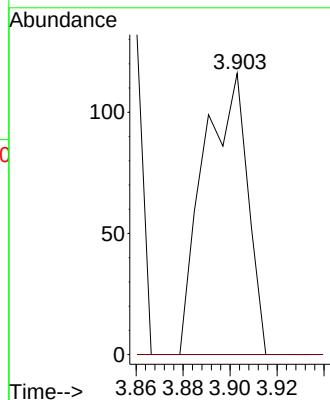

#25
2-Butanone
Concen: 1.011 ug/l
RT: 6.896 min Scan# 849
Delta R.T. -0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03

Tgt Ion: 43 Resp: 49
Ion Ratio Lower Upper
43 100
72 0.0 22.9 34.3#

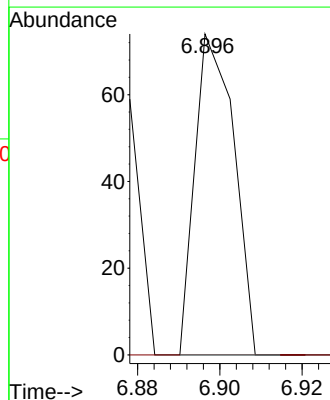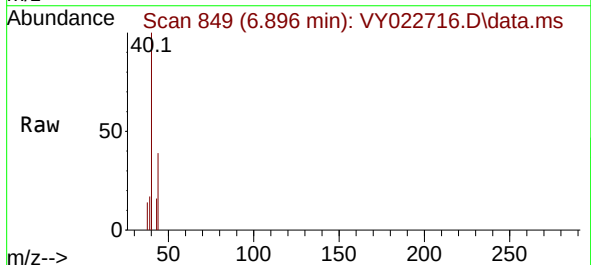

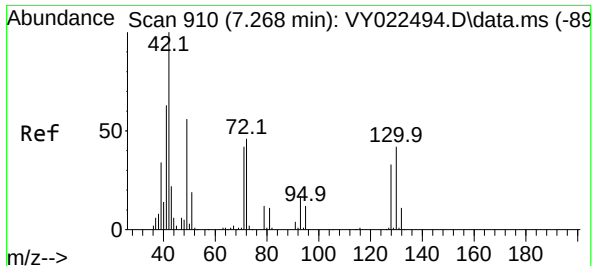

#29

Tetrahydrofuran

Concen: 1.151 ug/l





RT: 7.335 min Scan# 921

Delta R.T. 0.067 min

Lab File: VY022716.D

Acq: 17 Jun 2025 11:03

Tgt Ion: 42	Resp: 36
Ion Ratio	Lower Upper
42	100
72	0.0 37.4 56.2#
71	0.0 34.2 51.2#

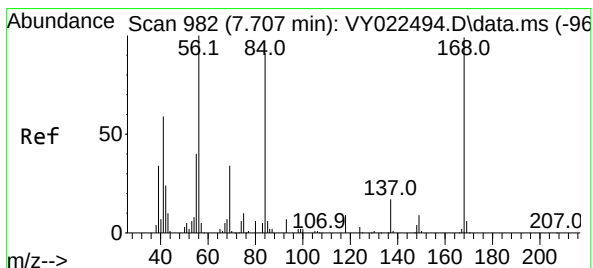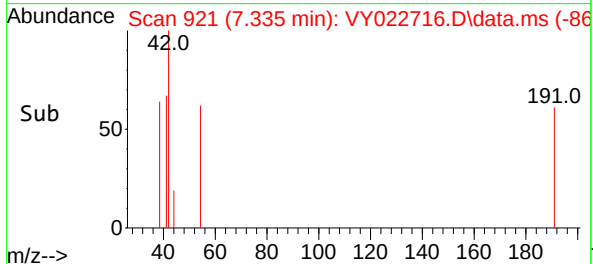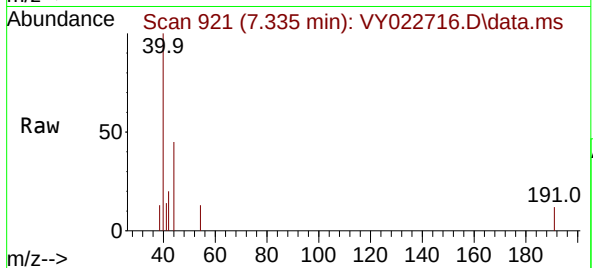

#31

Cyclohexane

Concen: 1.456 ug/l




RT: 7.713 min Scan# 983


Delta R.T. 0.006 min

Lab File: VY022716.D

Acq: 17 Jun 2025 11:03

Tgt Ion: 56	Resp: 463
Ion Ratio	Lower Upper
56	100
69	68.2 27.0 40.6#
84	53.0 72.6 109.0#

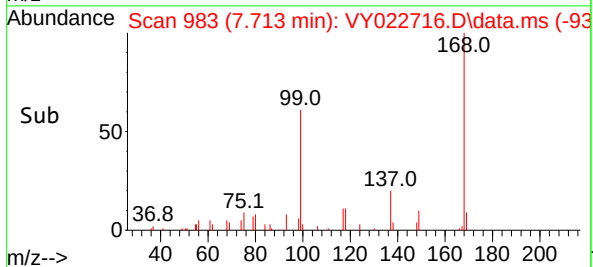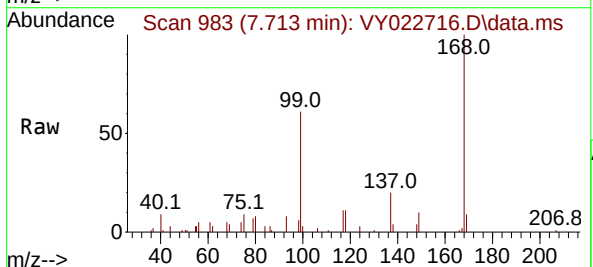



#33

1,2-Dichloroethane-d4

Concen: 31.213 ug/l

RT: 8.067 min Scan# 1041

Delta R.T. -0.000 min

Lab File: VY022716.D





Acq: 17 Jun 2025 11:03

Tgt Ion: 65 Resp: 5165

Ion Ratio Lower Upper

65 100

67 55.2 0.0 103.4

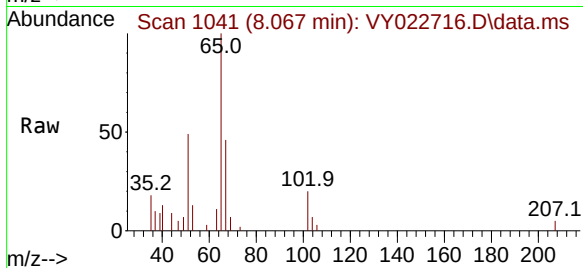

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.622 min Scan# 1132

Delta R.T. 0.006 min

Lab File: VY022716.D

Acq: 17 Jun 2025 11:03




Tgt Ion: 114 Resp: 21459


Ion Ratio Lower Upper

114 100

63 20.2 0.0 40.8





88 16.2 0.0 27.8

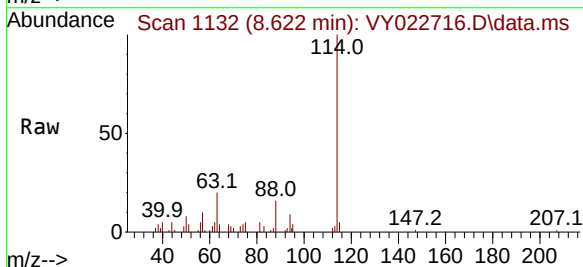

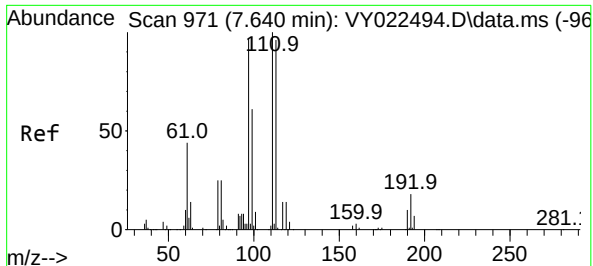




#35
Dibromofluoromethane
Concen: 42.667 ug/l
RT: 7.646 min Scan# 972
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion:	113	Resp:	5465
Ion	Ratio	Lower	Upper
113	100		
111	105.9	81.1	121.7
192	19.8	14.2	21.2

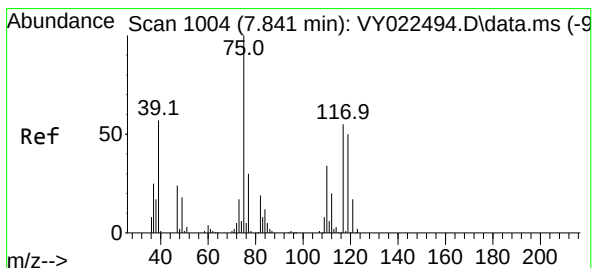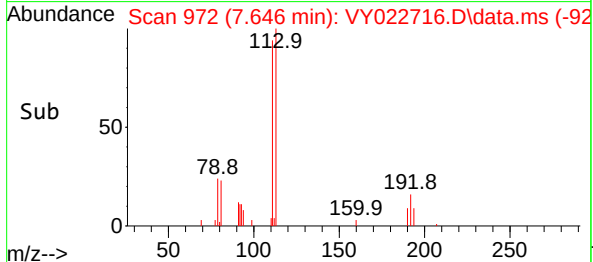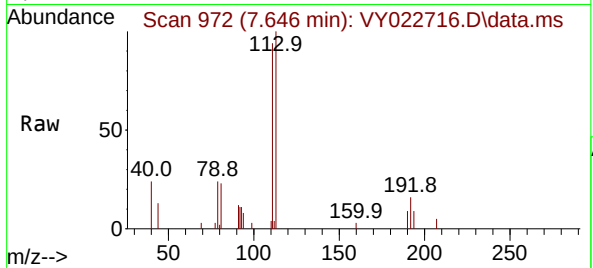

#36
1,1-Dichloropropene
Concen: 7.062 ug/l
RT: 7.707 min Scan# 982
Delta R.T. -0.134 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion:	75	Resp:	1468
Ion	Ratio	Lower	Upper
75	100		
110	0.0	16.9	50.7#
77	0.0	24.8	37.2#

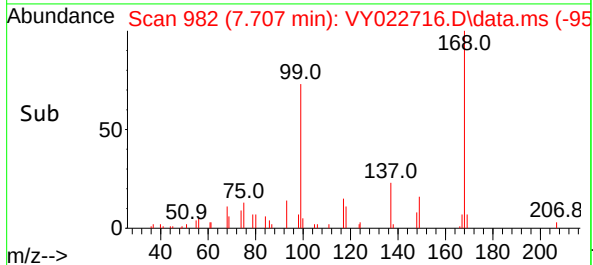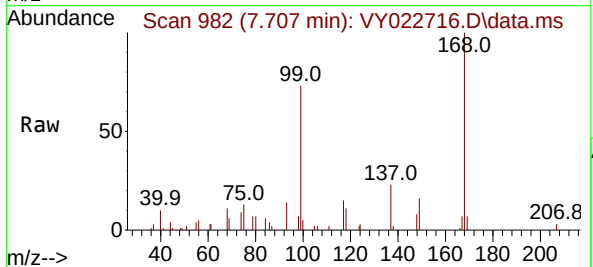






#38
Carbon Tetrachloride
Concen: 8.145 ug/l
RT: 7.707 min Scan# 982
Delta R.T. -0.116 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion:117 Resp: 1737
Ion Ratio Lower Upper
117 100
119 0.0 75.0 112.6#
121 0.0 25.0 37.4#

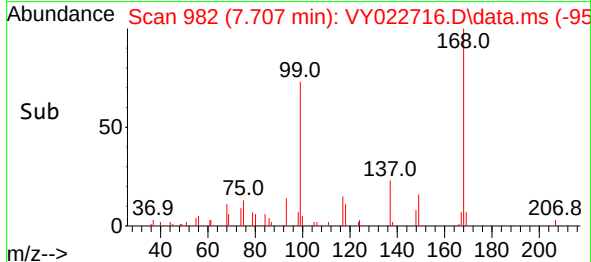

#50
Toluene-d8
Concen: 44.265 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. -0.000 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 98 Resp: 22909
Ion Ratio Lower Upper
98 100
100 65.4 51.4 77.0

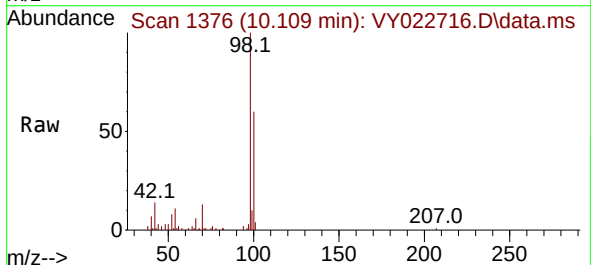






#59
2-Hexanone
Concen: 1.483 ug/l
RT: 10.768 min Scan# 1484
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion: 43 Resp: 99
Ion Ratio Lower Upper
43 100
58 77.8 27.3 81.8



#62
4-Bromofluorobenzene
Concen: 23.119 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 95 Resp: 3565
Ion Ratio Lower Upper
95 100
174 96.6 0.0 170.0
176 87.5 0.0 166.2

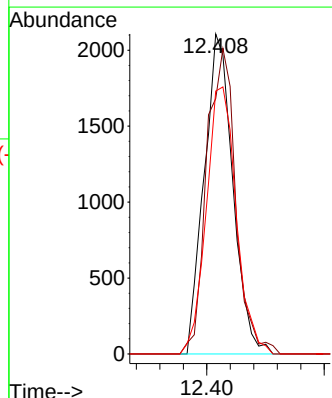






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 1591
Delta R.T. -0.000 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion:117	Resp:	12782
Ion Ratio	Lower	Upper
117	100	
82	57.5	44.6 66.8
119	27.3	25.4 38.0



#68
m/p-Xylenes
Concen: 1.021 ug/l
RT: 11.627 min Scan# 1625
Delta R.T. -0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion:106	Resp:	203
Ion Ratio	Lower	Upper
106	100	
91	213.3	159.4 239.0

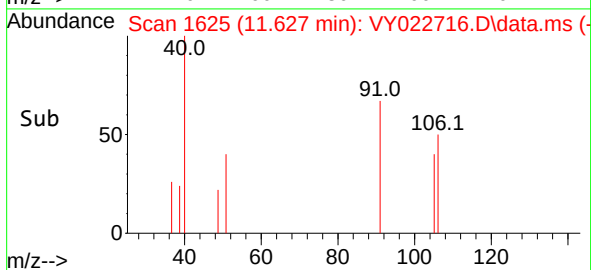






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.346 min Scan# 1907
 Delta R.T. -0.000 min
 Lab File: VY022716.D
 Acq: 17 Jun 2025 11:03


Tgt Ion:152 Resp: 3028
 Ion Ratio Lower Upper
 152 100
 115 62.7 28.9 86.7
 150 144.4 0.0 349.6

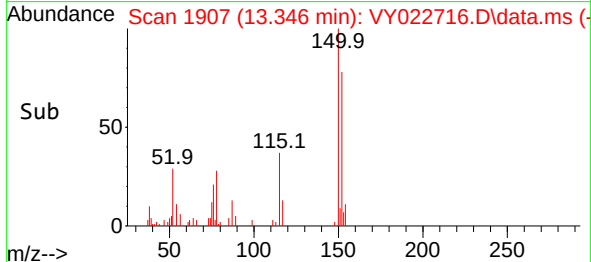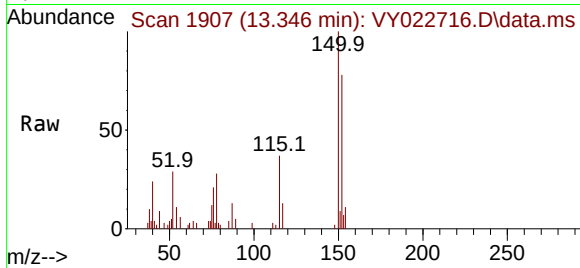

#73
 Isopropylbenzene
 Concen: 1.327 ug/l
 RT: 12.255 min Scan# 1728
 Delta R.T. -0.000 min
 Lab File: VY022716.D
 Acq: 17 Jun 2025 11:03





Tgt Ion:105 Resp: 330
 Ion Ratio Lower Upper
 105 100
 120 0.0 13.0 38.9#

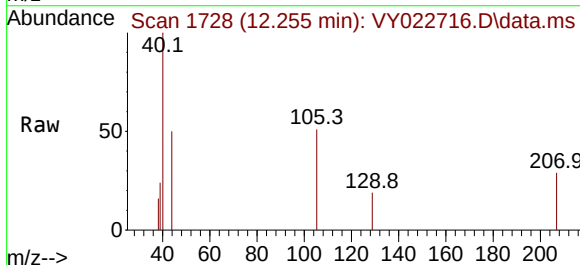






#74
N-amy1 acetate
Concen: 1.180 ug/l
RT: 12.078 min Scan# 1699
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion:	43	Resp:	74
Ion	Ratio	Lower	Upper
43	100		
70	0.0	34.2	51.2#
55	0.0	18.2	27.4#
61	0.0	19.0	28.6#

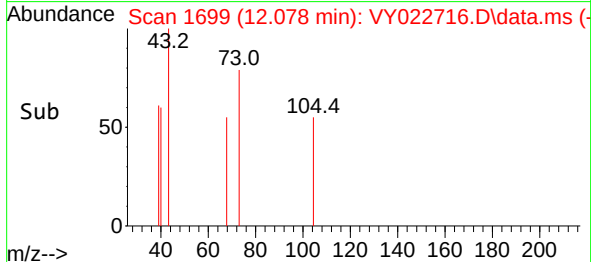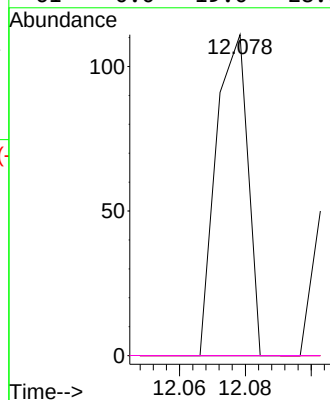

#76
1,2,3-Trichloropropane
Concen: 2.454 ug/l
RT: 12.536 min Scan# 1774
Delta R.T. -0.018 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion:	75	Resp:	85
Ion	Ratio	Lower	Upper
75	100		
77	228.2	0.0	0.0#

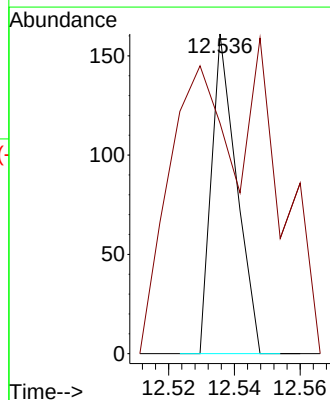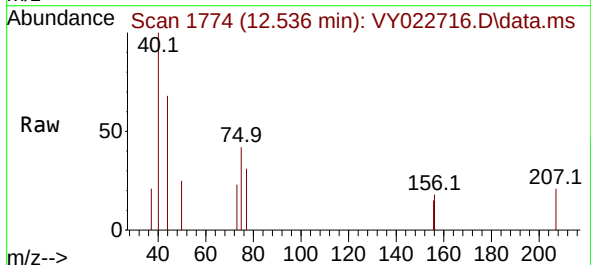






#77
Bromobenzene
Concen: 2.916 ug/l
RT: 12.536 min Scan# 1774
Delta R.T. -0.000 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion:156 Resp: 153
Ion Ratio Lower Upper
156 100
77 126.8 94.0 282.1
158 47.7 48.2 144.6#



#78
n-propylbenzene
Concen: 1.927 ug/l
RT: 12.603 min Scan# 1785
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 91 Resp: 585
Ion Ratio Lower Upper
91 100
120 0.0 10.8 32.4#

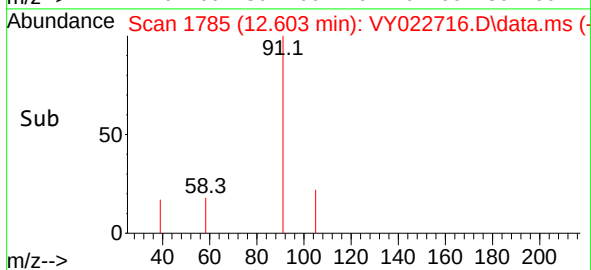






#79
2-Chlorotoluene
Concen: 2.144 ug/l
RT: 12.670 min Scan# 1796
Delta R.T. -0.012 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion: 91 Resp: 345
Ion Ratio Lower Upper
91 100
126 0.0 17.0 51.0#

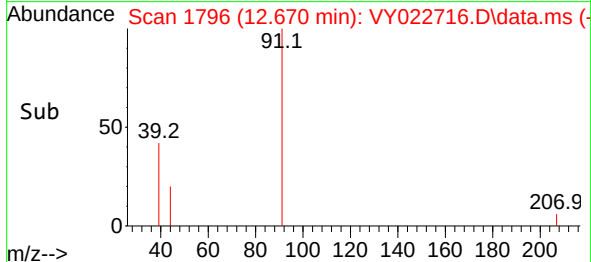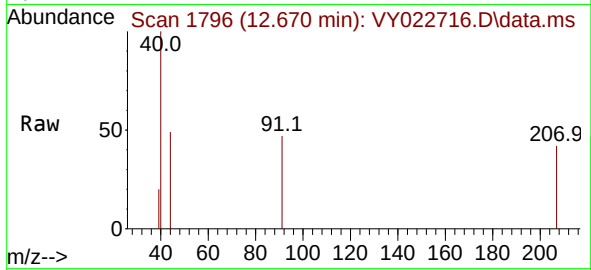

#80
1,3,5-Trimethylbenzene
Concen: 1.240 ug/l
RT: 12.743 min Scan# 1808
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 105 Resp: 242
Ion Ratio Lower Upper
105 100
120 13.6 24.1 72.4#








#81
trans-1,4-Dichloro-2-butene
Concen: 152.531 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.104 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion: 75 Resp: 2188
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.0 35.7 53.5#

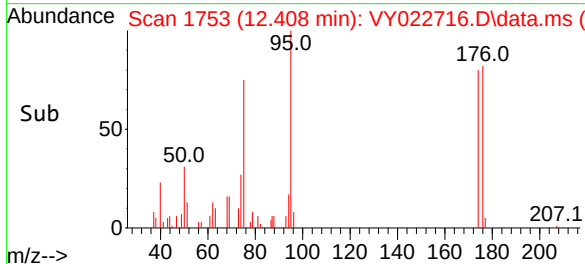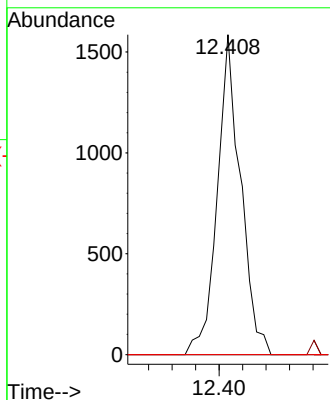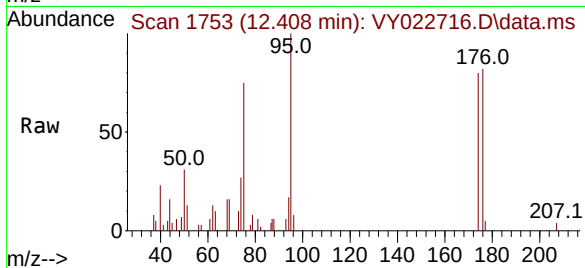

#82
4-Chlorotoluene
Concen: 1.711 ug/l
RT: 12.792 min Scan# 1816
Delta R.T. 0.012 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 91 Resp: 284
Ion Ratio Lower Upper
91 100
126 16.9 17.0 50.9#

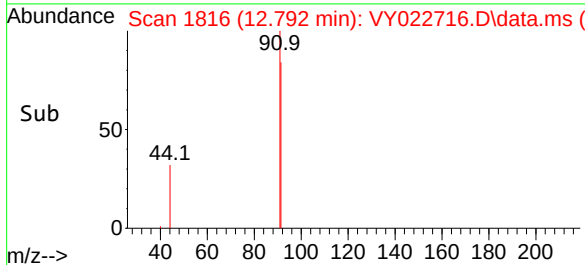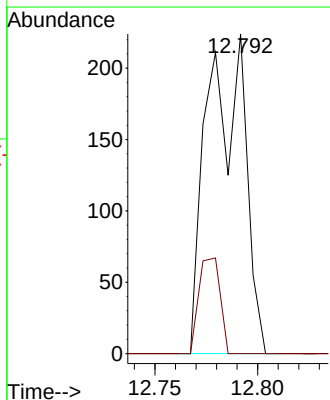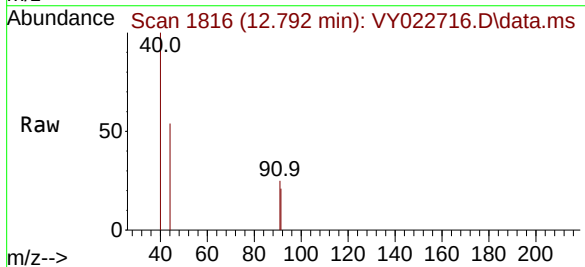






#83
tert-Butylbenzene
Concen: 1.073 ug/l
RT: 12.999 min Scan# 1850
Delta R.T. -0.000 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion	Ratio	Lower	Upper
119	100		
91	72.3	32.1	96.3
134	0.0	13.0	38.9#

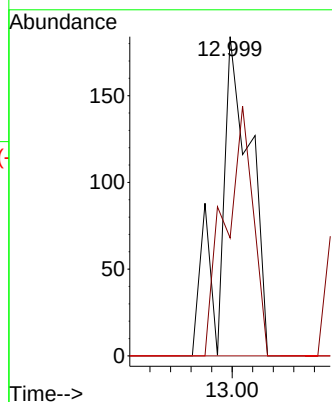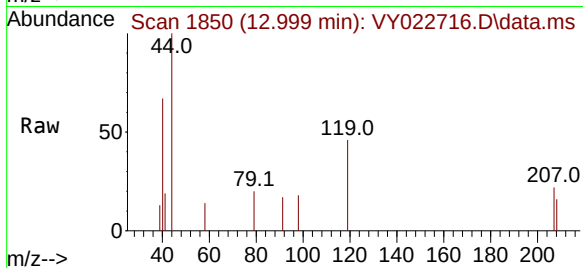

#85
sec-Butylbenzene
Concen: 1.375 ug/l
RT: 13.176 min Scan# 1879
Delta R.T. -0.000 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion	Ratio	Lower	Upper
105	100		
134	0.0	9.7	28.9#

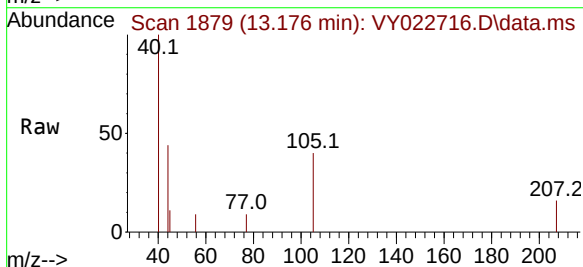






#86
p-Isopropyltoluene
Concen: 1.424 ug/l
RT: 13.298 min Scan# 1899
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion:119 Resp: 315
Ion Ratio Lower Upper
119 100
134 0.0 13.1 39.1#
91 0.0 11.6 34.8#

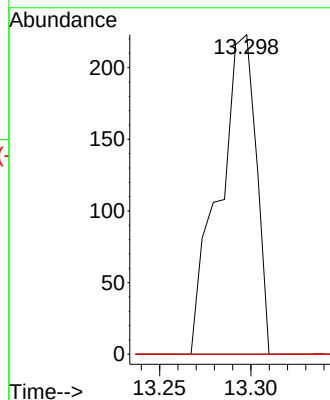

#88
1,4-Dichlorobenzene
Concen: 2.367 ug/l
RT: 13.371 min Scan# 1911
Delta R.T. -0.000 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion:146 Resp: 244
Ion Ratio Lower Upper
146 100
111 21.7 19.4 58.2
148 28.3 31.6 94.8#

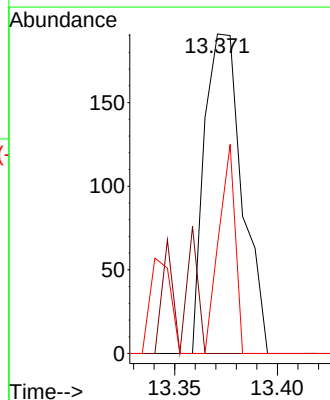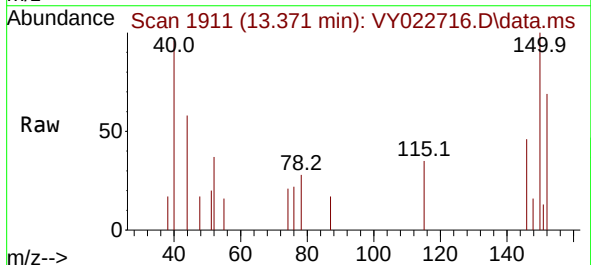






#89
n-Butylbenzene
Concen: 1.597 ug/l
RT: 13.615 min Scan# 1951
Delta R.T. -0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03


Tgt Ion: 91	Resp:	335
Ion Ratio	Lower	Upper
91	100	
92	0.0	25.9 77.8#
134	0.0	12.0 36.1#

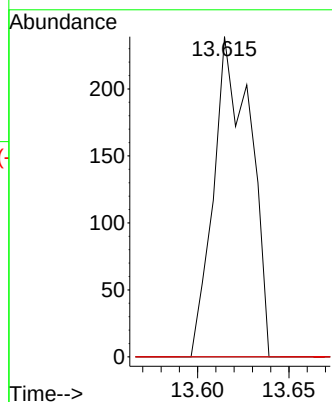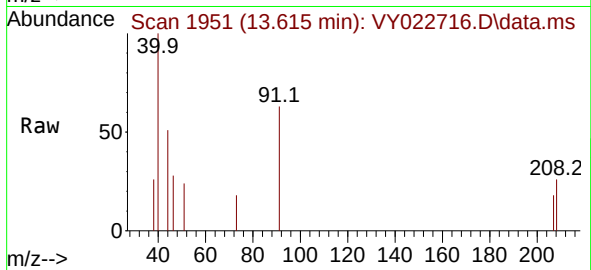

#91
1,2-Dichlorobenzene
Concen: 2.693 ug/l
RT: 13.663 min Scan# 1959
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03





Tgt Ion: 146	Resp:	243
Ion Ratio	Lower	Upper
146	100	
111	20.6	20.2 60.6
148	0.0	31.4 94.0#

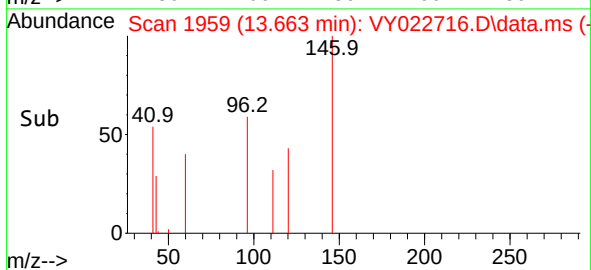






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 3.703 ug/l
 RT: 14.371 min Scan# 2075
 Delta R.T. 0.097 min
 Lab File: VY022716.D
 Acq: 17 Jun 2025 11:03


Tgt Ion: 75 Resp: 22
 Ion Ratio Lower Upper
 75 100
 155 0.0 39.9 119.6#
 157 0.0 54.0 162.0#

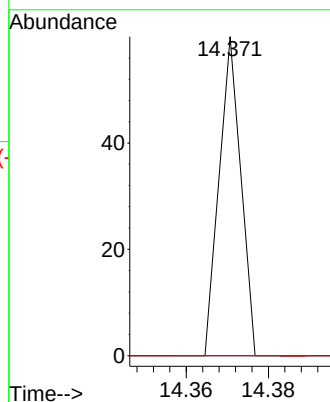

#93
 1,2,4-Trichlorobenzene
 Concen: 5.750 ug/l
 RT: 14.919 min Scan# 2165
 Delta R.T. -0.000 min
 Lab File: VY022716.D
 Acq: 17 Jun 2025 11:03





Tgt Ion: 180 Resp: 283
 Ion Ratio Lower Upper
 180 100
 182 39.6 48.4 145.3#
 145 0.0 15.5 46.5#

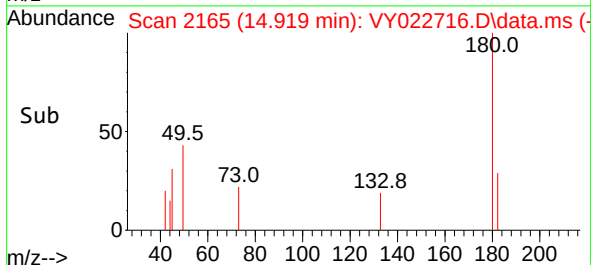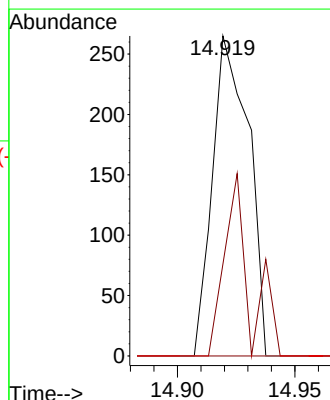



#95
Naphthalene
Concen: 5.813 ug/l
RT: 15.139 min Scan# 2201
Delta R.T. -0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03

Tgt Ion:128 Resp: 549
Ion Ratio Lower Upper
128 100
127 0.0 10.4 15.6#
129 10.2 8.9 13.3

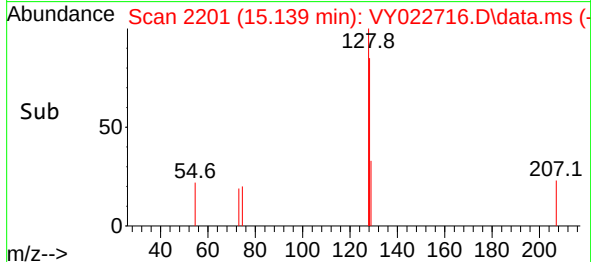

#96
1,2,3-Trichlorobenzene
Concen: 2.845 ug/l
RT: 15.334 min Scan# 2233
Delta R.T. 0.006 min
Lab File: VY022716.D
Acq: 17 Jun 2025 11:03

Tgt Ion:180 Resp: 120
Ion Ratio Lower Upper
180 100
182 31.7 47.1 141.3#
145 0.0 15.2 45.6#

