

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062123\
 Data File : VY014340.D
 Acq On : 21 Jun 2023 16:55
 Operator : KP/MD
 Sample : 03357-04
 Misc : 4.50g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-SCAN-01-G

Quant Time: Jun 22 01:57:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 09 18:07:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	35102	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	51690	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	47516	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	22312	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	23757	48.603	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	97.200%
35) Dibromofluoromethane	7.710	113	18409	50.219	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.440%
50) Toluene-d8	10.179	98	60623	44.235	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	88.480%
62) 4-Bromofluorobenzene	12.483	95	19542	40.141	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	80.280%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.954	59	330	Below Cal	#	89
16) Acetone	3.942	43	4612	31.302	ug/l	95
20) Methylene Chloride	4.716	84	6628	11.317	ug/l #	90
25) 2-Butanone	6.972	43	954	5.260	ug/l #	49
31) Cyclohexane	7.777	56	943	1.440	ug/l #	58
36) 1,1-Dichloropropene	7.789	75	2416	4.228	ug/l #	49
37) Ethyl Acetate	6.972	43	954	2.419	ug/l #	1
38) Carbon Tetrachloride	7.783	117	3547	5.378	ug/l #	12
52) Toluene	10.252	92	1162	1.103	ug/l #	74
55) 1,1,2-Trichloroethane	10.611	97	517	1.467	ug/l #	14
59) 2-Hexanone	10.800	43	313	1.154	ug/l #	27
67) Ethyl Benzene	11.599	91	4816	2.410	ug/l	96
68) m/p-Xylenes	11.697	106	7546	9.817	ug/l	97
69) o-Xylene	12.032	106	4534	6.239	ug/l	94
73) Isopropylbenzene	12.331	105	1857	1.091	ug/l	98
74) N-amyl acetate	12.130	43	998	1.850	ug/l #	76
76) 1,2,3-Trichloropropane	12.483	75	10828	36.990	ug/l #	100
78) n-propylbenzene	12.672	91	5562	2.675	ug/l	85
79) 2-Chlorotoluene	12.733	91	2401	2.007	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.812	105	8517	5.844	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.483	75	10828	79.958	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.123	105	29272	20.290	ug/l	97
85) sec-Butylbenzene	13.251	105	2830	1.572	ug/l	83
86) p-Isopropyltoluene	13.373	119	2017	1.309	ug/l	89
89) n-Butylbenzene	13.696	91	3066	2.145	ug/l #	72
90) Hexachloroethane	13.965	117	1757	5.722	ug/l #	8
92) 1,2-Dibromo-3-Chloropr...	14.336	75	121	1.671	ug/l #	3
95) Naphthalene	15.233	128	6638	6.729	ug/l #	87
96) 1,2,3-Trichlorobenzene	15.446	180	593	1.350	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062123\
Data File : VY014340.D
Acq On : 21 Jun 2023 16:55
Operator : KP/MD
Sample : 03357-04
Misc : 4.50g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G

Quant Time: Jun 22 01:57:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 09 18:07:13 2023
Response via : Initial Calibration




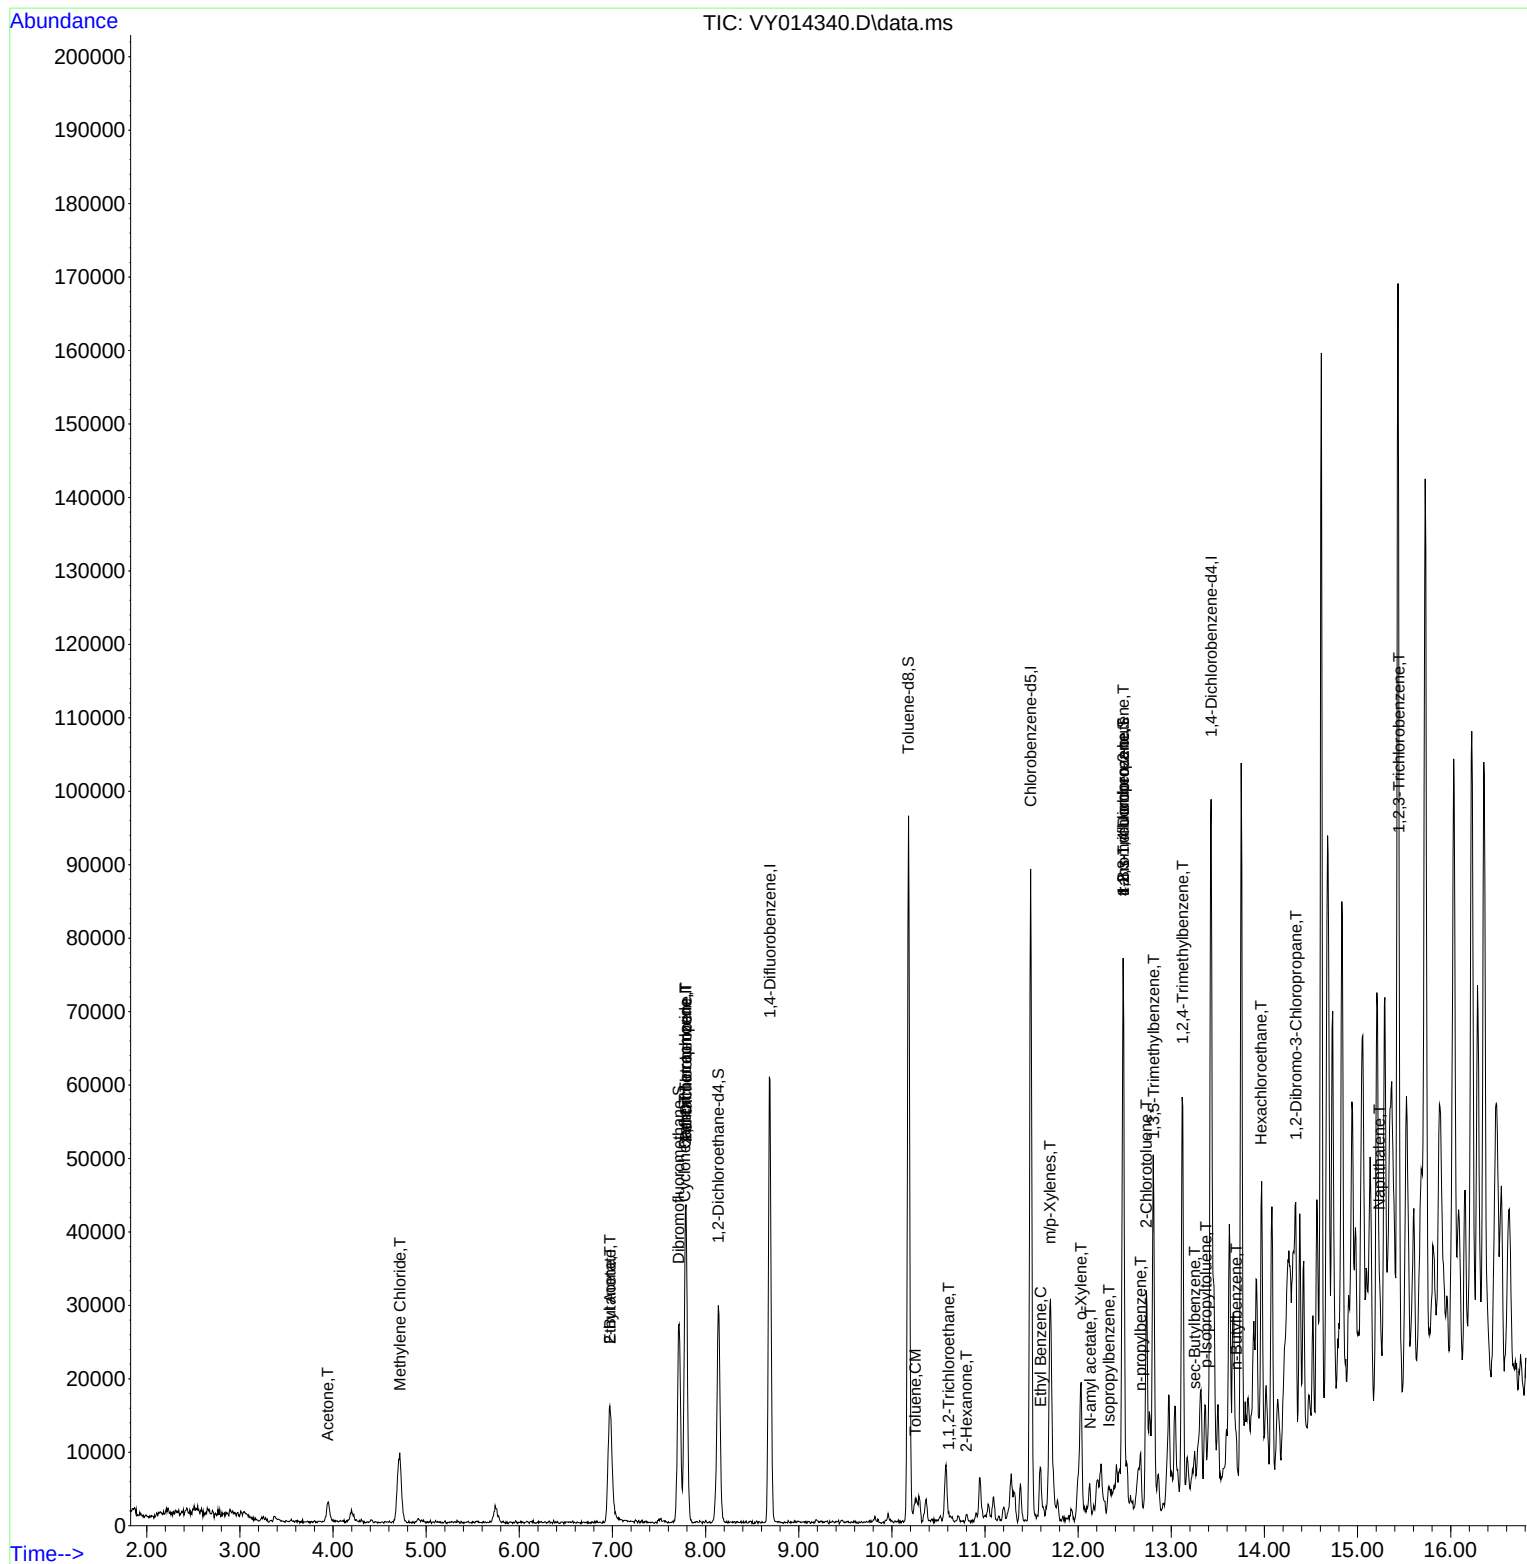


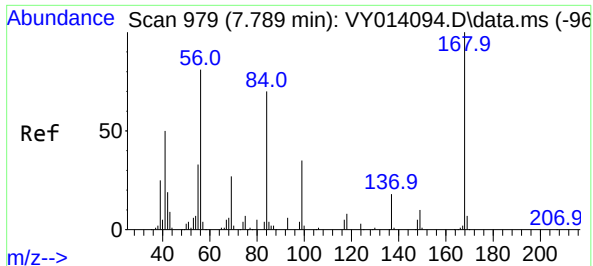

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion:168 Resp: 35102
Ion Ratio Lower Upper
168 100
99 54.9 43.4 65.0

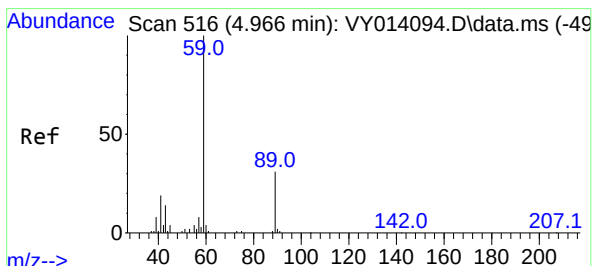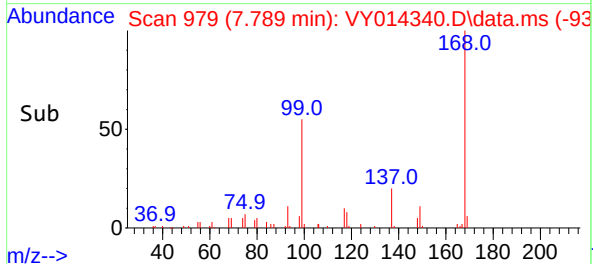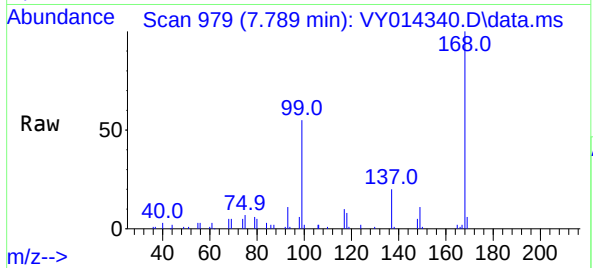

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.954 min Scan# 514
Delta R.T. -0.012 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 59 Resp: 330
Ion Ratio Lower Upper
59 100
57 0.0 3.0 4.4#


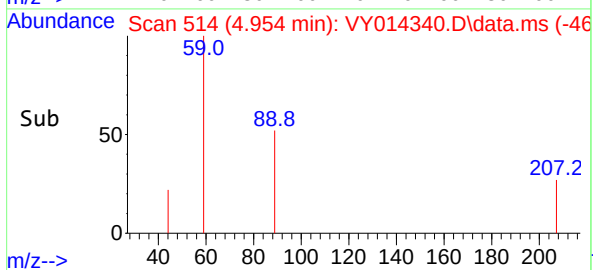

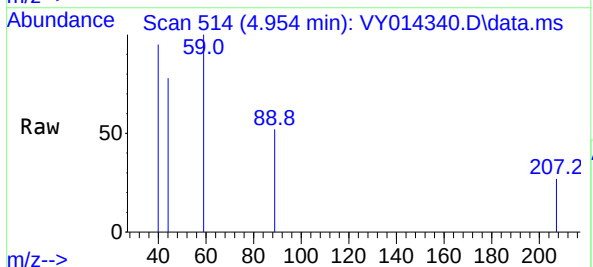




#16
Acetone
Concen: 31.302 ug/l
RT: 3.942 min Scan# 34
Delta R.T. -0.012 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 43 Resp: 4612
Ion Ratio Lower Upper
43 100
58 25.5 22.7 34.1



#20
Methylene Chloride
Concen: 11.317 ug/l
RT: 4.716 min Scan# 475
Delta R.T. 0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 84 Resp: 6628
Ion Ratio Lower Upper
84 100
49 119.2 106.9 160.3
51 31.5 33.2 49.8#
86 63.6 51.0 76.6


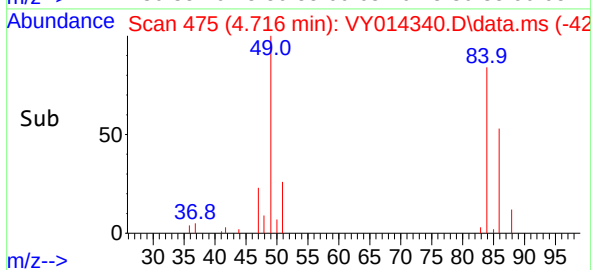






#25
2-Butanone
Concen: 5.260 ug/l
RT: 6.972 min Scan# 84
Delta R.T. -0.018 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 43 Resp: 954
Ion Ratio Lower Upper
43 100
72 0.0 20.5 30.7#

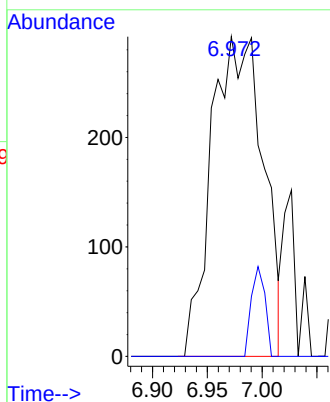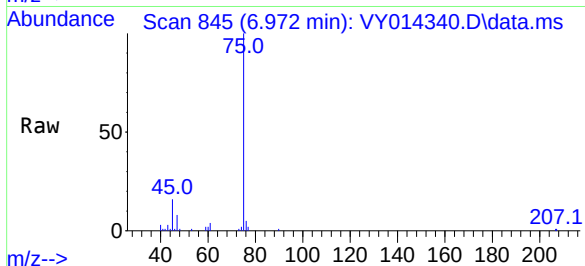

#31
Cyclohexane
Concen: 1.440 ug/l
RT: 7.777 min Scan# 977
Delta R.T. -0.012 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 56 Resp: 943
Ion Ratio Lower Upper
56 100
69 111.9 27.8 41.6#
84 79.5 66.4 99.6

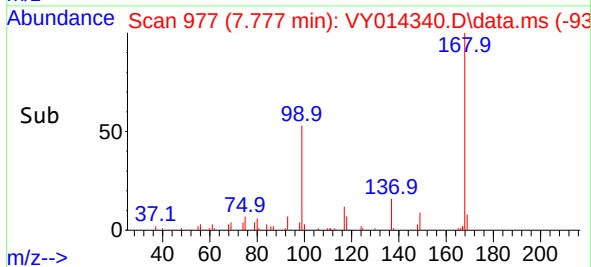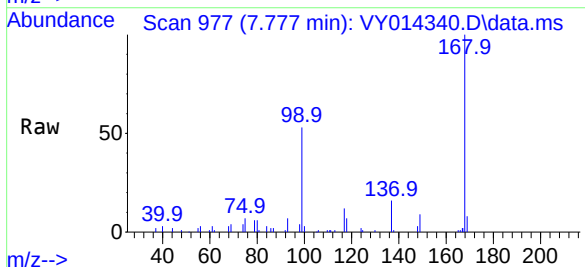

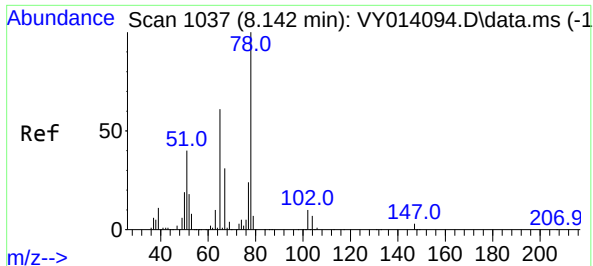

#33

1,2-Dichloroethane-d4

Concen: 48.603 ug/l

RT: 8.136 min Scan# 1036

Delta R.T. -0.006 min

Lab File: VY014340.D

Acq: 21 Jun 2023 16:55

Instrument :

MSVOA_Y

ClientSampleId :





WC-SCAN-01-G

Tgt Ion: 65 Resp: 23757

Ion Ratio Lower Upper

65 100

67 52.1 0.0 101.8

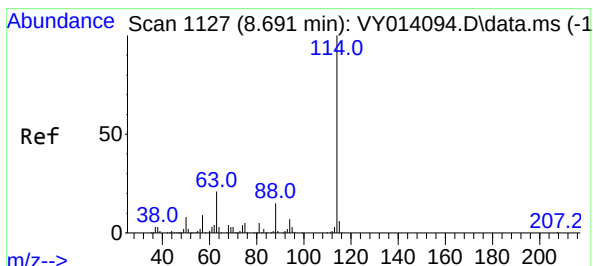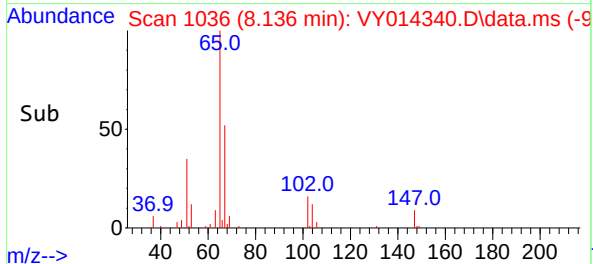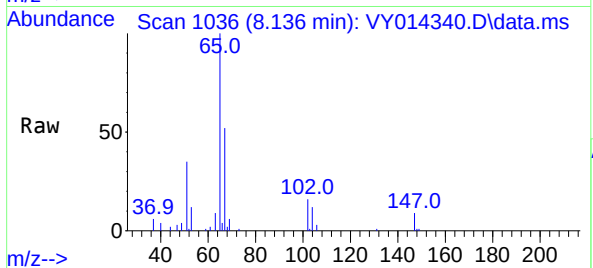

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY014340.D

Acq: 21 Jun 2023 16:55




Tgt Ion: 114 Resp: 51690


Ion Ratio Lower Upper

114 100

63 19.3 0.0 42.4

88 14.6 0.0 30.6


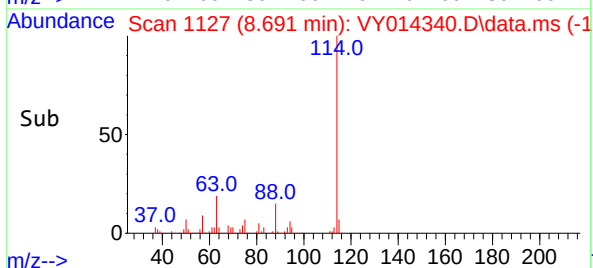
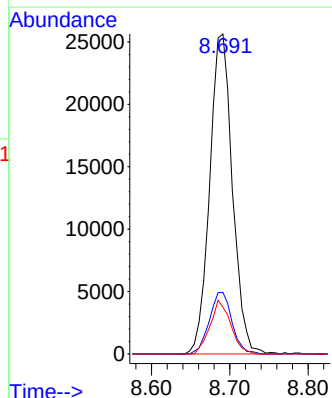
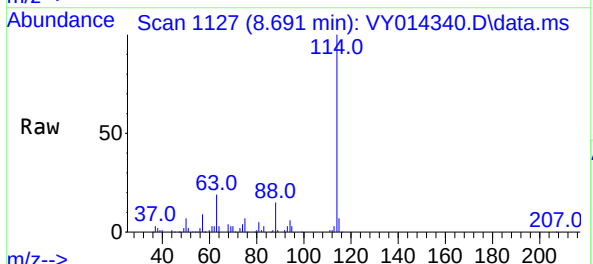




#35
Dibromofluoromethane
Concen: 50.219 ug/l
RT: 7.710 min Scan# 911
Delta R.T. -0.006 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion:113 Resp: 18409
Ion Ratio Lower Upper
113 100
111 102.1 81.3 121.9
192 22.3 16.9 25.3

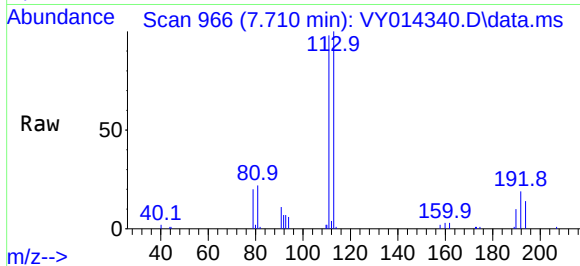

#36
1,1-Dichloropropene
Concen: 4.228 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.134 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 75 Resp: 2416
Ion Ratio Lower Upper
75 100
110 8.7 17.8 53.5#
77 0.0 24.4 36.6#

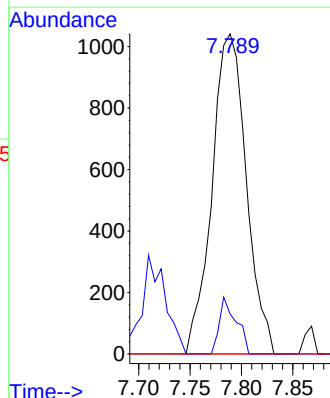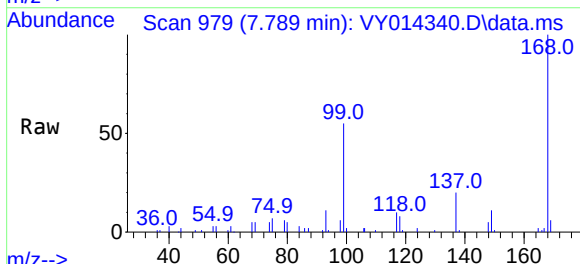



#37

Ethyl Acetate

Concen: 2.419 ug/l

RT: 6.972 min Scan# 84

Delta R.T. -0.103 min

Lab File: VY014340.D


Acq: 21 Jun 2023 16:55

Instrument :

MSVOA_Y

ClientSampleId :

WC-SCAN-01-G






Tgt Ion: 43 Resp: 954

Ion Ratio Lower Upper

43 100

61 99.9 10.1 15.1#

70 0.0 7.1 10.7#

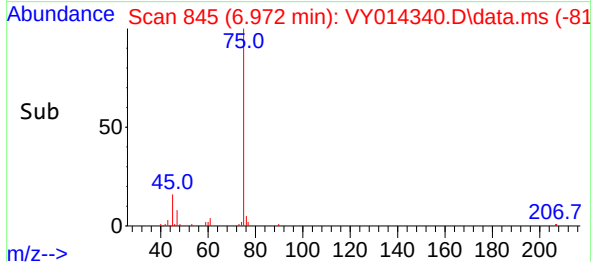

#38

Carbon Tetrachloride

Concen: 5.378 ug/l

RT: 7.783 min Scan# 978

Delta R.T. -0.115 min

Lab File: VY014340.D

Acq: 21 Jun 2023 16:55




Tgt Ion: 117 Resp: 3547


Ion Ratio Lower Upper

117 100

119 0.0 76.4 114.6#

121 0.0 25.8 38.6#


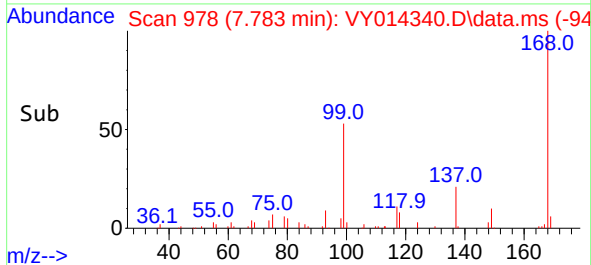
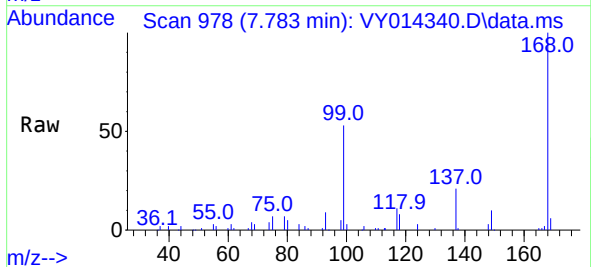





#50
Toluene-d8
Concen: 44.235 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.001 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 98 Resp: 60623
Ion Ratio Lower Upper
98 100
100 63.4 50.1 75.1

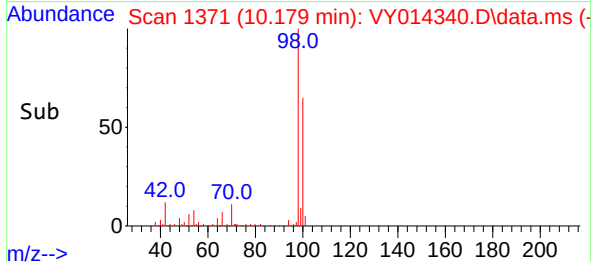

#52
Toluene
Concen: 1.103 ug/l
RT: 10.252 min Scan# 1383
Delta R.T. 0.006 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 92 Resp: 1162
Ion Ratio Lower Upper
92 100
91 142.3 143.8 215.6#


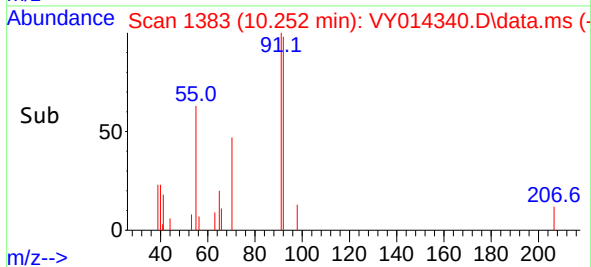

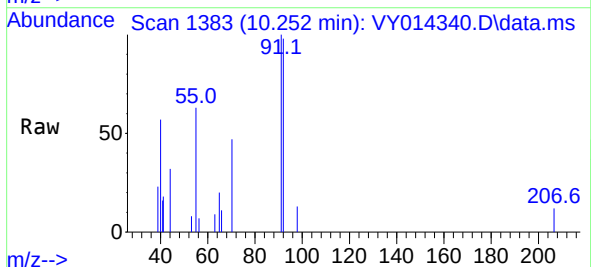




#55
1,1,2-Trichloroethane
Concen: 1.467 ug/l
RT: 10.611 min Scan# 1442
Delta R.T. -0.037 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 97	Resp: 517
Ion Ratio	Lower Upper
97 100	
83 0.0	72.0 108.0#
85 0.0	45.4 68.0#
99 0.0	50.3 75.5#

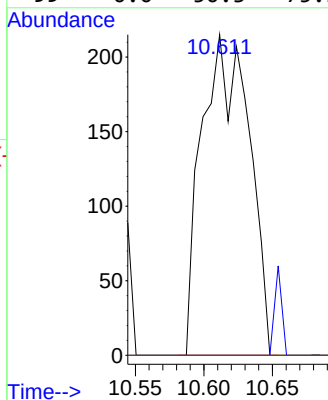

#59
2-Hexanone
Concen: 1.154 ug/l
RT: 10.800 min Scan# 1473
Delta R.T. -0.031 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 43	Resp: 313		
Ion Ratio	Lower	Upper	
43 100			
58 0.0	25.1	75.3#	


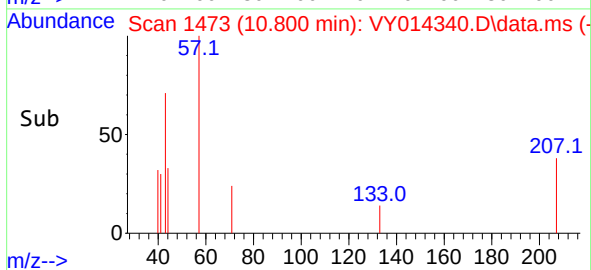
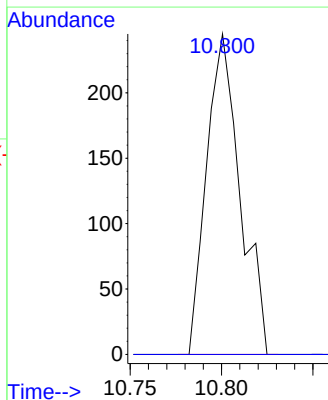
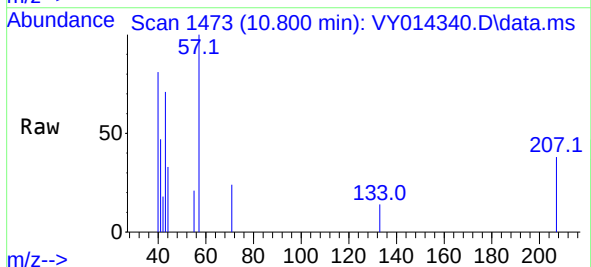




#62
4-Bromofluorobenzene
Concen: 40.141 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion:	95	Resp:	19542
Ion	Ratio	Lower	Upper
95	100		
174	91.8	0.0	178.2
176	86.8	0.0	173.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion:	117	Resp:	47516
Ion	Ratio	Lower	Upper
117	100		
82	51.9	43.4	65.0
119	33.2	26.3	39.5

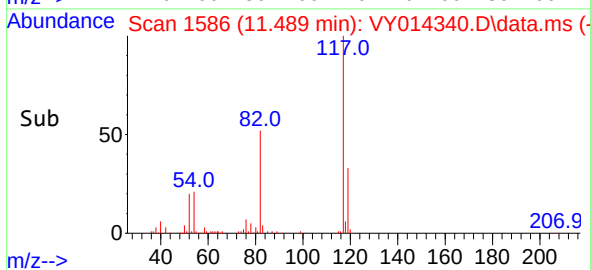



#67

Ethyl Benzene

Concen: 2.410 ug/l

RT: 11.599 min Scan# 1

Delta R.T. 0.006 min

Lab File: VY014340.D

Acq: 21 Jun 2023 16:55

Instrument :

MSVOA_Y

ClientSampleId :





WC-SCAN-01-G

Tgt Ion: 91 Resp: 4816

Ion Ratio Lower Upper

91 100

106 32.6 24.6 36.8

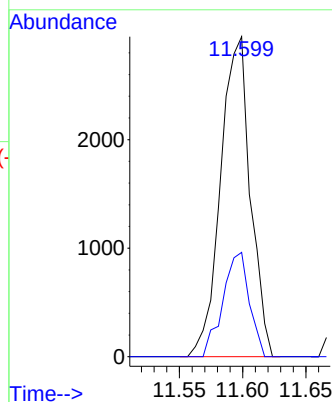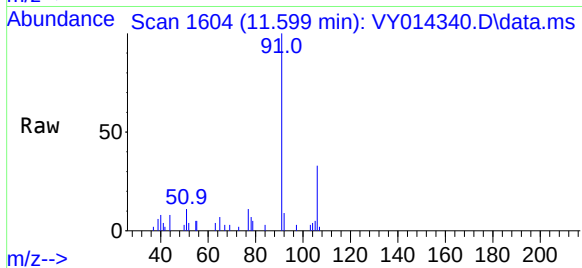

#68

m/p-Xylenes

Concen: 9.817 ug/l

RT: 11.697 min Scan# 1620

Delta R.T. -0.006 min

Lab File: VY014340.D




Acq: 21 Jun 2023 16:55


Tgt Ion:106 Resp: 7546

Ion Ratio Lower Upper

106 100

91 202.6 166.1 249.1


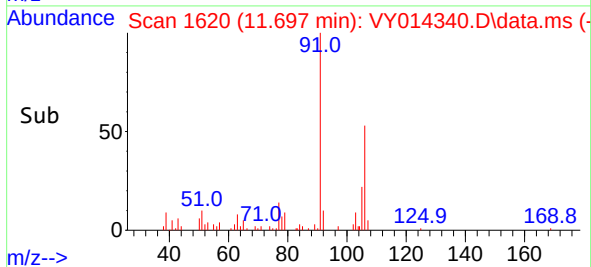

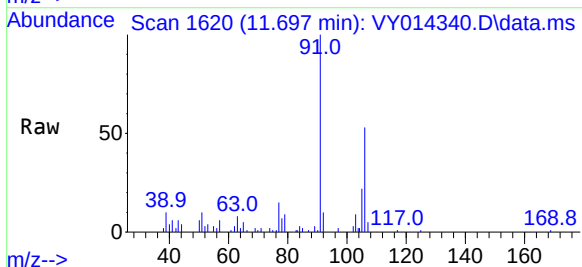




#69
o-Xylene
Concen: 6.239 ug/l
RT: 12.032 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion:106 Resp: 4534
Ion Ratio Lower Upper
106 100
91 207.4 108.1 324.3

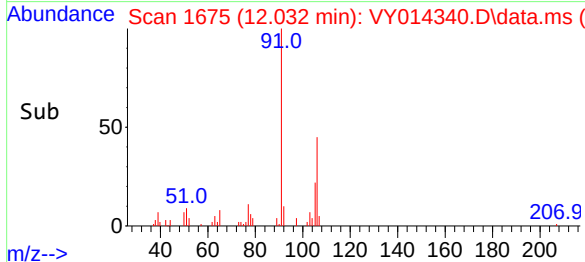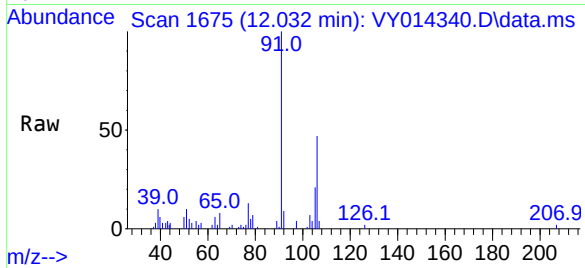

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion:152 Resp: 22312
Ion Ratio Lower Upper
152 100
115 59.9 28.8 86.5
150 160.0 0.0 348.8


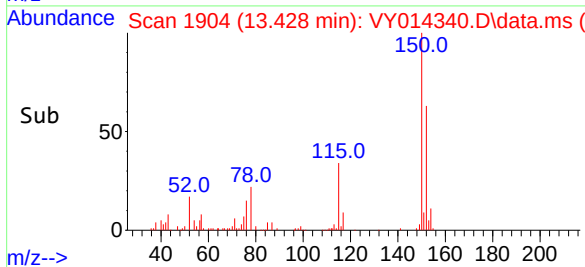

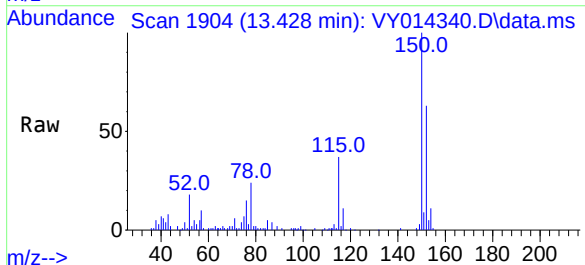




#73
Isopropylbenzene
Concen: 1.091 ug/l
RT: 12.331 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion:105 Resp: 1857
Ion Ratio Lower Upper
105 100
120 25.8 13.3 39.9

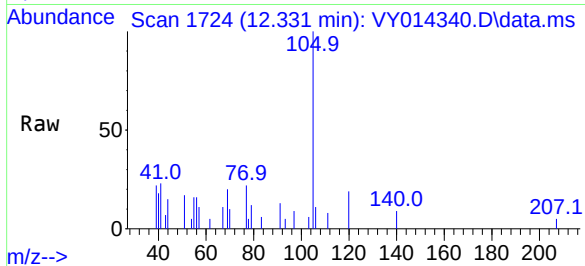

#74
N-ethyl acetate
Concen: 1.850 ug/l
RT: 12.130 min Scan# 1691
Delta R.T. -0.012 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 43 Resp: 998
Ion Ratio Lower Upper
43 100
70 28.7 29.7 44.5#
55 32.2 18.3 27.5#
61 0.0 17.5 26.3#


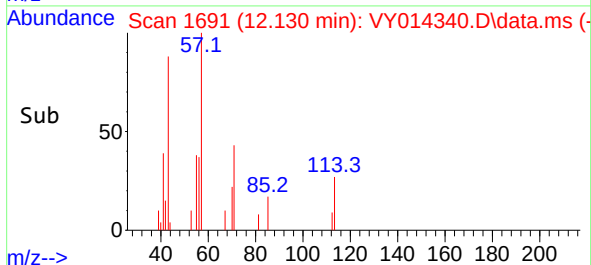
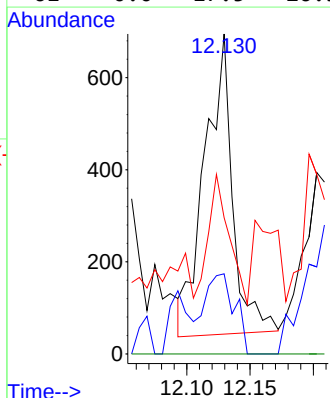
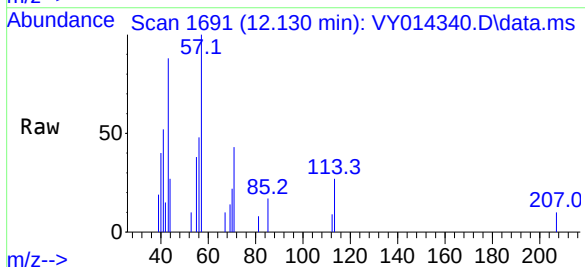




#76
1,2,3-Trichloropropane
Concen: 36.990 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 75 Resp: 10828
Ion Ratio Lower Upper
75 100
77 2.1 0.0 0.0#



#78
n-propylbenzene
Concen: 2.675 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 91 Resp: 5562
Ion Ratio Lower Upper
91 100
120 30.0 11.5 34.4









#79
2-Chlorotoluene
Concen: 2.007 ug/l
RT: 12.733 min Scan# 11
Delta R.T. -0.024 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 91 Resp: 2401
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.7#

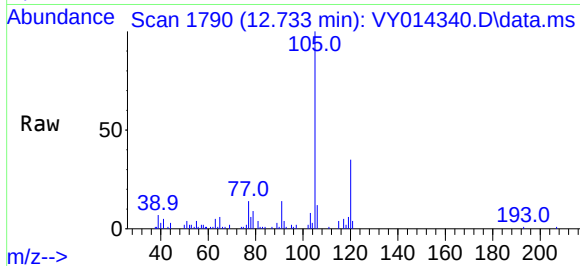

#80
1,3,5-Trimethylbenzene
Concen: 5.844 ug/l
RT: 12.812 min Scan# 1803
Delta R.T. 0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion: 105 Resp: 8517
Ion Ratio Lower Upper
105 100
120 51.9 23.9 71.7


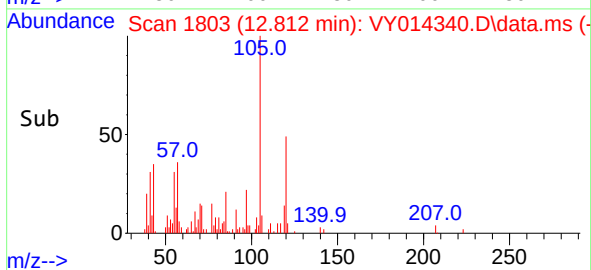

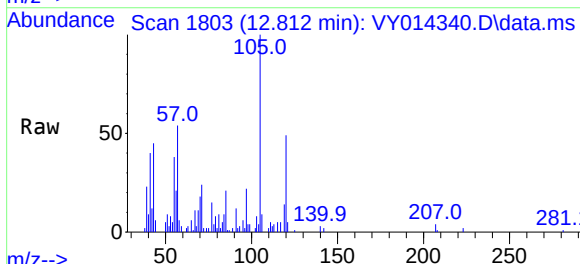




#81
trans-1,4-Dichloro-2-butene
Concen: 79.958 ug/l
RT: 12.483 min Scan# 11
Delta R.T. 0.104 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 75 Resp: 10828
Ion Ratio Lower Upper
75 100
53 0.5 77.8 116.8#
89 0.0 37.4 56.0#



#84
1,2,4-Trimethylbenzene
Concen: 20.290 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. 0.000 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55

Tgt Ion:105 Resp: 29272
Ion Ratio Lower Upper
105 100
120 46.2 22.2 66.6



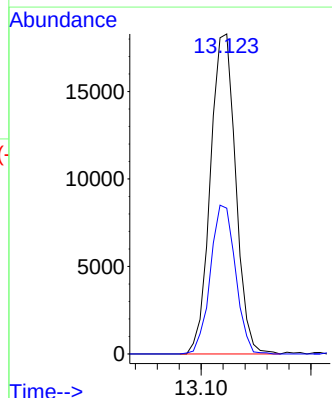





#85
 sec-Butylbenzene
 Concen: 1.572 ug/l
 RT: 13.251 min Scan# 1875
 Delta R.T. -0.006 min
 Lab File: VY014340.D
 Acq: 21 Jun 2023 16:55




Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-SCAN-01-G


Tgt Ion:105 Resp: 2830
 Ion Ratio Lower Upper
 105 100
 134 28.2 10.2 30.6

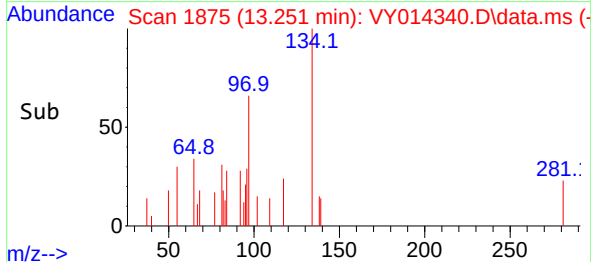

#86
 p-Isopropyltoluene
 Concen: 1.309 ug/l
 RT: 13.373 min Scan# 1895
 Delta R.T. 0.000 min
 Lab File: VY014340.D
 Acq: 21 Jun 2023 16:55

Tgt Ion:119 Resp: 2017
 Ion Ratio Lower Upper
 119 100
 134 27.5 13.3 39.8
 91 35.3 12.4 37.4

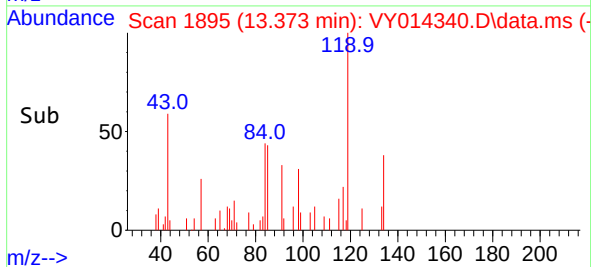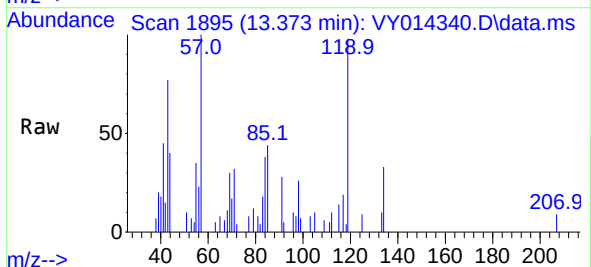



#89

n-Butylbenzene

Concen: 2.145 ug/l

RT: 13.696 min Scan# 1948

Delta R.T. 0.000 min

Lab File: VY014340.D

Acq: 21 Jun 2023 16:55

Instrument :

MSVOA_Y

ClientSampleId :

WC-SCAN-01-G





Tgt Ion: 91 Resp: 3066

Ion Ratio Lower Upper

91 100

92 62.2 25.4 76.0

134 0.0 12.6 37.6#

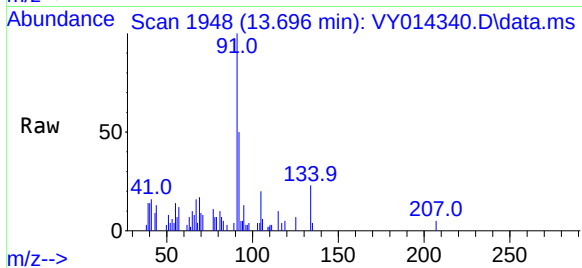

#90

Hexachloroethane

Concen: 5.722 ug/l

RT: 13.965 min Scan# 1992

Delta R.T. 0.001 min

Lab File: VY014340.D




Acq: 21 Jun 2023 16:55


Tgt Ion: 117 Resp: 1757

Ion Ratio Lower Upper

117 100

201 0.0 41.6 124.8#


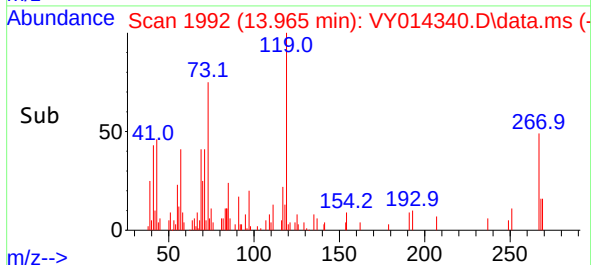
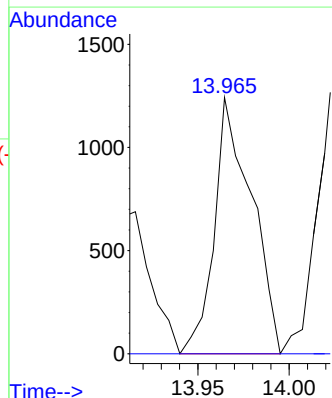
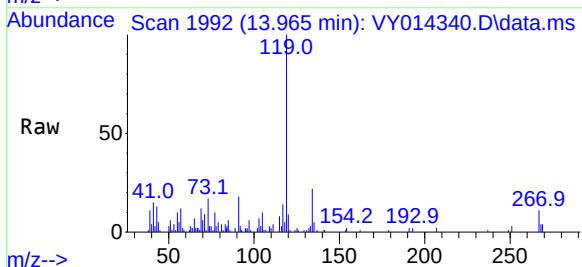




#92
1,2-Dibromo-3-Chloropropane
Concen: 1.671 ug/l
RT: 14.336 min Scan# 2053
Delta R.T. -0.019 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55




Instrument :
MSVOA_Y
ClientSampleId :
WC-SCAN-01-G


Tgt Ion: 75 Resp: 121
Ion Ratio Lower Upper
75 100
155 0.0 41.5 124.6#
157 0.0 51.8 155.5#

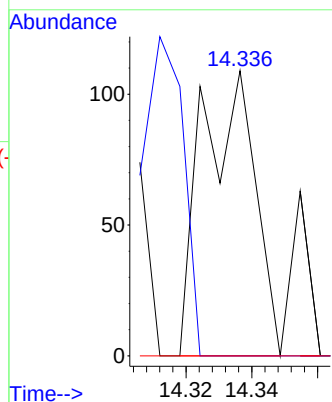

#95
Naphthalene
Concen: 6.729 ug/l
RT: 15.233 min Scan# 2200
Delta R.T. -0.006 min
Lab File: VY014340.D
Acq: 21 Jun 2023 16:55


Tgt Ion: 128 Resp: 6638
Ion Ratio Lower Upper
128 100
127 22.9 10.8 16.2#
129 10.5 8.6 13.0





#96
 1,2,3-Trichlorobenzene
 Concen: 1.350 ug/l
 RT: 15.446 min Scan# 21
 Delta R.T. 0.018 min
 Lab File: VY014340.D
 Acq: 21 Jun 2023 16:55

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-SCAN-01-G



Tgt Ion:180 Resp: 593
 Ion Ratio Lower Upper
 180 100
 182 72.8 47.3 141.8
 145 771.3 15.4 46.2#

