

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062123\
 Data File : VY014353.D
 Acq On : 21 Jun 2023 23:07
 Operator : KP/MD
 Sample : VY0621SBL02
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0621SBL02

Quant Time: Jun 22 02:00:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 09 18:07:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	189926	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	8.697	114	298104	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	281697	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	132251	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	126288	47.750	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	95.500%
35) Dibromofluoromethane	7.722	113	97037	45.900	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	91.800%
50) Toluene-d8	10.185	98	355197	44.941	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	89.880%
62) 4-Bromofluorobenzene	12.483	95	116260	41.409	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	82.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062123\
Data File : VY014353.D
Acq On : 21 Jun 2023 23:07
Operator : KP/MD
Sample : VY0621SBL02
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0621SBL02

Quant Time: Jun 22 02:00:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 09 18:07:13 2023
Response via : Initial Calibration




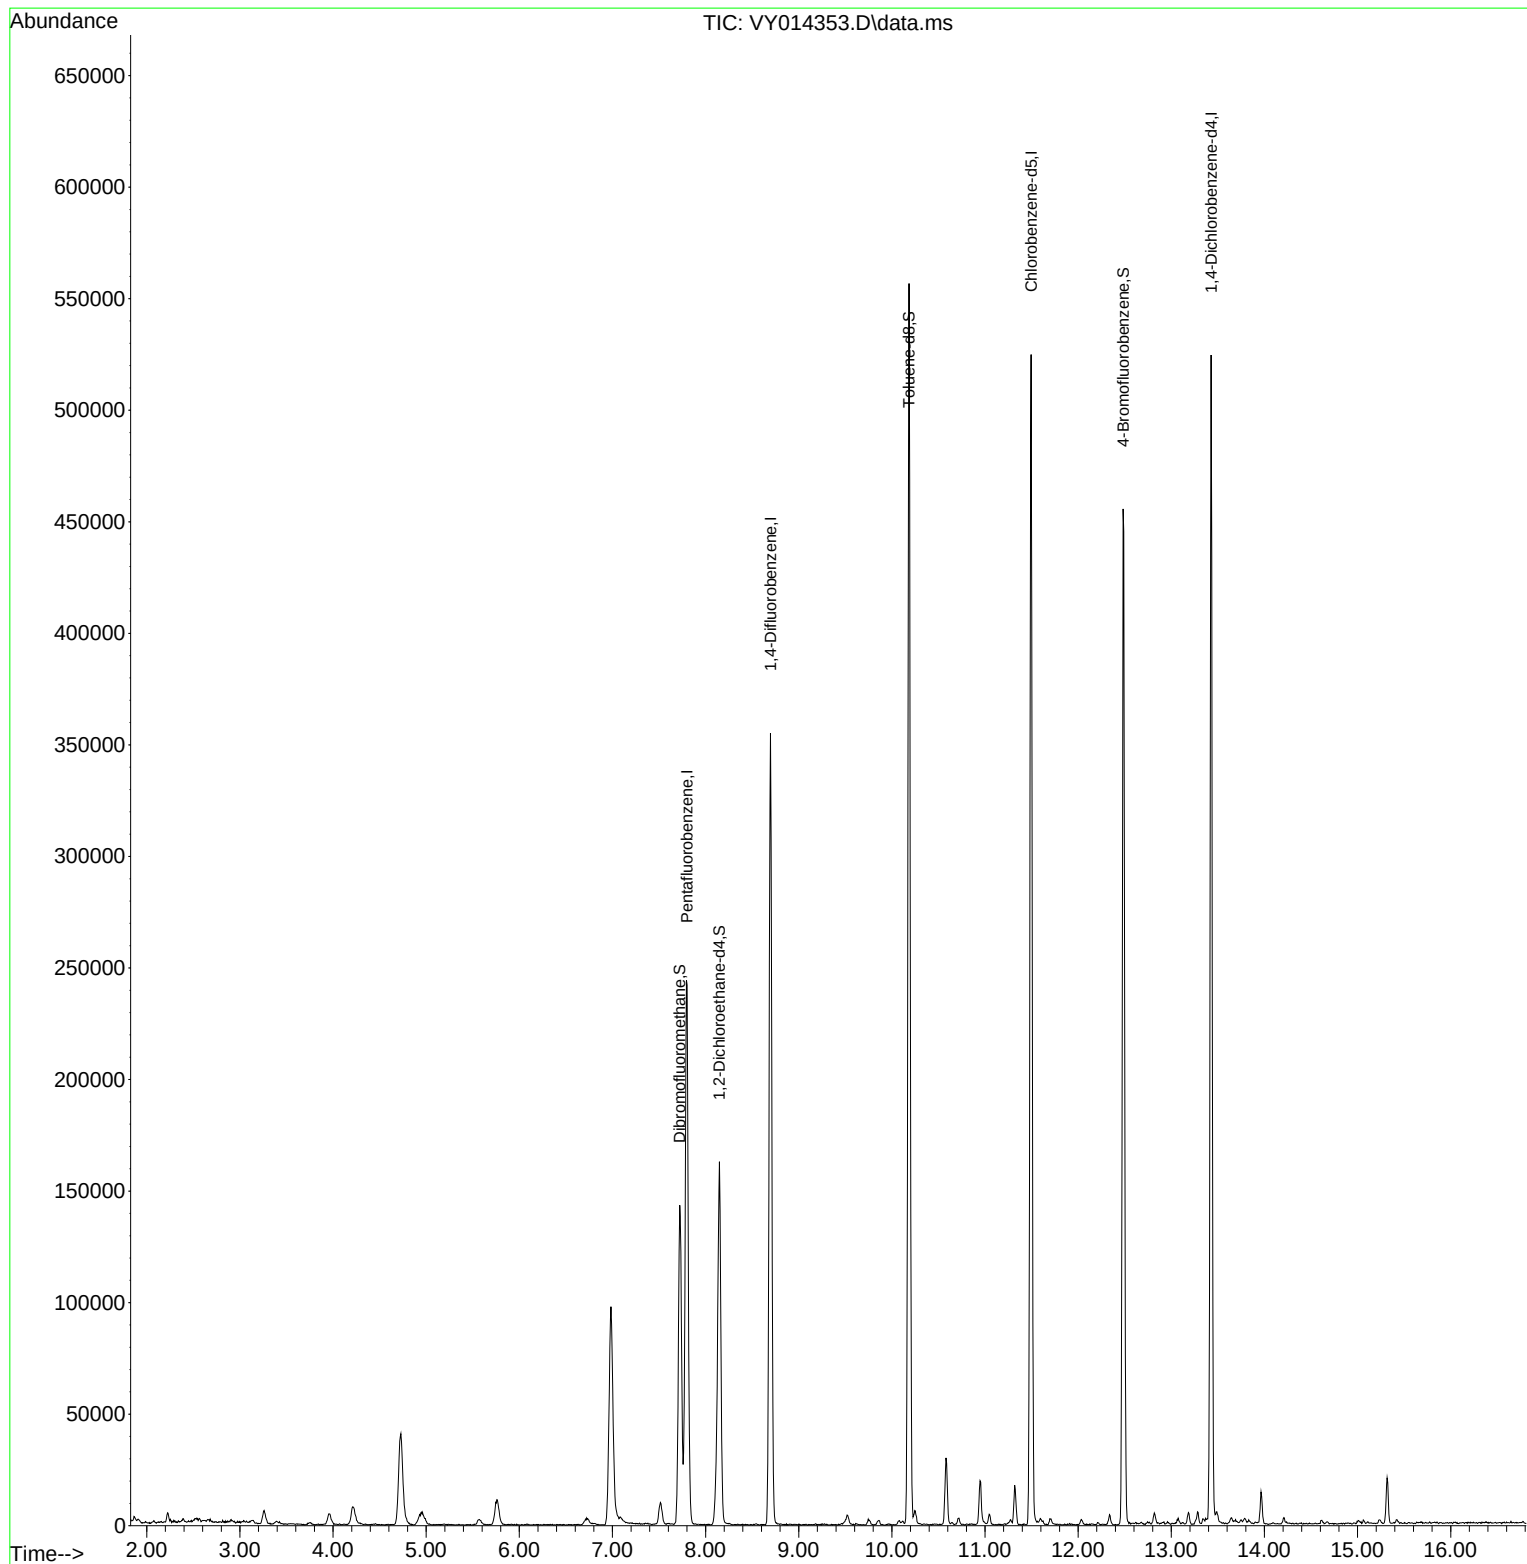


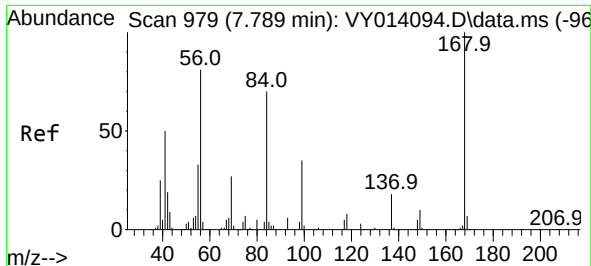

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY014353.D
Acq: 21 Jun 2023 23:07




Instrument :
MSVOA_Y
ClientSampleId :
VY0621SBL02


Tgt Ion:168 Resp: 189926
Ion Ratio Lower Upper
168 100
99 50.6 43.4 65.0

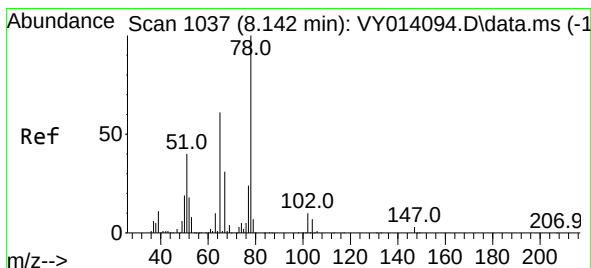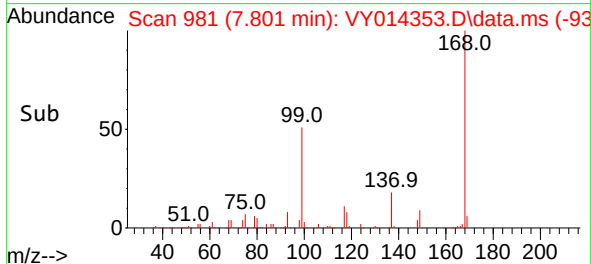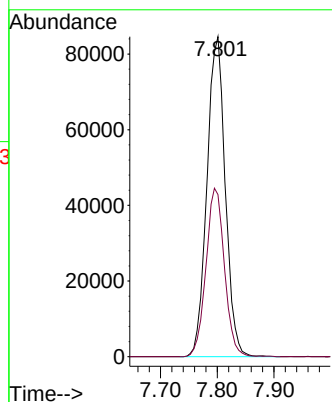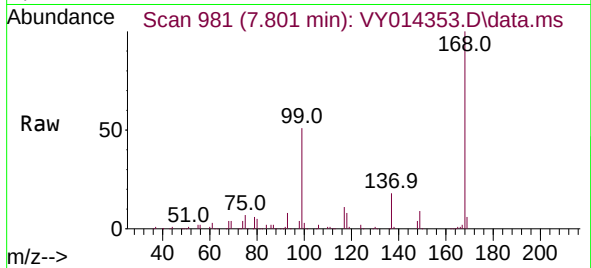

#33
1,2-Dichloroethane-d4
Concen: 47.750 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.007 min
Lab File: VY014353.D
Acq: 21 Jun 2023 23:07

Tgt Ion: 65 Resp: 126288
Ion Ratio Lower Upper
65 100
67 49.7 0.0 101.8

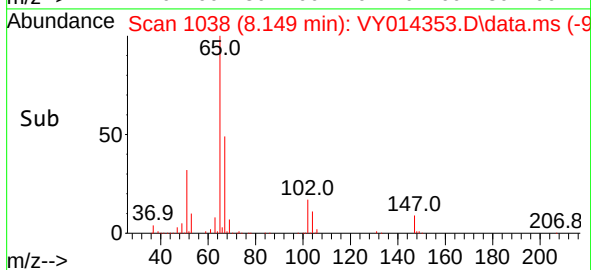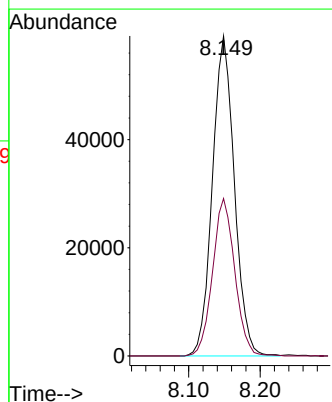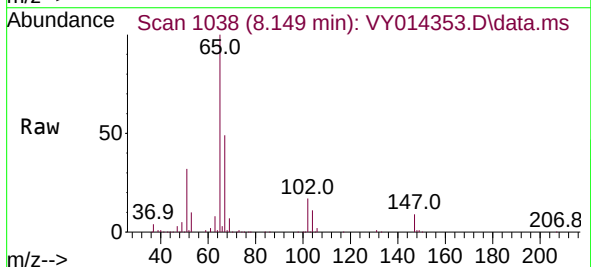

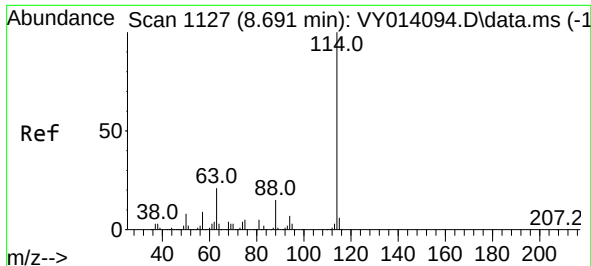

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY014353.D

Acq: 21 Jun 2023 23:07

Instrument :

MSVOA_Y

ClientSampleId :

VY0621SBL02





Tgt Ion:114 Resp: 298104

Ion Ratio Lower Upper

114 100

63 18.8 0.0 42.4

88 15.0 0.0 30.6

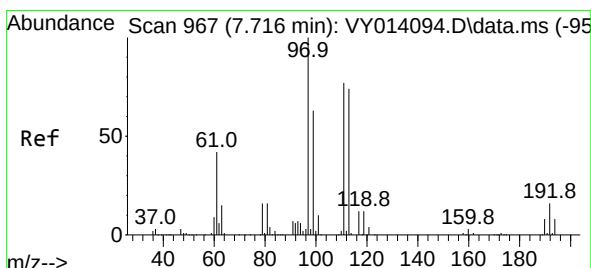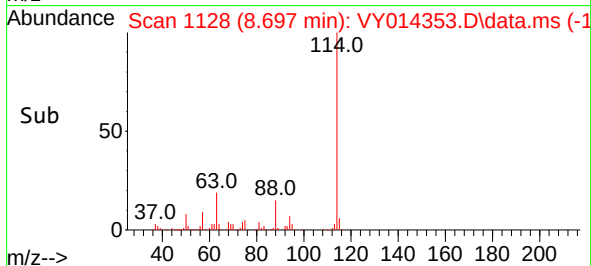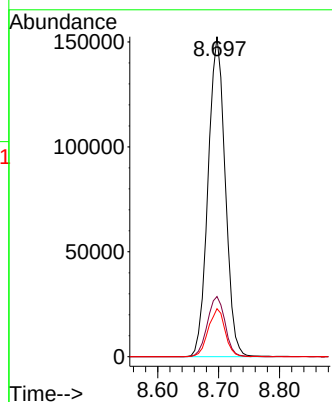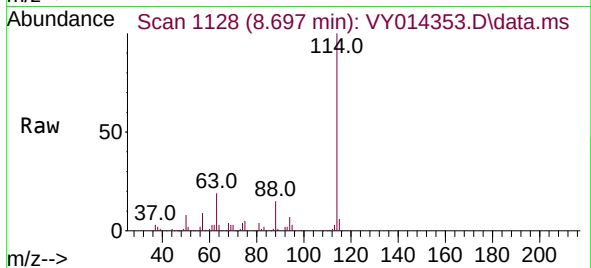

#35

Dibromofluoromethane

Concen: 45.900 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.006 min

Lab File: VY014353.D

Acq: 21 Jun 2023 23:07




Tgt Ion:113 Resp: 97037


Ion Ratio Lower Upper

113 100

111 103.8 81.3 121.9

192 22.4 16.9 25.3

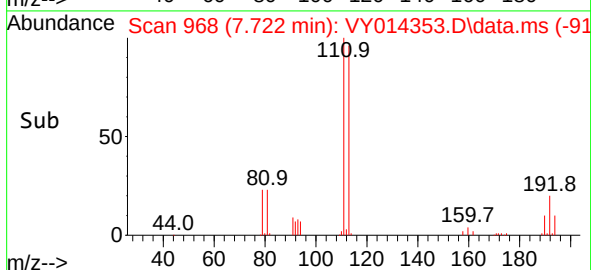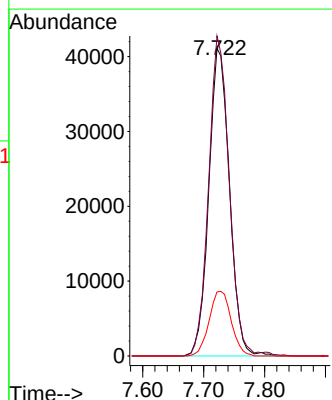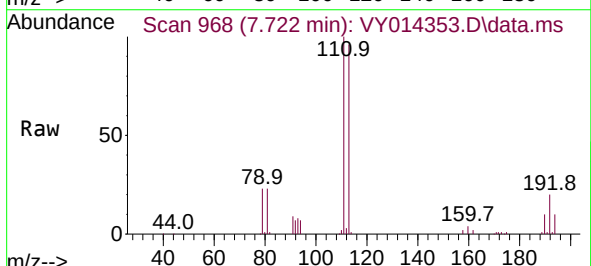

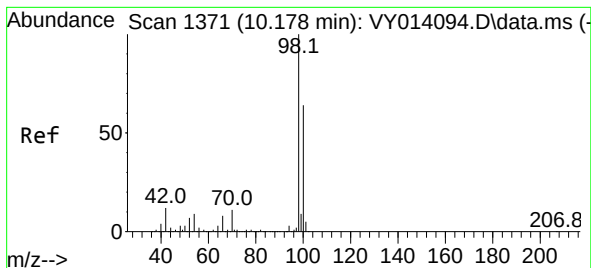

#50

Toluene-d8

Concen: 44.941 ug/l

RT: 10.185 min Scan# 1

Delta R.T. 0.007 min

Lab File: VY014353.D

Acq: 21 Jun 2023 23:07

Instrument :

MSVOA_Y

ClientSampleId :





VY0621SBL02

Tgt Ion: 98 Resp: 355197

Ion Ratio Lower Upper

98 100

100 63.5 50.1 75.1

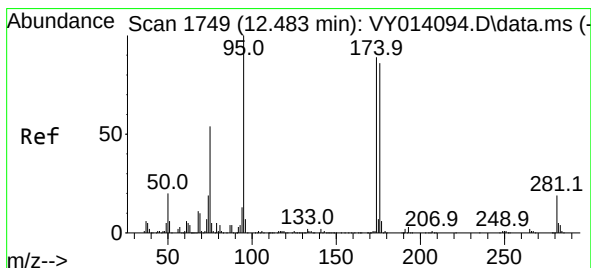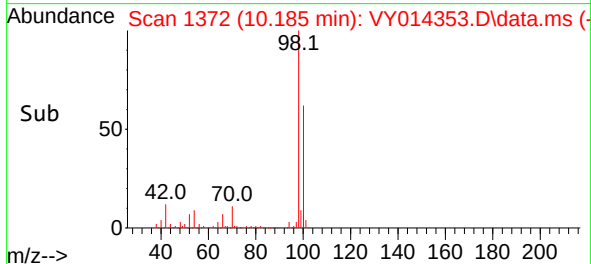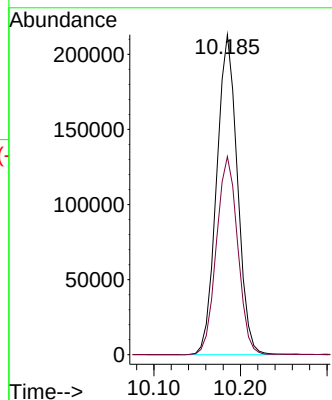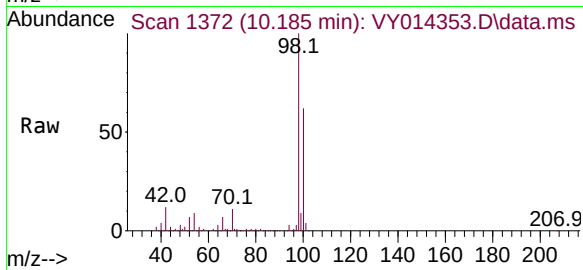

#62

4-Bromofluorobenzene

Concen: 41.409 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VY014353.D

Acq: 21 Jun 2023 23:07




Tgt Ion: 95 Resp: 116260


Ion Ratio Lower Upper

95 100

174 93.8 0.0 178.2

176 91.2 0.0 173.8

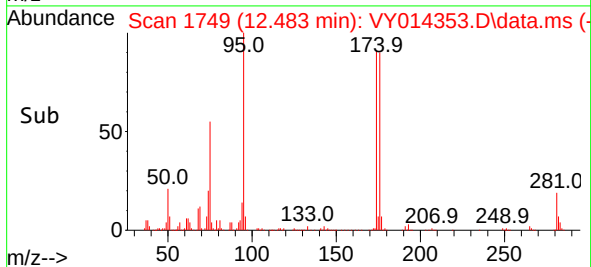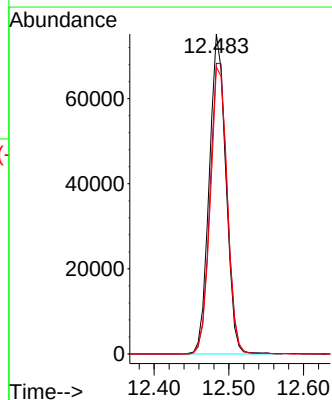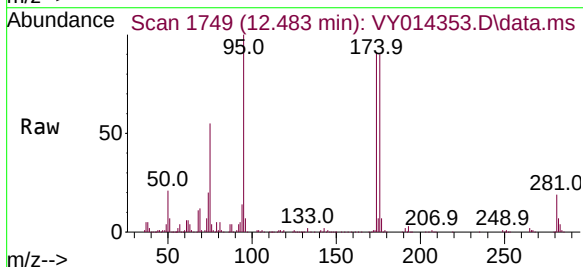

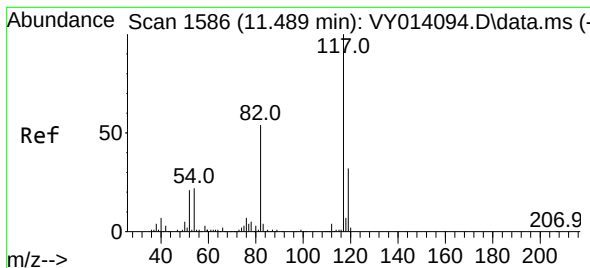

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.496 min Scan# 11

Delta R.T. 0.007 min

Lab File: VY014353.D

Acq: 21 Jun 2023 23:07

Instrument :

MSVOA_Y

ClientSampleId :

VY0621SBL02





Tgt Ion:117 Resp: 281697

Ion Ratio Lower Upper

117 100

82 53.7 43.4 65.0

119 31.6 26.3 39.5

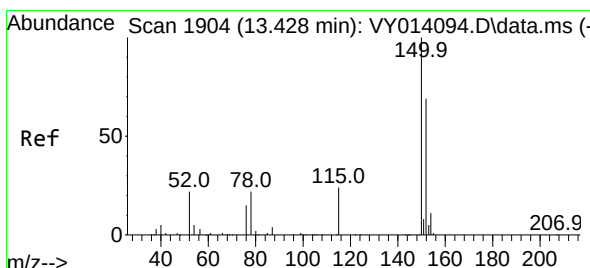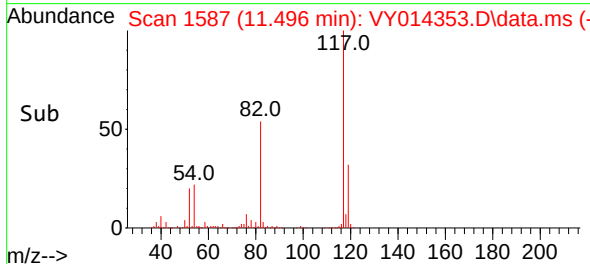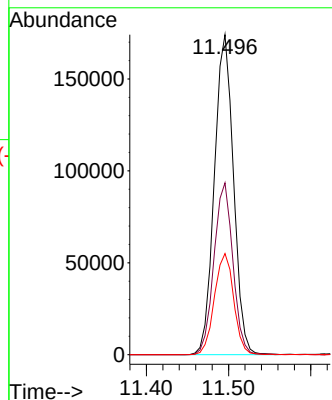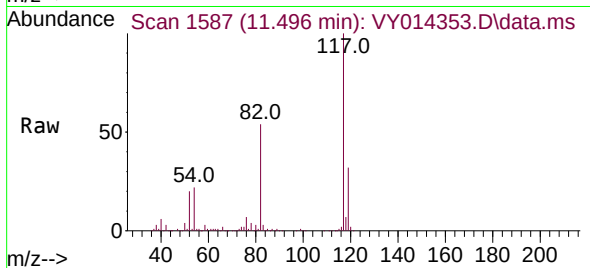

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY014353.D

Acq: 21 Jun 2023 23:07

Tgt Ion:152 Resp: 132251

Ion Ratio Lower Upper

152 100

115 57.4 28.8 86.5

150 157.1 0.0 348.8

