
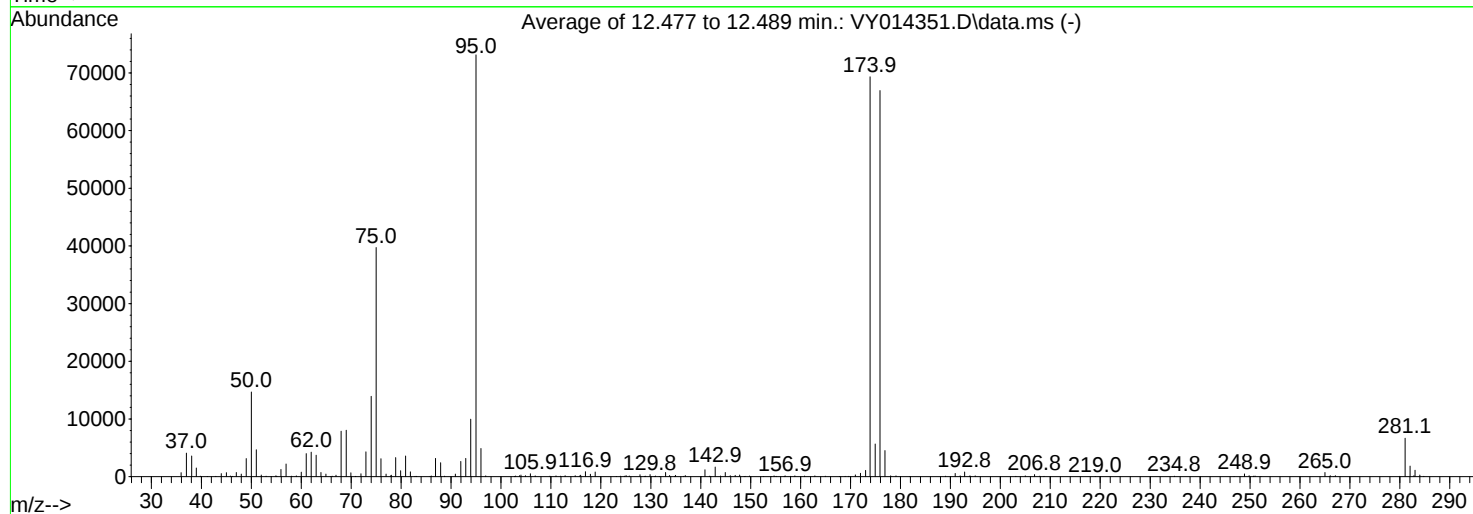


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062123\
Data File : VY014351.D
Acq On : 21 Jun 2023 21:33
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

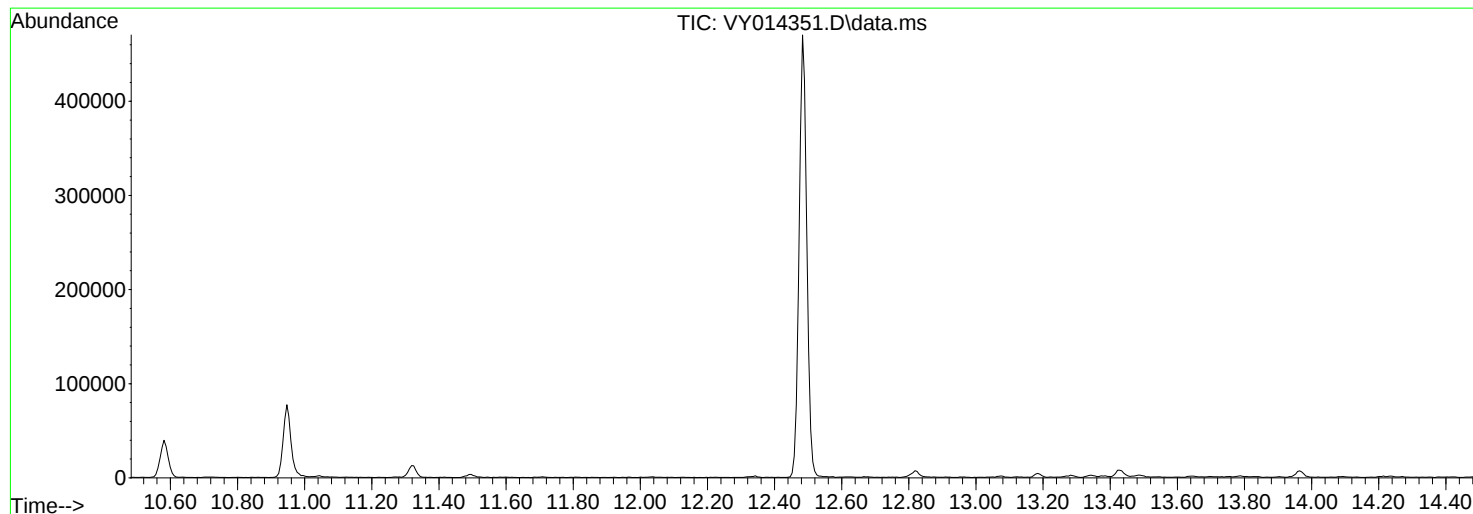

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	14687	PASS
75	95	30	60	54.3	39741	PASS
95	95	100	100	100.0	73136	PASS
96	95	5	9	6.7	4881	PASS
173	174	0.00	2	1.6	1086	PASS
174	95	50	100	94.8	69333	PASS
175	174	5	9	8.1	5650	PASS
176	174	95	101	96.5	66939	PASS
177	176	5	9	6.7	4514	PASS