
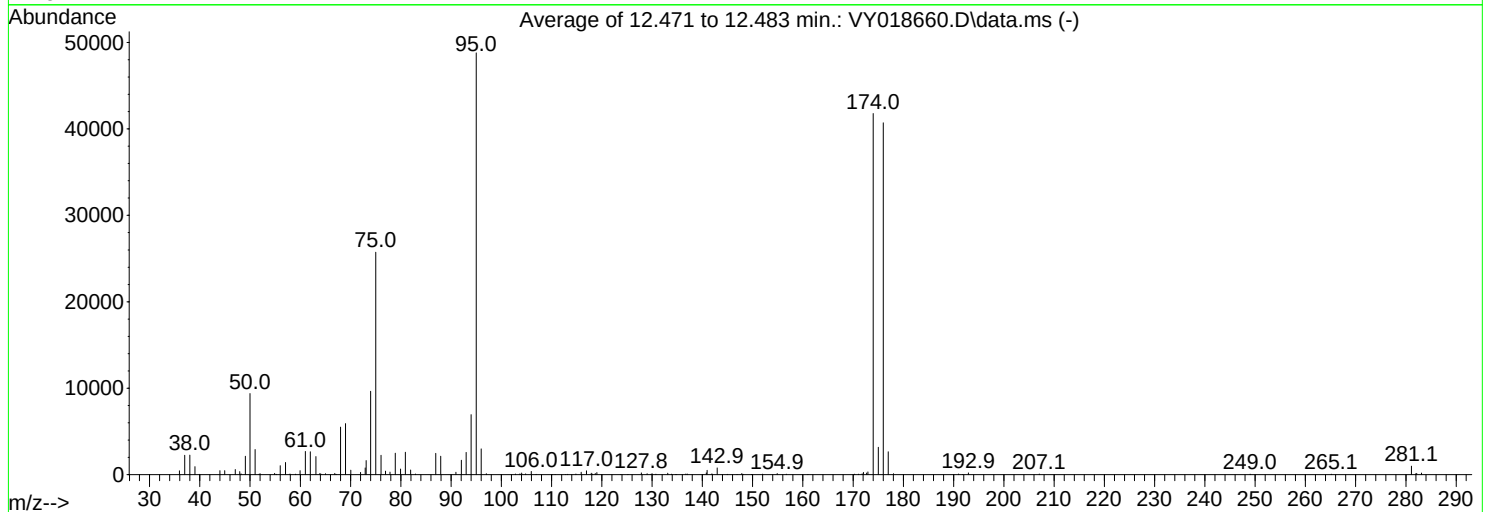


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY062124\  
Data File : VY018660.D  
Acq On : 21 Jun 2024 09:00  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y061324S.M  
Title : SW846 8260  
Last Update : Fri Jun 14 07:08:24 2024

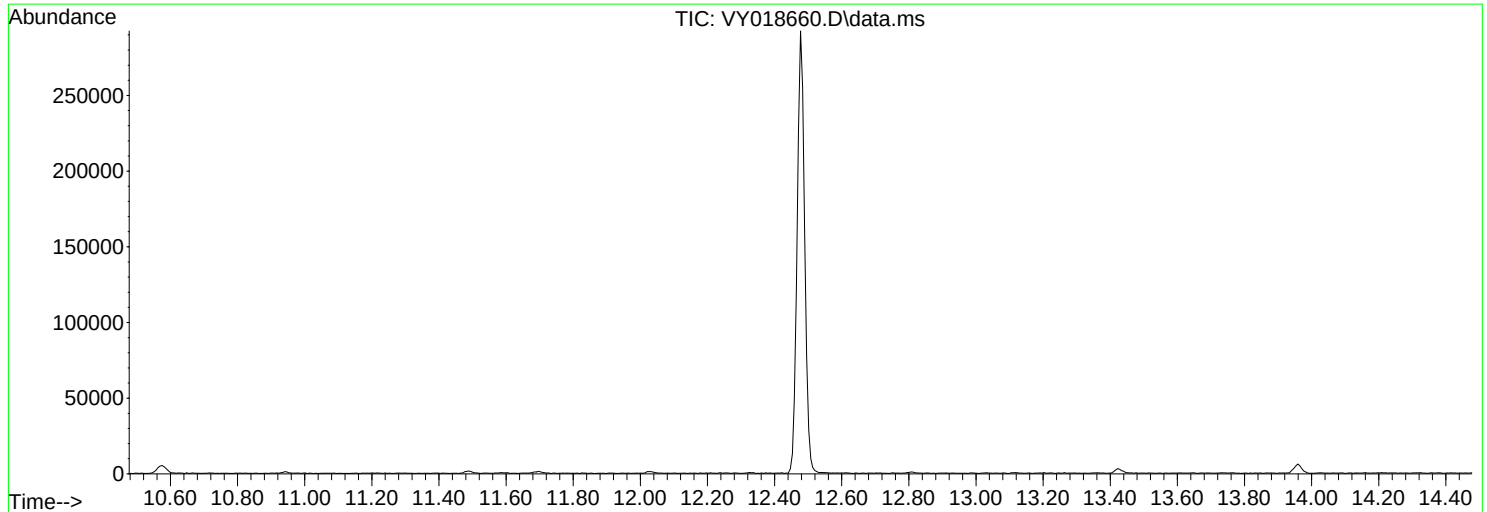

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.3         | 9395       | PASS                |
| 75             | 95              | 30              | 60              | 52.7         | 25739      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 48800      | PASS                |
| 96             | 95              | 5               | 9               | 6.1          | 2973       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.7          | 313        | PASS                |
| 174            | 95              | 50              | 100             | 85.6         | 41789      | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 3175       | PASS                |
| 176            | 174             | 95              | 101             | 97.4         | 40707      | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 2652       | PASS                |