

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062424\
 Data File : VY018672.D
 Acq On : 24 Jun 2024 10:18
 Operator : SY/MD
 Sample : VY0624SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0624SBL01

Quant Time: Jun 25 01:06:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061324S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 14 07:08:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.777	168	124394	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.679	114	226333	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	201561	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	74059	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	60716	48.480	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	96.960%
35) Dibromofluoromethane	7.704	113	69974	50.681	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.360%
50) Toluene-d8	10.173	98	258988	48.778	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.560%
62) 4-Bromofluorobenzene	12.477	95	74408	44.380	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	88.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062424\
Data File : VY018672.D
Acq On : 24 Jun 2024 10:18
Operator : SY/MD
Sample : VY0624SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0624SBL01


Quant Time: Jun 25 01:06:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061324S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 14 07:08:24 2024
Response via : Initial Calibration

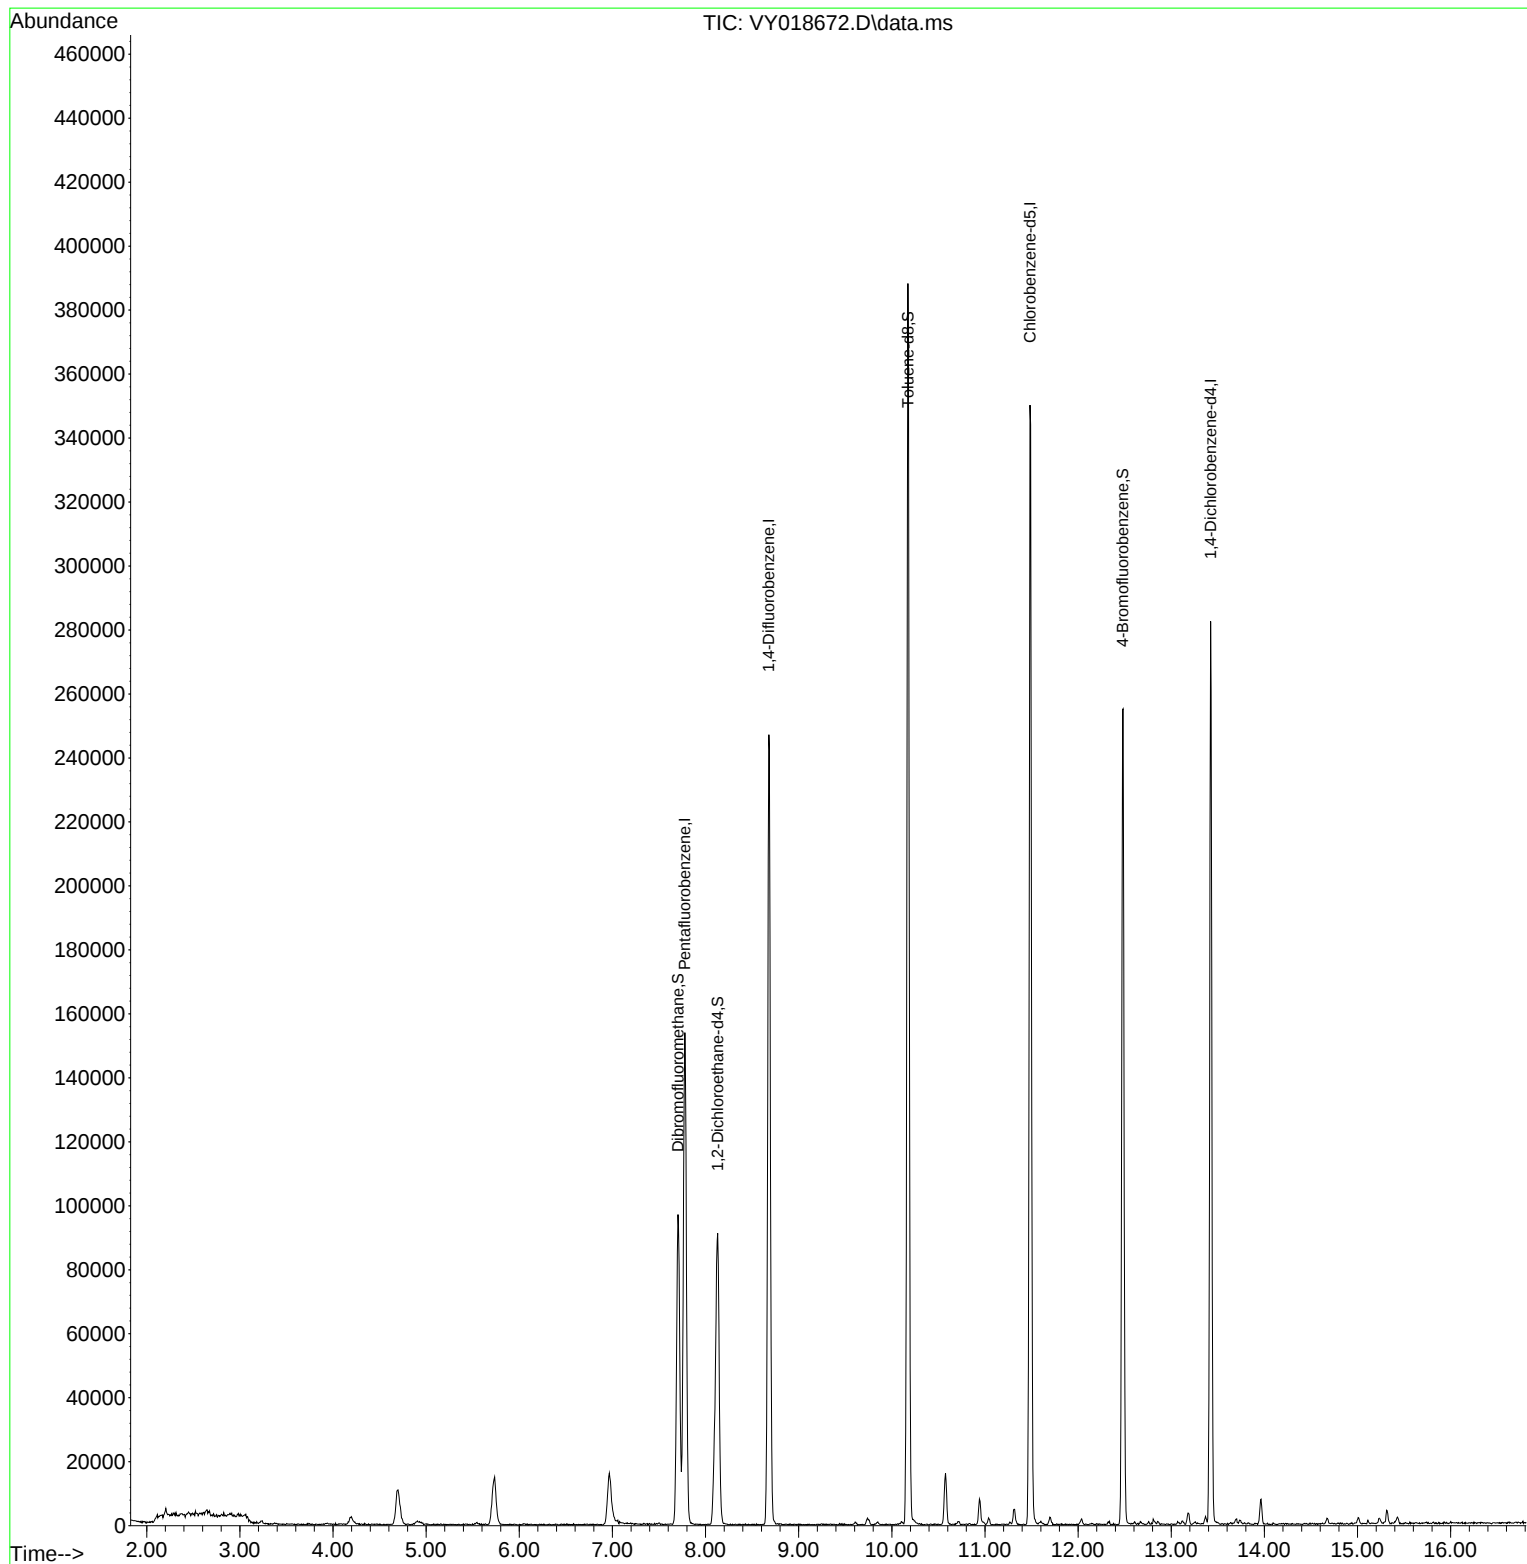



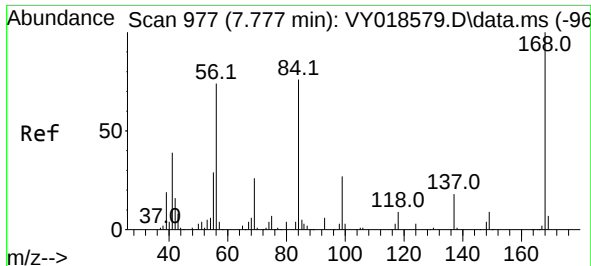


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18


Instrument :
MSVOA_Y
ClientSampleId :
VY0624SBL01

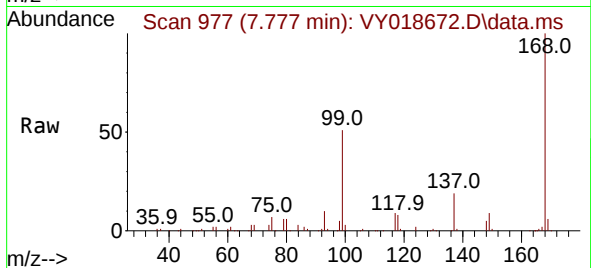



Tgt Ion:168 Resp: 124394
Ion Ratio Lower Upper
168 100
99 51.0 39.1 58.7

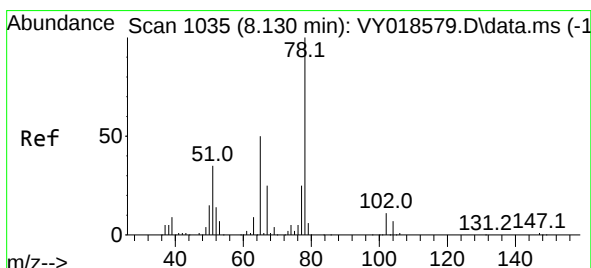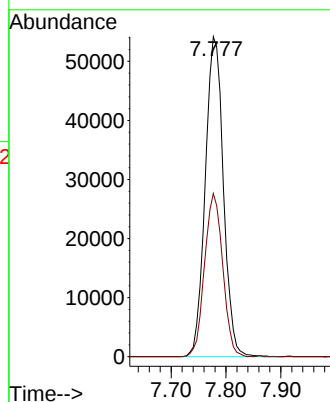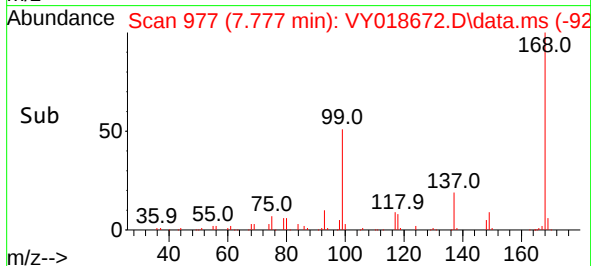


#33
1,2-Dichloroethane-d4
Concen: 48.480 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. 0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18

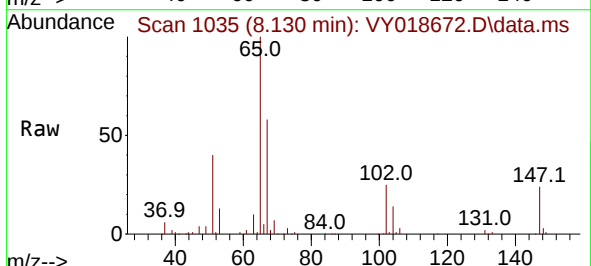

Tgt Ion: 65 Resp: 60716
Ion Ratio Lower Upper
65 100
67 55.6 0.0 109.6



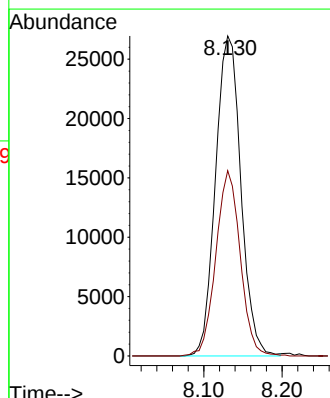
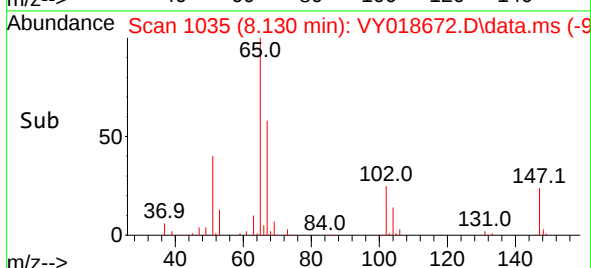


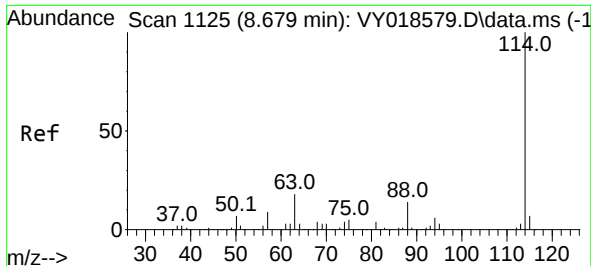

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.679 min Scan# 1125
Delta R.T. 0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18




Instrument :
MSVOA_Y
ClientSampleId :
VY0624SBL01


Tgt Ion:114 Resp: 226333
Ion Ratio Lower Upper
114 100
63 18.1 0.0 35.0
88 14.2 0.0 27.2

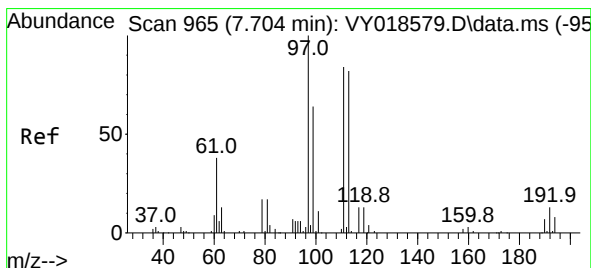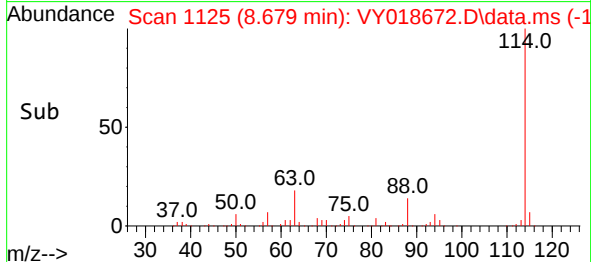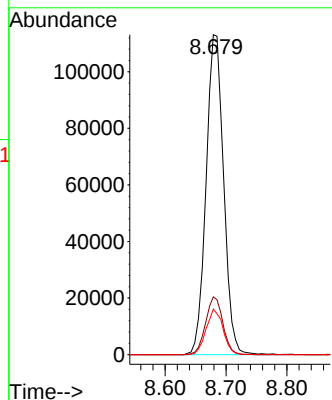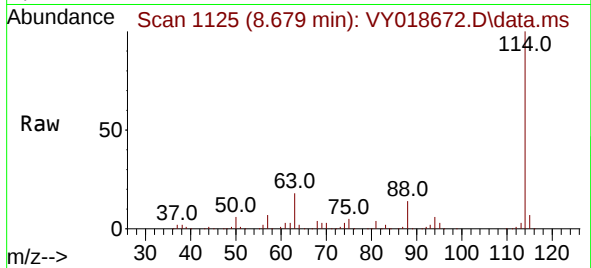

#35
Dibromofluoromethane
Concen: 50.681 ug/l
RT: 7.704 min Scan# 965
Delta R.T. 0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18

Tgt Ion:113 Resp: 69974
Ion Ratio Lower Upper
113 100
111 100.7 82.2 123.4
192 20.0 15.9 23.9


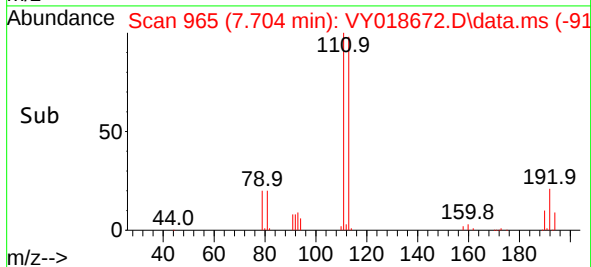
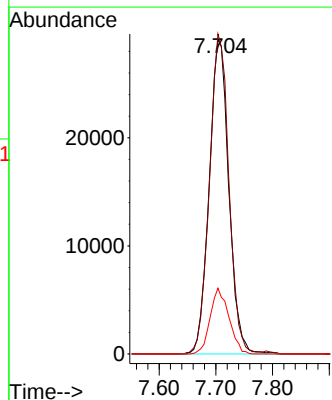
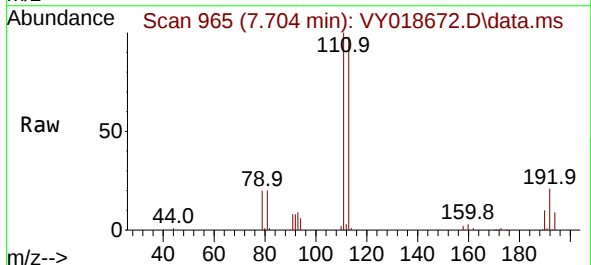


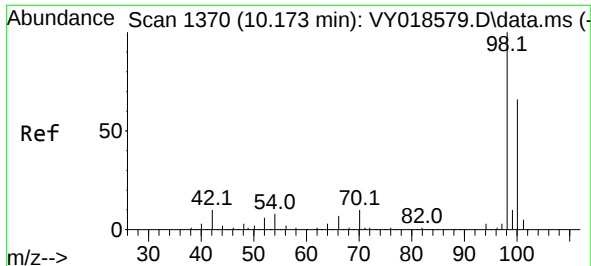

#50
Toluene-d8
Concen: 48.778 ug/l
RT: 10.173 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18




Instrument :
MSVOA_Y
ClientSampleId :
VY0624SBL01


Tgt Ion: 98 Resp: 258988
Ion Ratio Lower Upper
98 100
100 64.2 52.0 78.0

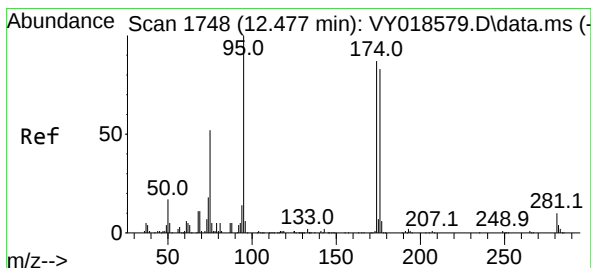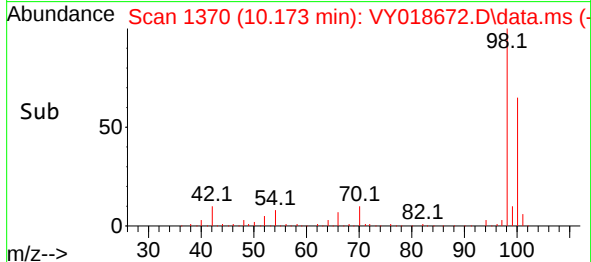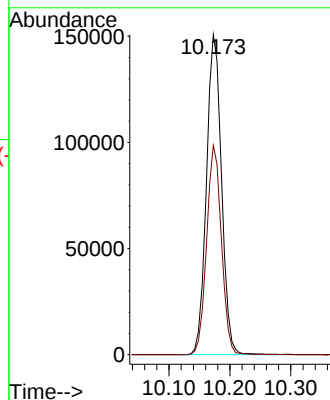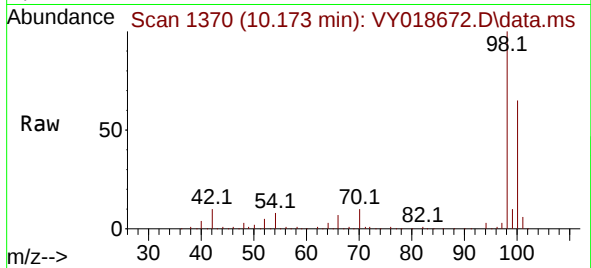

#62
4-Bromofluorobenzene
Concen: 44.380 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18

Tgt Ion: 95 Resp: 74408
Ion Ratio Lower Upper
95 100
174 90.0 0.0 175.6
176 86.9 0.0 171.4


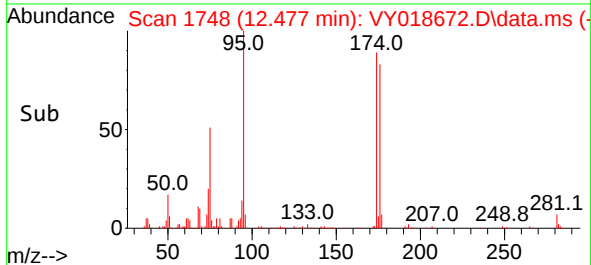
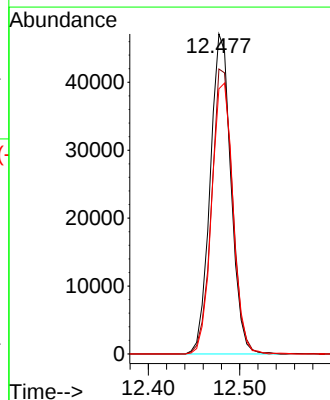
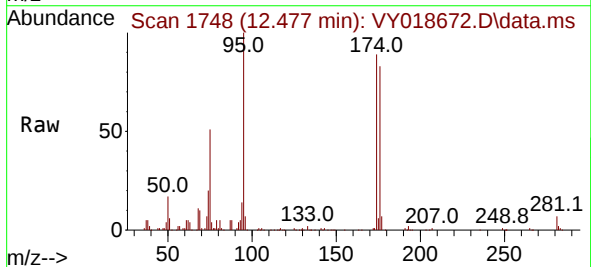


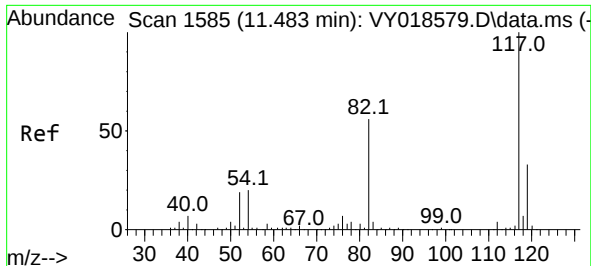

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.483 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18

Instrument :
MSVOA_Y
ClientSampleId :
VY0624SBL01

Tgt Ion:117 Resp: 201561
Ion Ratio Lower Upper
117 100
82 52.1 42.4 63.6
119 31.9 25.9 38.9

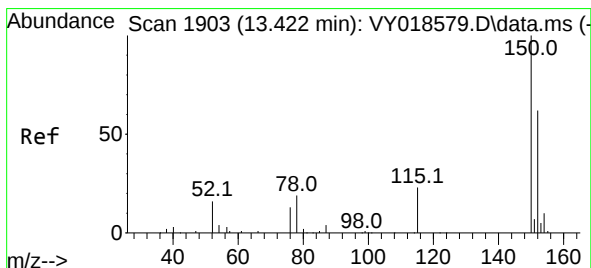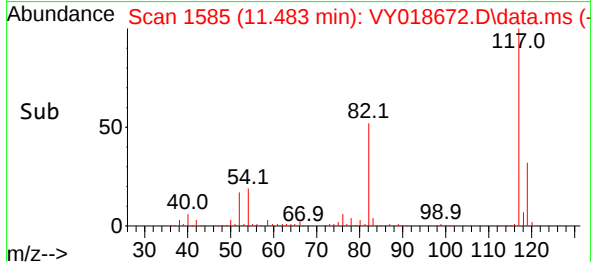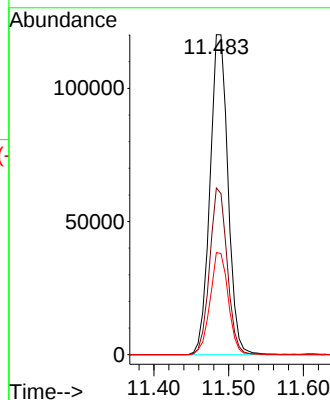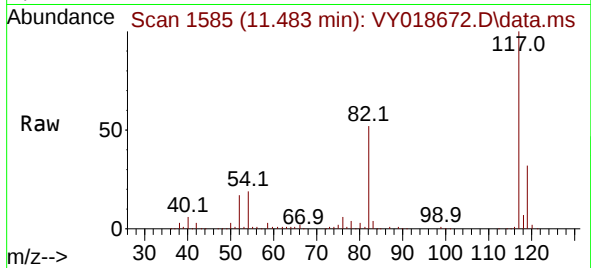

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY018672.D
Acq: 24 Jun 2024 10:18

Tgt Ion:152 Resp: 74059
Ion Ratio Lower Upper
152 100
115 55.4 28.2 84.7
150 158.6 0.0 345.6

