

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062425\
 Data File : VY022799.D
 Acq On : 24 Jun 2025 15:52
 Operator : SY/MD
 Sample : Q2393-10
 Misc : 4.54g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PARK AVE -5

Quant Time: Jun 25 01:27:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 24 08:29:52 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.707	168	316843	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.610	114	576057	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	531349	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	229194	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	165593	46.827	ug/l	-0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	93.660%
35) Dibromofluoromethane	7.634	113	171894	49.066	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.140%
50) Toluene-d8	10.103	98	673865	48.474	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.940%
62) 4-Bromofluorobenzene	12.402	95	230553	51.590	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	103.180%
Target Compounds						
					Qvalue	
7) Trichlorofluoromethane	3.043	101	16206	2.264	ug/l	92
16) Acetone	3.860	43	6248	9.348	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062425\
Data File : VY022799.D
Acq On : 24 Jun 2025 15:52
Operator : SY/MD
Sample : Q2393-10
Misc : 4.54g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PARK AVE -5

Quant Time: Jun 25 01:27:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 24 08:29:52 2025
Response via : Initial Calibration




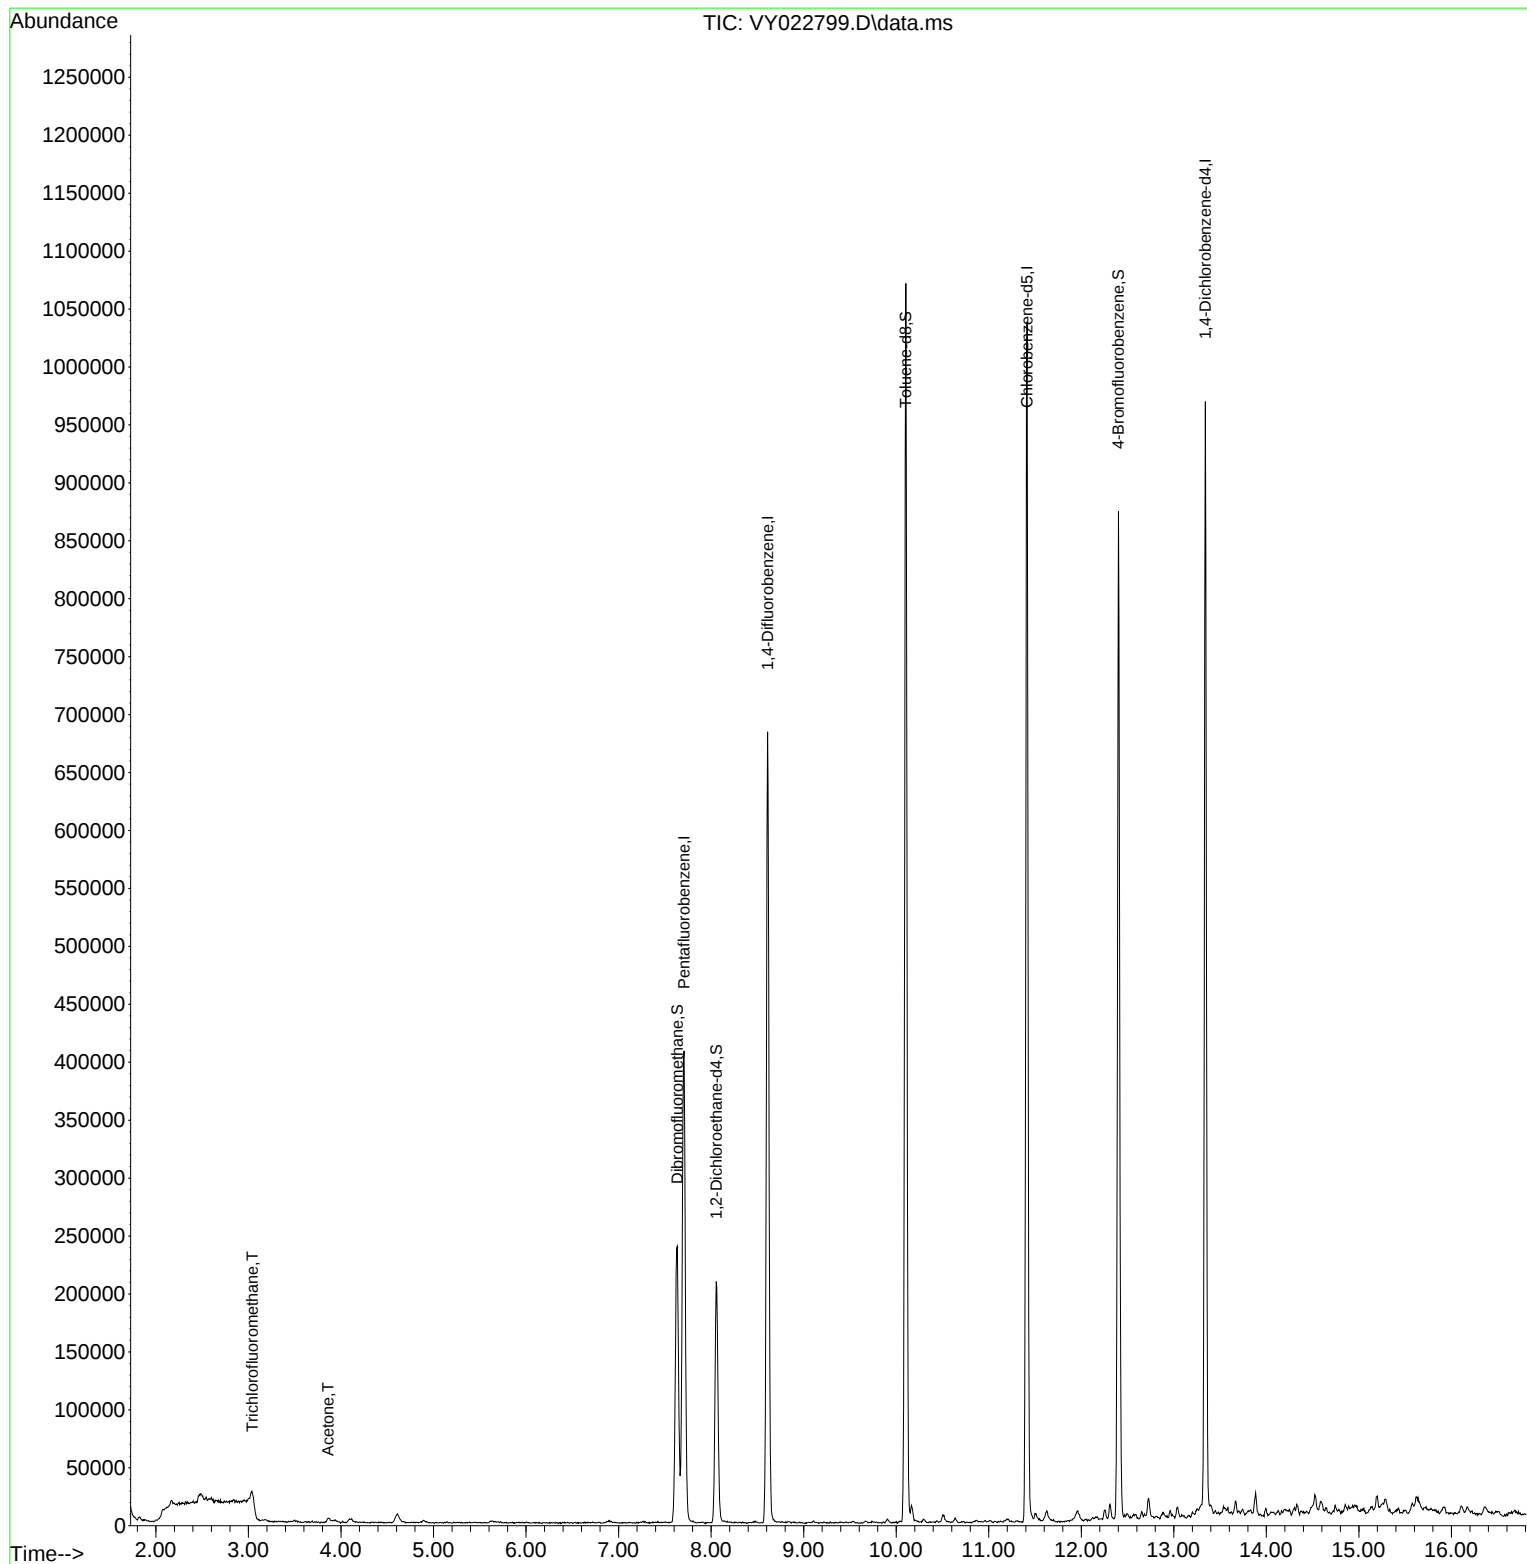




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. -0.006 min
Lab File: VY022799.D
Acq: 24 Jun 2025 15:52




Instrument :
MSVOA_Y
ClientSampleId :
PARK AVE -5


Tgt Ion:168 Resp: 316843
Ion Ratio Lower Upper
168 100
99 55.1 44.3 66.5

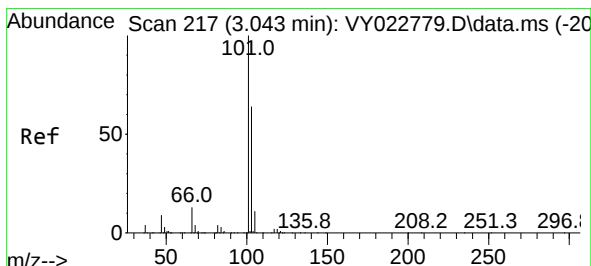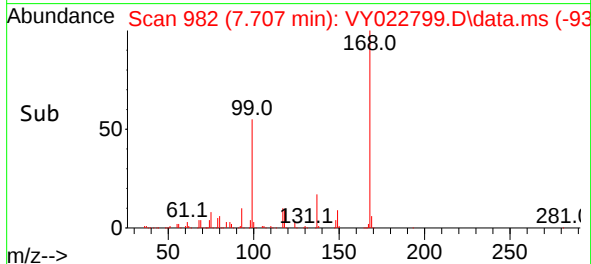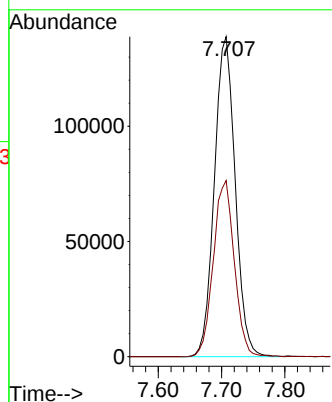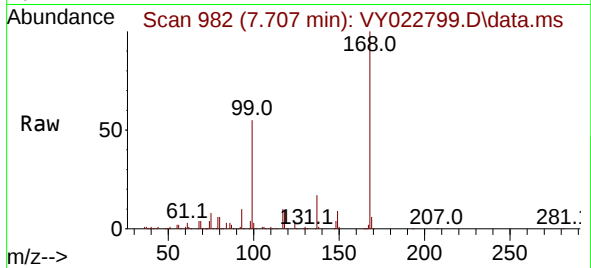

#7
Trichlorofluoromethane
Concen: 2.264 ug/l
RT: 3.043 min Scan# 217
Delta R.T. -0.012 min
Lab File: VY022799.D
Acq: 24 Jun 2025 15:52

Tgt Ion:101 Resp: 16206
Ion Ratio Lower Upper
101 100
103 59.2 52.2 78.2


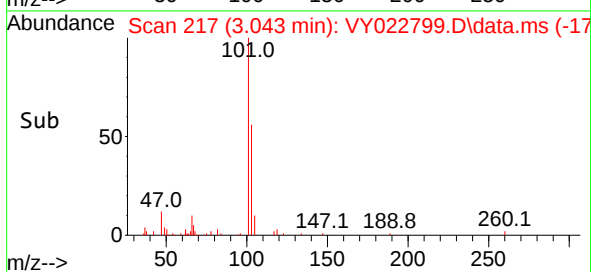
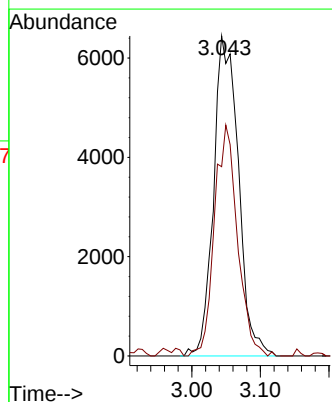
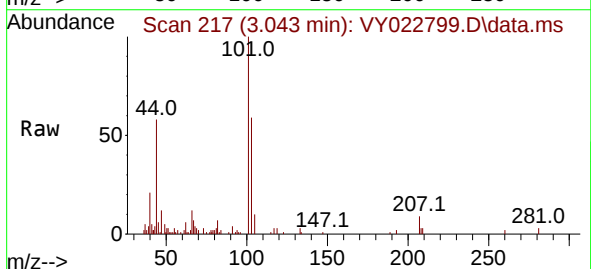


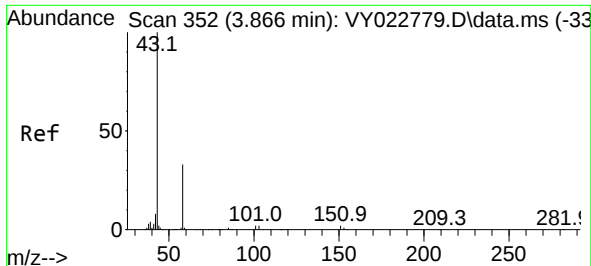

#16
Acetone
Concen: 9.348 ug/l
RT: 3.860 min Scan# 31
Delta R.T. -0.018 min
Lab File: VY022799.D
Acq: 24 Jun 2025 15:52




Instrument :
MSVOA_Y
ClientSampleId :
PARK AVE -5


Tgt Ion: 43 Resp: 6248
Ion Ratio Lower Upper
43 100
58 31.9 24.0 36.0

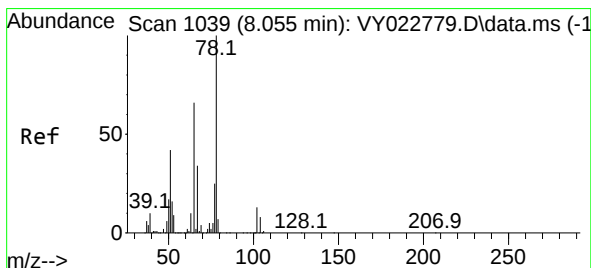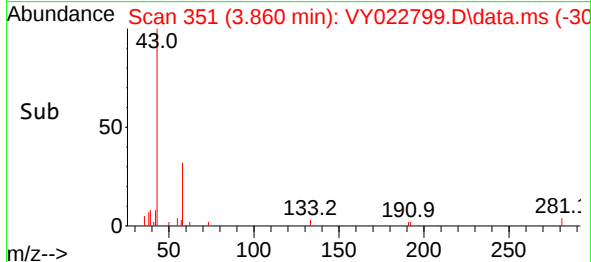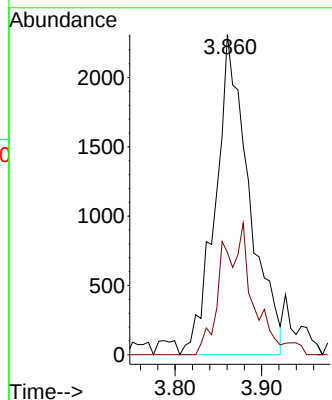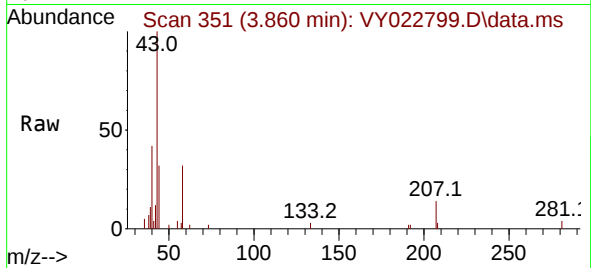

#33
1,2-Dichloroethane-d4
Concen: 46.827 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. -0.012 min
Lab File: VY022799.D
Acq: 24 Jun 2025 15:52

Tgt Ion: 65 Resp: 165593
Ion Ratio Lower Upper
65 100
67 51.2 0.0 103.4

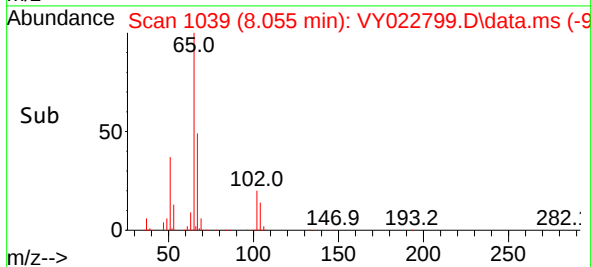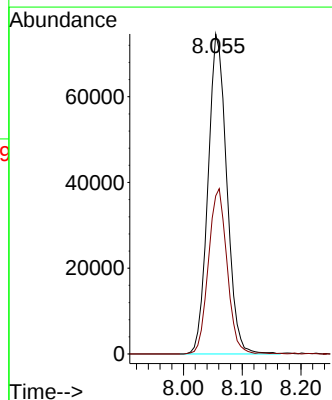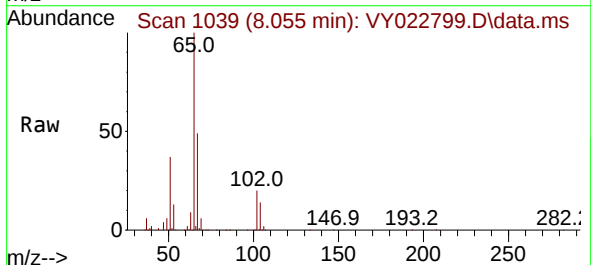

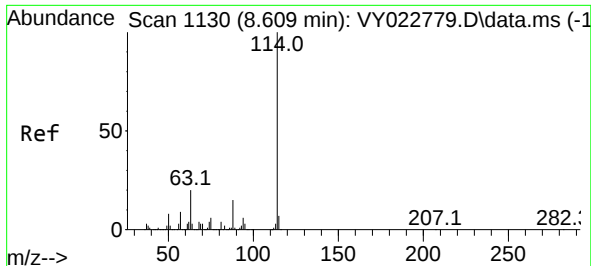

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.610 min Scan# 1130

Delta R.T. -0.006 min

Lab File: VY022799.D

Acq: 24 Jun 2025 15:52

Instrument :

MSVOA_Y

ClientSampleId :

PARK AVE -5





Tgt Ion:114 Resp: 576057

Ion Ratio Lower Upper

114 100

63 19.9 0.0 40.8

88 15.0 0.0 27.8

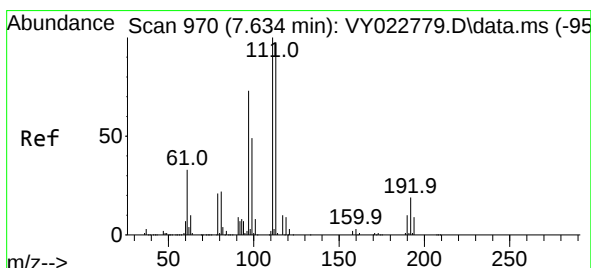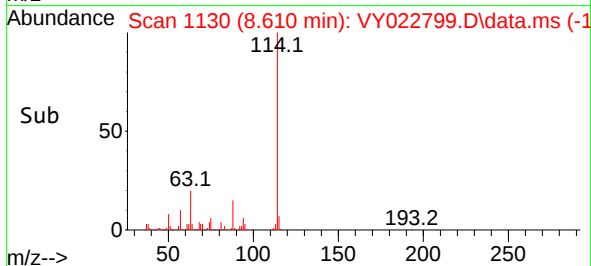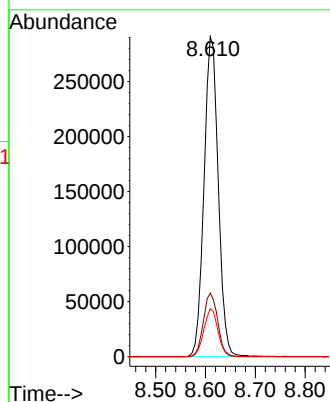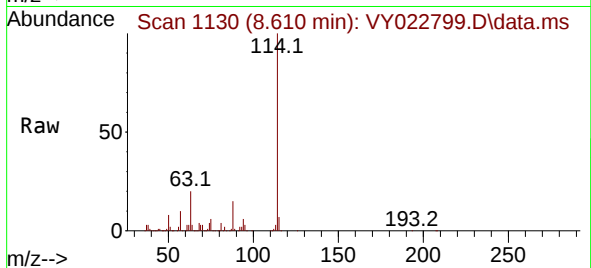

#35

Dibromofluoromethane

Concen: 49.066 ug/l

RT: 7.634 min Scan# 970

Delta R.T. -0.006 min

Lab File: VY022799.D

Acq: 24 Jun 2025 15:52




Tgt Ion:113 Resp: 171894


Ion Ratio Lower Upper

113 100

111 102.7 81.1 121.7

192 18.6 14.2 21.2

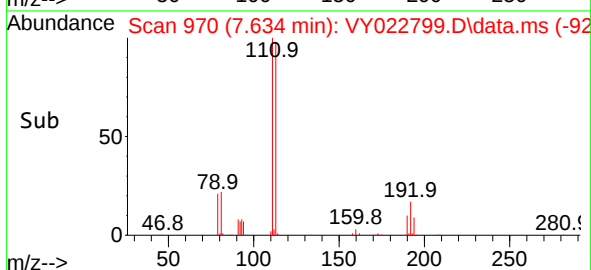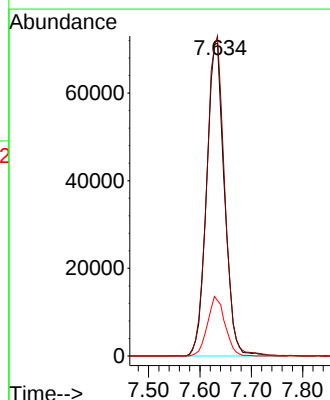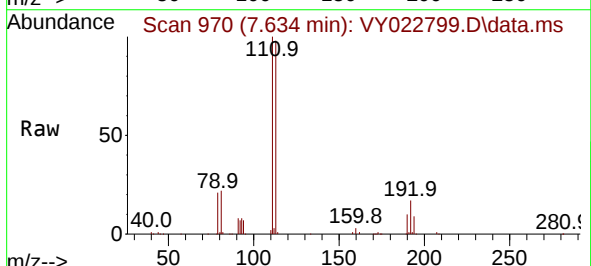

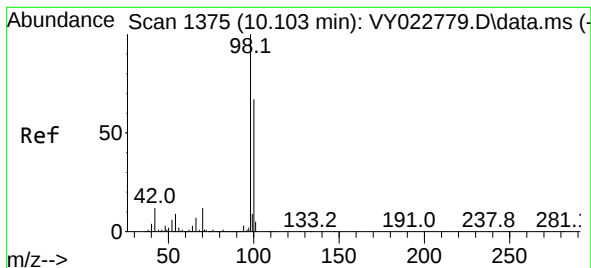

#50

Toluene-d8

Concen: 48.474 ug/l

RT: 10.103 min Scan# 1375

Delta R.T. -0.006 min

Lab File: VY022799.D

Acq: 24 Jun 2025 15:52

Instrument :

MSVOA_Y

ClientSampleId :





PARK AVE -5

Tgt Ion: 98 Resp: 673865

Ion Ratio Lower Upper

98 100

100 65.1 51.4 77.0

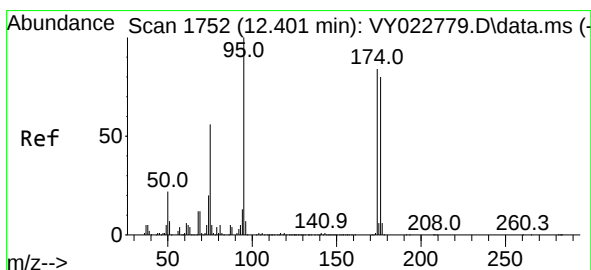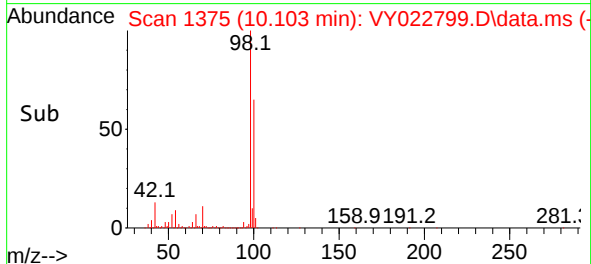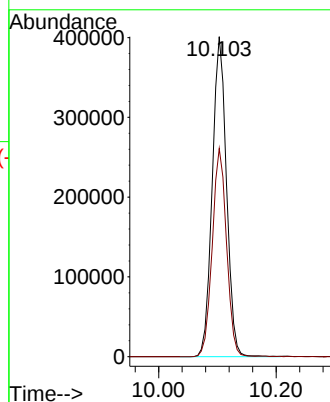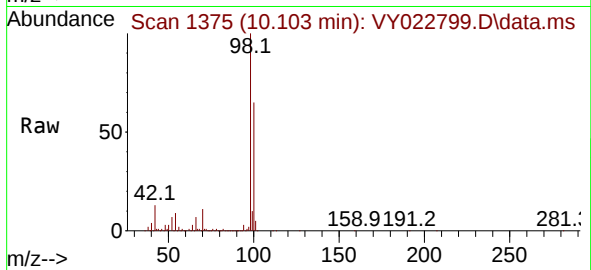

#62

4-Bromofluorobenzene

Concen: 51.590 ug/l

RT: 12.402 min Scan# 1752

Delta R.T. -0.006 min

Lab File: VY022799.D

Acq: 24 Jun 2025 15:52




Tgt Ion: 95 Resp: 230553


Ion Ratio Lower Upper

95 100

174 84.7 0.0 170.0

176 81.8 0.0 166.2

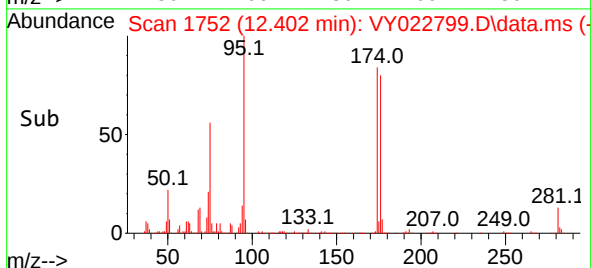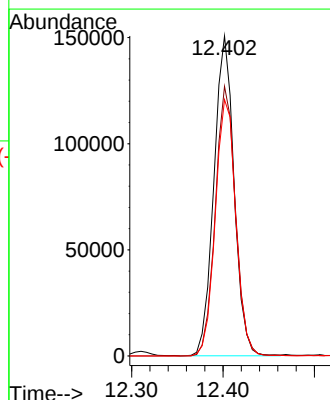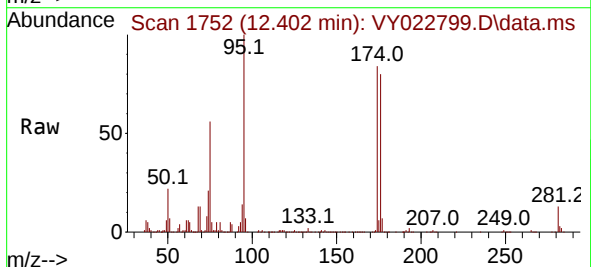

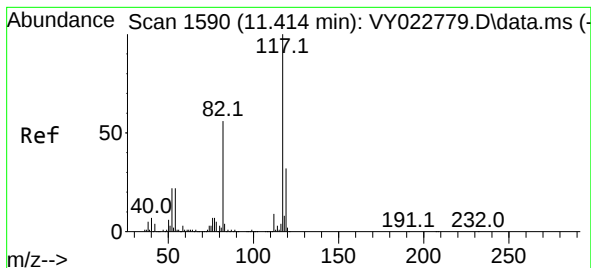

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY022799.D

Acq: 24 Jun 2025 15:52

Instrument :

MSVOA_Y

ClientSampleId :

PARK AVE -5





Tgt Ion:117 Resp: 531349

Ion Ratio Lower Upper

117 100

82 56.4 44.6 66.8

119 31.9 25.4 38.0

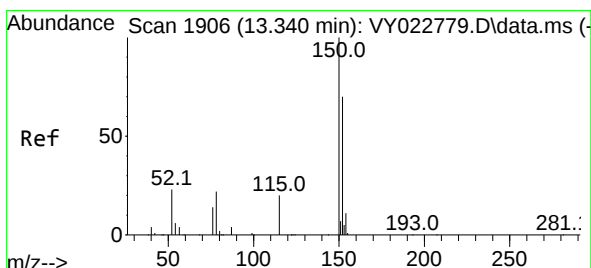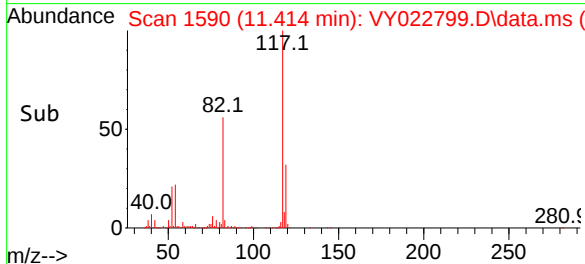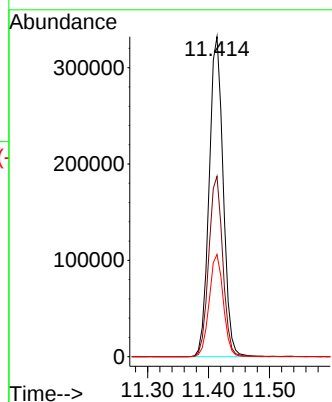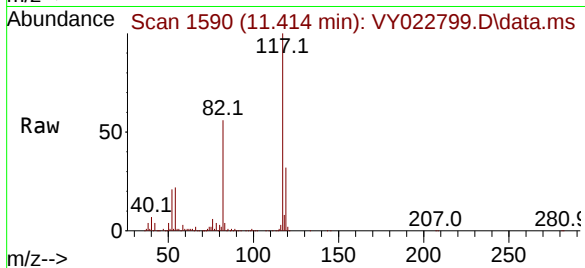

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.340 min Scan# 1906

Delta R.T. -0.006 min

Lab File: VY022799.D

Acq: 24 Jun 2025 15:52

Tgt Ion:152 Resp: 229194

Ion Ratio Lower Upper

152 100

115 56.6 28.9 86.7

150 157.7 0.0 349.6

