
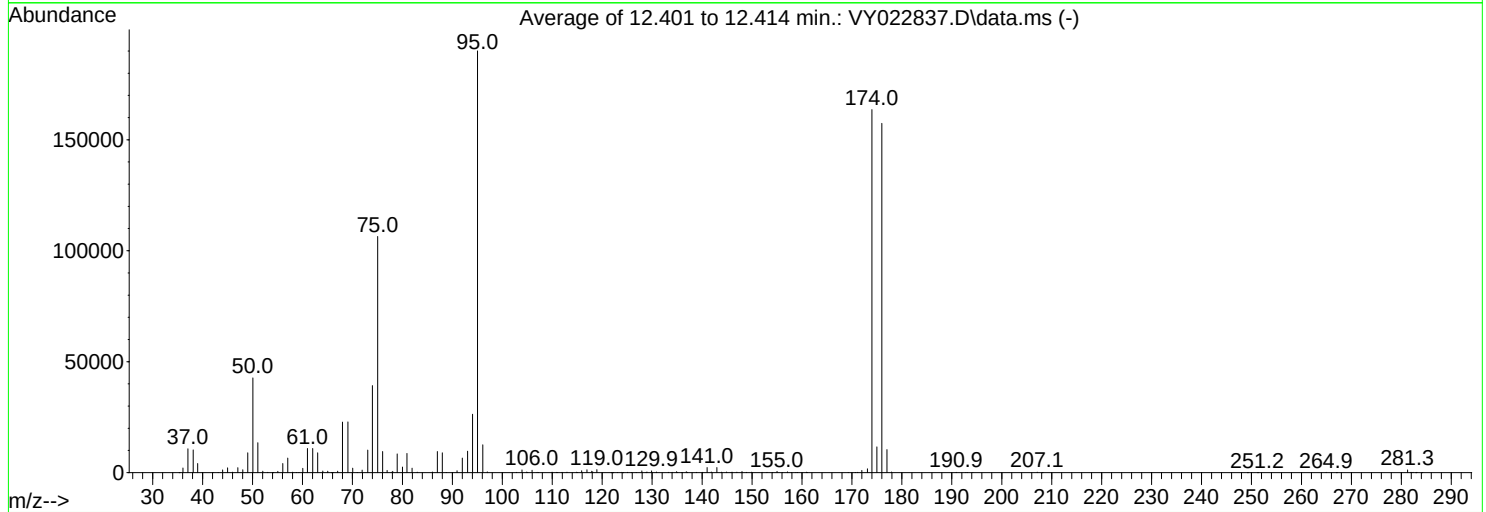


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062625\
Data File : VY022837.D
Acq On : 26 Jun 2025 08:22
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Title : SW846 8260
Last Update : Tue Jun 24 08:29:52 2025

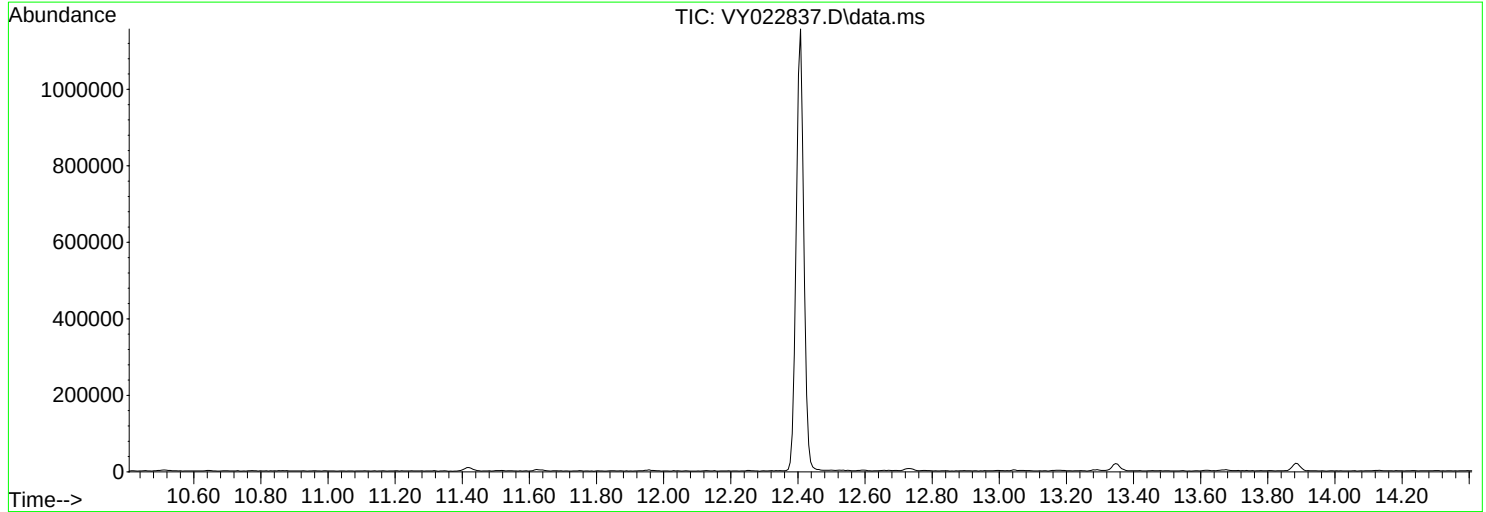

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	42709	PASS
75	95	30	60	56.0	106432	PASS
95	95	100	100	100.0	190080	PASS
96	95	5	9	6.6	12523	PASS
173	174	0.00	2	1.1	1740	PASS
174	95	50	100	86.1	163584	PASS
175	174	5	9	7.1	11621	PASS
176	174	95	101	96.2	157440	PASS
177	176	5	9	6.6	10420	PASS