
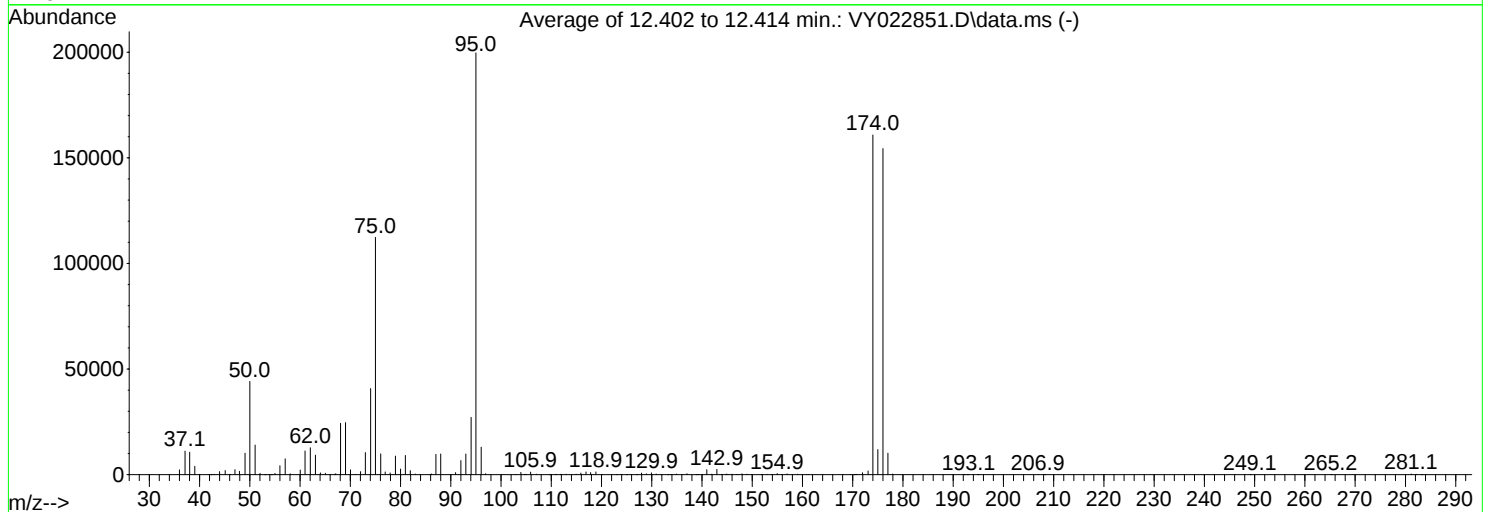


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062725\
Data File : VY022851.D
Acq On : 27 Jun 2025 08:31
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062325S.M
Title : SW846 8260
Last Update : Tue Jun 24 08:29:52 2025

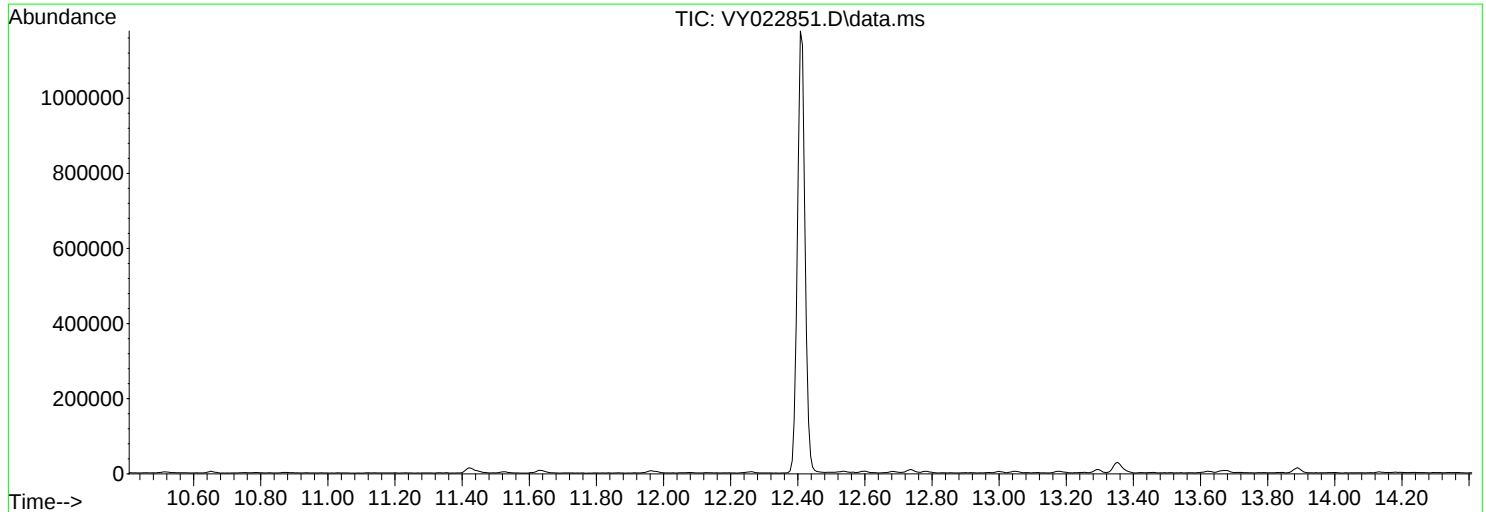

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	44155	PASS
75	95	30	60	56.2	112323	PASS
95	95	100	100	100.0	199701	PASS
96	95	5	9	6.5	13001	PASS
173	174	0.00	2	1.1	1732	PASS
174	95	50	100	80.5	160829	PASS
175	174	5	9	7.4	11902	PASS
176	174	95	101	96.0	154371	PASS
177	176	5	9	6.6	10181	PASS