

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070822\
 Data File : VY009485.D
 Acq On : 08 Jul 2022 16:13
 Operator : KP/MD
 Sample : N3595-05
 Misc : 4.20g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 20220488B-6B

Quant Time: Jul 11 02:15:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070722S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 08 11:00:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	184729	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	283135	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	234039	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	104097	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	72452	56.524	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 113.040%			
35) Dibromofluoromethane	7.710	113	59769	40.120	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 80.240%			
50) Toluene-d8	10.173	98	236347	59.388	ug/l	0.00
Spiked Amount 50.000	Range 78 - 125		Recovery = 118.780%			
62) 4-Bromofluorobenzene	12.477	95	88255	41.968	ug/l	0.00
Spiked Amount 50.000	Range 50 - 146		Recovery = 83.940%			
Target Compounds						Qvalue
10) Methyl Iodide	4.082	142	60	4.187	ug/l #	75
11) Tert butyl alcohol	4.930	59	516	Below Cal	#	77
13) Acrolein	3.729	56	497	33.227	ug/l #	14
16) Acetone	3.936	43	118693	264.126	ug/l	98
17) Carbon Disulfide	4.180	76	69310	17.003	ug/l	100
20) Methylene Chloride	4.704	84	7722	Below Cal		90
23) Vinyl Acetate	6.076	43	200	Below Cal	#	75
25) 2-Butanone	6.978	43	38602	53.101	ug/l	97
31) Cyclohexane	7.777	56	7440	2.455	ug/l #	53
36) 1,1-Dichloropropene	7.783	75	13808	5.693	ug/l #	50
37) Ethyl Acetate	6.978	43	38602	25.391	ug/l #	72
38) Carbon Tetrachloride	7.789	117	17187	6.626	ug/l #	14
39) Methylcyclohexane	9.179	83	14414	4.951	ug/l	99
40) Benzene	8.155	78	13139	1.845	ug/l #	84
43) Isopropyl Acetate	8.252	43	2922	1.030	ug/l #	56
55) 1,1,2-Trichloroethane	10.618	97	5452	3.572	ug/l #	26
59) 2-Hexanone	10.794	43	25787	24.946	ug/l #	35
68) m/p-Xylenes	11.703	106	4708	1.504	ug/l	91
69) o-Xylene	12.026	106	5925	1.975	ug/l	88
74) N-amyl acetate	12.117	43	99535	49.139	ug/l #	67
75) 1,1,2,2-Tetrachloroethane	12.550	83	8067	5.659	ug/l #	26
76) 1,2,3-Trichloropropane	12.477	75	45807	41.569	ug/l #	100
79) 2-Chlorotoluene	12.806	91	5055	1.050	ug/l	95
80) 1,3,5-Trimethylbenzene	12.806	105	19155	3.219	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.477	75	45807	85.077	ug/l #	14
82) 4-Chlorotoluene	12.806	91	5055	1.002	ug/l	95
84) 1,2,4-Trimethylbenzene	13.117	105	22673	3.828	ug/l	99
90) Hexachloroethane	13.965	117	1748	1.371	ug/l #	10
95) Naphthalene	15.227	128	6290	1.591	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070822\
Data File : VY009485.D
Acq On : 08 Jul 2022 16:13
Operator : KP/MD
Sample : N3595-05
Misc : 4.20g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B

Quant Time: Jul 11 02:15:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070722S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 08 11:00:56 2022
Response via : Initial Calibration




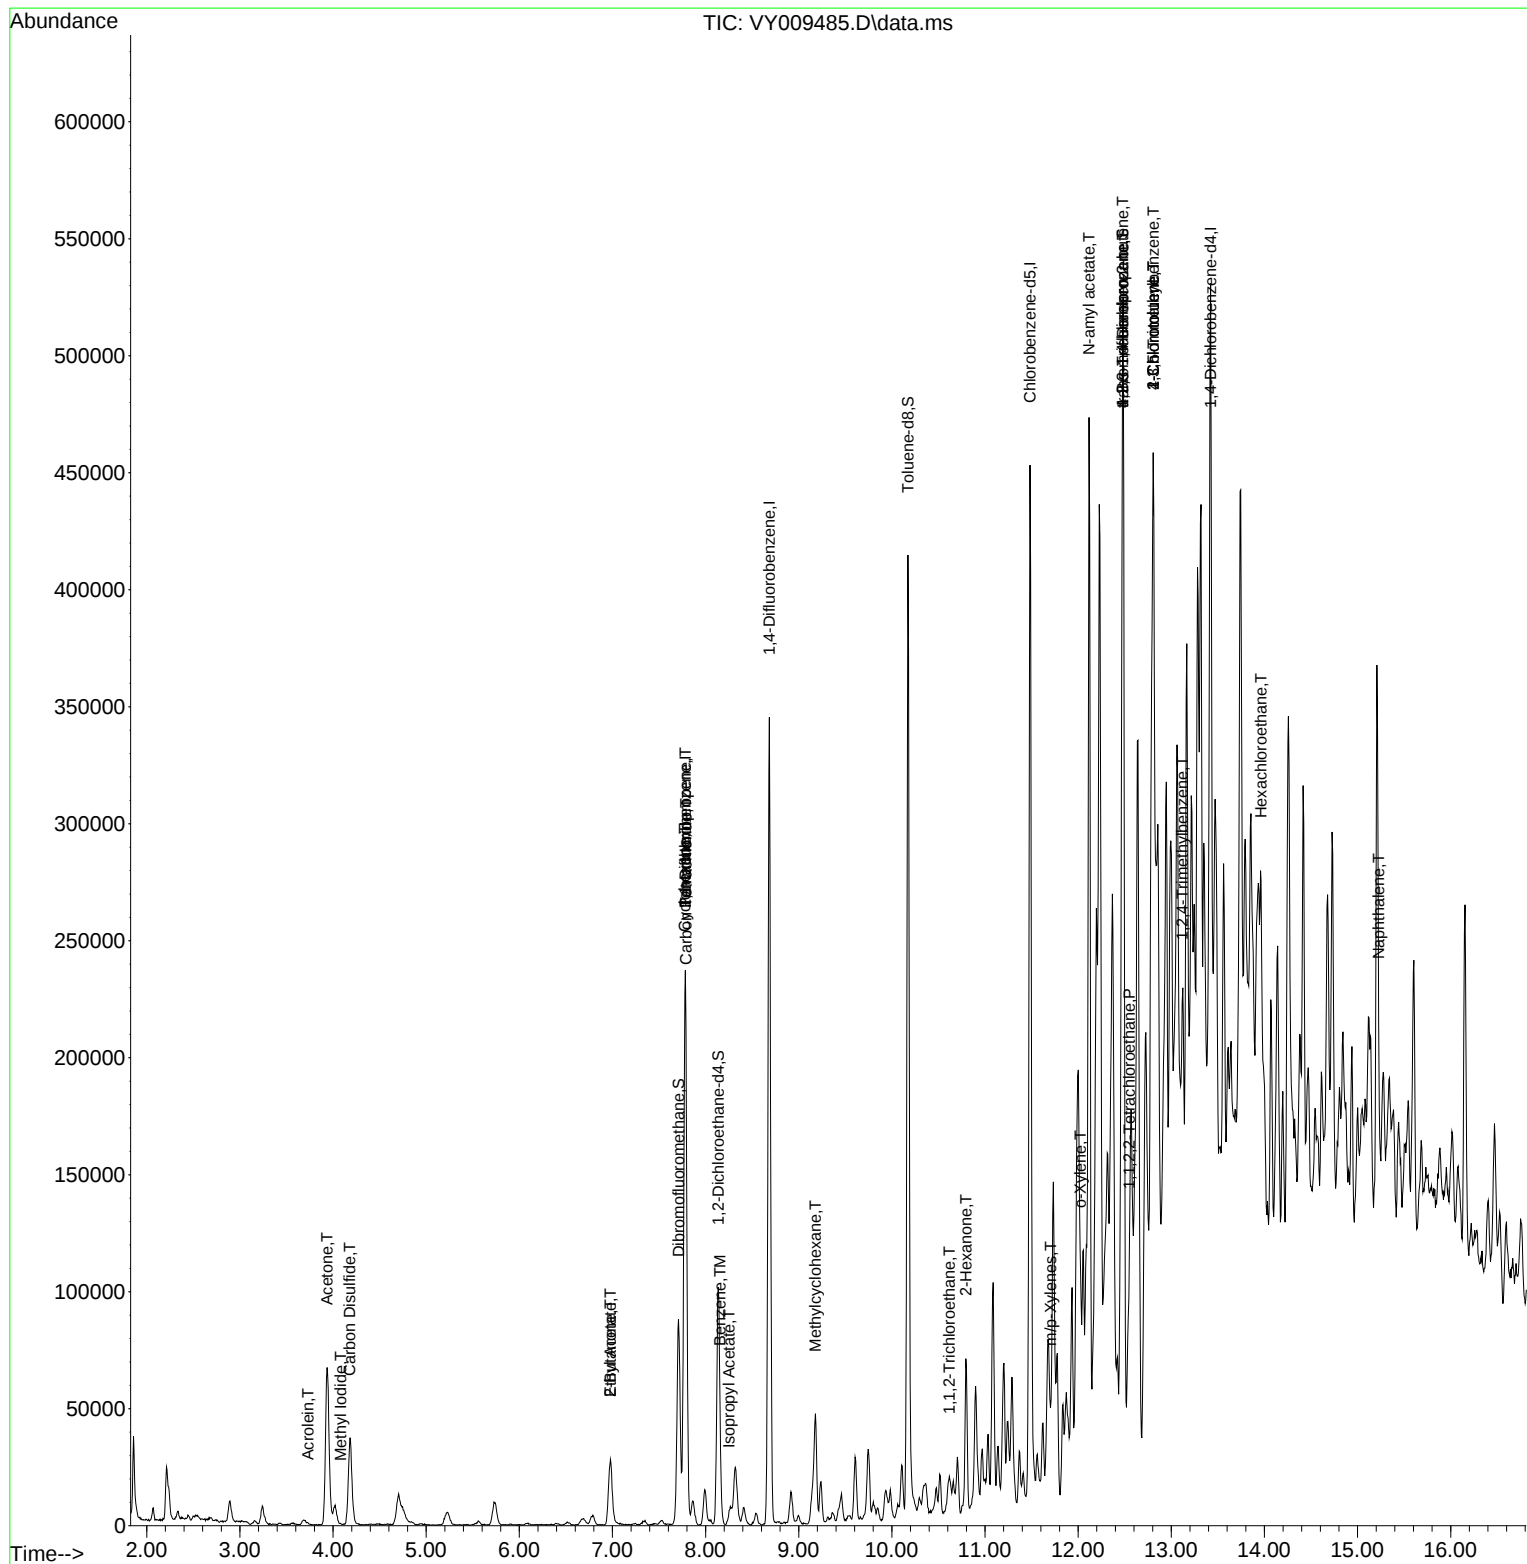


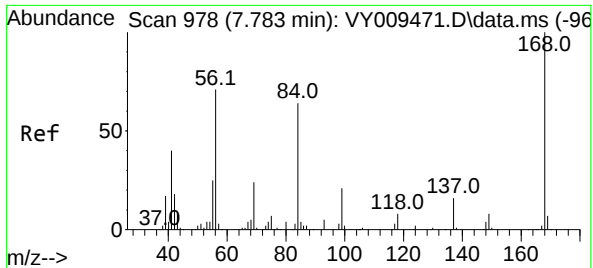

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion:168 Resp: 184729
Ion Ratio Lower Upper
168 100
99 51.5 46.9 70.3

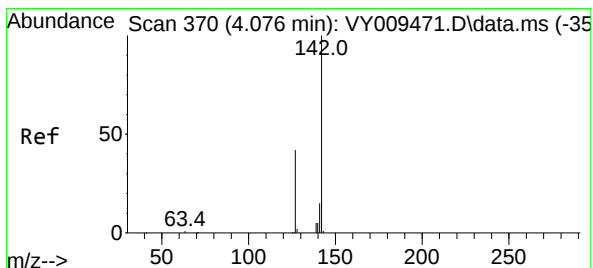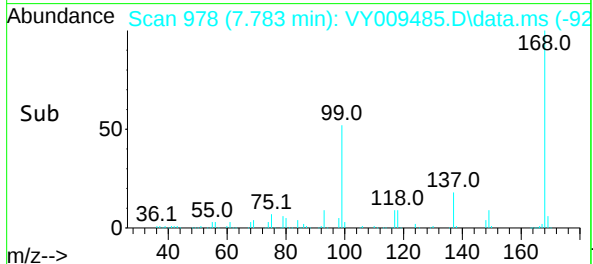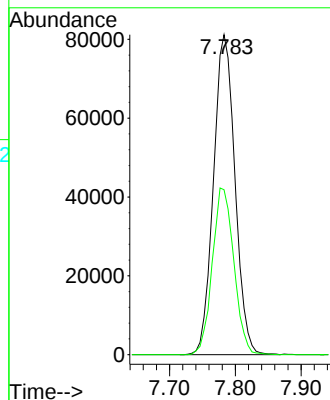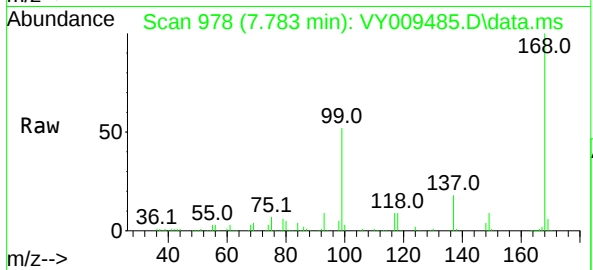

#10
Methyl Iodide
Concen: 4.187 ug/l
RT: 4.082 min Scan# 371
Delta R.T. 0.006 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion:142 Resp: 60
Ion Ratio Lower Upper
142 100
127 36.7 41.5 62.3#
141 0.0 11.9 17.9#

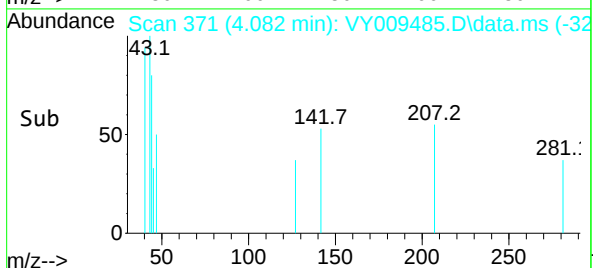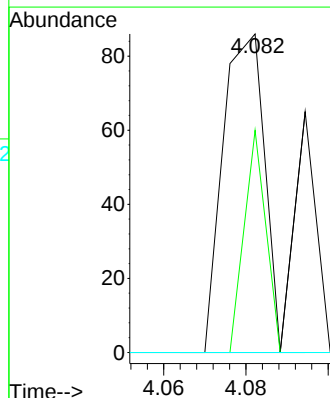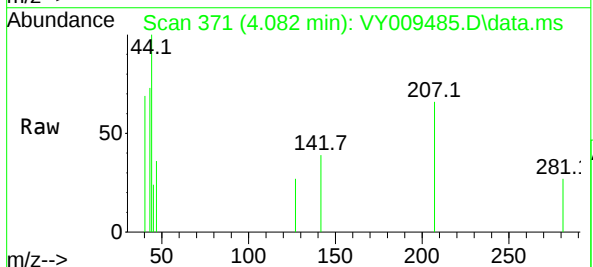



#11

Tert butyl alcohol

Concen: Below Cal

RT: 4.930 min Scan# 513

Delta R.T. -0.018 min

Lab File: VY009485.D

Acq: 08 Jul 2022 16:13

Instrument :

MSVOA_Y

ClientSampleId :





20220488B-6B

Tgt Ion: 59 Resp: 516

Ion Ratio Lower Upper

59 100

57 0.0 6.4 9.6#

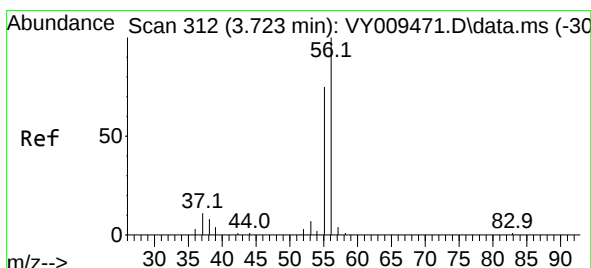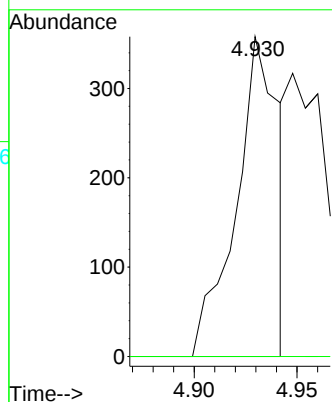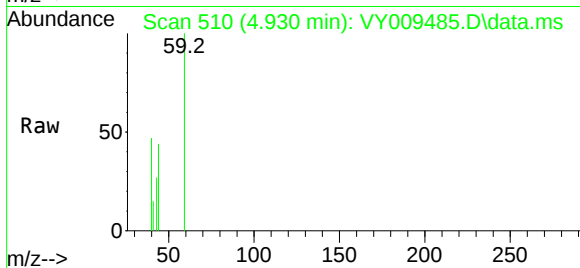

#13

Acrolein

Concen: 33.227 ug/l

RT: 3.729 min Scan# 313

Delta R.T. 0.006 min

Lab File: VY009485.D




Acq: 08 Jul 2022 16:13


Tgt Ion: 56 Resp: 497

Ion Ratio Lower Upper

56 100

55 0.0 57.6 86.4#


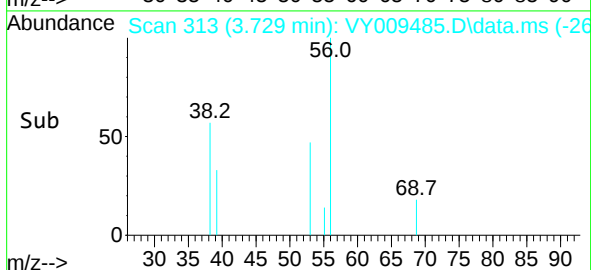

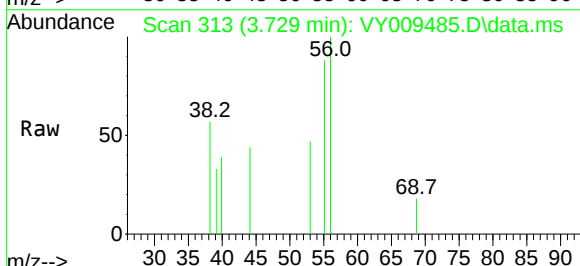




#16
Acetone
Concen: 264.126 ug/l
RT: 3.936 min Scan# 347
Delta R.T. -0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion: 43 Resp: 118693
Ion Ratio Lower Upper
43 100
58 28.4 22.0 33.0

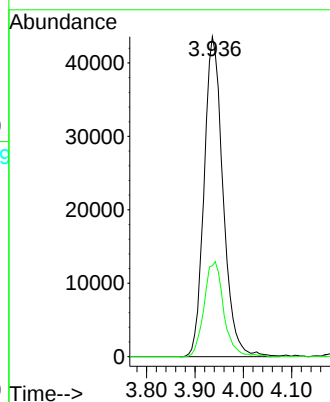

#17
Carbon Disulfide
Concen: 17.003 ug/l
RT: 4.180 min Scan# 387
Delta R.T. -0.006 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion: 76 Resp: 69310
Ion Ratio Lower Upper
76 100
78 9.1 7.4 11.0


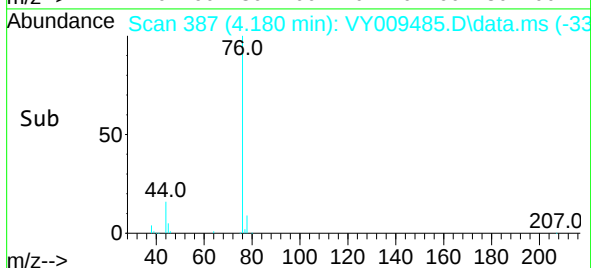
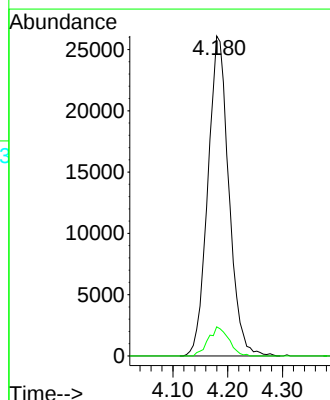





#20
Methylene Chloride
Concen: Below Cal
RT: 4.704 min Scan# 41
Delta R.T. 0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion:	84	Resp:	7722
Ion	Ratio	Lower	Upper
84	100		
49	129.3	114.4	171.6
51	39.8	35.3	52.9
86	75.6	53.7	80.5

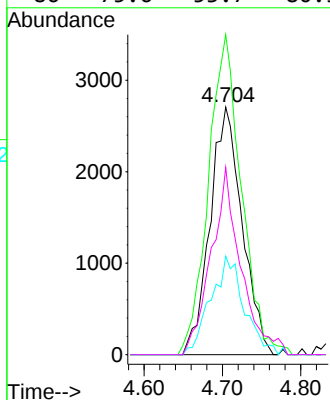

#23
Vinyl Acetate
Concen: Below Cal
RT: 6.076 min Scan# 698
Delta R.T. 0.025 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion:	43	Resp:	200
Ion	Ratio	Lower	Upper
43	100		
86	0.0	7.1	10.7#


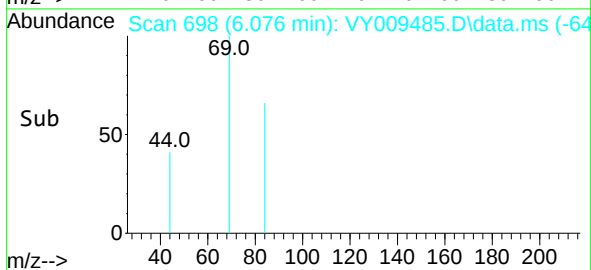
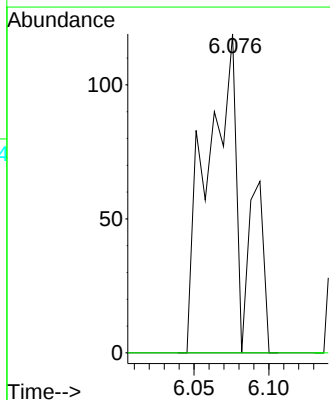



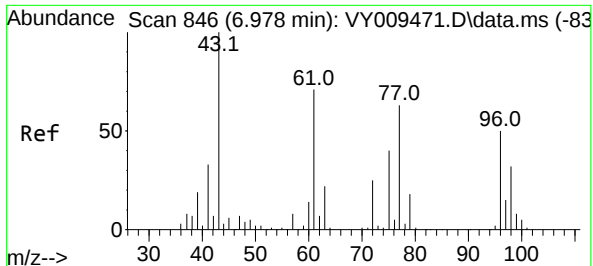

#25
2-Butanone
Concen: 53.101 ug/l
RT: 6.978 min Scan# 846
Delta R.T. 0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion: 43 Resp: 38602
Ion Ratio Lower Upper
43 100
72 23.8 17.7 26.5

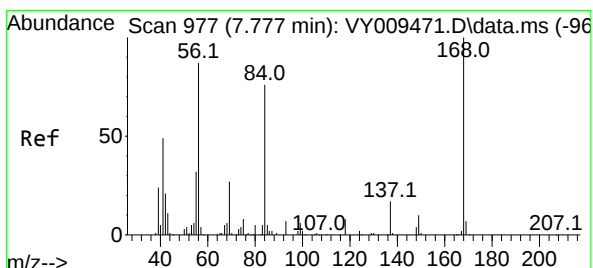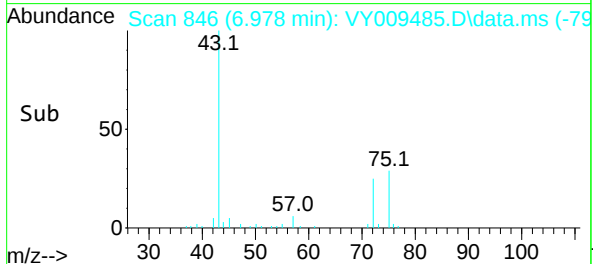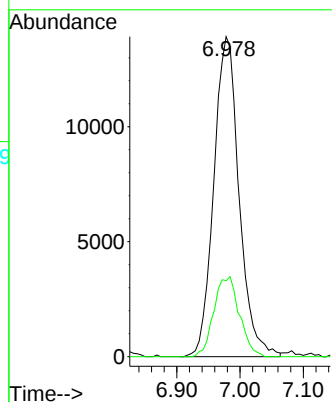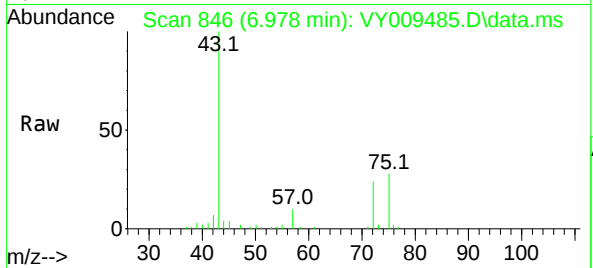

#31
Cyclohexane
Concen: 2.455 ug/l
RT: 7.777 min Scan# 977
Delta R.T. -0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion: 56 Resp: 7440
Ion Ratio Lower Upper
56 100
69 104.6 26.7 40.1#
84 98.9 67.2 100.8


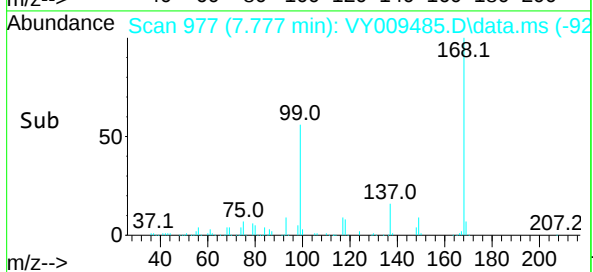
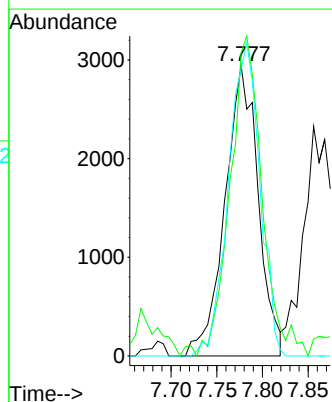
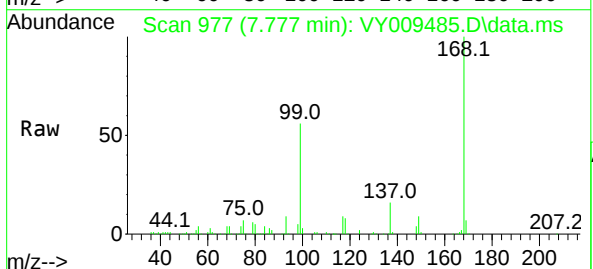


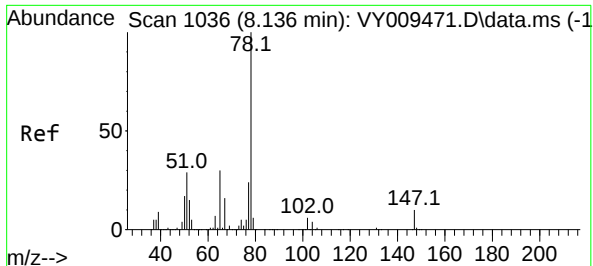

#33
 1,2-Dichloroethane-d4
 Concen: 56.524 ug/l
 RT: 8.136 min Scan# 1036
 Delta R.T. 0.000 min
 Lab File: VY009485.D
 Acq: 08 Jul 2022 16:13




Instrument :
 MSVOA_Y
 ClientSampleId :
 20220488B-6B


Tgt Ion: 65 Resp: 72452
 Ion Ratio Lower Upper
 65 100
 67 52.8 0.0 99.4

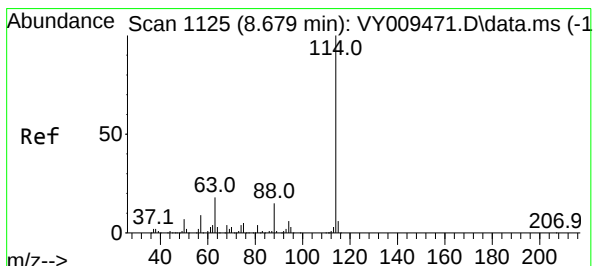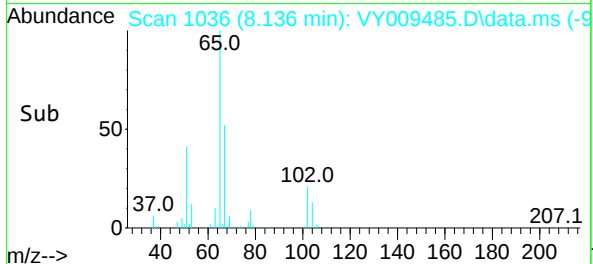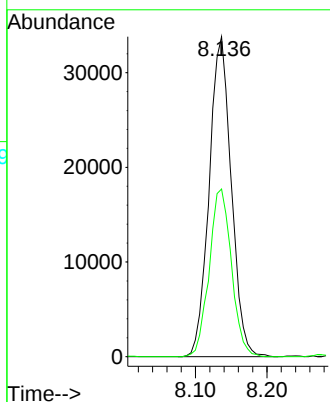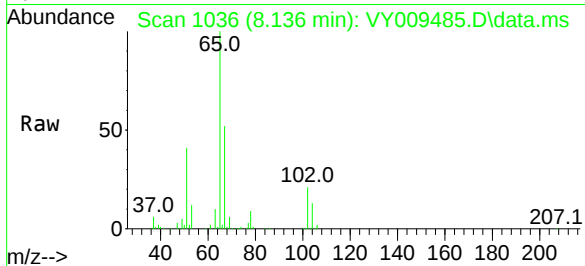

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.685 min Scan# 1126
 Delta R.T. 0.006 min
 Lab File: VY009485.D
 Acq: 08 Jul 2022 16:13

Tgt Ion: 114 Resp: 283135
 Ion Ratio Lower Upper
 114 100
 63 19.1 0.0 43.2
 88 15.2 0.0 31.8

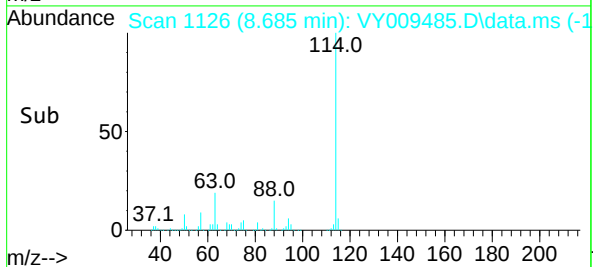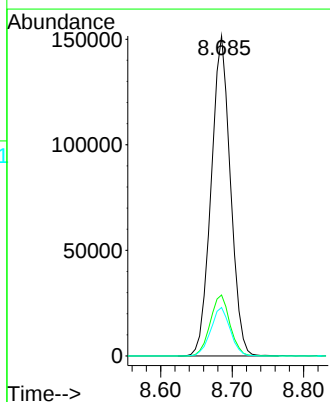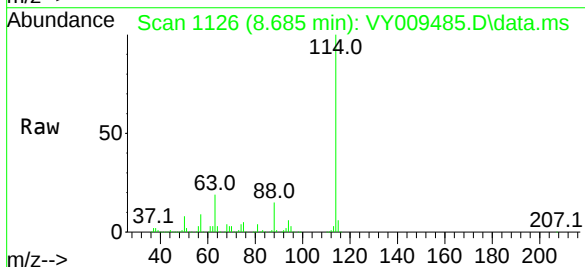



#35

Dibromofluoromethane

Concen: 40.120 ug/l

RT: 7.710 min Scan# 91

Delta R.T. -0.000 min

Lab File: VY009485.D

Acq: 08 Jul 2022 16:13

Instrument :

MSVOA_Y

ClientSampleId :

20220488B-6B





Tgt Ion:113 Resp: 59769

Ion Ratio Lower Upper

113 100

111 103.7 82.6 124.0

192 21.9 17.6 26.4

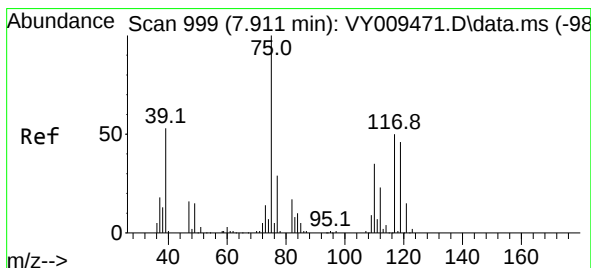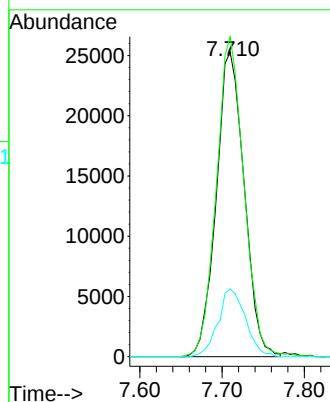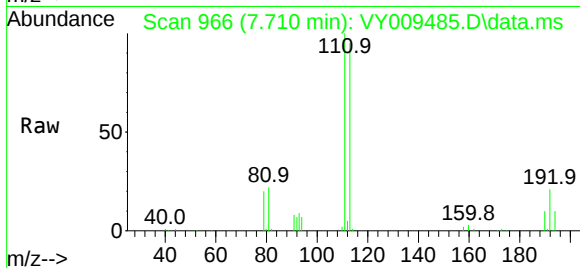

#36

1,1-Dichloropropene

Concen: 5.693 ug/l

RT: 7.783 min Scan# 978

Delta R.T. -0.128 min

Lab File: VY009485.D

Acq: 08 Jul 2022 16:13




Tgt Ion: 75 Resp: 13808


Ion Ratio Lower Upper

75 100

110 8.8 17.1 51.2#

77 0.0 24.4 36.6#

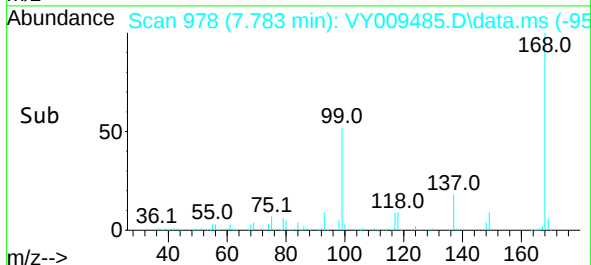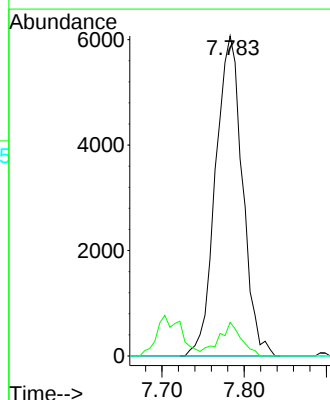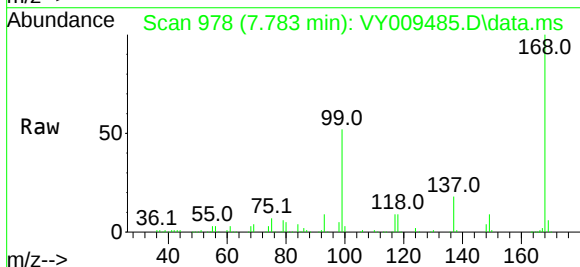



#37

Ethyl Acetate

Concen: 25.391 ug/l

RT: 6.978 min Scan# 84

Delta R.T. -0.085 min

Lab File: VY009485.D


Acq: 08 Jul 2022 16:13

Instrument :

MSVOA_Y

ClientSampleId :

20220488B-6B

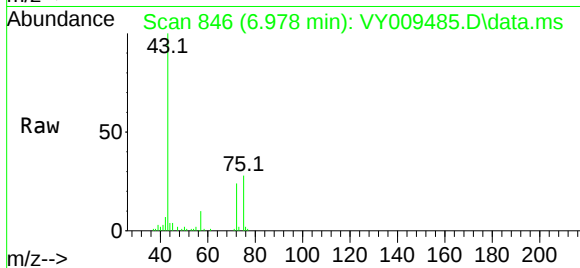




Tgt Ion: 43 Resp: 38602

Ion Ratio Lower Upper

43 100

61 0.3 9.7 14.5#

70 0.0 7.1 10.7#

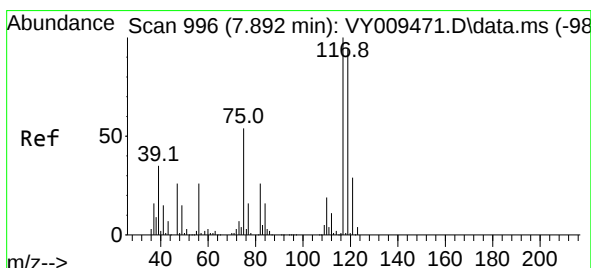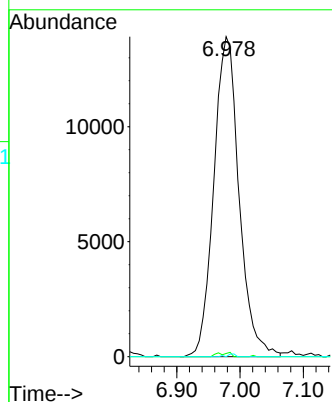

#38

Carbon Tetrachloride

Concen: 6.626 ug/l

RT: 7.789 min Scan# 979

Delta R.T. -0.103 min

Lab File: VY009485.D

Acq: 08 Jul 2022 16:13




Tgt Ion: 117 Resp: 17187


Ion Ratio Lower Upper

117 100

119 3.8 77.9 116.9#

121 0.0 24.8 37.2#

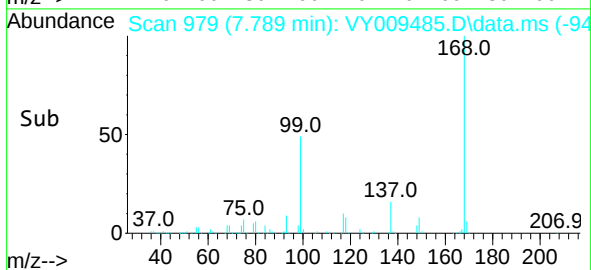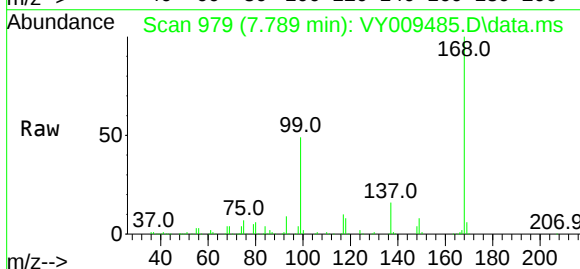

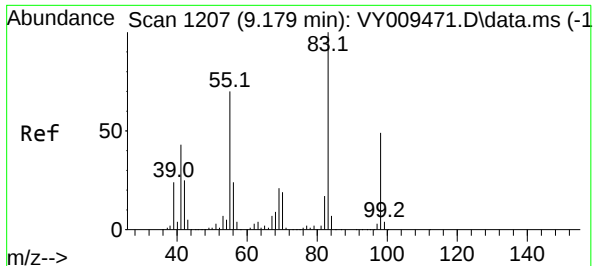

#39

Methylcyclohexane

Concen: 4.951 ug/l

RT: 9.179 min Scan# 1

Delta R.T. -0.000 min

Lab File: VY009485.D

Acq: 08 Jul 2022 16:13

Instrument :

MSVOA_Y

ClientSampleId :

20220488B-6B





Tgt Ion: 83 Resp: 14414

Ion Ratio Lower Upper

83 100

55 81.0 66.5 99.7

98 47.4 37.9 56.9

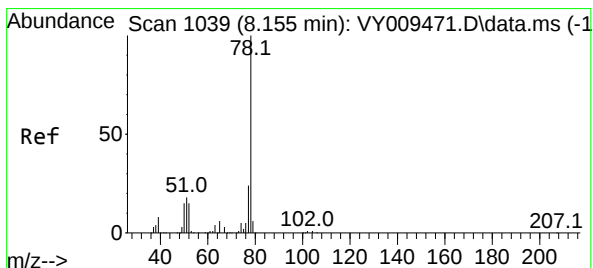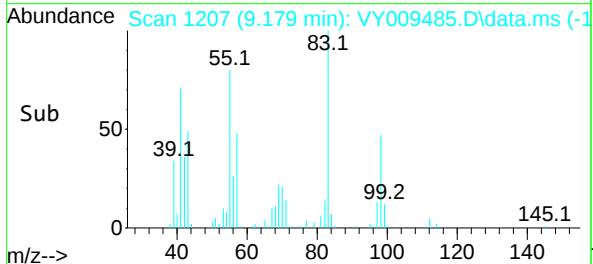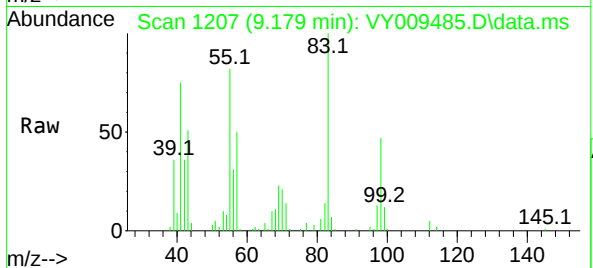

#40

Benzene

Concen: 1.845 ug/l

RT: 8.155 min Scan# 1039

Delta R.T. -0.000 min

Lab File: VY009485.D




Acq: 08 Jul 2022 16:13


Tgt Ion: 78 Resp: 13139

Ion Ratio Lower Upper

78 100

77 17.6 20.4 30.6#


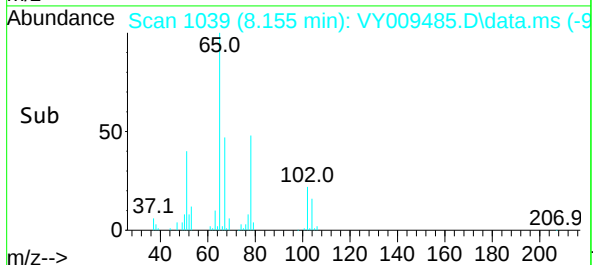

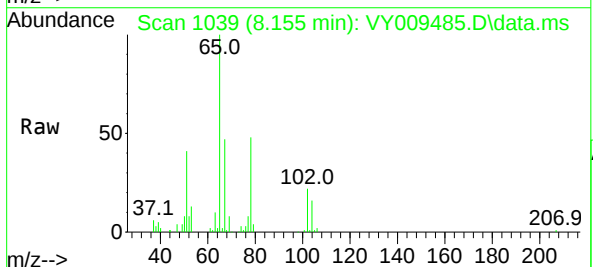




#43
Isopropyl Acetate
Concen: 1.030 ug/l
RT: 8.252 min Scan# 1055
Delta R.T. -0.012 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion: 43 Resp: 2922
Ion Ratio Lower Upper
43 100
61 0.0 20.2 30.2#
87 0.0 8.9 13.3#

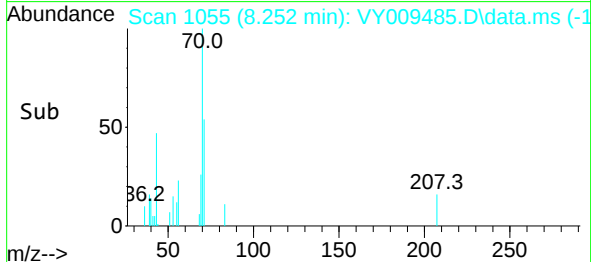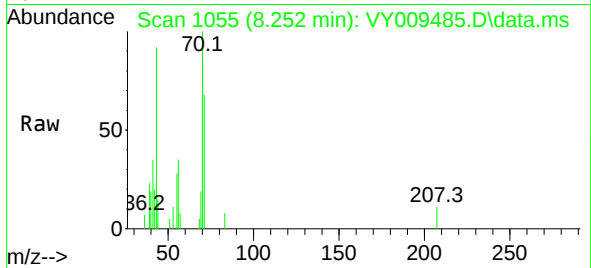

#50
Toluene-d8
Concen: 59.388 ug/l
RT: 10.173 min Scan# 1370
Delta R.T. -0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion: 98 Resp: 236347
Ion Ratio Lower Upper
98 100
100 65.4 50.2 75.2


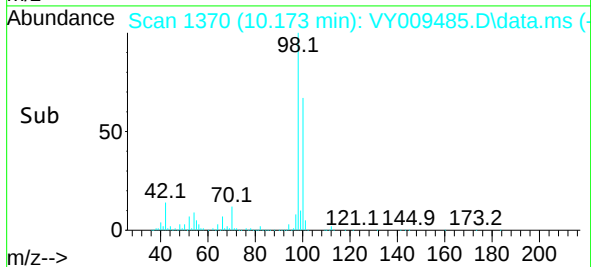

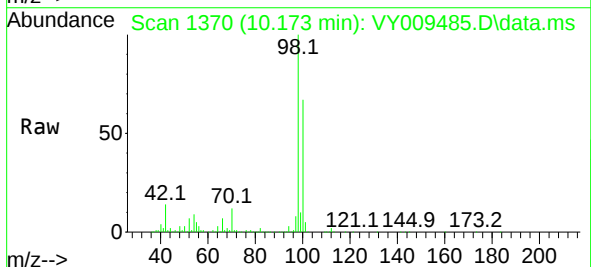




#55
1,1,2-Trichloroethane
Concen: 3.572 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.024 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion: 97	Resp: 5452
Ion Ratio	Lower Upper
97 100	
83 7.8	69.8 104.8#
85 21.3	44.3 66.5#
99 0.0	49.8 74.6#

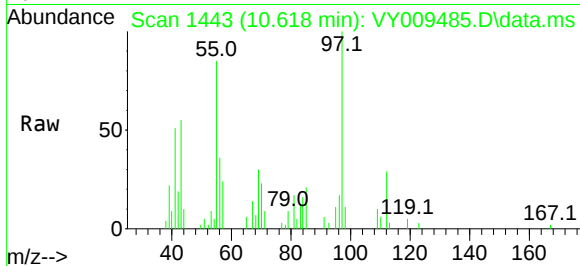

#59
2-Hexanone
Concen: 24.946 ug/l
RT: 10.794 min Scan# 1472
Delta R.T. -0.031 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion: 43	Resp: 25787		
Ion Ratio	Lower	Upper	
43 100			
58 4.5	24.4	73.4#	


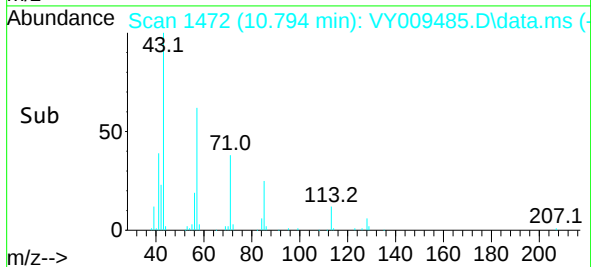

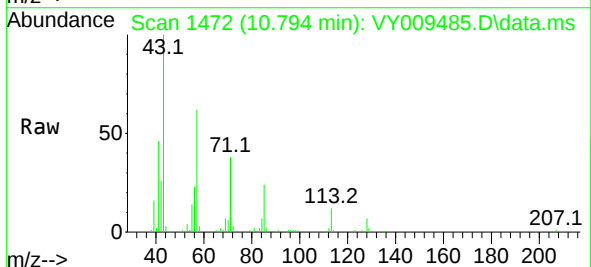




#62
4-Bromofluorobenzene
Concen: 41.968 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion: 95 Resp: 88255
Ion Ratio Lower Upper
95 100
174 80.2 0.0 177.0
176 78.8 0.0 175.8

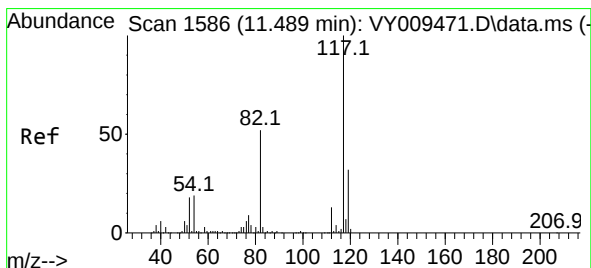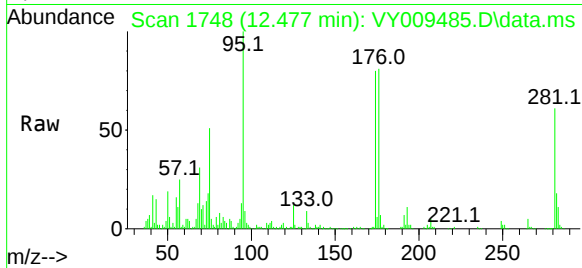

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.483 min Scan# 1585
Delta R.T. -0.006 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion: 117 Resp: 234039
Ion Ratio Lower Upper
117 100
82 53.4 43.0 64.4
119 31.3 25.4 38.0


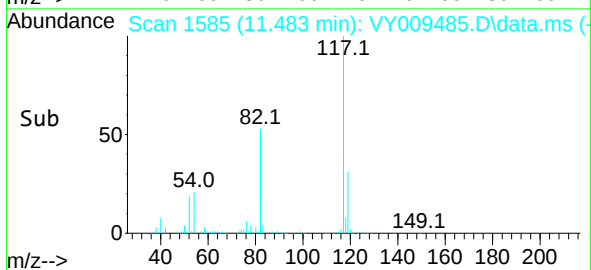

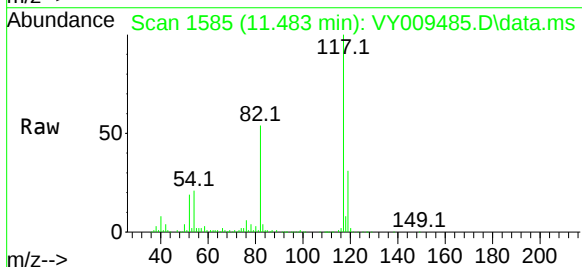


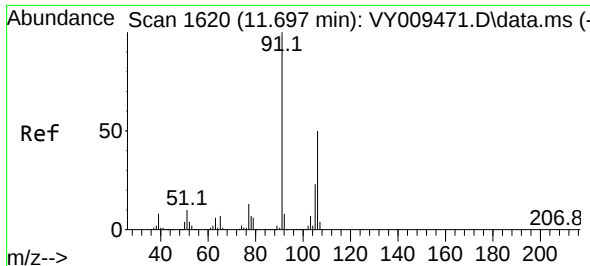

#68
m/p-Xylenes
Concen: 1.504 ug/l
RT: 11.703 min Scan# 1621
Delta R.T. 0.006 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion:106 Resp: 4708
Ion Ratio Lower Upper
106 100
91 221.8 166.6 249.8

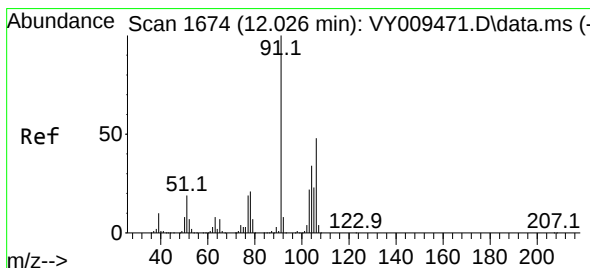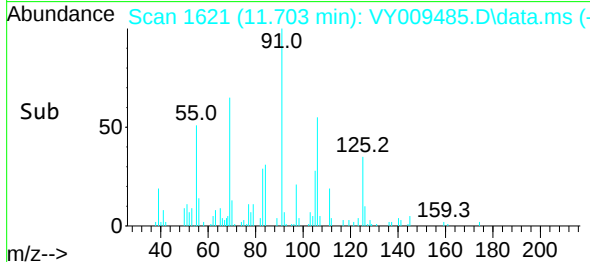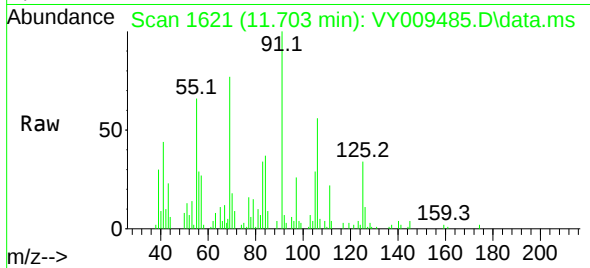

#69
o-Xylene
Concen: 1.975 ug/l
RT: 12.026 min Scan# 1674
Delta R.T. -0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion:106 Resp: 5925
Ion Ratio Lower Upper
106 100
91 200.6 110.3 331.0


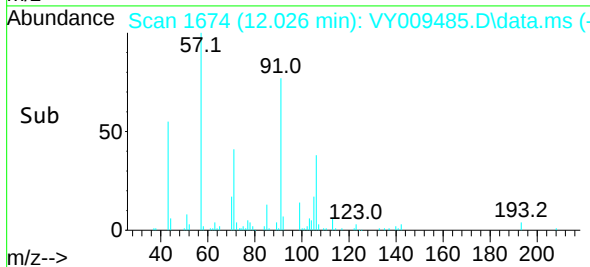

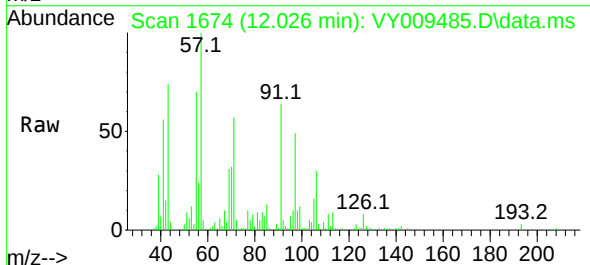




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion:152 Resp: 104097
Ion Ratio Lower Upper
152 100
115 55.3 28.2 84.7
150 148.9 0.0 347.6

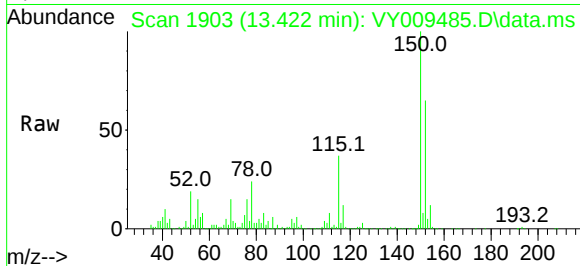

#74
N-ethyl acetate
Concen: 49.139 ug/l
RT: 12.117 min Scan# 1689
Delta R.T. -0.025 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion: 43 Resp: 99535
Ion Ratio Lower Upper
43 100
70 9.8 28.7 43.1#
55 21.7 17.3 25.9
61 0.0 17.0 25.6#


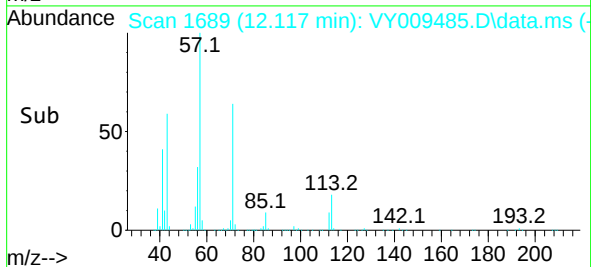

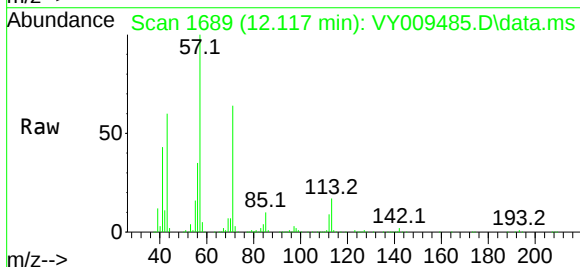




#75
 1,1,2,2-Tetrachloroethane
 Concen: 5.659 ug/l
 RT: 12.550 min Scan# 1760
 Delta R.T. -0.025 min
 Lab File: VY009485.D
 Acq: 08 Jul 2022 16:13




Instrument :
 MSVOA_Y
 ClientSampleId :
 20220488B-6B


Tgt Ion: 83 Resp: 8067
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.6 16.8#
 85 0.0 32.3 96.8#

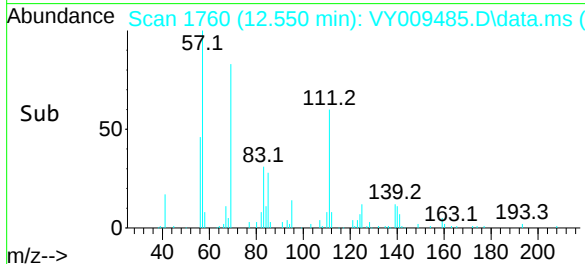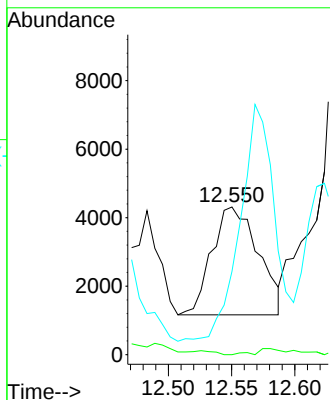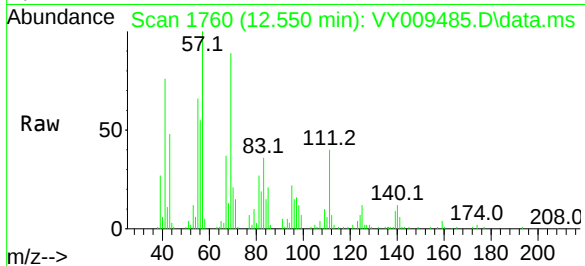

#76
 1,2,3-Trichloropropane
 Concen: 41.569 ug/l
 RT: 12.477 min Scan# 1748
 Delta R.T. -0.152 min
 Lab File: VY009485.D
 Acq: 08 Jul 2022 16:13

Tgt Ion: 75 Resp: 45807
 Ion Ratio Lower Upper
 75 100
 77 3.1 0.0 0.0#

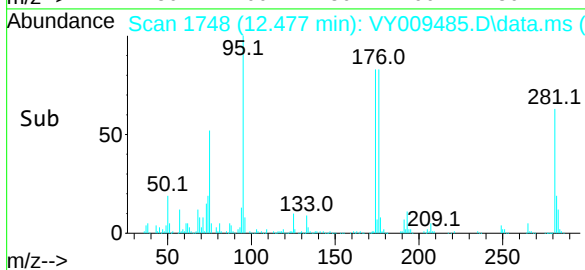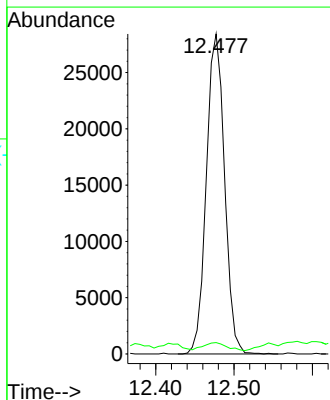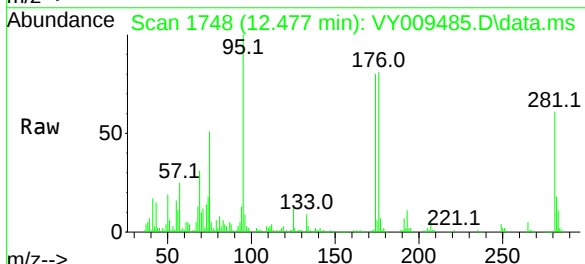



#79

2-Chlorotoluene

Concen: 1.050 ug/l

RT: 12.806 min Scan# 1802

Delta R.T. 0.055 min

Lab File: VY009485.D

Acq: 08 Jul 2022 16:13

Instrument :

MSVOA_Y

ClientSampleId :





20220488B-6B

Tgt Ion: 91 Resp: 5055

Ion Ratio Lower Upper

91 100

126 30.9 16.9 50.6

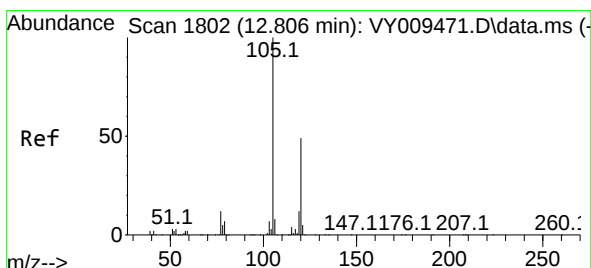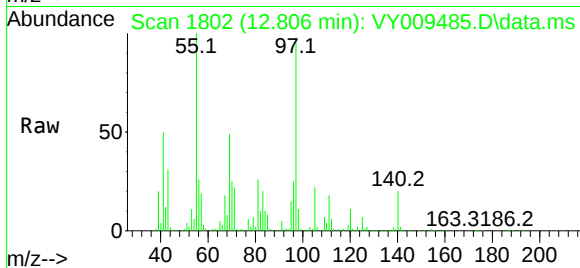

#80

1,3,5-Trimethylbenzene

Concen: 3.219 ug/l

RT: 12.806 min Scan# 1802

Delta R.T. 0.000 min

Lab File: VY009485.D




Acq: 08 Jul 2022 16:13


Tgt Ion: 105 Resp: 19155

Ion Ratio Lower Upper

105 100

120 49.8 24.4 73.4


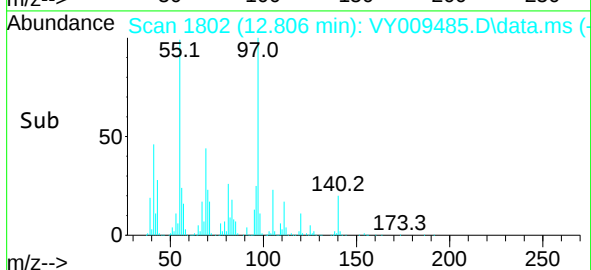

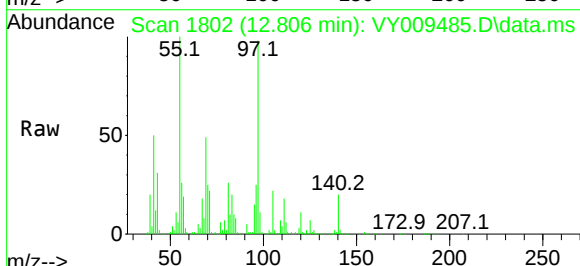




#81
trans-1,4-Dichloro-2-butene
Concen: 85.077 ug/l
RT: 12.477 min Scan# 1731
Delta R.T. 0.104 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13




Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B


Tgt Ion: 75 Resp: 45807
Ion Ratio Lower Upper
75 100
53 9.0 85.3 127.9#
89 1.7 37.0 55.4#

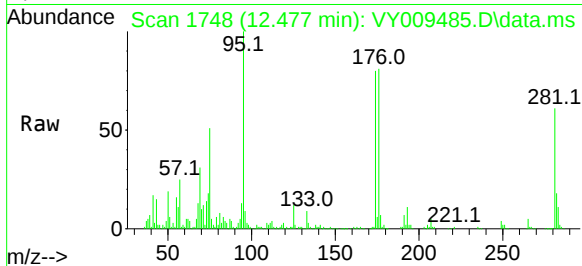

#82
4-Chlorotoluene
Concen: 1.002 ug/l
RT: 12.806 min Scan# 1802
Delta R.T. -0.043 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Tgt Ion: 91 Resp: 5055
Ion Ratio Lower Upper
91 100
126 30.9 17.0 51.0

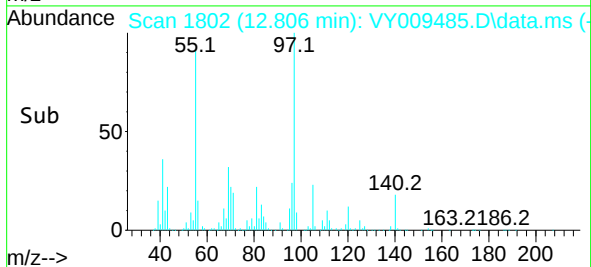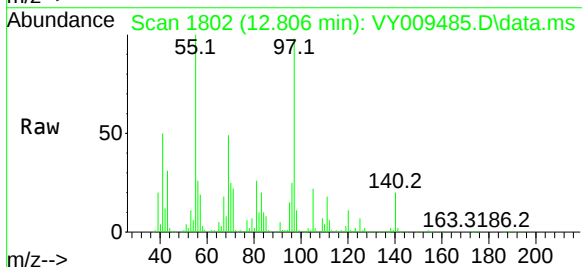

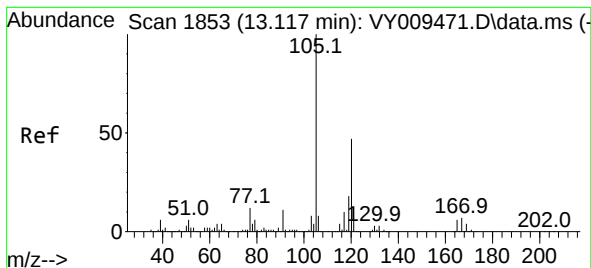

#84

1,2,4-Trimethylbenzene

Concen: 3.828 ug/l

RT: 13.117 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY009485.D

Acq: 08 Jul 2022 16:13

Instrument :

MSVOA_Y

ClientSampleId :





20220488B-6B

Tgt Ion:105 Resp: 22673

Ion Ratio Lower Upper

105 100

120 45.1 22.3 66.9

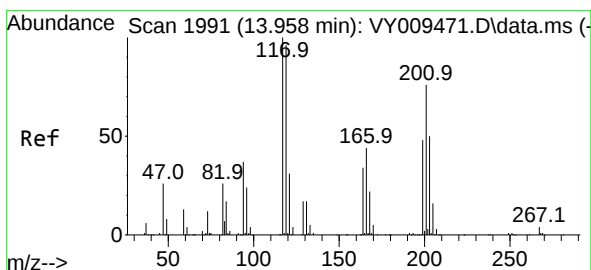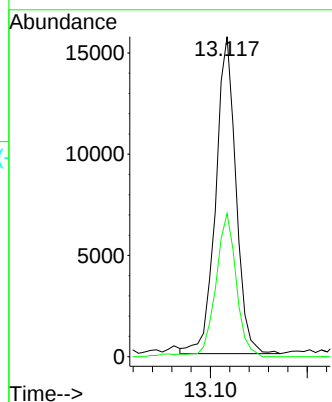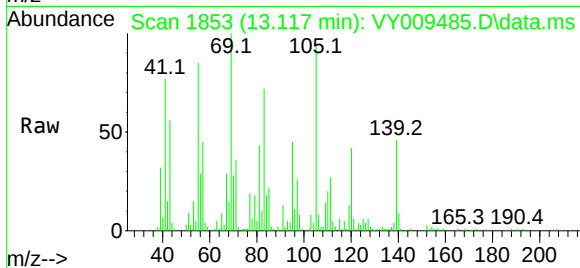

#90

Hexachloroethane

Concen: 1.371 ug/l

RT: 13.965 min Scan# 1992

Delta R.T. 0.007 min

Lab File: VY009485.D




Acq: 08 Jul 2022 16:13


Tgt Ion:117 Resp: 1748

Ion Ratio Lower Upper

117 100


201 3.1 43.0 128.8#

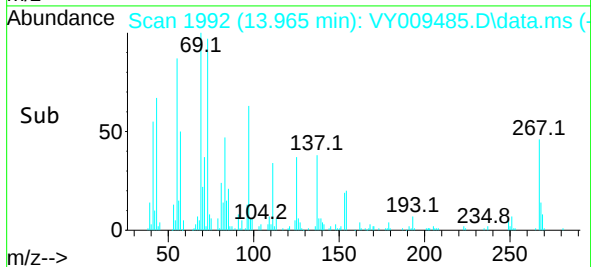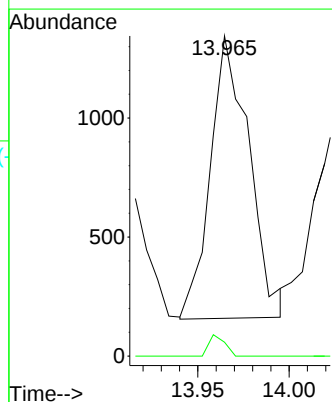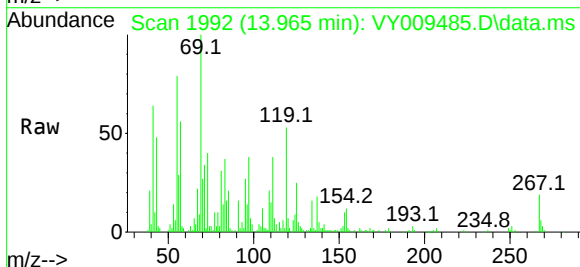

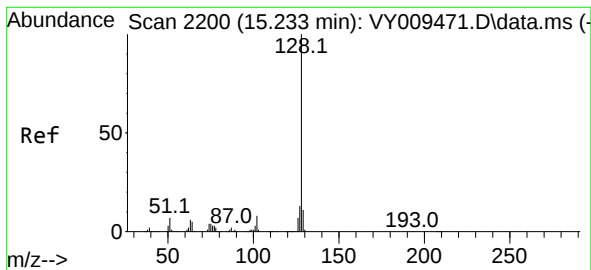

#95
Naphthalene
Concen: 1.591 ug/l
RT: 15.227 min Scan# 21
Delta R.T. -0.006 min
Lab File: VY009485.D
Acq: 08 Jul 2022 16:13

Instrument :
MSVOA_Y
ClientSampleId :
20220488B-6B

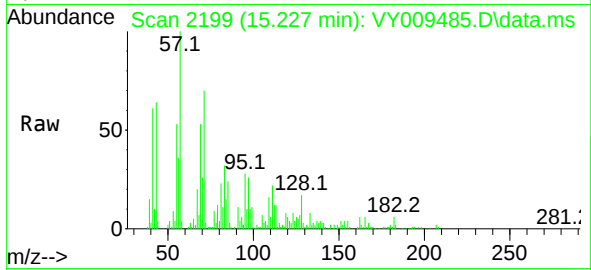

Tgt Ion:128 Resp: 6290
Ion Ratio Lower Upper
128 100
127 0.0 11.0 16.4#
129 8.2 8.4 12.6#

