


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070822\
Data File : VY009476.D
Acq On : 08 Jul 2022 09:31
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070722S.M
Title : SW846 8260
Last Update : Fri Jul 08 11:00:56 2022

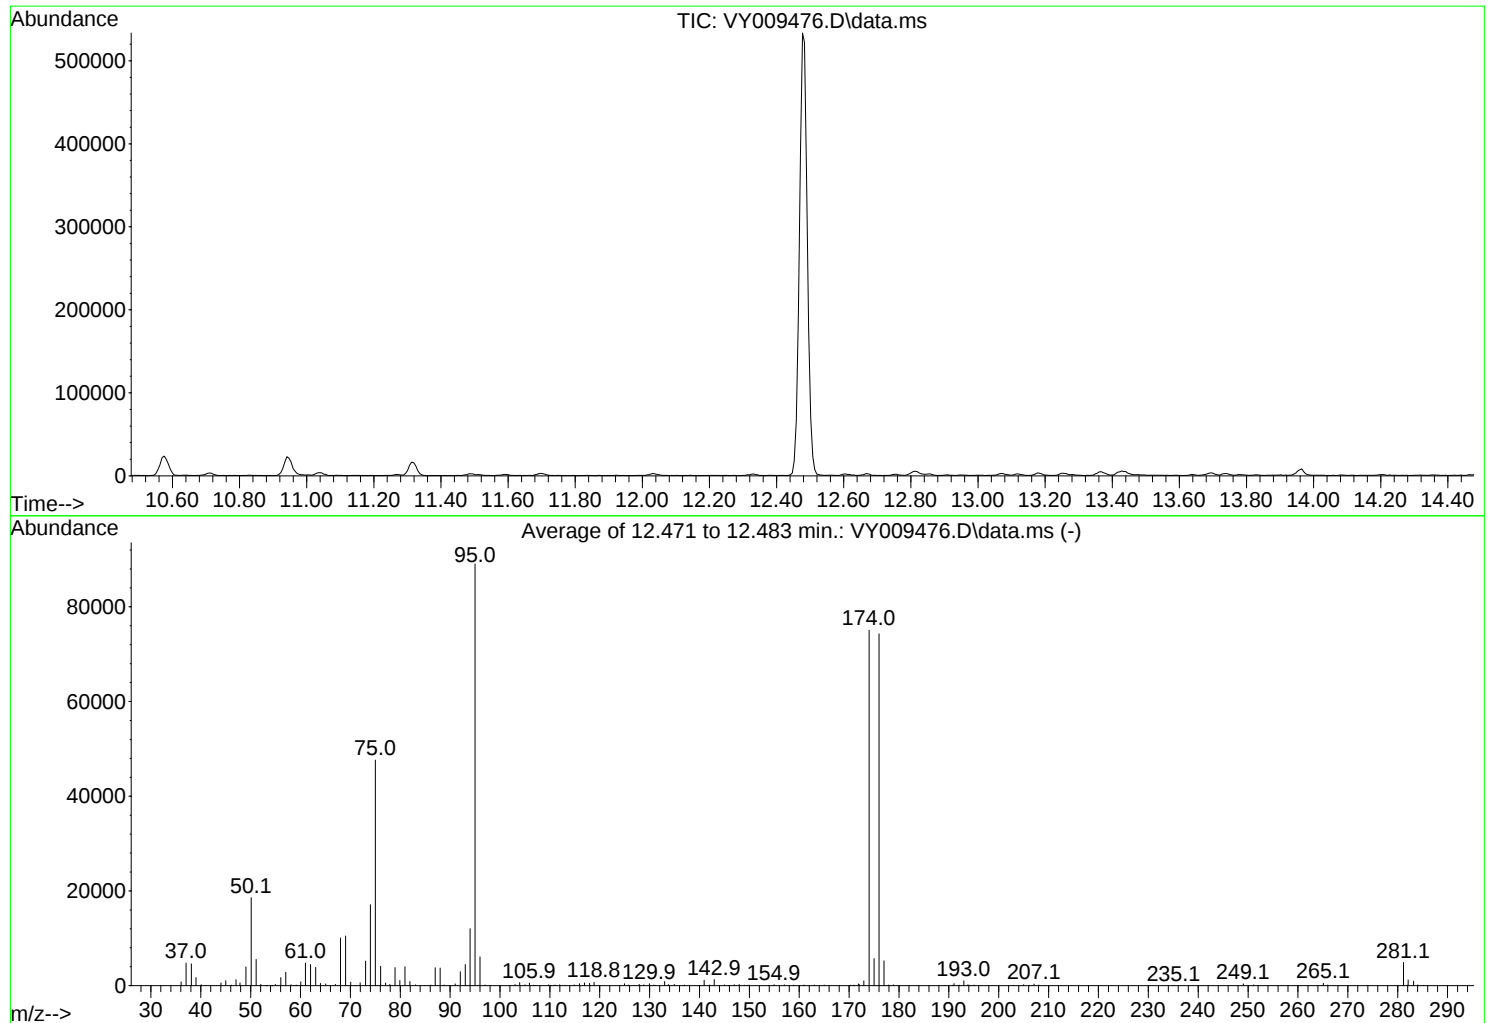

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	18579	PASS
75	95	30	60	53.5	47648	PASS
95	95	100	100	100.0	89080	PASS
96	95	5	9	6.8	6076	PASS
173	174	0.00	2	1.3	1007	PASS
174	95	50	100	84.3	75059	PASS
175	174	5	9	7.6	5705	PASS
176	174	95	101	99.0	74301	PASS
177	176	5	9	7.0	5228	PASS