
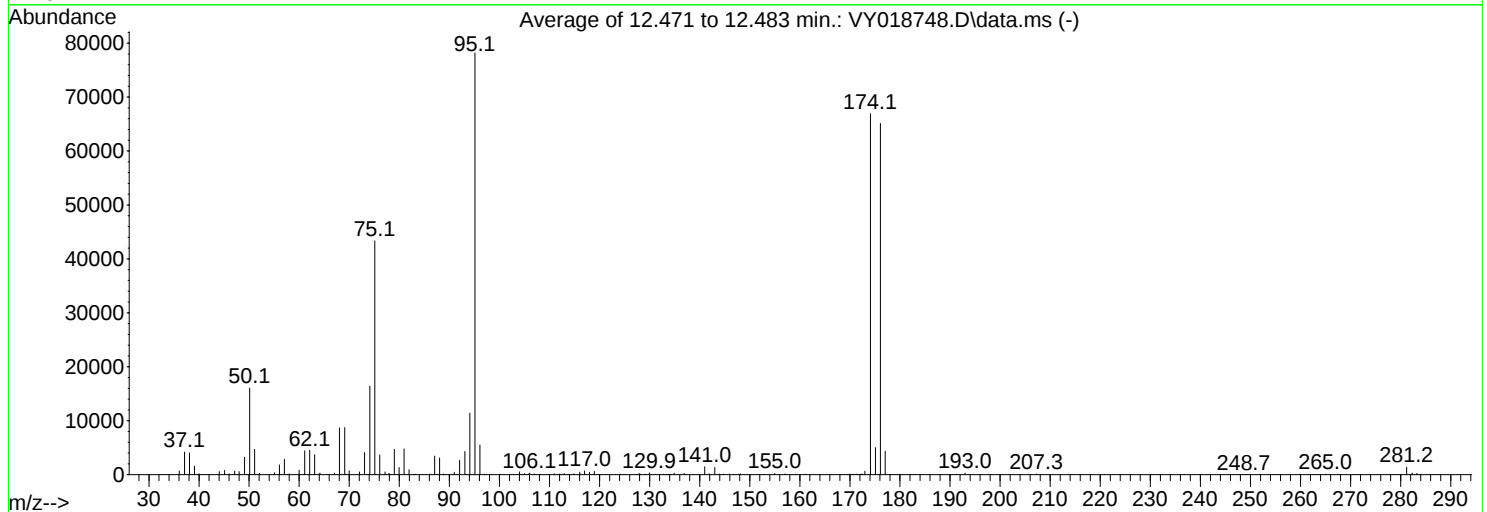


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY070924\
Data File : VY018748.D
Acq On : 09 Jul 2024 09:31
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Title : SW846 8260
Last Update : Tue Jul 09 14:28:51 2024

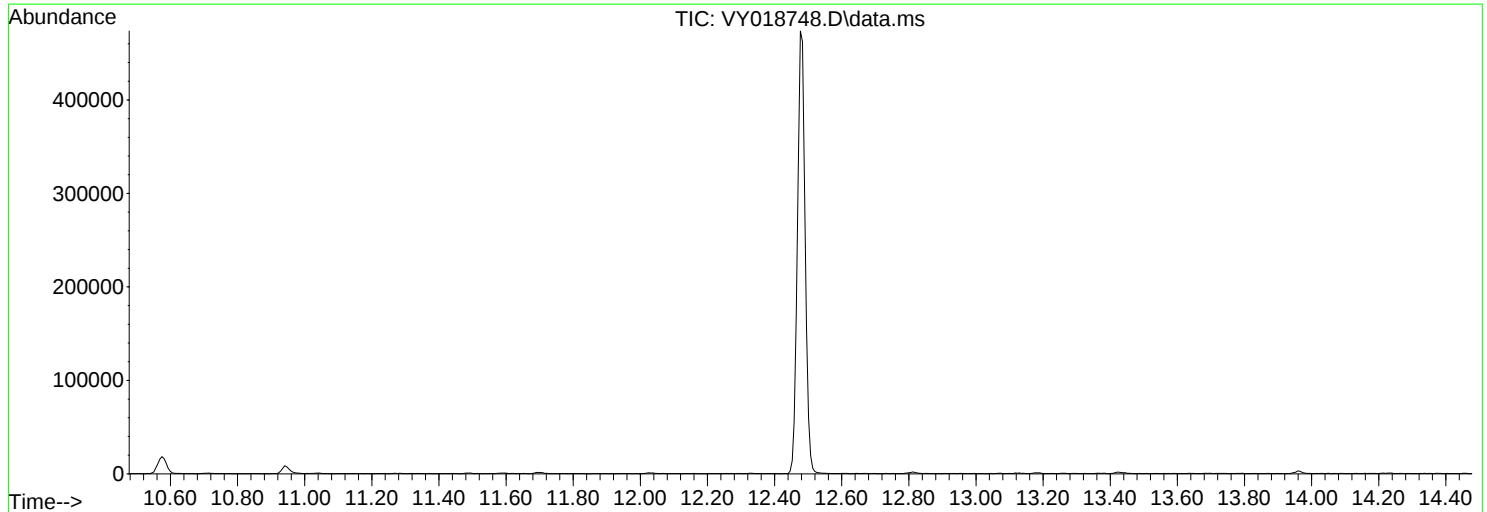

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	16063	PASS
75	95	30	60	55.4	43341	PASS
95	95	100	100	100.0	78205	PASS
96	95	5	9	7.0	5488	PASS
173	174	0.00	2	1.0	661	PASS
174	95	50	100	85.6	66939	PASS
175	174	5	9	7.5	5005	PASS
176	174	95	101	97.3	65109	PASS
177	176	5	9	6.7	4353	PASS