

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071224\
 Data File : VY018800.D
 Acq On : 12 Jul 2024 16:16
 Operator : SY/MD
 Sample : P3211-01
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Jul 12 23:41:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 09 14:28:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.777	168	6518	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	9462	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	6666	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.416	152	1565	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	2632	41.036	ug/l	0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	82.080%
35) Dibromofluoromethane	7.710	113	3346	56.461	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	112.920%
50) Toluene-d8	10.179	98	10426	46.437	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	92.880%
62) 4-Bromofluorobenzene	12.477	95	1983	25.862	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	51.720%
Target Compounds						
					Qvalue	
3) Chloromethane	2.113	50	204	2.458	ug/l #	43
5) Bromomethane	2.656	94	129	1.932	ug/l #	79
20) Methylene Chloride	4.692	84	331	Below Cal	#	32
36) 1,1-Dichloropropene	7.777	75	460	5.625	ug/l #	40
38) Carbon Tetrachloride	7.783	117	695	7.056	ug/l #	13
76) 1,2,3-Trichloropropane	12.483	75	1012	82.562	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.483	75	1012	184.780	ug/l #	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071224\
Data File : VY018800.D
Acq On : 12 Jul 2024 16:16
Operator : SY/MD
Sample : P3211-01
Misc : 5.07g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Jul 12 23:41:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 09 14:28:51 2024
Response via : Initial Calibration




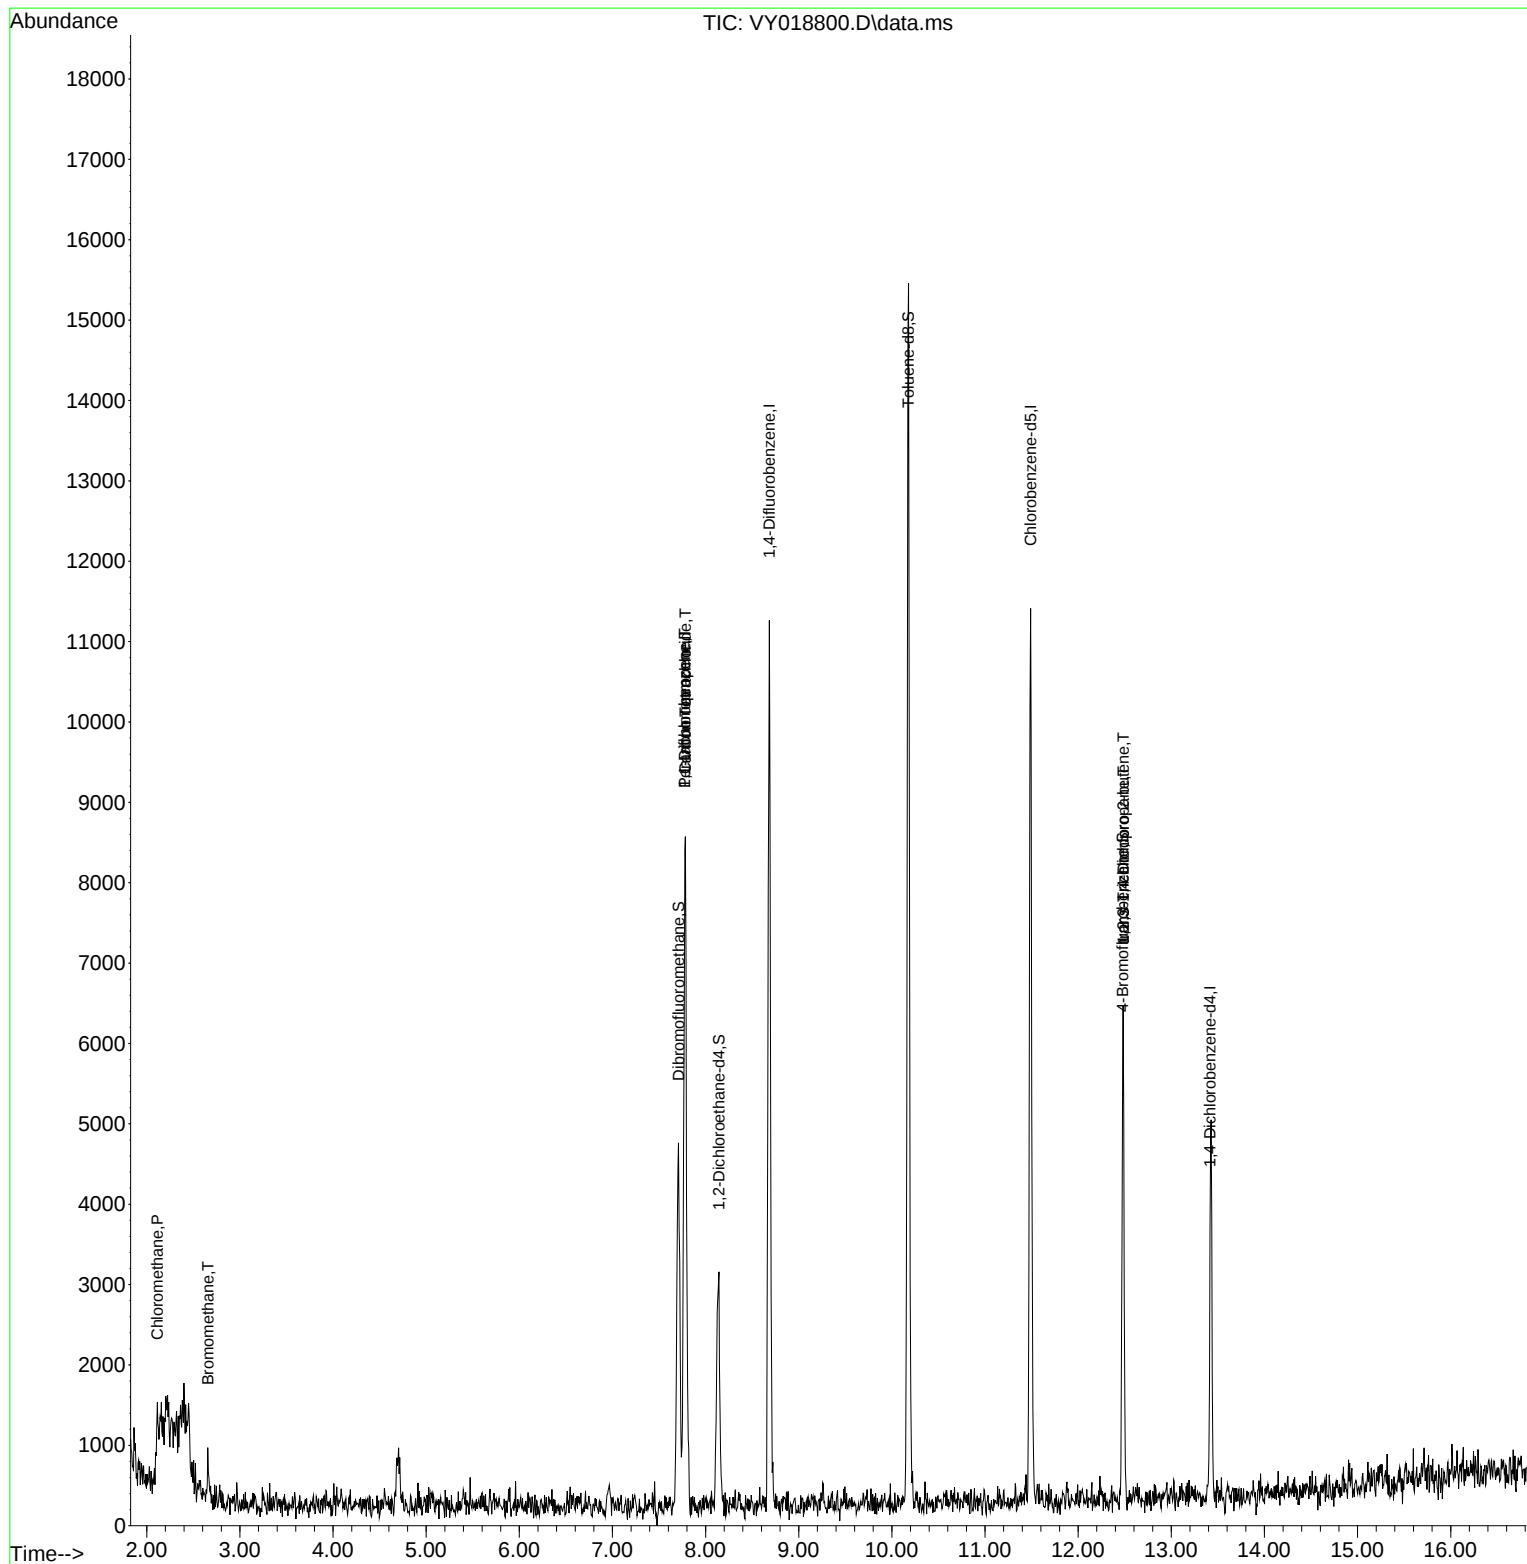


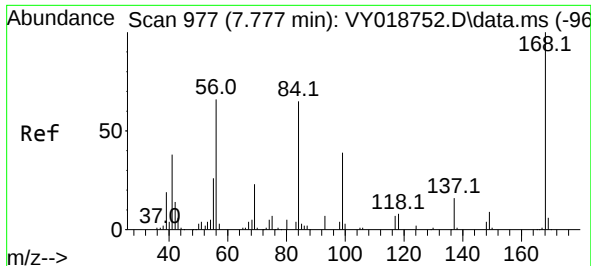

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 6518
Ion Ratio Lower Upper
168 100
99 50.7 39.1 58.7

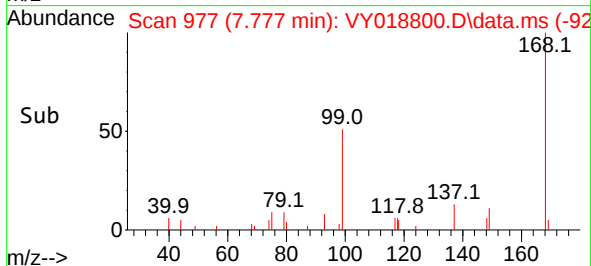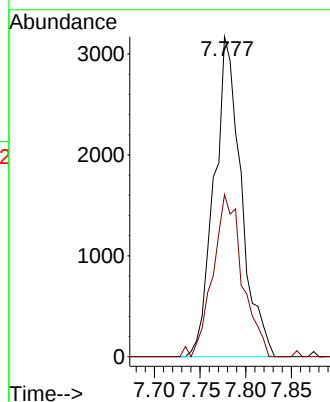

#3
Chloromethane
Concen: 2.458 ug/l
RT: 2.113 min Scan# 48
Delta R.T. 0.012 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Tgt Ion: 50 Resp: 204
Ion Ratio Lower Upper
50 100
52 0.0 25.6 38.4#


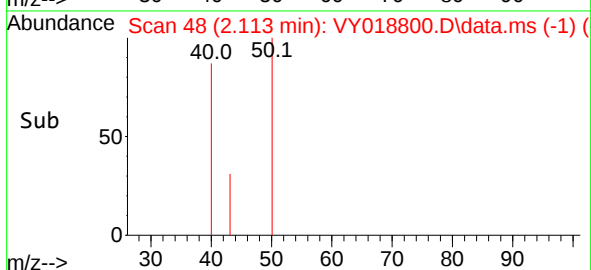
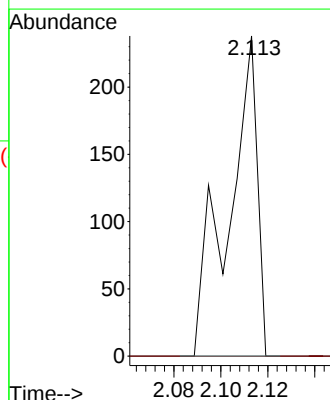
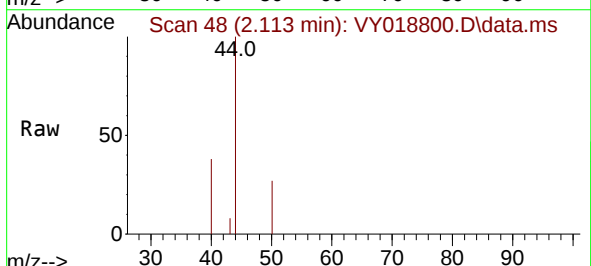


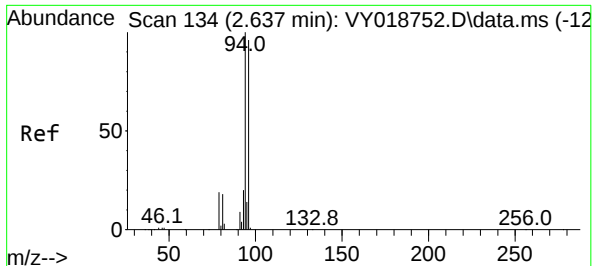

#5
Bromomethane
Concen: 1.932 ug/l
RT: 2.656 min Scan# 11
Delta R.T. 0.018 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 94 Resp: 129
Ion Ratio Lower Upper
94 100
96 112.6 74.1 111.1#

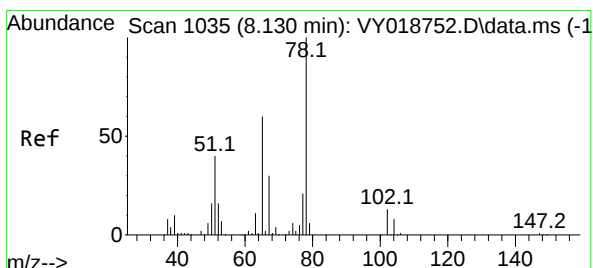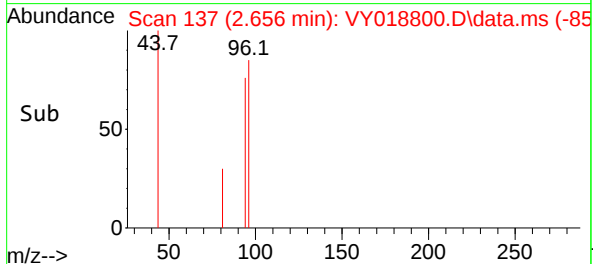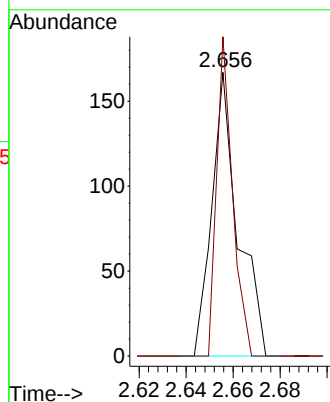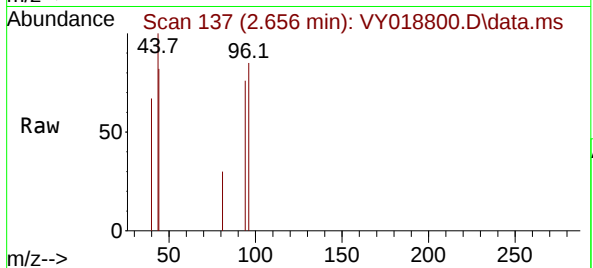

#33
1,2-Dichloroethane-d4
Concen: 41.036 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.012 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Tgt Ion: 65 Resp: 2632
Ion Ratio Lower Upper
65 100
67 61.6 0.0 109.6

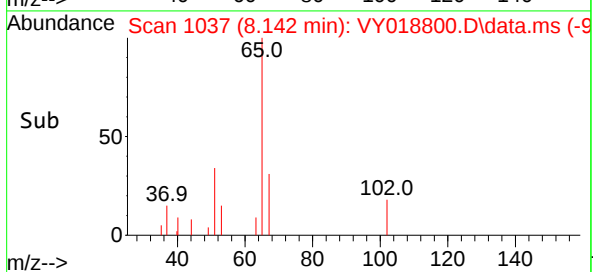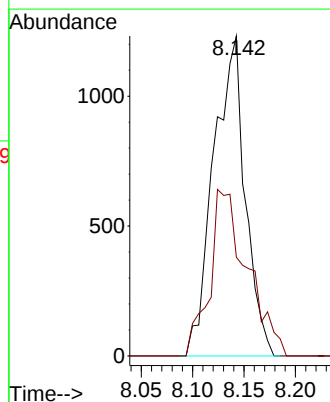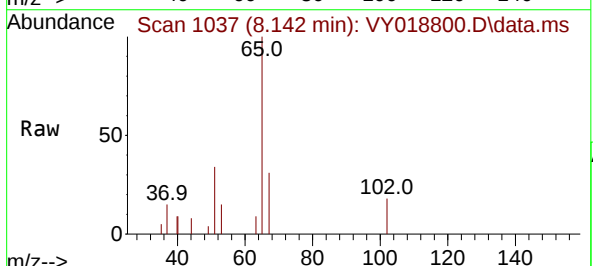

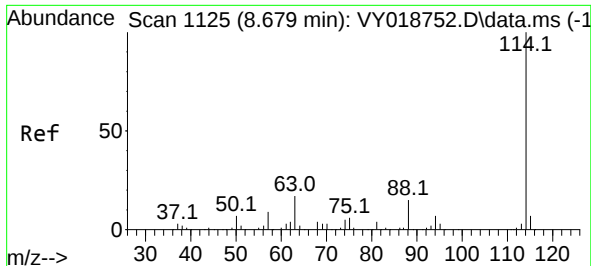

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VY018800.D

Acq: 12 Jul 2024 16:16

Instrument :

MSVOA_Y

ClientSampleId :





Tgt Ion:114 Resp: 9462

Ion Ratio Lower Upper

114 100

63 17.7 0.0 35.0

88 16.0 0.0 27.2

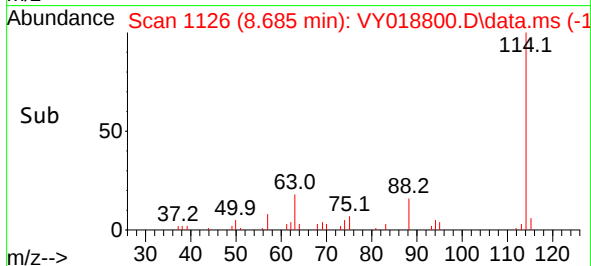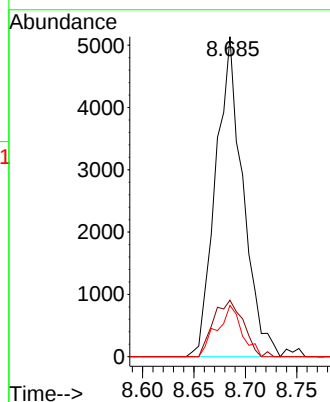

#35

Dibromofluoromethane

Concen: 56.461 ug/l

RT: 7.710 min Scan# 966

Delta R.T. 0.006 min

Lab File: VY018800.D

Acq: 12 Jul 2024 16:16




Tgt Ion:113 Resp: 3346


Ion Ratio Lower Upper

113 100

111 96.3 82.2 123.4


192 23.9 15.9 23.9

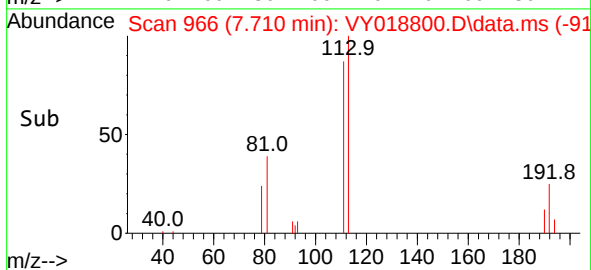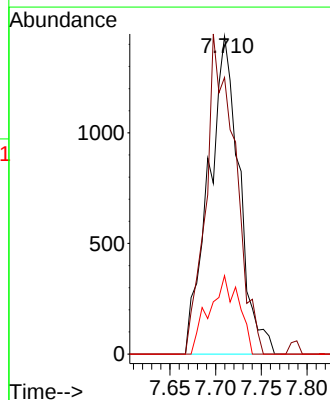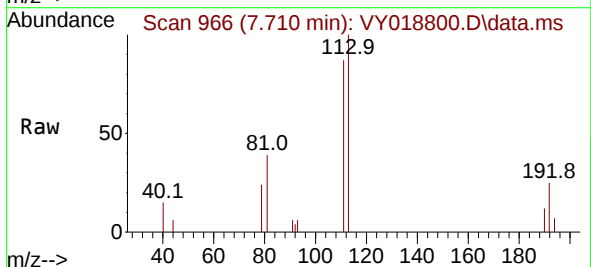



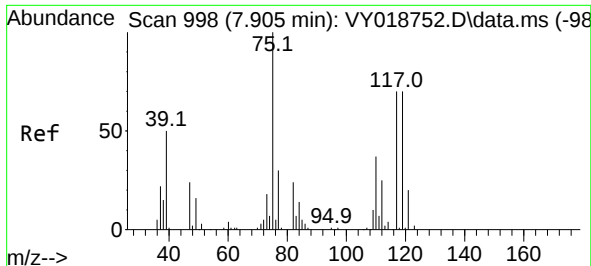


#36
1,1-Dichloropropene
Concen: 5.625 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.128 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Instrument :
MSVOA_Y
ClientSampleId :



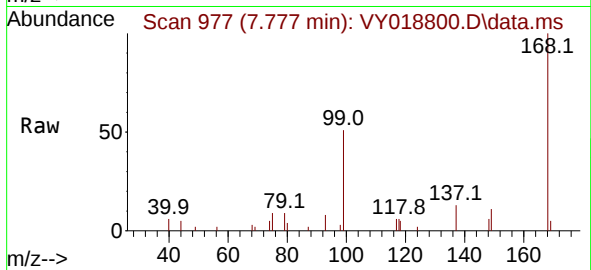



Tgt Ion: 75 Resp: 460
Ion Ratio Lower Upper
75 100
110 0.0 19.0 57.0#
77 0.0 25.3 37.9#

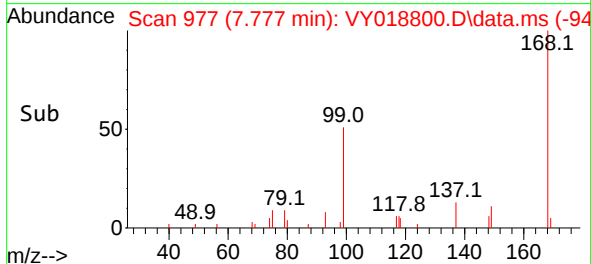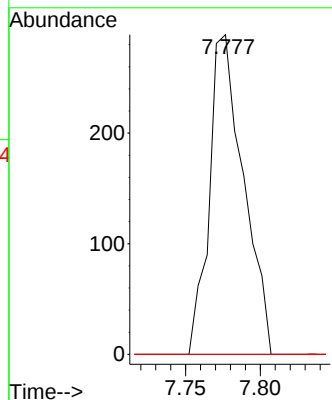

#38
Carbon Tetrachloride
Concen: 7.056 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.104 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Tgt Ion: 117 Resp: 695
Ion Ratio Lower Upper
117 100
119 0.0 75.8 113.6#
121 0.0 24.0 36.0#

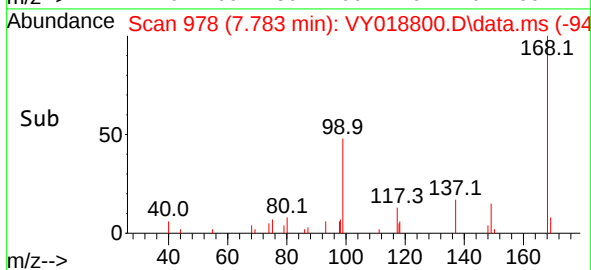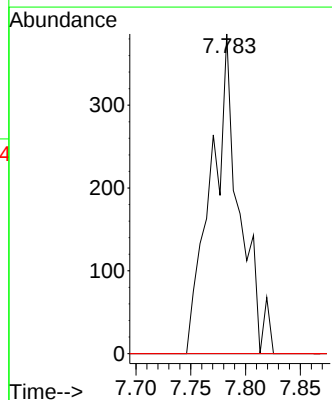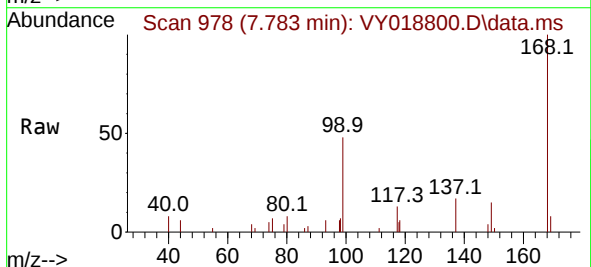



#50

Toluene-d8

Concen: 46.437 ug/l

RT: 10.179 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY018800.D

Acq: 12 Jul 2024 16:16

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 98 Resp: 10426

Ion Ratio Lower Upper

98 100

100 60.9 52.0 78.0

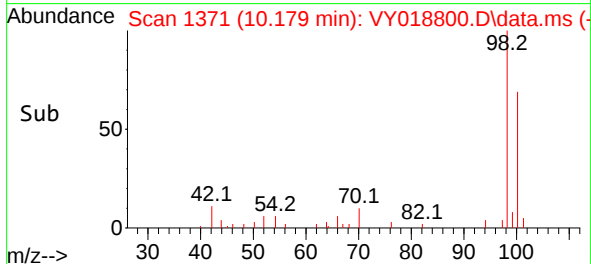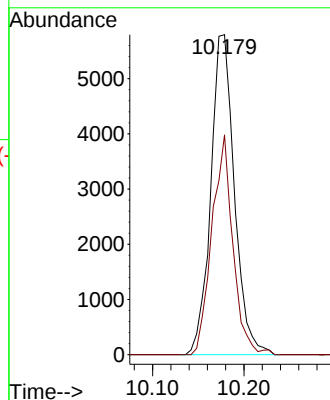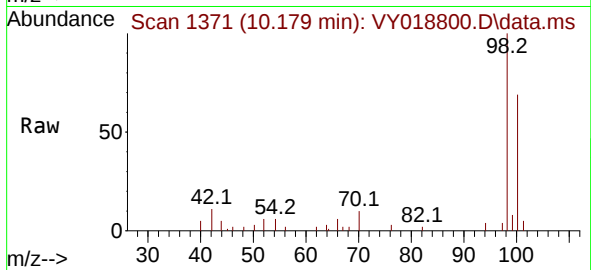

#62

4-Bromofluorobenzene

Concen: 25.862 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.000 min

Lab File: VY018800.D

Acq: 12 Jul 2024 16:16




Tgt Ion: 95 Resp: 1983


Ion Ratio Lower Upper

95 100

174 96.1 0.0 175.6


176 81.7 0.0 171.4

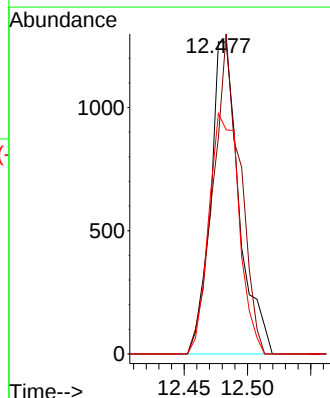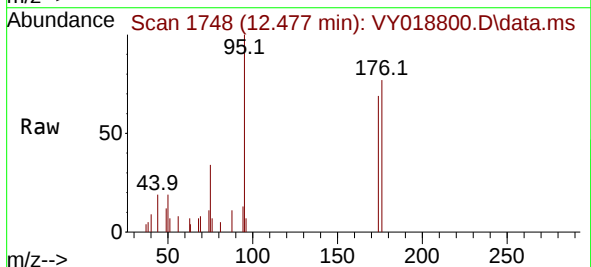






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Instrument :
MSVOA_Y
ClientSampleId :



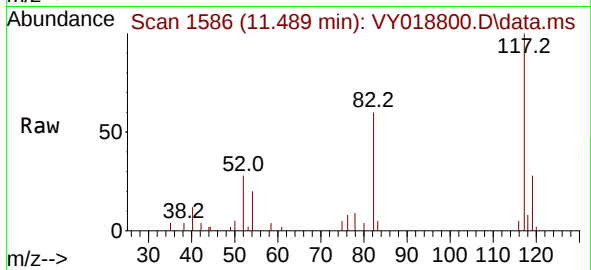



Tgt Ion:117 Resp: 6666
Ion Ratio Lower Upper
117 100
82 60.0 42.4 63.6
119 27.8 25.9 38.9

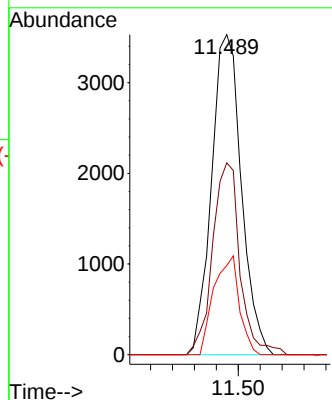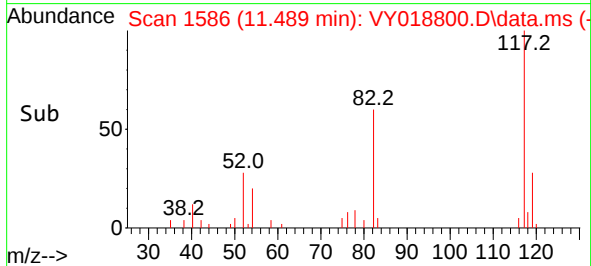

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.416 min Scan# 1902
Delta R.T. -0.006 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Tgt Ion:152 Resp: 1565
Ion Ratio Lower Upper
152 100
115 53.4 28.2 84.7
150 156.2 0.0 345.6


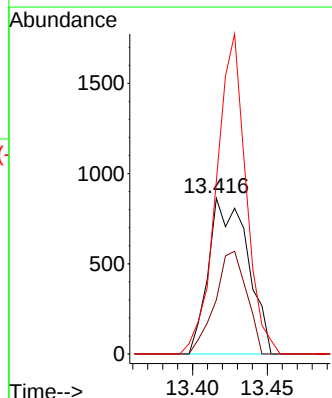
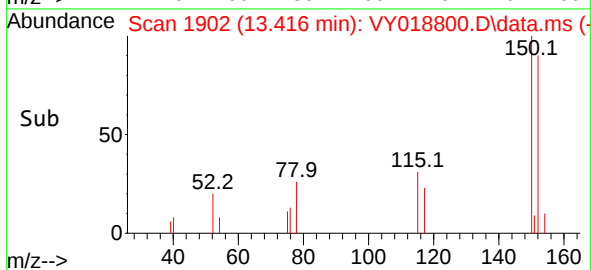
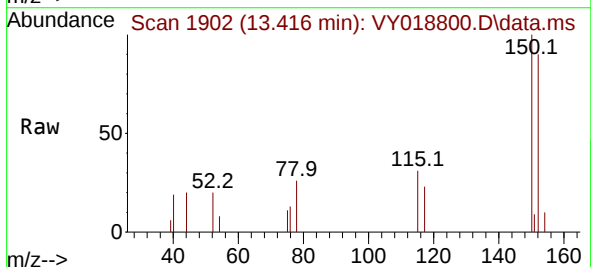


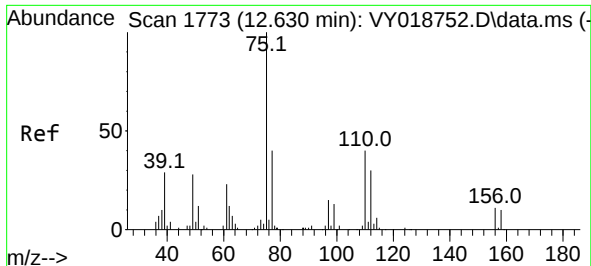

#76
1,2,3-Trichloropropane
Concen: 82.562 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.147 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Instrument :
MSVOA_Y
ClientSampleId :

Tgt Ion: 75 Resp: 1012
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0

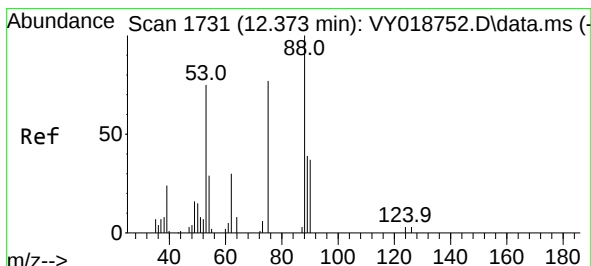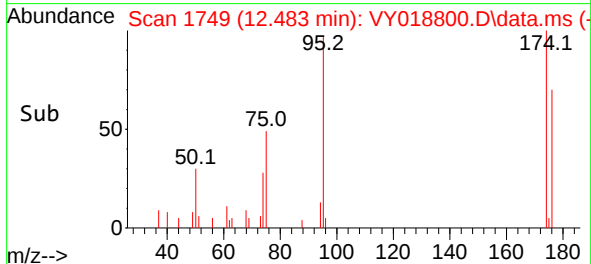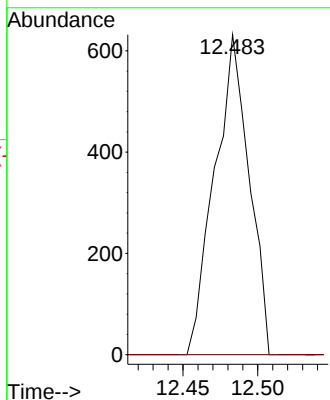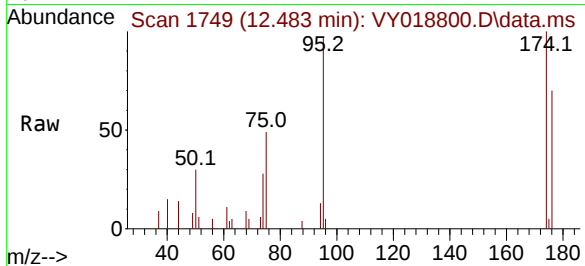

#81
trans-1,4-Dichloro-2-butene
Concen: 184.780 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.110 min
Lab File: VY018800.D
Acq: 12 Jul 2024 16:16

Tgt Ion: 75 Resp: 1012
Ion Ratio Lower Upper
75 100
53 0.0 66.8 100.2#
89 0.0 35.8 53.6#

