

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071825\
 Data File : VY023005.D
 Acq On : 18 Jul 2025 18:10
 Operator : SY/MD
 Sample : Q2638-09
 Misc : 4.73g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-TS-35-071725

Quant Time: Jul 19 02:14:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 19 01:50:49 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	238624	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	432683	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	412416	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	187775	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	160359	66.383	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	132.760%
35) Dibromofluoromethane	7.634	113	141908	51.703	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.400%
50) Toluene-d8	10.103	98	515996	47.407	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	94.820%
62) 4-Bromofluorobenzene	12.401	95	180693	52.738	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	105.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071825\
Data File : VY023005.D
Acq On : 18 Jul 2025 18:10
Operator : SY/MD
Sample : Q2638-09
Misc : 4.73g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-35-071725

Quant Time: Jul 19 02:14:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 19 01:50:49 2025
Response via : Initial Calibration




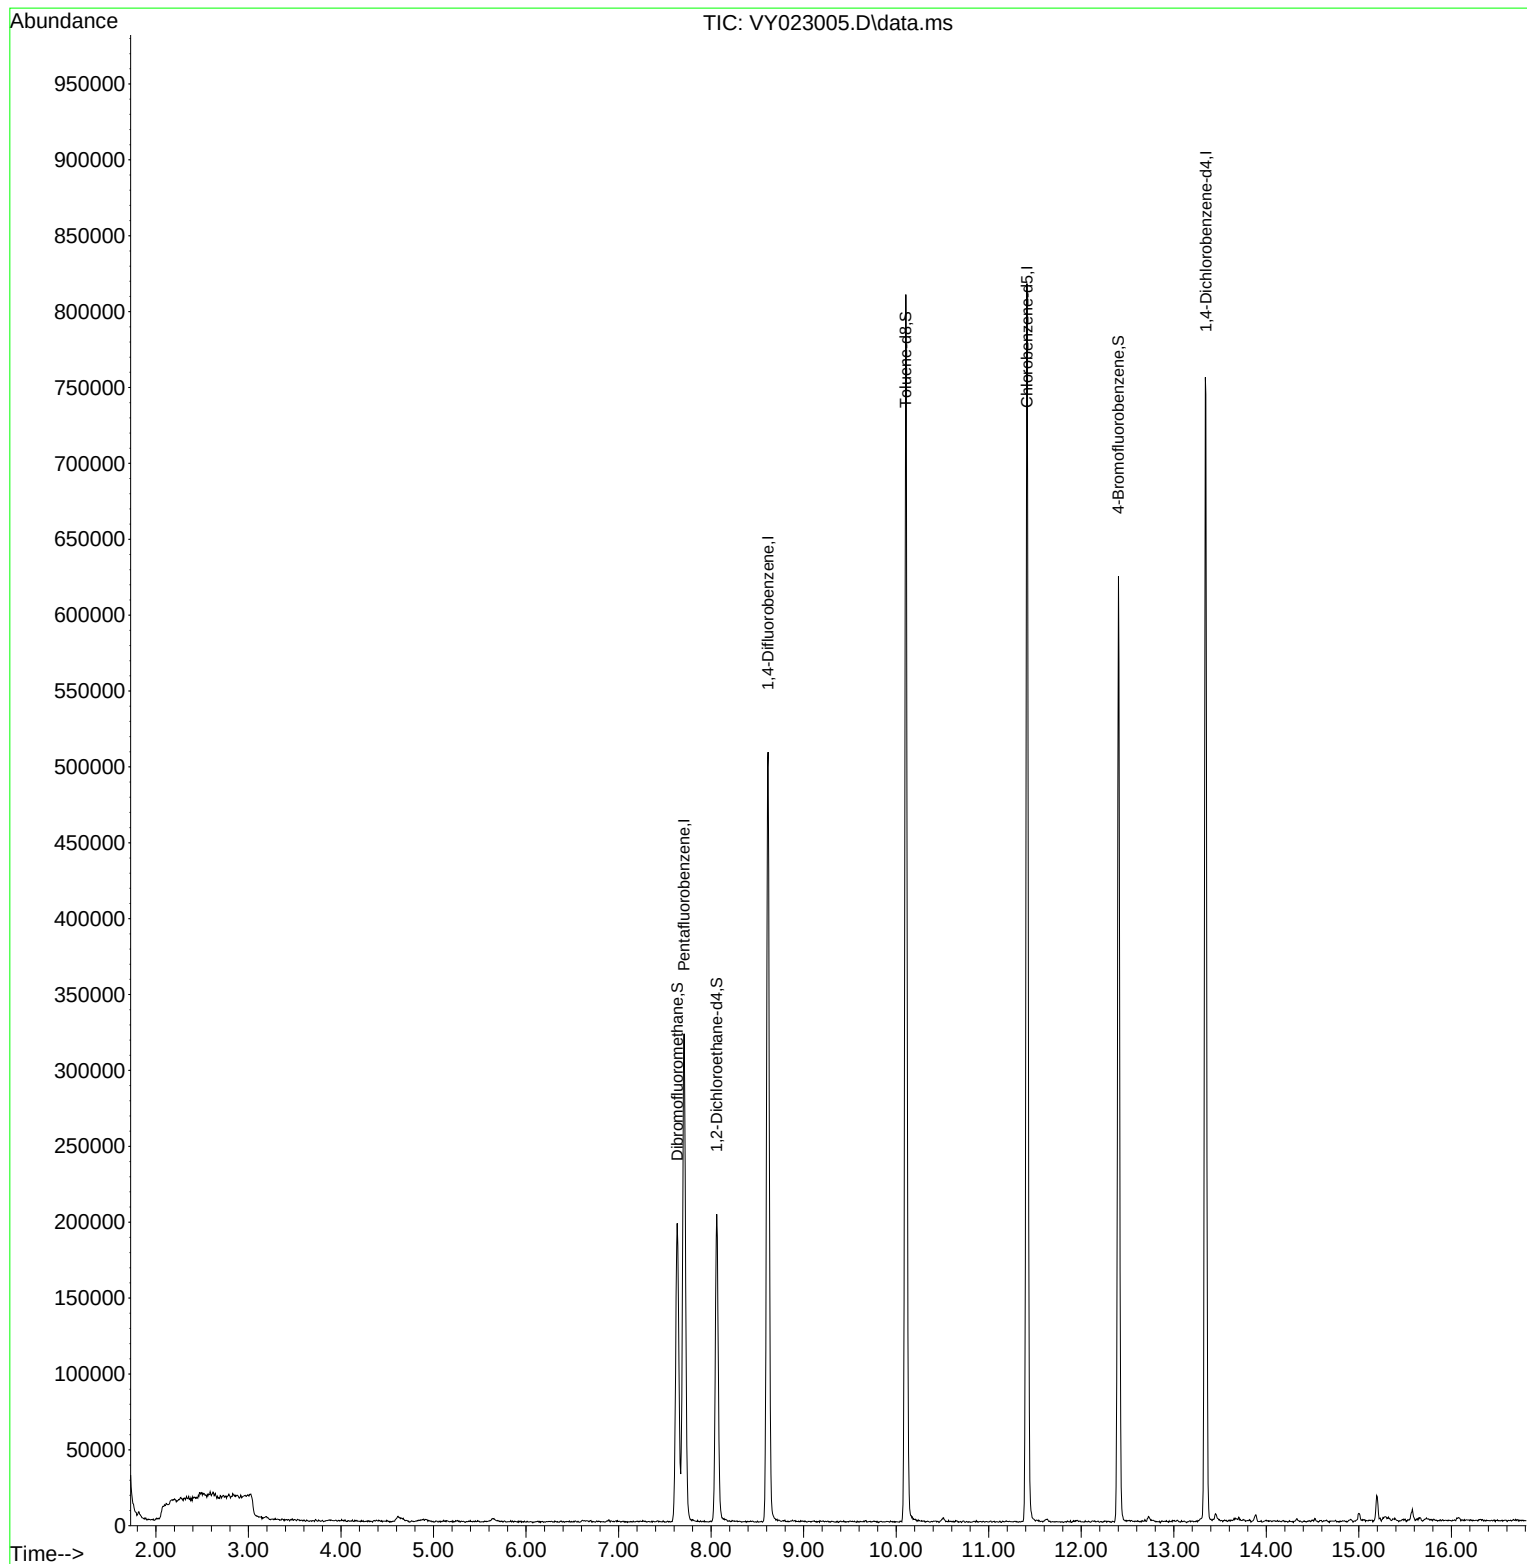


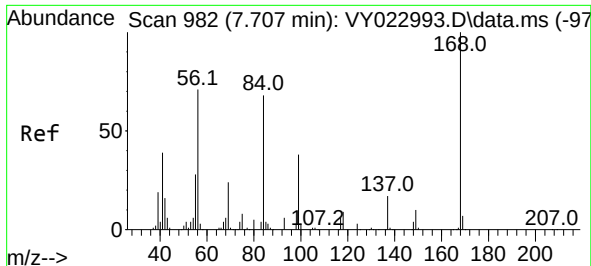

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023005.D
Acq: 18 Jul 2025 18:10




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-35-071725


Tgt Ion:168 Resp: 238624
Ion Ratio Lower Upper
168 100
99 59.4 44.4 66.6

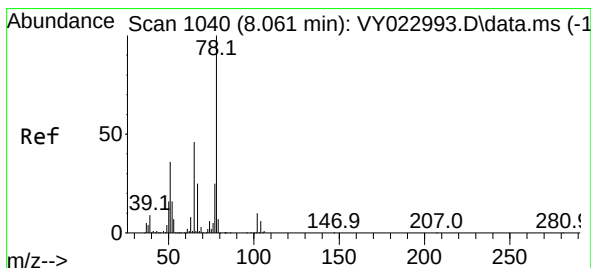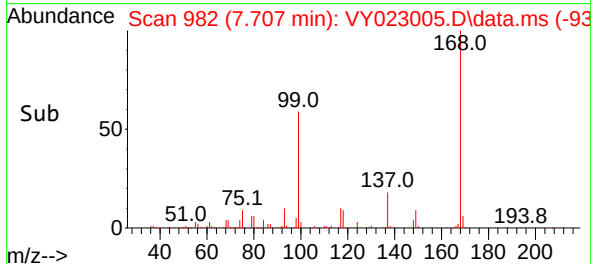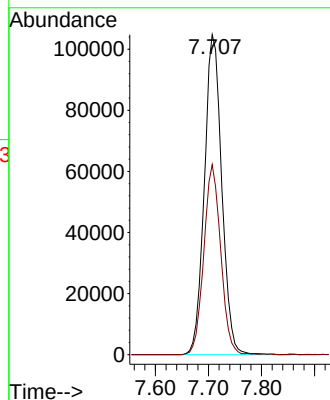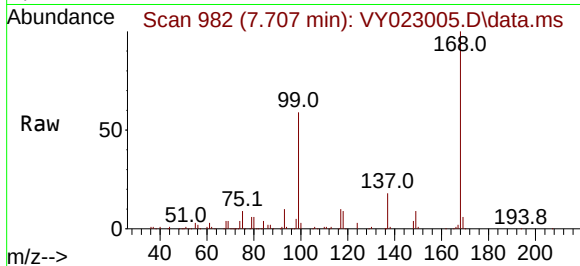

#33
1,2-Dichloroethane-d4
Concen: 66.383 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY023005.D
Acq: 18 Jul 2025 18:10

Tgt Ion: 65 Resp: 160359
Ion Ratio Lower Upper
65 100
67 52.6 0.0 107.4

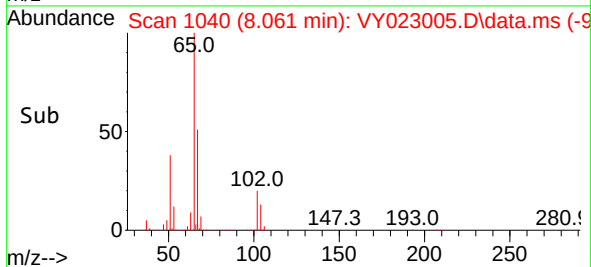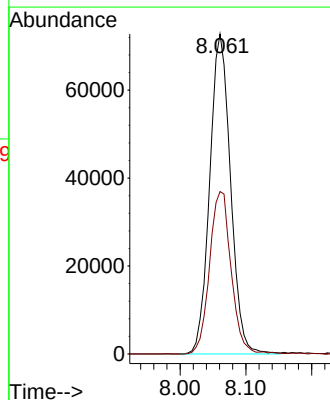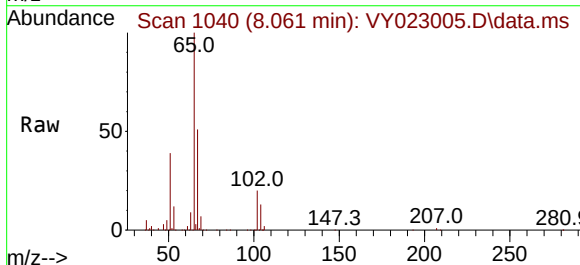

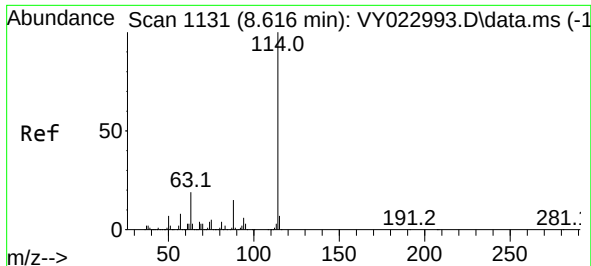

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VY023005.D

Acq: 18 Jul 2025 18:10

Instrument :

MSVOA_Y

ClientSampleId :

OU4-TS-35-071725





Tgt Ion:114 Resp: 432683

Ion Ratio Lower Upper

114 100

63 21.2 0.0 38.8

88 15.3 0.0 30.2

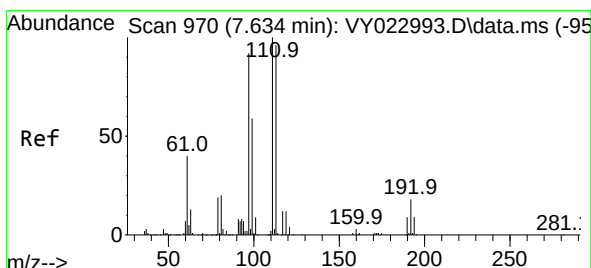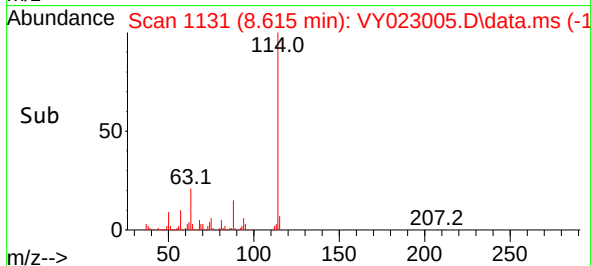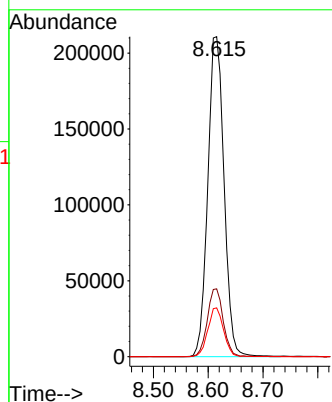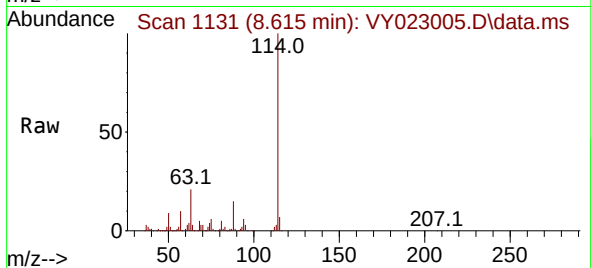

#35

Dibromofluoromethane

Concen: 51.703 ug/l

RT: 7.634 min Scan# 970

Delta R.T. -0.000 min

Lab File: VY023005.D

Acq: 18 Jul 2025 18:10




Tgt Ion:113 Resp: 141908


Ion Ratio Lower Upper

113 100

111 101.0 83.2 124.8

192 18.6 15.3 22.9


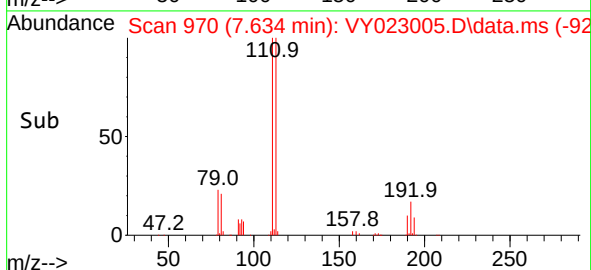
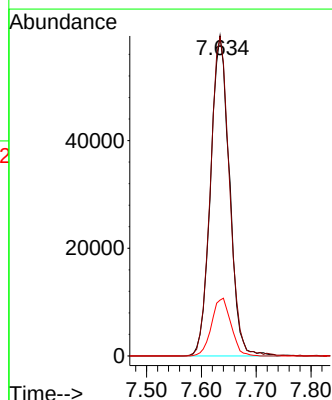
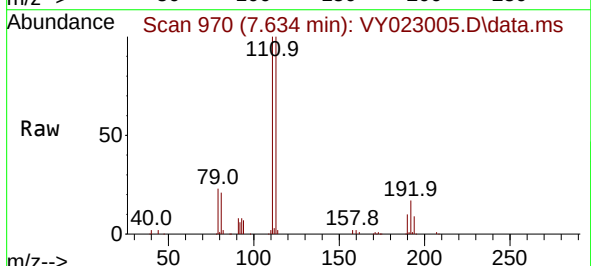


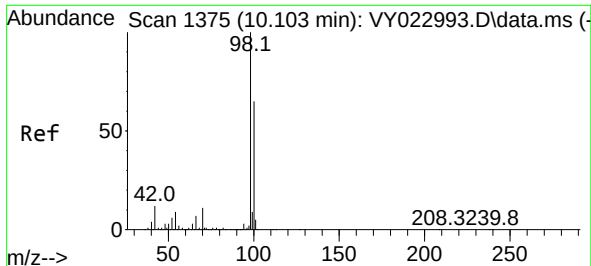

#50
Toluene-d8
Concen: 47.407 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY023005.D
Acq: 18 Jul 2025 18:10




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-35-071725


Tgt Ion: 98 Resp: 515996
Ion Ratio Lower Upper
98 100
100 63.8 52.2 78.2

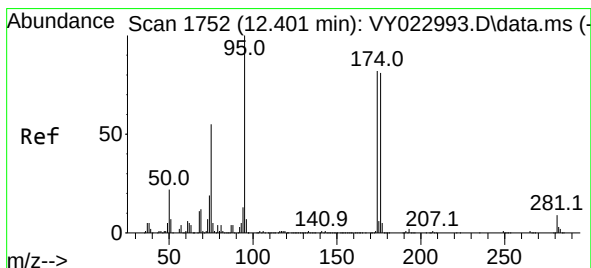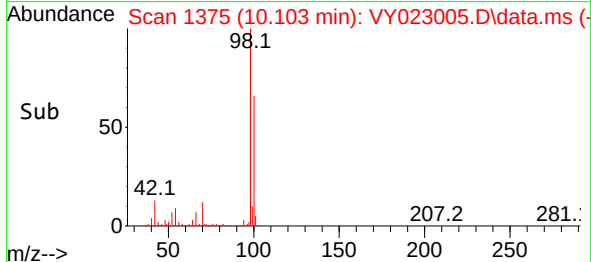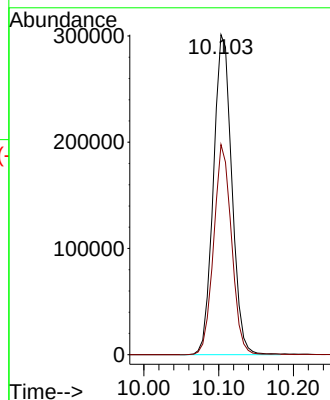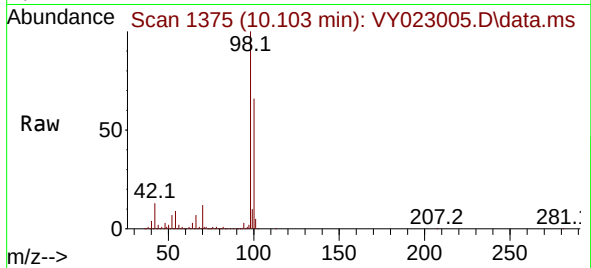

#62
4-Bromofluorobenzene
Concen: 52.738 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.000 min
Lab File: VY023005.D
Acq: 18 Jul 2025 18:10

Tgt Ion: 95 Resp: 180693
Ion Ratio Lower Upper
95 100
174 86.8 0.0 170.8
176 81.2 0.0 163.6

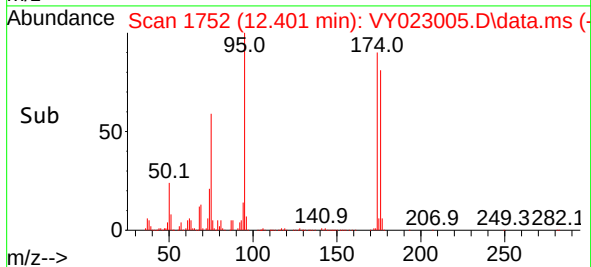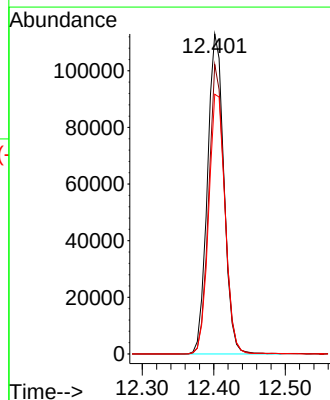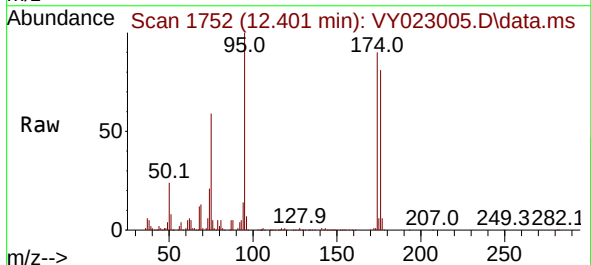

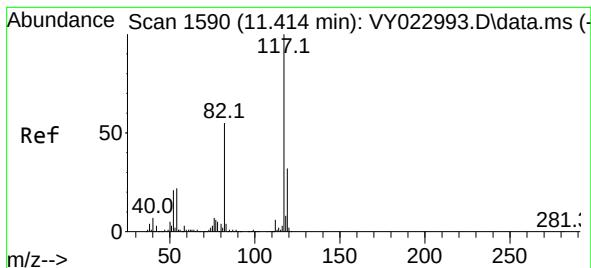

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.000 min

Lab File: VY023005.D

Acq: 18 Jul 2025 18:10

Instrument :

MSVOA_Y

ClientSampleId :

OU4-TS-35-071725





Tgt Ion:117 Resp: 412416

Ion Ratio Lower Upper

117 100

82 58.0 44.3 66.5

119 32.3 25.8 38.8

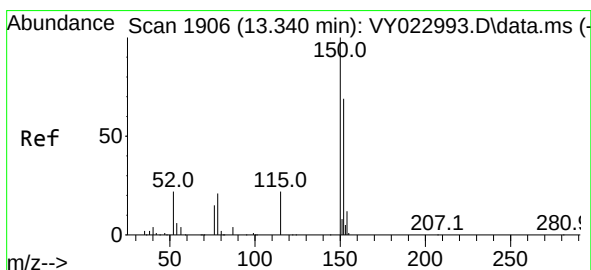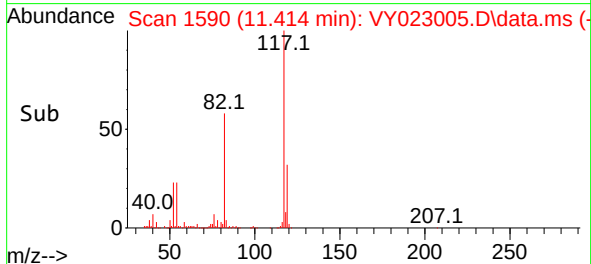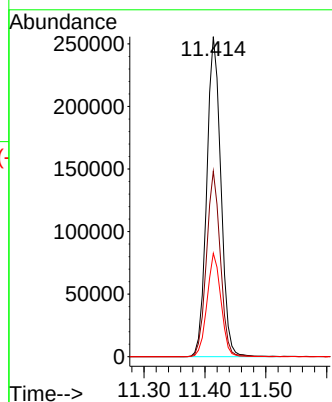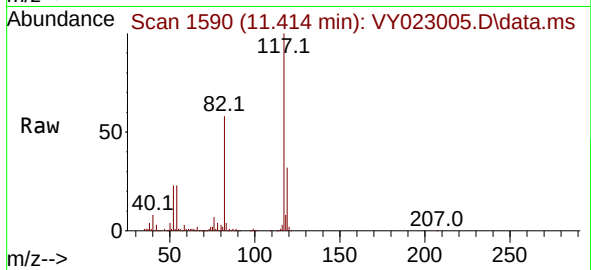

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023005.D

Acq: 18 Jul 2025 18:10

Tgt Ion:152 Resp: 187775

Ion Ratio Lower Upper

152 100

115 58.4 29.4 88.2

150 157.7 0.0 350.0

