

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071924\
 Data File : VY018883.D
 Acq On : 19 Jul 2024 15:41
 Operator : SY/MD
 Sample : P3302-01
 Misc : 4.99g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 285-290

Quant Time: Jul 19 23:05:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 09 14:28:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.777	168	12745	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	18106	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	12252	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	3807	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	4041	32.221	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	64.440%
35) Dibromofluoromethane	7.710	113	5206	45.908	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	91.820%
50) Toluene-d8	10.179	98	18292	42.576	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	85.160%
62) 4-Bromofluorobenzene	12.477	95	4146	28.258	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	56.520%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071924\
Data File : VY018883.D
Acq On : 19 Jul 2024 15:41
Operator : SY/MD
Sample : P3302-01
Misc : 4.99g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
285-290

Quant Time: Jul 19 23:05:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 09 14:28:51 2024
Response via : Initial Calibration




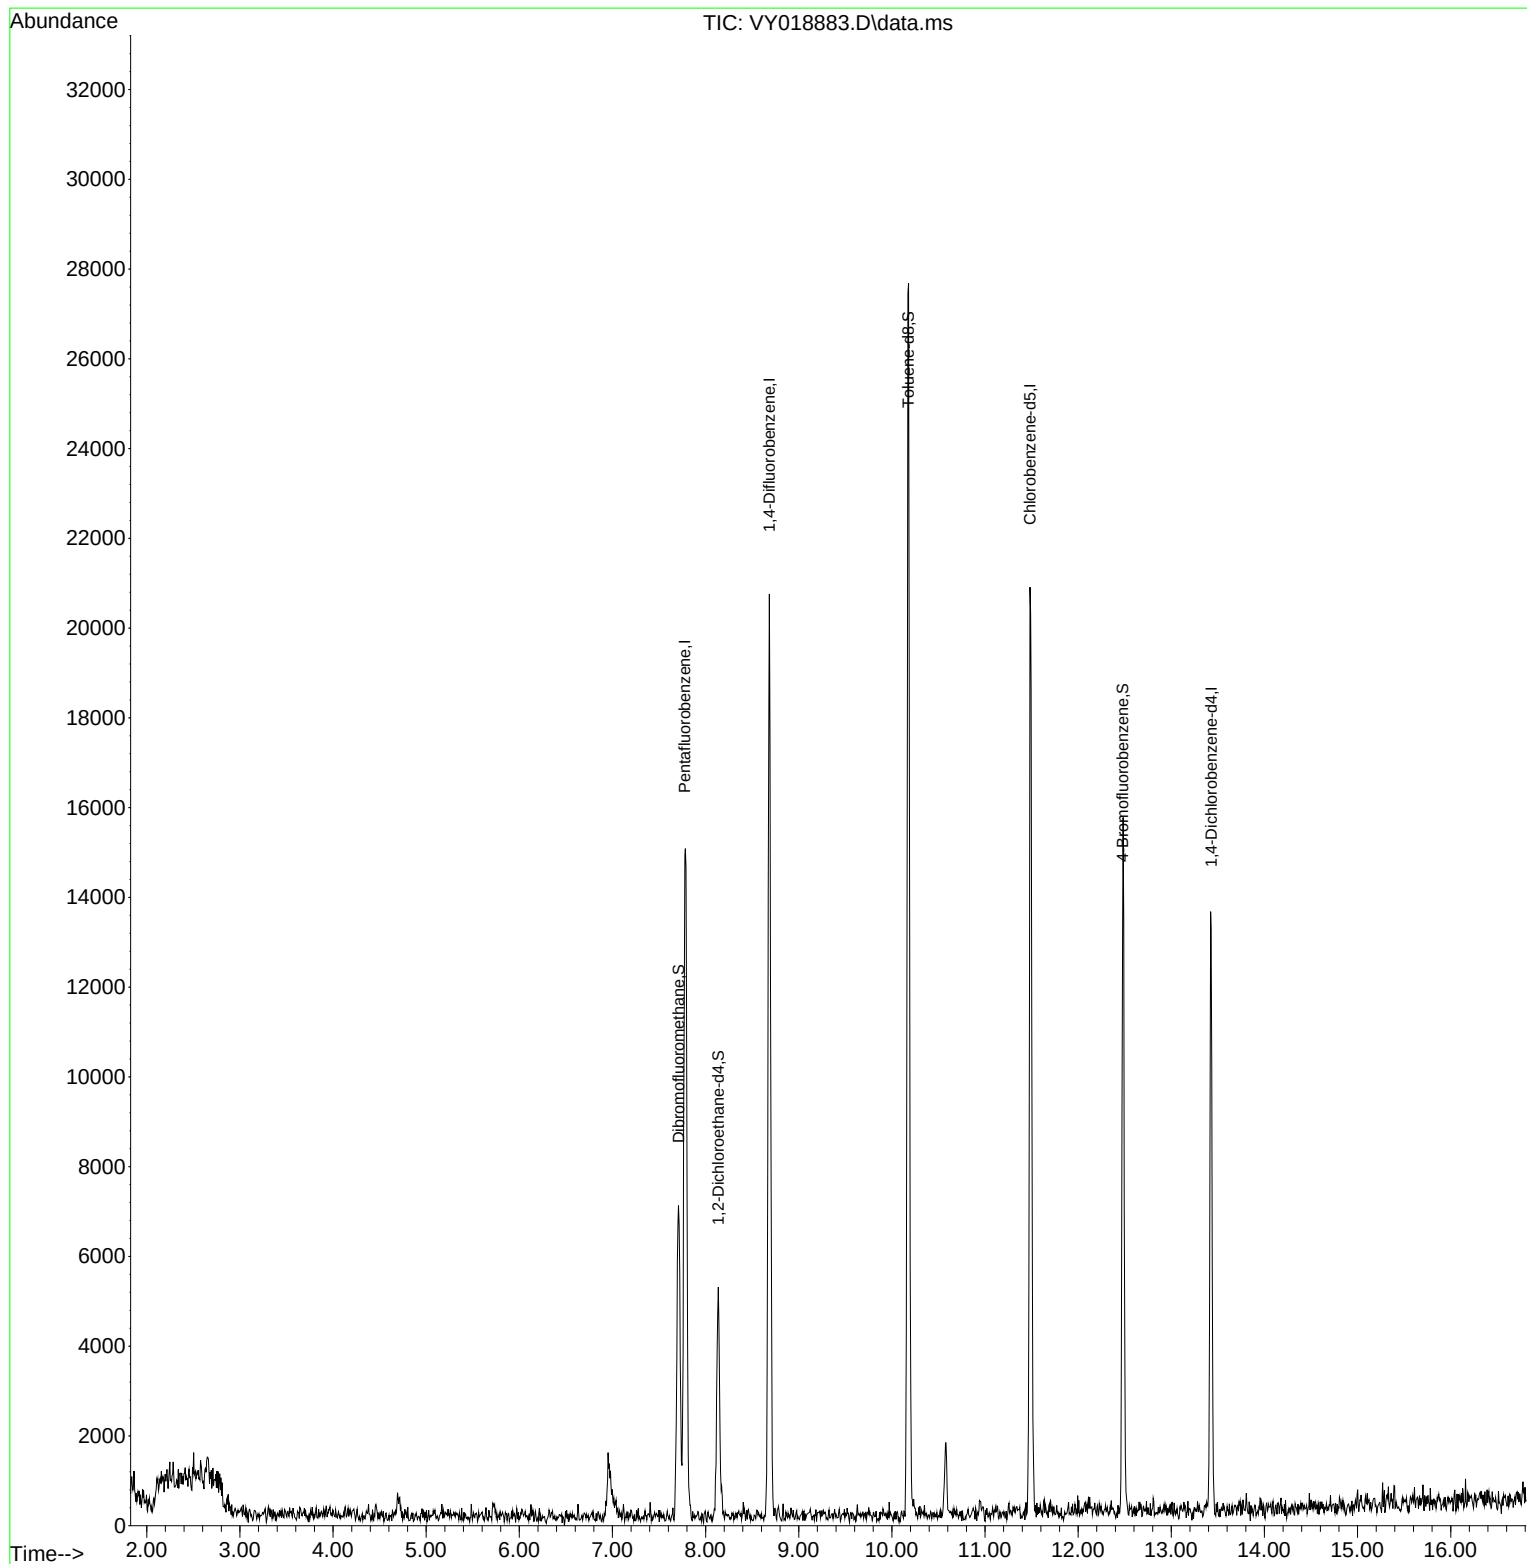


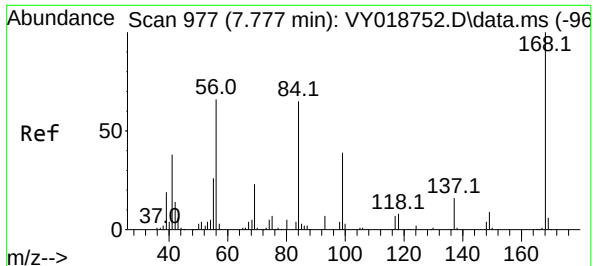

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY018883.D
Acq: 19 Jul 2024 15:41




Instrument :
MSVOA_Y
ClientSampleId :
285-290


Tgt Ion:168 Resp: 12745
Ion Ratio Lower Upper
168 100
99 50.6 39.1 58.7

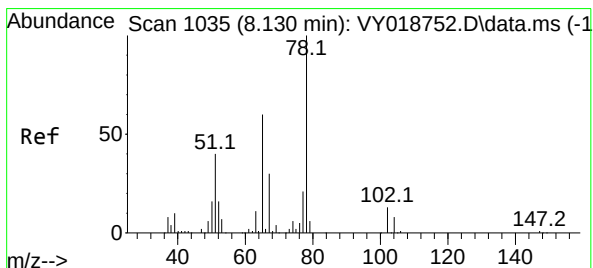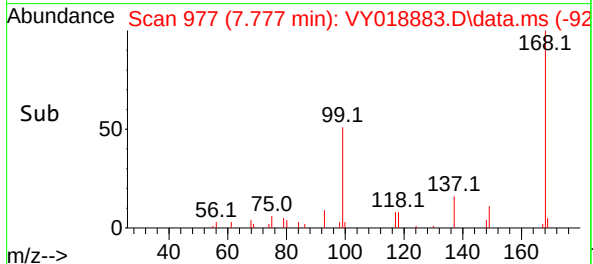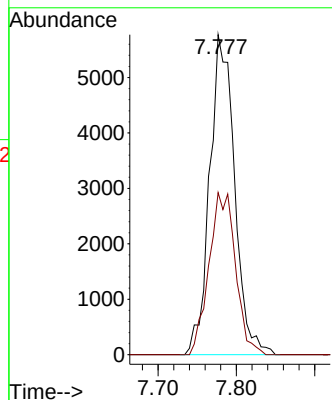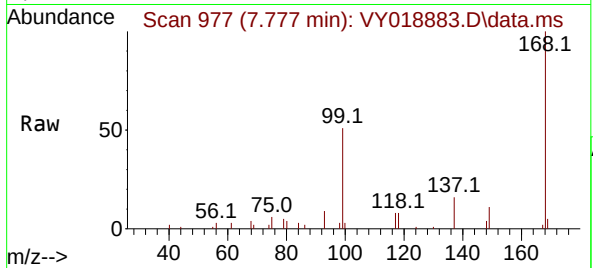

#33
1,2-Dichloroethane-d4
Concen: 32.221 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.006 min
Lab File: VY018883.D
Acq: 19 Jul 2024 15:41

Tgt Ion: 65 Resp: 4041
Ion Ratio Lower Upper
65 100
67 50.1 0.0 109.6

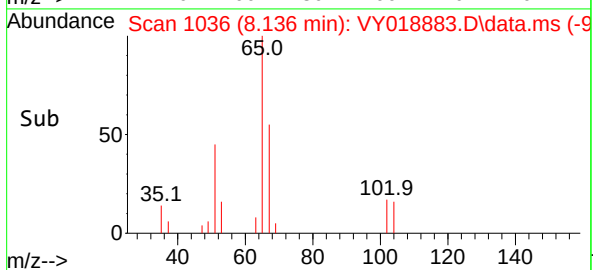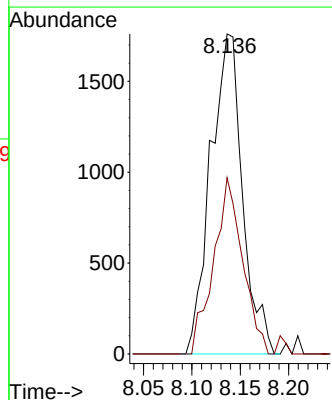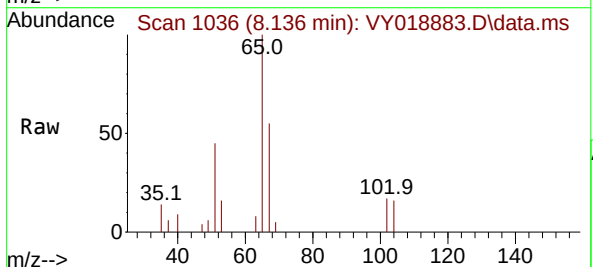

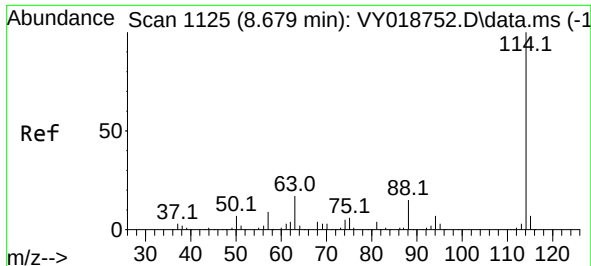

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1125

Delta R.T. 0.006 min

Lab File: VY018883.D

Acq: 19 Jul 2024 15:41

Instrument :

MSVOA_Y

ClientSampleId :

285-290





Tgt Ion:114 Resp: 18106

Ion Ratio Lower Upper

114 100

63 16.6 0.0 35.0

88 12.3 0.0 27.2

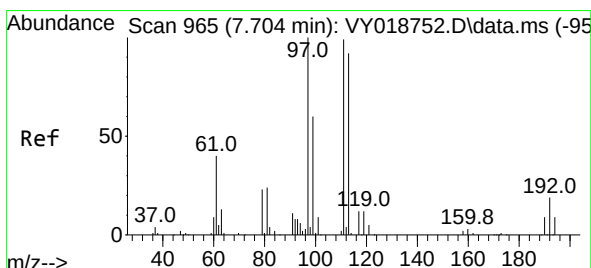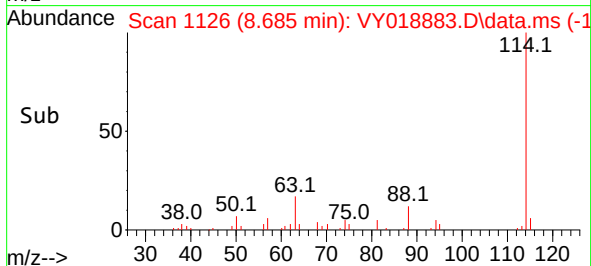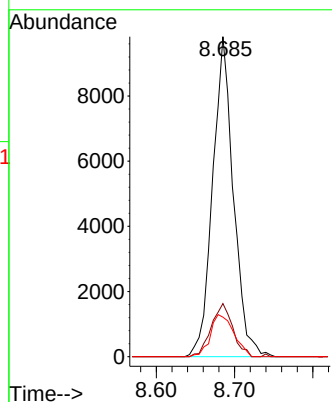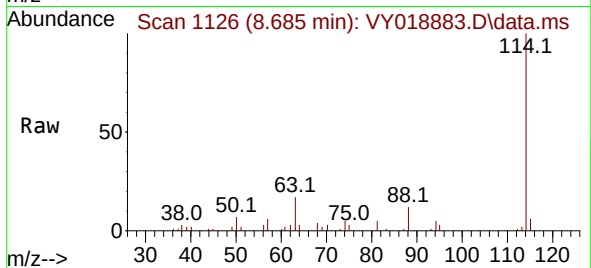

#35

Dibromofluoromethane

Concen: 45.908 ug/l

RT: 7.710 min Scan# 966

Delta R.T. 0.006 min

Lab File: VY018883.D

Acq: 19 Jul 2024 15:41




Tgt Ion:113 Resp: 5206


Ion Ratio Lower Upper

113 100

111 97.1 82.2 123.4

192 20.3 15.9 23.9

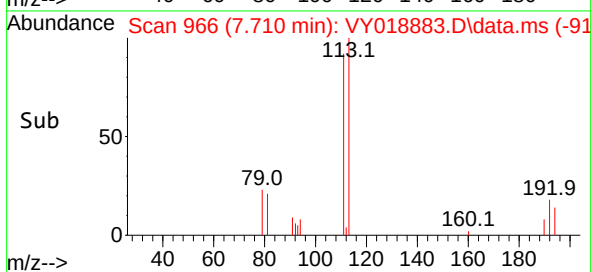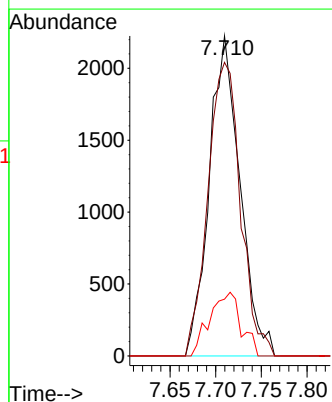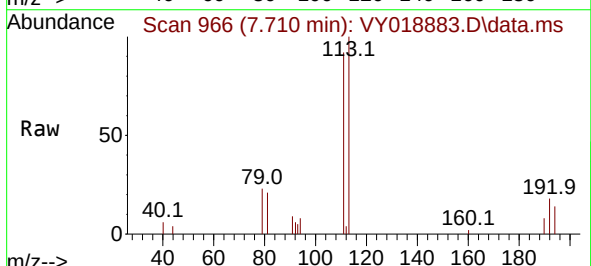

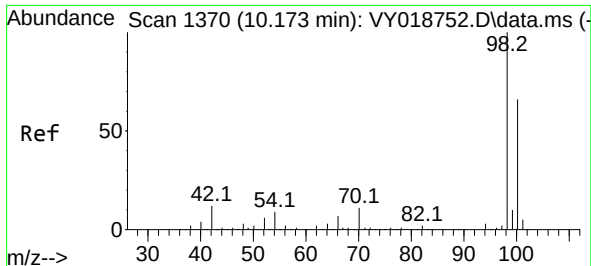

#50

Toluene-d8

Concen: 42.576 ug/l

RT: 10.179 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY018883.D

Acq: 19 Jul 2024 15:41

Instrument :

MSVOA_Y

ClientSampleId :





285-290

Tgt Ion: 98 Resp: 18292

Ion Ratio Lower Upper

98 100

100 66.6 52.0 78.0

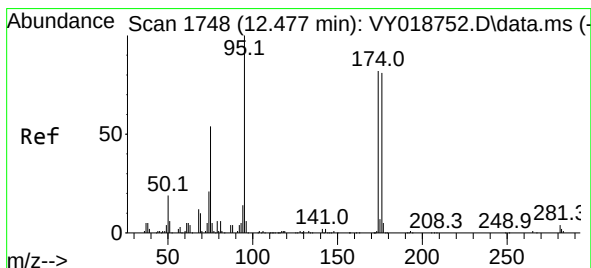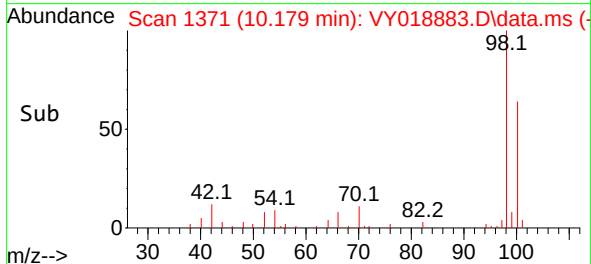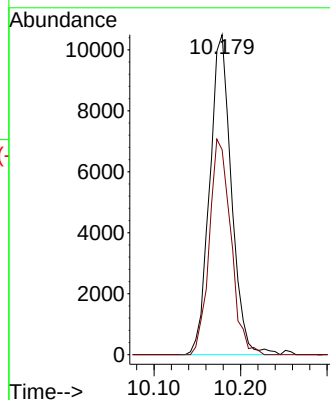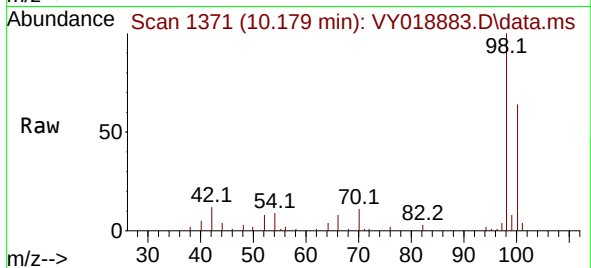

#62

4-Bromofluorobenzene

Concen: 28.258 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.000 min

Lab File: VY018883.D

Acq: 19 Jul 2024 15:41




Tgt Ion: 95 Resp: 4146


Ion Ratio Lower Upper

95 100

174 100.5 0.0 175.6

176 84.0 0.0 171.4


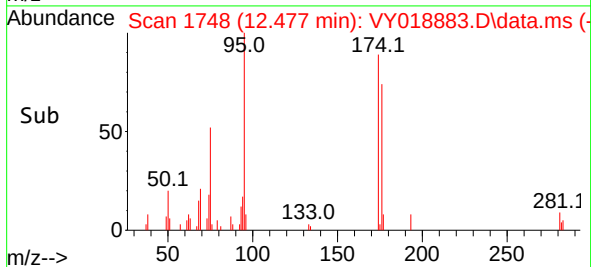
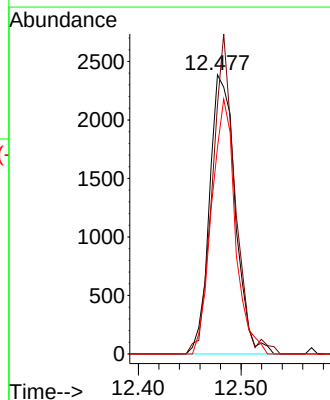
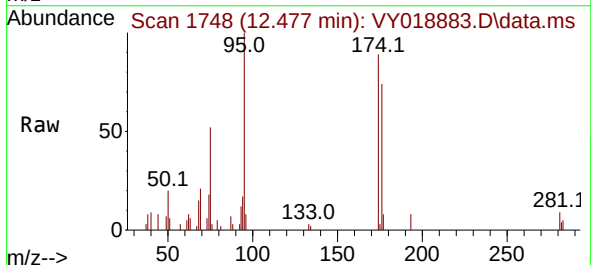


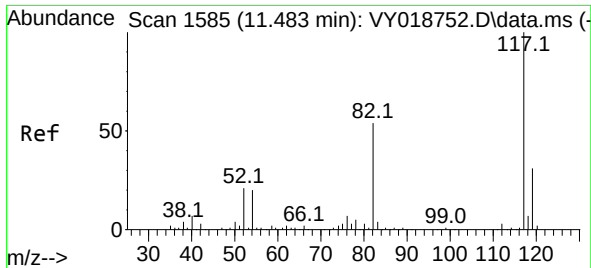

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.483 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY018883.D
Acq: 19 Jul 2024 15:41

Instrument :
MSVOA_Y
ClientSampleId :
285-290

Tgt Ion:117 Resp: 12252
Ion Ratio Lower Upper
117 100
82 55.9 42.4 63.6
119 23.8 25.9 38.9#

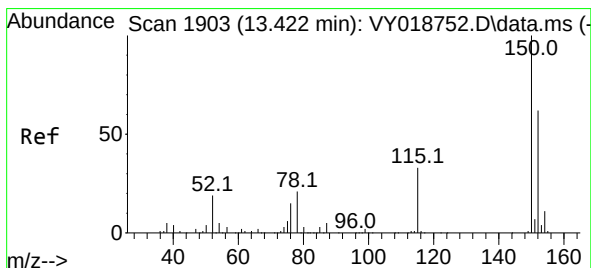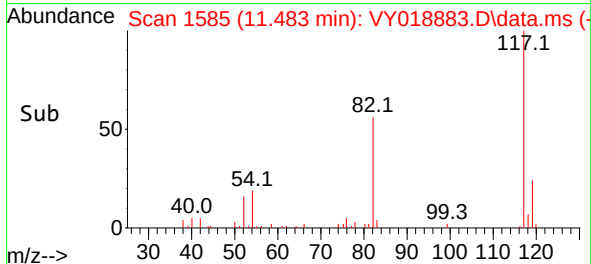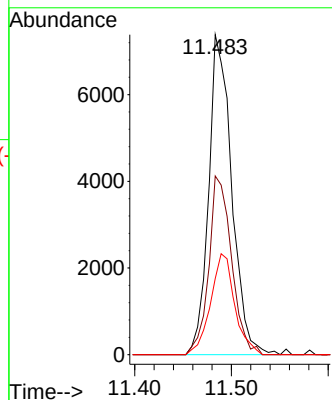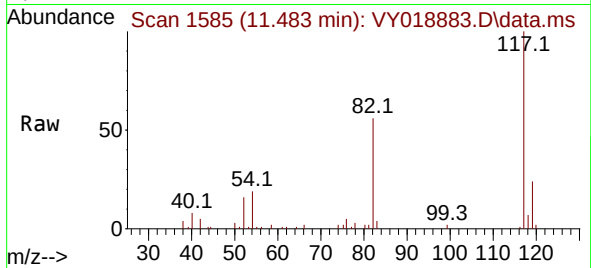

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY018883.D
Acq: 19 Jul 2024 15:41

Tgt Ion:152 Resp: 3807
Ion Ratio Lower Upper
152 100
115 64.9 28.2 84.7
150 158.7 0.0 345.6

