

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072125\
 Data File : VY023021.D
 Acq On : 21 Jul 2025 13:03
 Operator : SY/MD
 Sample : Q2639-09
 Misc : 4.53g/5.0mL/MSVOA_Y/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-TS-42-071725


Quant Time: Jul 22 04:50:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 19 01:50:49 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	305730	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	566544	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	540204	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	221582	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	169589	54.794	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 109.580%	
35) Dibromofluoromethane	7.634	113	177965	49.520	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 99.040%	
50) Toluene-d8	10.103	98	686049	48.138	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 96.280%	
62) 4-Bromofluorobenzene	12.401	95	229089	51.065	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 102.140%	
Target Compounds						Qvalue
13) Acrolein	3.665	56	135	1.535	ug/l	93
16) Acetone	3.872	43	1331	2.372	ug/l #	75
20) Methylene Chloride	4.610	84	15933	Below Cal	#	92
31) Cyclohexane	7.701	56	6830	1.108	ug/l #	27
36) 1,1-Dichloropropene	7.707	75	25407	4.488	ug/l #	51
38) Carbon Tetrachloride	7.707	117	30527	4.964	ug/l #	17
76) 1,2,3-Trichloropropane	12.401	75	123881	44.867	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.401	75	123881	133.634	ug/l #	12

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jul 22 04:50:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 19 01:50:49 2025
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-42-071725


Tgt Ion:168 Resp: 305730
Ion Ratio Lower Upper
168 100
99 57.9 44.4 66.6

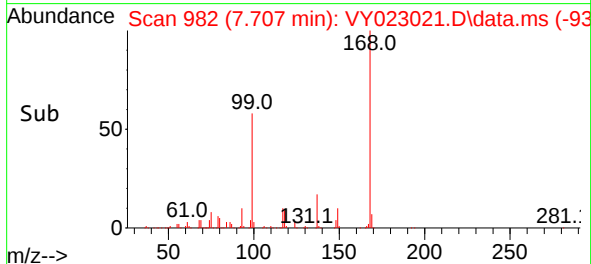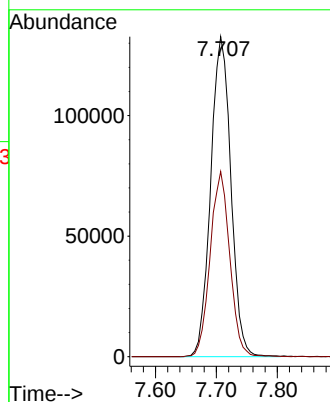

#13
Acrolein
Concen: 1.535 ug/l
RT: 3.665 min Scan# 319
Delta R.T. 0.012 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Tgt Ion: 56 Resp: 135
Ion Ratio Lower Upper
56 100
55 77.8 57.8 86.6


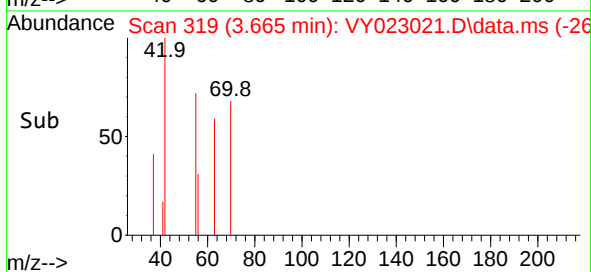
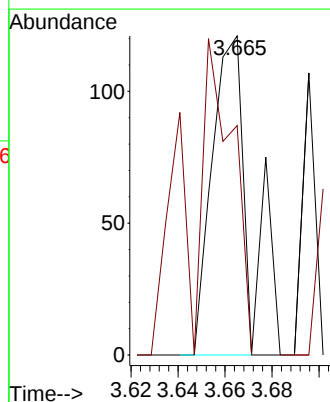
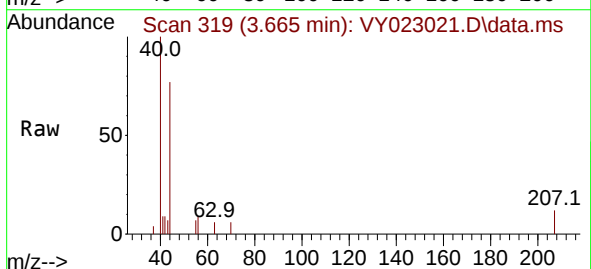




#16
Acetone
Concen: 2.372 ug/l
RT: 3.872 min Scan# 31
Delta R.T. 0.006 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-42-071725


Tgt Ion: 43 Resp: 1331
Ion Ratio Lower Upper
43 100
58 46.8 26.2 39.4#

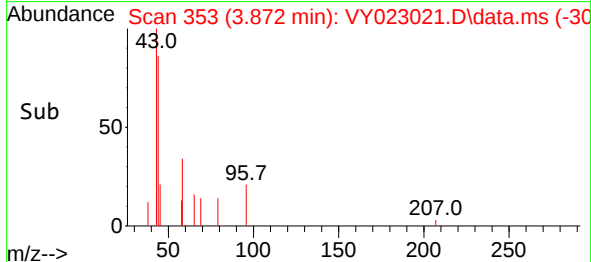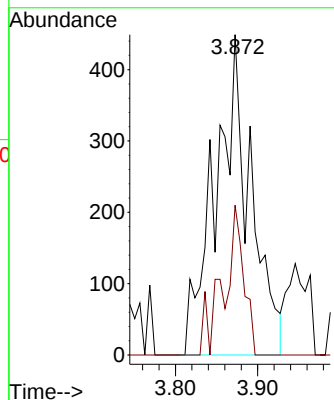

#20
Methylene Chloride
Concen: Below Cal
RT: 4.610 min Scan# 474
Delta R.T. 0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Tgt Ion: 84 Resp: 15933
Ion Ratio Lower Upper
84 100
49 123.7 98.2 147.4
51 25.8 30.5 45.7#
86 52.0 51.3 76.9


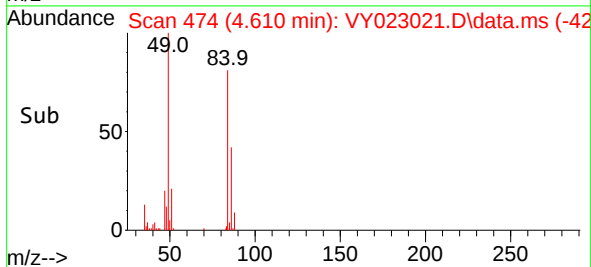
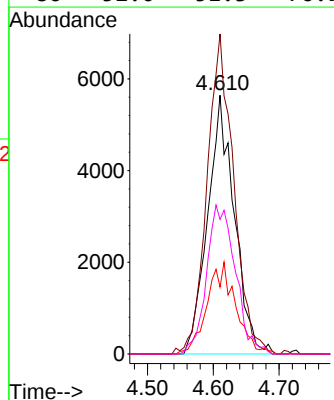
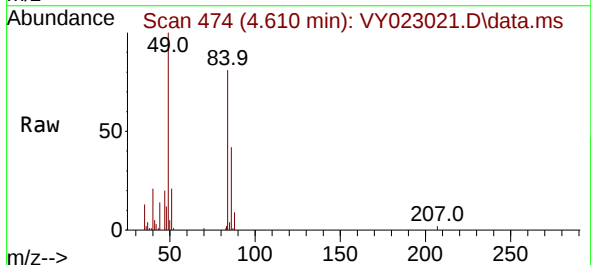




#31
Cyclohexane
Concen: 1.108 ug/l
RT: 7.701 min Scan# 981
Delta R.T. -0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-42-071725


Tgt Ion: 56 Resp: 6830
Ion Ratio Lower Upper
56 100
69 145.0 28.1 42.1#
84 119.2 73.5 110.3#

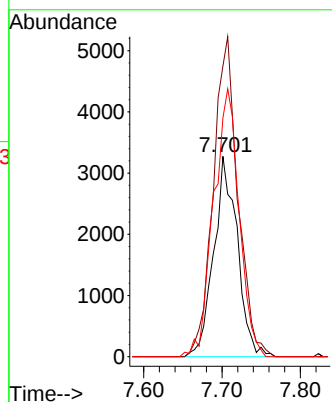

#33
1,2-Dichloroethane-d4
Concen: 54.794 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Tgt Ion: 65 Resp: 169589
Ion Ratio Lower Upper
65 100
67 53.1 0.0 107.4


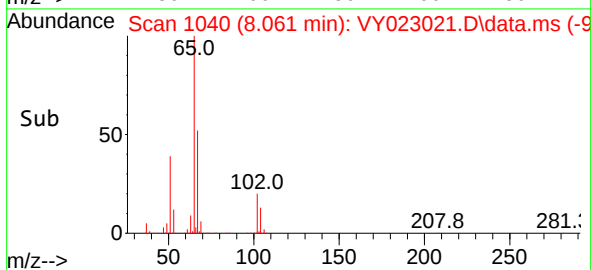
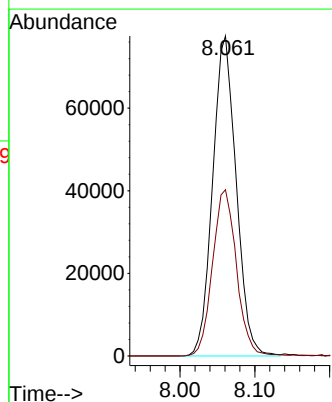
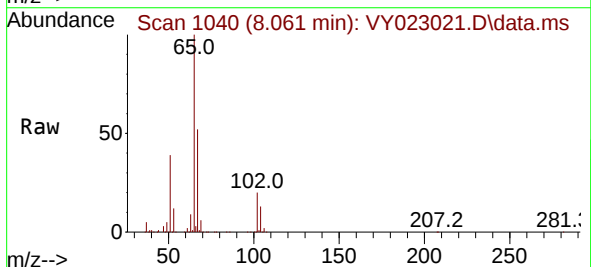




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.609 min Scan# 1131
Delta R.T. -0.006 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-42-071725


Tgt Ion:114 Resp: 566544
Ion Ratio Lower Upper
114 100
63 20.9 0.0 38.8
88 15.4 0.0 30.2

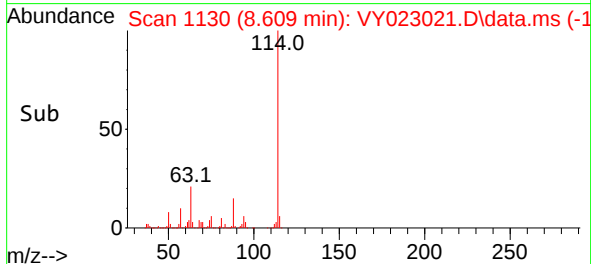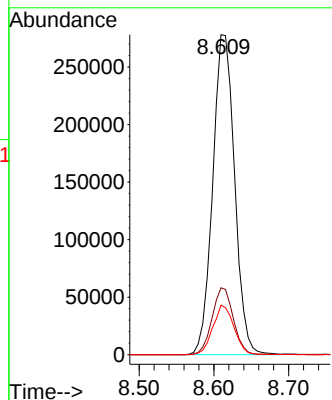

#35
Dibromofluoromethane
Concen: 49.520 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Tgt Ion:113 Resp: 177965
Ion Ratio Lower Upper
113 100
111 103.5 83.2 124.8
192 19.0 15.3 22.9

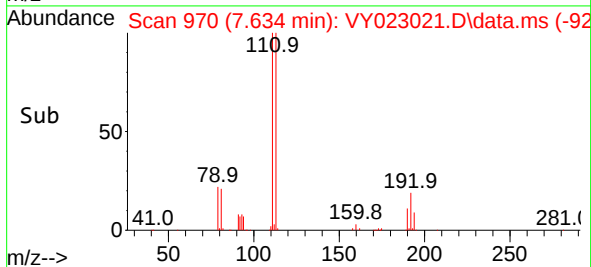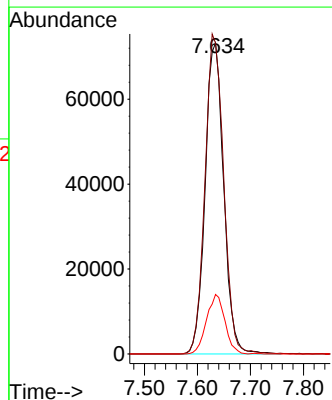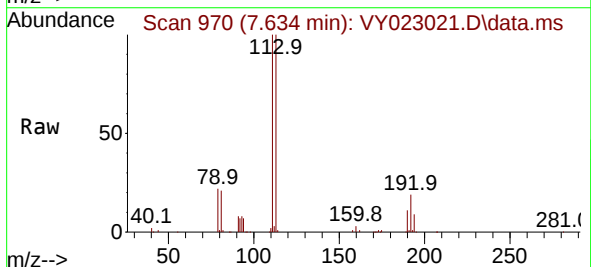



#36

1,1-Dichloropropene

Concen: 4.488 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.128 min

Lab File: VY023021.D

Acq: 21 Jul 2025 13:03

Instrument :

MSVOA_Y

ClientSampleId :

OU4-TS-42-071725





Tgt Ion: 75 Resp: 25407

Ion Ratio Lower Upper

75 100

110 9.6 17.3 51.9#

77 0.0 24.6 37.0#

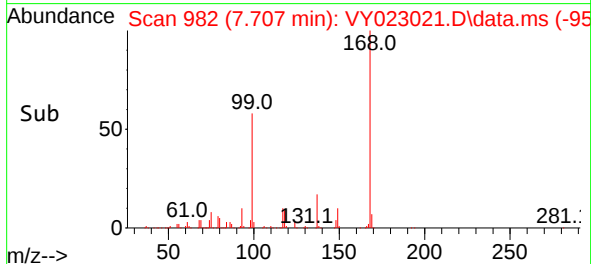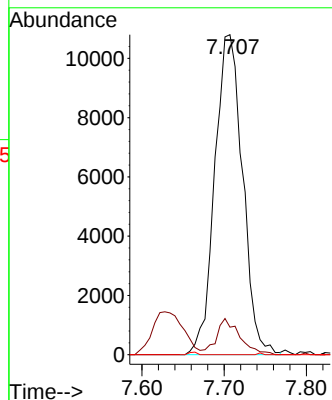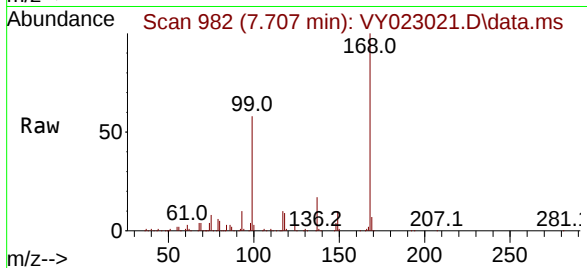

#38

Carbon Tetrachloride

Concen: 4.964 ug/l

RT: 7.707 min Scan# 982

Delta R.T. -0.110 min

Lab File: VY023021.D

Acq: 21 Jul 2025 13:03




Tgt Ion: 117 Resp: 30527


Ion Ratio Lower Upper

117 100

119 5.4 74.9 112.3#

121 0.0 24.6 37.0#



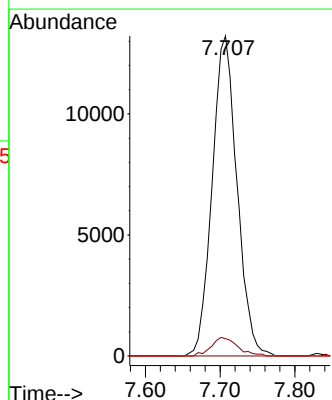
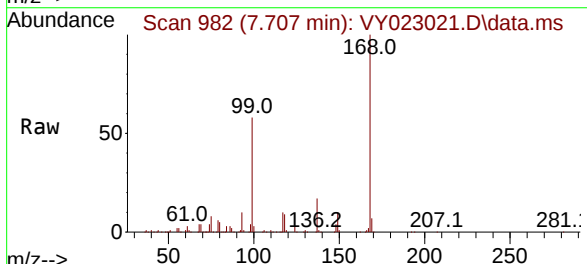




#50
Toluene-d8
Concen: 48.138 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. -0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-42-071725


Tgt Ion: 98 Resp: 686049
Ion Ratio Lower Upper
98 100
100 64.2 52.2 78.2

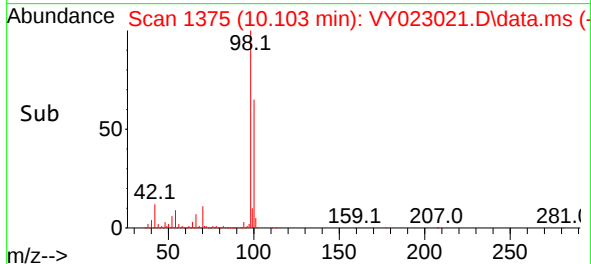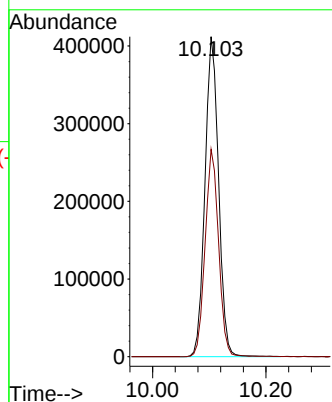

#62
4-Bromofluorobenzene
Concen: 51.065 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Tgt Ion: 95 Resp: 229089
Ion Ratio Lower Upper
95 100
174 84.2 0.0 170.8
176 80.9 0.0 163.6


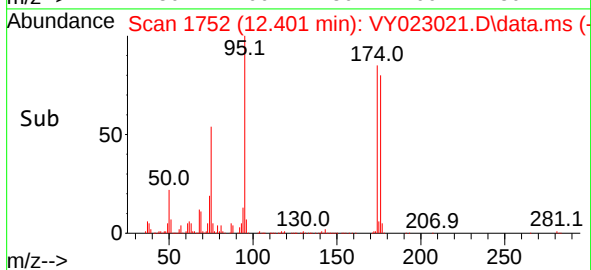
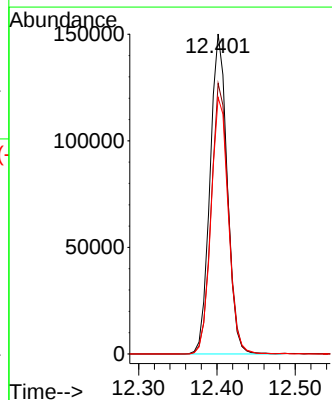
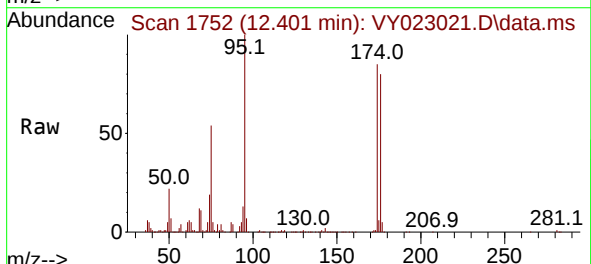


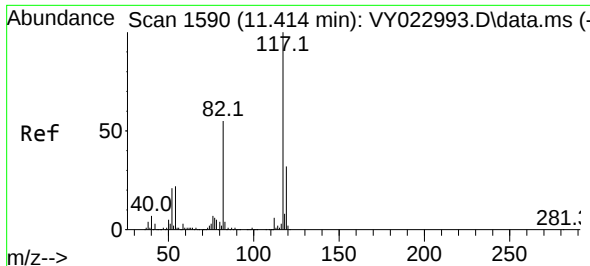

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03




Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-42-071725


Tgt Ion:117 Resp: 540204
Ion Ratio Lower Upper
117 100
82 56.3 44.3 66.5
119 32.9 25.8 38.8

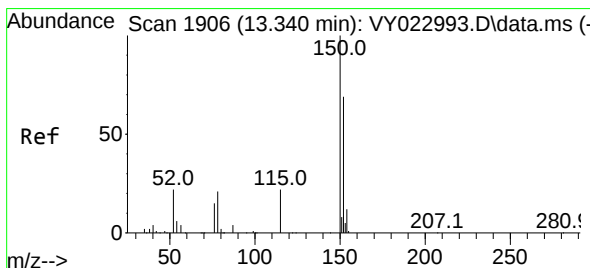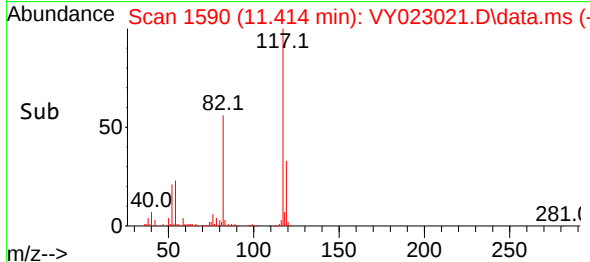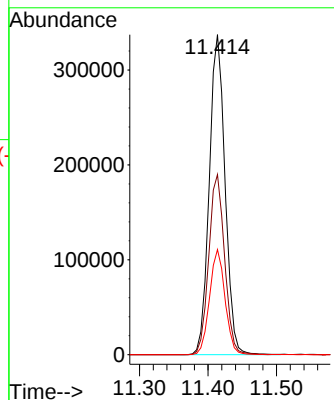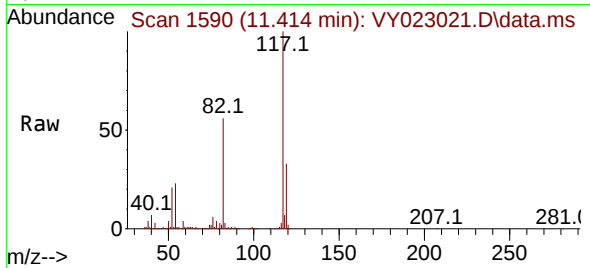

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.340 min Scan# 1906
Delta R.T. -0.000 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Tgt Ion:152 Resp: 221582
Ion Ratio Lower Upper
152 100
115 57.8 29.4 88.2
150 156.4 0.0 350.0


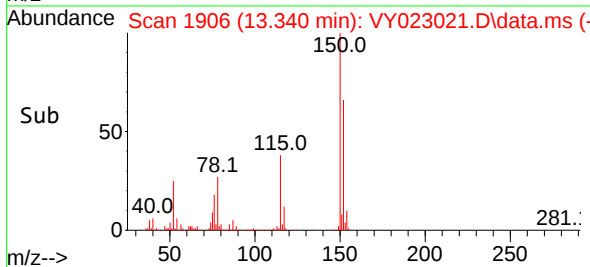
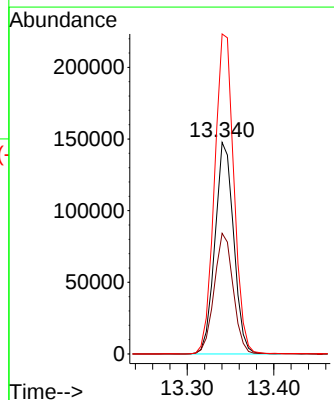
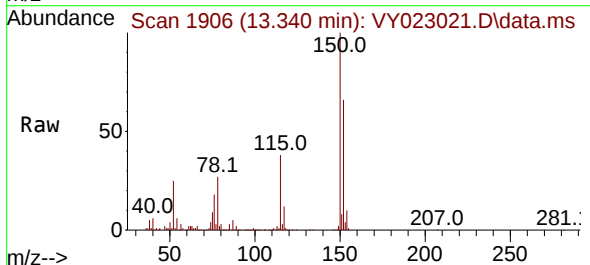




#76
1,2,3-Trichloropropane
Concen: 44.867 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.152 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Instrument :
MSVOA_Y
ClientSampleId :
OU4-TS-42-071725

Tgt Ion: 75 Resp: 123881
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

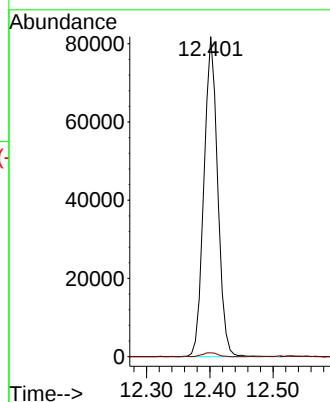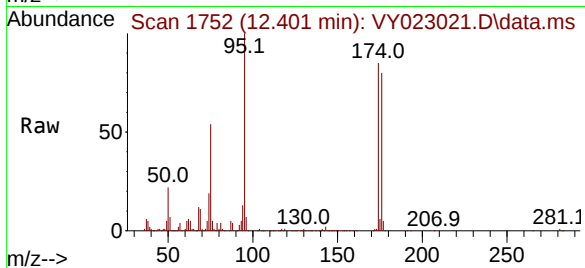

#81
trans-1,4-Dichloro-2-butene
Concen: 133.634 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. 0.104 min
Lab File: VY023021.D
Acq: 21 Jul 2025 13:03

Tgt Ion: 75 Resp: 123881
Ion Ratio Lower Upper
75 100
53 0.1 76.1 114.1#
89 0.0 36.1 54.1#

