

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072125\
 Data File : VY023036.D
 Acq On : 21 Jul 2025 18:54
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VIBLK

Quant Time: Jul 22 04:56:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 19 01:50:49 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	274387	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	539119	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	567438	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	271419	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	170008	61.204	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.400%
35) Dibromofluoromethane	7.634	113	172191	50.351	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.700%
50) Toluene-d8	10.103	98	679319	50.091	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	100.180%
62) 4-Bromofluorobenzene	12.402	95	261640	61.288	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	122.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072125\
Data File : VY023036.D
Acq On : 21 Jul 2025 18:54
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK

Quant Time: Jul 22 04:56:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071825S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 19 01:50:49 2025
Response via : Initial Calibration




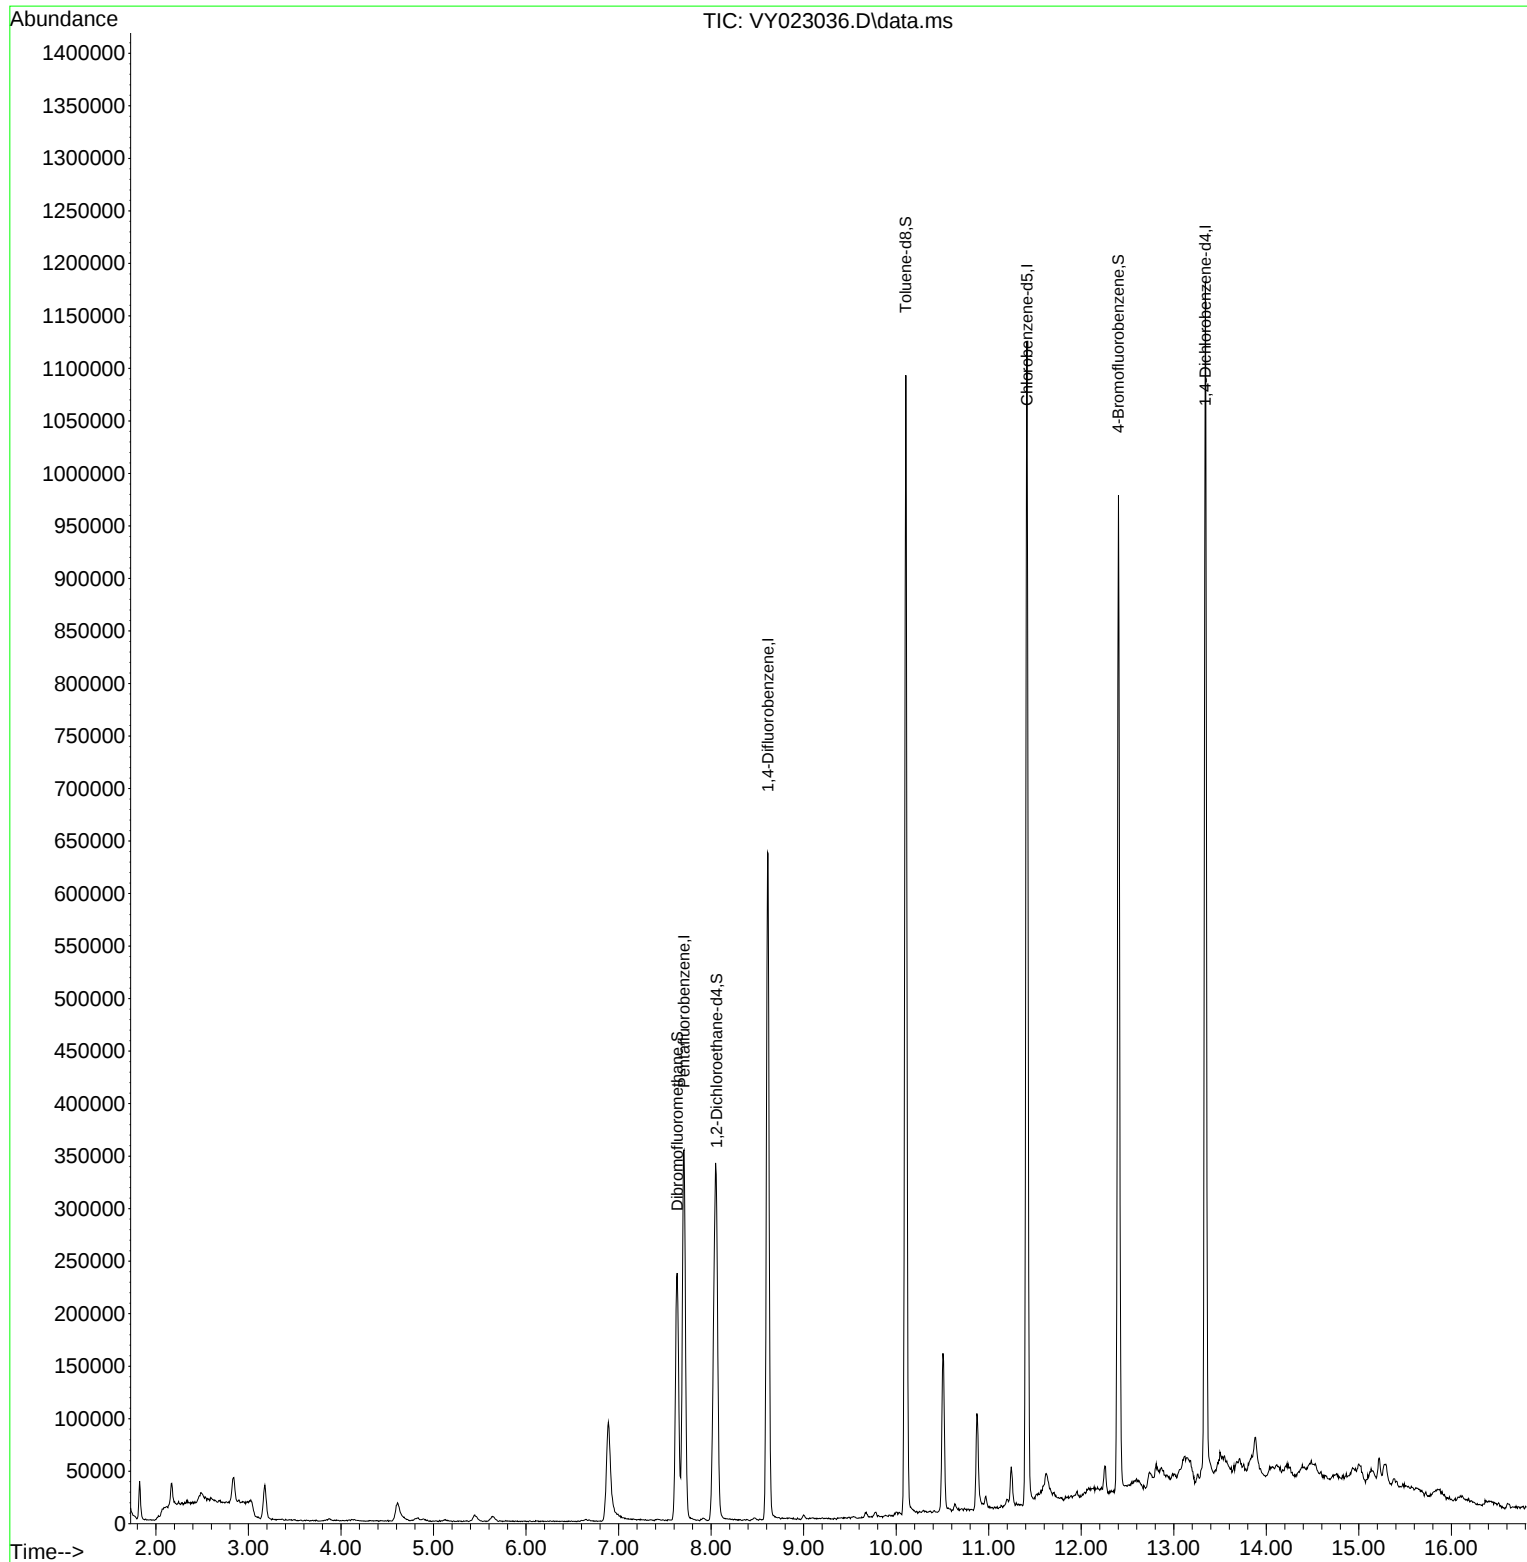


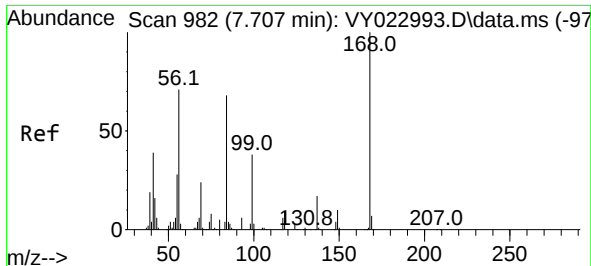

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 982
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 274387
Ion Ratio Lower Upper
168 100
99 56.5 44.4 66.6

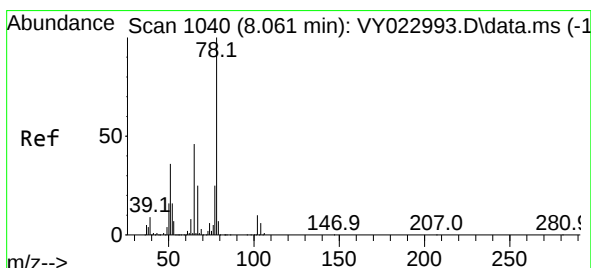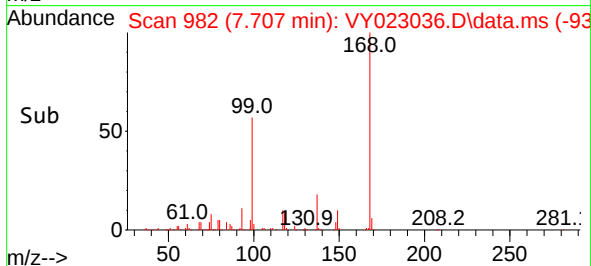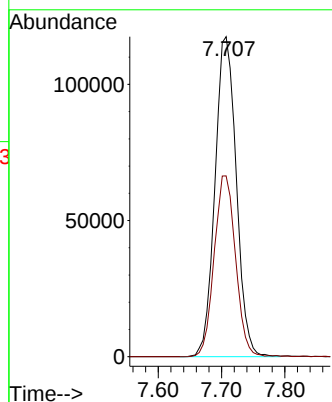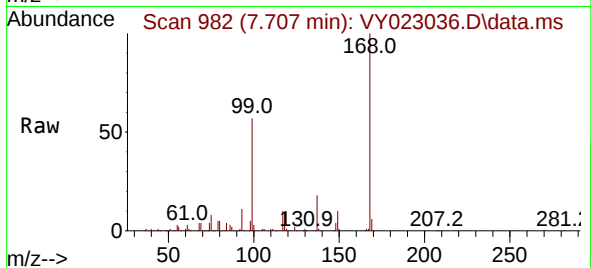

#33
1,2-Dichloroethane-d4
Concen: 61.204 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54

Tgt Ion: 65 Resp: 170008
Ion Ratio Lower Upper
65 100
67 53.7 0.0 107.4


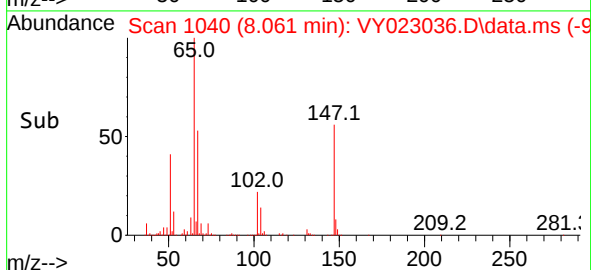
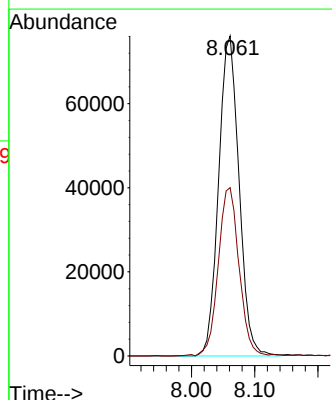
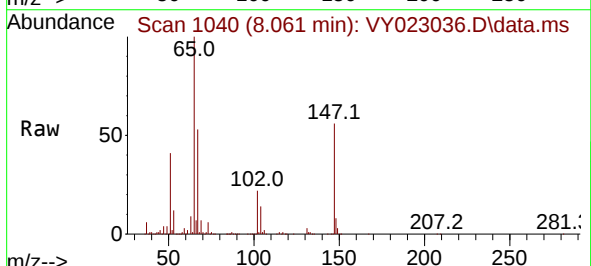


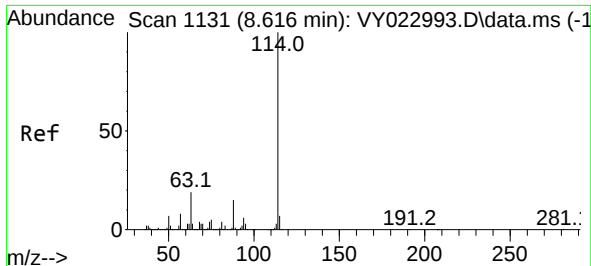

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:114 Resp: 539119
Ion Ratio Lower Upper
114 100
63 19.1 0.0 38.8
88 14.6 0.0 30.2

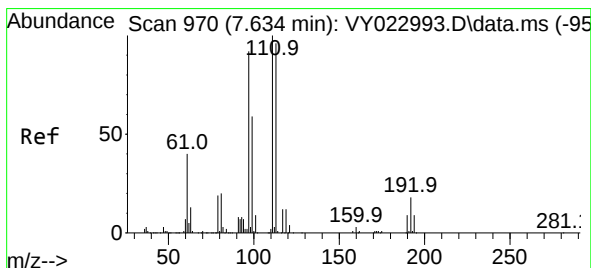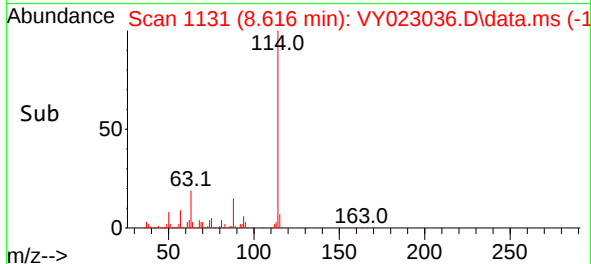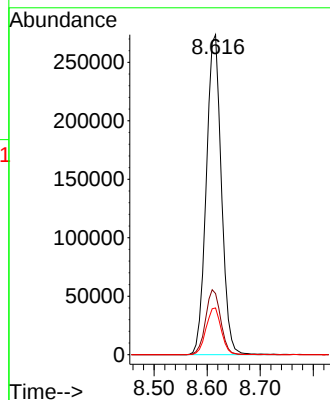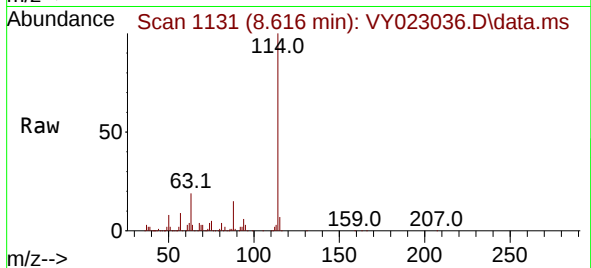

#35
Dibromofluoromethane
Concen: 50.351 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54

Tgt Ion:113 Resp: 172191
Ion Ratio Lower Upper
113 100
111 101.7 83.2 124.8
192 19.2 15.3 22.9


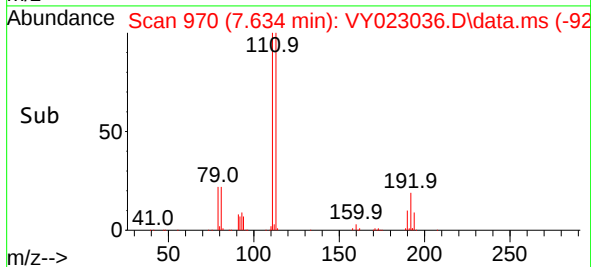
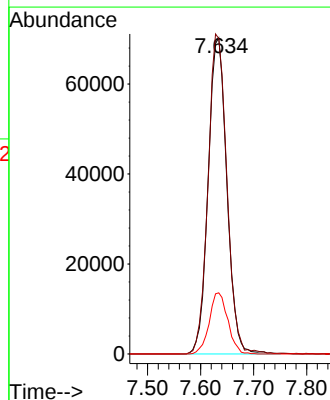
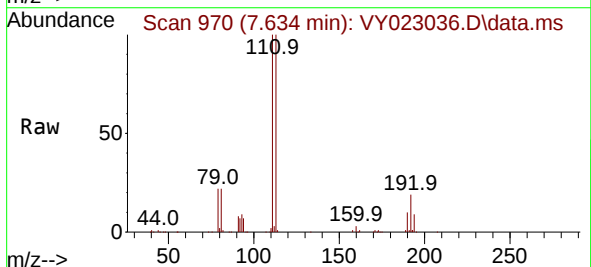


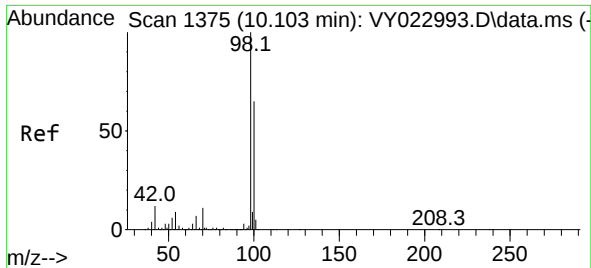

#50
Toluene-d8
Concen: 50.091 ug/l
RT: 10.103 min Scan# 1375
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 679319
Ion Ratio Lower Upper
98 100
100 64.6 52.2 78.2

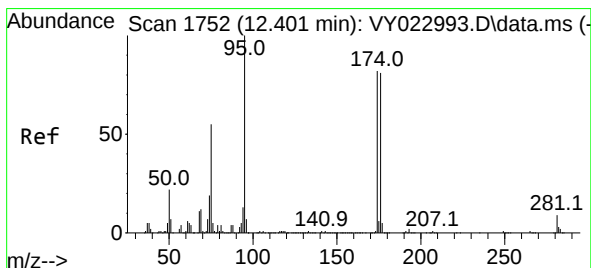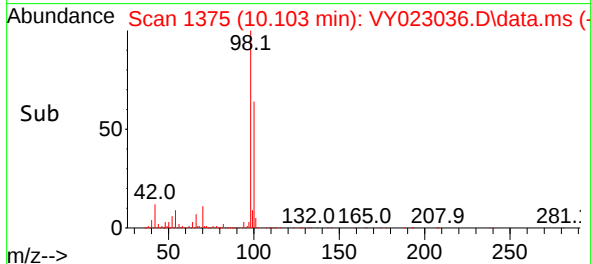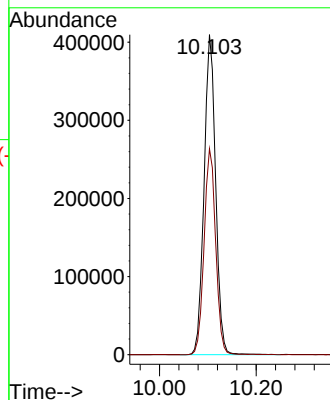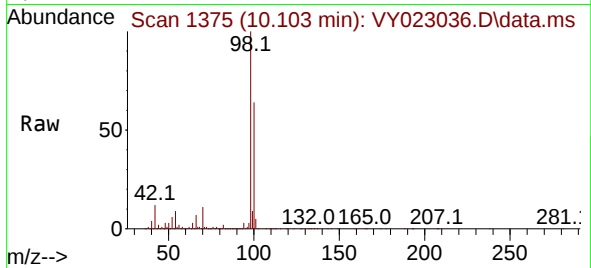

#62
4-Bromofluorobenzene
Concen: 61.288 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54

Tgt Ion: 95 Resp: 261640
Ion Ratio Lower Upper
95 100
174 85.4 0.0 170.8
176 81.7 0.0 163.6


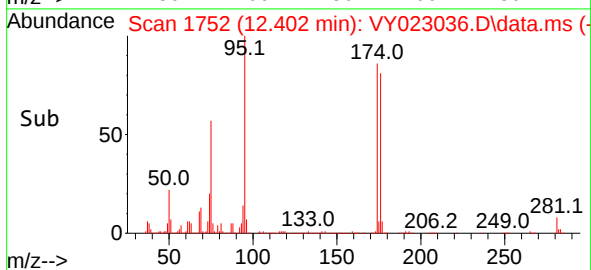
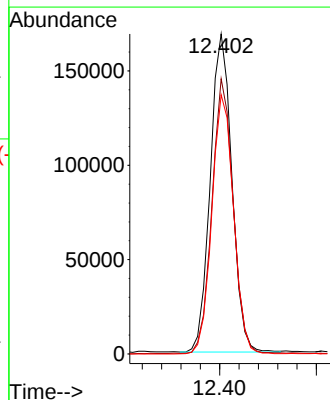
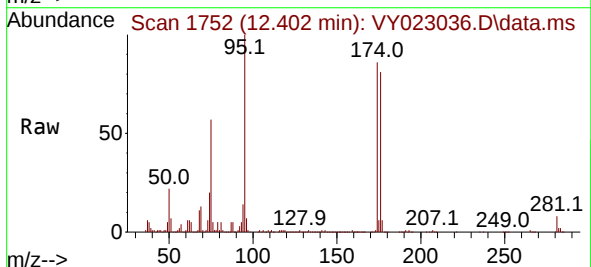


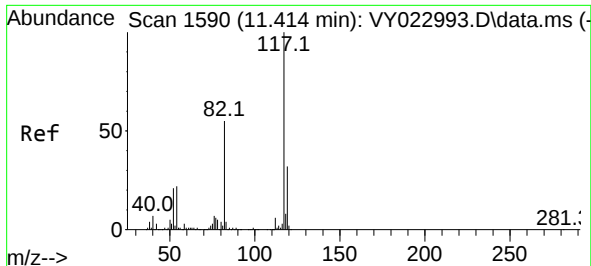

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 567438
Ion Ratio Lower Upper
117 100
82 56.4 44.3 66.5
119 32.0 25.8 38.8

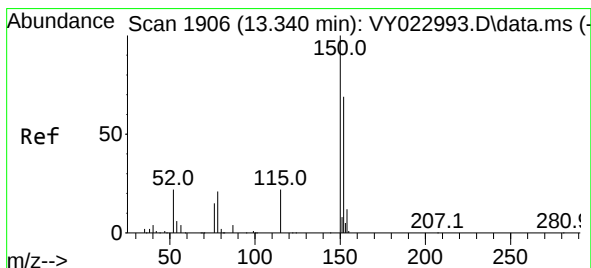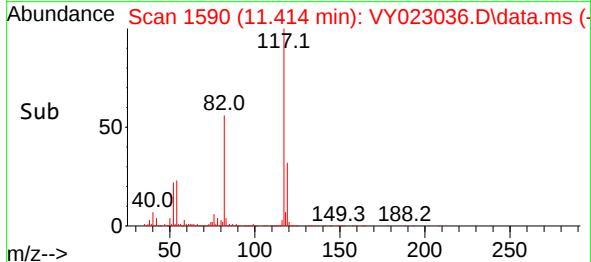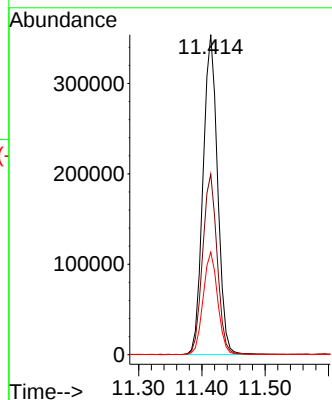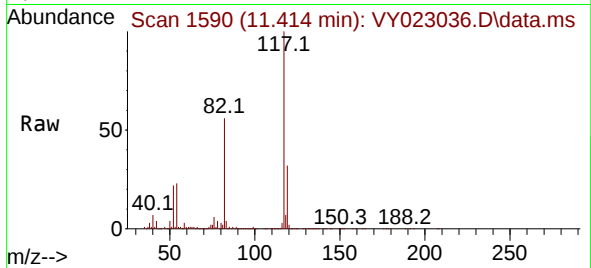

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.340 min Scan# 1906
Delta R.T. 0.000 min
Lab File: VY023036.D
Acq: 21 Jul 2025 18:54

Tgt Ion:152 Resp: 271419
Ion Ratio Lower Upper
152 100
115 58.0 29.4 88.2
150 156.3 0.0 350.0

