
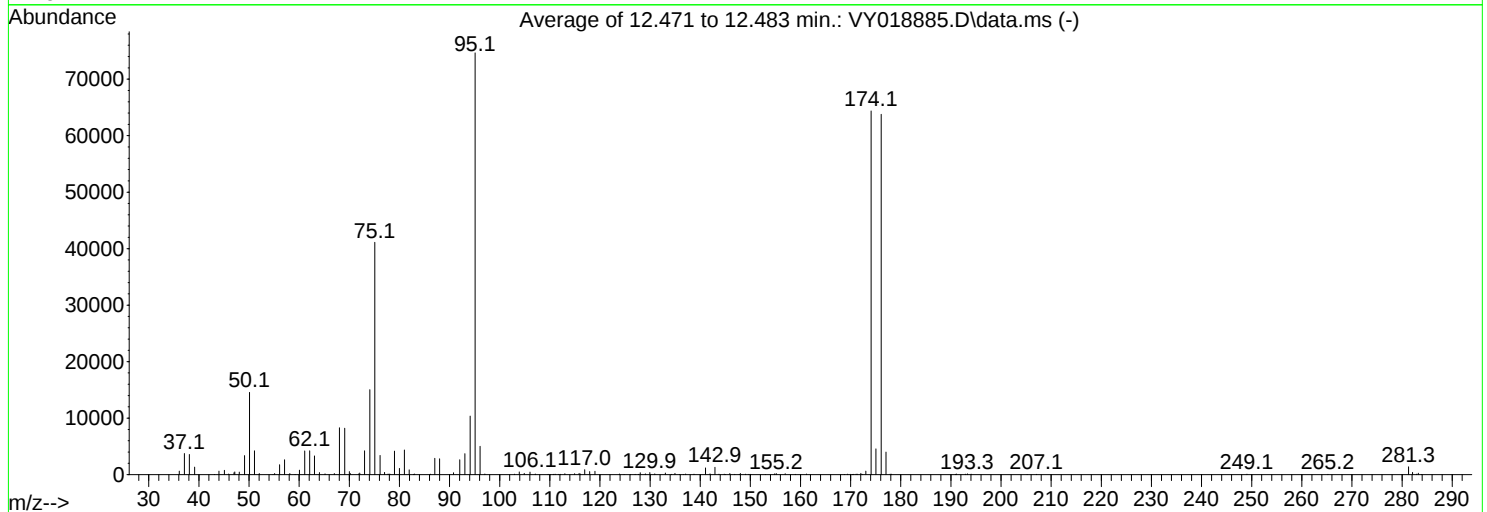


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072224\
Data File : VY018885.D
Acq On : 22 Jul 2024 09:05
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Title : SW846 8260
Last Update : Tue Jul 09 14:28:51 2024

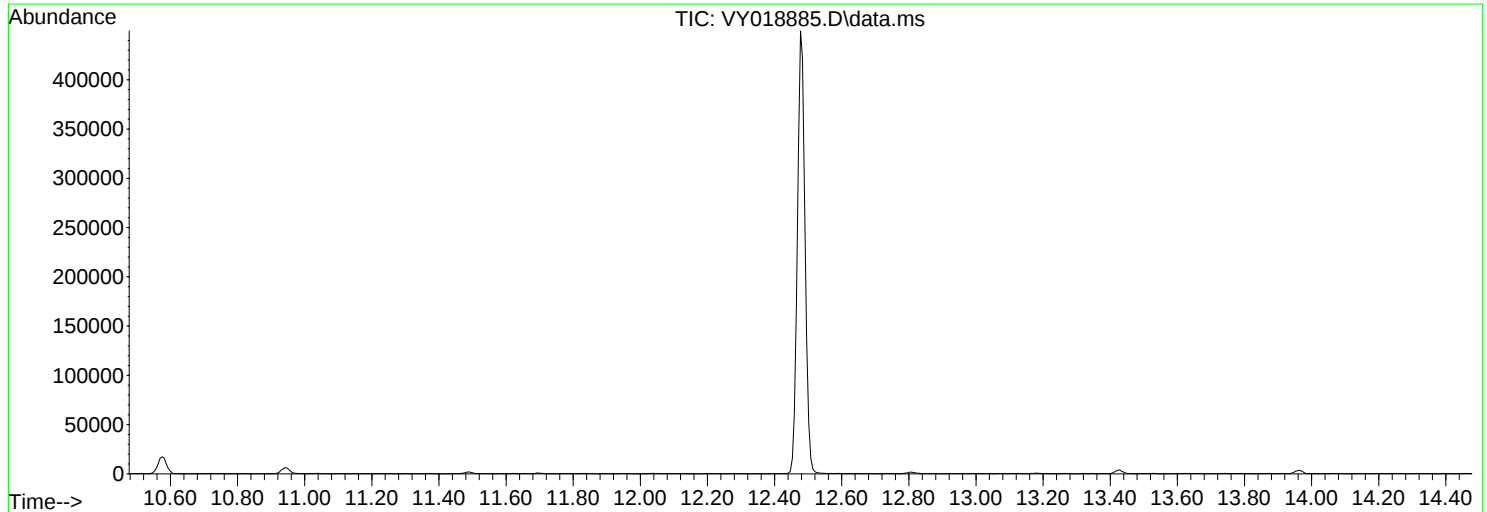

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	14562	PASS
75	95	30	60	55.1	41112	PASS
95	95	100	100	100.0	74659	PASS
96	95	5	9	6.7	5008	PASS
173	174	0.00	2	1.0	621	PASS
174	95	50	100	86.2	64360	PASS
175	174	5	9	7.1	4567	PASS
176	174	95	101	99.1	63789	PASS
177	176	5	9	6.3	3987	PASS