Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072424\
Data File : VY018902.D
Acq On : 24 Jul 2024 10:48
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jul 25 01:24:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 09 14:28:51 2024
Response via : Initial Calibration

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	7.783	168	104871	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	158102	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	136419	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	68808	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	46466	45.027	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 90.060%			
35) Dibromofluoromethane	7.704	113	48815	49.297	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 98.600%			
50) Toluene-d8	10.173	98	173691	46.298	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 92.600%			
62) 4-Bromofluorobenzene	12.477	95	58851	45.935	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 91.880%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.900	85	42983	48.914	ug/l	99
3) Chloromethane	2.107	50	59712	44.716	ug/l	97
4) Vinyl Chloride	2.241	62	72859	46.641	ug/l	100
5) Bromomethane	2.643	94	53168	49.481	ug/l	96
6) Chloroethane	2.784	64	47976	47.273	ug/l	98
7) Trichlorofluoromethane	3.113	101	102463	50.196	ug/l	99
8) Diethyl Ether	3.515	74	25452	51.158	ug/l	99
9) 1,1,2-Trichlorotrifluo...	3.887	101	52470	50.100	ug/l	94
10) Methyl Iodide	4.070	142	59037	52.347	ug/l	93
11) Tert butyl alcohol	4.936	59	17752	169.815	ug/l #	82
12) 1,1-Dichloroethene	3.857	96	48852	48.216	ug/l	96
13) Acrolein	3.716	56	9479	113.177	ug/l	93
14) Allyl chloride	4.460	41	64362	51.276	ug/l	94
15) Acrylonitrile	5.149	53	49081	250.067	ug/l	99
16) Acetone	3.930	43	51993	273.284	ug/l #	83
17) Carbon Disulfide	4.180	76	129982	45.816	ug/l	96
18) Methyl Acetate	4.460	43	27520	49.783	ug/l	97
19) Methyl tert-butyl Ether	5.204	73	120081	51.090	ug/l	98
20) Methylene Chloride	4.698	84	60044	56.359	ug/l	99
21) trans-1,2-Dichloroethene	5.210	96	52483	49.079	ug/l	93
22) Diisopropyl ether	6.106	45	141176	51.706	ug/l	94
23) Vinyl Acetate	6.045	43	554998	258.010	ug/l	97
24) 1,1-Dichloroethane	6.003	63	88368	50.691	ug/l	99
25) 2-Butanone	6.972	43	68319	256.182	ug/l	90
26) 2,2-Dichloropropane	6.960	77	83788	51.801	ug/l	99
27) cis-1,2-Dichloroethene	6.972	96	63562	51.054	ug/l	100
28) Bromochloromethane	7.326	49	36159	51.643	ug/l	95
29) Tetrahydrofuran	7.338	42	41022	250.911	ug/l	93
30) Chloroform	7.496	83	101689	52.339	ug/l	98
31) Cyclohexane	7.777	56	73205	46.174	ug/l	99
32) 1,1,1-Trichloroethane	7.691	97	95510	52.865	ug/l	99
36) 1,1-Dichloropropene	7.911	75	70590	51.656	ug/l	98
37) Ethyl Acetate	7.063	43	30653	53.965	ug/l	95
38) Carbon Tetrachloride	7.893	117	89652	54.470	ug/l	99
39) Methylcyclohexane	9.179	83	89973	51.377	ug/l	97
40) Benzene	8.155	78	208276	52.539	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072424\
Data File : VY018902.D
Acq On : 24 Jul 2024 10:48
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

Quant Time: Jul 25 01:24:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 09 14:28:51 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units		Dev(Min)
41) Methacrylonitrile	7.301	41	17415	53.776	ug/l		88
42) 1,2-Dichloroethane	8.228	62	58569	52.770	ug/l		97
43) Isopropyl Acetate	8.264	43	58206	51.498	ug/l	#	81
44) Trichloroethene	8.935	130	61707	54.456	ug/l		99
45) 1,2-Dichloropropane	9.209	63	46287	53.620	ug/l		97
46) Dibromomethane	9.301	93	30373	54.281	ug/l		97
47) Bromodichloromethane	9.490	83	77993	55.795	ug/l		97
48) Methyl methacrylate	9.283	41	26870	52.303	ug/l		90
49) 1,4-Dioxane	9.295	88	6962	1061.415	ug/l	#	93
51) 4-Methyl-2-Pentanone	10.063	43	150324	260.499	ug/l		93
52) Toluene	10.240	92	133313	50.596	ug/l		100
53) t-1,3-Dichloropropene	10.459	75	65949	54.643	ug/l		98
54) cis-1,3-Dichloropropene	9.923	75	77772	54.928	ug/l	#	90
55) 1,1,2-Trichloroethane	10.642	97	38487	54.317	ug/l		94
56) Ethyl methacrylate	10.508	69	49657	53.230	ug/l	#	85
57) 1,3-Dichloropropane	10.782	76	62701	53.381	ug/l		99
58) 2-Chloroethyl Vinyl ether	9.776	63	119507	268.145	ug/l		93
59) 2-Hexanone	10.825	43	107104	265.300	ug/l		90
60) Dibromochloromethane	10.977	129	54637	56.121	ug/l		99
61) 1,2-Dibromoethane	11.087	107	36008	52.272	ug/l		98
64) Tetrachloroethene	10.715	164	60492	54.783	ug/l		97
65) Chlorobenzene	11.514	112	157151	54.609	ug/l		99
66) 1,1,1,2-Tetrachloroethane	11.587	131	55002	55.473	ug/l		97
67) Ethyl Benzene	11.587	91	268843	53.328	ug/l		97
68) m/p-Xylenes	11.703	106	209192	105.742	ug/l		97
69) o-Xylene	12.026	106	101802	54.735	ug/l		98
70) Styrene	12.044	104	168901	54.425	ug/l		97
71) Bromoform	12.203	173	32006	59.221	ug/l	#	97
73) Isopropylbenzene	12.325	105	263272	52.280	ug/l		98
74) N-amyl acetate	12.142	43	52946	51.410	ug/l		91
75) 1,1,2,2-Tetrachloroethane	12.581	83	40419	50.914	ug/l		99
76) 1,2,3-Trichloropropane	12.629	75	27554m	51.128	ug/l		
77) Bromobenzene	12.605	156	62832	52.264	ug/l		94
78) n-propylbenzene	12.672	91	307989	51.502	ug/l		97
79) 2-Chlorotoluene	12.751	91	173481	51.591	ug/l		97
80) 1,3,5-Trimethylbenzene	12.812	105	221543	53.767	ug/l		100
81) trans-1,4-Dichloro-2-b...	12.373	75	12389	51.450	ug/l	#	82
82) 4-Chlorotoluene	12.855	91	181284	52.356	ug/l		98
83) tert-Butylbenzene	13.075	119	204204	53.680	ug/l		99
84) 1,2,4-Trimethylbenzene	13.117	105	214459	52.377	ug/l		98
85) sec-Butylbenzene	13.251	105	290710	53.840	ug/l		97
86) p-Isopropyltoluene	13.367	119	248859	53.387	ug/l		95
87) 1,3-Dichlorobenzene	13.361	146	128664	54.492	ug/l		100
88) 1,4-Dichlorobenzene	13.446	146	125430	53.598	ug/l		99
89) n-Butylbenzene	13.696	91	224660	53.161	ug/l		98
90) Hexachloroethane	13.958	117	48749	56.233	ug/l		98
91) 1,2-Dichlorobenzene	13.739	146	110895	54.370	ug/l		99
92) 1,2-Dibromo-3-Chloropr...	14.355	75	6674	51.882	ug/l		95
93) 1,2,4-Trichlorobenzene	15.007	180	70237	56.412	ug/l		98
94) Hexachlorobutadiene	15.111	225	42904	59.784	ug/l		97
95) Naphthalene	15.233	128	118696	55.571	ug/l		99
96) 1,2,3-Trichlorobenzene	15.422	180	59714	56.053	ug/l		98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072424\
Data File : VY018902.D
Acq On : 24 Jul 2024 10:48
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

Quant Time: Jul 25 01:24:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 09 14:28:51 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072424\
Data File : VY018902.D
Acq On : 24 Jul 2024 10:48
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jul 25 01:24:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 09 14:28:51 2024
Response via : Initial Calibration

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

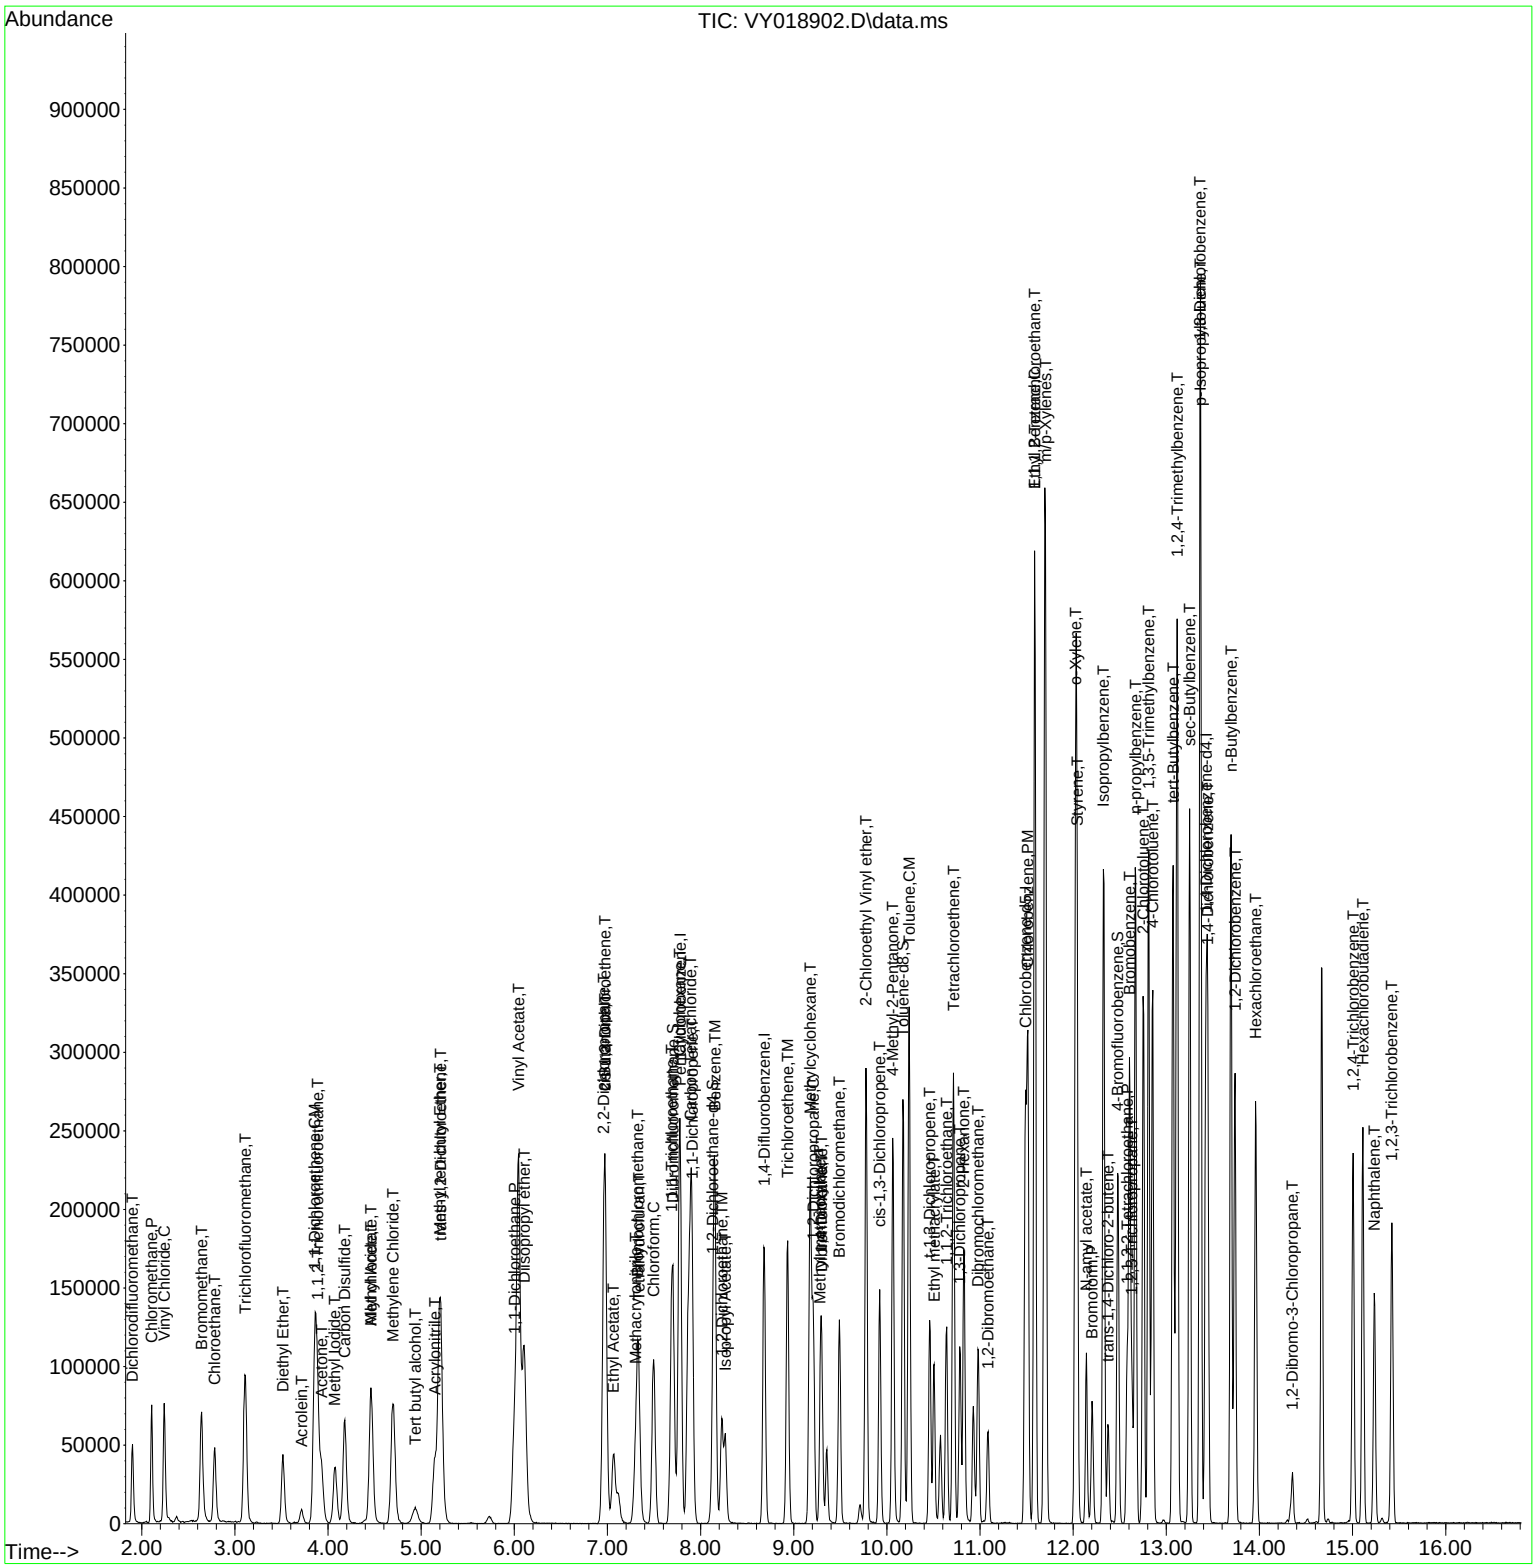

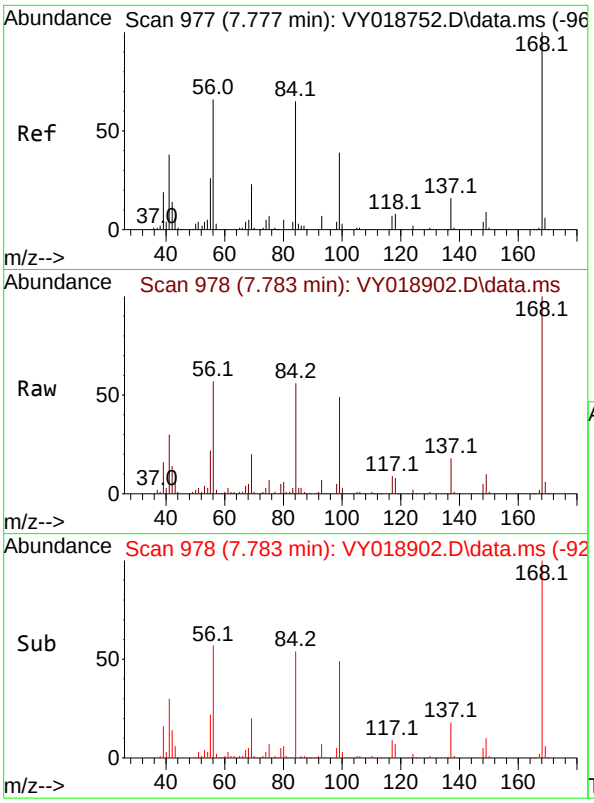

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 9
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:168 Resp: 10487

Ion	Ratio	Lower	Upper
168	100		
99	49.2	39.1	58.7



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

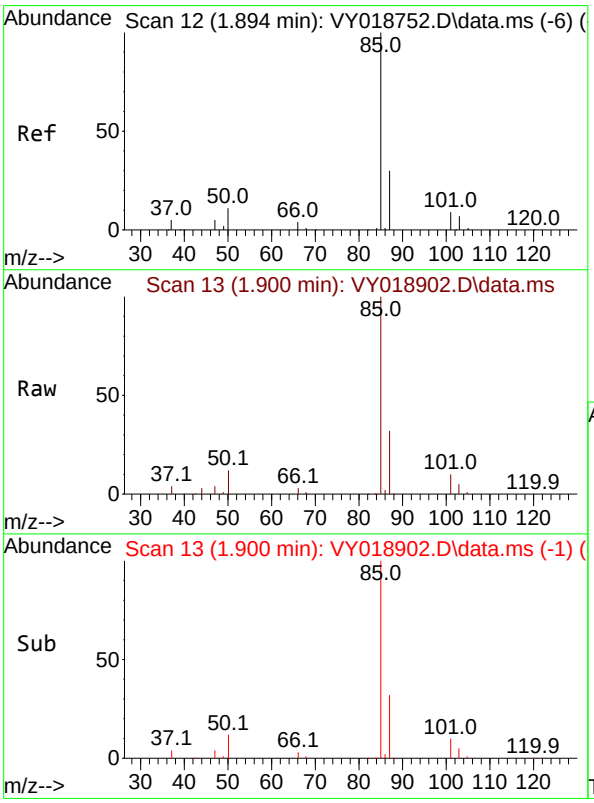

#2
Dichlorodifluoromethane
Concen: 48.914 ug/l
RT: 1.900 min Scan# 13
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 85 Resp: 42983

Ion	Ratio	Lower	Upper
85	100		
87	31.7	16.0	48.0



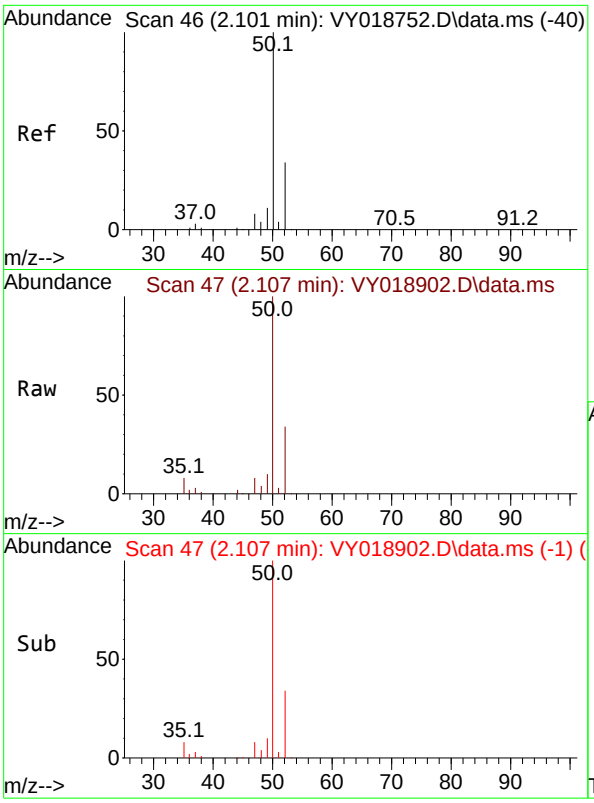

#3
Chloromethane
Concen: 44.716 ug/l
RT: 2.107 min Scan# 4
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 50 Resp: 5971

Ion	Ratio	Lower	Upper
50	100		
52	33.9	25.6	38.4



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

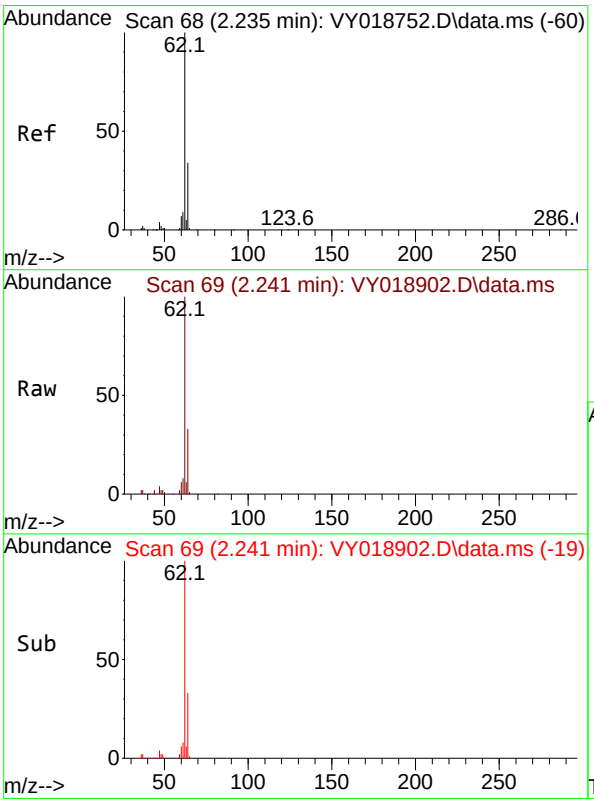

#4
Vinyl Chloride
Concen: 46.641 ug/l
RT: 2.241 min Scan# 69
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 62 Resp: 72859

Ion	Ratio	Lower	Upper
62	100		
64	32.6	26.1	39.1



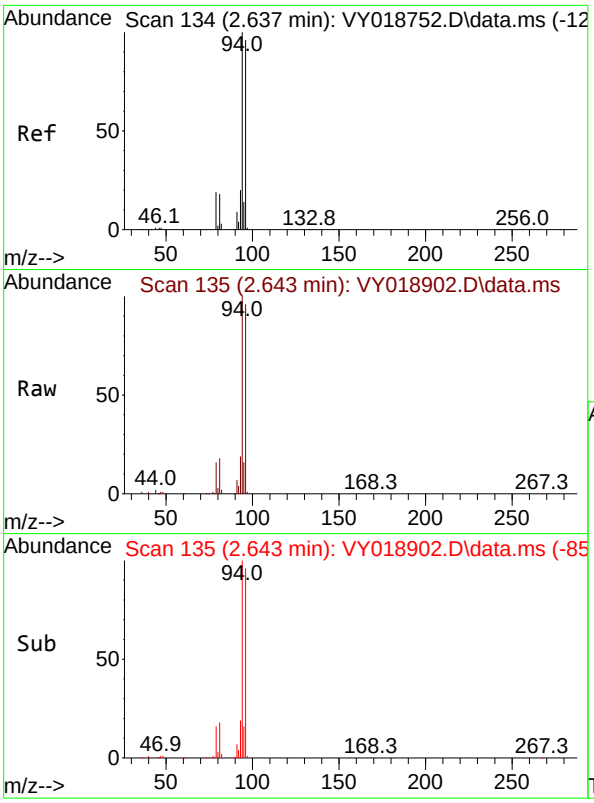

#5
Bromomethane
Concen: 49.481 ug/l
RT: 2.643 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 94 Resp: 5316

Ion	Ratio	Lower	Upper
94	100		
96	96.3	74.1	111.1



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

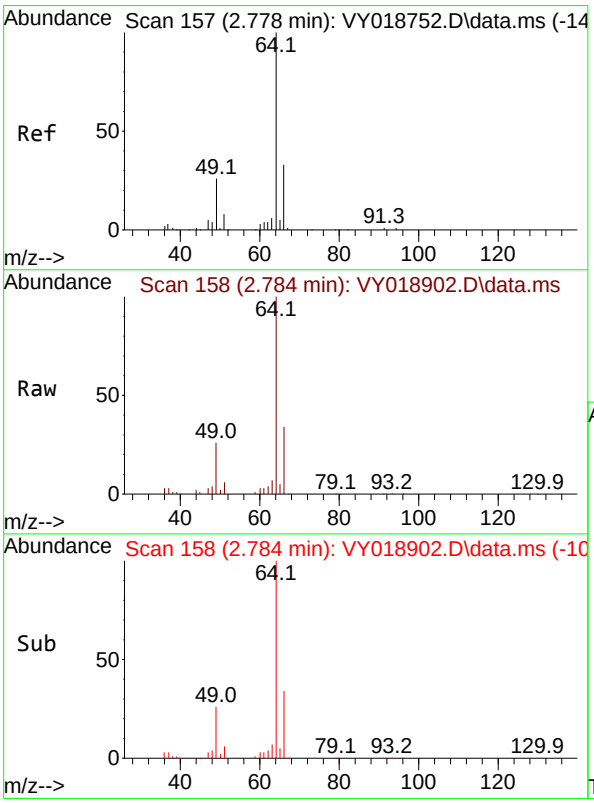

#6
Chloroethane
Concen: 47.273 ug/l
RT: 2.784 min Scan# 158
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 64 Resp: 47976

Ion	Ratio	Lower	Upper
64	100		
66	33.5	26.1	39.1



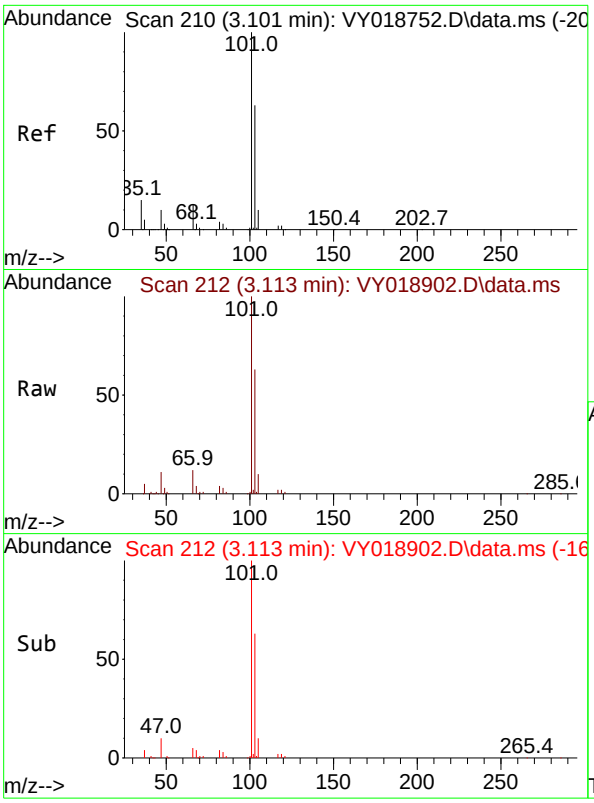

#7
Trichlorofluoromethane
Concen: 50.196 ug/l
RT: 3.113 min Scan# 21
Delta R.T. 0.012 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:101 Resp: 10246

Ion	Ratio	Lower	Upper
101	100		
103	62.6	49.3	73.9

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



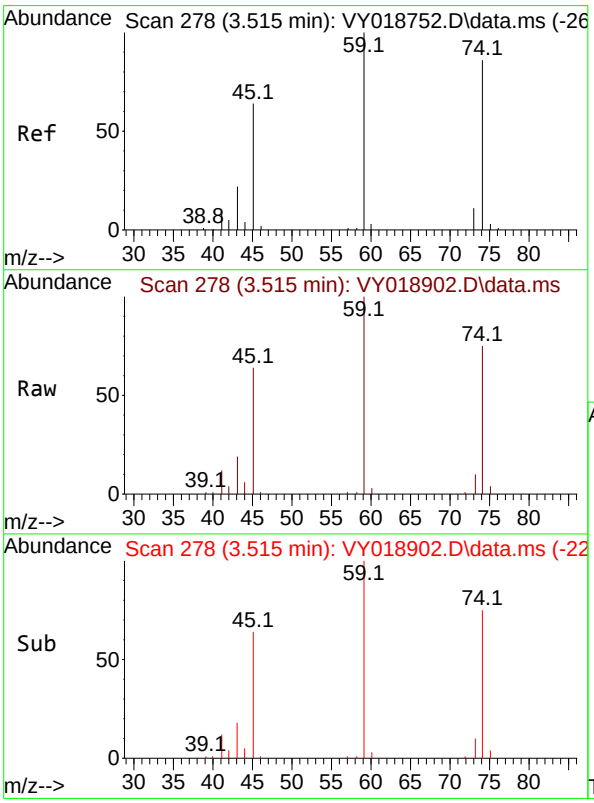

#8
Diethyl Ether
Concen: 51.158 ug/l
RT: 3.515 min Scan# 278
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 74 Resp: 25452

Ion	Ratio	Lower	Upper
74	100		
45	83.5	41.3	124.1



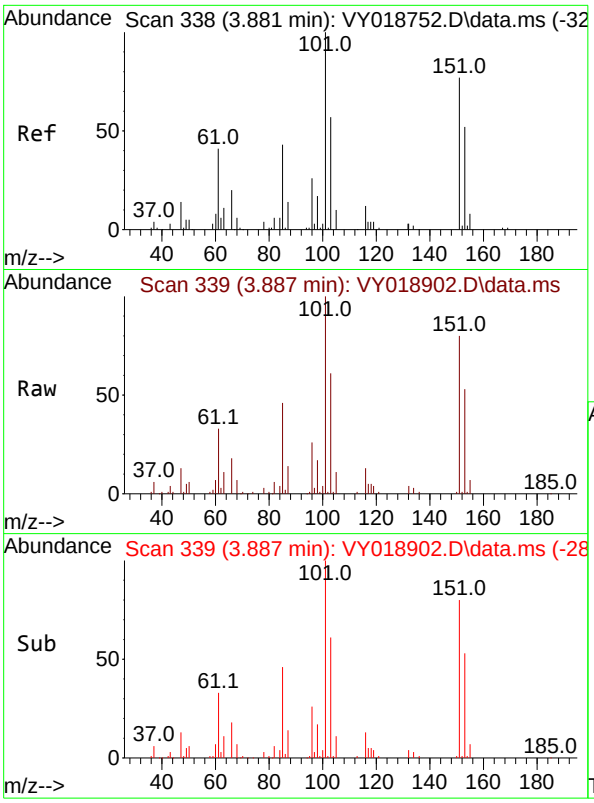

#9
1,1,2-Trichlorotrifluoroethane
Concen: 50.100 ug/l
RT: 3.887 min Scan# 3
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:101 Resp: 5247

Ion	Ratio	Lower	Upper
101	100		
85	47.1	34.5	51.7
151	82.0	61.7	92.5

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



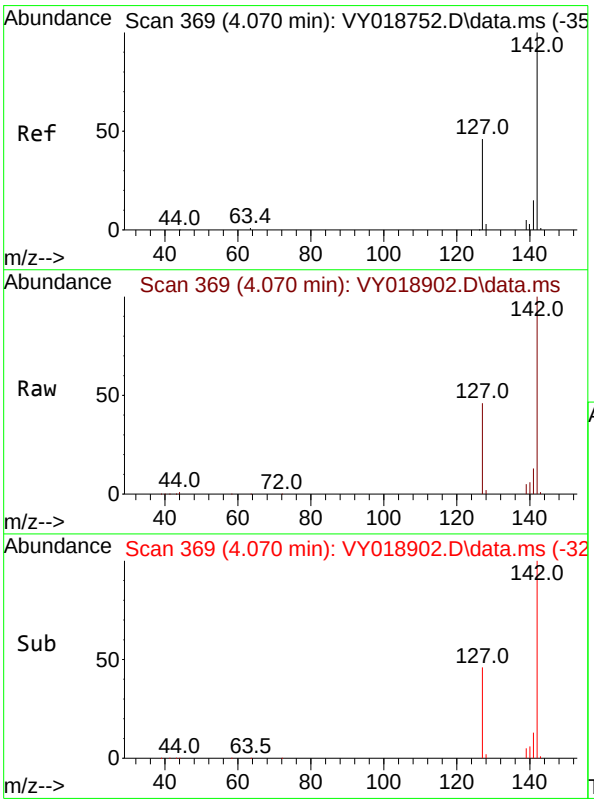

#10
Methyl Iodide
Concen: 52.347 ug/l
RT: 4.070 min Scan# 369
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:142 Resp: 59037

Ion	Ratio	Lower	Upper
142	100		
127	46.8	32.8	49.2
141	13.4	11.4	17.2



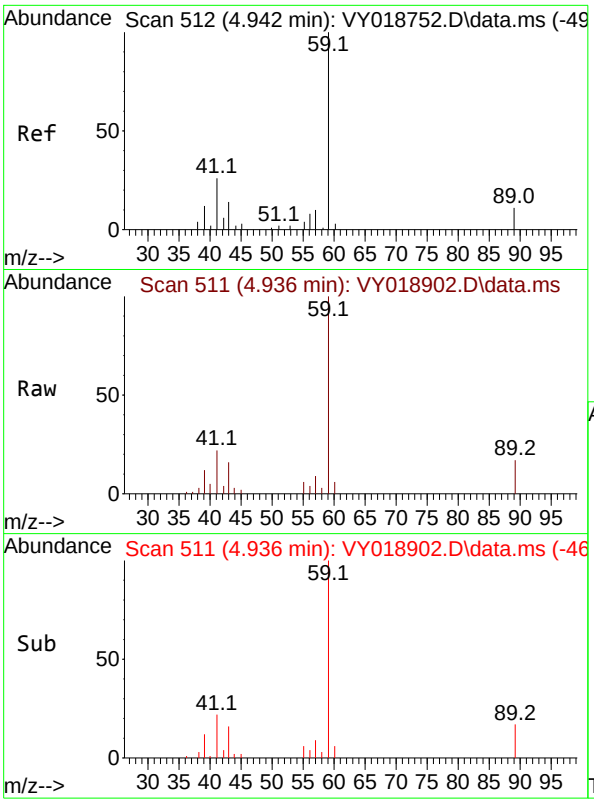

#11
Tert butyl alcohol
Concen: 169.815 ug/l
RT: 4.936 min Scan# 5
Delta R.T. -0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 59 Resp: 1775

Ion	Ratio	Lower	Upper
59	100		
57	9.7	3.0	4.6

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



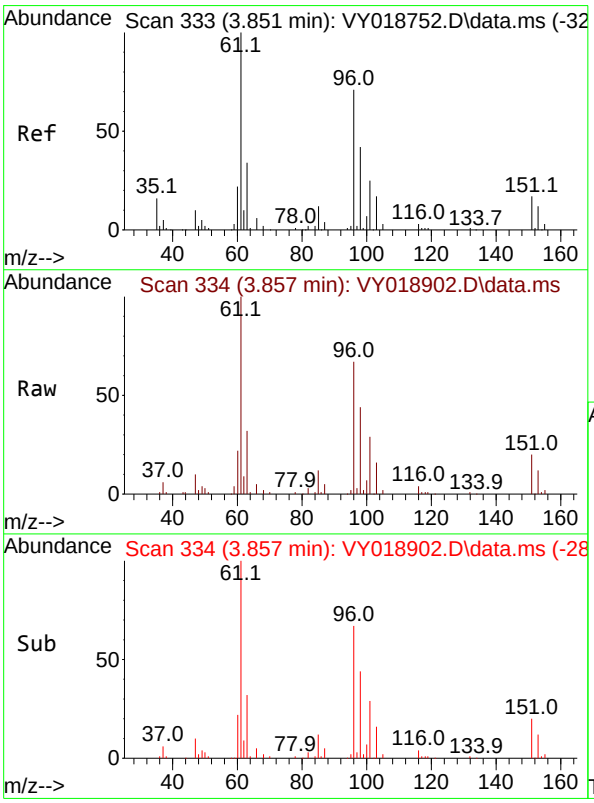

#12
1,1-Dichloroethene
Concen: 48.216 ug/l
RT: 3.857 min Scan# 334
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 96 Resp: 48852

Ion	Ratio	Lower	Upper
96	100		
61	149.2	114.6	171.8
98	66.2	50.8	76.2



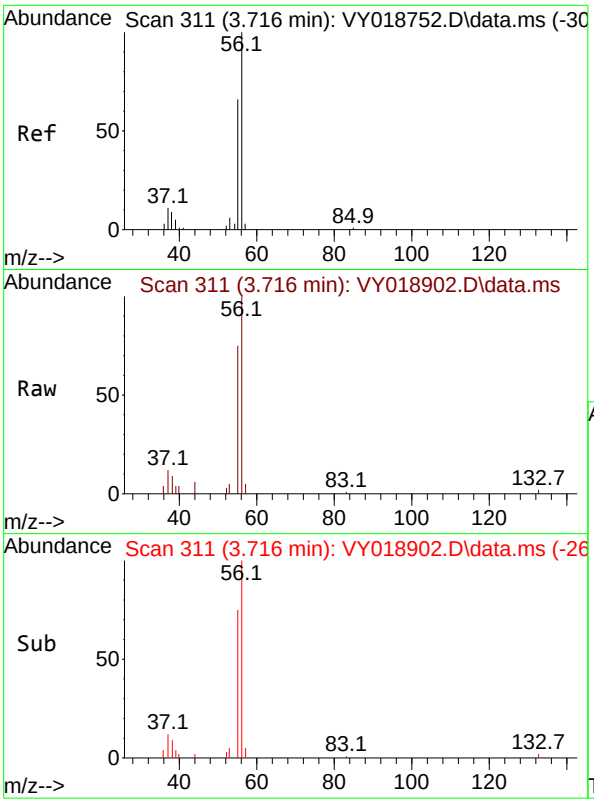

#13
Acrolein
Concen: 113.177 ug/l
RT: 3.716 min Scan# 3
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 56 Resp: 947

Ion	Ratio	Lower	Upper
56	100		
55	75.4	55.7	83.5



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

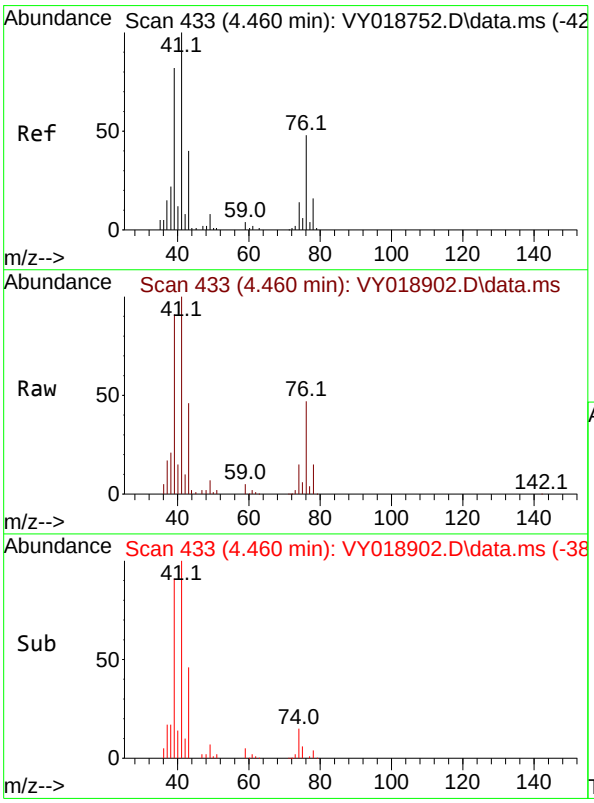

#14
Allyl chloride
Concen: 51.276 ug/l
RT: 4.460 min Scan# 433
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 41 Resp: 64362

Ion	Ratio	Lower	Upper
41	100		
39	79.8	58.3	87.5
76	46.1	39.0	58.6



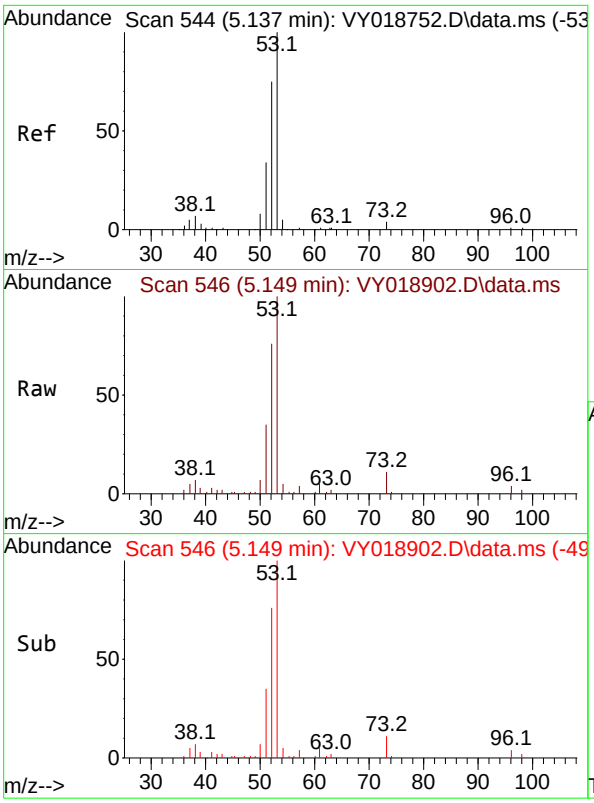

#15
Acrylonitrile
Concen: 250.067 ug/l
RT: 5.149 min Scan# 54
Delta R.T. 0.012 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 53 Resp: 4908

Ion	Ratio	Lower	Upper
53	100		
52	81.3	64.7	97.1
51	36.8	28.4	42.6

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



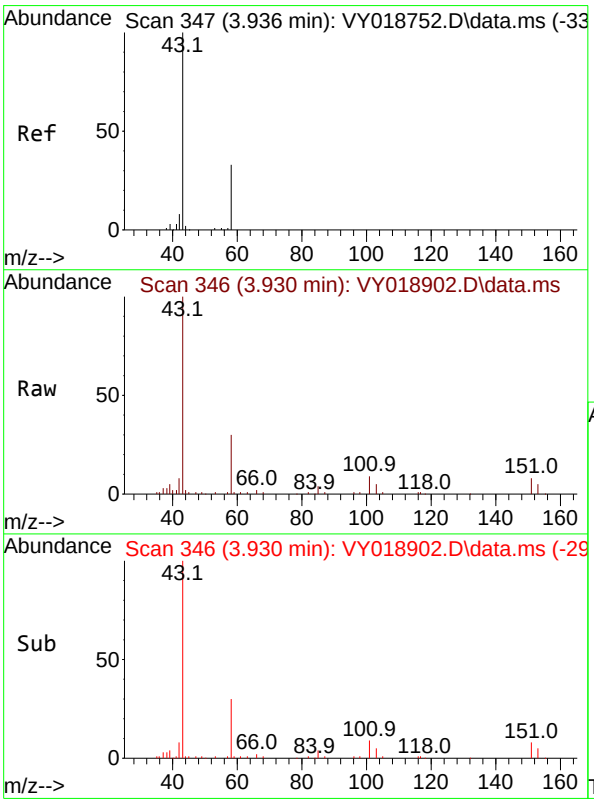

#16
Acetone
Concen: 273.284 ug/l
RT: 3.930 min Scan# 346
Delta R.T. -0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 51993

Ion	Ratio	Lower	Upper
43	100		
58	29.3	31.7	47.5#



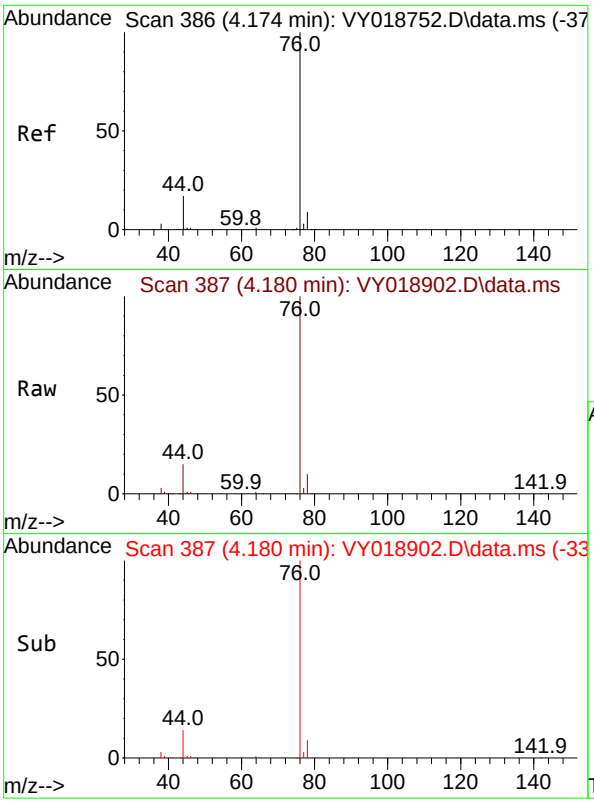

#17
Carbon Disulfide
Concen: 45.816 ug/l
RT: 4.180 min Scan# 3
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 76 Resp: 12998

Ion	Ratio	Lower	Upper
76	100		
78	9.8	6.8	10.2

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



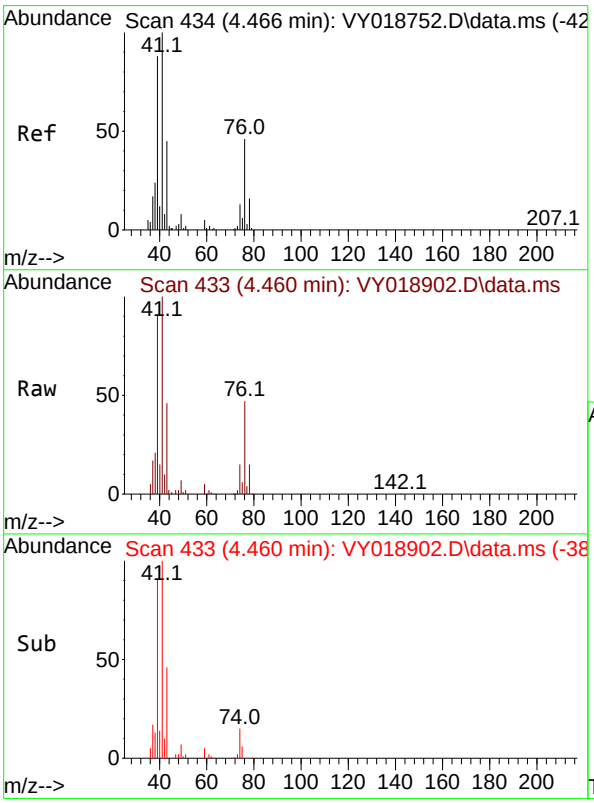

#18
Methyl Acetate
Concen: 49.783 ug/l
RT: 4.460 min Scan# 433
Delta R.T. -0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 27520

Ion	Ratio	Lower	Upper
43	100		
74	27.6	23.3	34.9



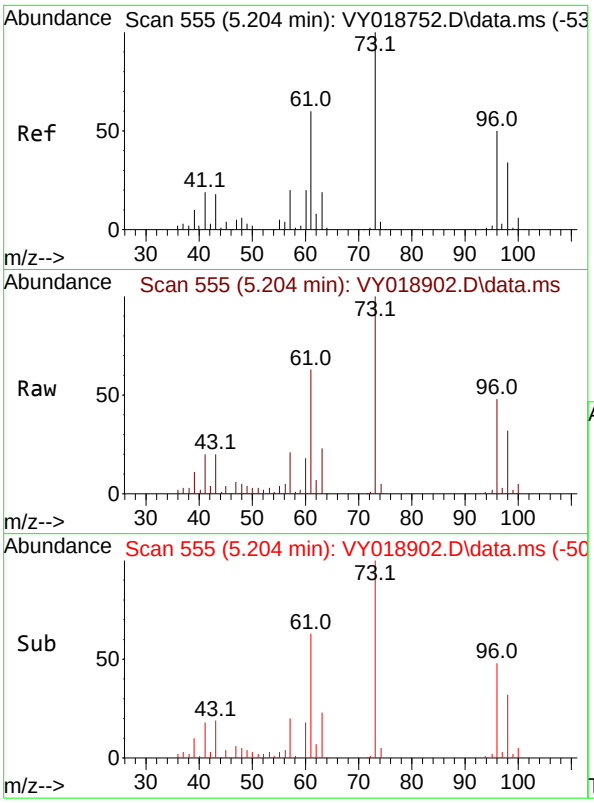

#19
Methyl tert-butyl Ether
Concen: 51.090 ug/l
RT: 5.204 min Scan# 5
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 73 Resp: 12008

Ion	Ratio	Lower	Upper
73	100		
57	20.7	17.3	25.9

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



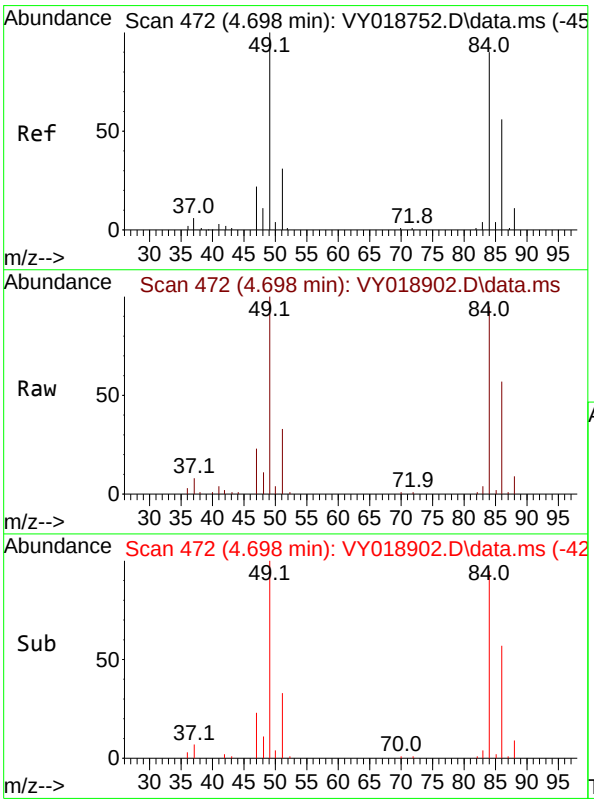

#20
Methylene Chloride
Concen: 56.359 ug/l
RT: 4.698 min Scan# 472
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 84 Resp: 60044

Ion	Ratio	Lower	Upper
84	100		
49	105.7	84.4	126.6
51	35.1	26.0	39.0
86	60.5	49.5	74.3



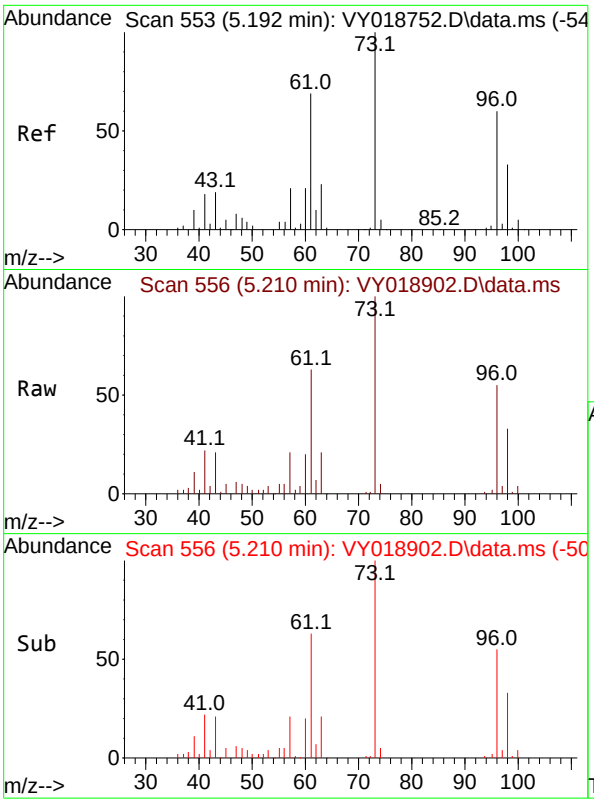

#21
trans-1,2-Dichloroethene
Concen: 49.079 ug/l
RT: 5.210 min Scan# 5
Delta R.T. 0.018 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 96 Resp: 5248

Ion	Ratio	Lower	Upper
96	100		
61	113.1	97.5	146.3
98	58.8	50.5	75.7



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

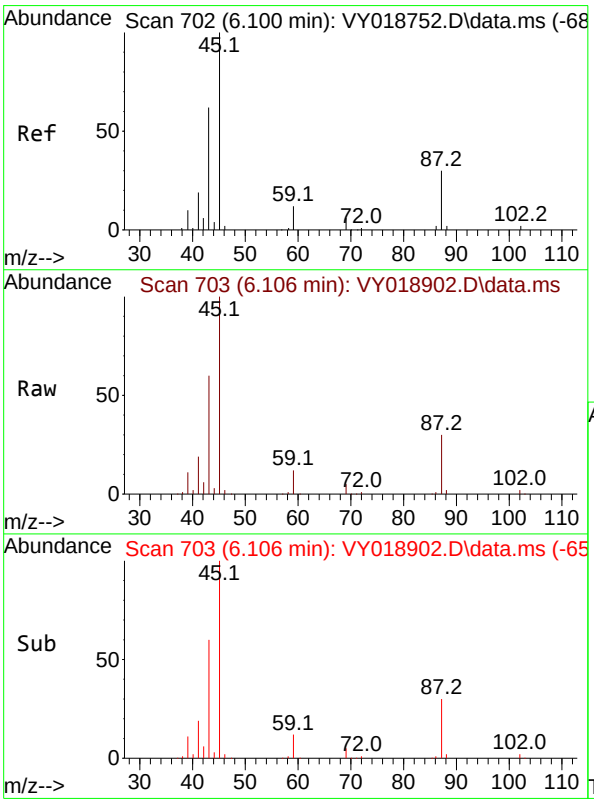

#22
Diisopropyl ether
Concen: 51.706 ug/l
RT: 6.106 min Scan# 703
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 45 Resp: 141176

Ion	Ratio	Lower	Upper
45	100		
43	59.4	42.2	63.2
87	30.1	25.0	37.6
59	12.4	10.5	15.7



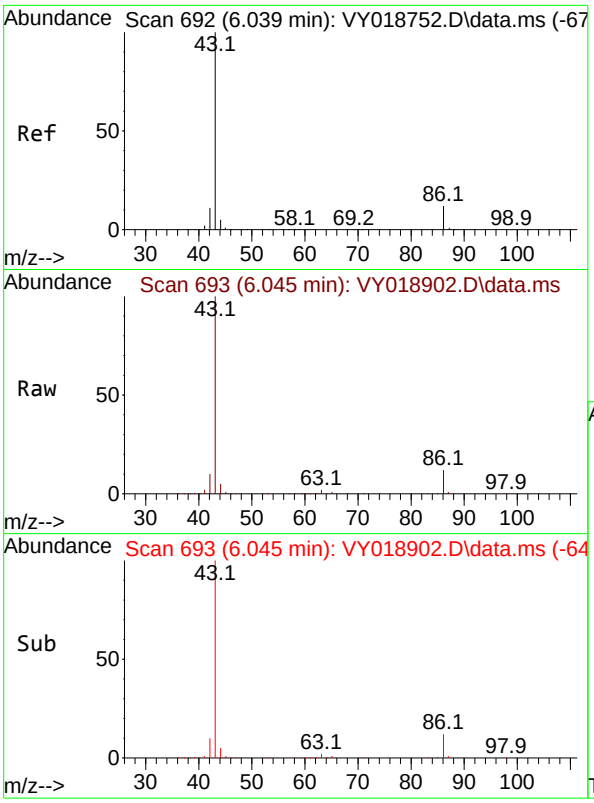

#23
Vinyl Acetate
Concen: 258.010 ug/l
RT: 6.045 min Scan# 6
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 55499

Ion	Ratio	Lower	Upper
43	100		
86	12.0	10.6	16.0

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



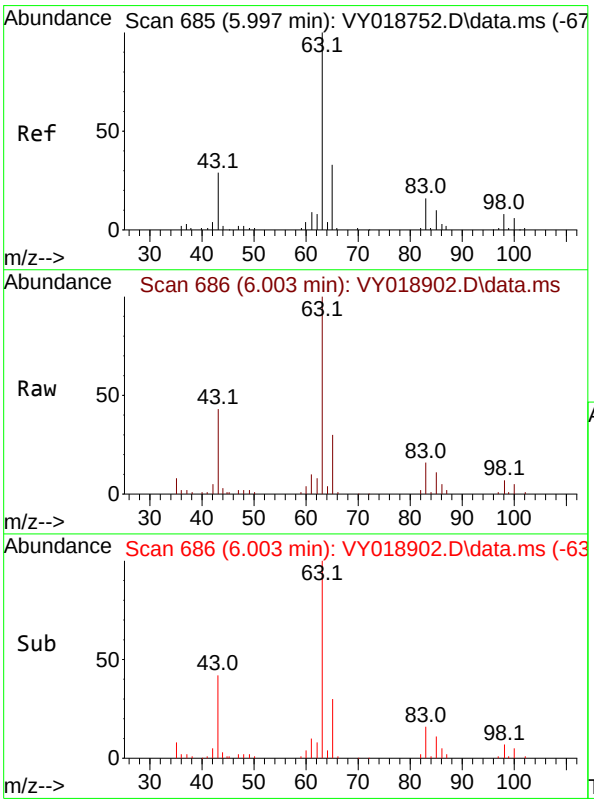

#24
1,1-Dichloroethane
Concen: 50.691 ug/l
RT: 6.003 min Scan# 686
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 63 Resp: 88368

Ion	Ratio	Lower	Upper
63	100		
98	7.3	4.0	12.2
100	5.3	2.6	8.0



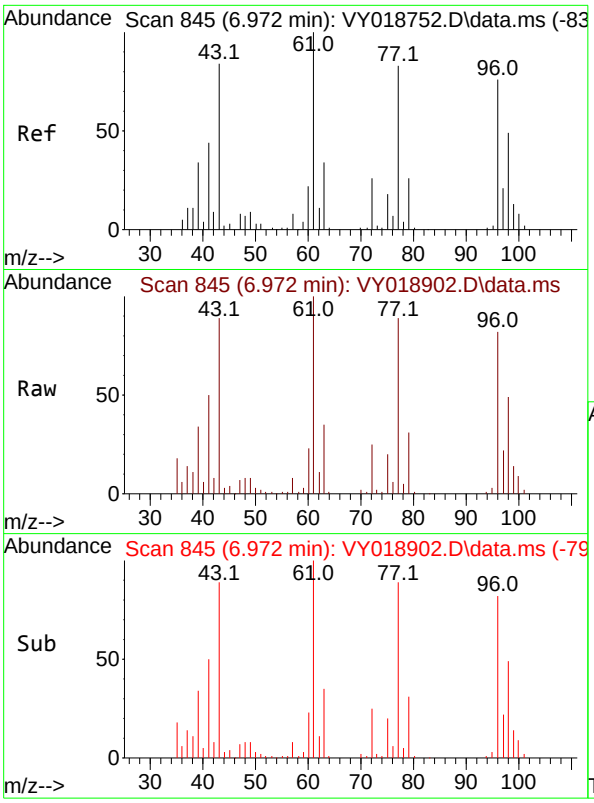

#25
2-Butanone
Concen: 256.182 ug/l
RT: 6.972 min Scan# 84
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 6831

Ion	Ratio	Lower	Upper
43	100		
72	28.3	27.3	40.9

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



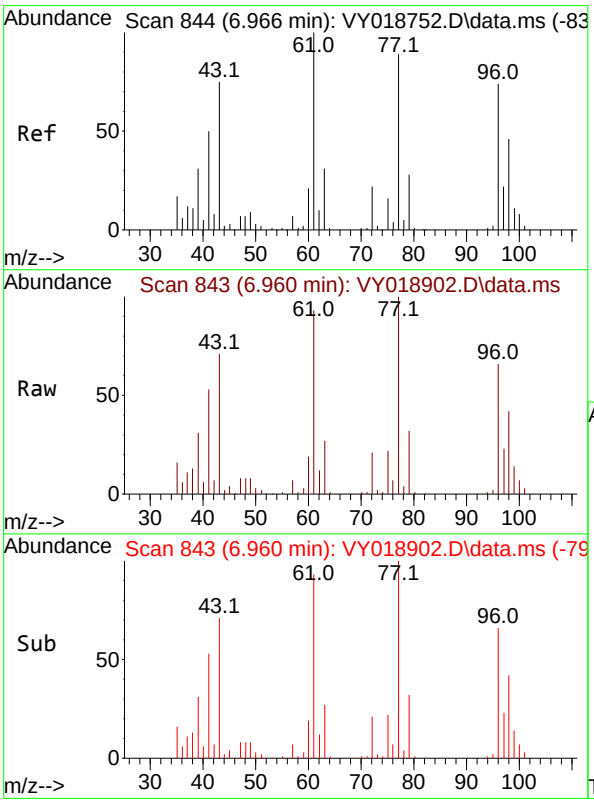

#26
2,2-Dichloropropane
Concen: 51.801 ug/l
RT: 6.960 min Scan# 843
Delta R.T. -0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 77 Resp: 83788

Ion	Ratio	Lower	Upper
77	100		
97	23.4	12.0	36.1



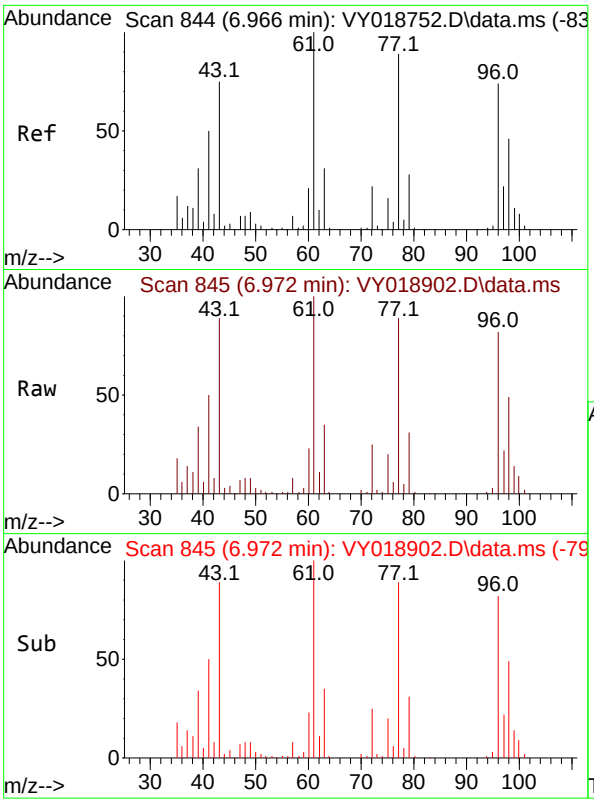

#27
cis-1,2-Dichloroethene
Concen: 51.054 ug/l
RT: 6.972 min Scan# 84
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 96 Resp: 6356

Ion	Ratio	Lower	Upper
96	100		
61	128.2	0.0	256.2
98	64.0	0.0	130.0

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



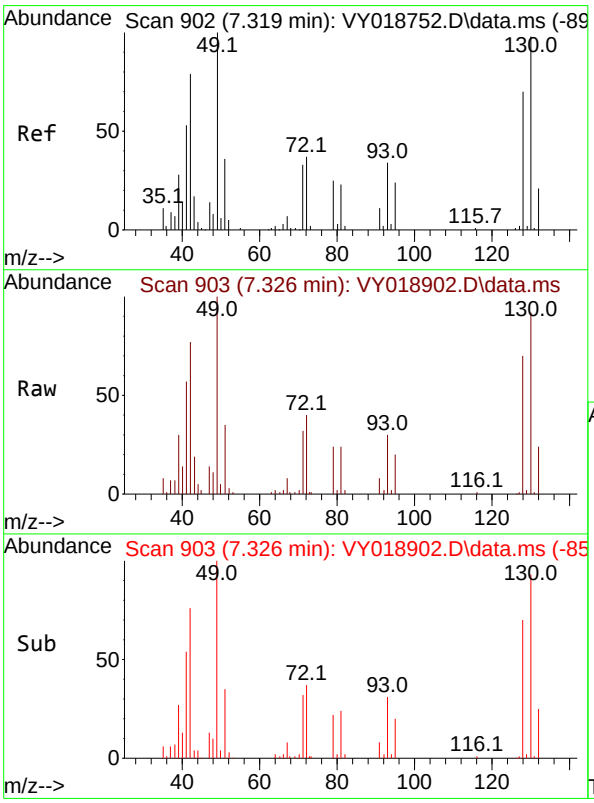

#28
Bromochloromethane
Concen: 51.643 ug/l
RT: 7.326 min Scan# 903
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 49 Resp: 36159

Ion	Ratio	Lower	Upper
49	100		
129	2.3	0.0	4.6
130	95.3	72.7	109.1



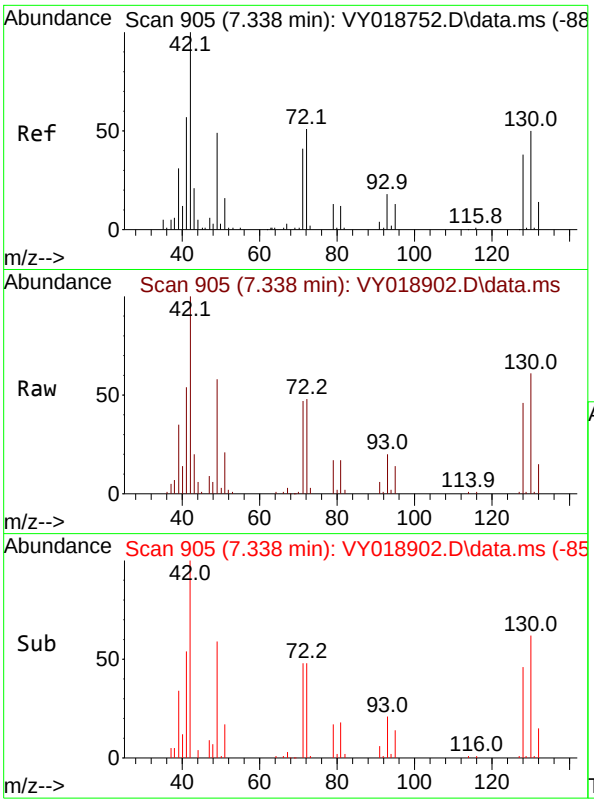

#29
Tetrahydrofuran
Concen: 250.911 ug/l
RT: 7.338 min Scan# 9
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 42 Resp: 4102

Ion	Ratio	Lower	Upper
42	100		
72	49.7	43.0	64.4
71	45.5	40.8	61.2

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



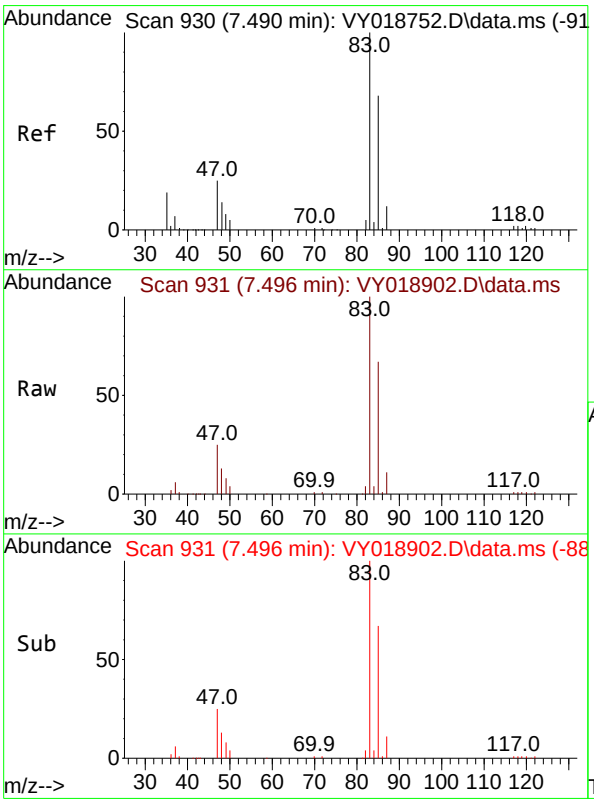

#30
Chloroform
Concen: 52.339 ug/l
RT: 7.496 min Scan# 931
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 83 Resp: 101689

Ion	Ratio	Lower	Upper
83	100		
85	66.6	52.2	78.4



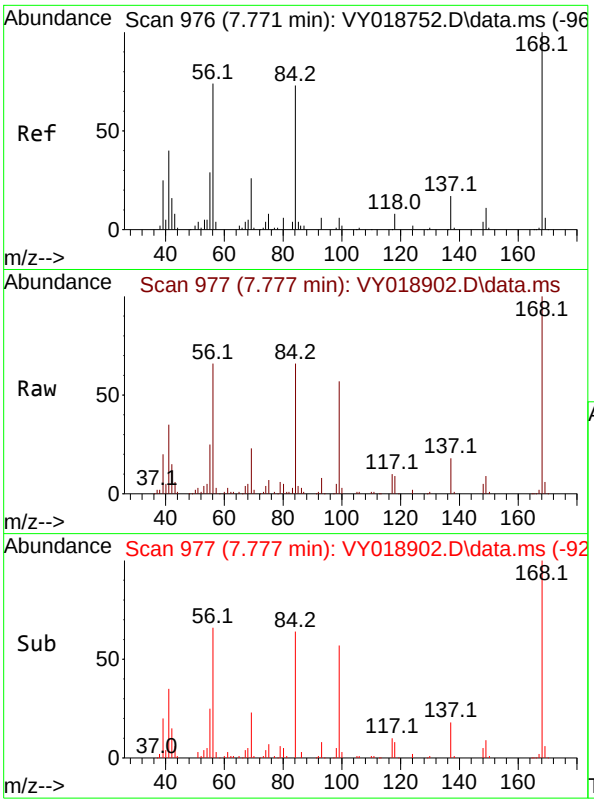

#31
Cyclohexane
Concen: 46.174 ug/l
RT: 7.777 min Scan# 9
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 56 Resp: 7320

Ion	Ratio	Lower	Upper
56	100		
69	35.0	28.7	43.1
84	98.4	77.7	116.5



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

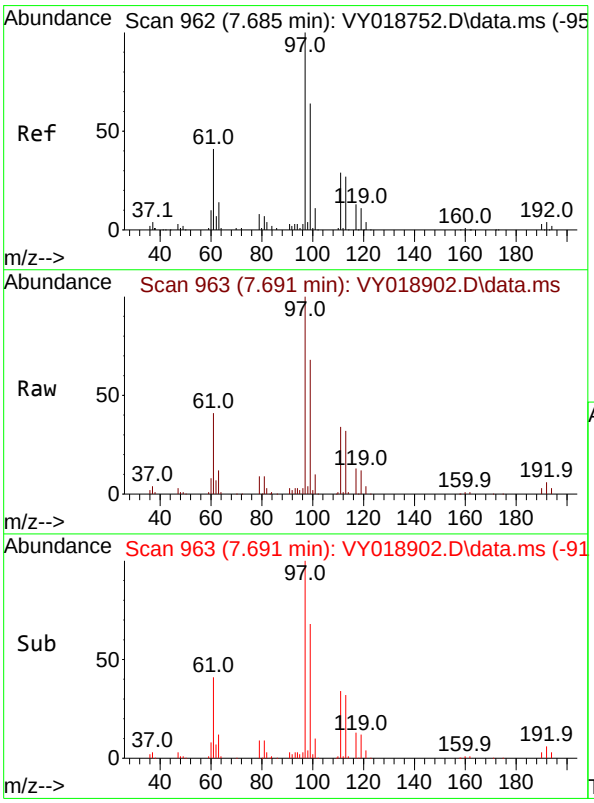

#32
1,1,1-Trichloroethane
Concen: 52.865 ug/l
RT: 7.691 min Scan# 963
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 97 Resp: 95510

Ion	Ratio	Lower	Upper
97	100		
99	64.1	50.3	75.5
61	41.5	32.6	48.8



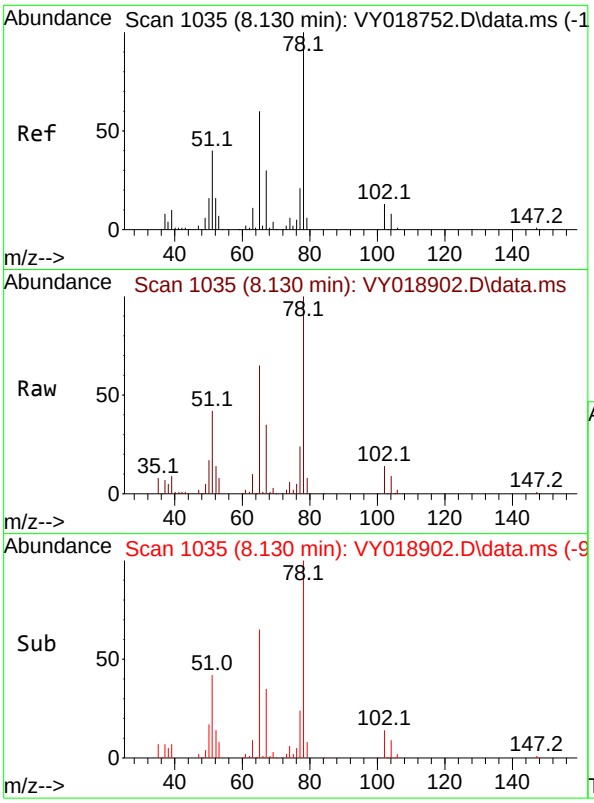

#33
1,2-Dichloroethane-d4
Concen: 45.027 ug/l
RT: 8.130 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 65 Resp: 4646

Ion	Ratio	Lower	Upper
65	100		
67	50.3	0.0	109.6



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

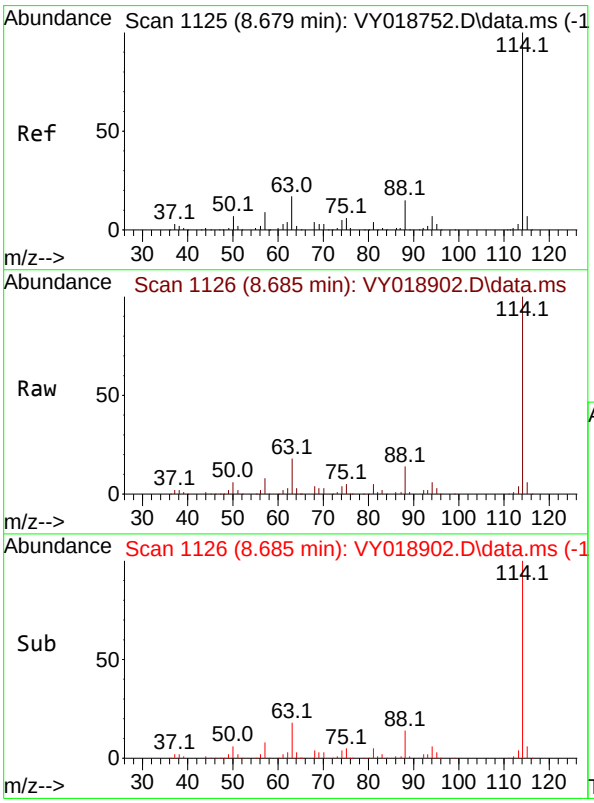

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:114 Resp: 158102

Ion	Ratio	Lower	Upper
114	100		
63	17.8	0.0	35.0
88	14.2	0.0	27.2



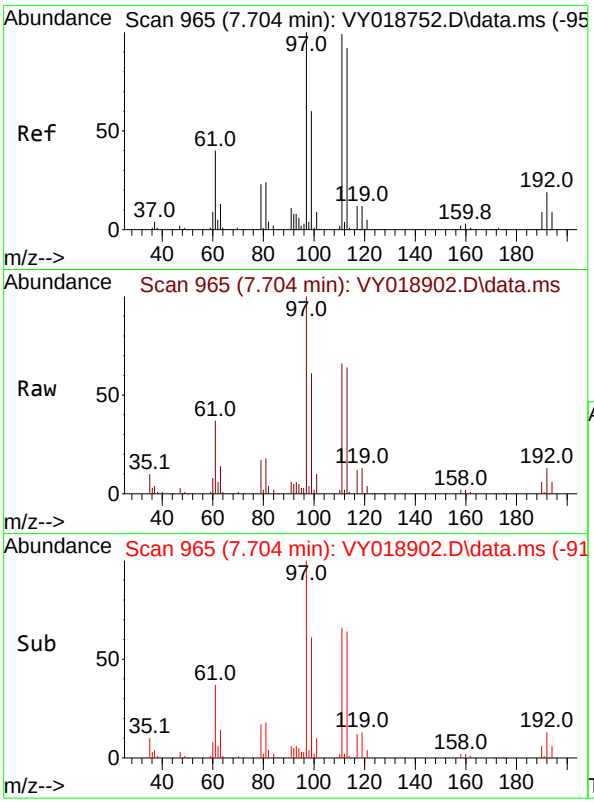

#35
Dibromofluoromethane
Concen: 49.297 ug/l
RT: 7.704 min Scan# 9
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:113 Resp: 4881

Ion	Ratio	Lower	Upper
113	100		
111	103.3	82.2	123.4
192	20.5	15.9	23.9



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

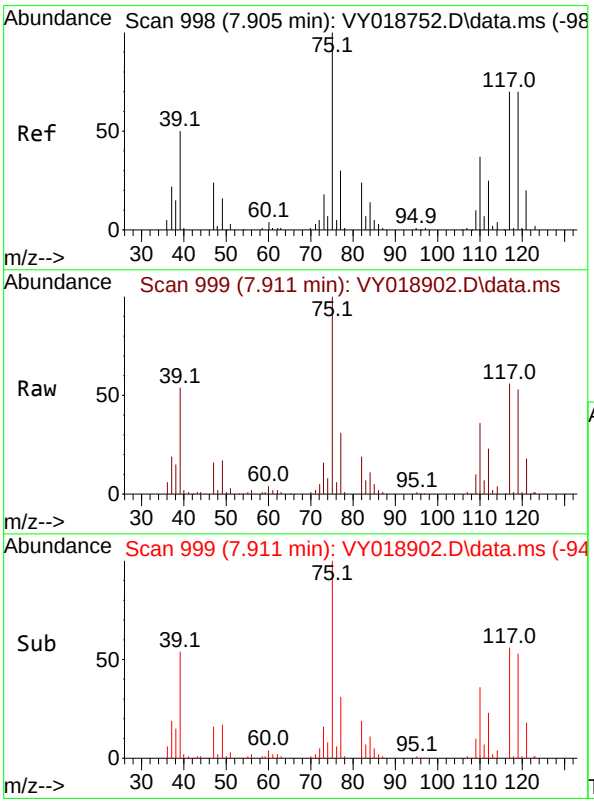

#36
1,1-Dichloropropene
Concen: 51.656 ug/l
RT: 7.911 min Scan# 999
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 75 Resp: 70590

Ion	Ratio	Lower	Upper
75	100		
110	36.9	19.0	57.0
77	30.5	25.3	37.9



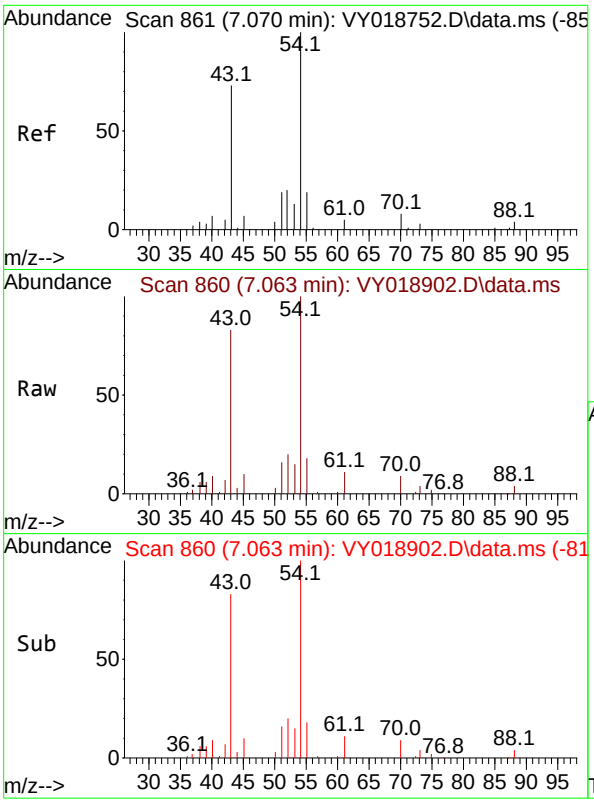

#37
Ethyl Acetate
Concen: 53.965 ug/l
RT: 7.063 min Scan# 8
Delta R.T. -0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 3065

Ion	Ratio	Lower	Upper
43	100		
61	13.3	12.6	19.0
70	10.7	7.8	11.8

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



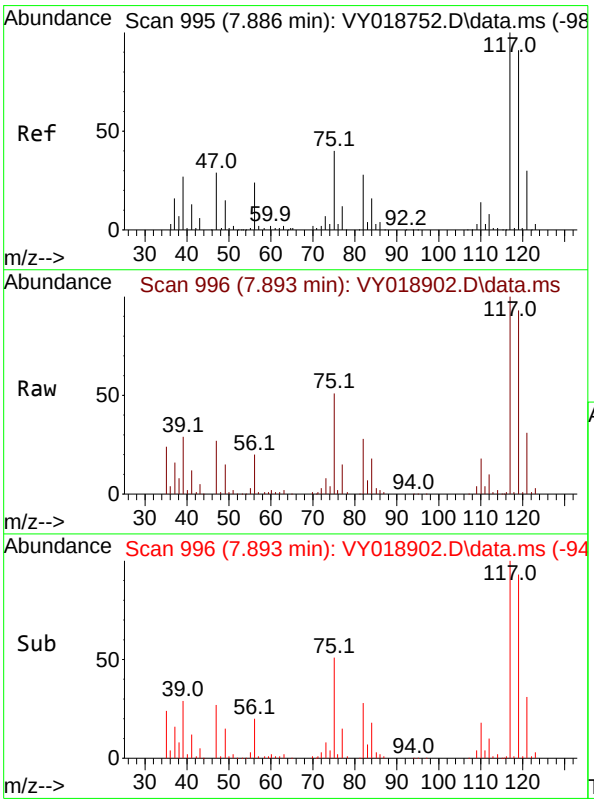

#38
Carbon Tetrachloride
Concen: 54.470 ug/l
RT: 7.893 min Scan# 996
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:117 Resp: 89652

Ion	Ratio	Lower	Upper
117	100		
119	93.4	75.8	113.6
121	31.0	24.0	36.0



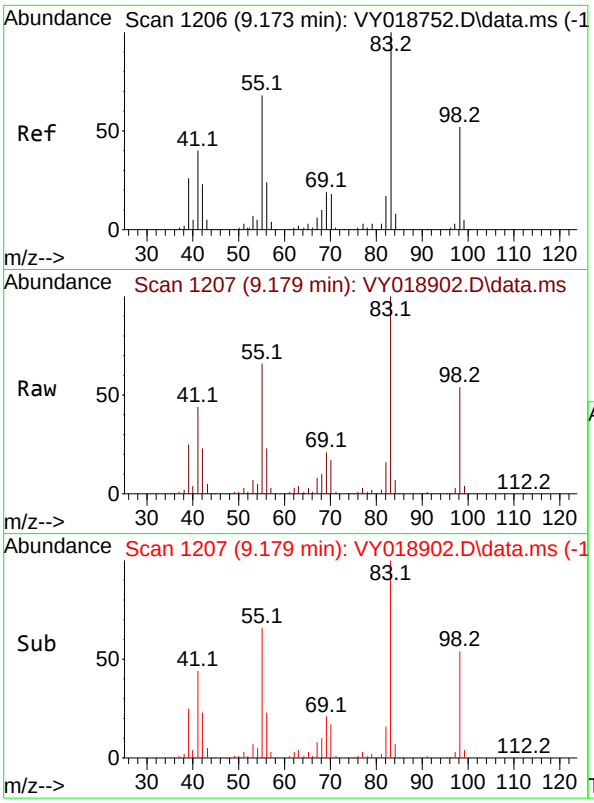

#39
Methylcyclohexane
Concen: 51.377 ug/l
RT: 9.179 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 83 Resp: 8997

Ion	Ratio	Lower	Upper
83	100		
55	66.1	51.5	77.3
98	53.9	40.5	60.7

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



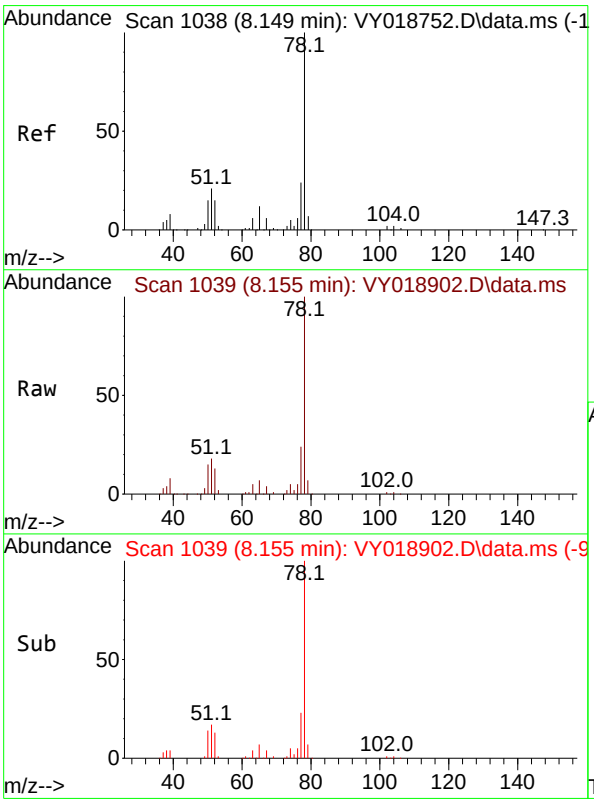

#40
Benzene
Concen: 52.539 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 78 Resp: 208276

Ion	Ratio	Lower	Upper
78	100		
77	23.6	19.5	29.3



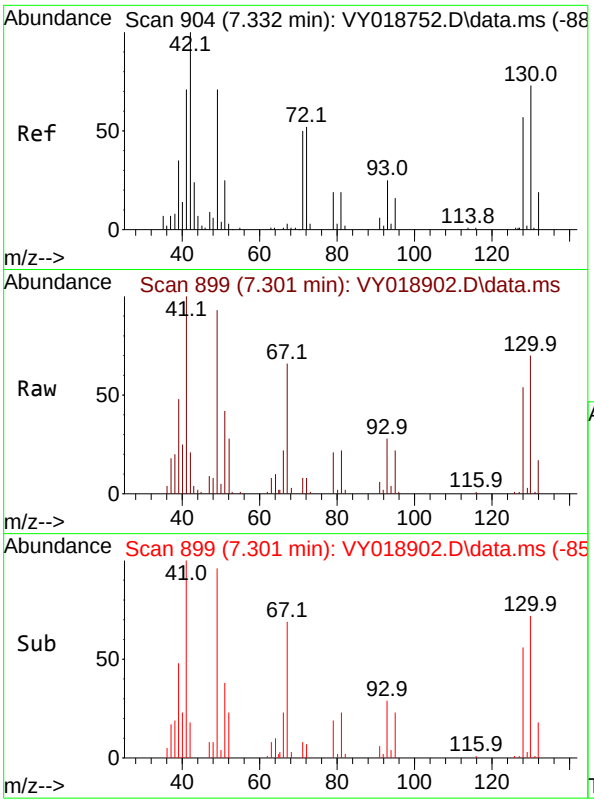

#41
Methacrylonitrile
Concen: 53.776 ug/l
RT: 7.301 min Scan# 8
Delta R.T. -0.031 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 41 Resp: 1741

Ion	Ratio	Lower	Upper
41	100		
39	52.5	48.0	72.0
67	79.5	75.1	112.7
52	32.8	29.8	44.6



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

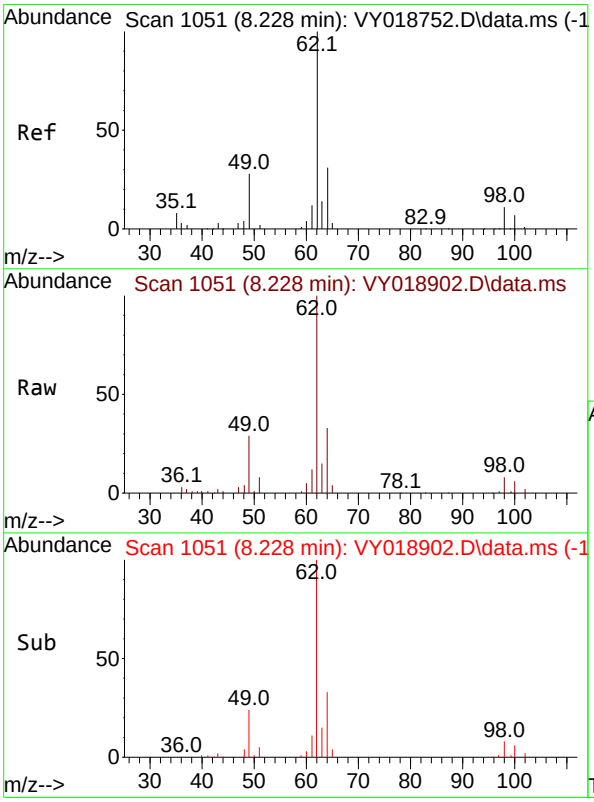

#42
1,2-Dichloroethane
Concen: 52.770 ug/l
RT: 8.228 min Scan# 1051
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 62 Resp: 58569

Ion	Ratio	Lower	Upper
62	100		
98	9.7	0.0	22.0



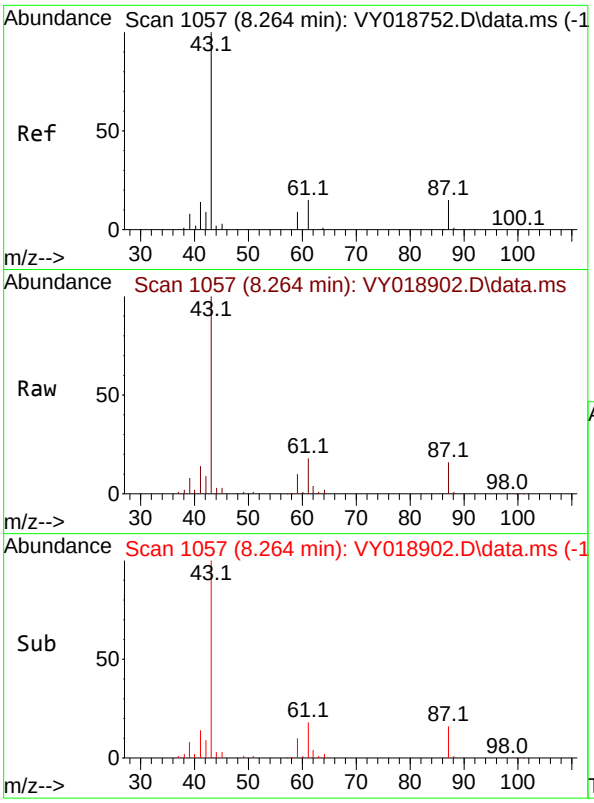

#43
Isopropyl Acetate
Concen: 51.498 ug/l
RT: 8.264 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 5820

Ion	Ratio	Lower	Upper
43	100		
61	19.8	27.9	41.9#
87	15.3	13.1	19.7

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



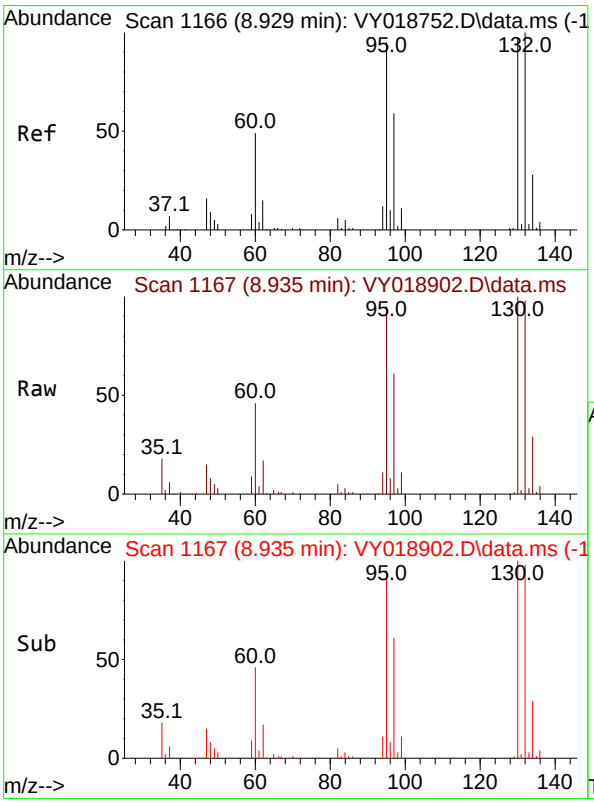

#44
Trichloroethene
Concen: 54.456 ug/l
RT: 8.935 min Scan# 1167
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:130 Resp: 61707

Ion	Ratio	Lower	Upper
130	100		
95	94.7	0.0	188.0



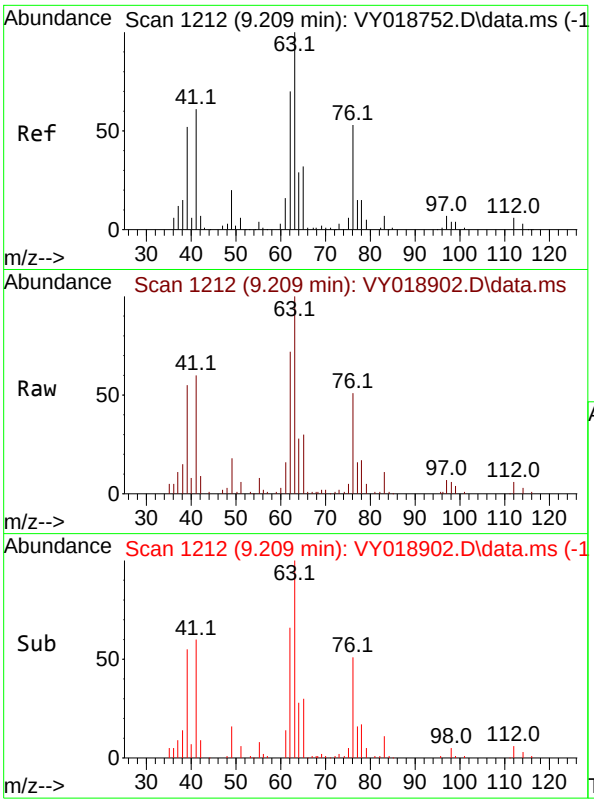

#45
1,2-Dichloropropane
Concen: 53.620 ug/l
RT: 9.209 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 63 Resp: 4628

Ion	Ratio	Lower	Upper
63	100		
65	30.1	25.4	38.2

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



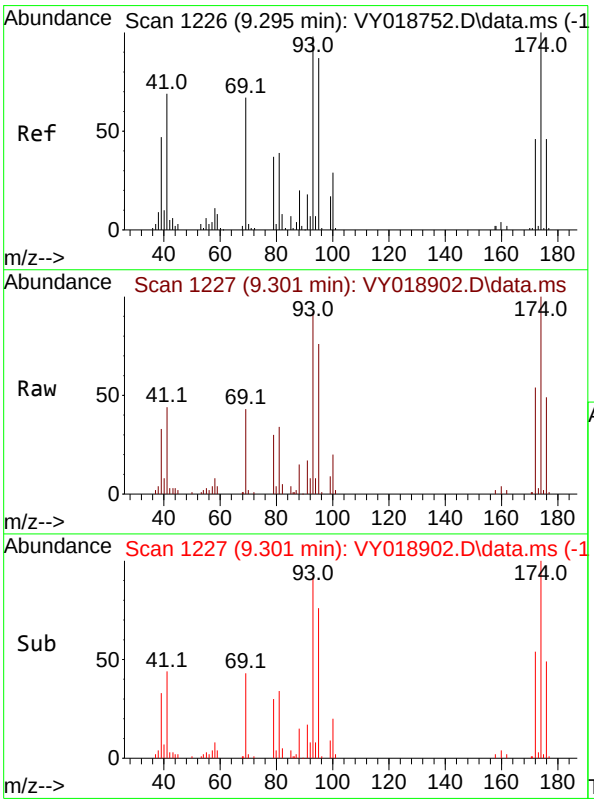

#46
Dibromomethane
Concen: 54.281 ug/l
RT: 9.301 min Scan# 1227
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 93 Resp: 30373

Ion	Ratio	Lower	Upper
93	100		
95	81.8	66.2	99.4
174	105.6	80.9	121.3



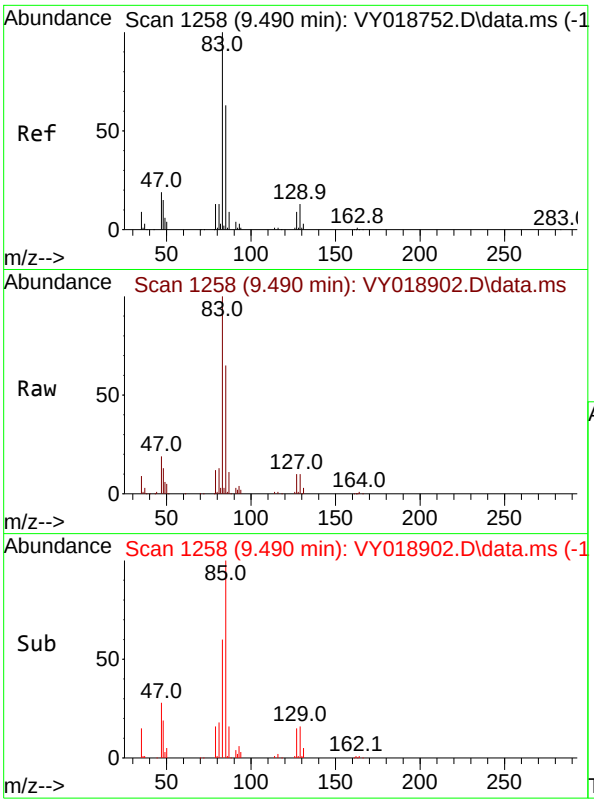

#47
Bromodichloromethane
Concen: 55.795 ug/l
RT: 9.490 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 83 Resp: 7799

Ion	Ratio	Lower	Upper
83	100		
85	65.1	50.1	75.1
127	9.7	7.4	11.0



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

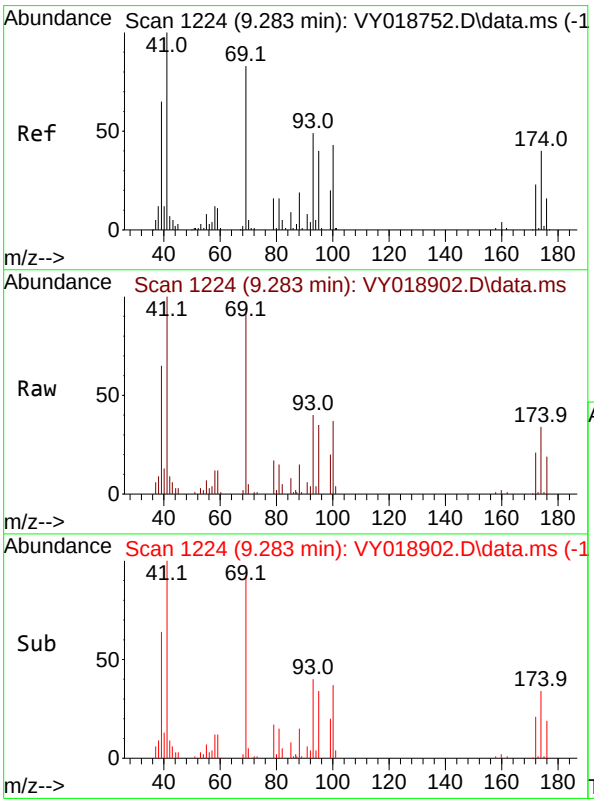

#48
Methyl methacrylate
Concen: 52.303 ug/l
RT: 9.283 min Scan# 1224
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 41 Resp: 26870

Ion	Ratio	Lower	Upper
41	100		
69	95.1	84.1	126.1
39	62.8	43.6	65.4



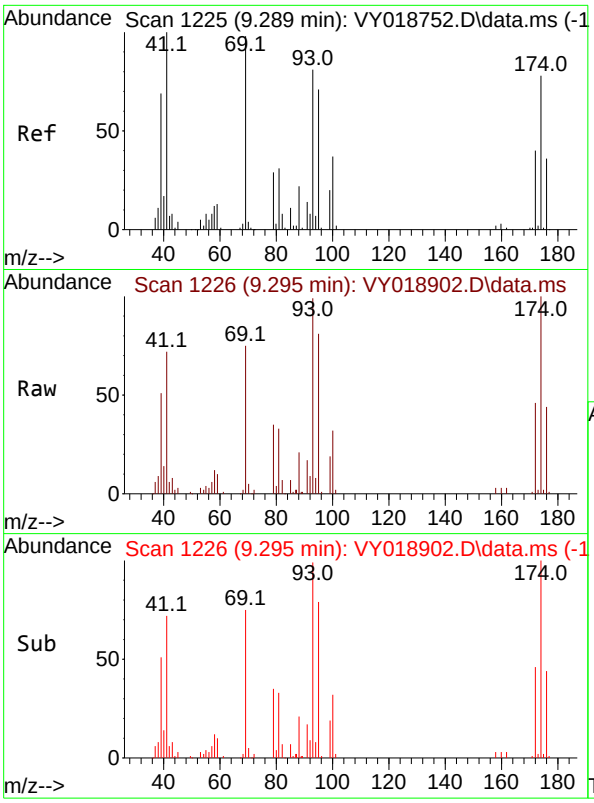

#49
1,4-Dioxane
Concen: 1061.415 ug/l
RT: 9.295 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 88 Resp: 696

Ion	Ratio	Lower	Upper
88	100		
43	31.0	0.0	0.0
58	56.2	49.3	73.9



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

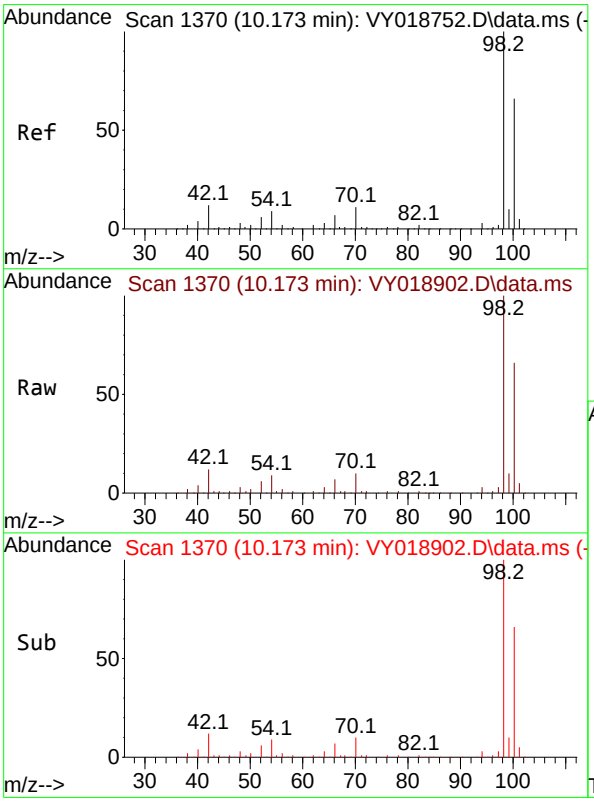

#50
Toluene-d8
Concen: 46.298 ug/l
RT: 10.173 min Scan# 1370
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 98 Resp: 173691

Ion	Ratio	Lower	Upper
98	100		
100	66.5	52.0	78.0



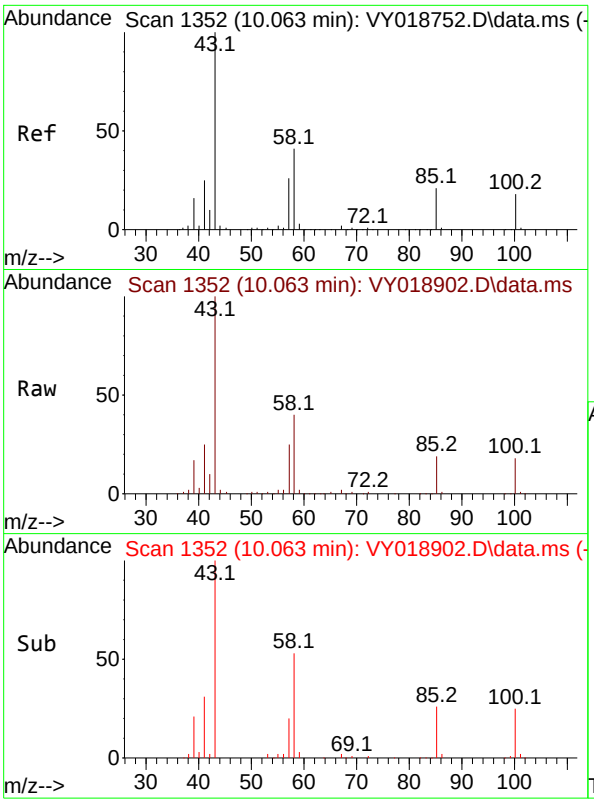

#51
4-Methyl-2-Pentanone
Concen: 260.499 ug/l
RT: 10.063 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 15032

Ion	Ratio	Lower	Upper
43	100		
58	39.7	35.7	53.5

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



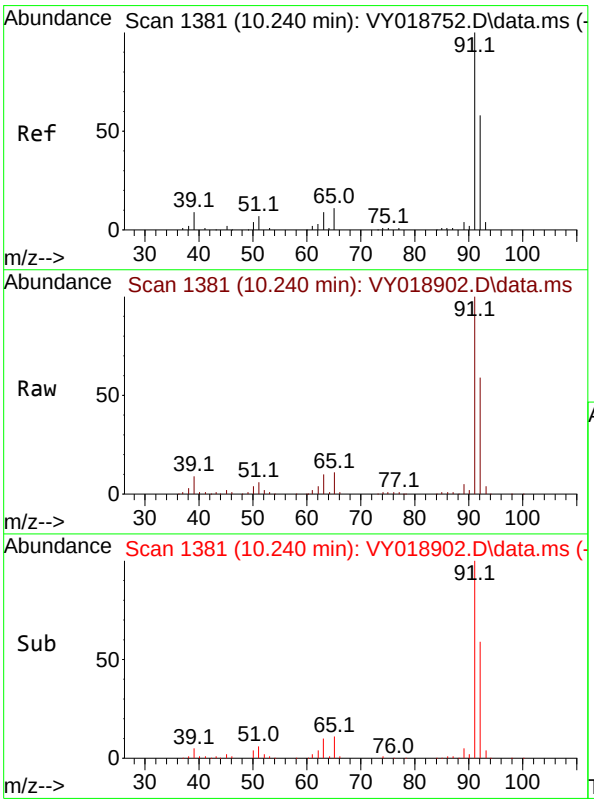

#52
Toluene
Concen: 50.596 ug/l
RT: 10.240 min Scan# 1381
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 92 Resp: 133313

Ion	Ratio	Lower	Upper
92	100		
91	173.8	139.0	208.6



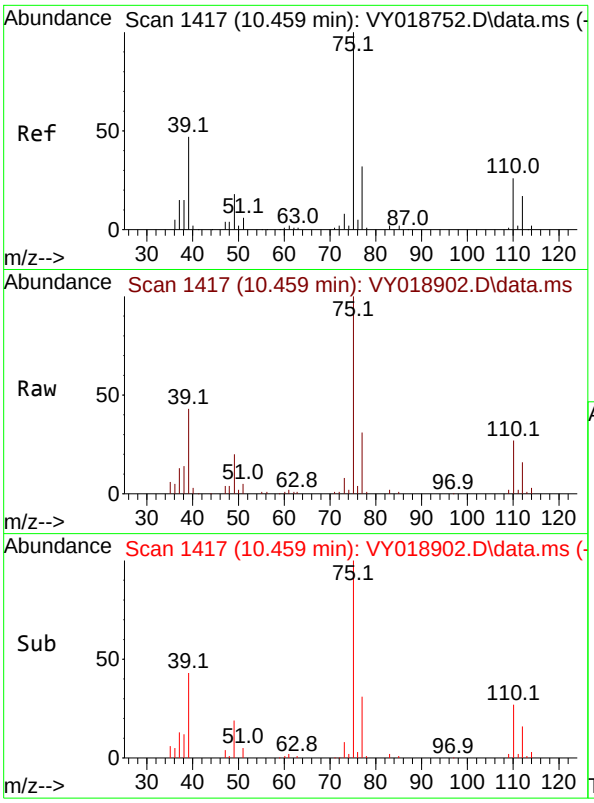

#53
t-1,3-Dichloropropene
Concen: 54.643 ug/l
RT: 10.459 min Scan# 14
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 75 Resp: 6594

Ion	Ratio	Lower	Upper
75	100		
77	31.3	24.1	36.1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



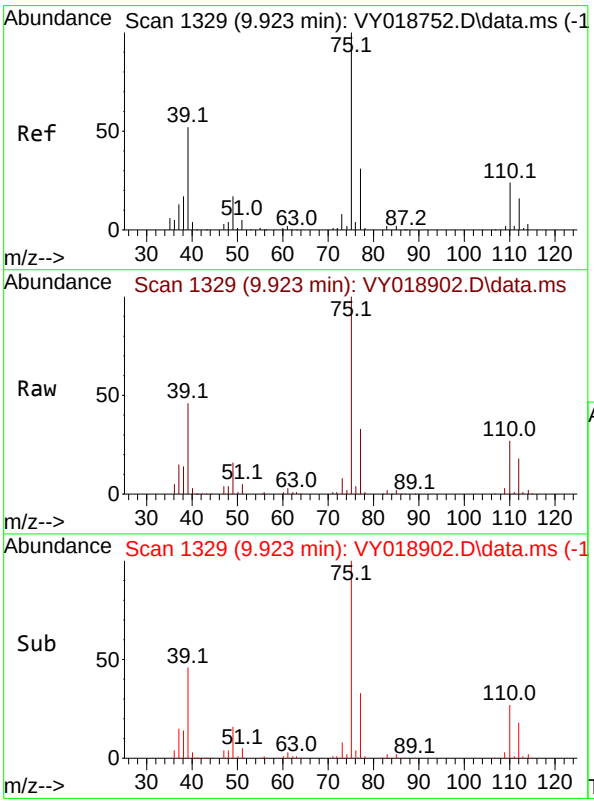

#54
cis-1,3-Dichloropropene
Concen: 54.928 ug/l
RT: 9.923 min Scan# 1329
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 75 Resp: 77772

Ion	Ratio	Lower	Upper
75	100		
77	33.3	25.4	38.0
39	46.4	29.8	44.6#



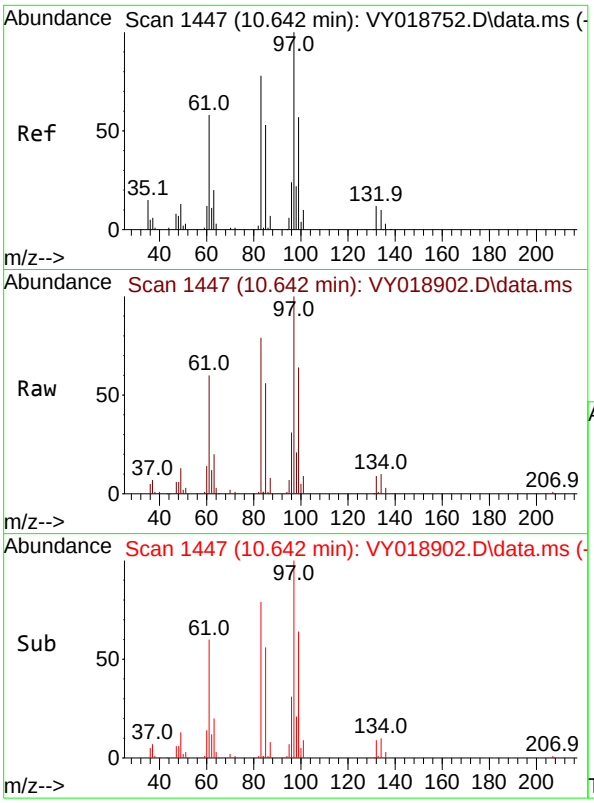

#55
1,1,2-Trichloroethane
Concen: 54.317 ug/l
RT: 10.642 min Scan# 14
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 97 Resp: 3848

Ion	Ratio	Lower	Upper
97	100		
83	78.7	67.5	101.3
85	56.1	42.9	64.3
99	64.5	46.6	70.0



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

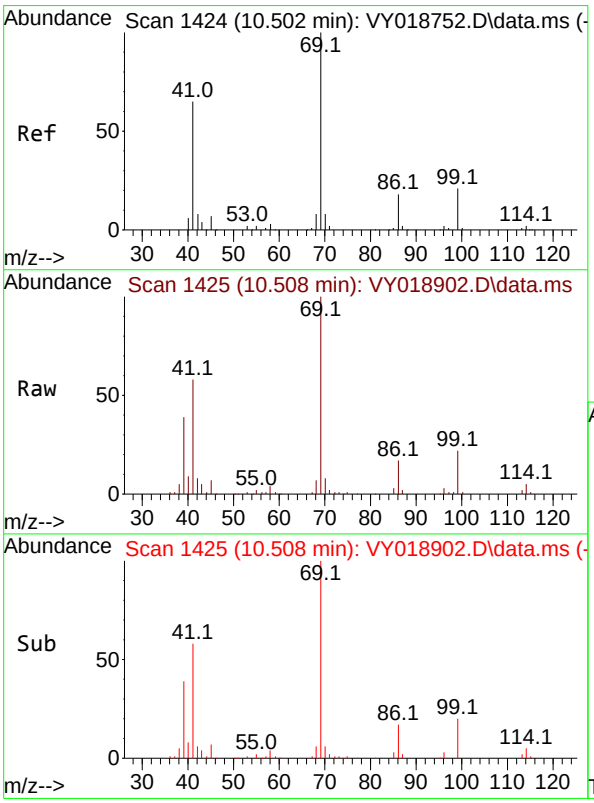

#56
Ethyl methacrylate
Concen: 53.230 ug/l
RT: 10.508 min Scan# 1425
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 69 Resp: 49657

Ion	Ratio	Lower	Upper
69	100		
41	61.9	42.3	63.5
39	39.3	22.9	34.3#



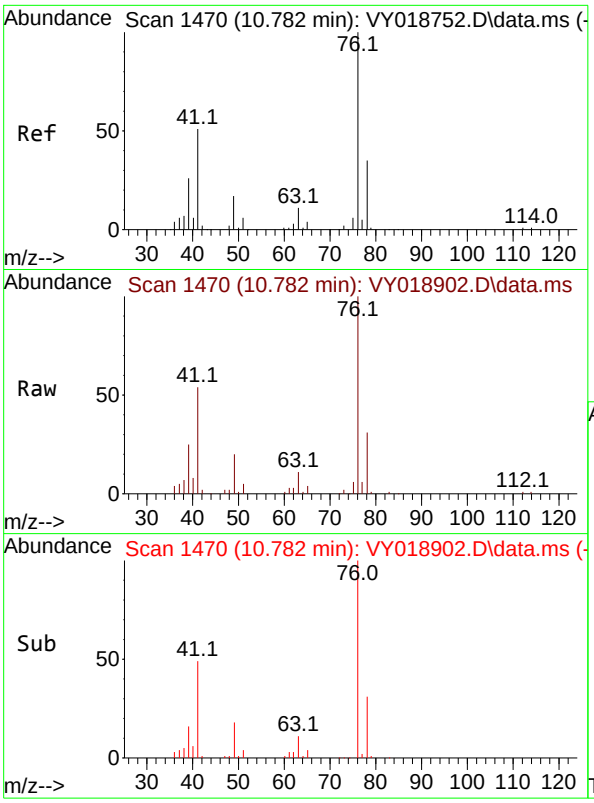

#57
1,3-Dichloropropane
Concen: 53.381 ug/l
RT: 10.782 min Scan# 14
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 76 Resp: 6270

Ion	Ratio	Lower	Upper
76	100		
78	32.4	26.2	39.4

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



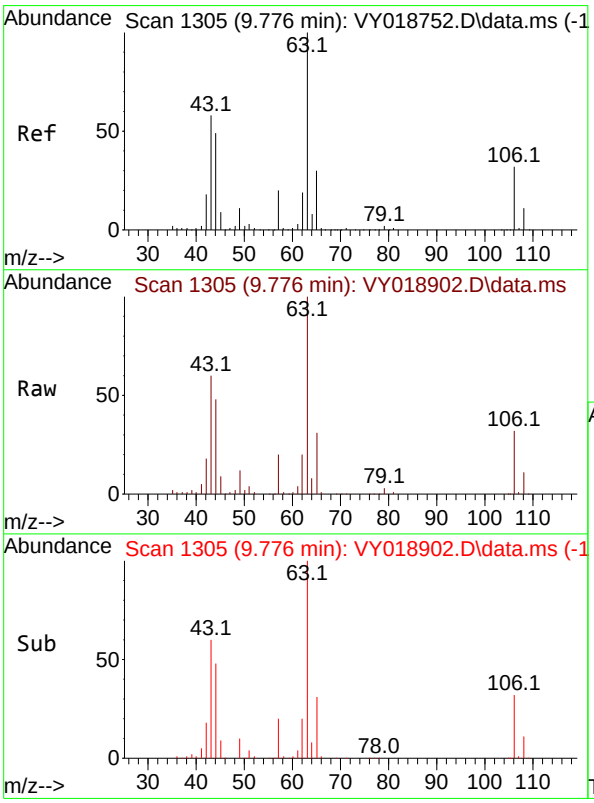

#58
2-Chloroethyl Vinyl ether
Concen: 268.145 ug/l
RT: 9.776 min Scan# 1305
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 63 Resp: 119507

Ion	Ratio	Lower	Upper
63	100		
106	33.5	23.7	35.5



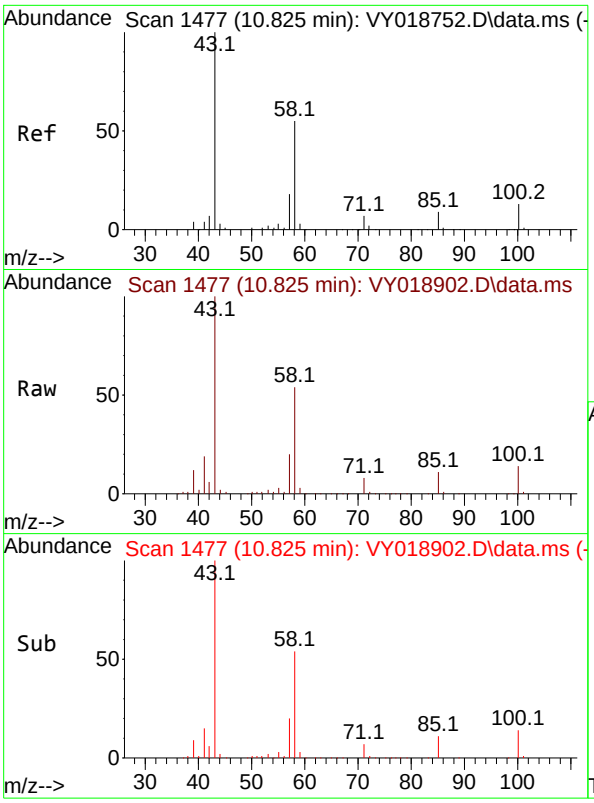

#59
2-Hexanone
Concen: 265.300 ug/l
RT: 10.825 min Scan# 14
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 10710

Ion	Ratio	Lower	Upper
43	100		
58	55.0	31.4	94.0

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



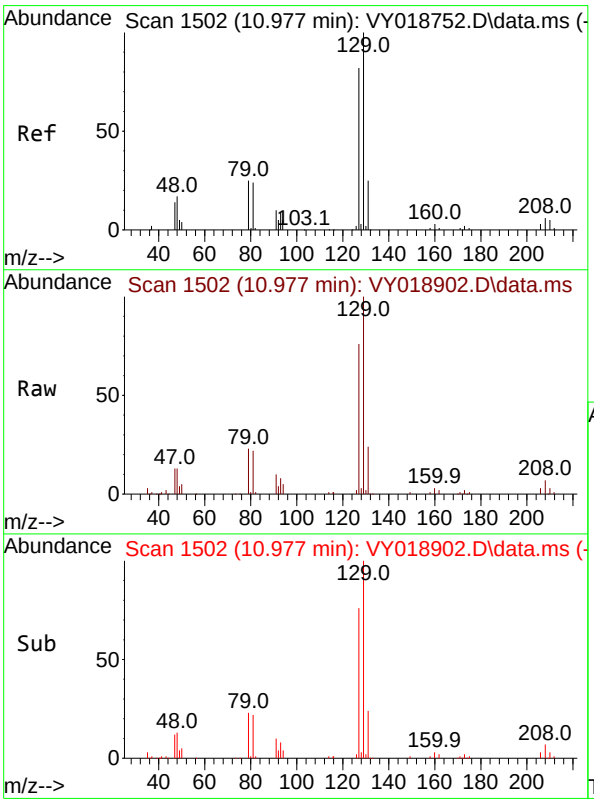

#60
Dibromochloromethane
Concen: 56.121 ug/l
RT: 10.977 min Scan# 1502
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:129 Resp: 54637

Ion	Ratio	Lower	Upper
129	100		
127	76.8	39.0	117.0



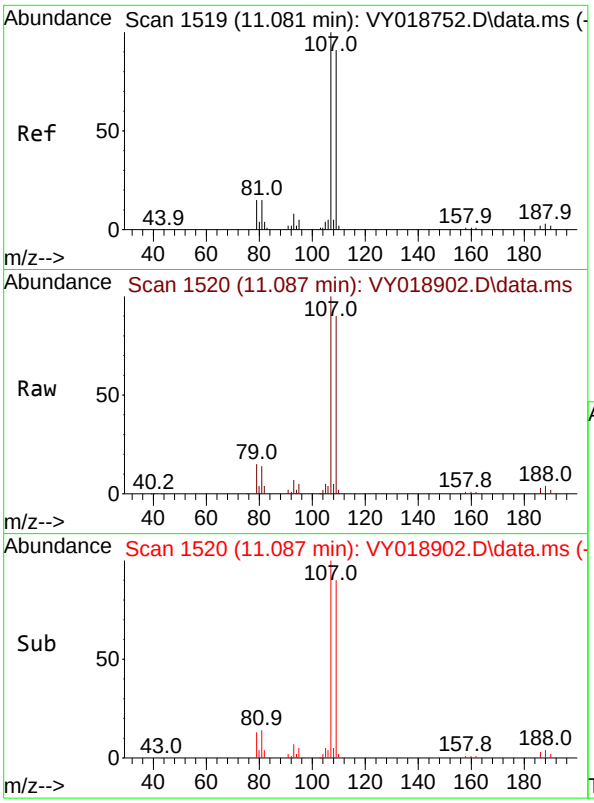

#61
1,2-Dibromoethane
Concen: 52.272 ug/l
RT: 11.087 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:107 Resp: 3600

Ion	Ratio	Lower	Upper
107	100		
109	92.9	75.9	113.9

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



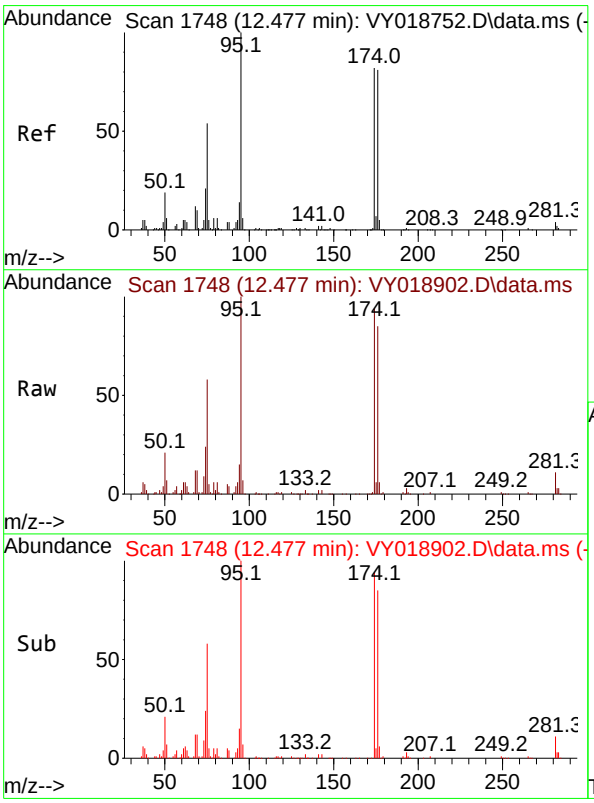

#62
4-Bromofluorobenzene
Concen: 45.935 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 95 Resp: 58851

Ion	Ratio	Lower	Upper
95	100		
174	95.6	0.0	175.6
176	89.6	0.0	171.4



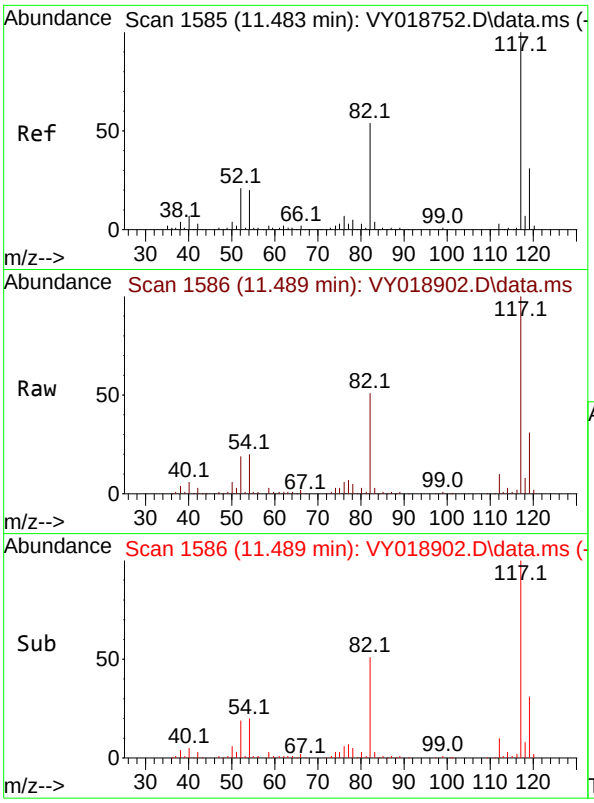

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:117 Resp: 13641

Ion	Ratio	Lower	Upper
117	100		
82	51.0	42.4	63.6
119	31.1	25.9	38.9



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

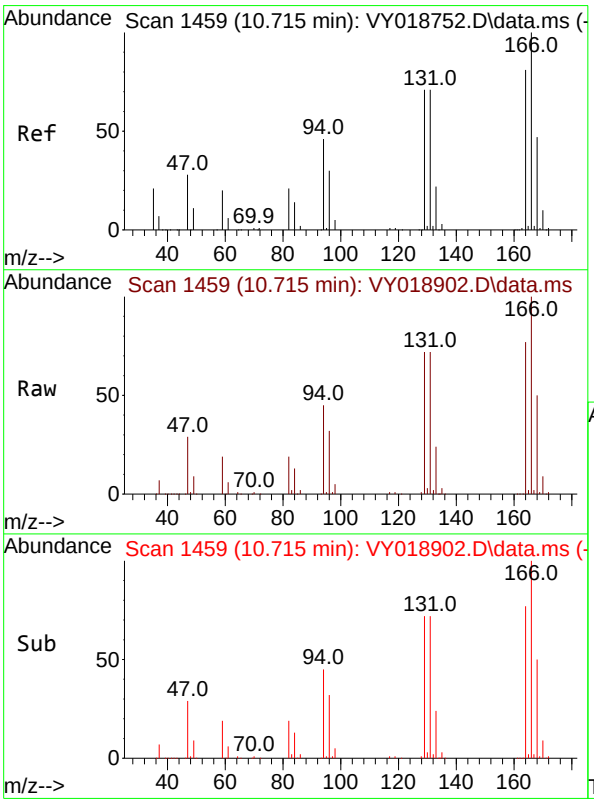

#64
Tetrachloroethene
Concen: 54.783 ug/l
RT: 10.715 min Scan# 1459
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:164 Resp: 60492

Ion	Ratio	Lower	Upper
164	100		
166	129.7	102.6	154.0
129	93.9	72.0	108.0
131	92.8	70.0	105.0



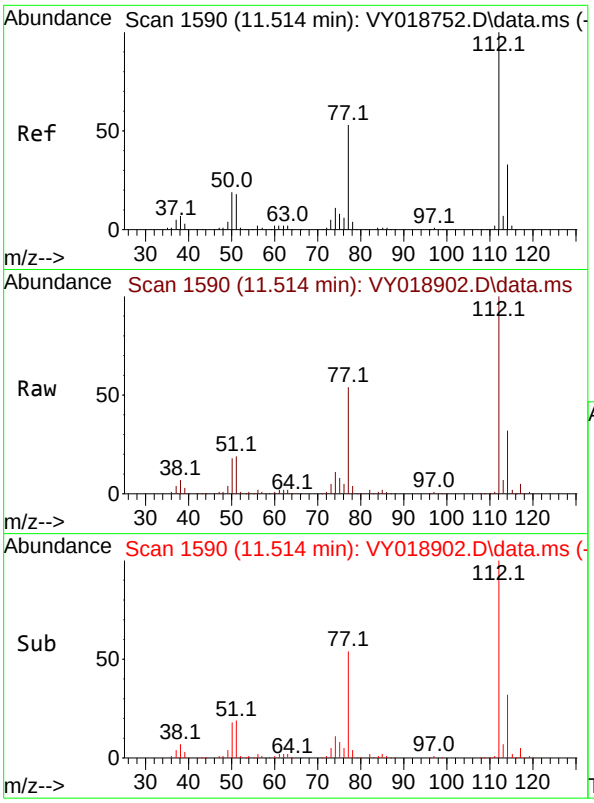

#65
Chlorobenzene
Concen: 54.609 ug/l
RT: 11.514 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:112 Resp: 15715

Ion	Ratio	Lower	Upper
112	100		
114	32.4	26.4	39.6



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

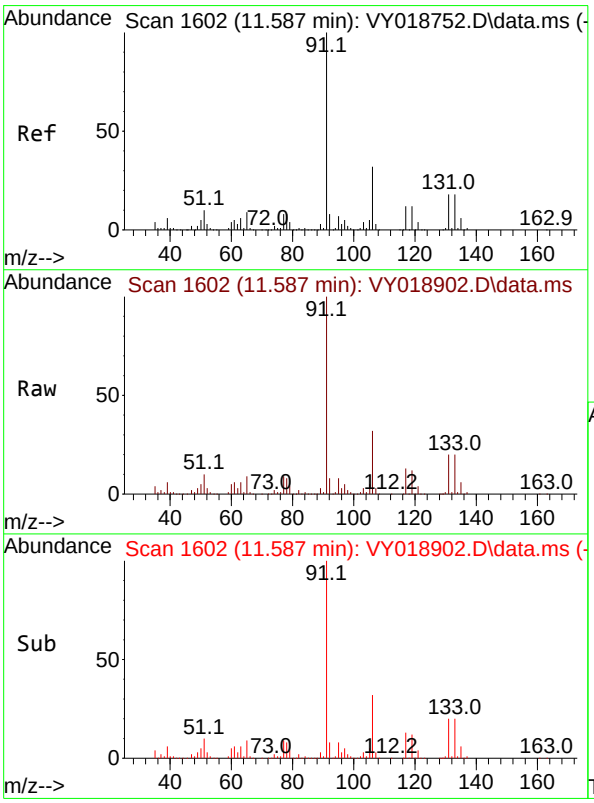

#66
1,1,1,2-Tetrachloroethane
Concen: 55.473 ug/l
RT: 11.587 min Scan# 1602
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:131 Resp: 55002

Ion	Ratio	Lower	Upper
131	100		
133	96.0	47.8	143.3
119	63.0	34.1	102.2



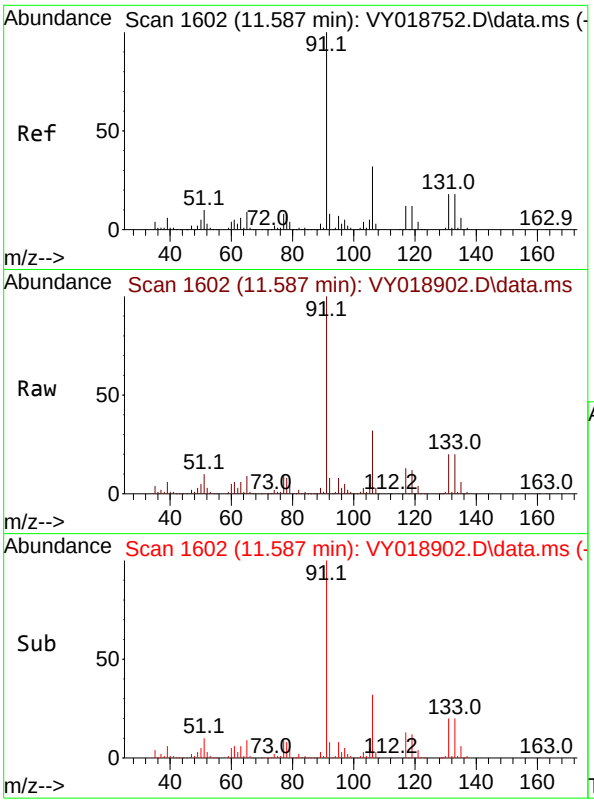

#67
Ethyl Benzene
Concen: 53.328 ug/l
RT: 11.587 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 91 Resp: 26884

Ion	Ratio	Lower	Upper
91	100		
106	32.3	24.5	36.7



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

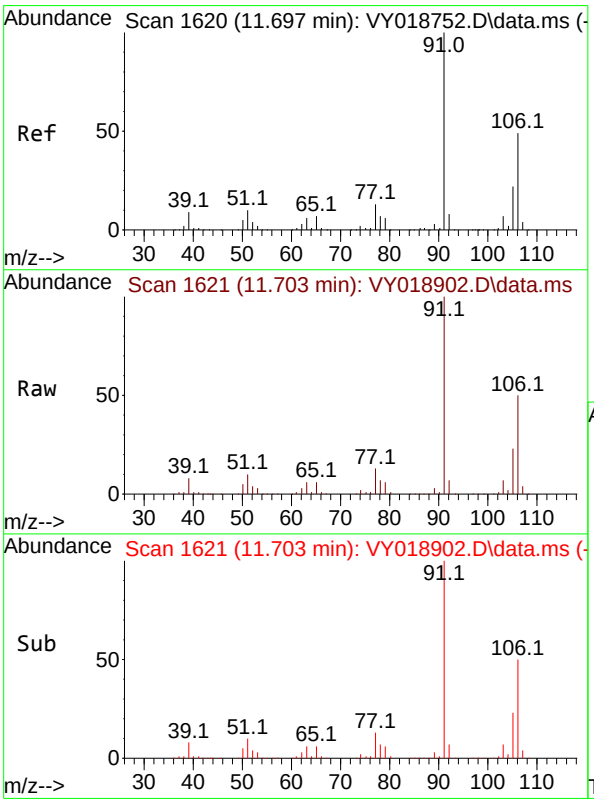

#68
m/p-Xylenes
Concen: 105.742 ug/l
RT: 11.703 min Scan# 1621
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:106 Resp: 209192

Ion	Ratio	Lower	Upper
106	100		
91	200.1	156.0	234.0



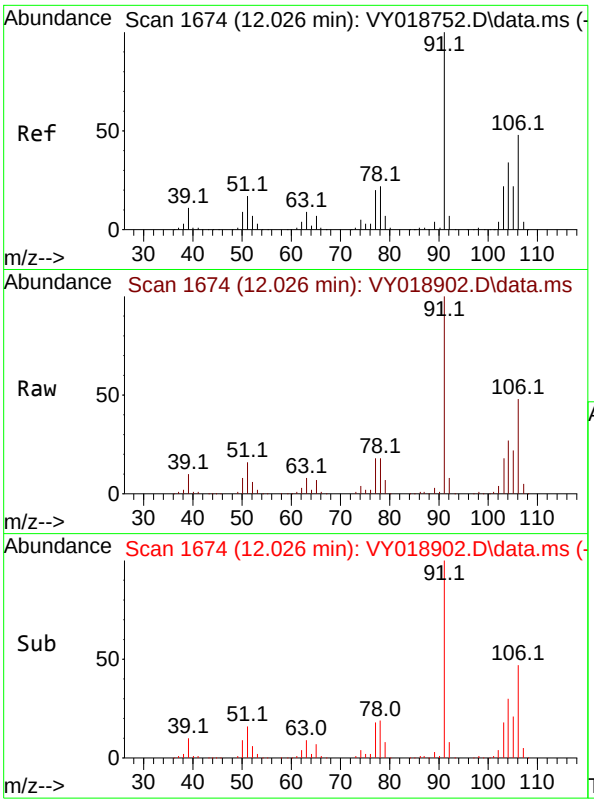

#69
o-Xylene
Concen: 54.735 ug/l
RT: 12.026 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:106 Resp: 10180

Ion	Ratio	Lower	Upper
106	100		
91	204.7	103.6	310.8



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

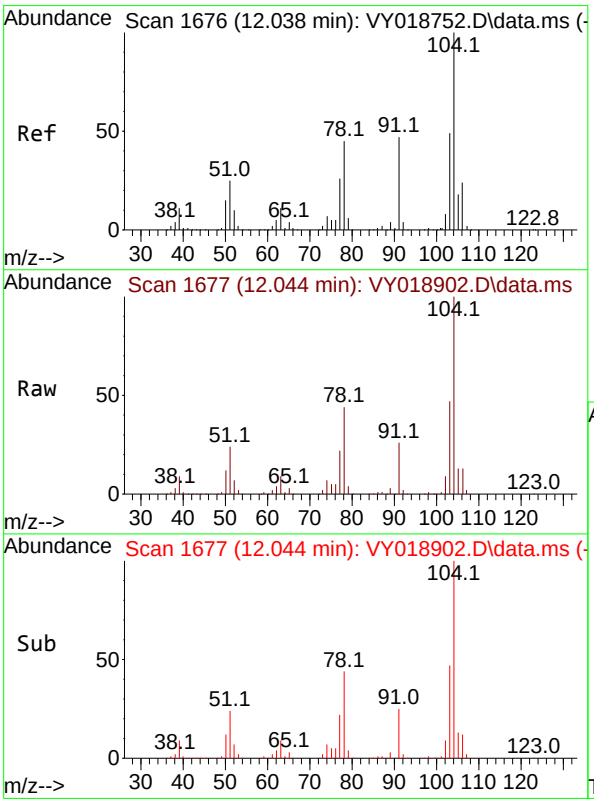

#70
Styrene
Concen: 54.425 ug/l
RT: 12.044 min Scan# 1677
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:104 Resp: 168901

Ion	Ratio	Lower	Upper
104	100		
78	49.2	37.0	55.4
103	53.8	44.2	66.2



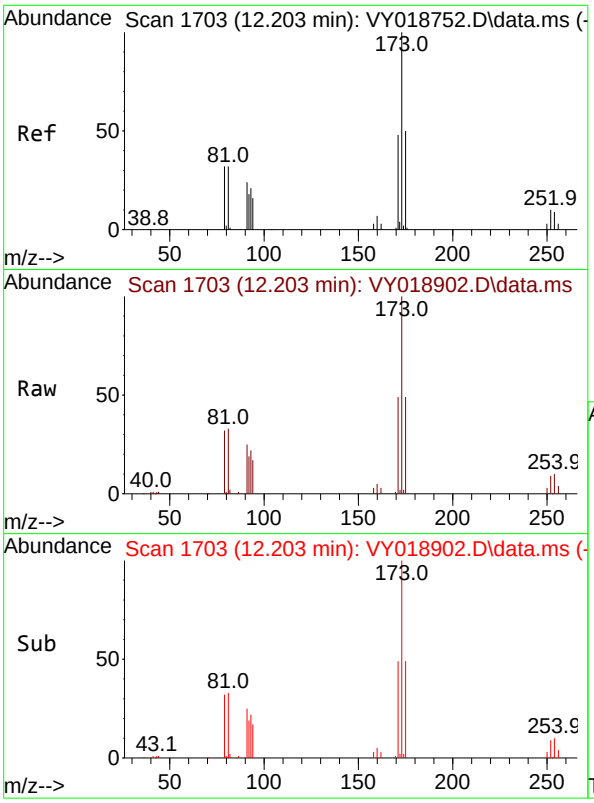

#71
Bromoform
Concen: 59.221 ug/l
RT: 12.203 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:173 Resp: 3200

Ion	Ratio	Lower	Upper
173	100		
175	47.9	25.1	75.3
254	0.4	0.0	0.0

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



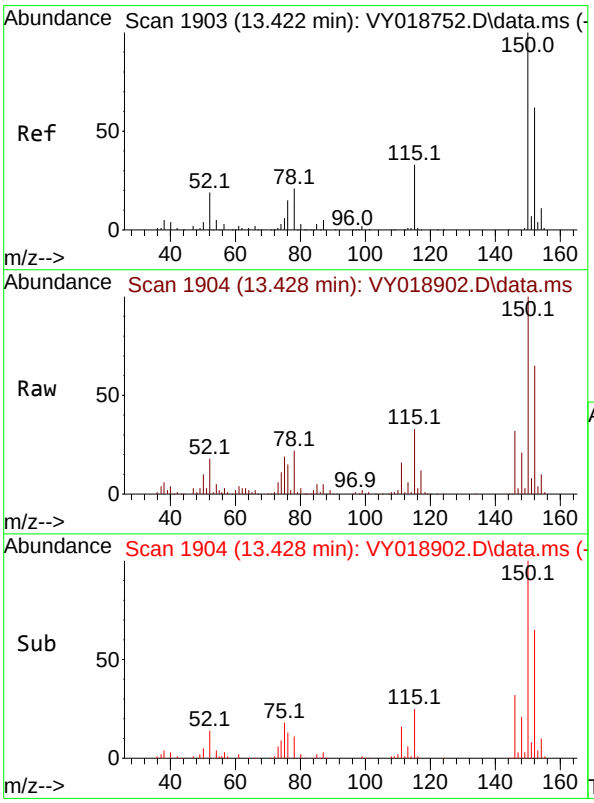

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:152 Resp: 68808

Ion	Ratio	Lower	Upper
152	100		
115	57.6	28.2	84.7
150	174.5	0.0	345.6



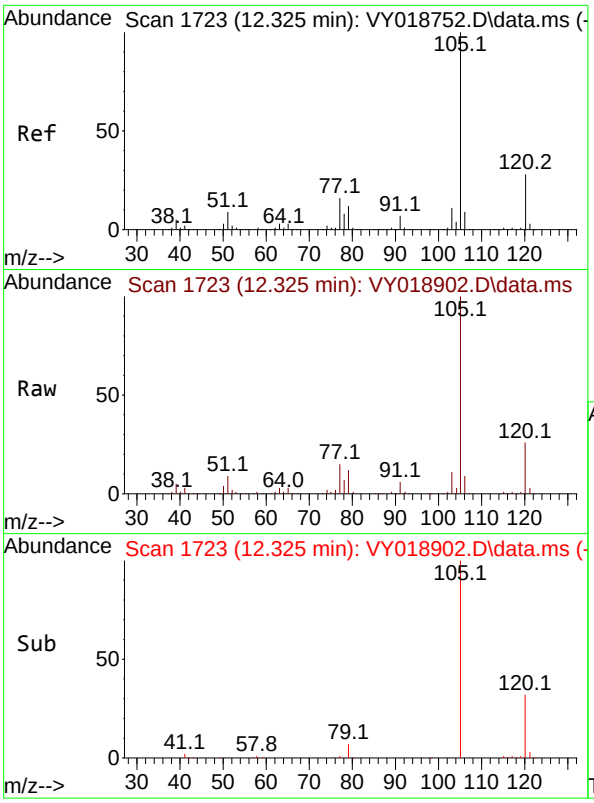

#73
Isopropylbenzene
Concen: 52.280 ug/l
RT: 12.325 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:105 Resp: 26327

Ion	Ratio	Lower	Upper
105	100		
120	27.8	13.4	40.1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



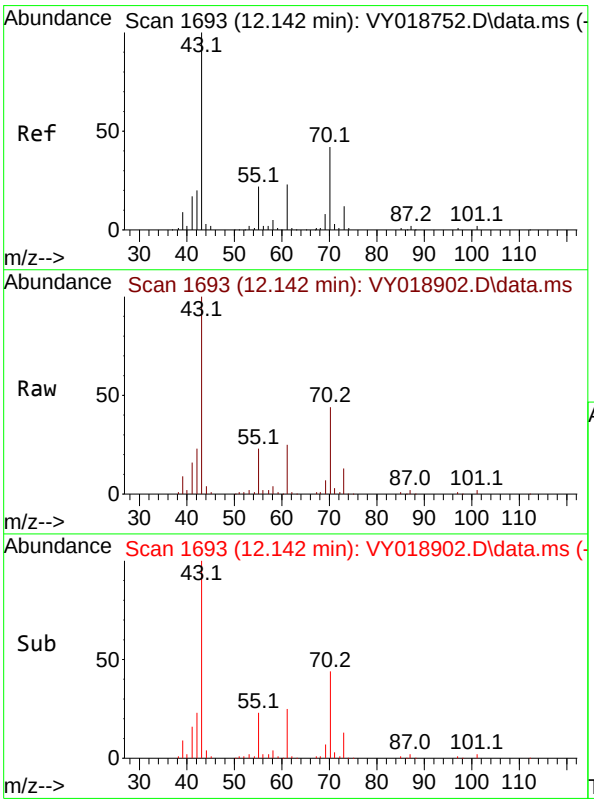

#74
N-amyl acetate
Concen: 51.410 ug/l
RT: 12.142 min Scan# 1693
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 43 Resp: 52946

Ion	Ratio	Lower	Upper
43	100		
70	45.0	41.4	62.2
55	23.4	23.3	34.9
61	24.0	22.6	33.8



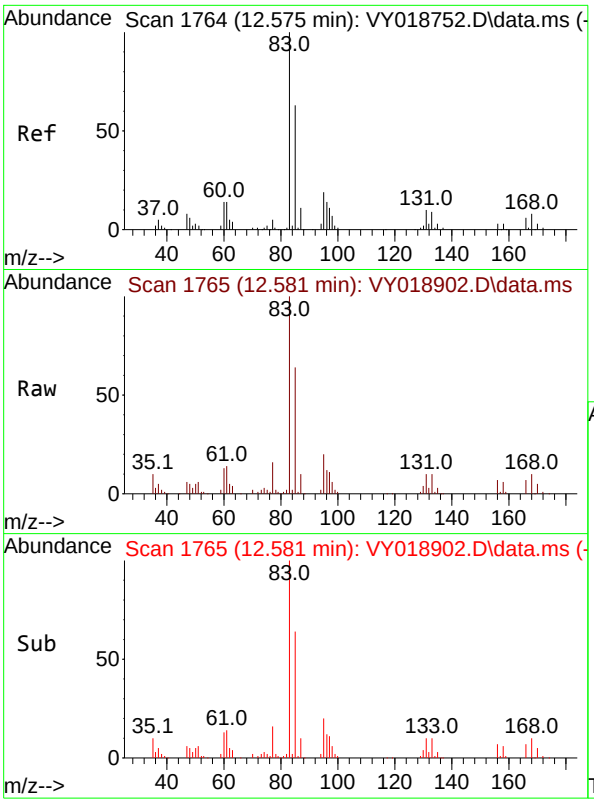

#75
1,1,2,2-Tetrachloroethane
Concen: 50.914 ug/l
RT: 12.581 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 83 Resp: 4041

Ion	Ratio	Lower	Upper
83	100		
131	12.1	5.0	14.9
85	64.0	32.0	96.0

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



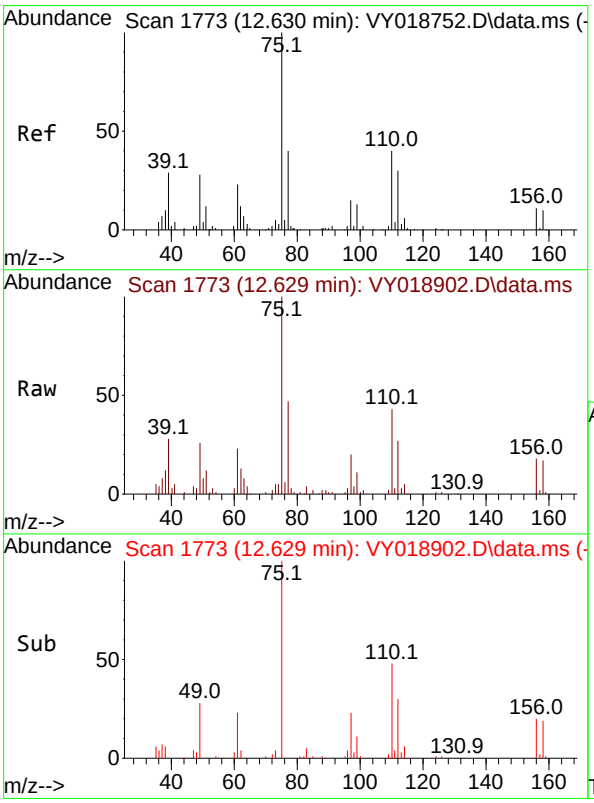

#76
1,2,3-Trichloropropane
Concen: 51.128 ug/l m
RT: 12.629 min Scan# 1773
Delta R.T. -0.001 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 75 Resp: 27554

Ion	Ratio	Lower	Upper
75	100		
77	0.0	0.0	0.0



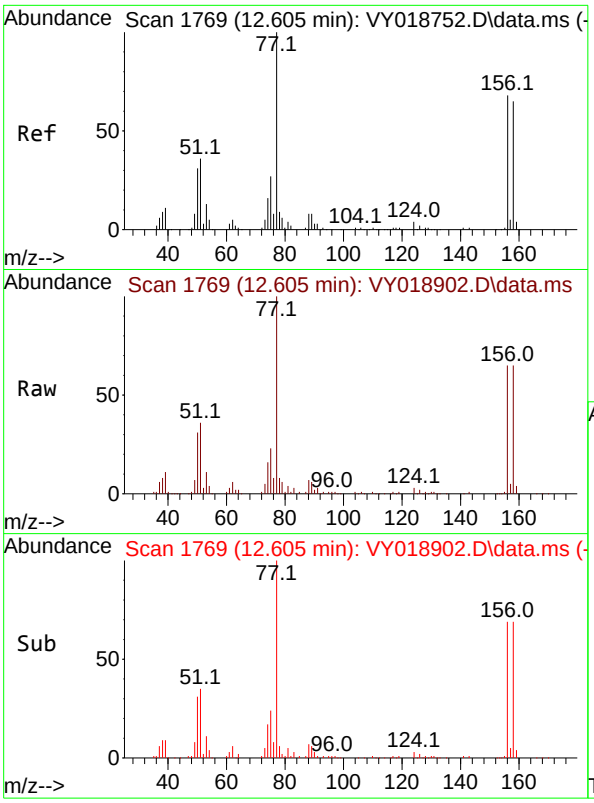

#77
Bromobenzene
Concen: 52.264 ug/l
RT: 12.605 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:156 Resp: 6283

Ion	Ratio	Lower	Upper
156	100		
77	162.6	87.1	261.3
158	98.4	48.6	145.9

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



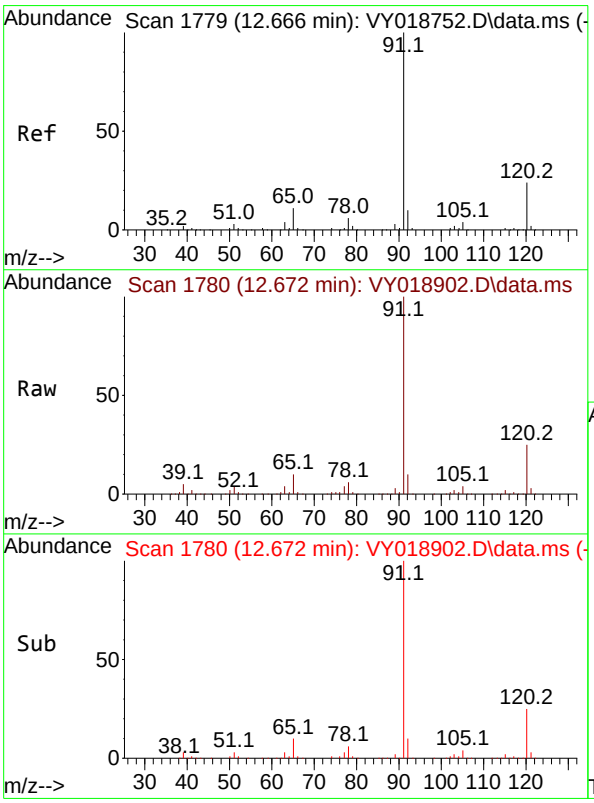

#78
n-propylbenzene
Concen: 51.502 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 91 Resp: 307989

Ion	Ratio	Lower	Upper
91	100		
120	24.3	11.5	34.4



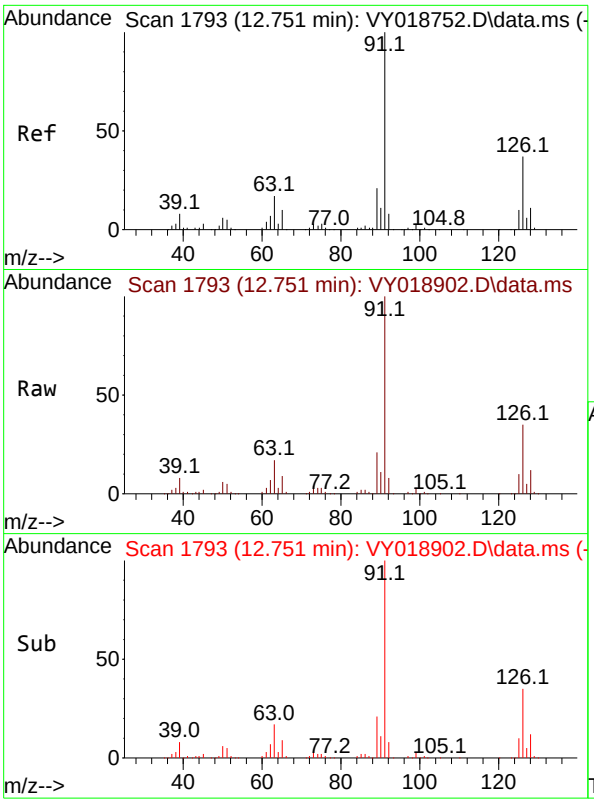

#79
2-Chlorotoluene
Concen: 51.591 ug/l
RT: 12.751 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 91 Resp: 17348

Ion	Ratio	Lower	Upper
91	100		
126	37.3	17.8	53.5



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

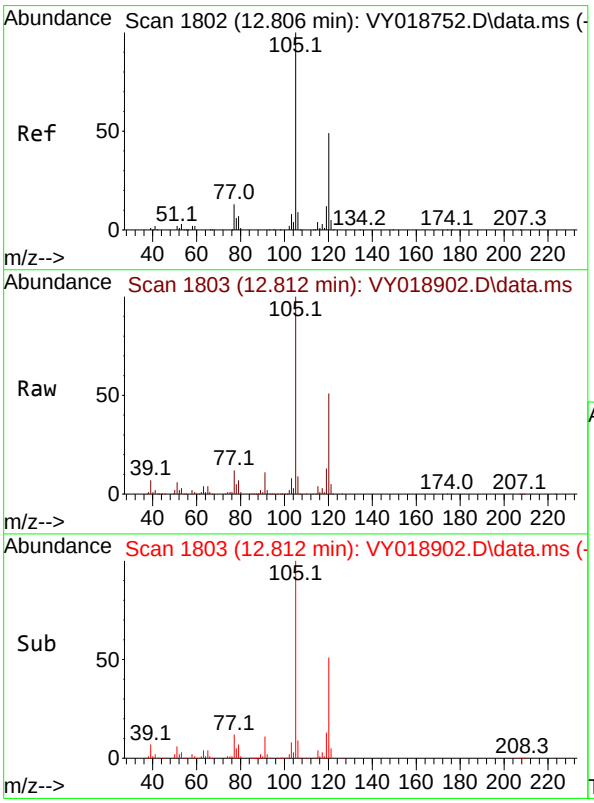

#80
1,3,5-Trimethylbenzene
Concen: 53.767 ug/l
RT: 12.812 min Scan# 1803
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:105 Resp: 221543

Ion	Ratio	Lower	Upper
105	100		
120	50.2	25.1	75.2



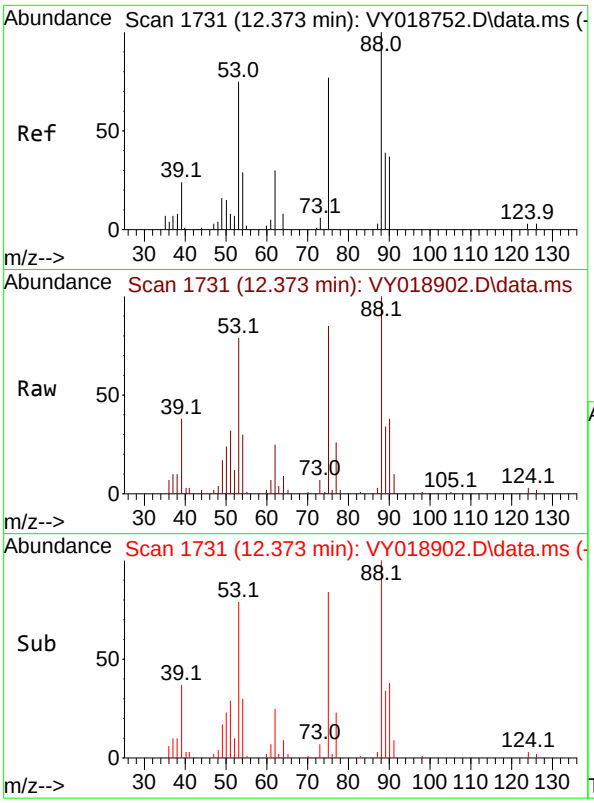

#81
trans-1,4-Dichloro-2-butene
Concen: 51.450 ug/l
RT: 12.373 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 75 Resp: 1238

Ion	Ratio	Lower	Upper
75	100		
53	105.9	66.8	100.2
89	47.8	35.8	53.6

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



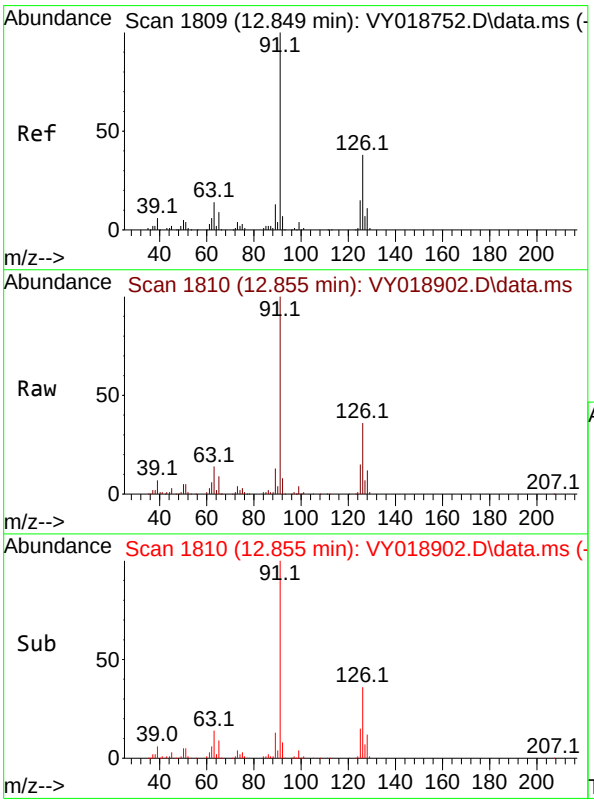

#82
4-Chlorotoluene
Concen: 52.356 ug/l
RT: 12.855 min Scan# 1810
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 91 Resp: 181284

Ion	Ratio	Lower	Upper
91	100		
126	36.7	17.6	52.9



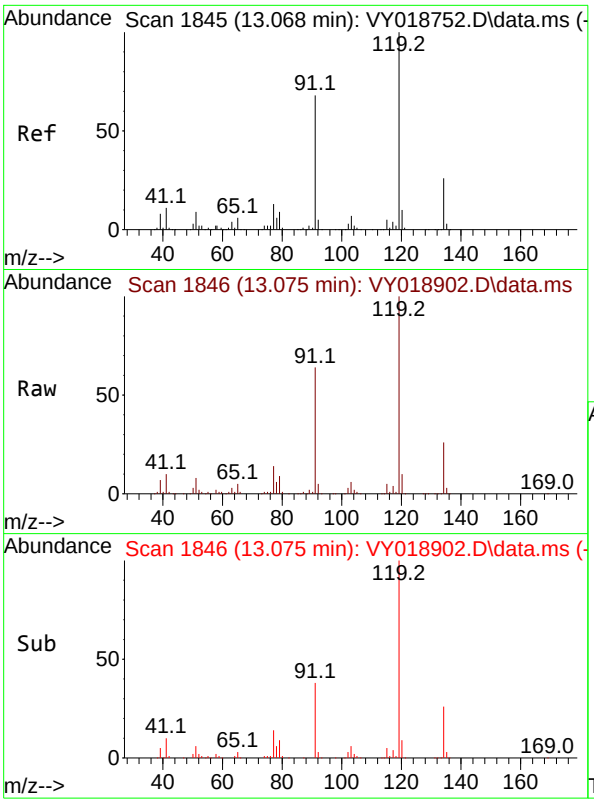

#83
tert-Butylbenzene
Concen: 53.680 ug/l
RT: 13.075 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:119 Resp: 20420

Ion	Ratio	Lower	Upper
119	100		
91	63.5	31.3	93.8
134	27.6	13.4	40.1



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

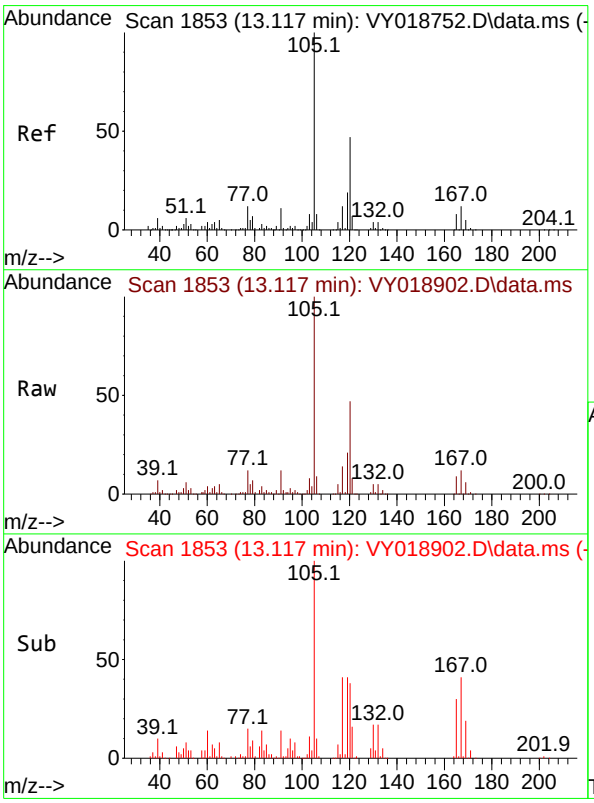

#84
1,2,4-Trimethylbenzene
Concen: 52.377 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:105 Resp: 214459

Ion	Ratio	Lower	Upper
105	100		
120	47.9	23.2	69.6



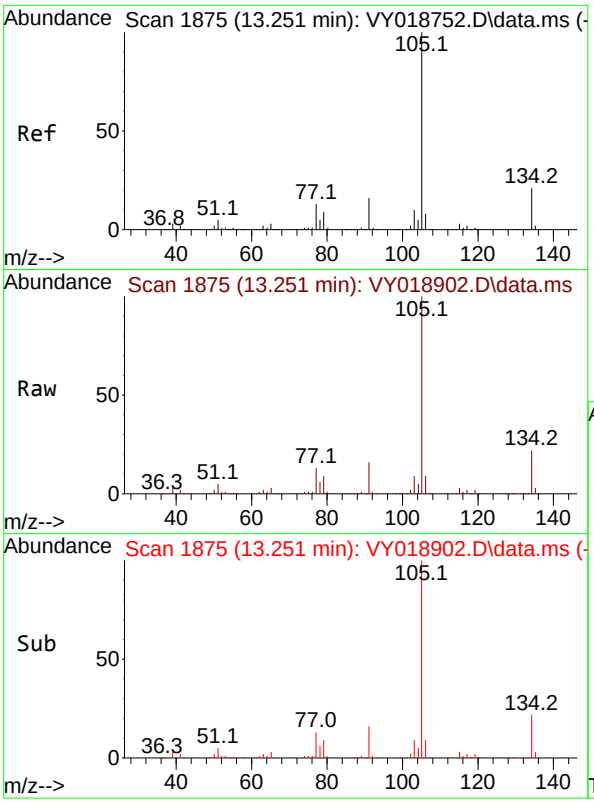

#85
sec-Butylbenzene
Concen: 53.840 ug/l
RT: 13.251 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:105 Resp: 29071

Ion	Ratio	Lower	Upper
105	100		
134	21.4	10.1	30.1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



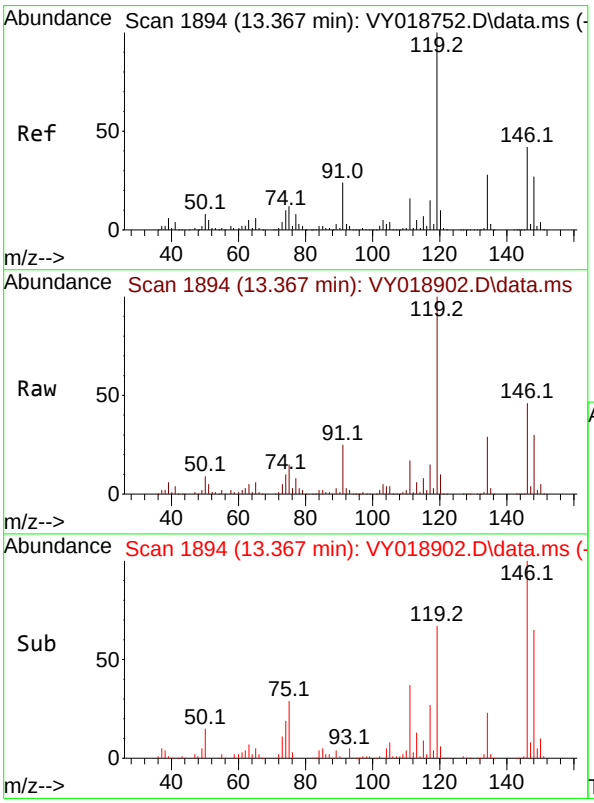

#86
p-Isopropyltoluene
Concen: 53.387 ug/l
RT: 13.367 min Scan# 1894
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:119 Resp: 248859

Ion	Ratio	Lower	Upper
119	100		
134	28.2	13.1	39.3
91	24.4	10.7	32.1



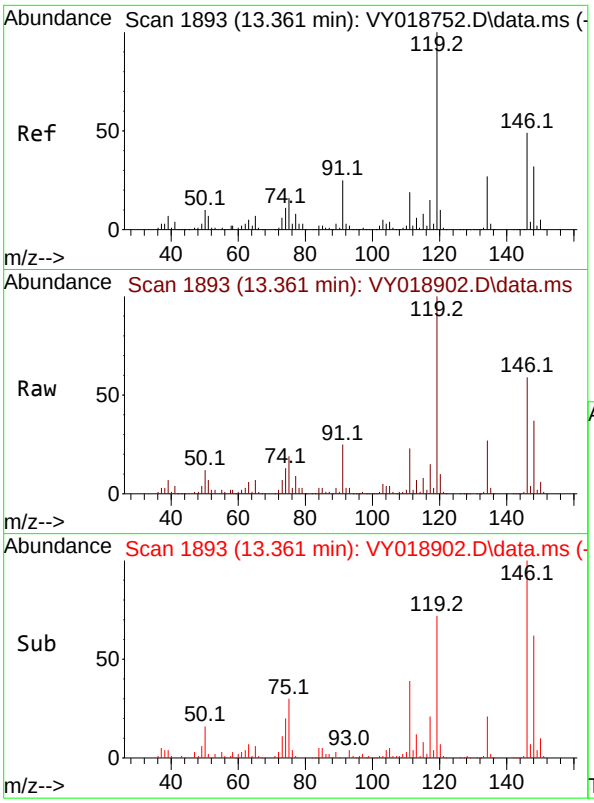

#87
1,3-Dichlorobenzene
Concen: 54.492 ug/l
RT: 13.361 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:146 Resp: 12866

Ion	Ratio	Lower	Upper
146	100		
111	37.7	19.0	57.0
148	63.4	31.7	95.1



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

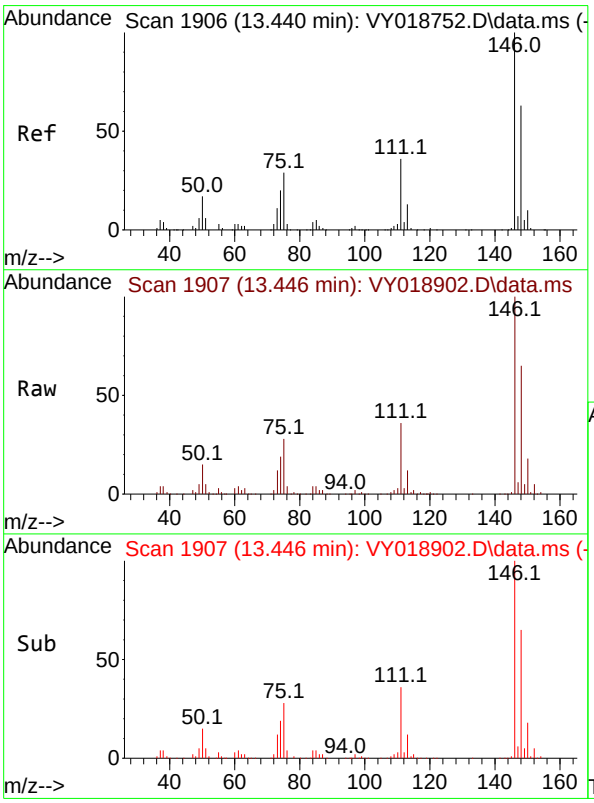

#88
1,4-Dichlorobenzene
Concen: 53.598 ug/l
RT: 13.446 min Scan# 1907
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:146 Resp: 125430

Ion	Ratio	Lower	Upper
146	100		
111	37.7	18.4	55.4
148	63.6	32.4	97.2



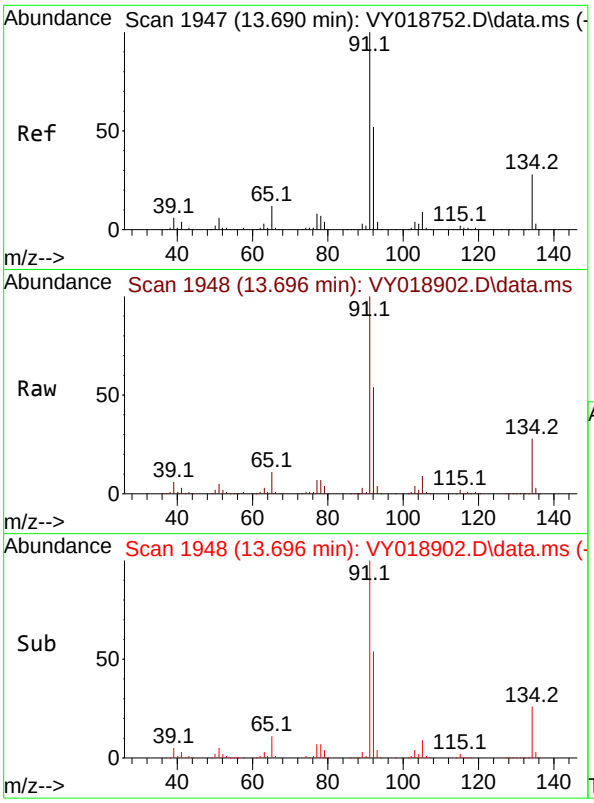

#89
n-Butylbenzene
Concen: 53.161 ug/l
RT: 13.696 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 91 Resp: 22466

Ion	Ratio	Lower	Upper
91	100		
92	52.7	26.6	79.7
134	28.3	12.9	38.7

Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024



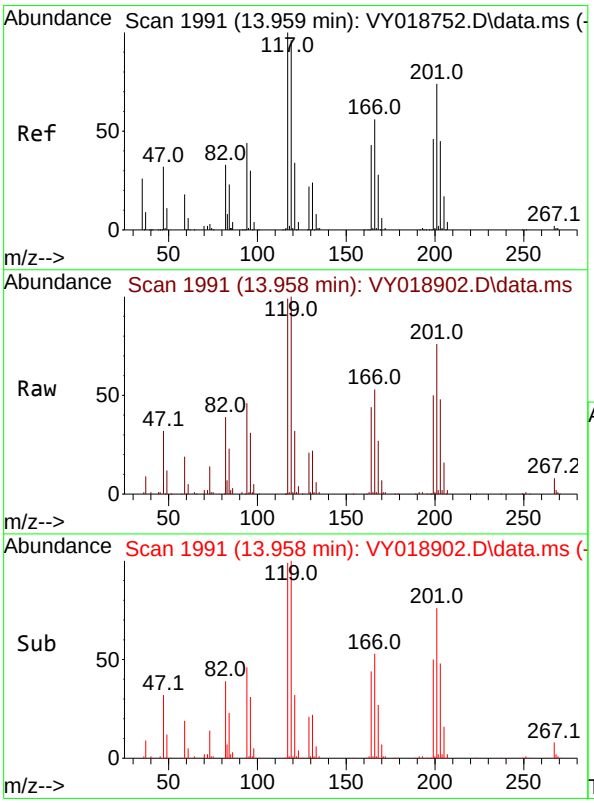

#90
Hexachloroethane
Concen: 56.233 ug/l
RT: 13.958 min Scan# 1991
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:117 Resp: 48749

Ion	Ratio	Lower	Upper
117	100		
201	76.3	37.4	112.2



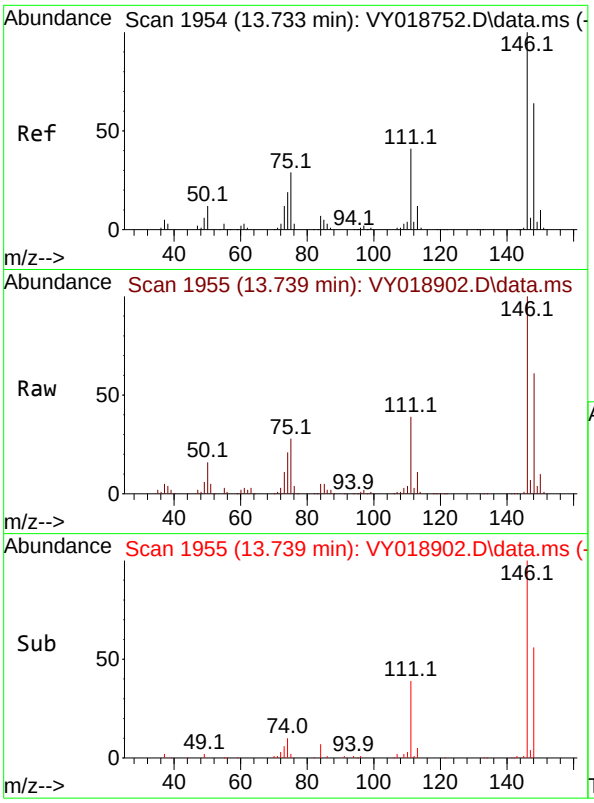

#91
1,2-Dichlorobenzene
Concen: 54.370 ug/l
RT: 13.739 min Scan# 1
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:146 Resp: 11089

Ion	Ratio	Lower	Upper
146	100		
111	39.1	19.9	59.7
148	63.9	31.8	95.4



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

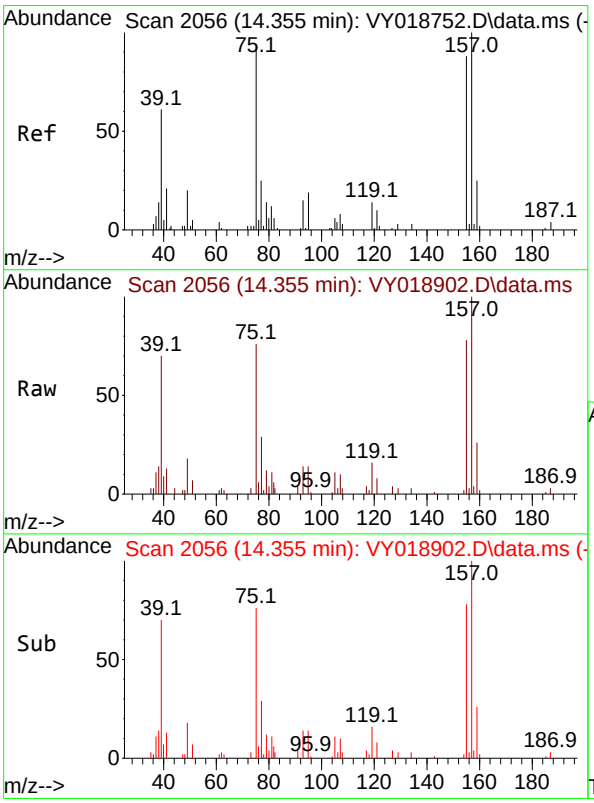

#92
1,2-Dibromo-3-Chloropropane
Concen: 51.882 ug/l
RT: 14.355 min Scan# 2056
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion: 75 Resp: 6674

Ion	Ratio	Lower	Upper
75	100		
155	93.4	48.6	145.8
157	117.8	62.7	188.2



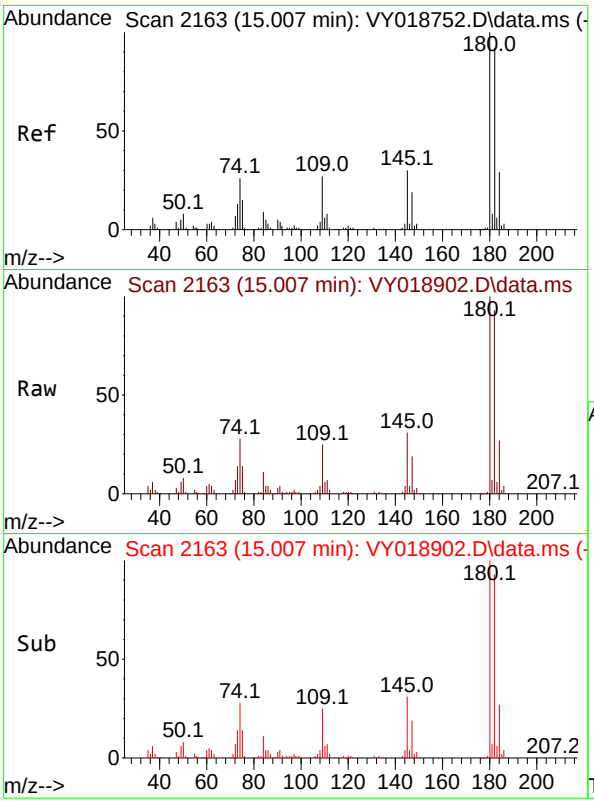

#93
1,2,4-Trichlorobenzene
Concen: 56.412 ug/l
RT: 15.007 min Scan# 2
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:180 Resp: 7023

Ion	Ratio	Lower	Upper
180	100		
182	95.0	47.9	143.8
145	31.4	14.2	42.6



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

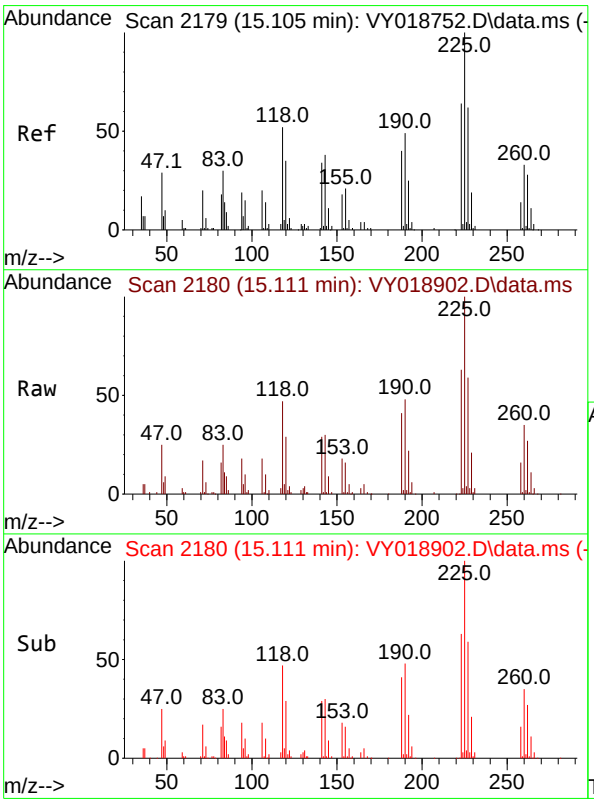

#94
Hexachlorobutadiene
Concen: 59.784 ug/l
RT: 15.111 min Scan# 2180
Delta R.T. 0.006 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:225 Resp: 42904

Ion	Ratio	Lower	Upper
225	100		
223	60.3	30.4	91.2
227	59.7	31.9	95.9



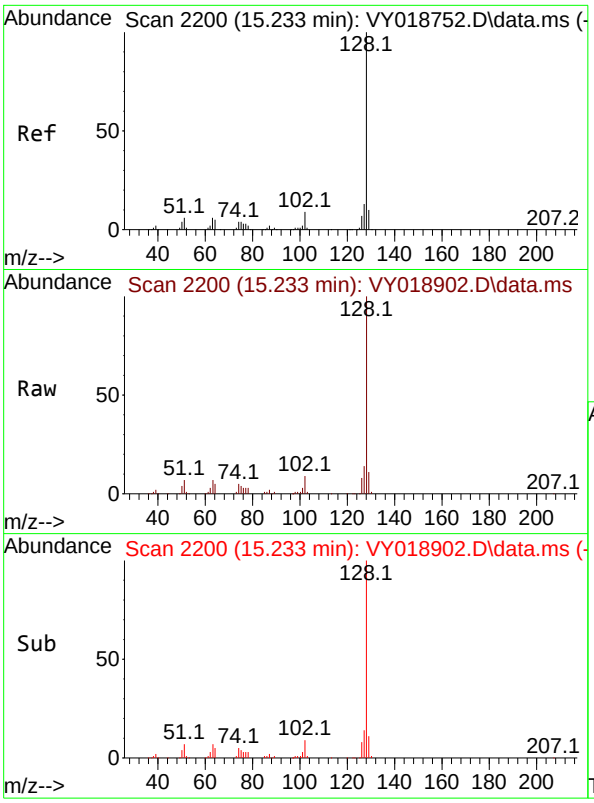

#95
Naphthalene
Concen: 55.571 ug/l
RT: 15.233 min Scan# 2
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:128 Resp: 11869

Ion	Ratio	Lower	Upper
128	100		
127	13.7	10.6	16.0
129	10.8	8.6	13.0



Instrument :
MSVOA_Y
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/25/2024
Supervised By :Semsettin Yesilyurt 07/25/2024

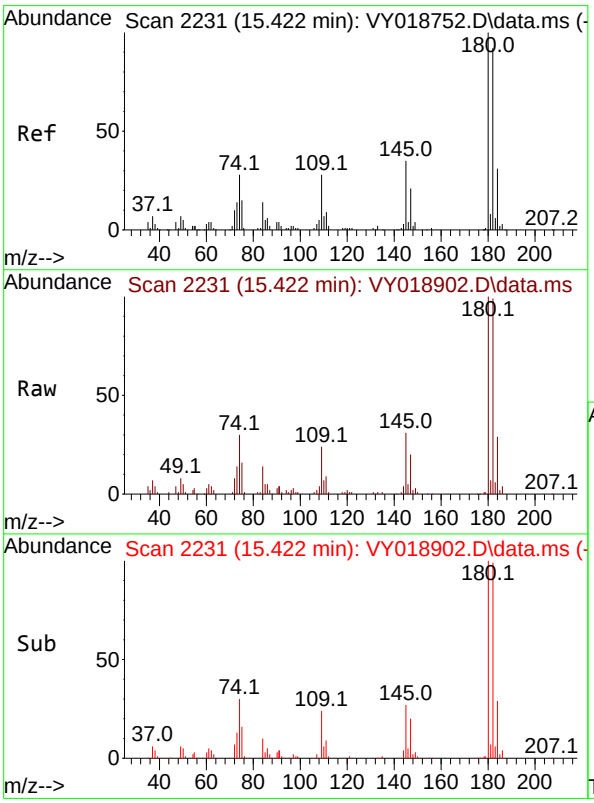

#96
1,2,3-Trichlorobenzene
Concen: 56.053 ug/l
RT: 15.422 min Scan# 2231
Delta R.T. -0.000 min
Lab File: VY018902.D
Acq: 24 Jul 2024 10:48

Tgt Ion:180 Resp: 59714

Ion	Ratio	Lower	Upper
180	100		
182	96.4	47.6	142.9
145	32.7	15.4	46.1