
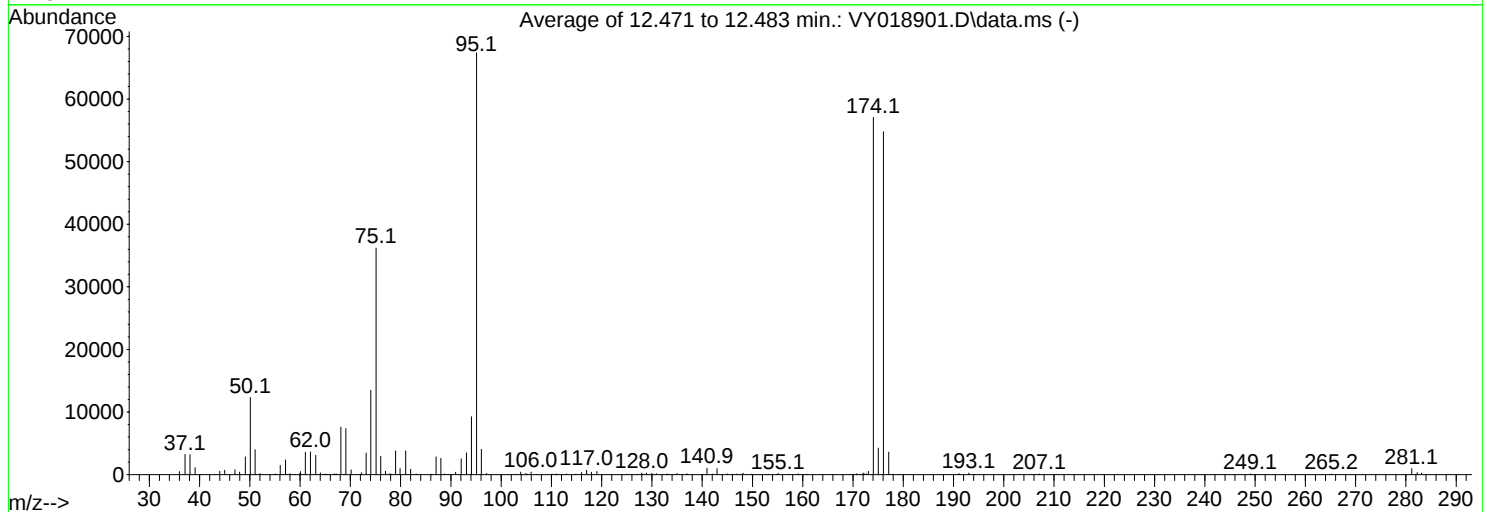


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072424\
Data File : VY018901.D
Acq On : 24 Jul 2024 08:40
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Title : SW846 8260
Last Update : Tue Jul 09 14:28:51 2024

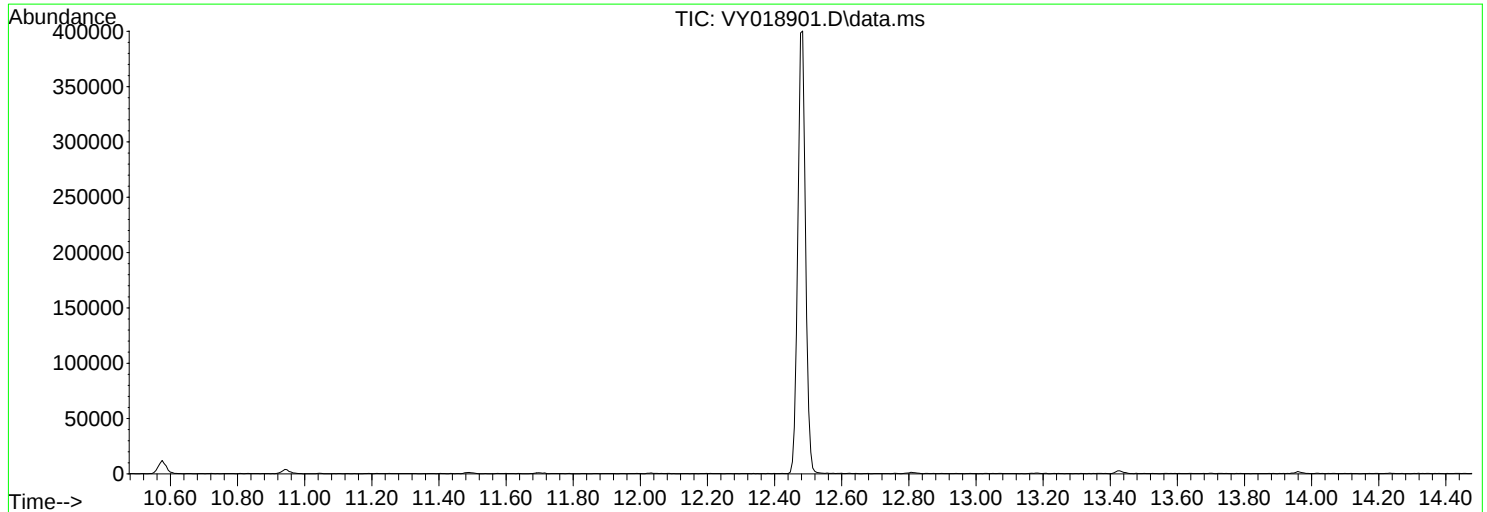

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	12317	PASS
75	95	30	60	53.7	36187	PASS
95	95	100	100	100.0	67384	PASS
96	95	5	9	6.0	4048	PASS
173	174	0.00	2	0.9	520	PASS
174	95	50	100	84.7	57075	PASS
175	174	5	9	7.5	4256	PASS
176	174	95	101	96.0	54784	PASS
177	176	5	9	6.6	3618	PASS