



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080924\
Data File : VY018953.D
Acq On : 09 Aug 2024 08:37
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080824S.M
Title : SW846 8260
Last Update : Fri Aug 09 04:24:33 2024

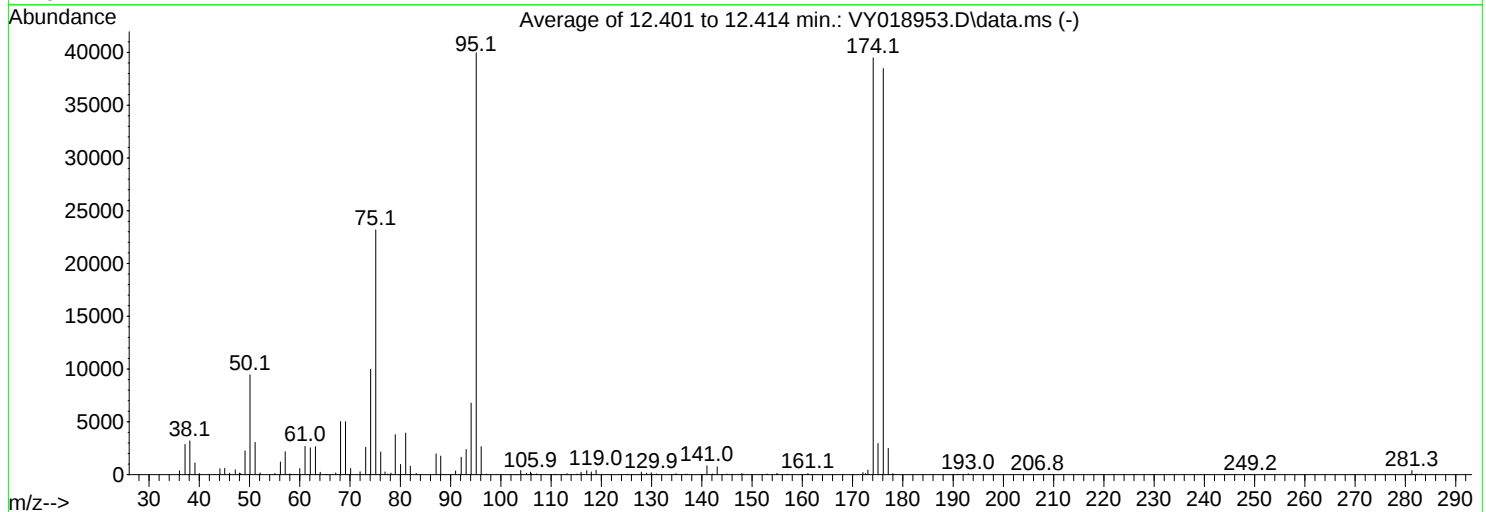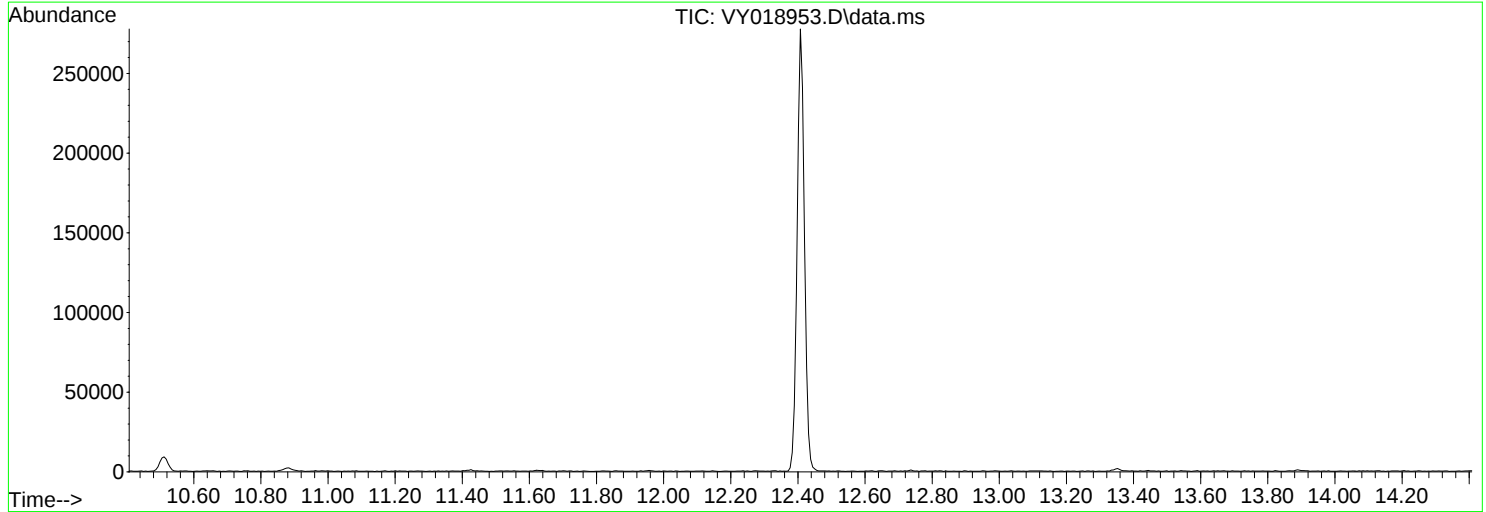

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	9461	PASS
75	95	30	60	58.0	23189	PASS
95	95	100	100	100.0	39955	PASS
96	95	5	9	6.7	2661	PASS
173	174	0.00	2	1.1	439	PASS
174	95	50	100	98.8	39480	PASS
175	174	5	9	7.5	2956	PASS
176	174	95	101	97.4	38469	PASS
177	176	5	9	6.5	2488	PASS