

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081224\
 Data File : VY019003.D
 Acq On : 12 Aug 2024 15:34
 Operator : SY/MD
 Sample : P3519-19
 Misc : 5.99g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OU4-CF-02-080624

Quant Time: Aug 13 01:16:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080824S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 09 04:24:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	66118	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.603	114	108650	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	92107	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	33306	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	36941	63.635	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	127.280%
35) Dibromofluoromethane	7.622	113	41720	60.121	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	120.240%
50) Toluene-d8	10.103	98	148481	55.706	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	111.420%
62) 4-Bromofluorobenzene	12.407	95	36682	46.387	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	92.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081224\
Data File : VY019003.D
Acq On : 12 Aug 2024 15:34
Operator : SY/MD
Sample : P3519-19
Misc : 5.99g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OU4-CF-02-080624

Quant Time: Aug 13 01:16:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080824S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 09 04:24:33 2024
Response via : Initial Calibration




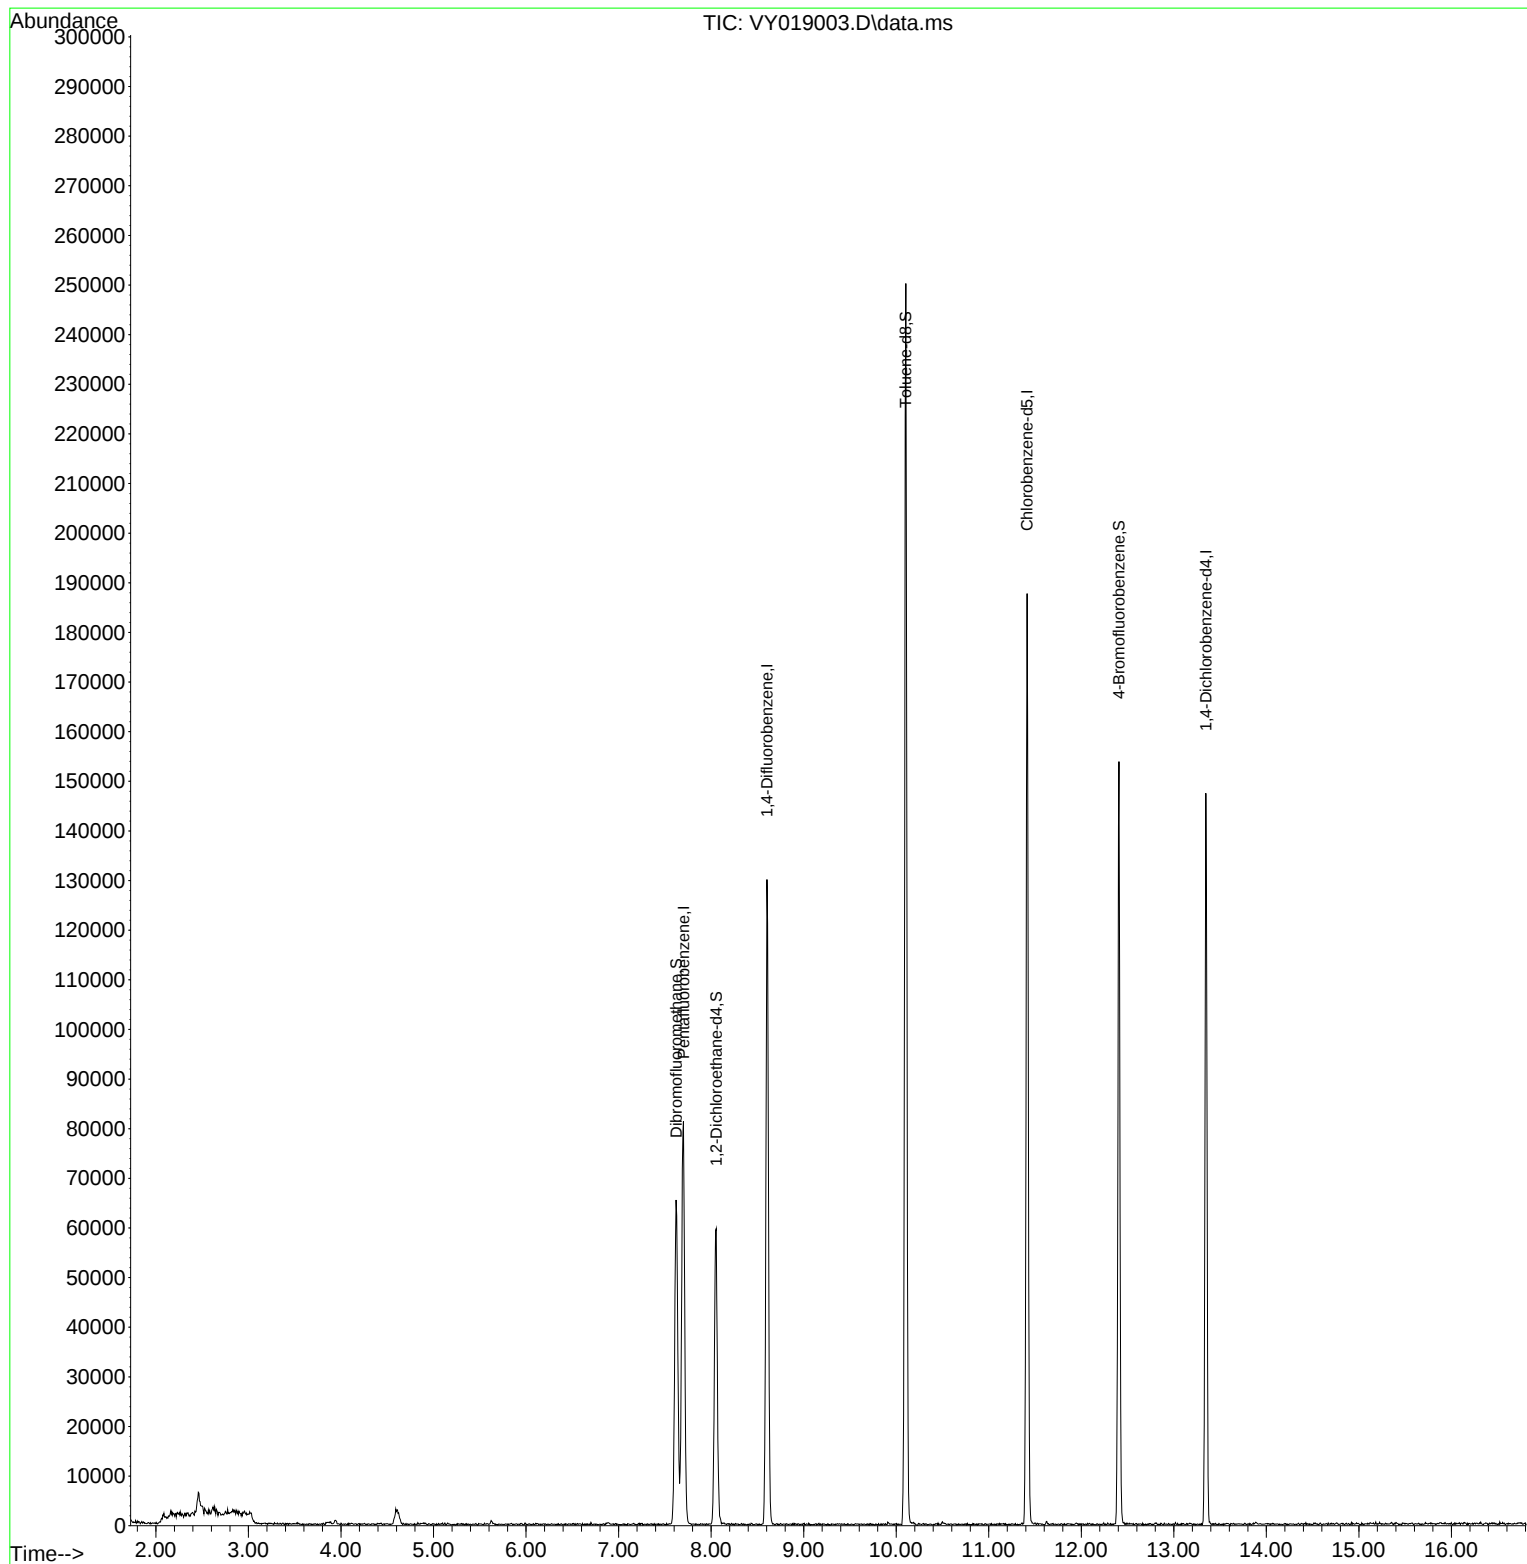


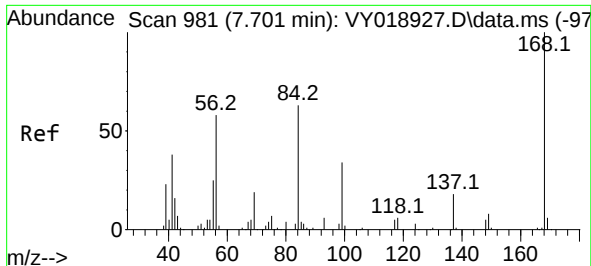

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 981
Delta R.T. -0.000 min
Lab File: VY019003.D
Acq: 12 Aug 2024 15:34




Instrument :
MSVOA_Y
ClientSampleId :
OU4-CF-02-080624


Tgt Ion:168 Resp: 66118
Ion Ratio Lower Upper
168 100
99 45.8 39.1 58.7

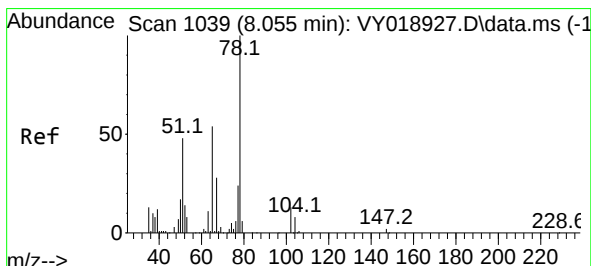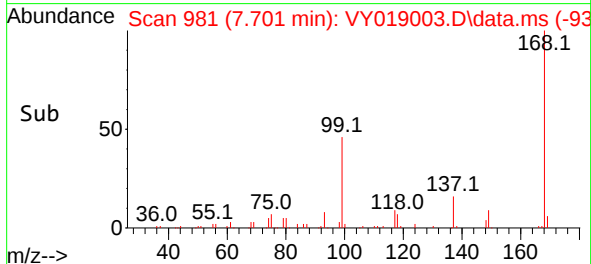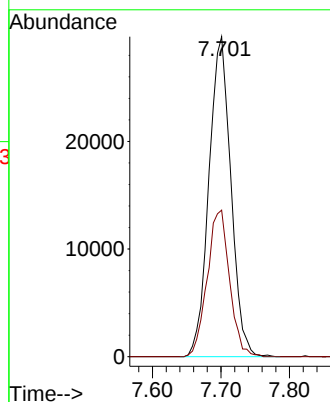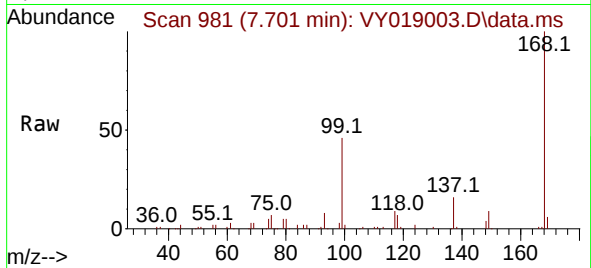

#33
1,2-Dichloroethane-d4
Concen: 63.635 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. -0.000 min
Lab File: VY019003.D
Acq: 12 Aug 2024 15:34

Tgt Ion: 65 Resp: 36941
Ion Ratio Lower Upper
65 100
67 54.2 0.0 109.6

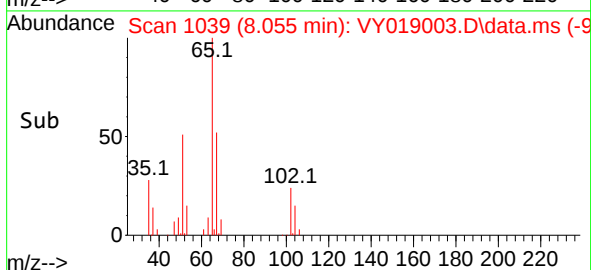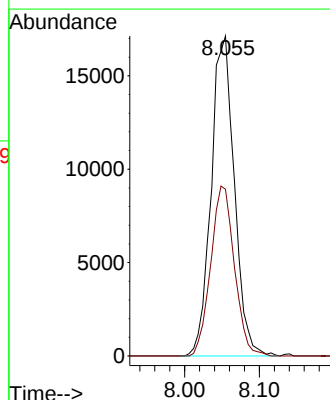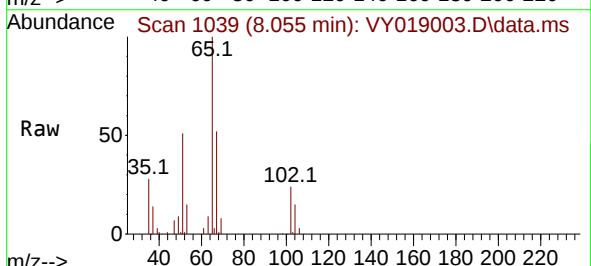

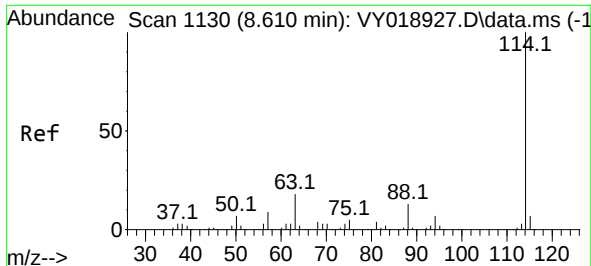

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.603 min Scan# 1129

Delta R.T. -0.006 min

Lab File: VY019003.D

Acq: 12 Aug 2024 15:34

Instrument :

MSVOA_Y

ClientSampleId :

OU4-CF-02-080624





Tgt Ion:114 Resp: 108650

Ion Ratio Lower Upper

114 100

63 18.0 0.0 35.0

88 12.1 0.0 27.2

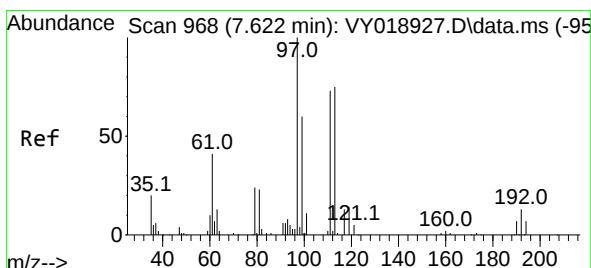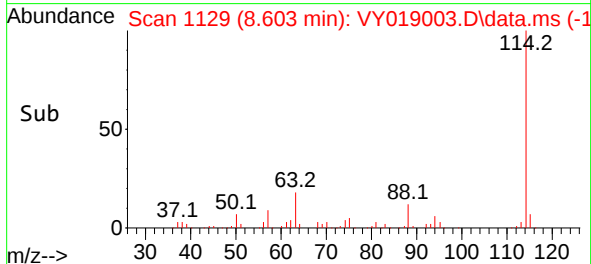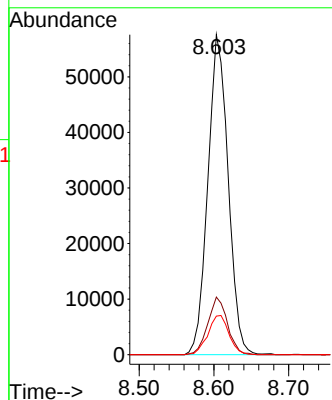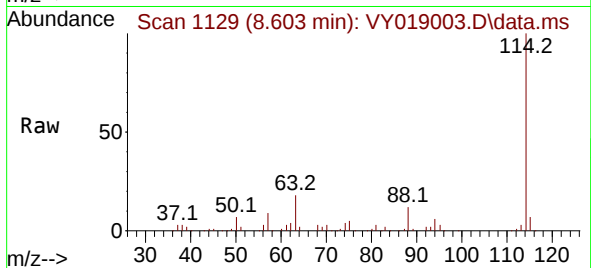

#35

Dibromofluoromethane

Concen: 60.121 ug/l

RT: 7.622 min Scan# 968

Delta R.T. -0.000 min

Lab File: VY019003.D

Acq: 12 Aug 2024 15:34




Tgt Ion:113 Resp: 41720


Ion Ratio Lower Upper

113 100

111 100.4 82.2 123.4

192 20.4 15.9 23.9


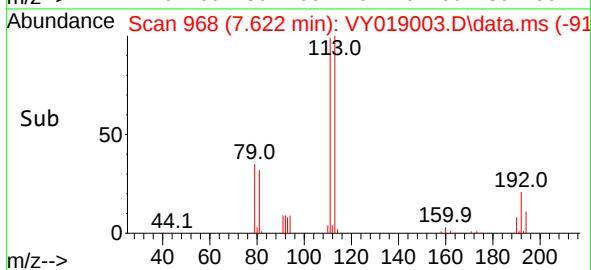
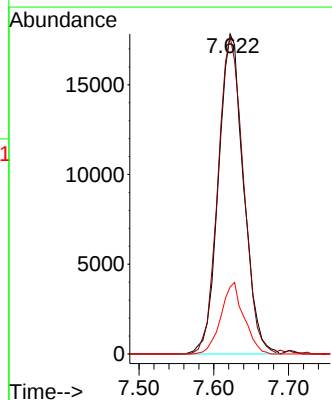
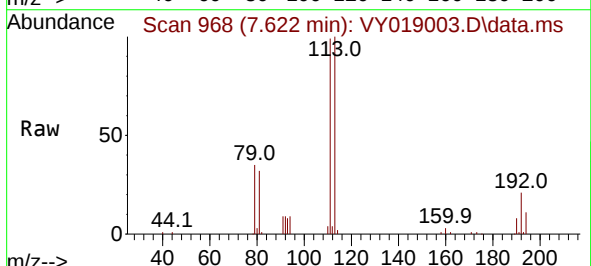


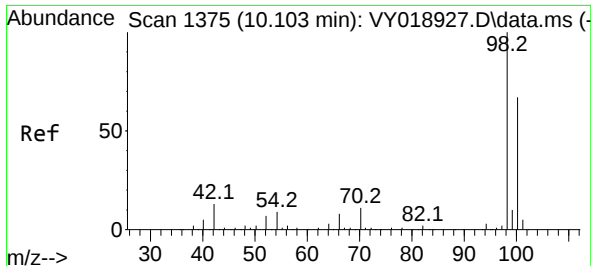

#50
Toluene-d8
Concen: 55.706 ug/l
RT: 10.103 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY019003.D
Acq: 12 Aug 2024 15:34




Instrument :
MSVOA_Y
ClientSampleId :
OU4-CF-02-080624


Tgt Ion: 98 Resp: 148481
Ion Ratio Lower Upper
98 100
100 67.0 52.0 78.0

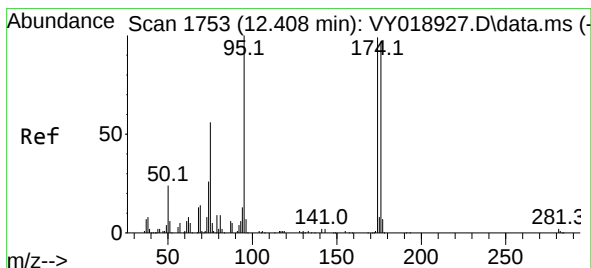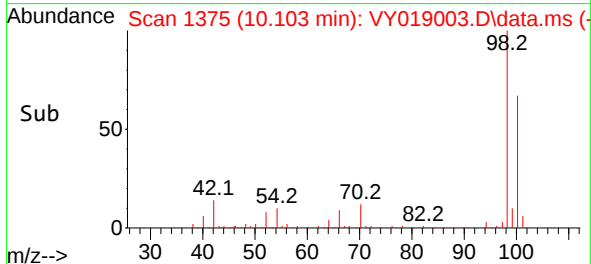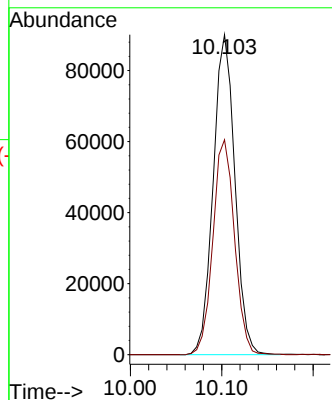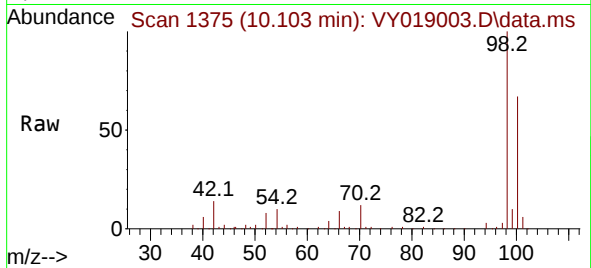

#62
4-Bromofluorobenzene
Concen: 46.387 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY019003.D
Acq: 12 Aug 2024 15:34

Tgt Ion: 95 Resp: 36682
Ion Ratio Lower Upper
95 100
174 105.7 0.0 175.6
176 100.1 0.0 171.4

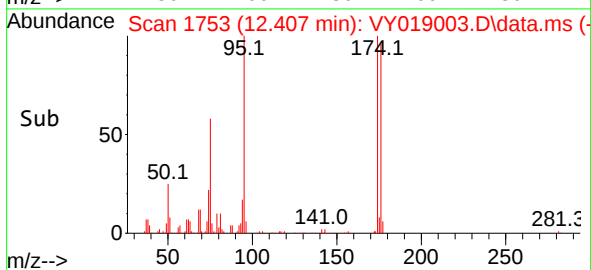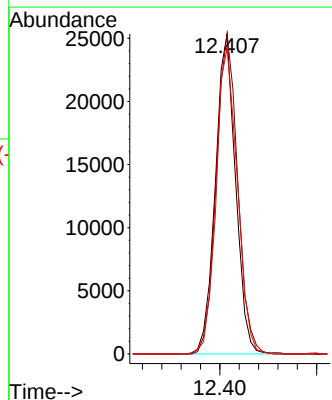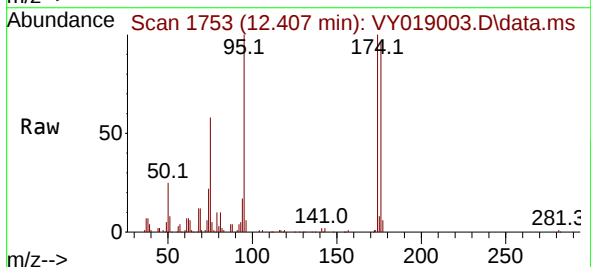

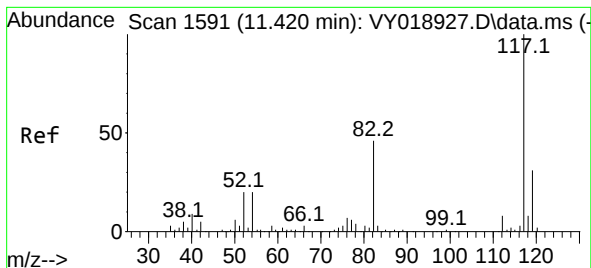

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY019003.D

Acq: 12 Aug 2024 15:34

Instrument :

MSVOA_Y

ClientSampleId :

OU4-CF-02-080624





Tgt Ion:117 Resp: 92107

Ion Ratio Lower Upper

117 100

82 48.3 42.4 63.6

119 30.4 25.9 38.9

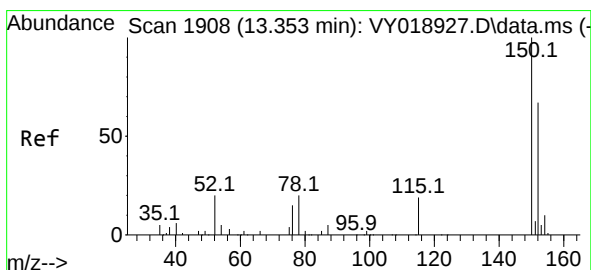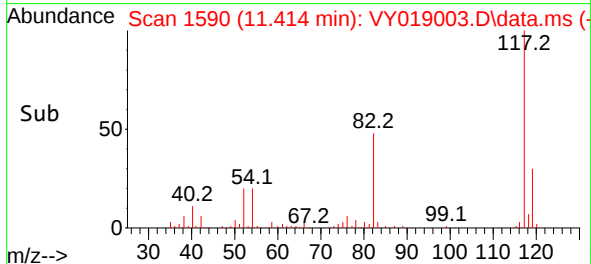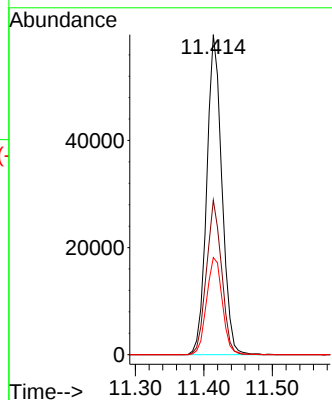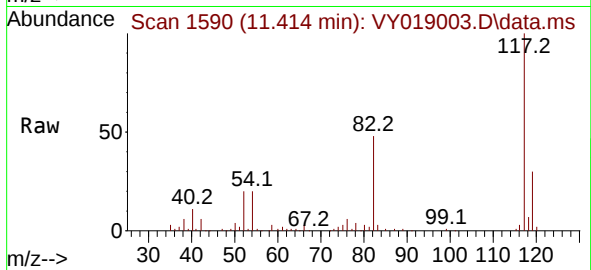

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.006 min

Lab File: VY019003.D

Acq: 12 Aug 2024 15:34

Tgt Ion:152 Resp: 33306

Ion Ratio Lower Upper

152 100

115 52.2 28.2 84.7

150 159.1 0.0 345.6

