
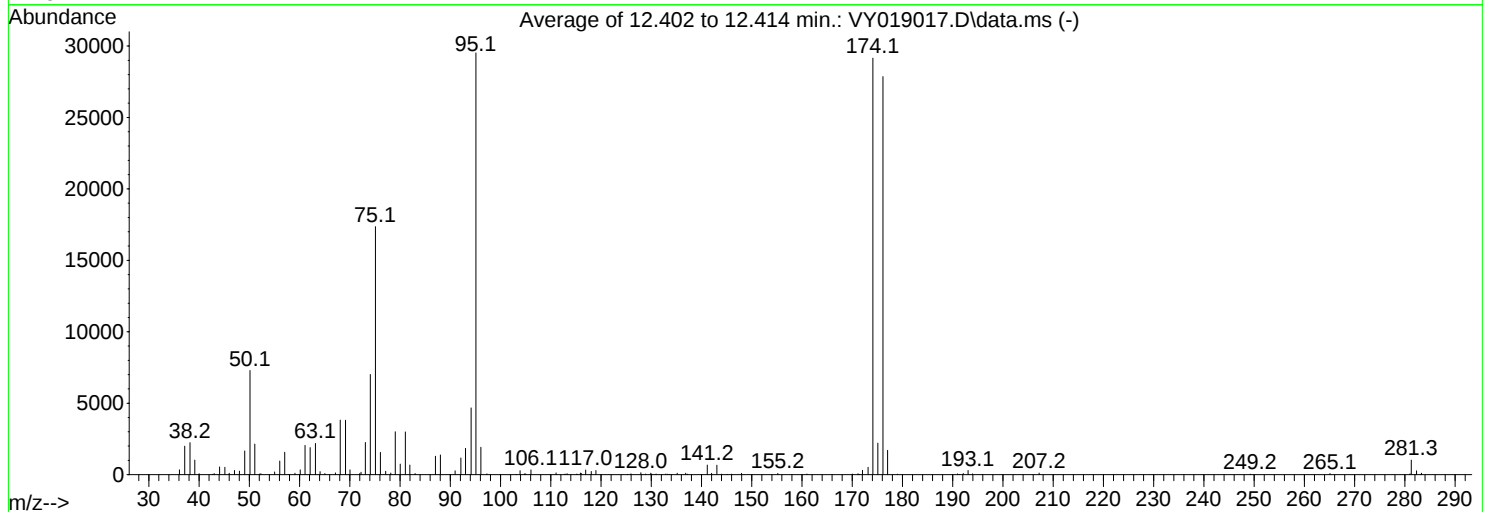


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081324\
Data File : VY019017.D
Acq On : 13 Aug 2024 09:29
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080824S.M
Title : SW846 8260
Last Update : Fri Aug 09 04:24:33 2024

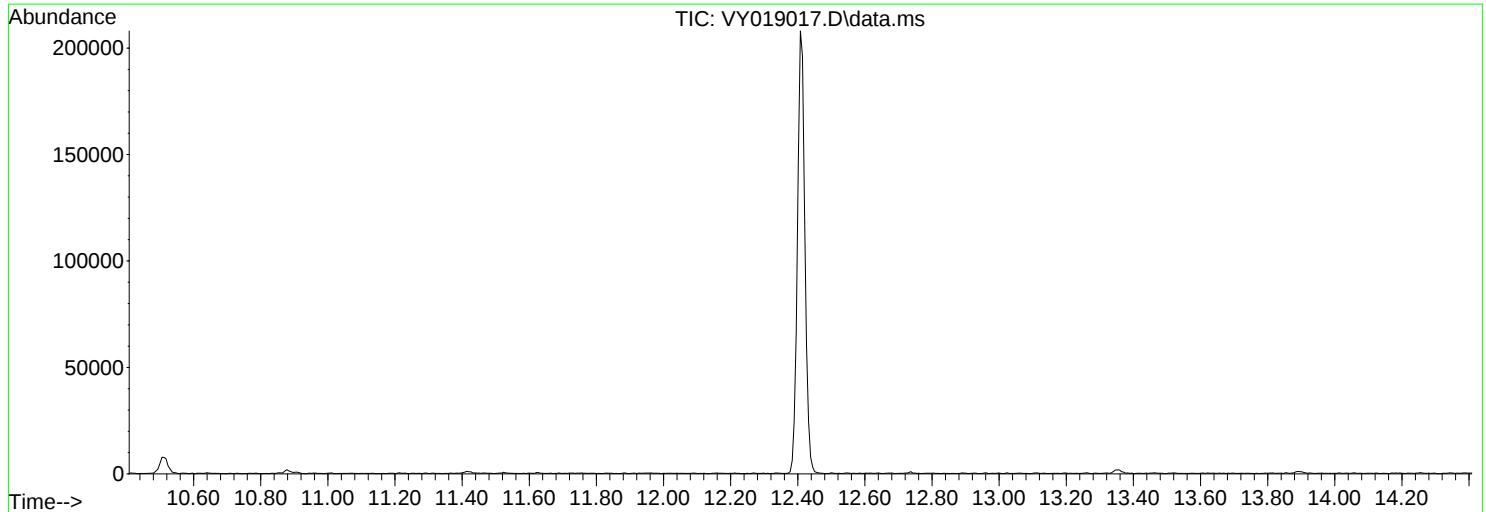

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.7	7287	PASS
75	95	30	60	58.8	17363	PASS
95	95	100	100	100.0	29523	PASS
96	95	5	9	6.5	1920	PASS
173	174	0.00	2	1.8	511	PASS
174	95	50	100	98.7	29147	PASS
175	174	5	9	7.6	2203	PASS
176	174	95	101	95.6	27869	PASS
177	176	5	9	6.1	1700	PASS