

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081424\
 Data File : VY019053.D
 Acq On : 14 Aug 2024 12:58
 Operator : SY/MD
 Sample : P3579-01
 Misc : 4.23g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VCPS-B1-081224-0-16

Quant Time: Aug 14 21:45:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080824S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 09 04:24:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	46176	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.603	114	75661	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	55325	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	15022	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	19474	48.034	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	96.060%
35) Dibromofluoromethane	7.622	113	25025	51.786	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.580%
50) Toluene-d8	10.103	98	84420	45.482	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	90.960%
62) 4-Bromofluorobenzene	12.408	95	15194	27.591	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	55.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081424\
Data File : VY019053.D
Acq On : 14 Aug 2024 12:58
Operator : SY/MD
Sample : P3579-01
Misc : 4.23g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VCPS-B1-081224-0-16

Quant Time: Aug 14 21:45:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080824S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 09 04:24:33 2024
Response via : Initial Calibration




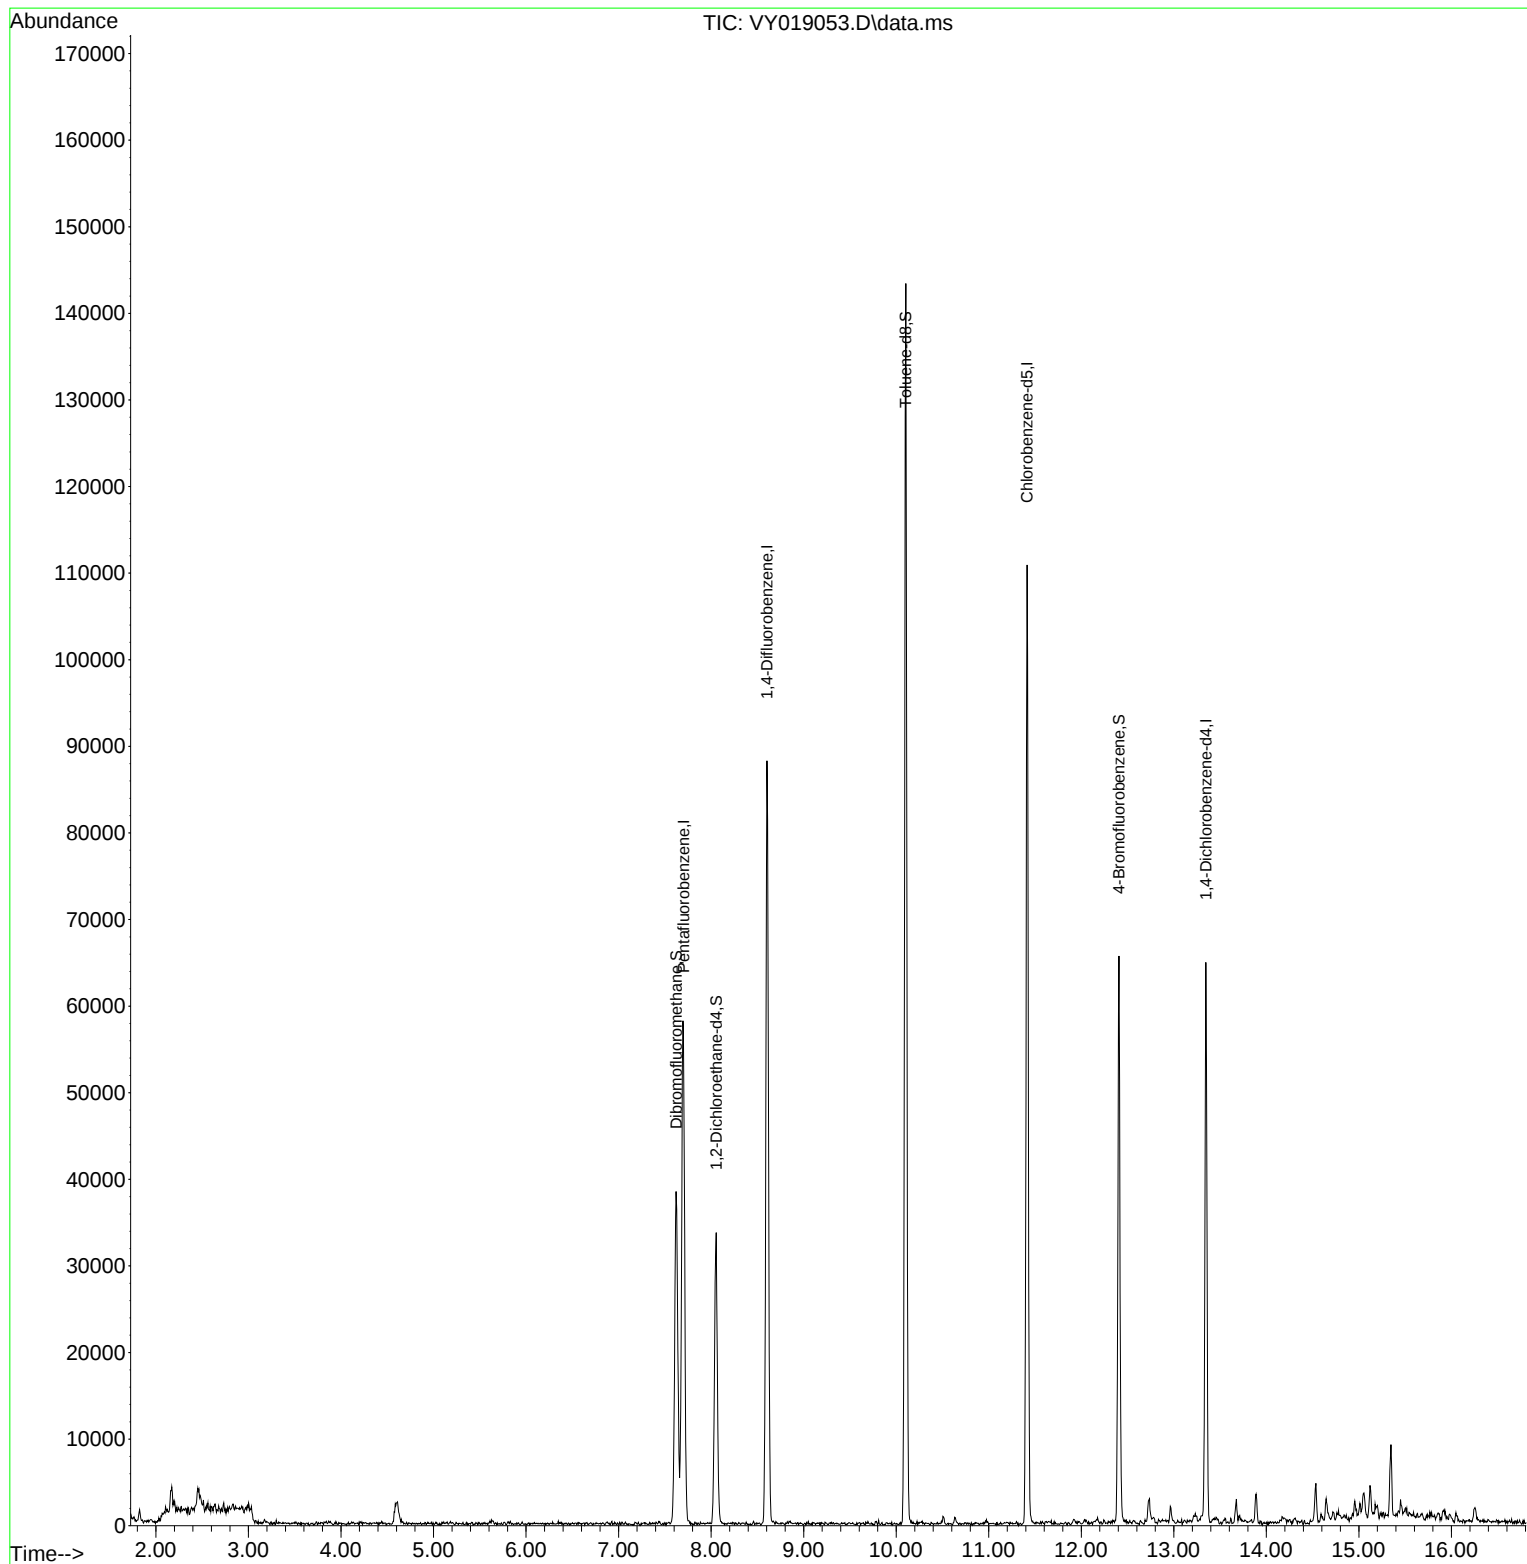


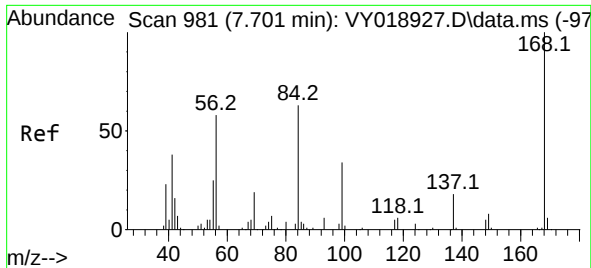

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY019053.D
Acq: 14 Aug 2024 12:58




Instrument :
MSVOA_Y
ClientSampleId :
VCPS-B1-081224-0-16


Tgt Ion:168 Resp: 46176
Ion Ratio Lower Upper
168 100
99 43.1 39.1 58.7

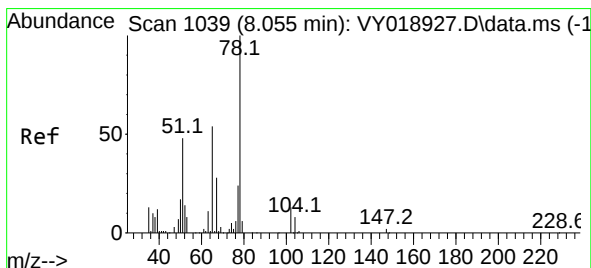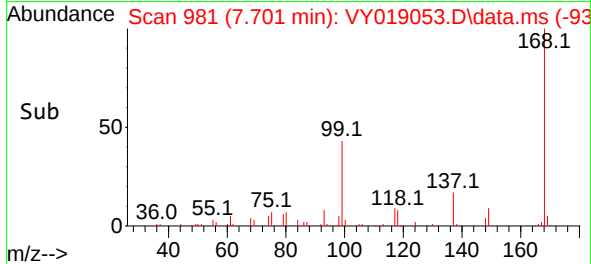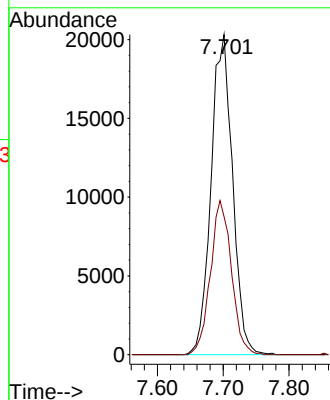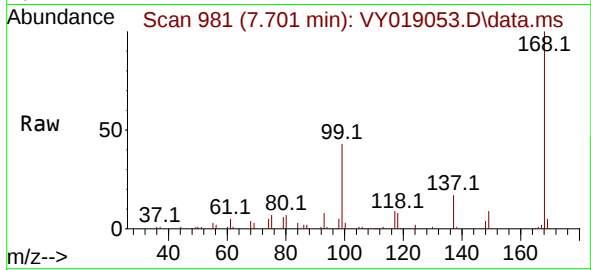

#33
1,2-Dichloroethane-d4
Concen: 48.034 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. -0.000 min
Lab File: VY019053.D
Acq: 14 Aug 2024 12:58

Tgt Ion: 65 Resp: 19474
Ion Ratio Lower Upper
65 100
67 54.5 0.0 109.6

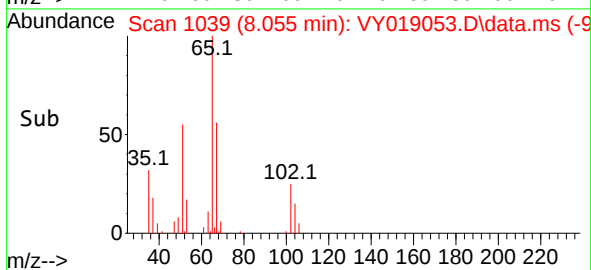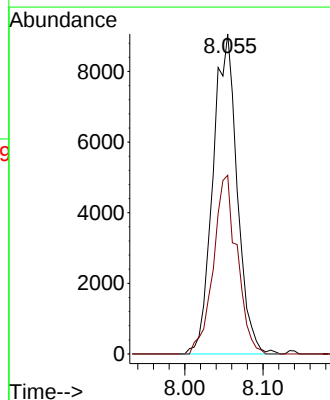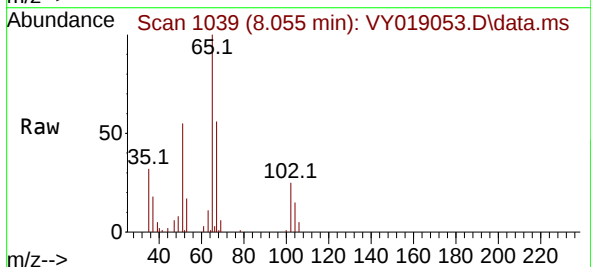

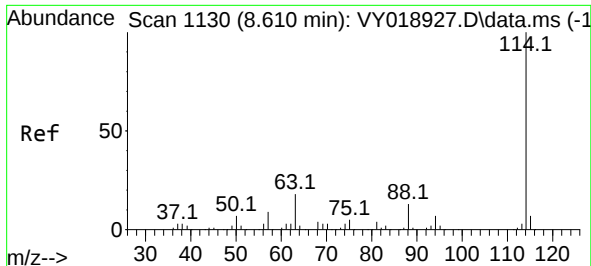

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.603 min Scan# 1130

Delta R.T. -0.006 min

Lab File: VY019053.D

Acq: 14 Aug 2024 12:58

Instrument :

MSVOA_Y

ClientSampleId :

VCPS-B1-081224-0-16





Tgt Ion:114 Resp: 75661

Ion Ratio Lower Upper

114 100

63 18.1 0.0 35.0

88 12.0 0.0 27.2

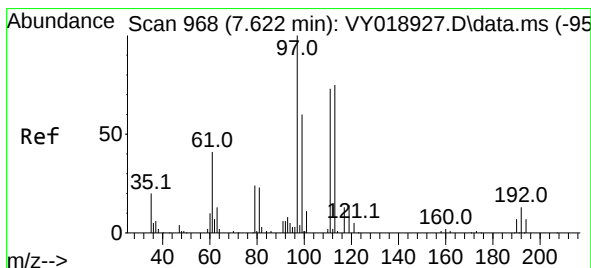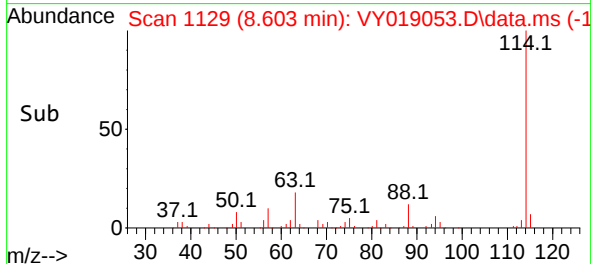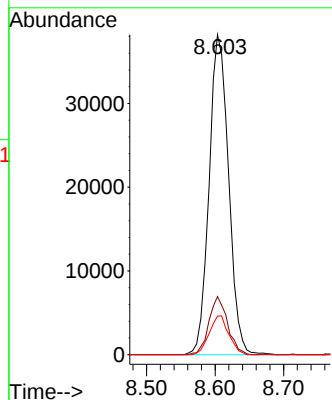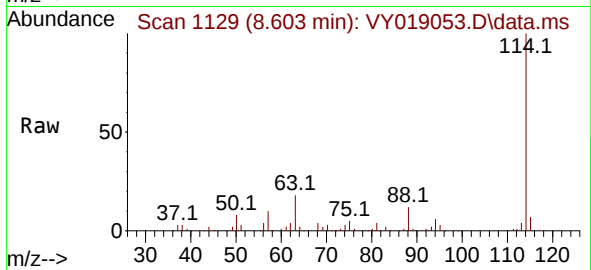

#35

Dibromofluoromethane

Concen: 51.786 ug/l

RT: 7.622 min Scan# 968

Delta R.T. -0.000 min

Lab File: VY019053.D

Acq: 14 Aug 2024 12:58




Tgt Ion:113 Resp: 25025


Ion Ratio Lower Upper

113 100

111 99.6 82.2 123.4

192 21.0 15.9 23.9

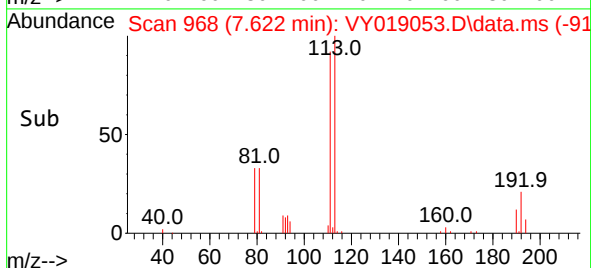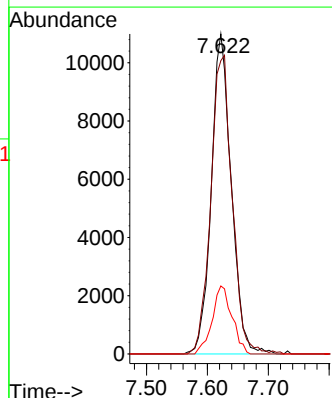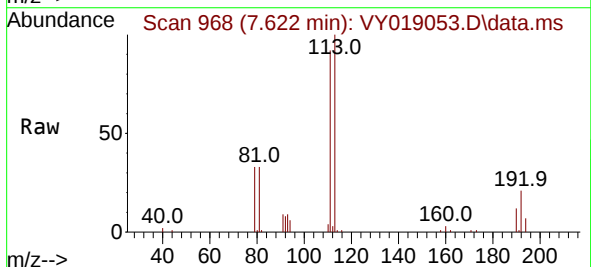

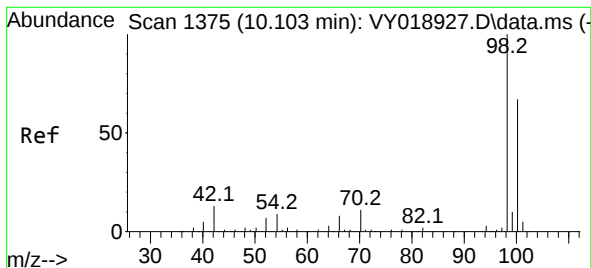

#50

Toluene-d8

Concen: 45.482 ug/l

RT: 10.103 min Scan# 1

Delta R.T. 0.000 min

Lab File: VY019053.D

Acq: 14 Aug 2024 12:58

Instrument :

MSVOA_Y

ClientSampleId :





VCPS-B1-081224-0-16

Tgt Ion: 98 Resp: 84420

Ion Ratio Lower Upper

98 100

100 66.9 52.0 78.0

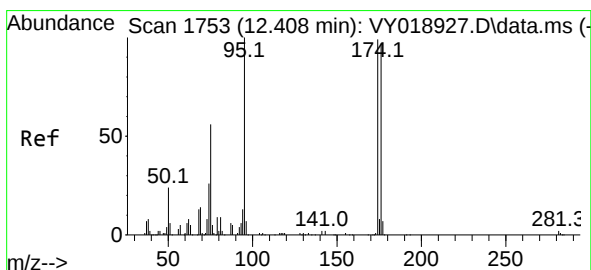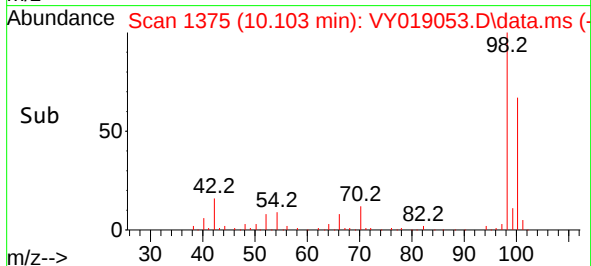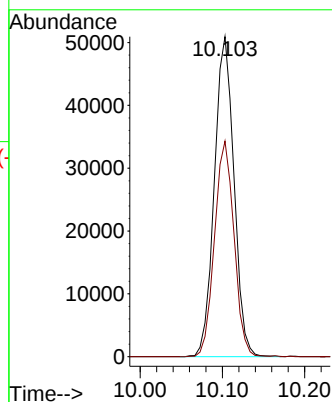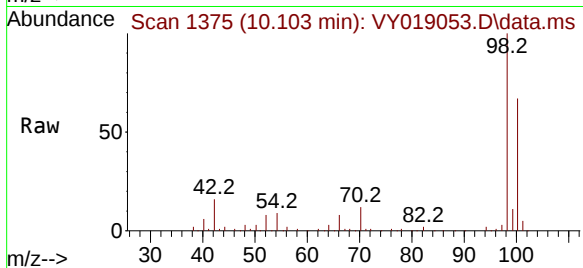

#62

4-Bromofluorobenzene

Concen: 27.591 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. -0.000 min

Lab File: VY019053.D

Acq: 14 Aug 2024 12:58




Tgt Ion: 95 Resp: 15194


Ion Ratio Lower Upper

95 100

174 106.8 0.0 175.6

176 103.8 0.0 171.4

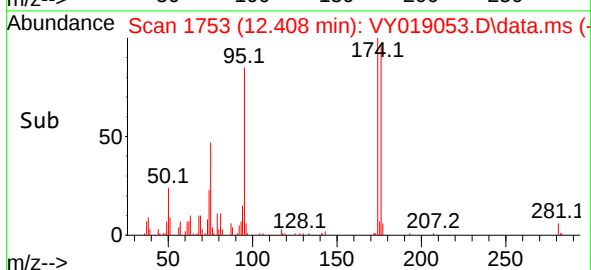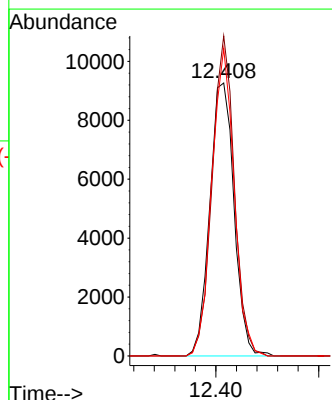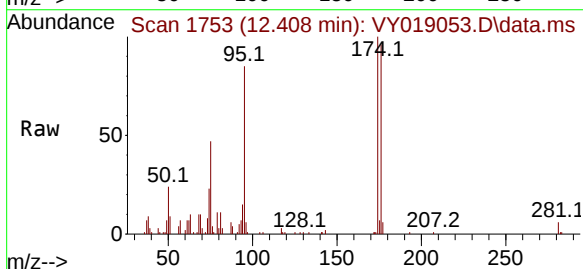

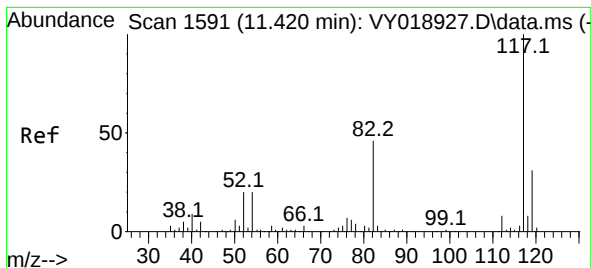

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY019053.D

Acq: 14 Aug 2024 12:58

Instrument :

MSVOA_Y

ClientSampleId :

VCPS-B1-081224-0-16





Tgt Ion:117 Resp: 55325

Ion Ratio Lower Upper

117 100

82 50.8 42.4 63.6

119 32.2 25.9 38.9

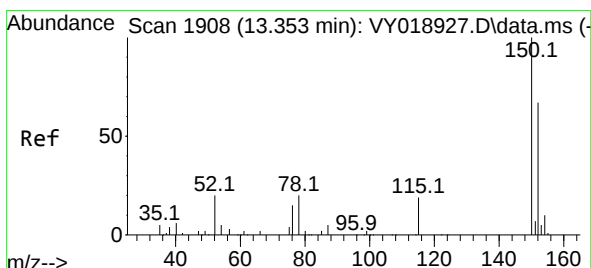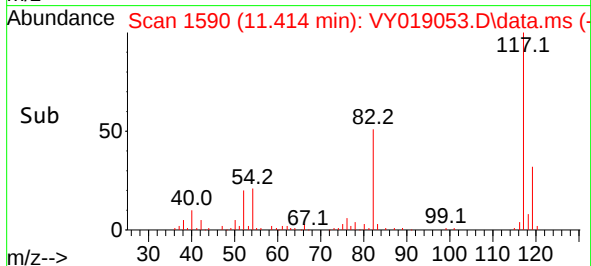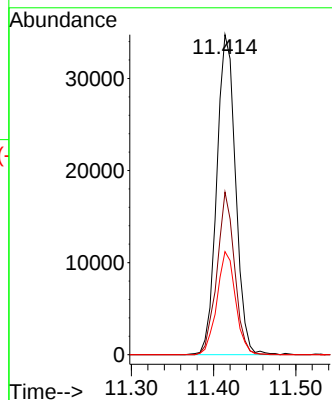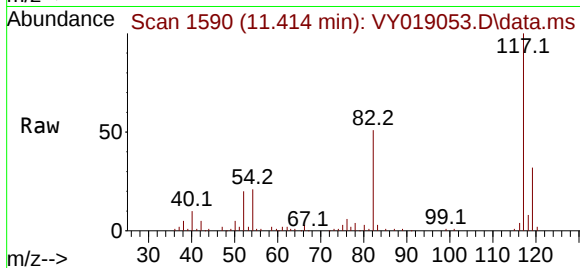

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.006 min

Lab File: VY019053.D

Acq: 14 Aug 2024 12:58

Tgt Ion:152 Resp: 15022

Ion Ratio Lower Upper

152 100

115 49.3 28.2 84.7

150 148.3 0.0 345.6

