
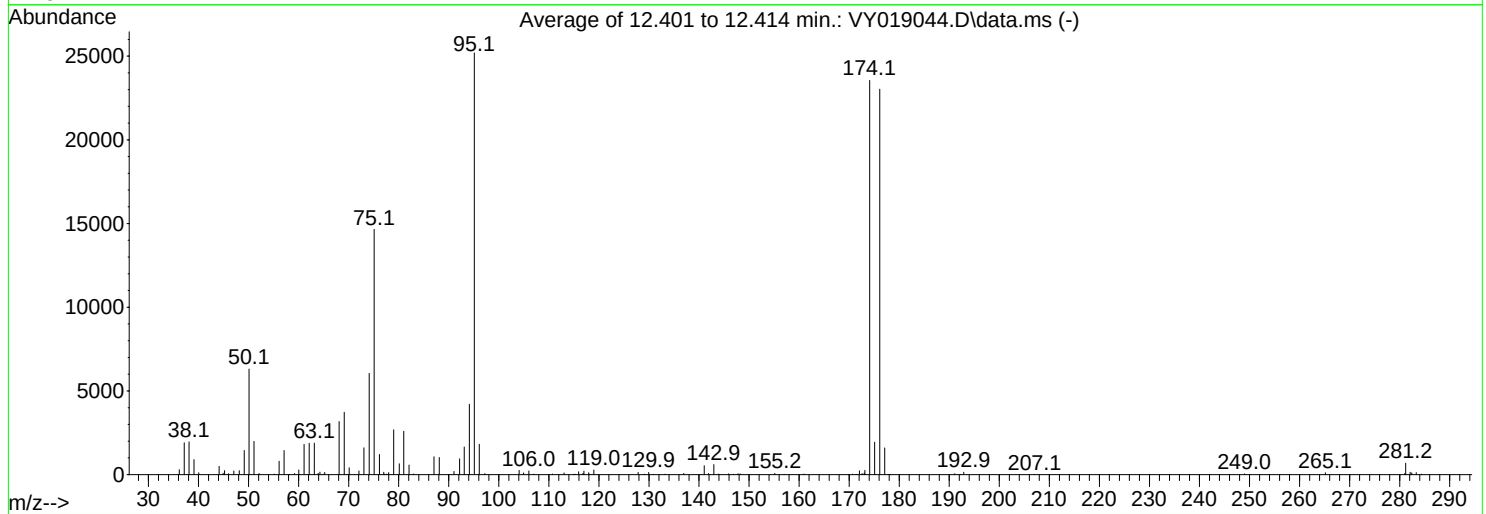


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081424\
Data File : VY019044.D
Acq On : 14 Aug 2024 08:36
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080824S.M
Title : SW846 8260
Last Update : Wed Aug 14 22:08:26 2024

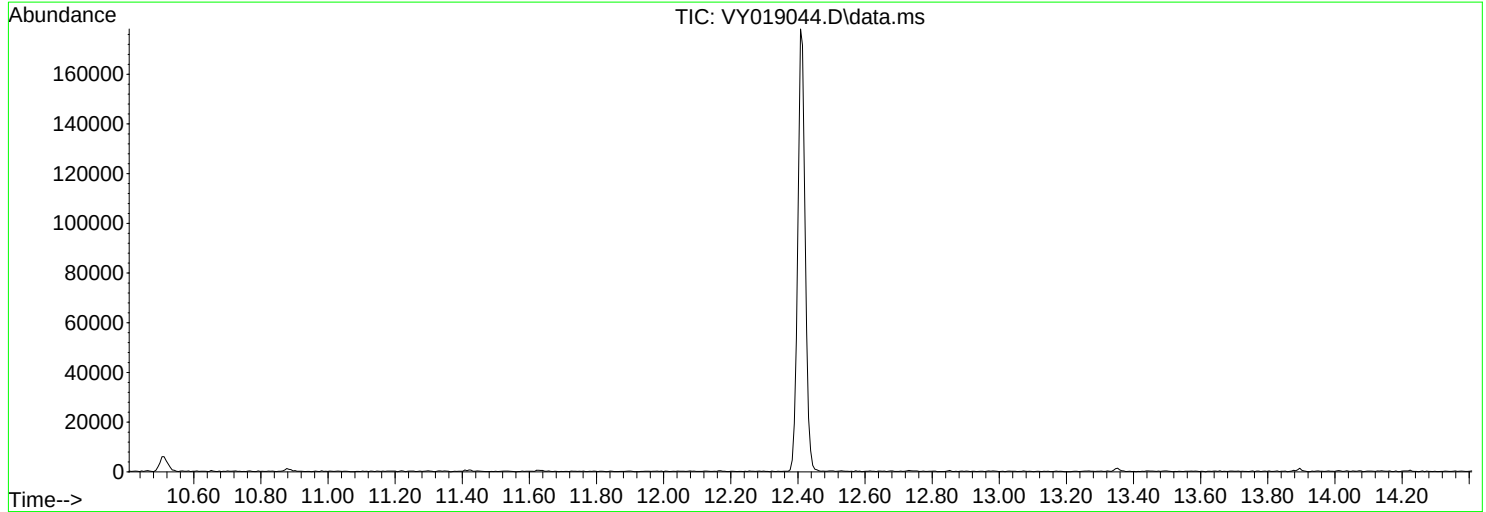

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	6307	PASS
75	95	30	60	58.1	14650	PASS
95	95	100	100	100.0	25197	PASS
96	95	5	9	7.2	1814	PASS
173	174	0.00	2	1.1	260	PASS
174	95	50	100	93.5	23555	PASS
175	174	5	9	8.2	1936	PASS
176	174	95	101	97.7	23025	PASS
177	176	5	9	6.9	1595	PASS