

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082025\
 Data File : VY023177.D
 Acq On : 20 Aug 2025 15:45
 Operator : SY/MD
 Sample : Q2892-07
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 3-FLOOR-NORTH-D

Quant Time: Aug 21 01:40:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	496959	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	948133	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	845587	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.340	152	329619	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	269775	56.958	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.920%
35) Dibromofluoromethane	7.634	113	299461	52.784	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.560%
50) Toluene-d8	10.109	98	1153895	52.063	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	104.120%
62) 4-Bromofluorobenzene	12.402	95	330174	46.323	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	92.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082025\
Data File : VY023177.D
Acq On : 20 Aug 2025 15:45
Operator : SY/MD
Sample : Q2892-07
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
3-FLOOR-NORTH-D

Quant Time: Aug 21 01:40:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration




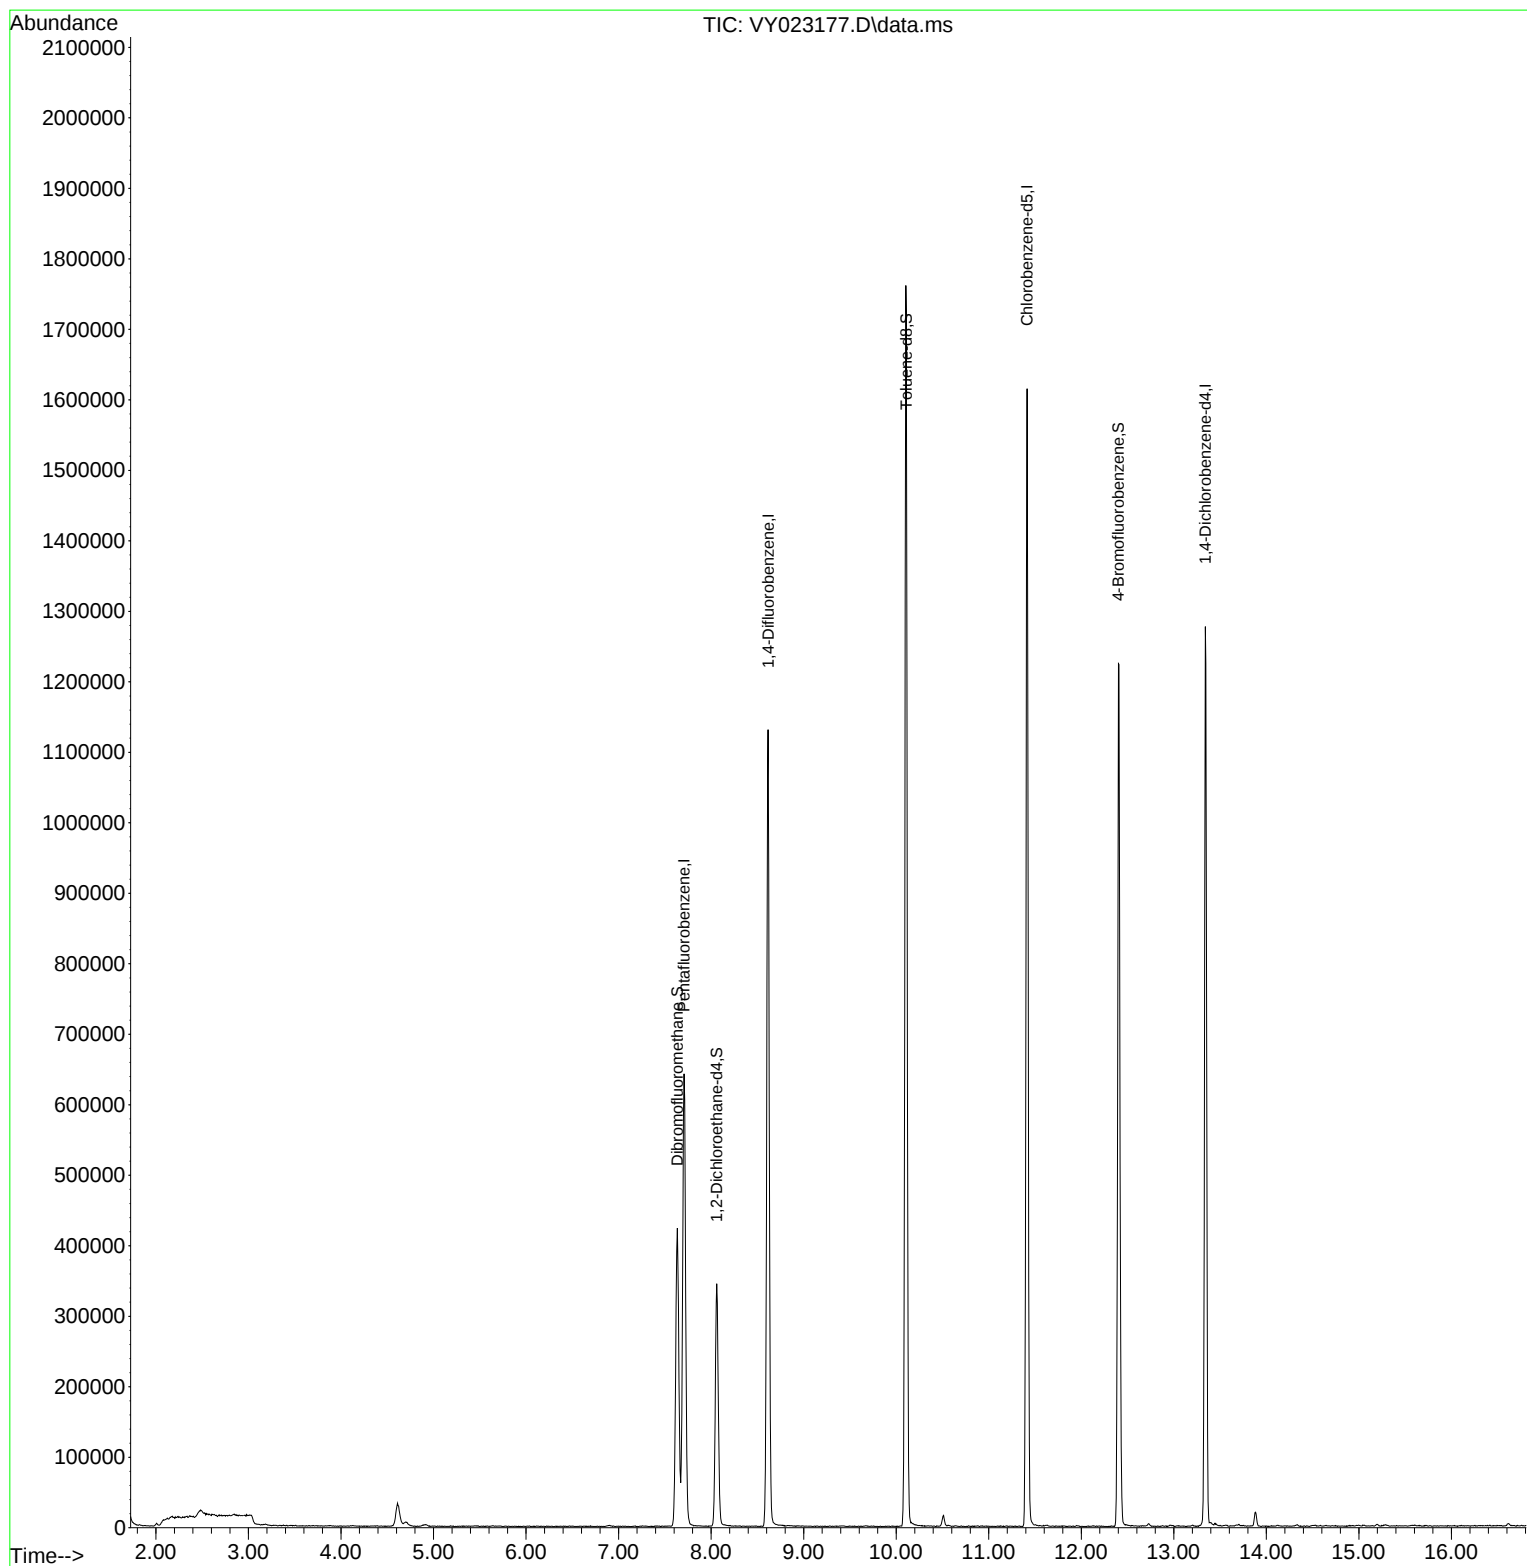


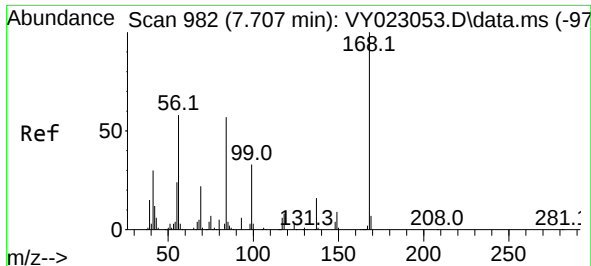

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY023177.D
Acq: 20 Aug 2025 15:45




Instrument :
MSVOA_Y
ClientSampleId :
3-FLOOR-NORTH-D


Tgt Ion:168 Resp: 496959
Ion Ratio Lower Upper
168 100
99 55.2 42.8 64.2

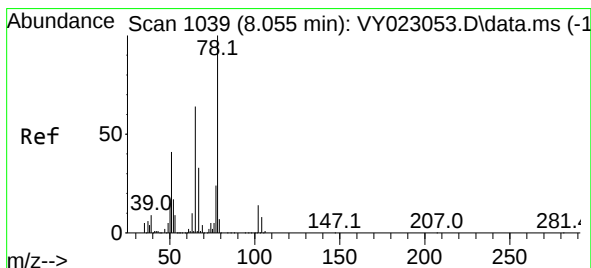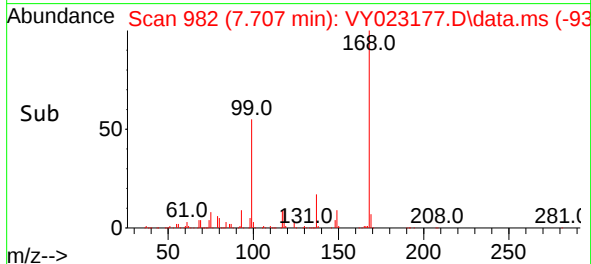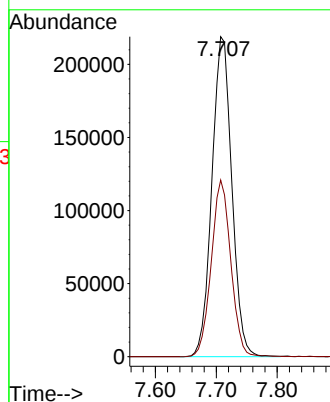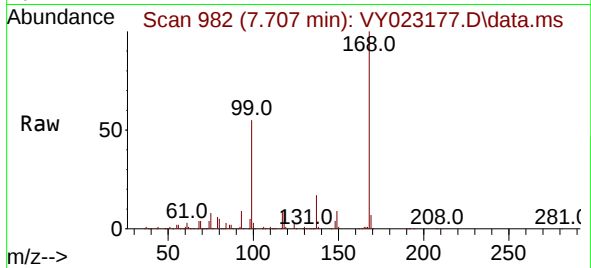

#33
1,2-Dichloroethane-d4
Concen: 56.958 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023177.D
Acq: 20 Aug 2025 15:45

Tgt Ion: 65 Resp: 269775
Ion Ratio Lower Upper
65 100
67 52.6 0.0 106.8


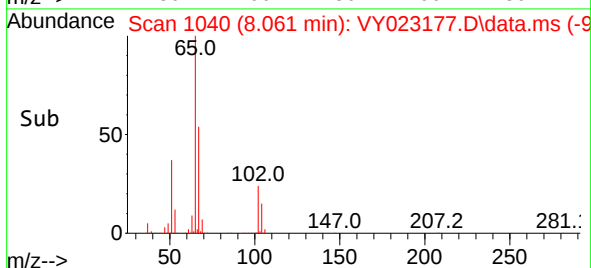
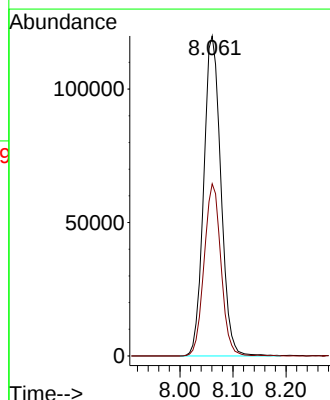
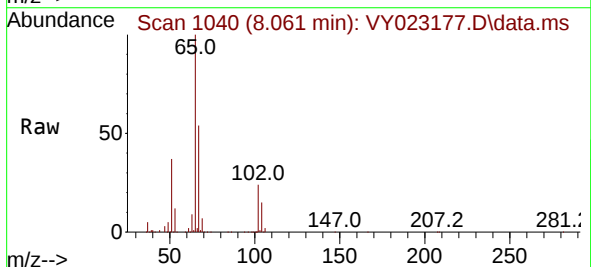


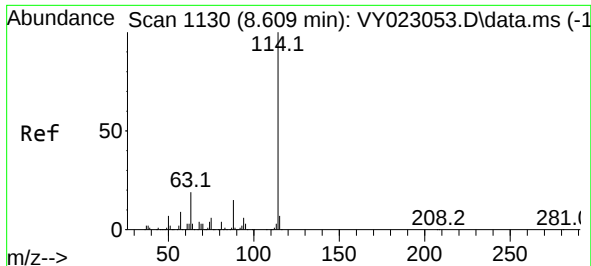

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VY023177.D
Acq: 20 Aug 2025 15:45




Instrument :
MSVOA_Y
ClientSampleId :
3-FLOOR-NORTH-D


Tgt Ion:114 Resp: 948133
Ion Ratio Lower Upper
114 100
63 18.6 0.0 38.4
88 14.8 0.0 30.0

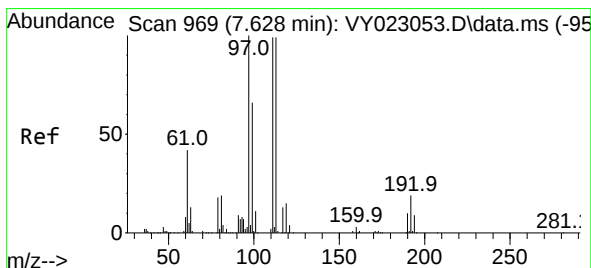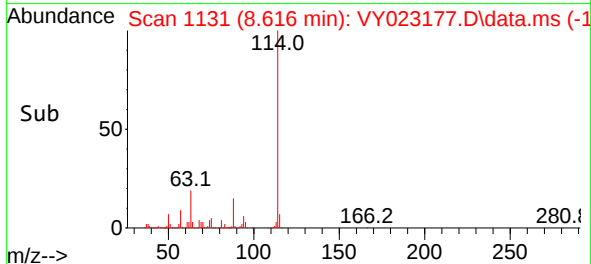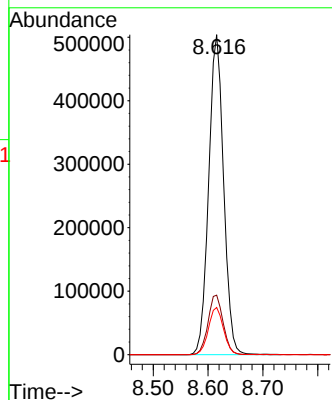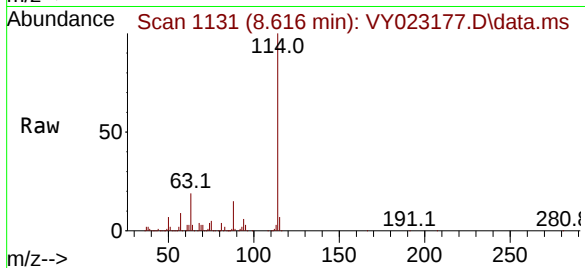

#35
Dibromofluoromethane
Concen: 52.784 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY023177.D
Acq: 20 Aug 2025 15:45

Tgt Ion:113 Resp: 299461
Ion Ratio Lower Upper
113 100
111 103.1 81.1 121.7
192 19.9 16.2 24.4


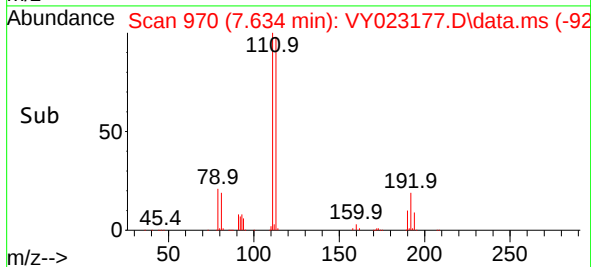
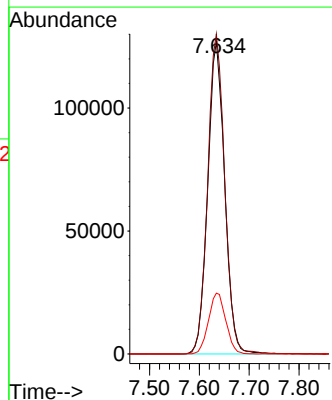
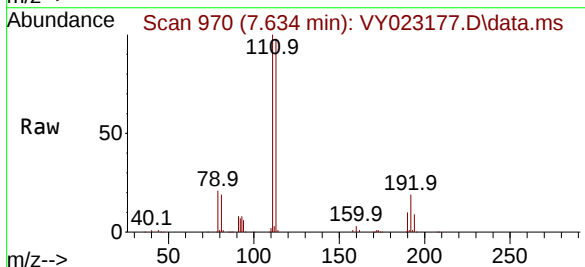


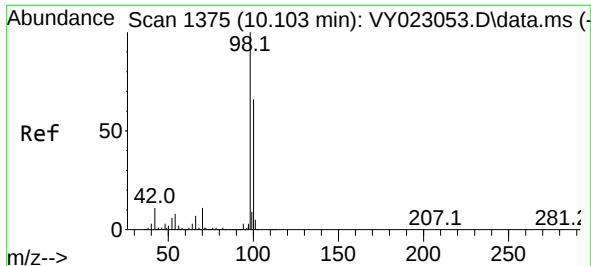

#50
Toluene-d8
Concen: 52.063 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023177.D
Acq: 20 Aug 2025 15:45




Instrument :
MSVOA_Y
ClientSampleId :
3-FLOOR-NORTH-D


Tgt Ion: 98 Resp: 1153895
Ion Ratio Lower Upper
98 100
100 64.7 52.3 78.5

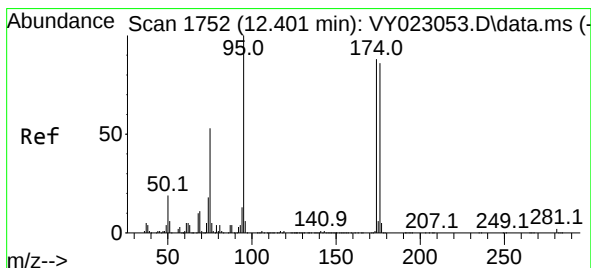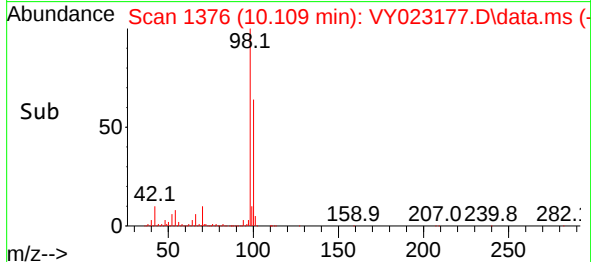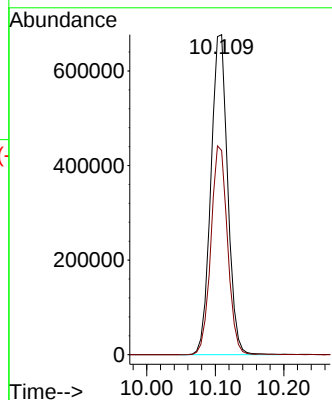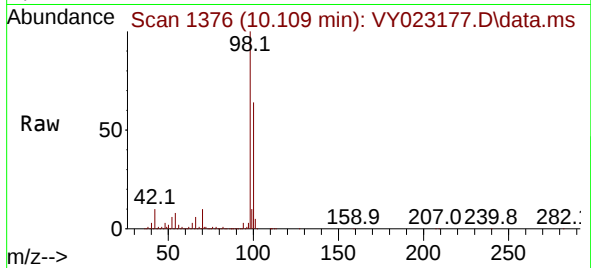

#62
4-Bromofluorobenzene
Concen: 46.323 ug/l
RT: 12.402 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VY023177.D
Acq: 20 Aug 2025 15:45

Tgt Ion: 95 Resp: 330174
Ion Ratio Lower Upper
95 100
174 88.0 0.0 171.6
176 85.2 0.0 167.6

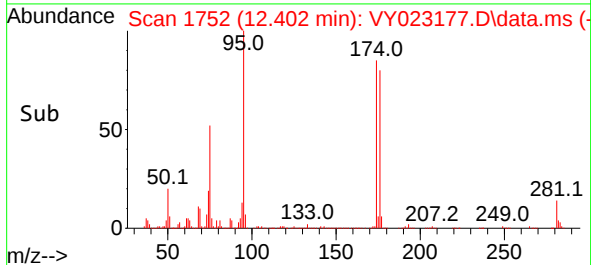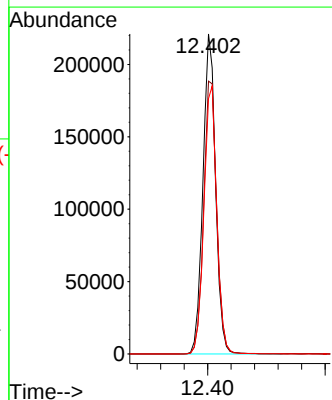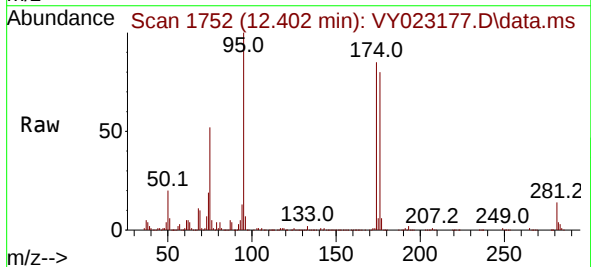

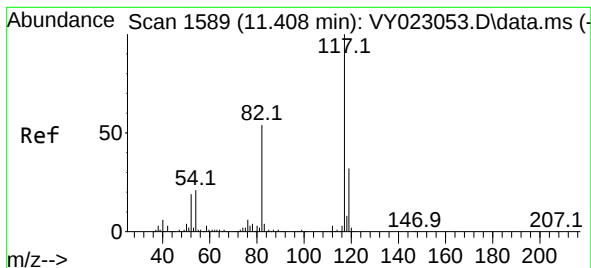

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY023177.D

Acq: 20 Aug 2025 15:45

Instrument :

MSVOA_Y

ClientSampleId :

3-FLOOR-NORTH-D





Tgt Ion:117 Resp: 845587

Ion Ratio Lower Upper

117 100

82 54.0 43.4 65.0

119 32.1 25.6 38.4

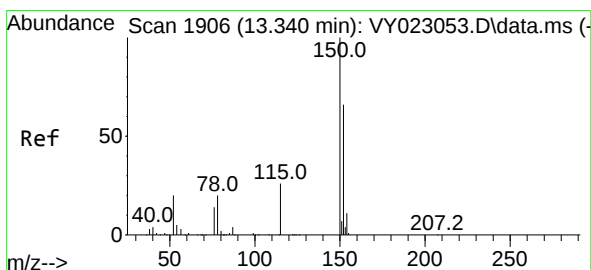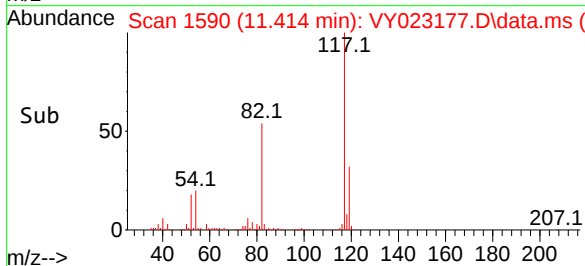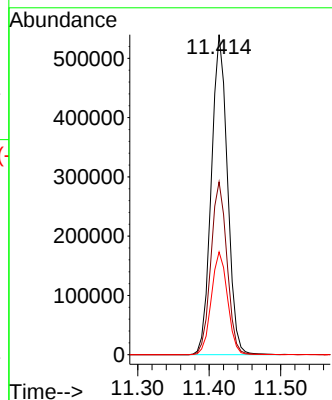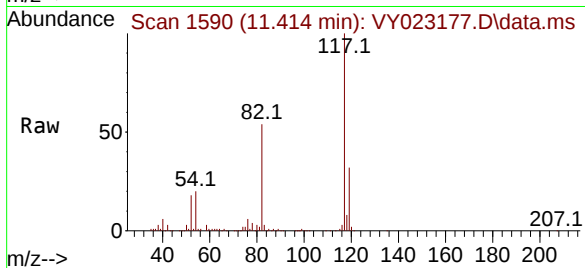

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.340 min Scan# 1906

Delta R.T. 0.000 min

Lab File: VY023177.D

Acq: 20 Aug 2025 15:45

Tgt Ion:152 Resp: 329619

Ion Ratio Lower Upper

152 100

115 56.4 28.2 84.6

150 157.2 0.0 348.0

