


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082124\
Data File : VY019165.D
Acq On : 21 Aug 2024 12:15
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Title : SW846 8260
Last Update : Fri Aug 16 05:10:30 2024

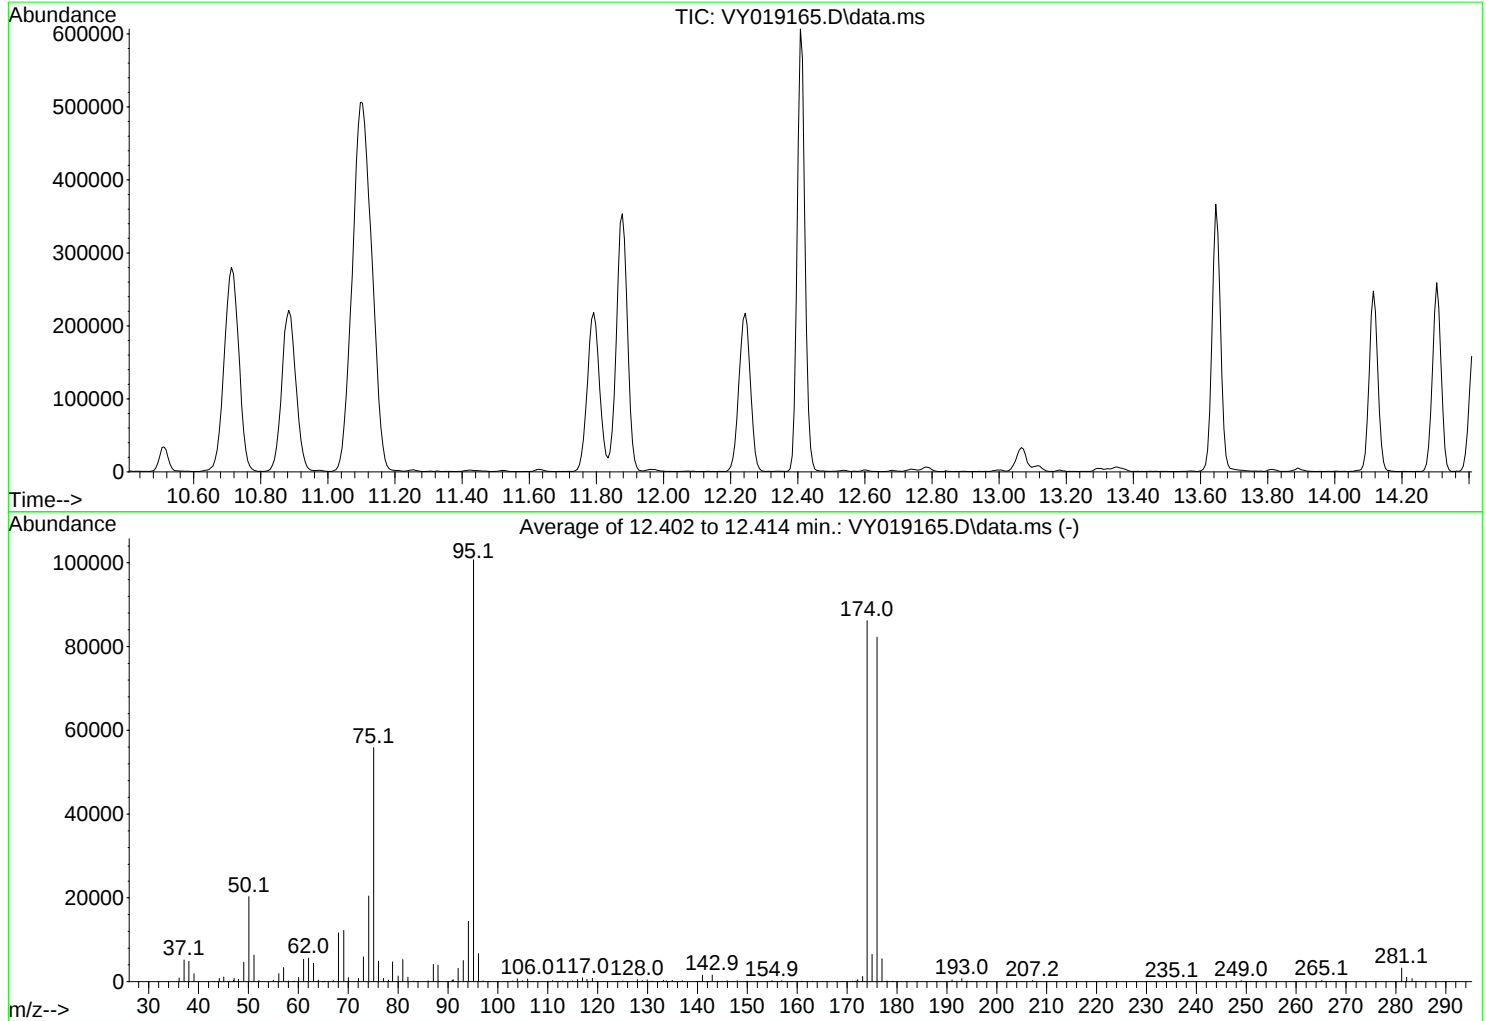

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	20275	PASS
75	95	30	60	55.5	55899	PASS
95	95	100	100	100.0	100707	PASS
96	95	5	9	6.7	6703	PASS
173	174	0.00	2	1.4	1211	PASS
174	95	50	100	85.6	86179	PASS
175	174	5	9	7.6	6552	PASS
176	174	95	101	95.4	82253	PASS
177	176	5	9	6.6	5454	PASS