

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082225\
 Data File : VY023191.D
 Acq On : 22 Aug 2025 14:27
 Operator : SY/MD
 Sample : Q2917-01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 OR-02-082025

Quant Time: Aug 25 05:17:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 13 02:10:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	36308	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.615	114	47542	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	31437	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	6317	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	13065	37.756	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	75.520%
35) Dibromofluoromethane	7.634	113	12049	42.355	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	84.720%
50) Toluene-d8	10.109	98	48621	43.750	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	87.500%
62) 4-Bromofluorobenzene	12.401	95	8571	23.981	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	47.960%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082225\
Data File : VY023191.D
Acq On : 22 Aug 2025 14:27
Operator : SY/MD
Sample : Q2917-01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
OR-02-082025

Quant Time: Aug 25 05:17:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081225S.M
Quant Title : SW846 8260
QLast Update : Wed Aug 13 02:10:11 2025
Response via : Initial Calibration



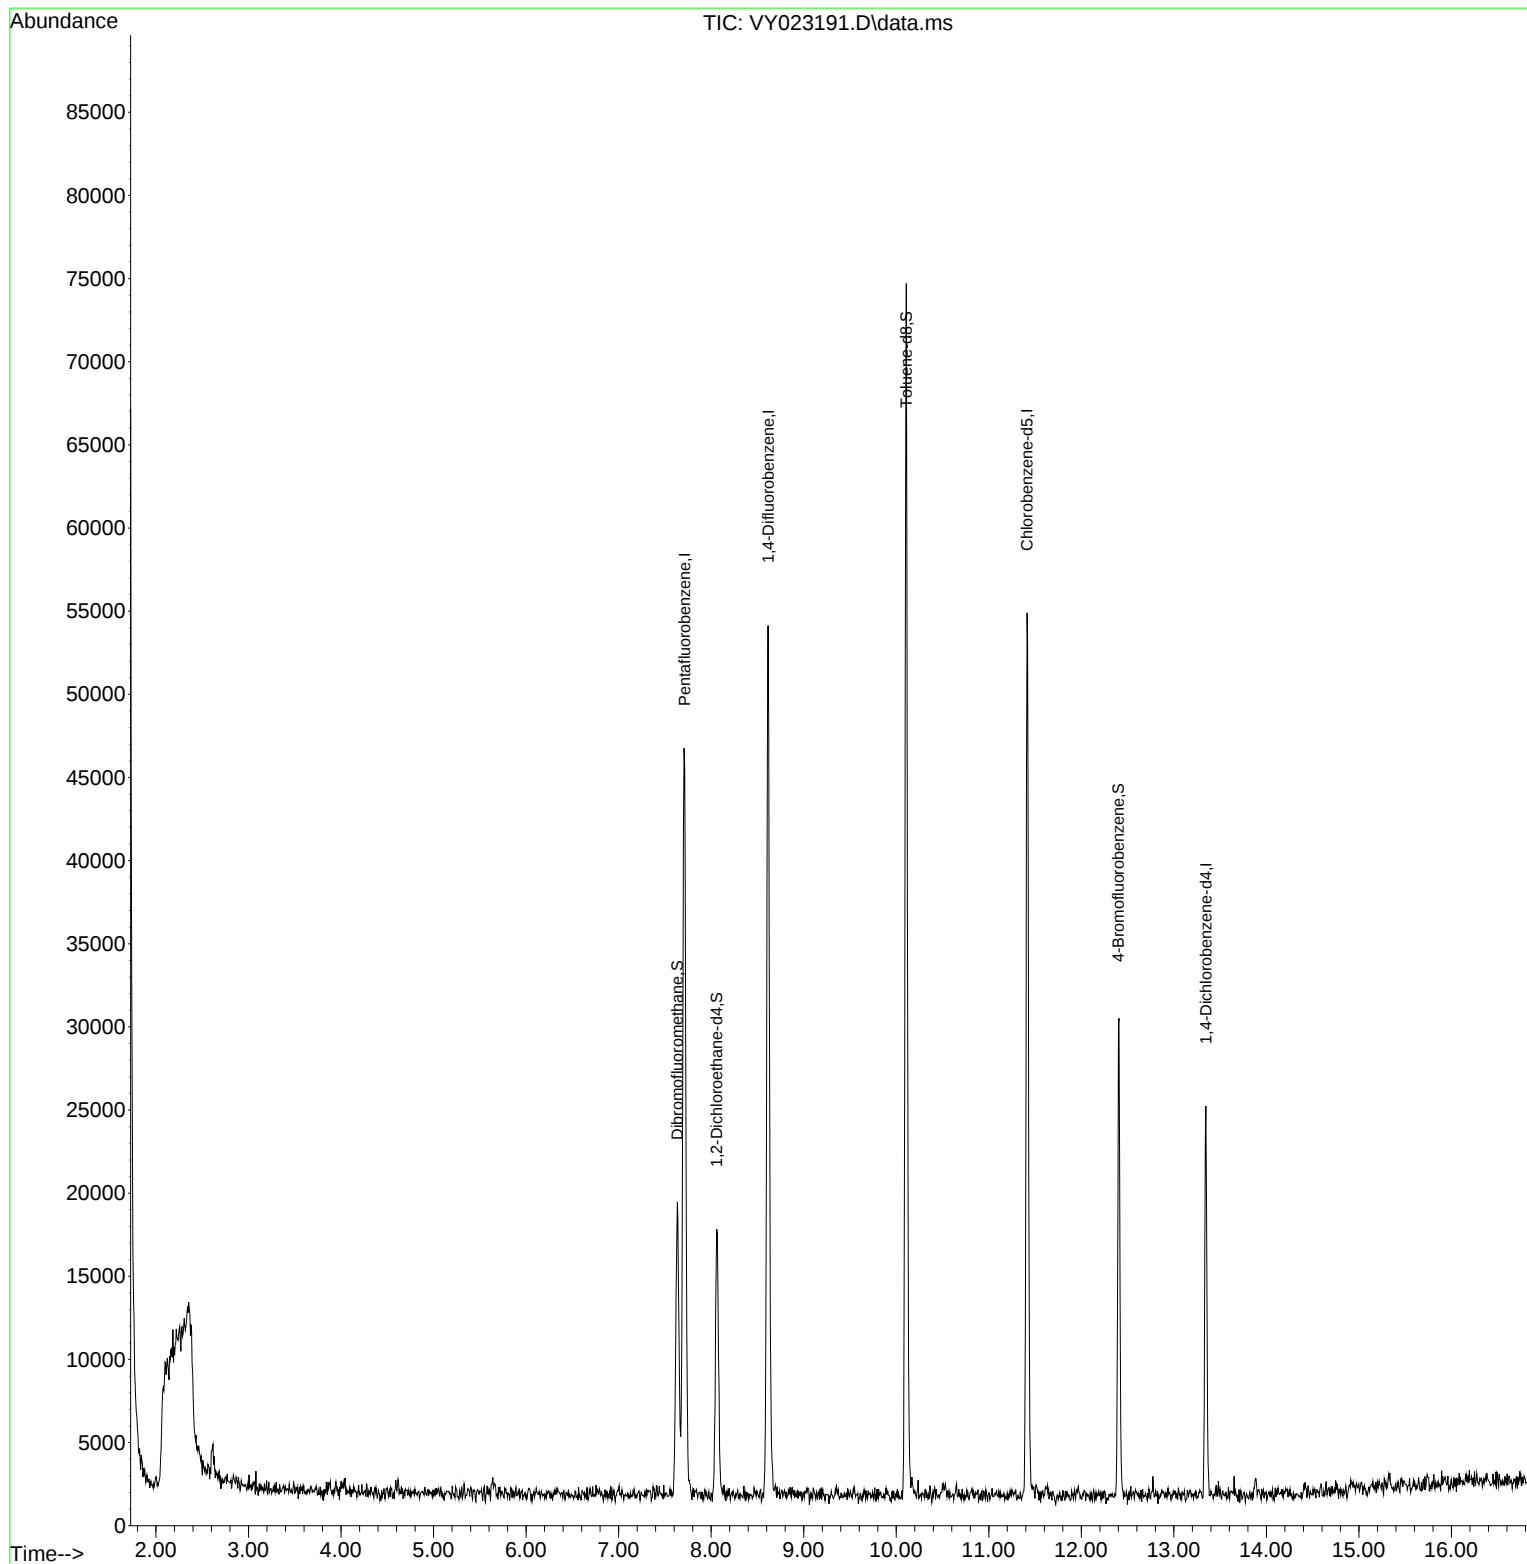




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023191.D
Acq: 22 Aug 2025 14:27




Instrument :
MSVOA_Y
ClientSampleId :
OR-02-082025

Tgt Ion:168 Resp: 36308
Ion Ratio Lower Upper
168 100
99 55.4 42.8 64.2

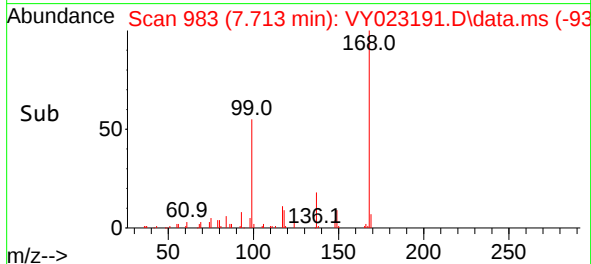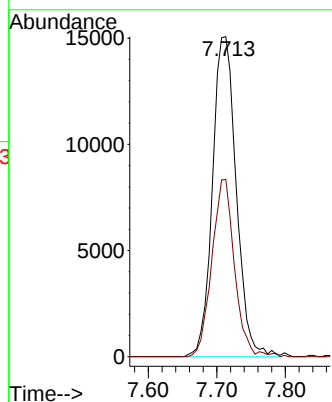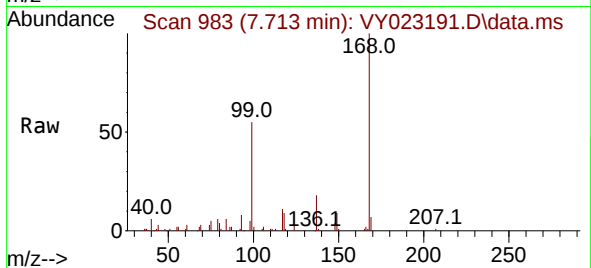

#33
1,2-Dichloroethane-d4
Concen: 37.756 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VY023191.D
Acq: 22 Aug 2025 14:27

Tgt Ion: 65 Resp: 13065
Ion Ratio Lower Upper
65 100
67 54.1 0.0 106.8

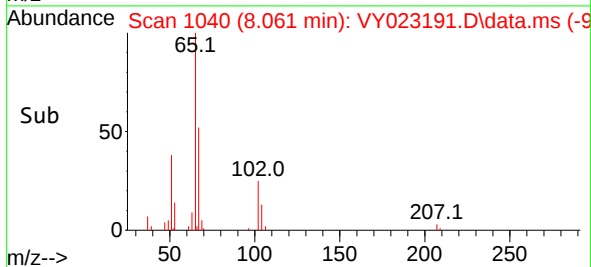
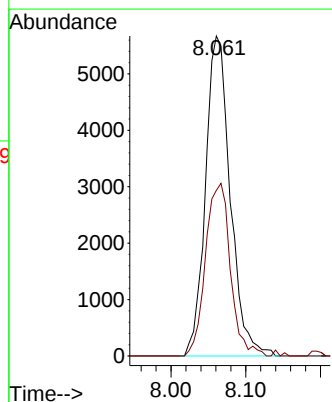
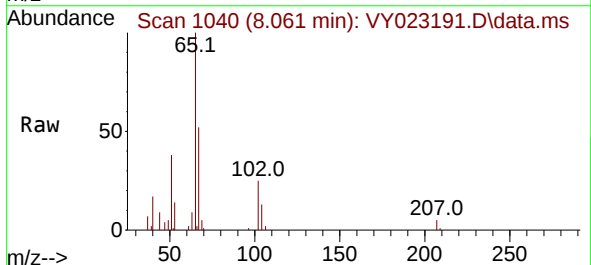




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.615 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VY023191.D
Acq: 22 Aug 2025 14:27




Instrument :
MSVOA_Y
ClientSampleId :
OR-02-082025


Tgt Ion:114 Resp: 47542
Ion Ratio Lower Upper
114 100
63 17.9 0.0 38.4
88 14.3 0.0 30.0

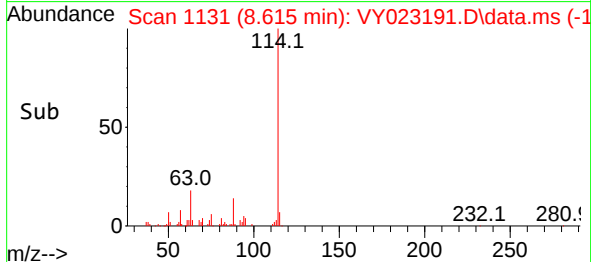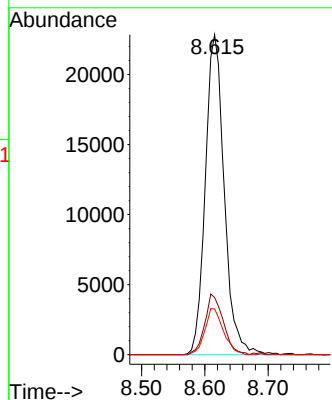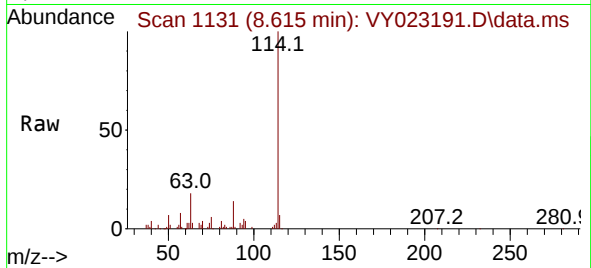

#35
Dibromofluoromethane
Concen: 42.355 ug/l
RT: 7.634 min Scan# 970
Delta R.T. 0.006 min
Lab File: VY023191.D
Acq: 22 Aug 2025 14:27

Tgt Ion:113 Resp: 12049
Ion Ratio Lower Upper
113 100
111 109.2 81.1 121.7
192 22.6 16.2 24.4


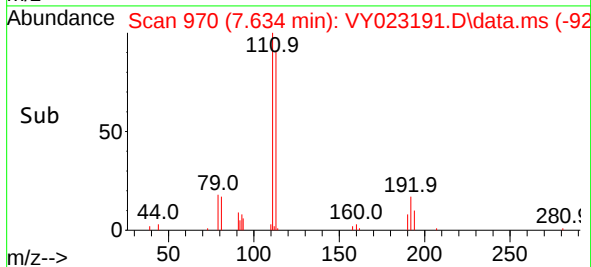
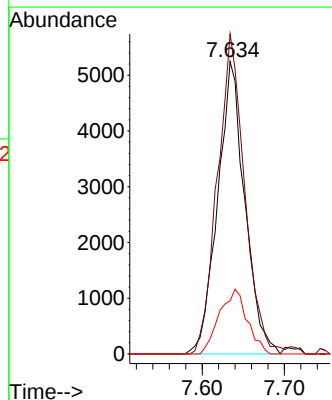
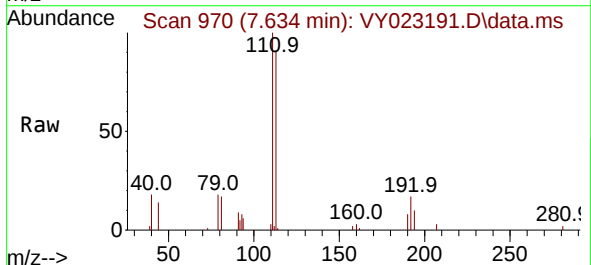


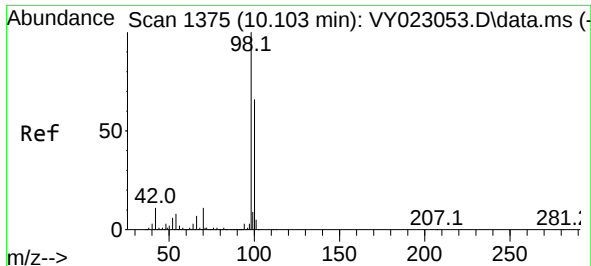

#50
Toluene-d8
Concen: 43.750 ug/l
RT: 10.109 min Scan# 1375
Delta R.T. 0.006 min
Lab File: VY023191.D
Acq: 22 Aug 2025 14:27




Instrument :
MSVOA_Y
ClientSampleId :
OR-02-082025


Tgt Ion: 98 Resp: 48621
Ion Ratio Lower Upper
98 100
100 66.2 52.3 78.5

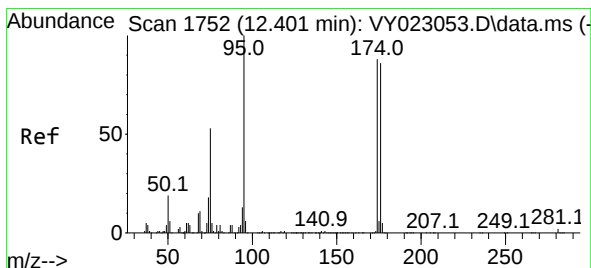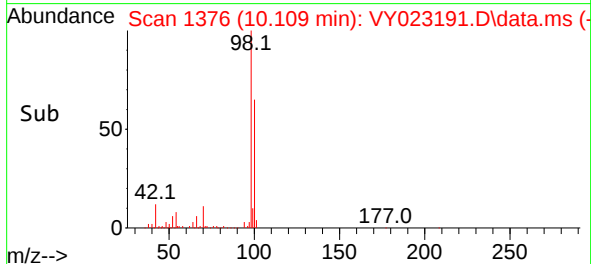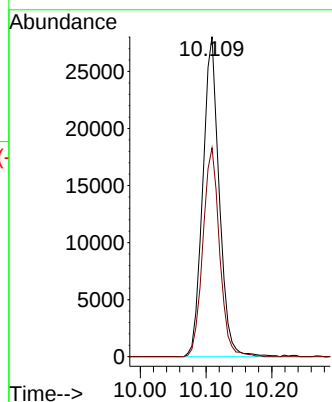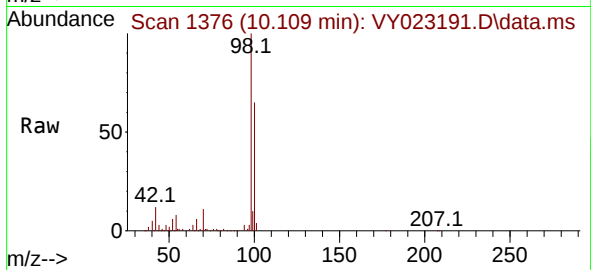

#62
4-Bromofluorobenzene
Concen: 23.981 ug/l
RT: 12.401 min Scan# 1752
Delta R.T. -0.000 min
Lab File: VY023191.D
Acq: 22 Aug 2025 14:27

Tgt Ion: 95 Resp: 8571
Ion Ratio Lower Upper
95 100
174 93.7 0.0 171.6
176 88.1 0.0 167.6

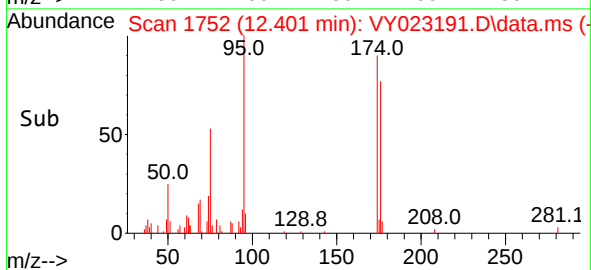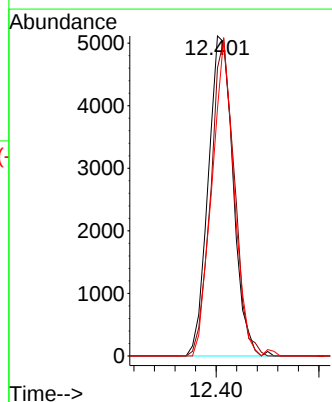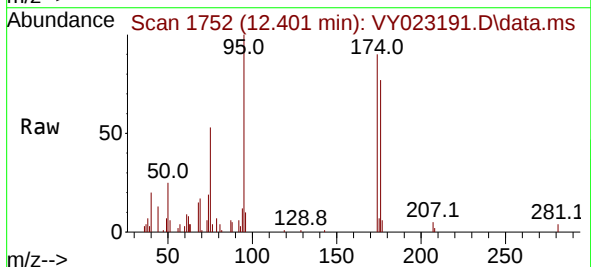

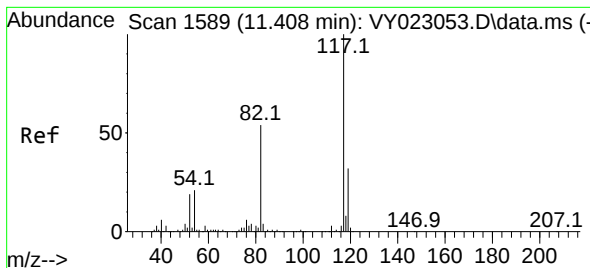

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY023191.D

Acq: 22 Aug 2025 14:27

Instrument :

MSVOA_Y

ClientSampleId :

OR-02-082025





Tgt Ion:117 Resp: 31437

Ion Ratio Lower Upper

117 100

82 54.9 43.4 65.0

119 30.3 25.6 38.4

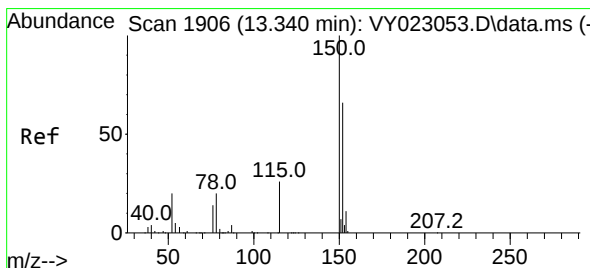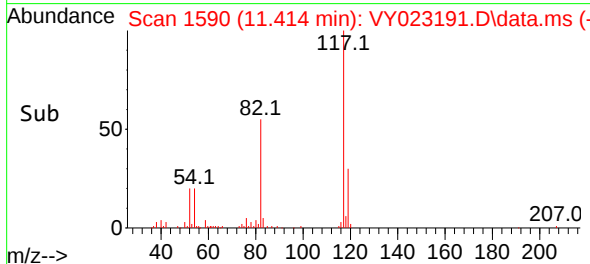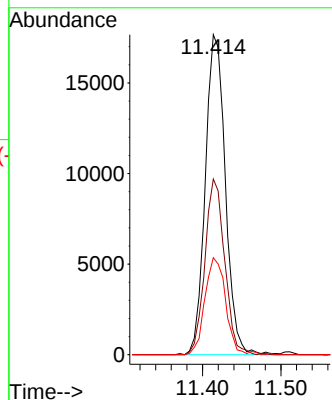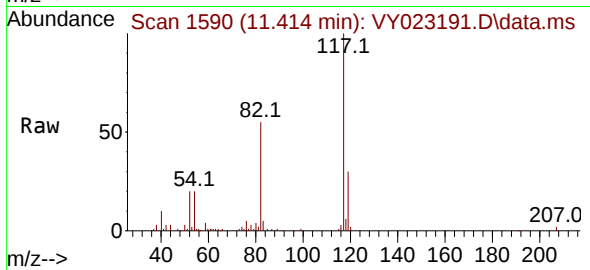

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.006 min

Lab File: VY023191.D

Acq: 22 Aug 2025 14:27

Tgt Ion:152 Resp: 6317

Ion Ratio Lower Upper

152 100

115 55.9 28.2 84.6

150 149.5 0.0 348.0

