

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082824\
 Data File : VY019326.D
 Acq On : 28 Aug 2024 13:27
 Operator : SY/MD
 Sample : VY0828SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0828SBL01

Quant Time: Aug 29 01:31:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 05:10:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	109356	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	191693	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	178659	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	69188	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	53216	48.546	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	97.100%
35) Dibromofluoromethane	7.628	113	61374	48.966	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.940%
50) Toluene-d8	10.103	98	218530	48.448	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.900%
62) 4-Bromofluorobenzene	12.407	95	66852	43.477	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	86.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082824\
Data File : VY019326.D
Acq On : 28 Aug 2024 13:27
Operator : SY/MD
Sample : VY0828SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0828SBL01

Quant Time: Aug 29 01:31:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 05:10:30 2024
Response via : Initial Calibration




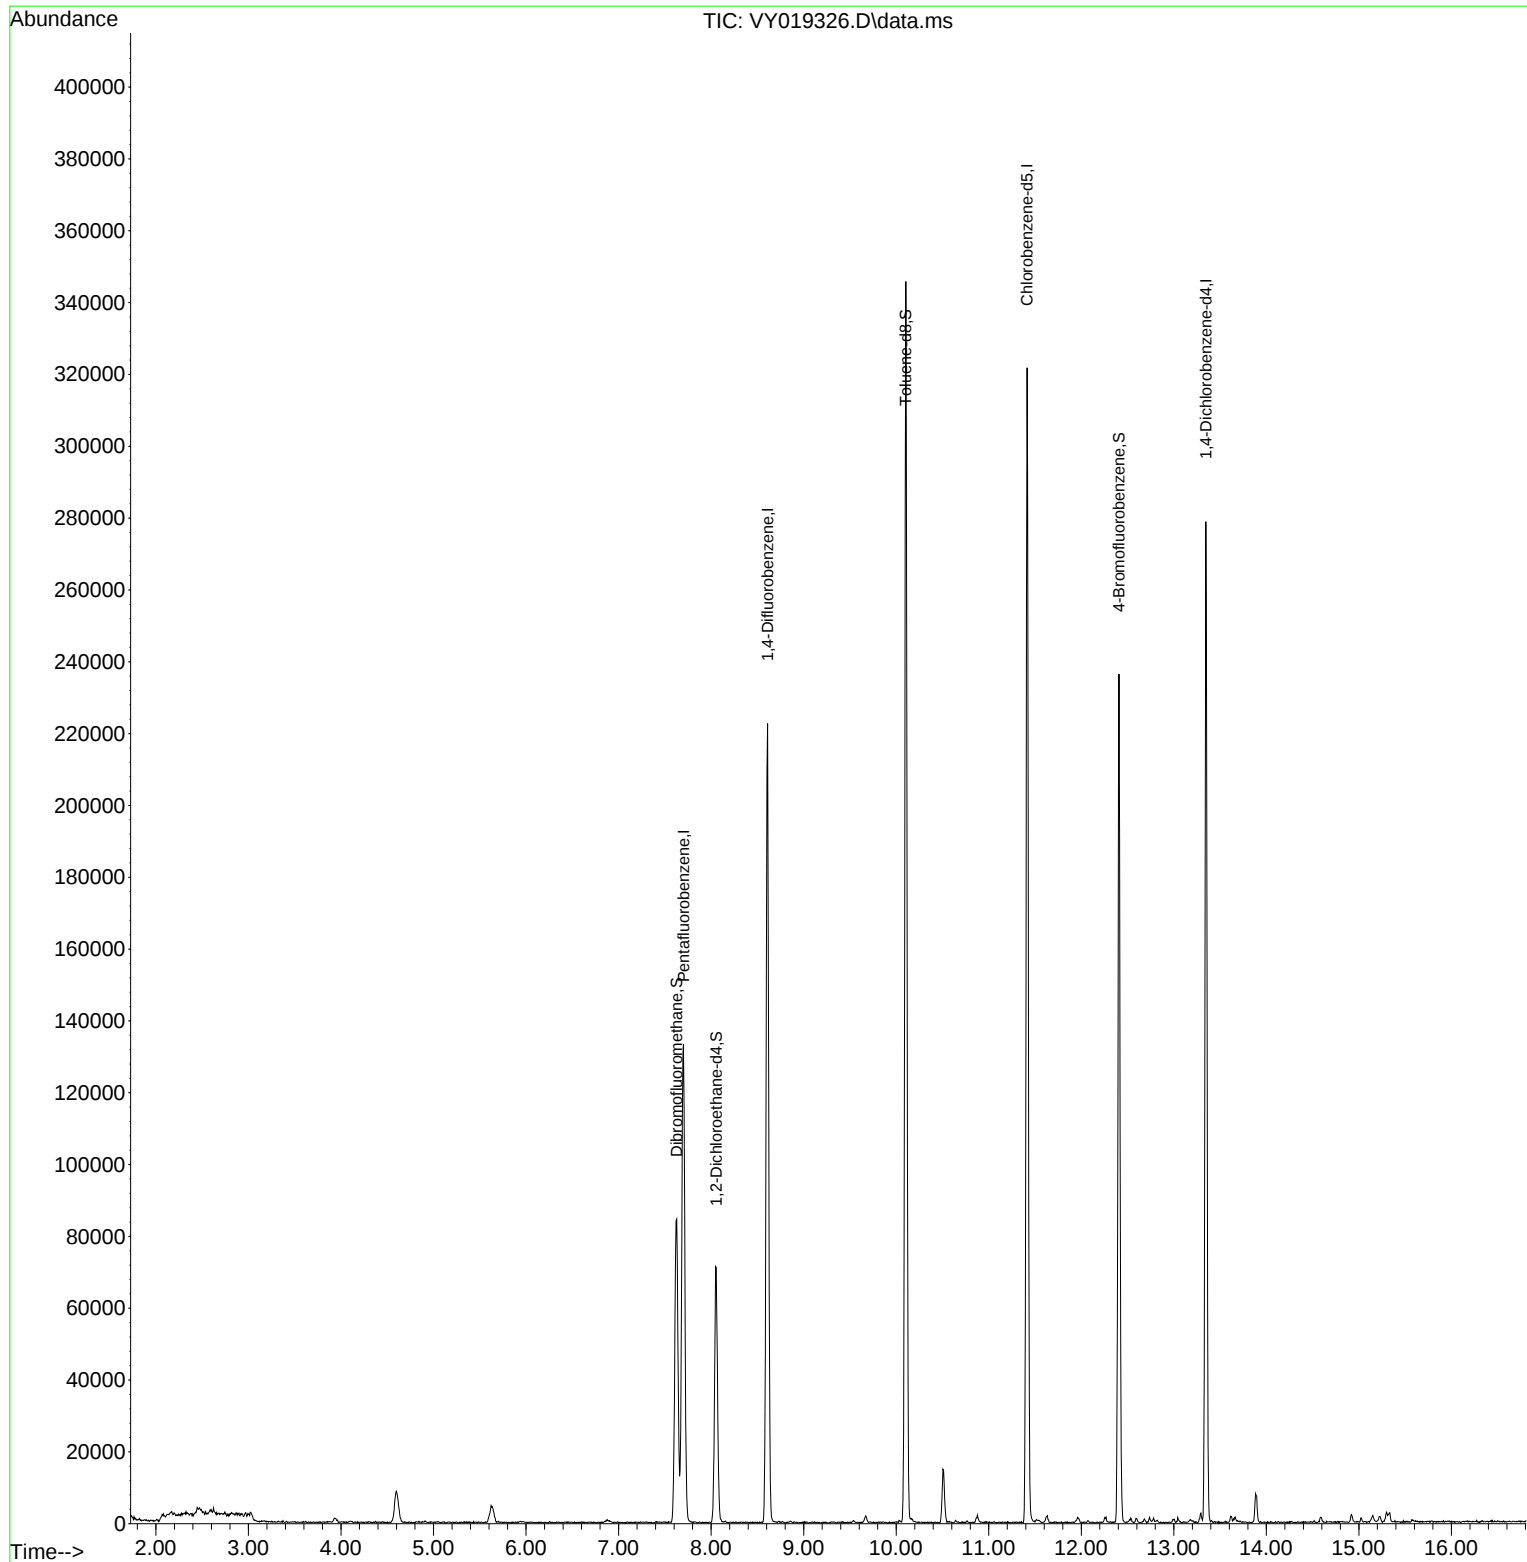


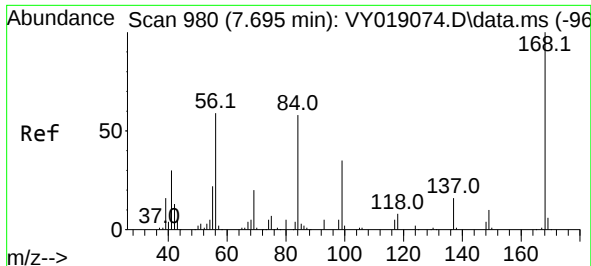

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY019326.D
Acq: 28 Aug 2024 13:27




Instrument :
MSVOA_Y
ClientSampleId :
VY0828SBL01

Tgt Ion:168 Resp: 109356
Ion Ratio Lower Upper
168 100
99 50.0 39.1 58.7

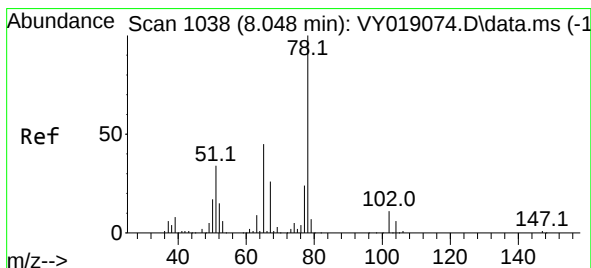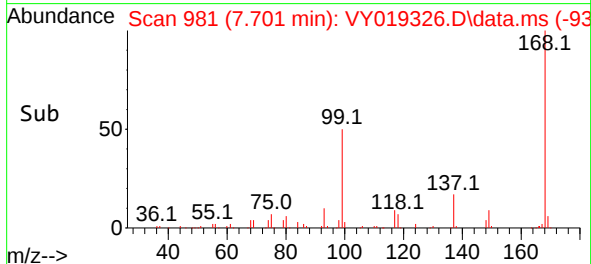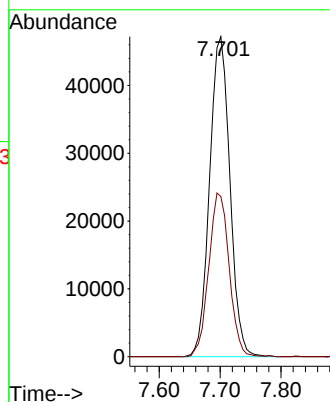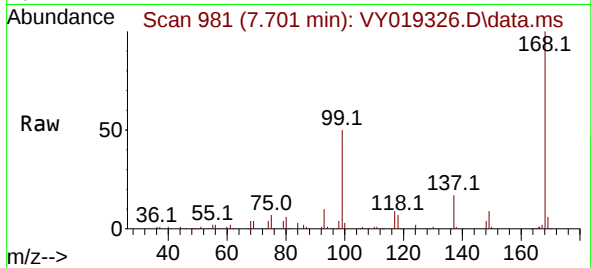

#33
1,2-Dichloroethane-d4
Concen: 48.546 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY019326.D
Acq: 28 Aug 2024 13:27

Tgt Ion: 65 Resp: 53216
Ion Ratio Lower Upper
65 100
67 53.3 0.0 109.6

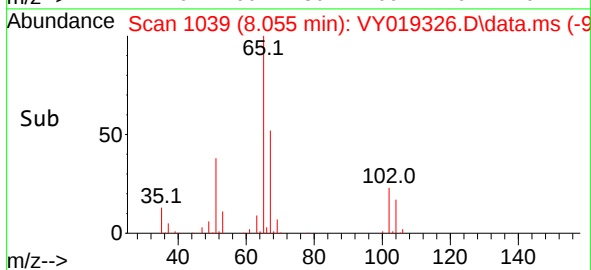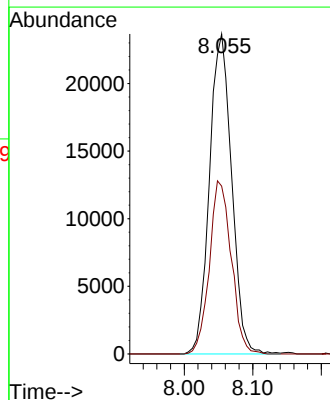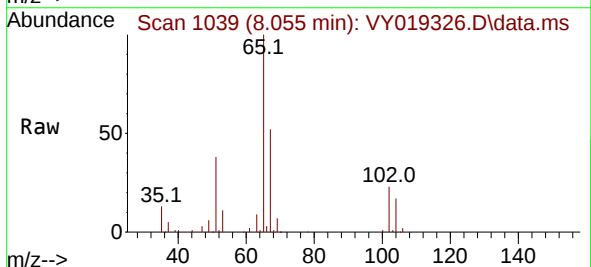



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.609 min Scan# 1129

Delta R.T. 0.006 min

Lab File: VY019326.D

Acq: 28 Aug 2024 13:27

Instrument :

MSVOA_Y

ClientSampleId :

VY0828SBL01




Tgt Ion:114 Resp: 191693

Ion Ratio Lower Upper

114 100

63 18.4 0.0 35.0

88 14.2 0.0 27.2

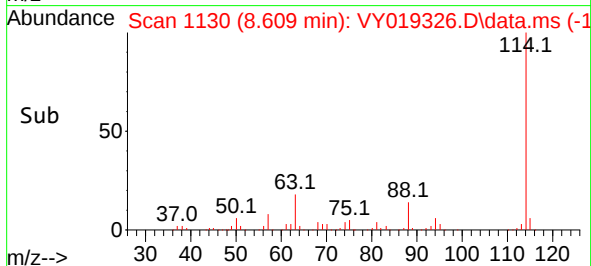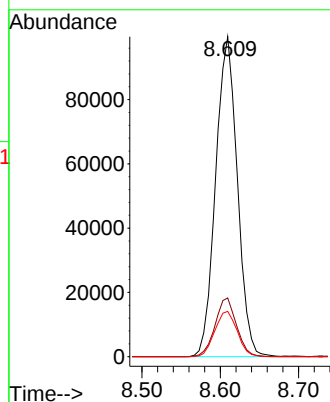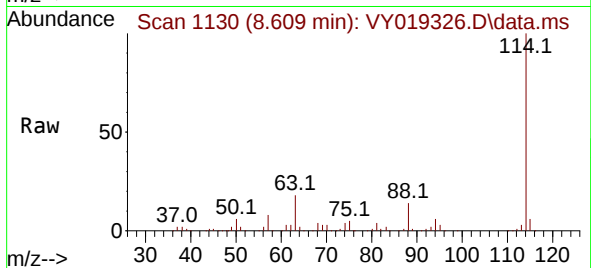

#35

Dibromofluoromethane

Concen: 48.966 ug/l

RT: 7.628 min Scan# 969

Delta R.T. 0.006 min

Lab File: VY019326.D

Acq: 28 Aug 2024 13:27




Tgt Ion:113 Resp: 61374


Ion Ratio Lower Upper

113 100

111 101.5 82.2 123.4

192 19.3 15.9 23.9

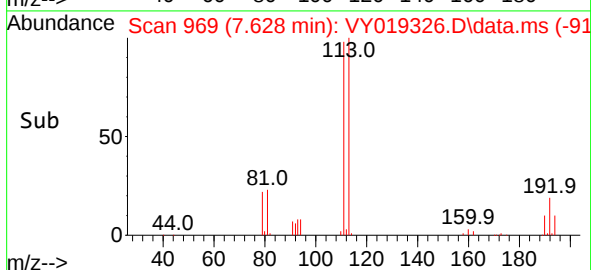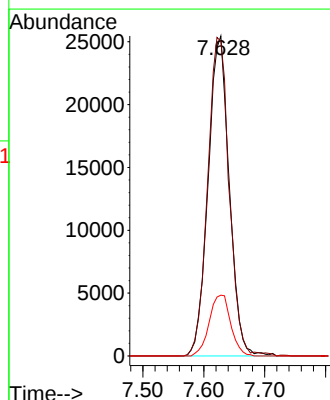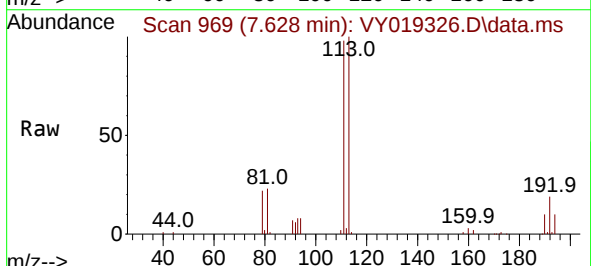

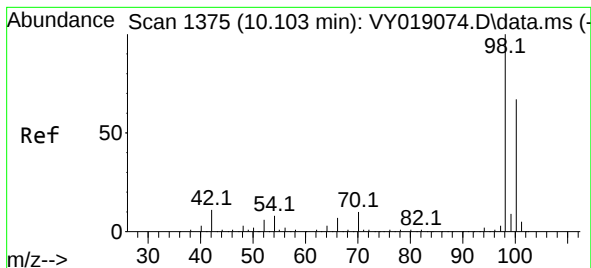

#50

Toluene-d8

Concen: 48.448 ug/l

RT: 10.103 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY019326.D

Acq: 28 Aug 2024 13:27

Instrument :

MSVOA_Y

ClientSampleId :





VY0828SBL01

Tgt Ion: 98 Resp: 218530

Ion Ratio Lower Upper

98 100

100 66.8 52.0 78.0

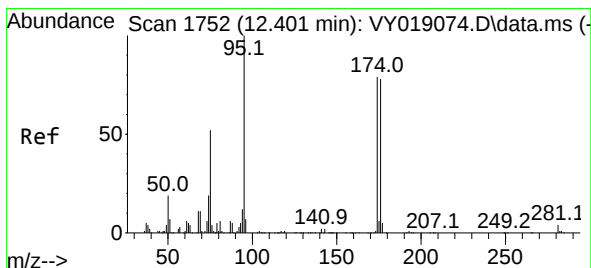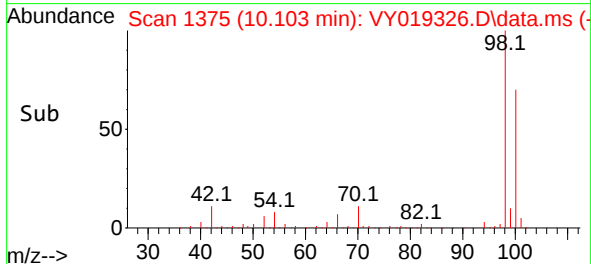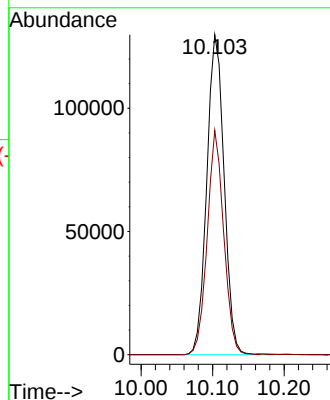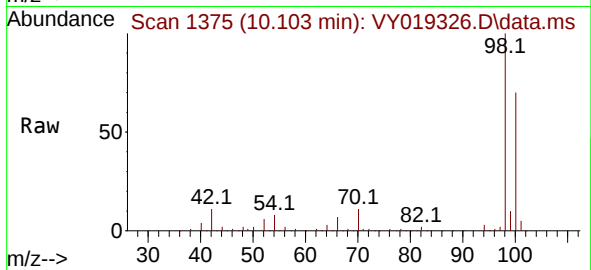

#62

4-Bromofluorobenzene

Concen: 43.477 ug/l

RT: 12.407 min Scan# 1753

Delta R.T. 0.006 min

Lab File: VY019326.D

Acq: 28 Aug 2024 13:27




Tgt Ion: 95 Resp: 66852


Ion Ratio Lower Upper

95 100

174 88.7 0.0 175.6

176 86.6 0.0 171.4


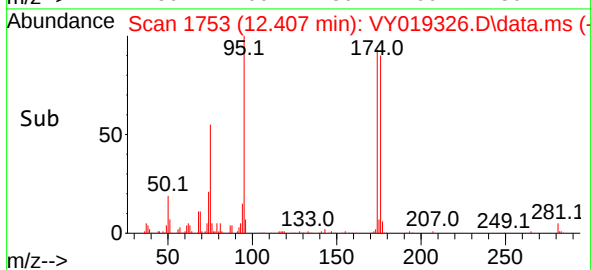
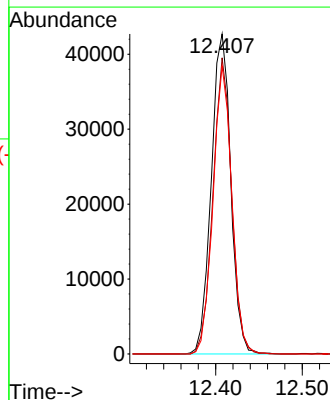
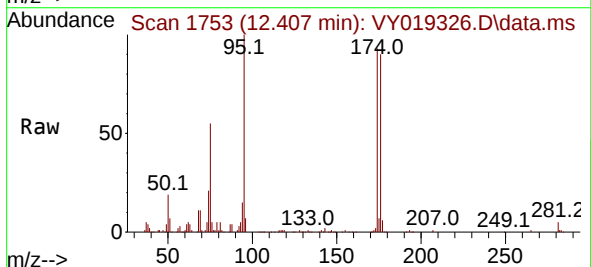


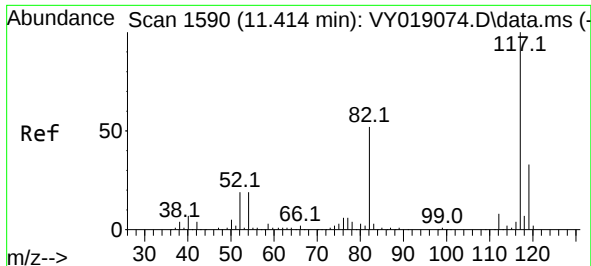

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY019326.D
Acq: 28 Aug 2024 13:27

Instrument :
MSVOA_Y
ClientSampleId :
VY0828SBL01

Tgt Ion:117 Resp: 178659
Ion Ratio Lower Upper
117 100
82 48.9 42.4 63.6
119 31.4 25.9 38.9

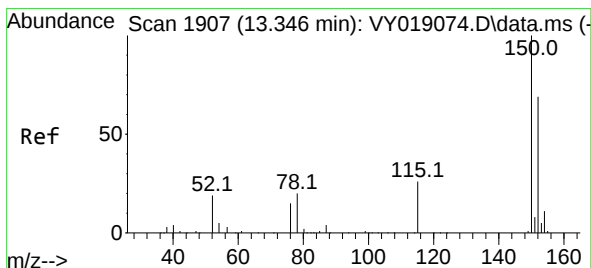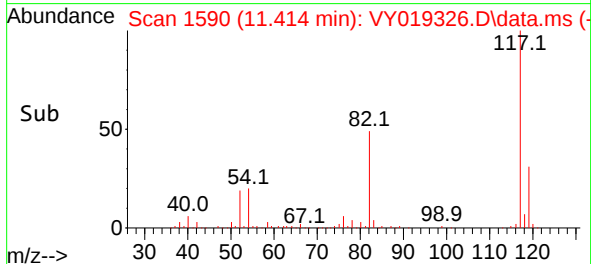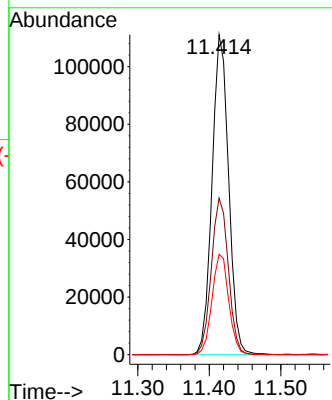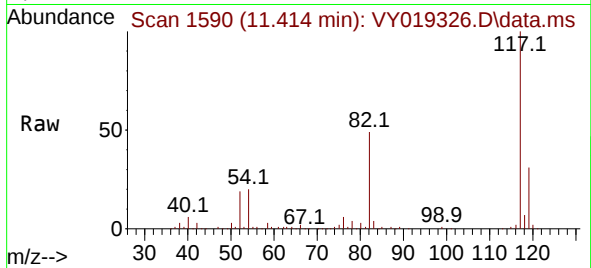

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY019326.D
Acq: 28 Aug 2024 13:27

Tgt Ion:152 Resp: 69188
Ion Ratio Lower Upper
152 100
115 55.6 28.2 84.7
150 154.2 0.0 345.6

