
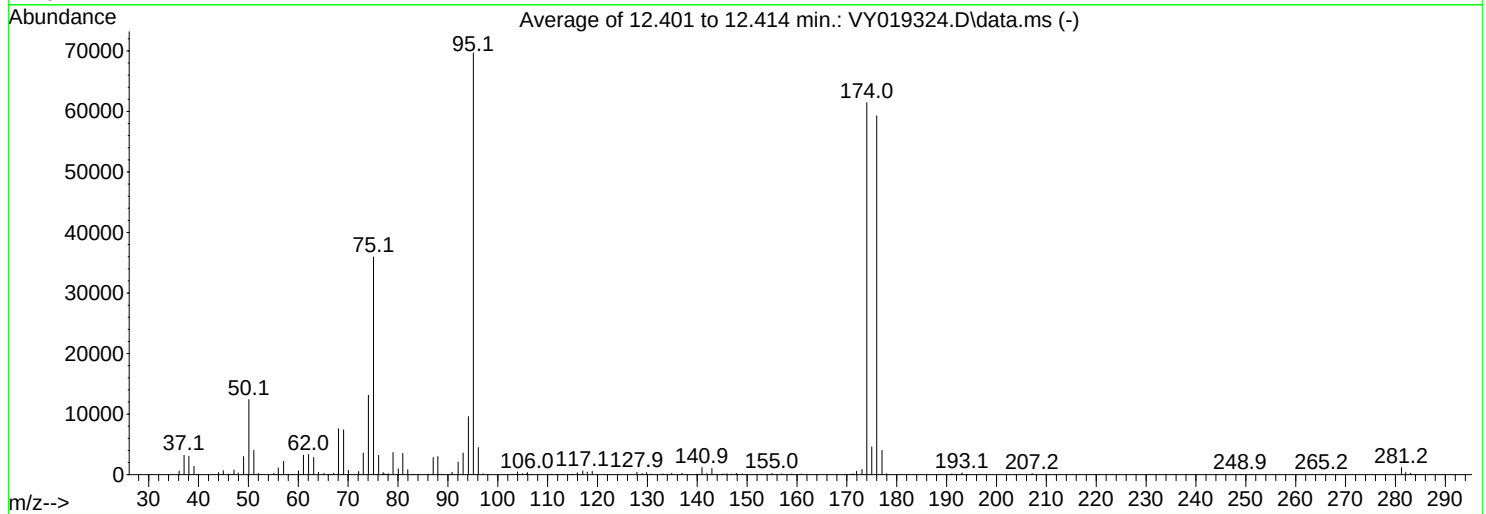


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082824\
Data File : VY019324.D
Acq On : 28 Aug 2024 11:42
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Title : SW846 8260
Last Update : Fri Aug 16 05:10:30 2024

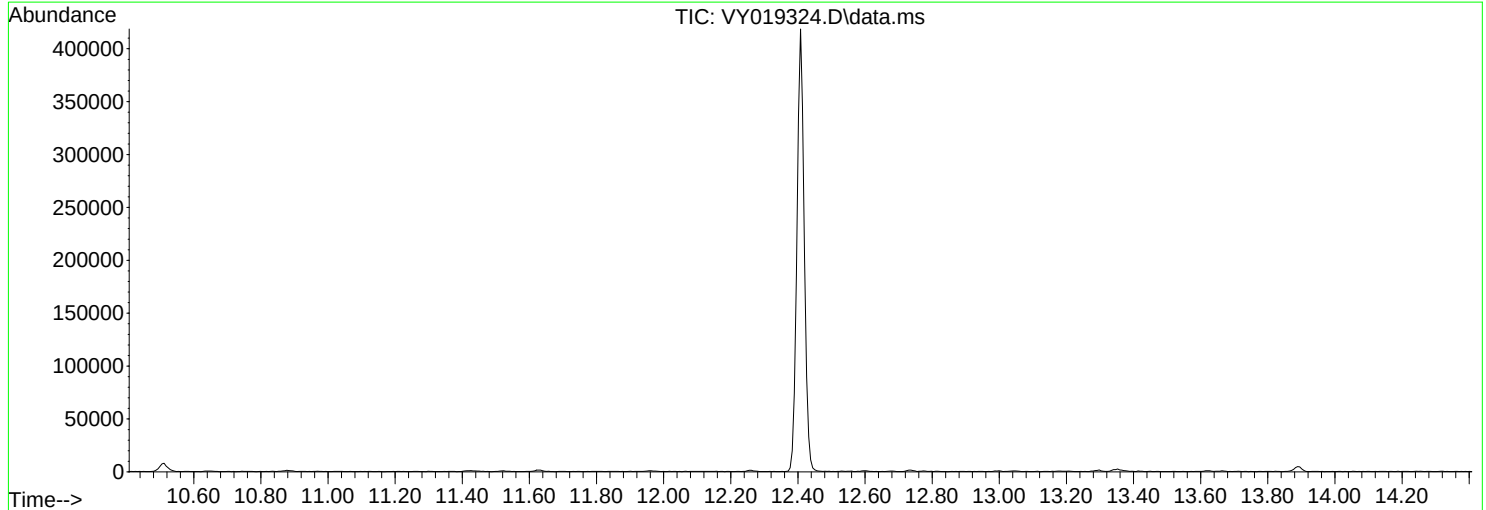

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	12404	PASS
75	95	30	60	51.6	35960	PASS
95	95	100	100	100.0	69680	PASS
96	95	5	9	6.4	4468	PASS
173	174	0.00	2	1.4	843	PASS
174	95	50	100	88.2	61469	PASS
175	174	5	9	7.4	4574	PASS
176	174	95	101	96.4	59267	PASS
177	176	5	9	6.7	3988	PASS